
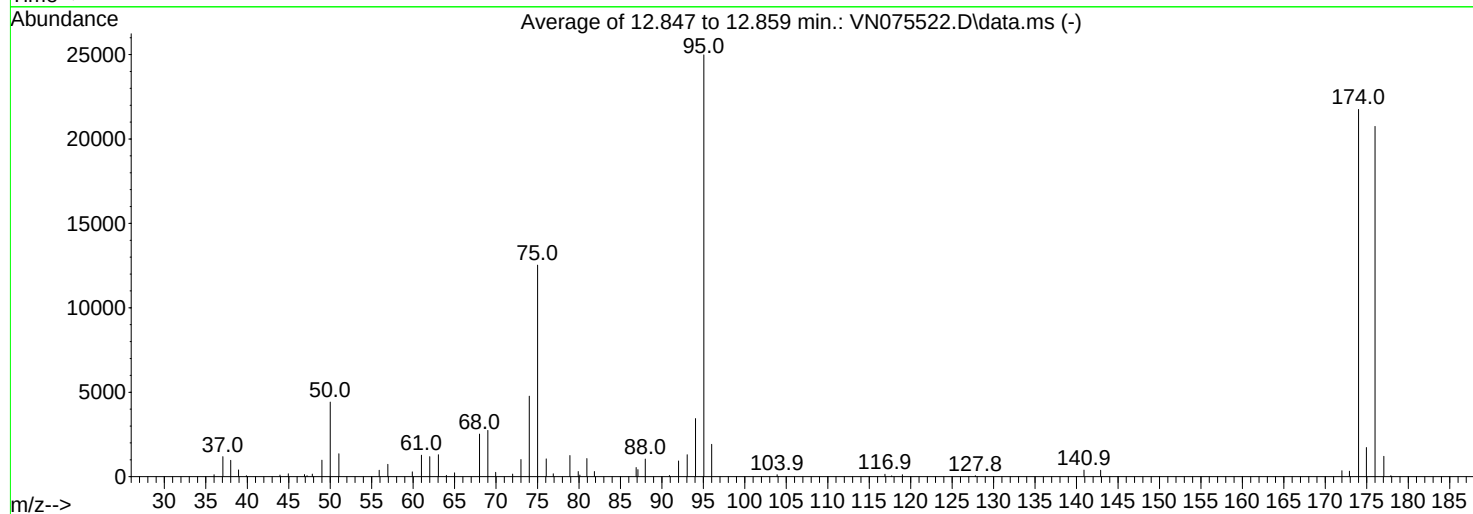


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120222\
 Data File : VN075522.D
 Acq On : 02 Dec 2022 10:50
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Title : SW846 8260
 Last Update : Wed Nov 23 00:18:03 2022

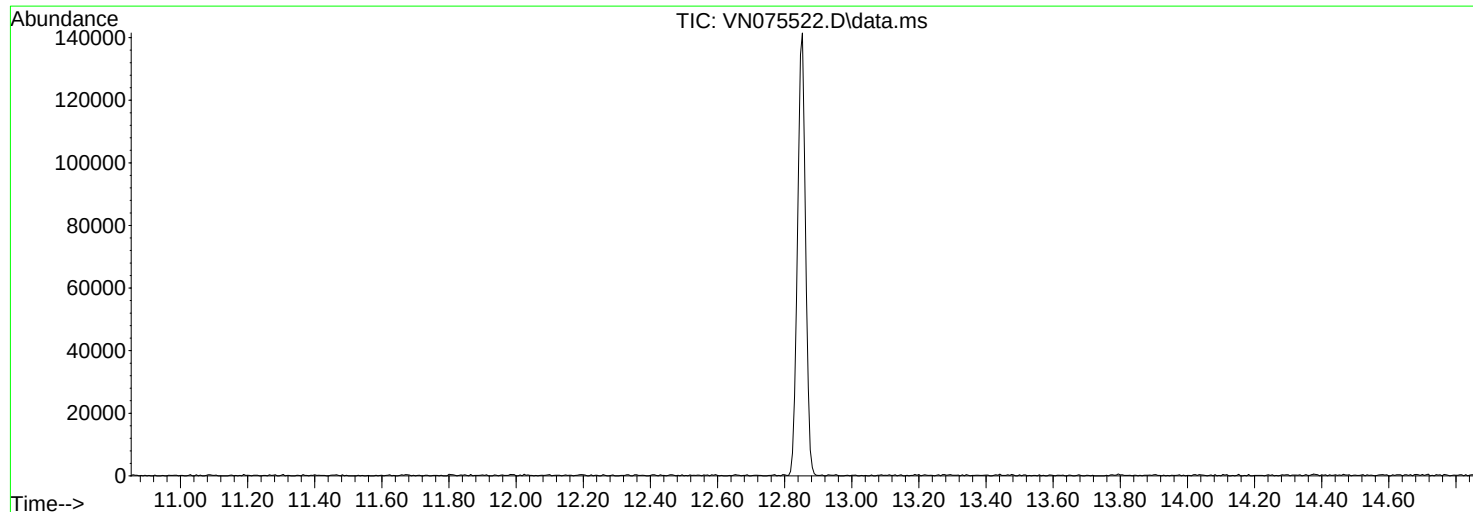

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	4416	PASS
75	95	30	60	50.1	12527	PASS
95	95	100	100	100.0	24987	PASS
96	95	5	9	7.7	1916	PASS
173	174	0.00	2	1.5	321	PASS
174	95	50	100	87.1	21755	PASS
175	174	5	9	8.0	1730	PASS
176	174	95	101	95.4	20747	PASS
177	176	5	9	5.8	1207	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	115	50.00	4416	69.00	2738	80.95	1071
37.05	1187	51.05	1352	69.95	257	81.85	307
38.00	963	55.90	376	72.00	149	86.90	53
38.95	399	56.95	732	73.00	1018	87.10	41
39.90	61	59.90	281	74.00	4771	88.00	1041
43.95	92	61.00	1271	75.00	12527	90.90	66
44.95	167	62.00	1188	76.05	1055	92.00	929
46.90	127	63.05	1298	76.90	173	93.05	1303
47.20	58	64.00	78	78.90	1247	94.05	3439
47.85	150	65.00	226	79.90	304	95.05	24987
49.00	974	68.00	2519	80.10	99	96.00	1916

Average of 12.847 to 12.859 min.: VN075522.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.90	114	176.00	20747				
116.90	140	177.05	1207				
117.70	52	177.90	54				
119.00	118						
127.80	60						
140.90	387						
142.90	384						
172.00	355						
172.90	321						
174.00	21755						
174.95	1730						

Instrument :

MSVOA_N

ClientSampleId :

BFB