
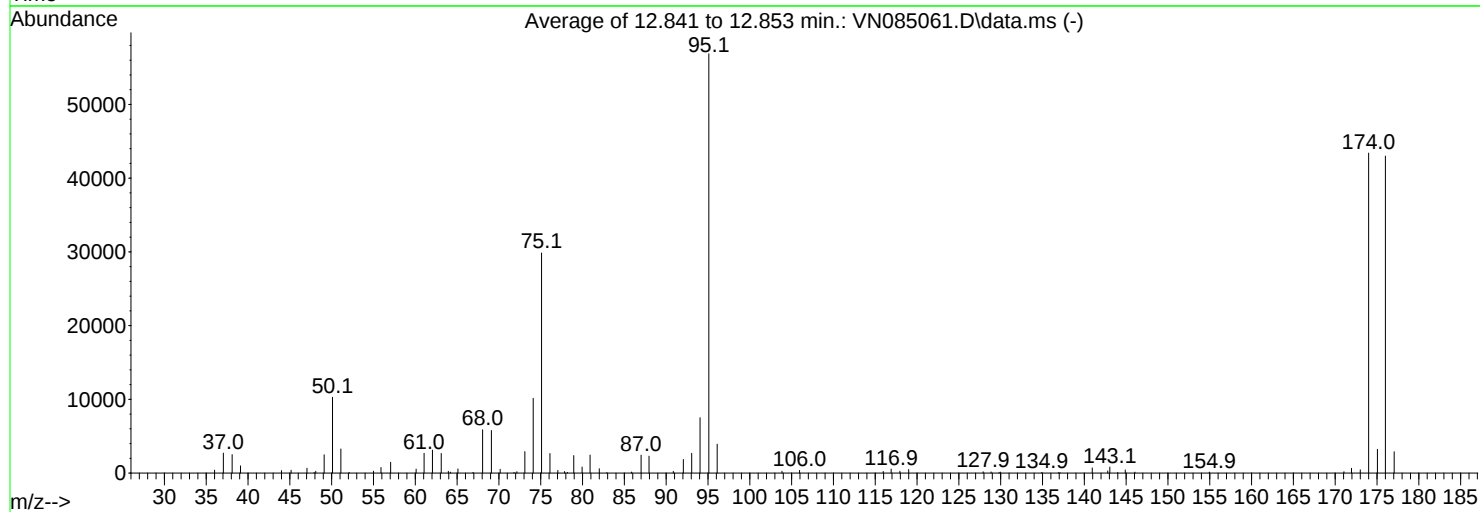


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120224\
Data File : VN085061.D
Acq On : 02 Dec 2024 09:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

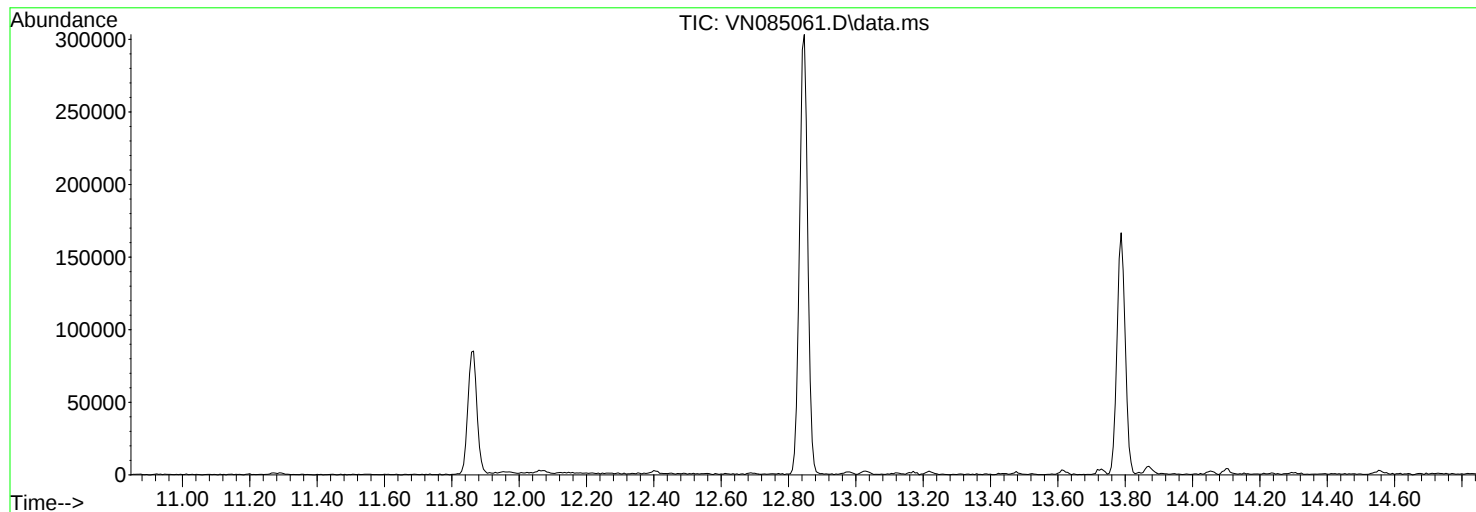

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	10289	PASS
75	95	30	60	52.5	29851	PASS
95	95	100	100	100.0	56877	PASS
96	95	5	9	6.9	3929	PASS
173	174	0.00	2	1.0	445	PASS
174	95	50	100	76.3	43400	PASS
175	174	5	9	7.4	3222	PASS
176	174	95	101	99.1	43003	PASS
177	176	5	9	6.7	2898	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	398	51.10	3268	65.10	575	77.05	368
37.05	2711	52.10	64	66.90	94	77.85	217
38.10	2508	55.00	263	68.05	5875	78.20	90
39.10	975	55.90	764	69.10	5775	78.95	2374
44.00	331	57.05	1473	70.15	513	79.95	821
45.15	391	60.10	541	71.80	95	80.90	2447
47.05	661	61.05	2691	72.15	199	82.00	592
47.90	77	62.05	3121	73.10	2914	82.90	54
48.10	246	63.10	2670	74.10	10142	85.85	145
49.10	2489	63.95	241	75.10	29851	87.00	2439
50.10	10289	64.20	129	76.10	2658	87.95	2296

Average of 12.841 to 12.853 min.: VN085061.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.85	240	119.00	486	144.00	72		
92.05	1848	127.90	185	144.90	424		
93.05	2685	128.85	164	146.05	130		
94.05	7513	129.80	72	154.95	135		
95.10	56877	129.95	141	171.05	198		
96.10	3929	134.90	68	171.95	645		
103.85	256	136.90	62	173.00	445		
105.95	362	137.10	56	174.00	43400		
115.95	230	140.95	702	175.05	3222		
116.90	545	142.80	293	176.00	43003		
117.95	252	143.05	813	177.05	2898		

Instrument :

MSVOA_N

ClientSampleId :

BFB