

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120225\
 Data File : VN088398.D
 Acq On : 02 Dec 2025 10:40
 Operator : JC\MD
 Sample : VN1202MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1202MBL01

Quant Time: Dec 03 01:24:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 25 01:34:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	171979	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	394708	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.841	117	389937	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	179883	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	204008	62.970	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	125.940%#
35) Dibromofluoromethane	8.147	113	149305	54.584	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	109.160%
50) Toluene-d8	10.541	98	523434	51.431	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.860%
62) 4-Bromofluorobenzene	12.823	95	184788	52.916	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	105.840%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120225\
Data File : VN088398.D
Acq On : 02 Dec 2025 10:40
Operator : JC\MD
Sample : VN1202MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1202MBL01

Quant Time: Dec 03 01:24:40 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 25 01:34:52 2025
Response via : Initial Calibration




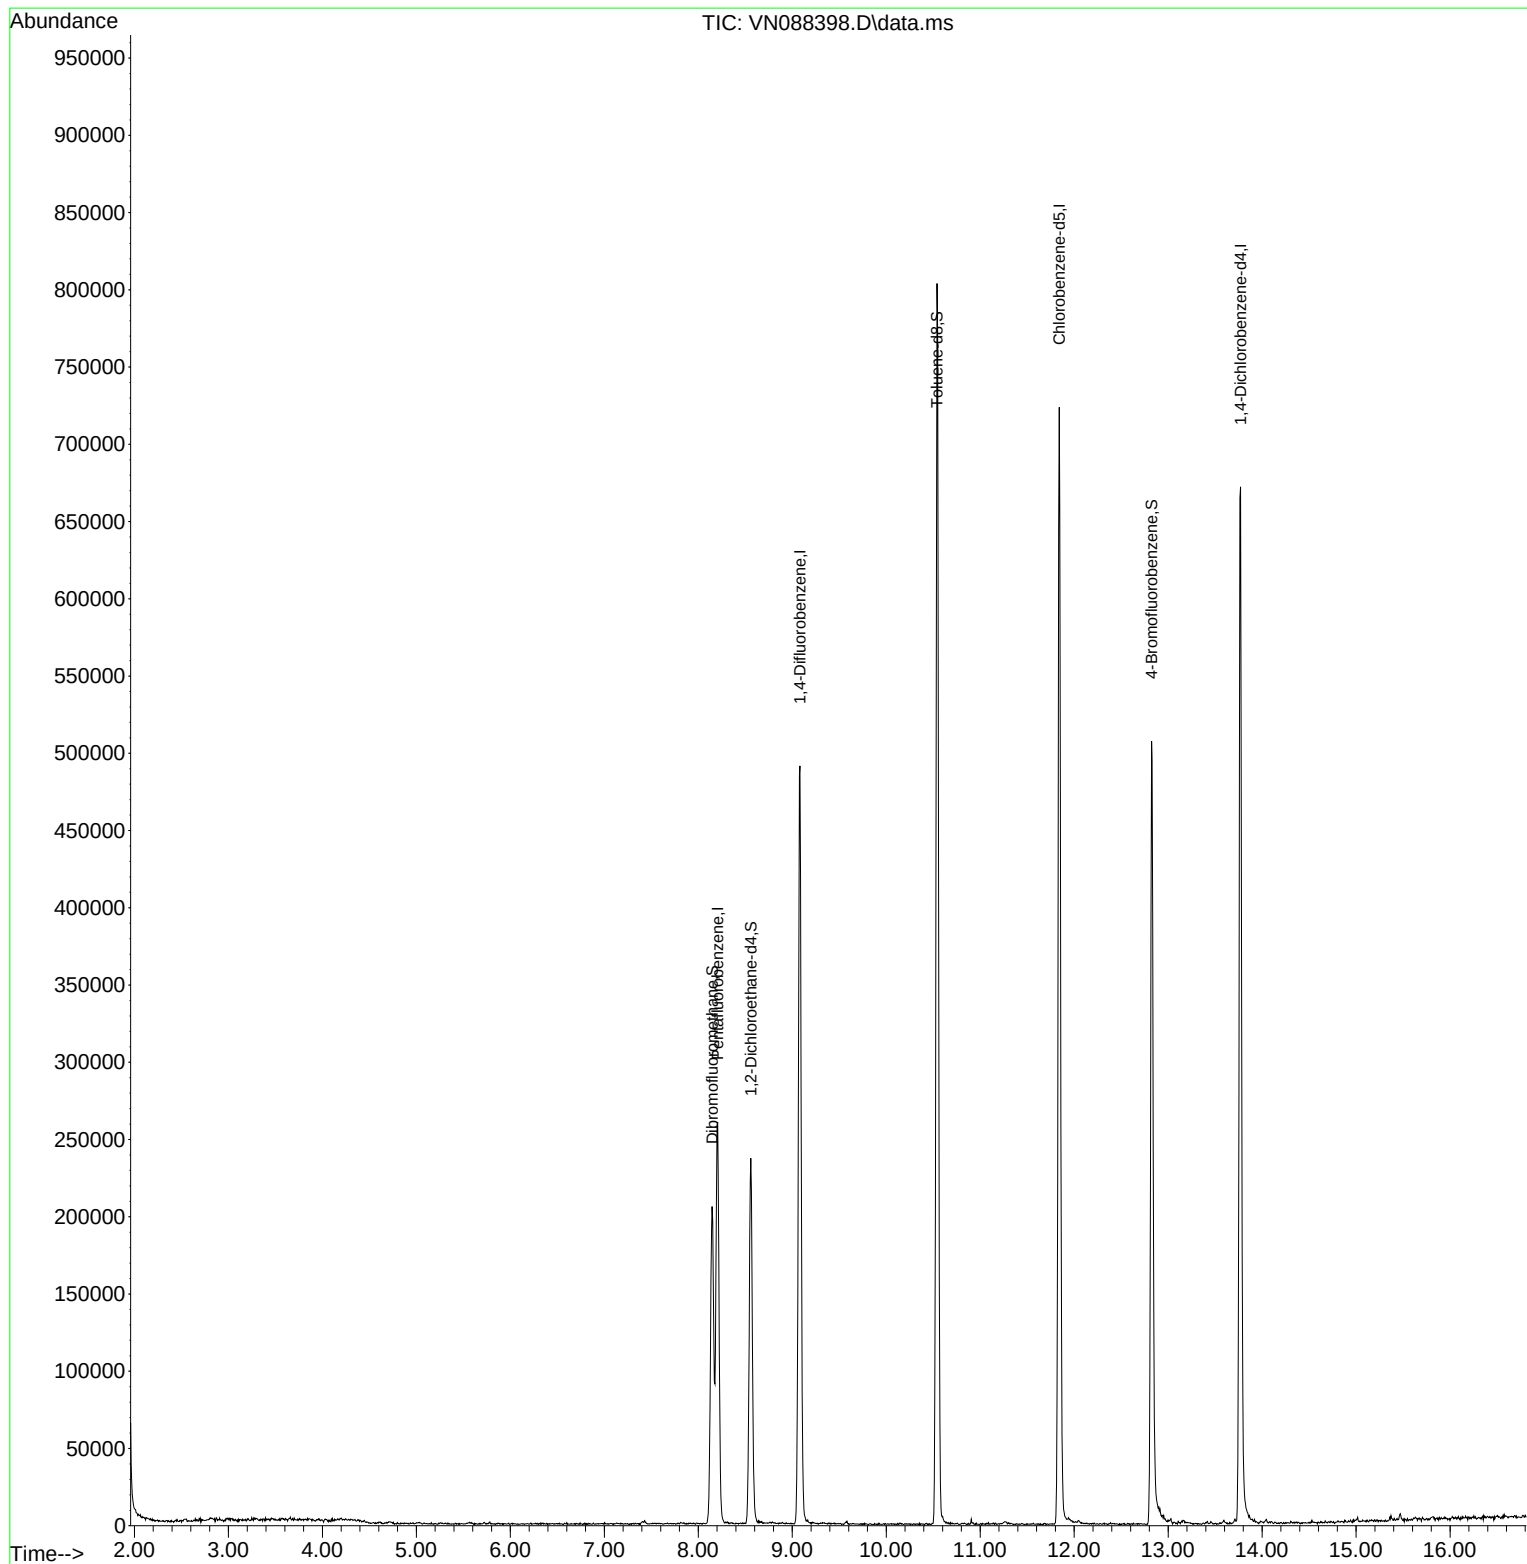


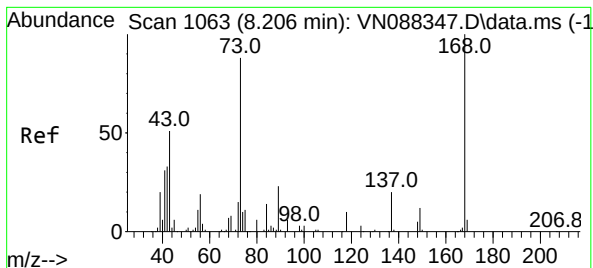

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1063
Delta R.T. 0.000 min
Lab File: VN088398.D
Acq: 02 Dec 2025 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN1202MBL01


Tgt Ion:168 Resp: 171979
Ion Ratio Lower Upper
168 100
99 66.7 57.1 85.7

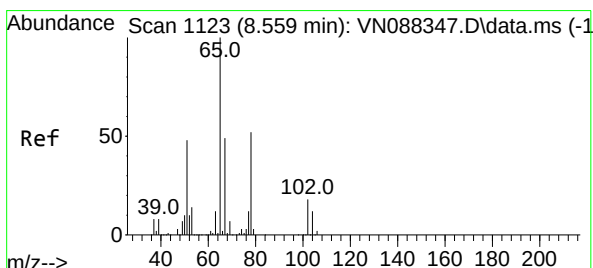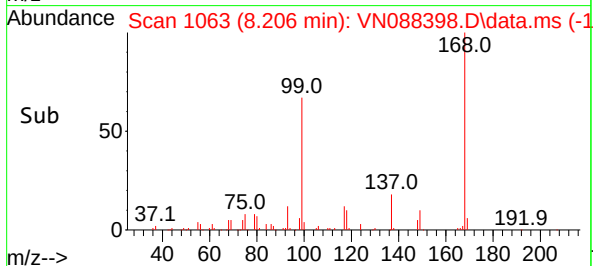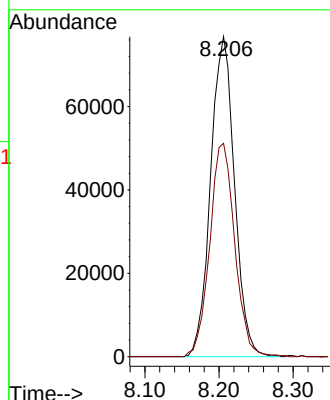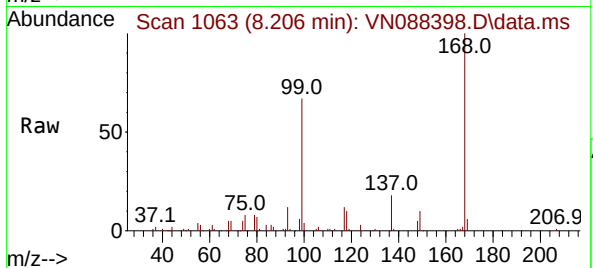

#33
1,2-Dichloroethane-d4
Concen: 62.970 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. 0.000 min
Lab File: VN088398.D
Acq: 02 Dec 2025 10:40

Tgt Ion: 65 Resp: 204008
Ion Ratio Lower Upper
65 100
67 49.0 0.0 100.8

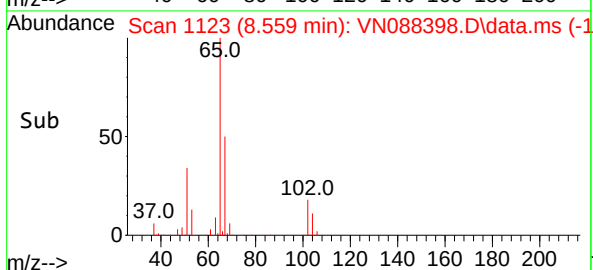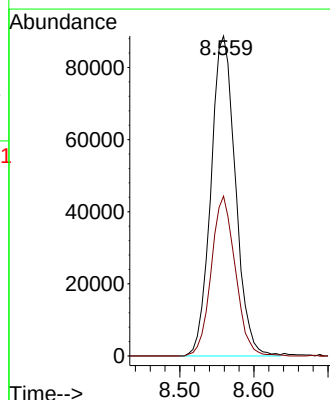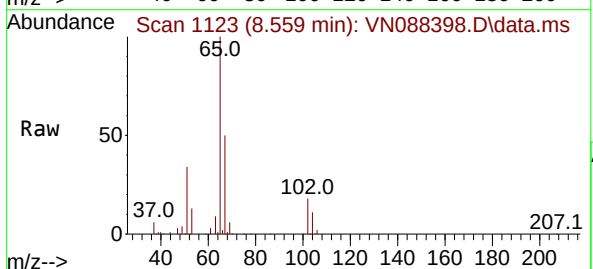

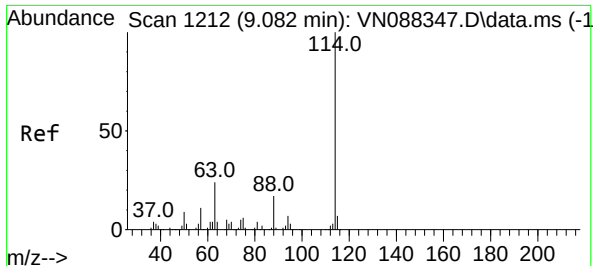

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.082 min Scan# 11

Delta R.T. 0.000 min

Lab File: VN088398.D

Acq: 02 Dec 2025 10:40

Instrument :

MSVOA_N

ClientSampleId :

VN1202MBL01





Tgt Ion:114 Resp: 394708

Ion Ratio Lower Upper

114 100

63 22.8 0.0 49.0

88 16.1 0.0 34.0

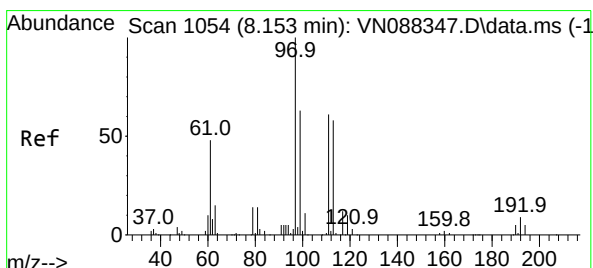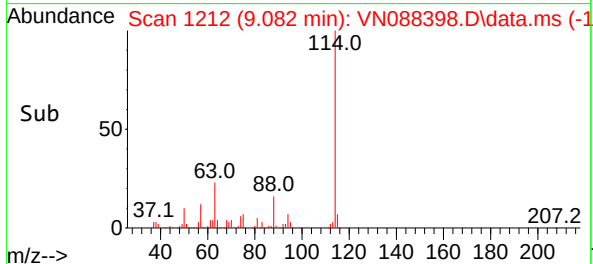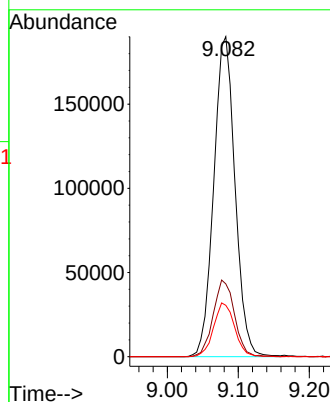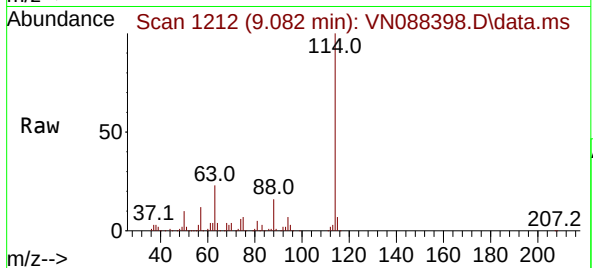

#35

Dibromofluoromethane

Concen: 54.584 ug/l

RT: 8.147 min Scan# 1053

Delta R.T. -0.006 min

Lab File: VN088398.D

Acq: 02 Dec 2025 10:40




Tgt Ion:113 Resp: 149305


Ion Ratio Lower Upper

113 100

111 103.1 82.5 123.7

192 16.5 12.8 19.2


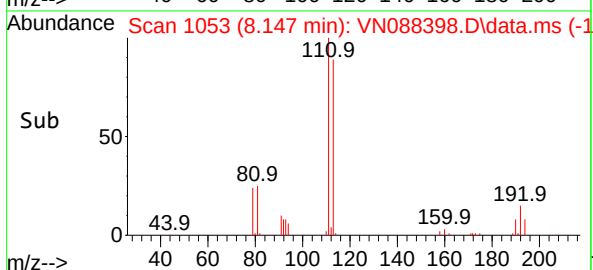
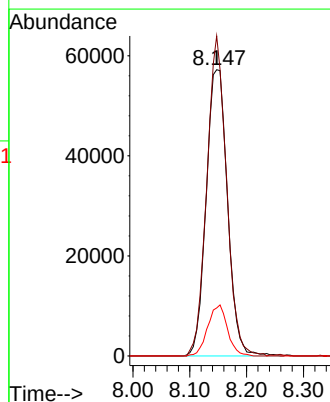
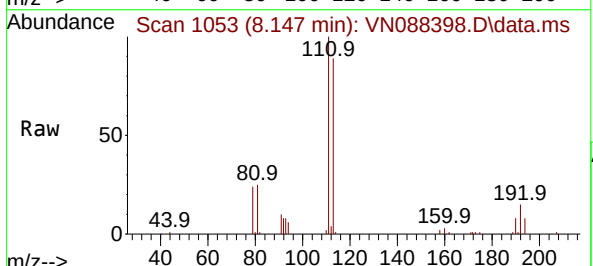


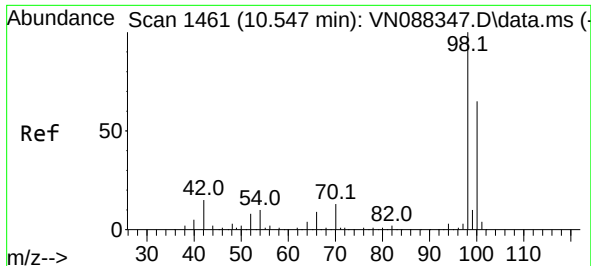

#50
Toluene-d8
Concen: 51.431 ug/l
RT: 10.541 min Scan# 1461
Delta R.T. -0.006 min
Lab File: VN088398.D
Acq: 02 Dec 2025 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN1202MBL01


Tgt Ion: 98 Resp: 523434
Ion Ratio Lower Upper
98 100
100 63.9 52.2 78.2

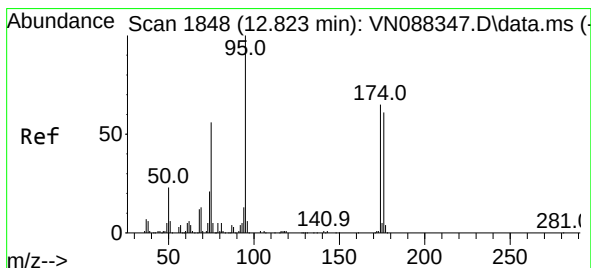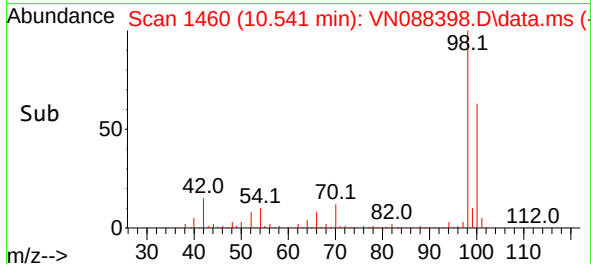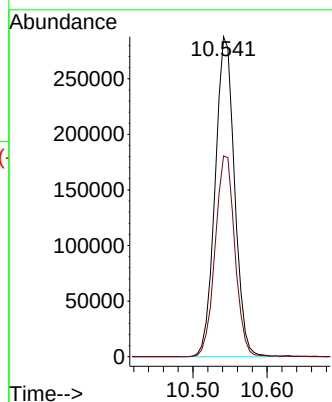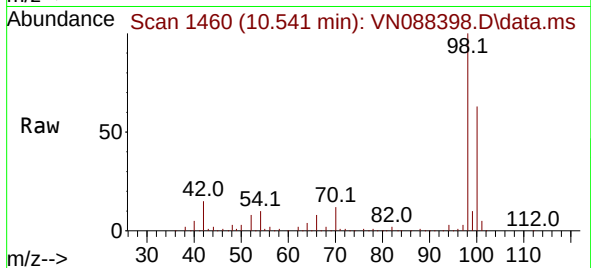

#62
4-Bromofluorobenzene
Concen: 52.916 ug/l
RT: 12.823 min Scan# 1848
Delta R.T. 0.000 min
Lab File: VN088398.D
Acq: 02 Dec 2025 10:40

Tgt Ion: 95 Resp: 184788
Ion Ratio Lower Upper
95 100
174 70.5 0.0 139.0
176 66.8 0.0 132.4


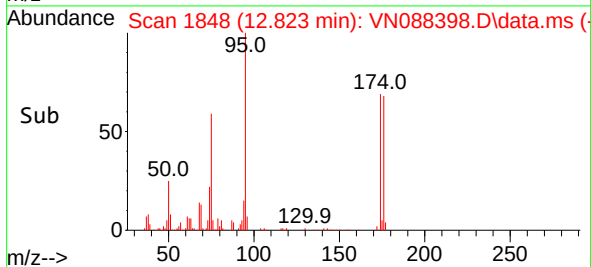
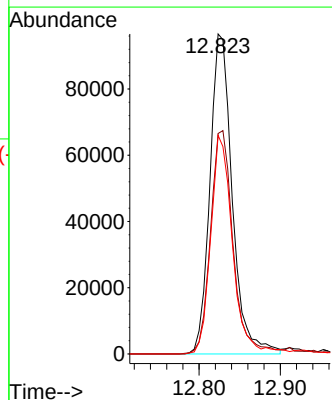
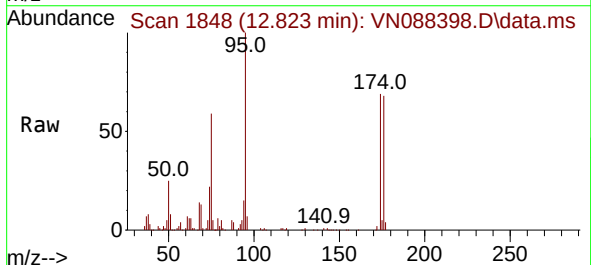


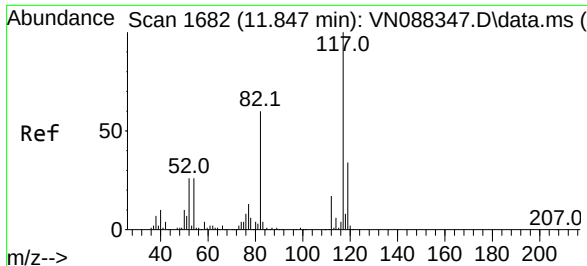

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.841 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN088398.D
Acq: 02 Dec 2025 10:40

Instrument :
MSVOA_N
ClientSampleId :
VN1202MBL01

Tgt Ion:117 Resp: 389937
Ion Ratio Lower Upper
117 100
82 62.2 47.8 71.8
119 32.3 26.9 40.3

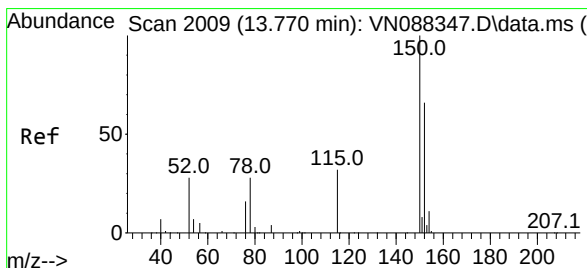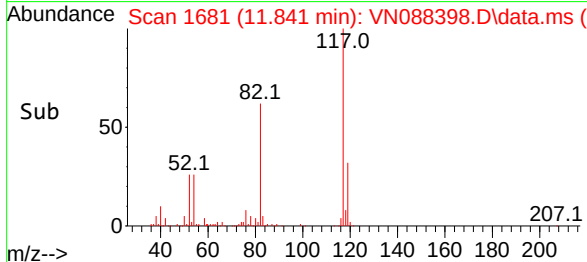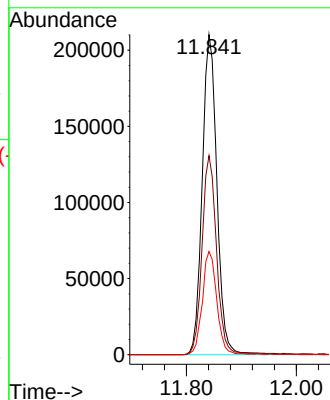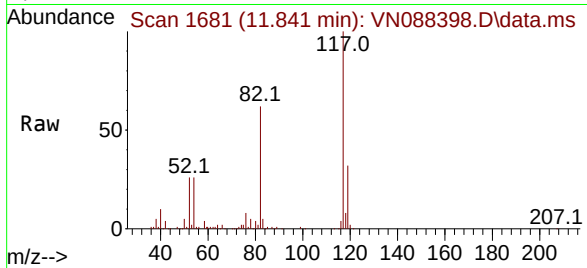

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.000 min
Lab File: VN088398.D
Acq: 02 Dec 2025 10:40

Tgt Ion:152 Resp: 179883
Ion Ratio Lower Upper
152 100
115 65.8 33.0 98.9
150 159.4 0.0 349.0

