

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120225\
 Data File : VN088405.D
 Acq On : 02 Dec 2025 13:16
 Operator : JC\MD
 Sample : Q3716-04DL 200X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW7DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
 Title : SW846 8260

Signal : TIC: VN088405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.336	59	65	73	rVB3	22070	40200	1.12%	0.178%
2	2.536	89	99	110	rBV	80382	153481	4.29%	0.678%
3	3.271	215	224	236	rBV2	107095	258961	7.24%	1.144%
4	3.665	281	291	303	rVV4	46737	157542	4.41%	0.696%
5	3.871	317	326	337	rVB2	36813	95904	2.68%	0.424%
6	4.048	348	356	364	rBV3	20365	54685	1.53%	0.242%
7	4.148	364	373	384	rVV2	65510	189995	5.31%	0.839%
8	5.142	534	542	554	rBV6	11230	37564	1.05%	0.166%
9	5.342	567	576	578	rVV5	22574	66214	1.85%	0.292%
10	5.365	578	580	594	rVB4	20003	49383	1.38%	0.218%
11	7.312	901	911	922	rBV3	33620	104002	2.91%	0.459%
12	7.989	1018	1026	1034	rVB3	16502	40073	1.12%	0.177%
13	8.147	1043	1053	1057	rBV	203080	473818	13.25%	2.093%
14	8.206	1057	1063	1075	rVV	287364	710409	19.87%	3.138%
15	8.430	1092	1101	1110	rVV3	20657	49961	1.40%	0.221%
16	8.565	1113	1124	1137	rVV2	260885	844261	23.61%	3.729%
17	8.741	1140	1154	1165	rVV4	56832	195389	5.46%	0.863%
18	9.083	1200	1212	1224	rBV	515421	1098882	30.73%	4.854%
19	9.577	1283	1296	1300	rBV7	33707	91718	2.57%	0.405%
20	9.988	1360	1366	1375	rVB2	42791	85088	2.38%	0.376%
21	10.124	1378	1389	1395	rVV3	59495	141683	3.96%	0.626%
22	10.183	1395	1399	1413	rVB4	15773	40038	1.12%	0.177%
23	10.318	1413	1422	1435	rBV3	17461	44960	1.26%	0.199%
24	10.541	1453	1460	1465	rBV	798190	1448590	40.51%	6.398%
25	10.606	1465	1471	1485	rVV	1142450	2144288	59.97%	9.471%
26	11.841	1671	1681	1691	rBV	747868	1381328	38.63%	6.101%
27	11.941	1691	1698	1707	rVV	425635	745329	20.84%	3.292%
28	12.041	1707	1715	1735	rVB	1820498	3575739	100.00%	15.794%
29	12.376	1763	1772	1782	rBV	757644	1344357	37.60%	5.938%
30	12.829	1840	1849	1867	rVB	524886	1026075	28.70%	4.532%
31	13.012	1875	1880	1885	rBV	67756	119092	3.33%	0.526%
32	13.071	1885	1890	1894	rVV	352216	633272	17.71%	2.797%
33	13.106	1894	1896	1899	rVV	167409	235290	6.58%	1.039%
34	13.147	1899	1903	1916	rVB	215819	386018	10.80%	1.705%
35	13.312	1924	1931	1939	rBV2	130483	239139	6.69%	1.056%
36	13.459	1949	1956	1969	rBV	721573	1181750	33.05%	5.220%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120225\
Data File : VN088405.D
Acq On : 02 Dec 2025 13:16
Operator : JC\MD
Sample : Q3716-04DL 200X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW7DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Title : SW846 8260

37	13.765	2001	2008	2030	rVB2	754020	1666636	46.61%	7.361%
38	13.929	2030	2036	2037	rBV4	26460	38031	1.06%	0.168%
39	13.971	2037	2043	2059	rVV4	125281	451070	12.61%	1.992%
40	14.218	2080	2085	2088	rBV3	40926	72119	2.02%	0.319%
41	14.247	2088	2090	2095	rVV2	40069	53651	1.50%	0.237%
42	14.306	2095	2100	2107	rVB	64829	107265	3.00%	0.474%
43	14.423	2114	2120	2124	rVB2	36011	64394	1.80%	0.284%
44	14.629	2149	2155	2158	rVV	39553	67821	1.90%	0.300%
45	14.665	2158	2161	2166	rVV	53501	88230	2.47%	0.390%
46	14.906	2197	2202	2213	rVB7	38701	96781	2.71%	0.427%
47	15.029	2213	2223	2229	rBV2	55536	144685	4.05%	0.639%
48	15.412	2279	2288	2297	rVB8	16061	44595	1.25%	0.197%
49	15.612	2311	2322	2332	rBV2	81865	181118	5.07%	0.800%
50	16.753	2508	2516	2522	rBV2	33619	79573	2.23%	0.351%




Sum of corrected areas: 22640447

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120225\
Data File : VN088405.D
Acq On : 02 Dec 2025 13:16
Operator : JC\MD
Sample : Q3716-04DL 200X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

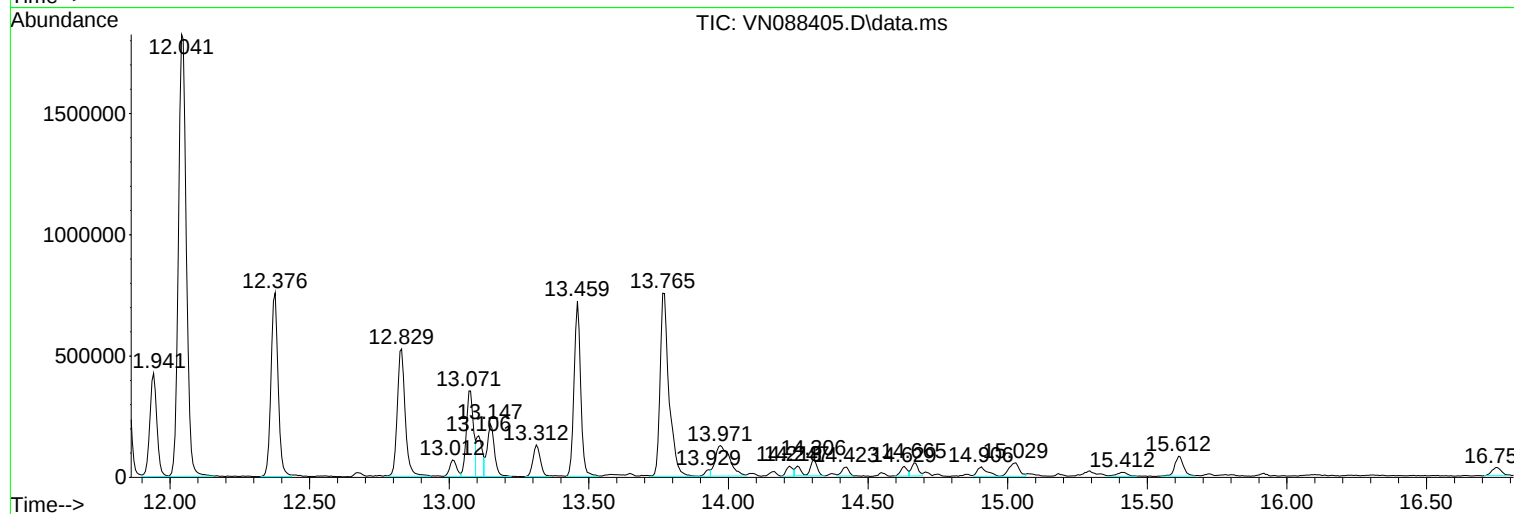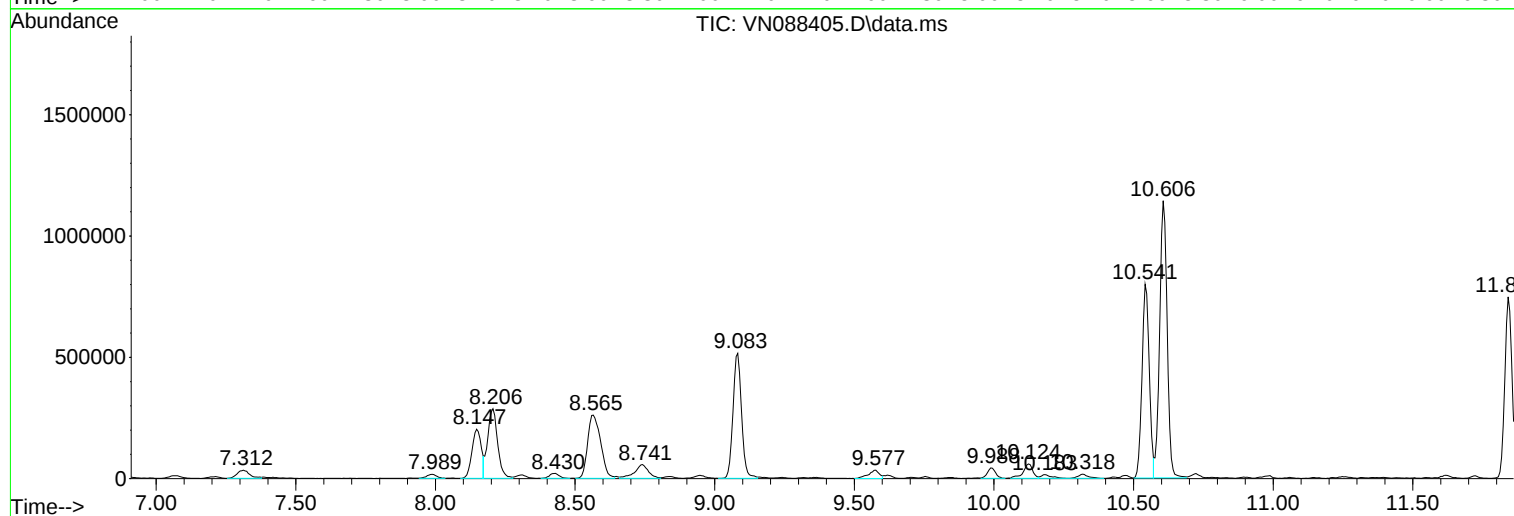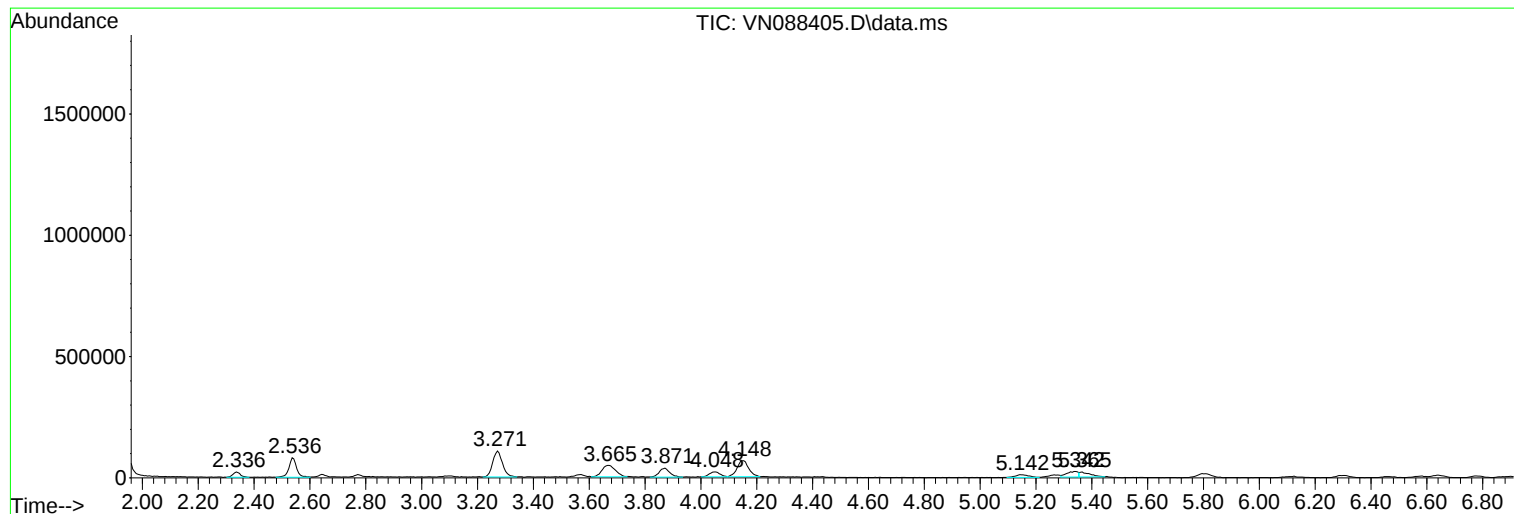

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120225\
Data File : VN088405.D
Acq On : 02 Dec 2025 13:16
Operator : JC\MD
Sample : Q3716-04DL 200X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120225\
Data File : VN088405.D
Acq On : 02 Dec 2025 13:16
Operator : JC\MD
Sample : Q3716-04DL 200X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc