

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120318\
 Data File : VN052641.D
 Acq On : 3 Dec 2018 19:36
 Operator : MD\SY
 Sample : PB115231ZHE#12
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 24 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 PB115231ZHE#12

Quant Time: Dec 04 00:35:14 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 03 03:24:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1248296	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1933781	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1715760	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	663546	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	660859	48.62	ug/l	0.00
Spiked Amount			Recovery	=	97.24%	
35) Dibromofluoromethane	7.59	113	593917	49.82	ug/l	0.00
Spiked Amount			Recovery	=	99.64%	
50) Toluene-d8	10.09	98	2356736	50.79	ug/l	0.00
Spiked Amount			Recovery	=	101.58%	
62) 4-Bromofluorobenzene	12.40	95	747451	47.93	ug/l	0.00
Spiked Amount			Recovery	=	95.86%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.82	43	16432	4.584	ug/l	98
18) Methyl Acetate	4.33	43	6405	0.623	ug/l #	66
20) Methylene Chloride	4.56	84	168009	11.976	ug/l	98
25) 2-Butanone	6.85	43	2128	0.419	ug/l #	90
29) Tetrahydrofuran	7.21	42	735	0.224	ug/l #	79
31) Cyclohexane	7.67	56	21791	0.570	ug/l #	1
36) 1,1-Dichloropropene	7.67	75	86802	4.753	ug/l #	49
38) Carbon Tetrachloride	7.67	117	108752	6.579	ug/l #	16
43) Isopropyl Acetate	8.17	43	70326	3.729	ug/l #	75
45) 1,2-Dichloropropane	9.27	63	3344	0.231	ug/l #	43
48) Methyl methacrylate	9.18	41	14295	1.454	ug/l #	13
49) 1,4-Dioxane	9.27	88	398	3.900	ug/l #	1
51) 4-Methyl-2-Pentanone	10.03	43	15618	1.476	ug/l #	36
54) cis-1,3-Dichloropropene	9.90	75	127471	6.349	ug/l #	62
56) Ethyl methacrylate	10.54	69	1487	2.782	ug/l #	1
57) 1,3-Dichloropropane	10.77	76	26089	1.299	ug/l #	43
59) 2-Hexanone	10.77	43	358852	50.528	ug/l #	52
71) Bromoform	12.40	173	4562	0.560	ug/l #	1
74) N-amyl acetate	11.88	43	41824	3.180	ug/l #	52
76) 1,2,3-Trichloropropane	12.40	75	357636	34.952	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.73	105	28511	0.687	ug/l	99
81) trans-1,4-Dichloro-2-buten	12.40	75	357636	116.723	ug/l #	11
95) Naphthalene	15.14	128	385	3.443	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN120318\
Data File : VN052641.D
Acq On : 3 Dec 2018 19:36
Operator : MD\SY
Sample : PB115231ZHE#12
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 24 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
PB115231ZHE#12

Quant Time: Dec 04 00:35:14 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 03 03:24:02 2018
Response via : Initial Calibration

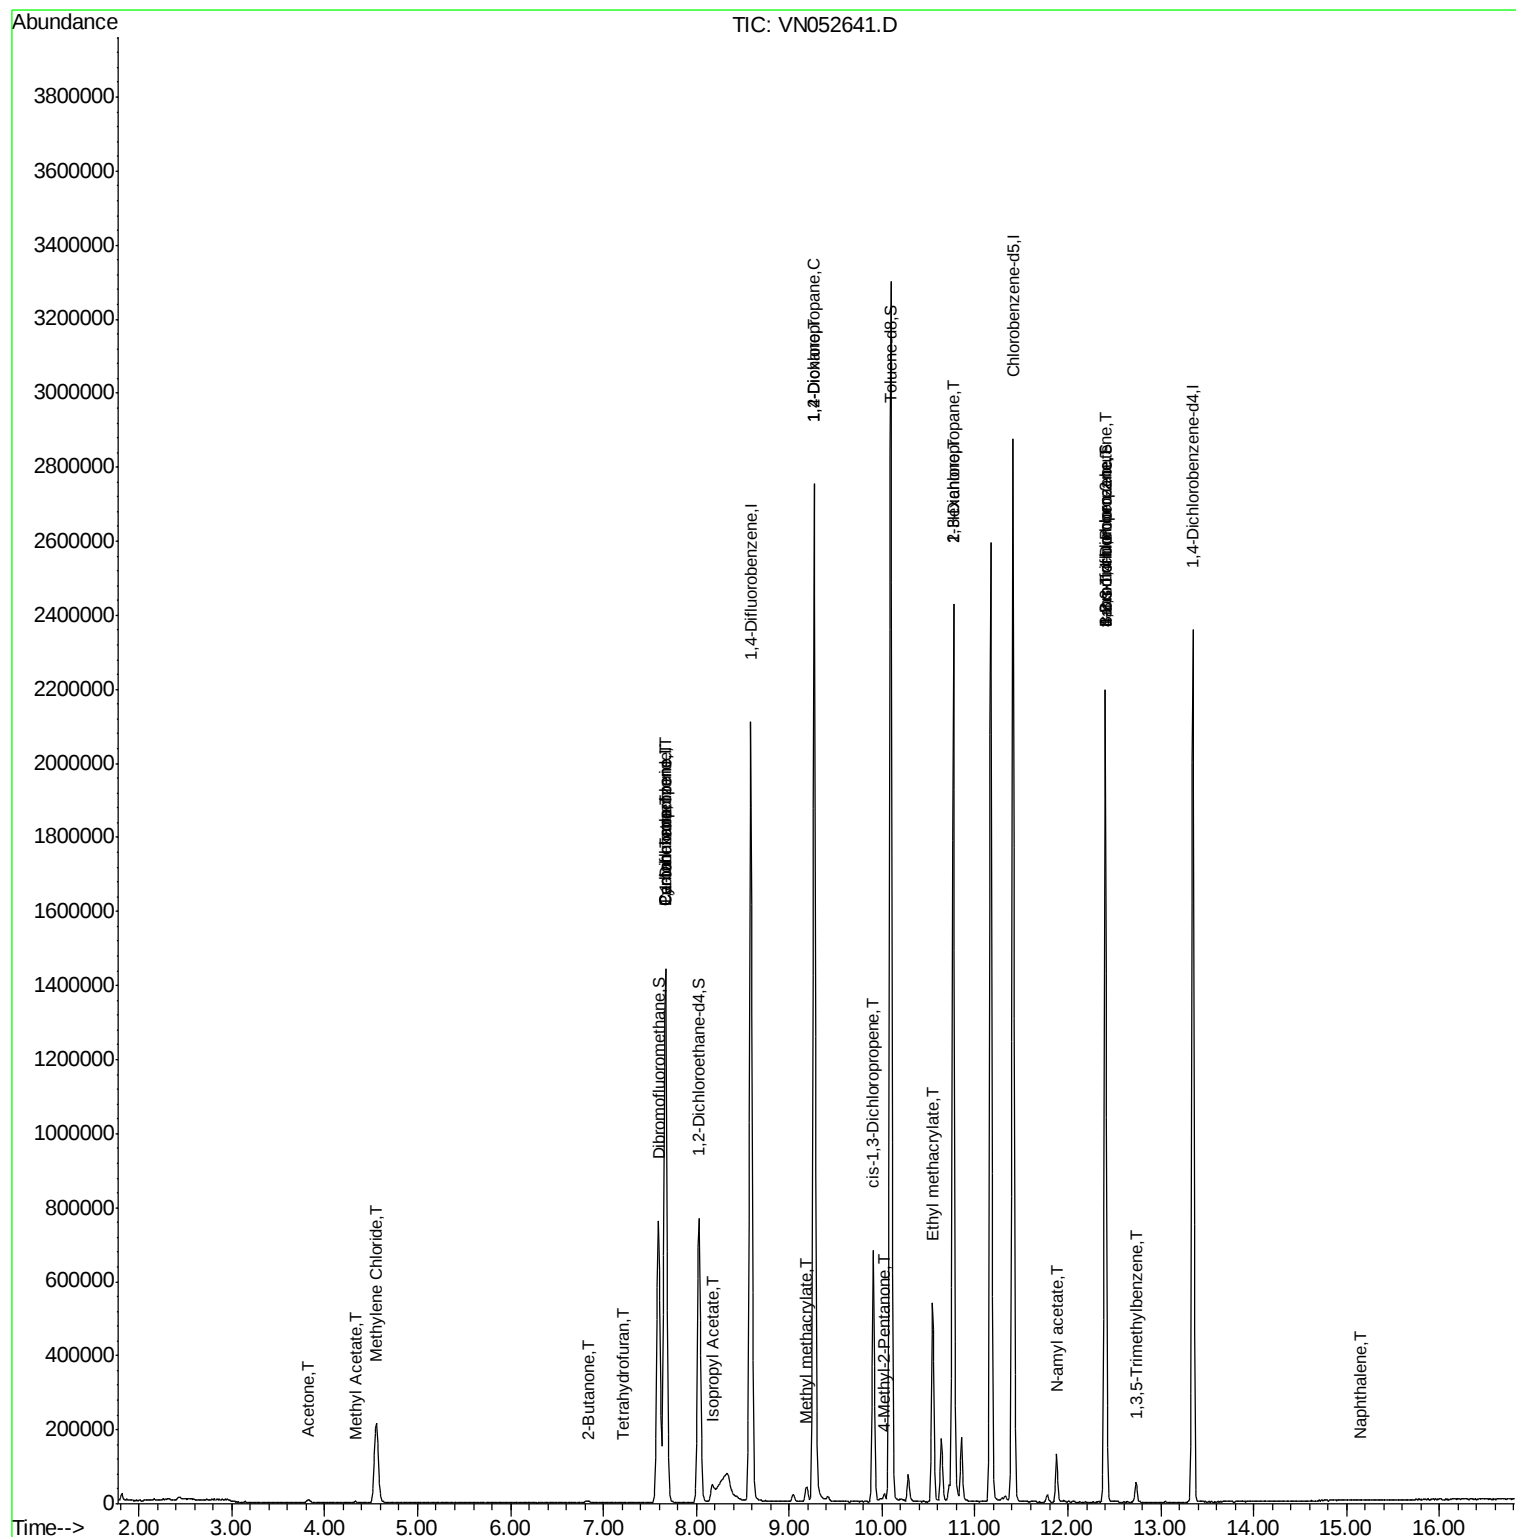

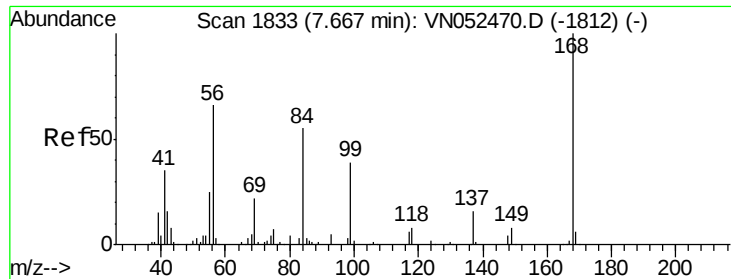

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36

Instrument :

MSVOA_N

ClientSampleId :


PB115231ZHE#12

Tot Ion:168 Resp: 1248296

Ion Ratio Lower Upper

168 100

99 51.0 41.7 62.5



Abundance Ion 167.90 (167.60 to 168.60): VN052641.D (-1740) (-)

Ion 98.90 (98.60 to 99.60): VN052641.D (-1740) (-)

7.67

600000

500000

400000



300000

200000

100000

0

Time-->

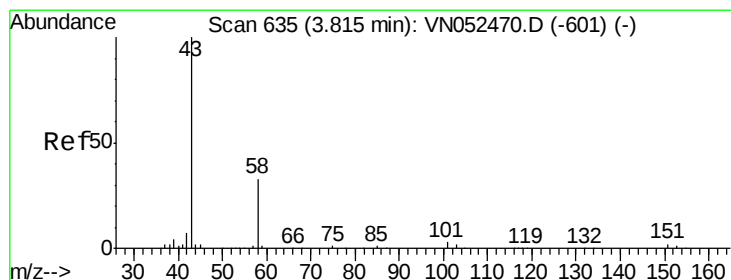

#16

Acetone

Concen: 4.584 ug/l

RT: 3.82 min Scan# 637

Delta R.T. 0.01 min

Lab File: VN052641.D


Acq: 3 Dec 2018 19:36

Tgt Ion: 43 Resp: 16432

Ion Ratio Lower Upper

43 100

58 31.1 26.0 39.0

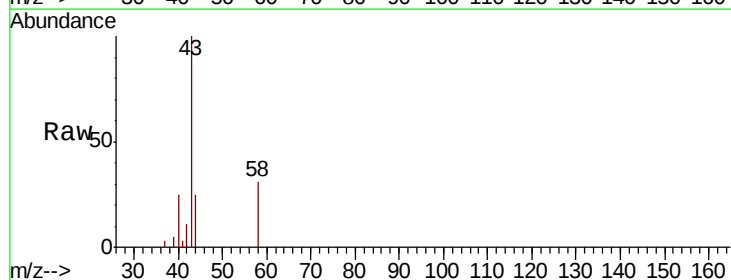

Abundance Ion 43.00 (42.70 to 43.70): VN052641.D (-542) (-)

Ion 58.00 (57.70 to 58.70): VN052641.D (-542) (-)

3.82

6000

5000

4000


3000


2000

1000

0

Time-->







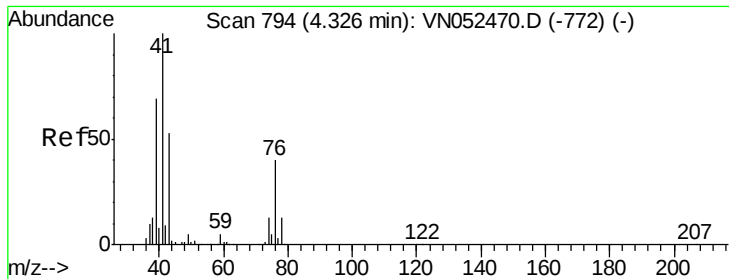

#18
Methyl Acetate
Concen: 0.623 ug/l
RT: 4.33 min Scan# 796
Delta R.T. 0.01 min
Lab File: VN052641.D
Acq: 3 Dec 2018 19:36




Instrument :
MSVOA_N
ClientSampleId :
PB115231ZHE#12


Tot Ion: 43 Resp: 6405
Ion Ratio Lower Upper
43 100
74 6.7 18.6 27.8#

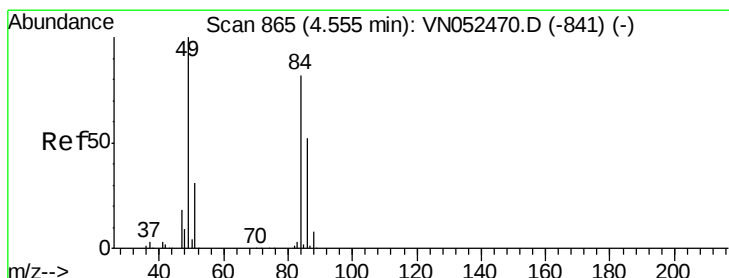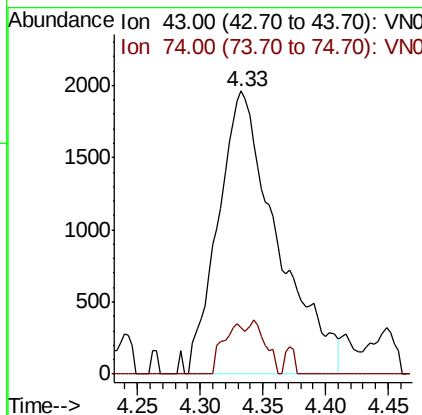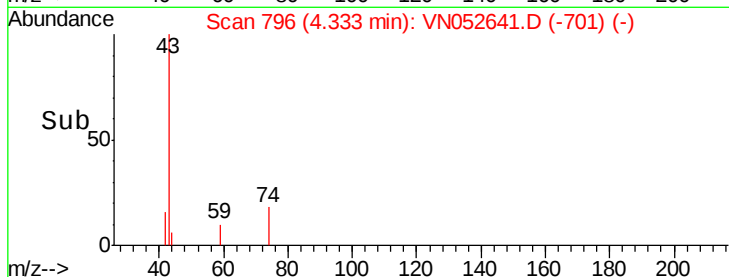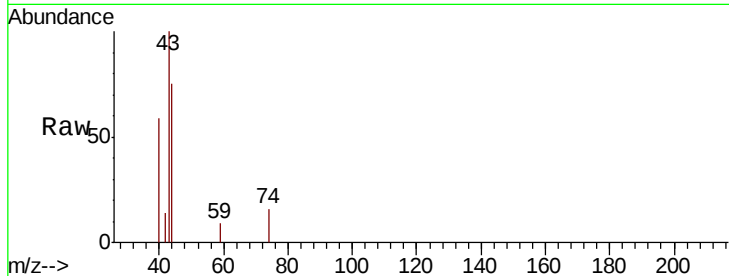

#20
Methylene Chloride
Concen: 11.976 ug/l
RT: 4.56 min Scan# 866
Delta R.T. 0.00 min
Lab File: VN052641.D
Acq: 3 Dec 2018 19:36

Tgt Ion: 84 Resp: 168009
Ion Ratio Lower Upper
84 100
49 119.8 98.0 147.0
51 37.6 30.1 45.1
86 64.6 50.7 76.1

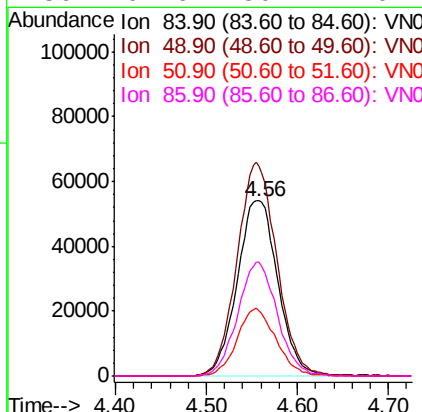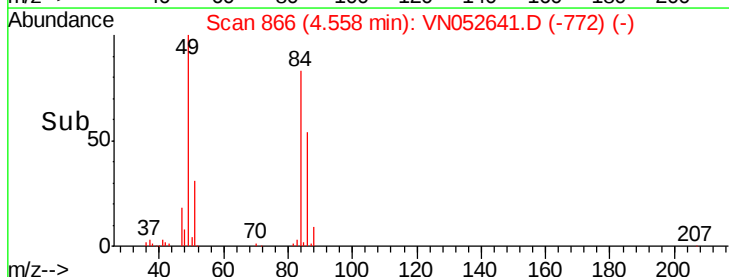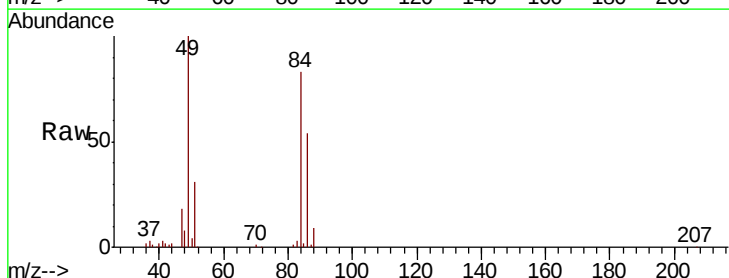



#25

2-Butanone

Concen: 0.419 ug/l

RT: 6.85 min Scan# 1579

Delta R.T. 0.02 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36

Instrument :

MSVOA_N

ClientSampleId :


PB115231ZHE#12

Tot Ion: 43 Resp: 2128

Ion Ratio Lower Upper

43 100

72 30.3 20.1 30.1#

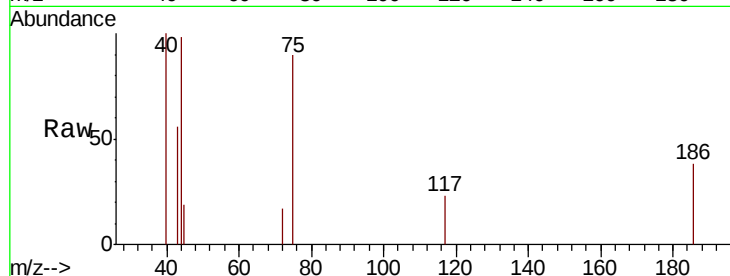

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

6.85

800



600

400

200

0

Time-->



#29

Tetrahydrofuran

Concen: 0.224 ug/l

RT: 7.21 min Scan# 1691

Delta R.T. -0.00 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36


Tgt Ion: 42 Resp: 735

Ion Ratio Lower Upper

42 100

72 53.3 33.3 49.9#

71 25.4 32.0 48.0#



Abundance Ion 42.00 (41.70 to 42.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

Ion 71.00 (70.70 to 71.70): VN0

800


600


400

200

0

Time-->




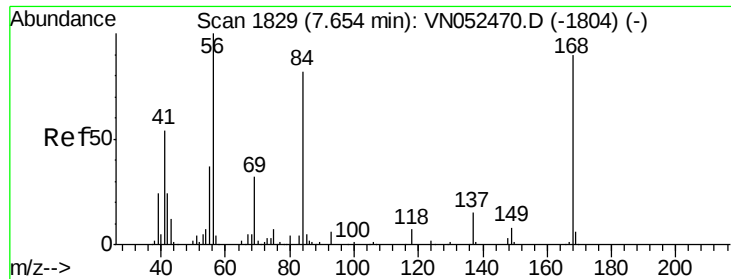




#31
Cyclohexane
Concen: 0.570 ug/l
RT: 7.67 min Scan# 1833
Delta R.T. 0.01 min
Lab File: VN052641.D
Acq: 3 Dec 2018 19:36

Instrument :
MSVOA_N
ClientSampleId :
PB115231ZHE#12

Tot Ion: 56 Resp: 21791
Ion Ratio Lower Upper
56 100
69 182.7 25.8 38.6#
84 158.2 65.3 97.9#

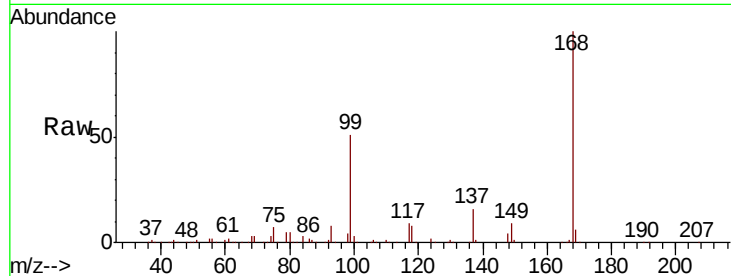


Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0

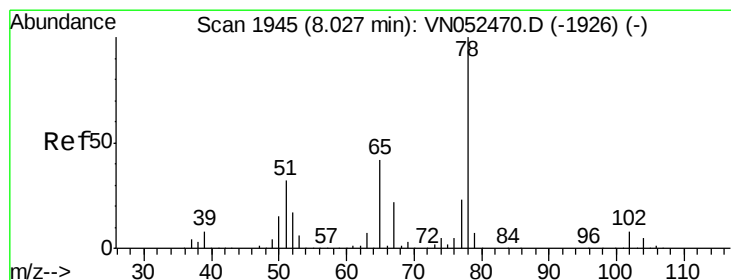
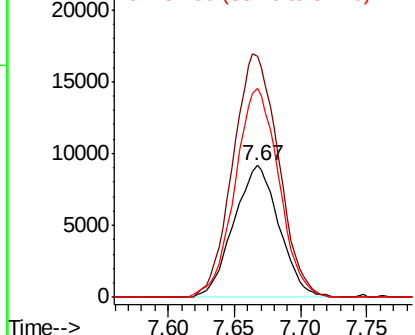



#33
1,2-Dichloroethane-d4
Concen: N.D. ug/l
RT: 8.03 min Scan# 1945
Delta R.T. -0.00 min
Lab File: VN052641.D
Acq: 3 Dec 2018 19:36

Tgt Ion: 65 Resp: 660859
Ion Ratio Lower Upper
65 100
67 54.6 0.0 109.8



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

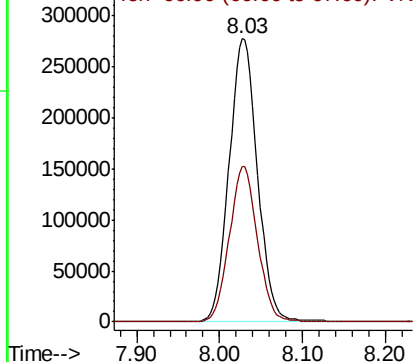

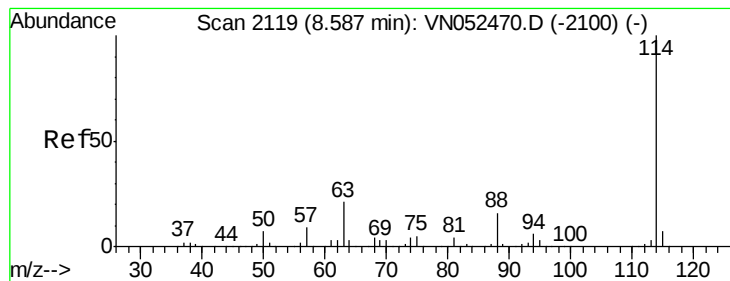

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. -0.00 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36

Instrument :

MSVOA_N

ClientSampleId :

PB115231ZHE#12


Tot Ion:114 Resp: 1933781

Ion Ratio Lower Upper

114 100

63 20.4 0.0 41.8




88 15.3 0.0 31.6



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

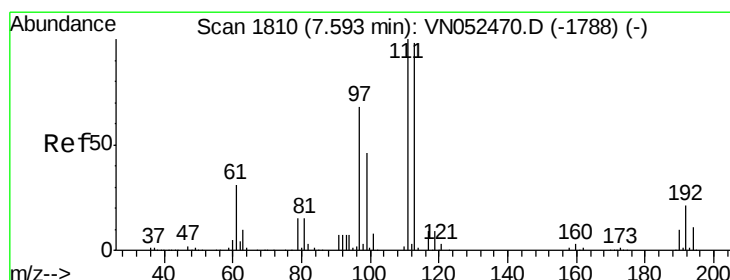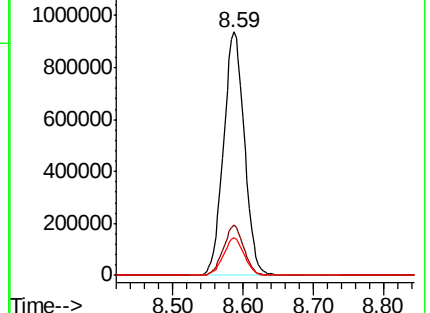

#35

Dibromofluoromethane

Concen: 50.000 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. -0.00 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36


Tgt Ion:113 Resp: 593917

Ion Ratio Lower Upper

113 100

111 102.4 82.0 123.0



192 22.2 17.0 25.6

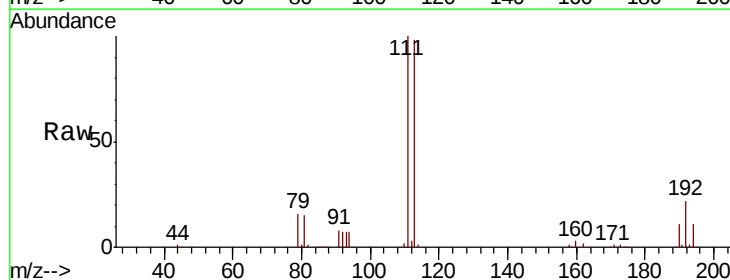


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

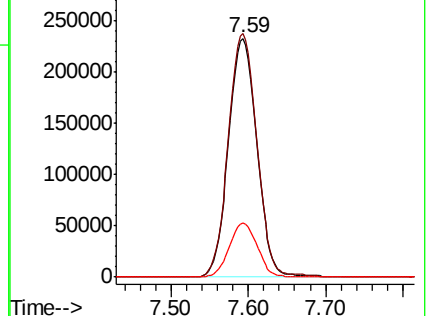


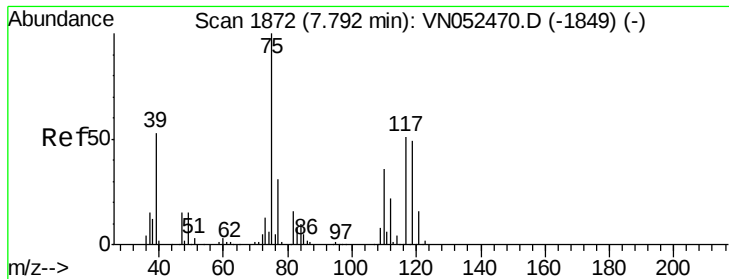

#36
 1,1-Dichloropropene
 Concen: 4.753 ug/l
 RT: 7.67 min Scan# 1833
 Delta R.T. -0.13 min
 Lab File: VN052641.D
 Acq: 3 Dec 2018 19:36

Instrument :
 MSVOA_N
 ClientSampleId :
 PB115231ZHE#12

Tot Ion	75	Resp	86802
Ion Ratio	100	Lower	Upper
110	8.3	17.5	52.6#
77	0.0	24.5	36.7#



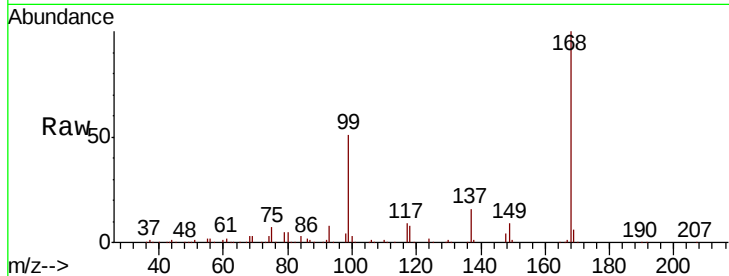


Abundance

Ion 74.90 (74.60 to 75.60): VN0


Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VN0

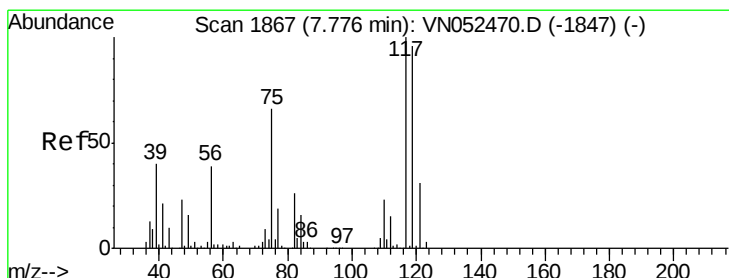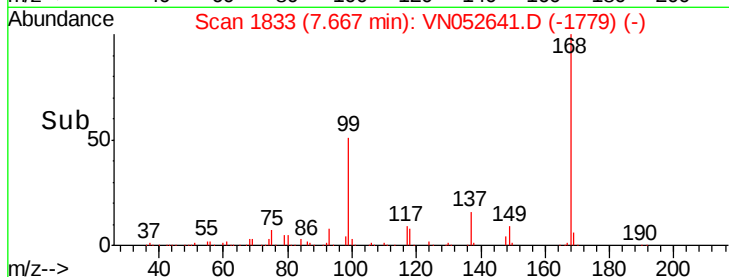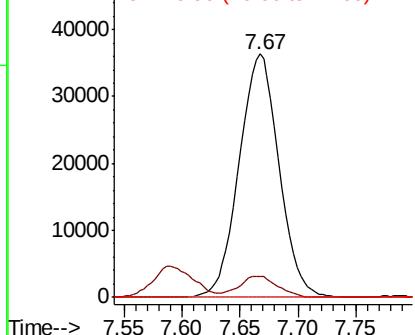

#38
 Carbon Tetrachloride
 Concen: 6.579 ug/l
 RT: 7.67 min Scan# 1833
 Delta R.T. -0.11 min
 Lab File: VN052641.D
 Acq: 3 Dec 2018 19:36

Tgt Ion	117	Resp	108752
Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td>	100	Lower	Upper
119	4.9	76.8	115.2#
121	0.0	24.9	37.3#


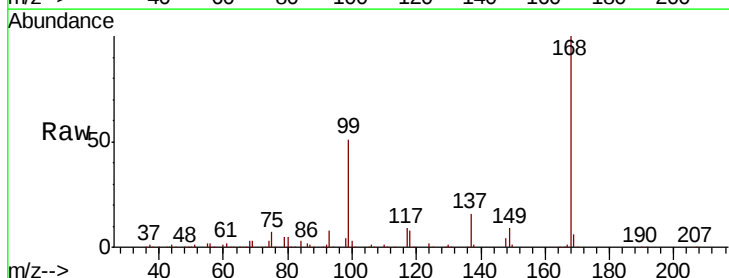



Abundance

Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

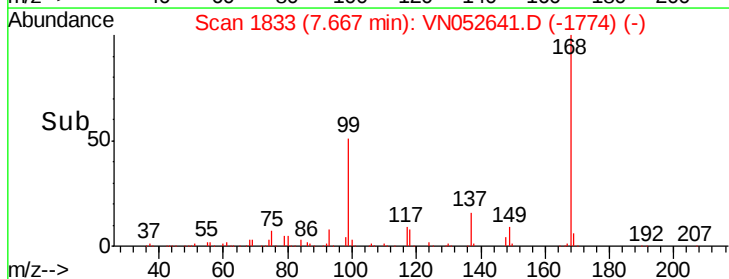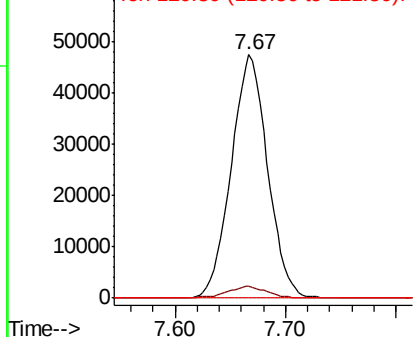

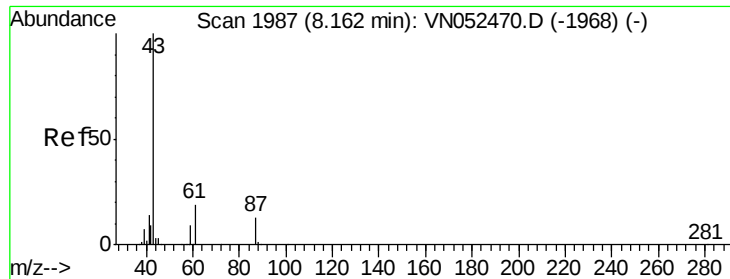

#43

Isopropyl Acetate

Concen: 3.729 ug/l

RT: 8.17 min Scan# 1989

Delta R.T. 0.01 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36

Instrument :

MSVOA_N

ClientSampleId :

PB115231ZHE#12


Tot Ion: 43 Resp: 70326

Ion Ratio Lower Upper

43 100

61 13.1 24.1 36.1#




87 8.4 10.6 15.8#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

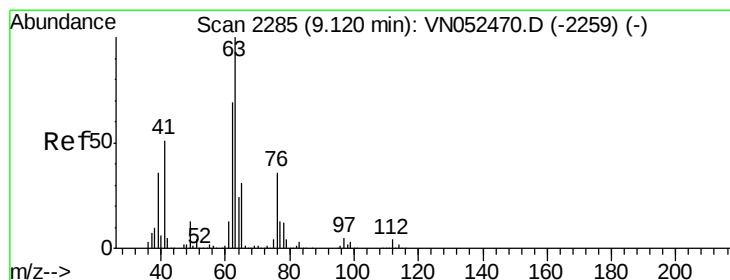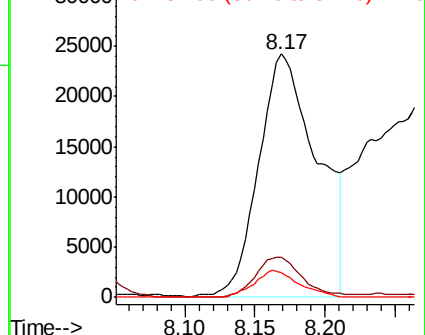

#45

1,2-Dichloropropane

Concen: 0.231 ug/l

RT: 9.27 min Scan# 2331

Delta R.T. 0.15 min

Lab File: VN052641.D


Acq: 3 Dec 2018 19:36

Tgt Ion: 63 Resp: 3344

Ion Ratio Lower Upper



63 100


65 0.0 25.0 37.6#

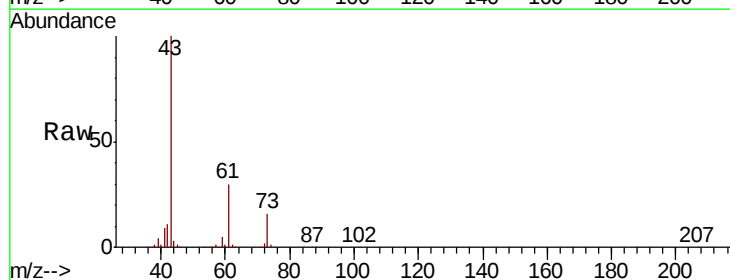

Abundance Ion 62.90 (62.60 to 63.60): VN0

Ion 64.90 (64.60 to 65.60): VN0




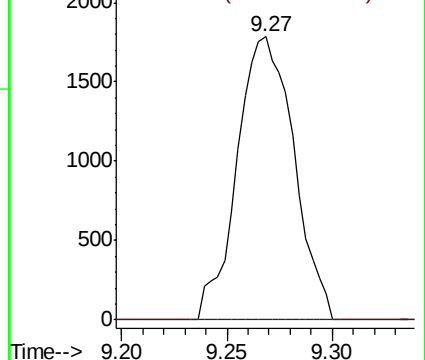




#48
Methvl methacrylate
Concen: 1.454 ug/l
RT: 9.18 min Scan# 2303
Delta R.T. -0.02 min
Lab File: VN052641.D
Acq: 3 Dec 2018 19:36




Instrument :
MSVOA_N
ClientSampleId :
PB115231ZHE#12


Tot Ion: 41 Resp: 14295
Ion Ratio Lower Upper
41 100
69 0.0 70.0 105.0#
39 0.0 42.6 64.0#

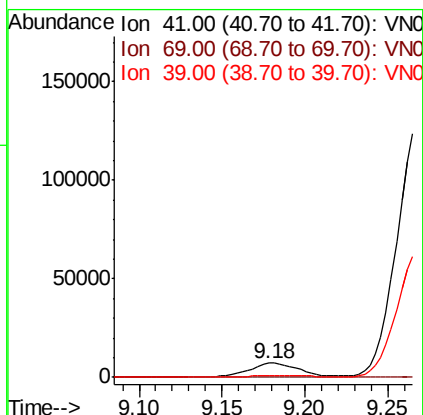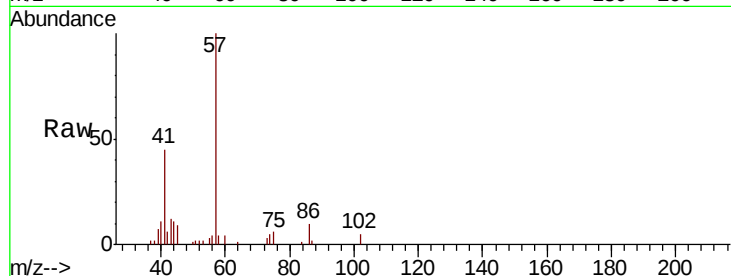

#49
1,4-Dioxane
Concen: 3.900 ug/l
RT: 9.27 min Scan# 2330
Delta R.T. 0.06 min
Lab File: VN052641.D
Acq: 3 Dec 2018 19:36

Tgt Ion: 88 Resp: 398
Ion Ratio Lower Upper
88 100
43 687533.4 26.4 39.6#
58 3141.7 55.4 83.0#

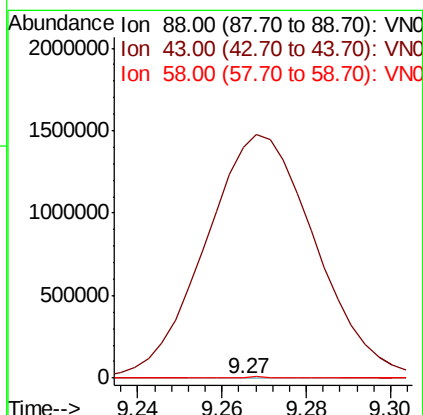



#50

Toluene-d8

Concen: 3.900 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36

Instrument :

MSVOA_N

ClientSampleId :





PB115231ZHE#12

Tot Ion: 98 Resp: 2356736

Ion Ratio Lower Upper

98 100

100 64.2 51.3 76.9

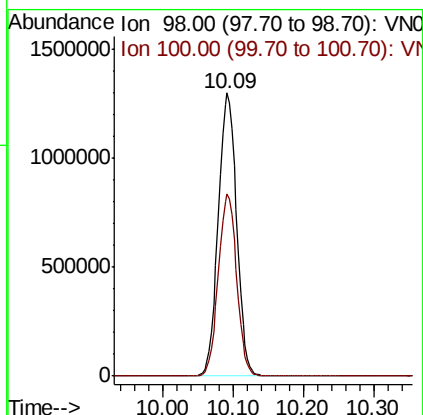

#51

4-Methyl-2-Pentanone

Concen: 1.476 ug/l

RT: 10.03 min Scan# 2567

Delta R.T. 0.04 min

Lab File: VN052641.D




Acq: 3 Dec 2018 19:36


Tgt Ion: 43 Resp: 15618

Ion Ratio Lower Upper

43 100

58 0.0 31.5 47.3#

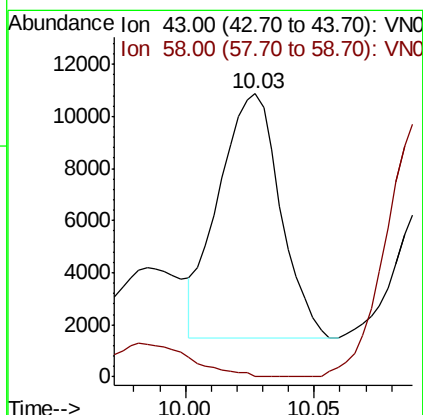



#54

cis-1,3-Dichloropropene

Concen: 6.349 ug/l

RT: 9.90 min Scan# 2529

Delta R.T. 0.06 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36

Instrument :

MSVOA_N

ClientSampleId :

PB115231ZHE#12





Tot Ion: 75 Resp: 127471

Ion Ratio Lower Upper

75 100

77 0.6 26.2 39.2#

39 29.0 36.0 54.0#

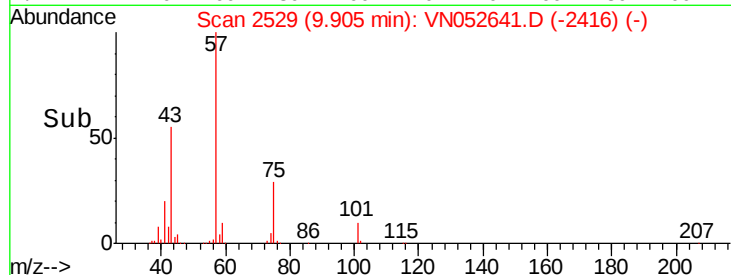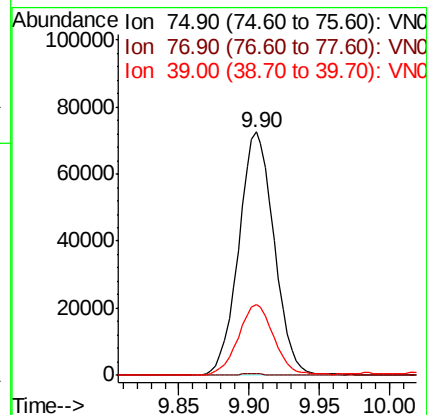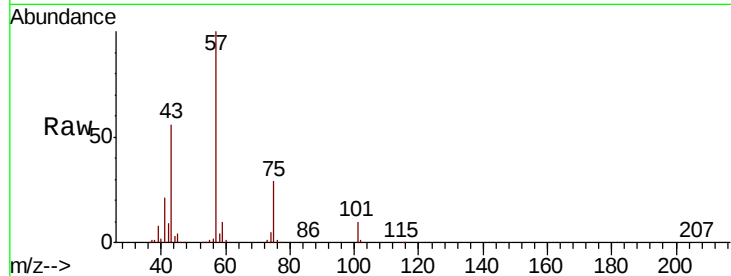

#56

Ethyl methacrylate

Concen: 2.782 ug/l

RT: 10.54 min Scan# 2727

Delta R.T. 0.11 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36




Tgt Ion: 69 Resp: 1487


Ion Ratio Lower Upper

69 100

41 6619.0 52.6 79.0#

39 2711.3 25.9 38.9#



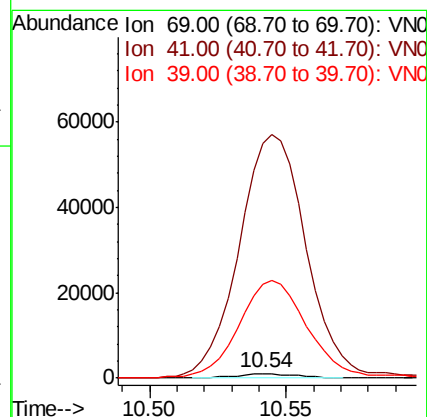
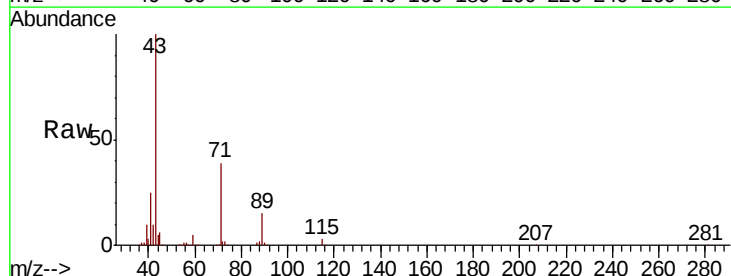




#57
 1,3-Dichloropropane
 Concen: 1.299 ug/l
 RT: 10.77 min Scan# 2797
 Delta R.T. 0.06 min
 Lab File: VN052641.D
 Acq: 3 Dec 2018 19:36




Instrument :
 MSVOA_N
 ClientSampleId :
 PB115231ZHE#12


Tot Ion: 76 Resp: 26089
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.6 38.4#

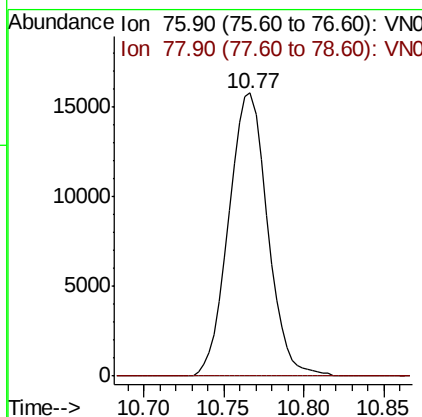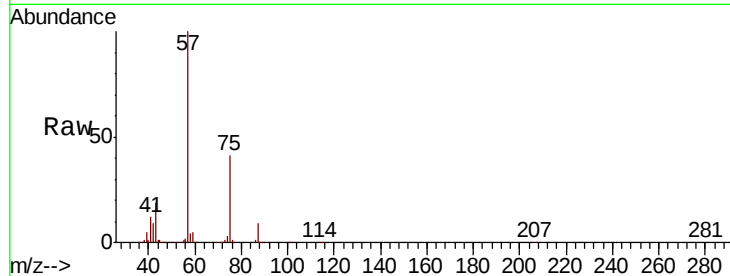

#59
 2-Hexanone
 Concen: 50.528 ug/l
 RT: 10.77 min Scan# 2797
 Delta R.T. 0.01 min
 Lab File: VN052641.D
 Acq: 3 Dec 2018 19:36

Tgt Ion: 43 Resp: 358852
 Ion Ratio Lower Upper
 43 100
 58 19.8 27.4 82.0#

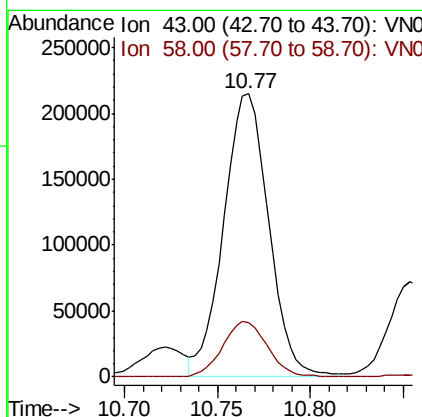



#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36

Instrument :

MSVOA_N

ClientSampleId :

PB115231ZHE#12


Tot Ion: 95 Resp: 747451

Ion Ratio Lower Upper

95 100

174 88.4 0.0 173.0

176 85.7 0.0 166.2

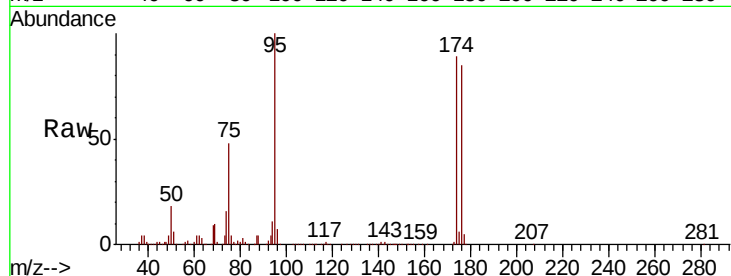



Abundance Ion 94.90 (94.60 to 95.60): VN052470.D (-3291) (-)

Ion 173.80 (173.50 to 174.50): VN052470.D (-3291) (-)

Ion 175.80 (175.50 to 176.50): VN052470.D (-3291) (-)

12.40

Time-->



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2997

Delta R.T. -0.00 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36


Tgt Ion: 117 Resp: 1715760

Ion Ratio Lower Upper

117 100

82 53.5 43.6 65.4

119 32.0 25.4 38.2




Abundance Ion 116.90 (116.60 to 117.60): VN052470.D (-2980) (-)


Ion 82.00 (81.70 to 82.70): VN052470.D (-2980) (-)

Ion 118.90 (118.60 to 119.60): VN052470.D (-2980) (-)

11.41

Time-->





#71

Bromoform

Concen: 0.560 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.28 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36

Instrument :

MSVOA_N

ClientSampleId :

PB115231ZHE#12


Tot Ion:173 Resp: 4562

Ion Ratio Lower Upper

173 100

175 888.5 24.4 73.2#




254 0.0 0.1 0.1#



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

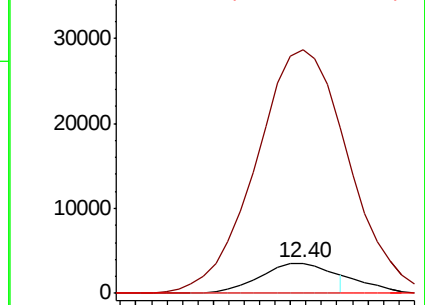

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3599

Delta R.T. -0.00 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36


Tgt Ion:152 Resp: 663546

Ion Ratio Lower Upper

152 100

115 55.8 28.4 85.2



150 155.7 0.0 346.0




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

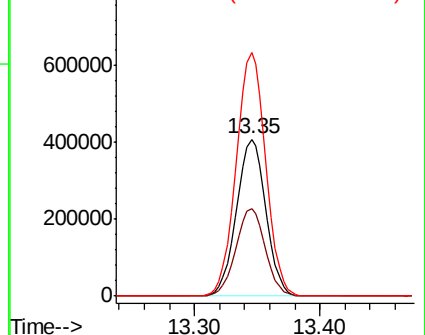



#74

N-amvl acetate

Concen: 3.180 ug/l

RT: 11.88 min Scan# 3143

Delta R.T. -0.19 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36

Instrument :

MSVOA_N

ClientSampleId :

PB115231ZHE#12

Tot Ion: 43 Resp: 41824


Ion Ratio Lower Upper

43 100

70 1.8 33.8 50.8#

55 4.6 20.0 30.0#

61 10.8 19.7 29.5#

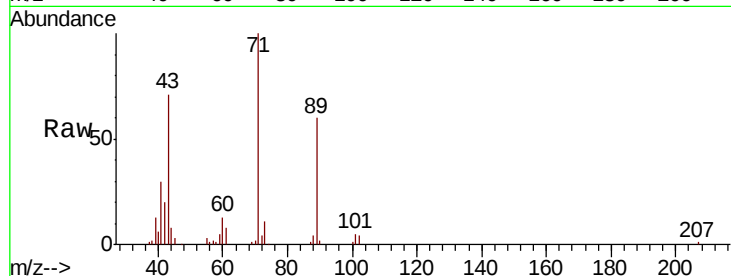




Abundance

Ion 43.00 (42.70 to 43.70): VNO

Ion 70.00 (69.70 to 70.70): VNO

Ion 55.00 (54.70 to 55.70): VNO

Ion 61.00 (60.70 to 61.70): VNO

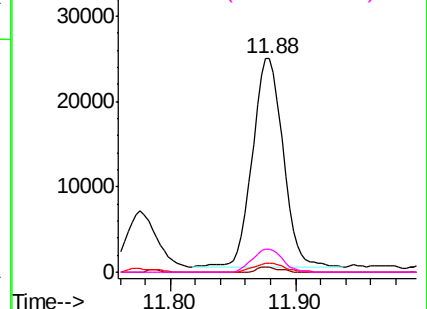

#76

1,2,3-Trichloropropane

Concen: 34.952 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. -0.15 min

Lab File: VN052641.D


Acq: 3 Dec 2018 19:36

Tgt Ion: 75 Resp: 357636

Ion Ratio Lower Upper

75 100



77 1.2 0.0 0.0#




Abundance

Ion 74.90 (74.60 to 75.60): VNO

Ion 77.00 (76.70 to 77.70): VNO

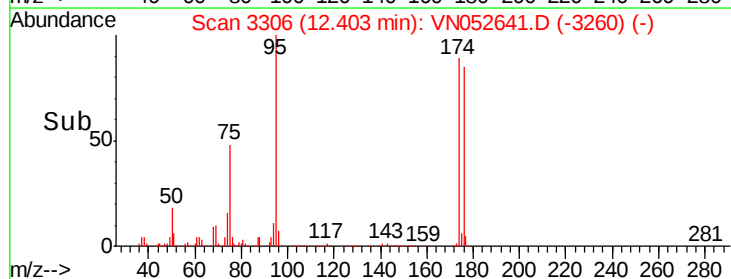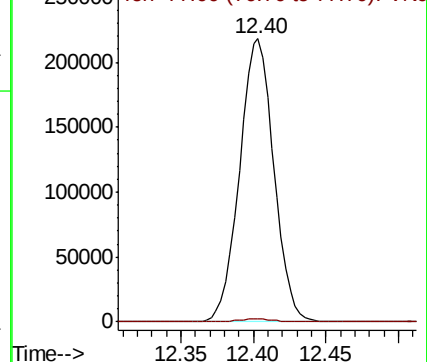

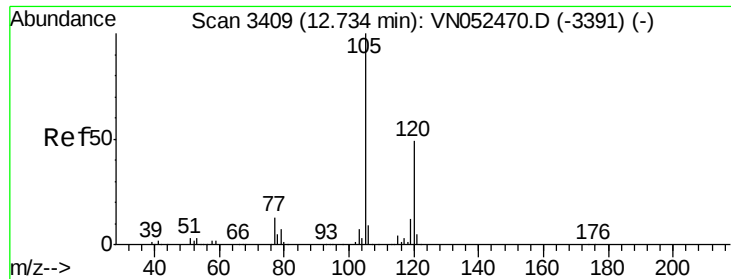

#80

1,3,5-Trimethylbenzene

Concen: 0.687 ug/l

RT: 12.73 min Scan# 3409

Delta R.T. -0.00 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36

Instrument :

MSVOA_N

ClientSampleId :


PB115231ZHE#12

Tot Ion:105 Resp: 28511

Ion Ratio Lower Upper

105 100

120 47.9 24.3 73.0

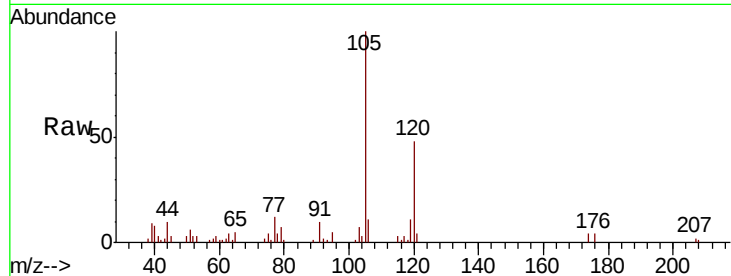

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

12.73

15000



10000

5000

0

12.70 12.75 12.80

Time-->



#81

trans-1,4-Dichloro-2-butene

Concen: 116.723 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.10 min

Lab File: VN052641.D

Acq: 3 Dec 2018 19:36


Tgt Ion: 75 Resp: 357636

Ion Ratio Lower Upper

75 100

53 0.0 77.4 116.0#

89 0.0 35.4 53.2#



Abundance Ion 74.90 (74.60 to 75.60): VNO

Ion 53.00 (52.70 to 53.70): VNO

Ion 88.90 (88.60 to 89.60): VNO

300000

250000

200000

150000


100000


50000

0

12.35 12.40 12.45

Time-->




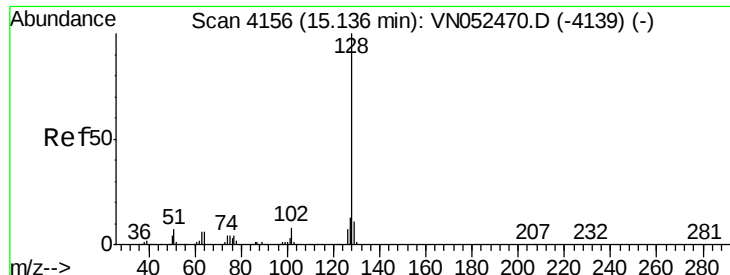

#95
Naphthalene
Concen: 3.443 ug/l
RT: 15.14 min Scan# 4156
Delta R.T. 0.00 min
Lab File: VN052641.D
Acq: 3 Dec 2018 19:36

Instrument :
MSVOA_N
ClientSampleId :
PB115231ZHE#12

Tot Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.2	15.2#
129	0.0	8.7	13.1#

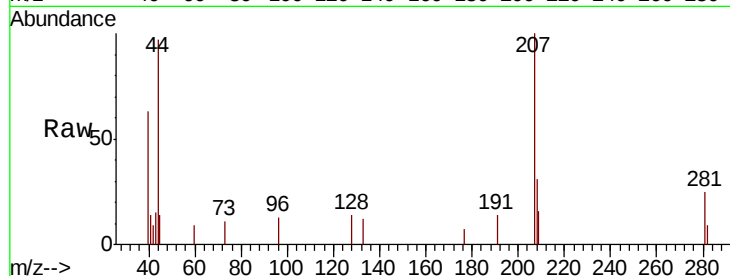

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

