


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN120318\  
Data File : VN052618.D  
Acq On : 3 Dec 2018 8:48  
Operator : MD\SY  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 1 Sample Multiplier: 28

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N112718W.M  
Title : SW846 8260  
Last Update : Mon Dec 03 03:24:02 2018

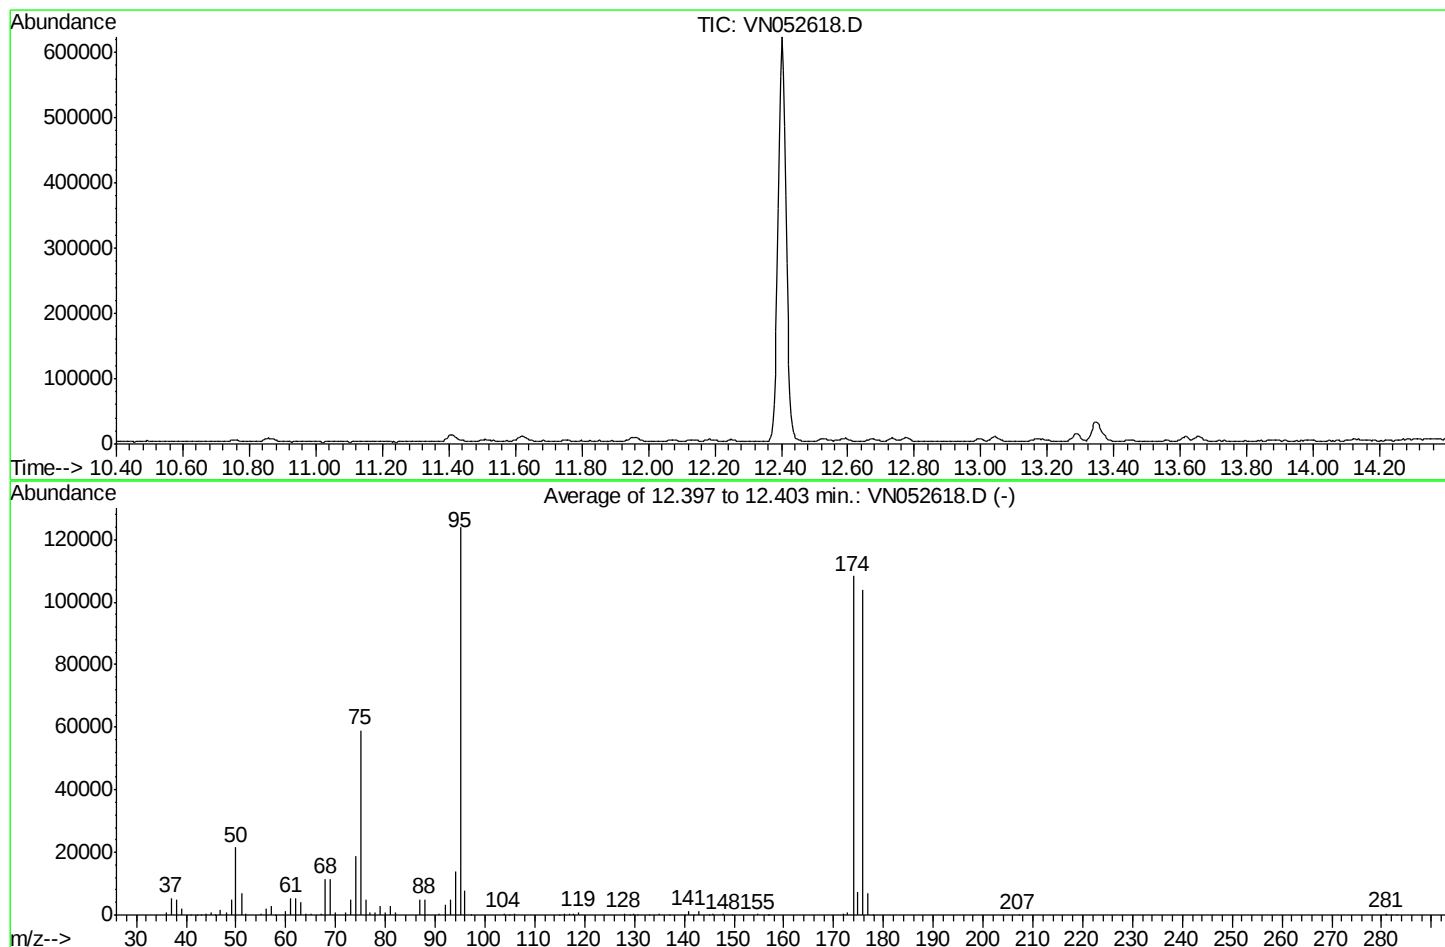

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.4      | 21578   | PASS             |
| 75          | 95           | 30           | 60           | 47.6      | 58957   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 123866  | PASS             |
| 96          | 95           | 5            | 9            | 6.3       | 7790    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.9       | 927     | PASS             |
| 174         | 95           | 50           | 100          | 87.4      | 108250  | PASS             |
| 175         | 174          | 5            | 9            | 6.9       | 7466    | PASS             |
| 176         | 174          | 95           | 101          | 96.1      | 104008  | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 7036    | PASS             |