



Methylene Chloride

Response Ratio

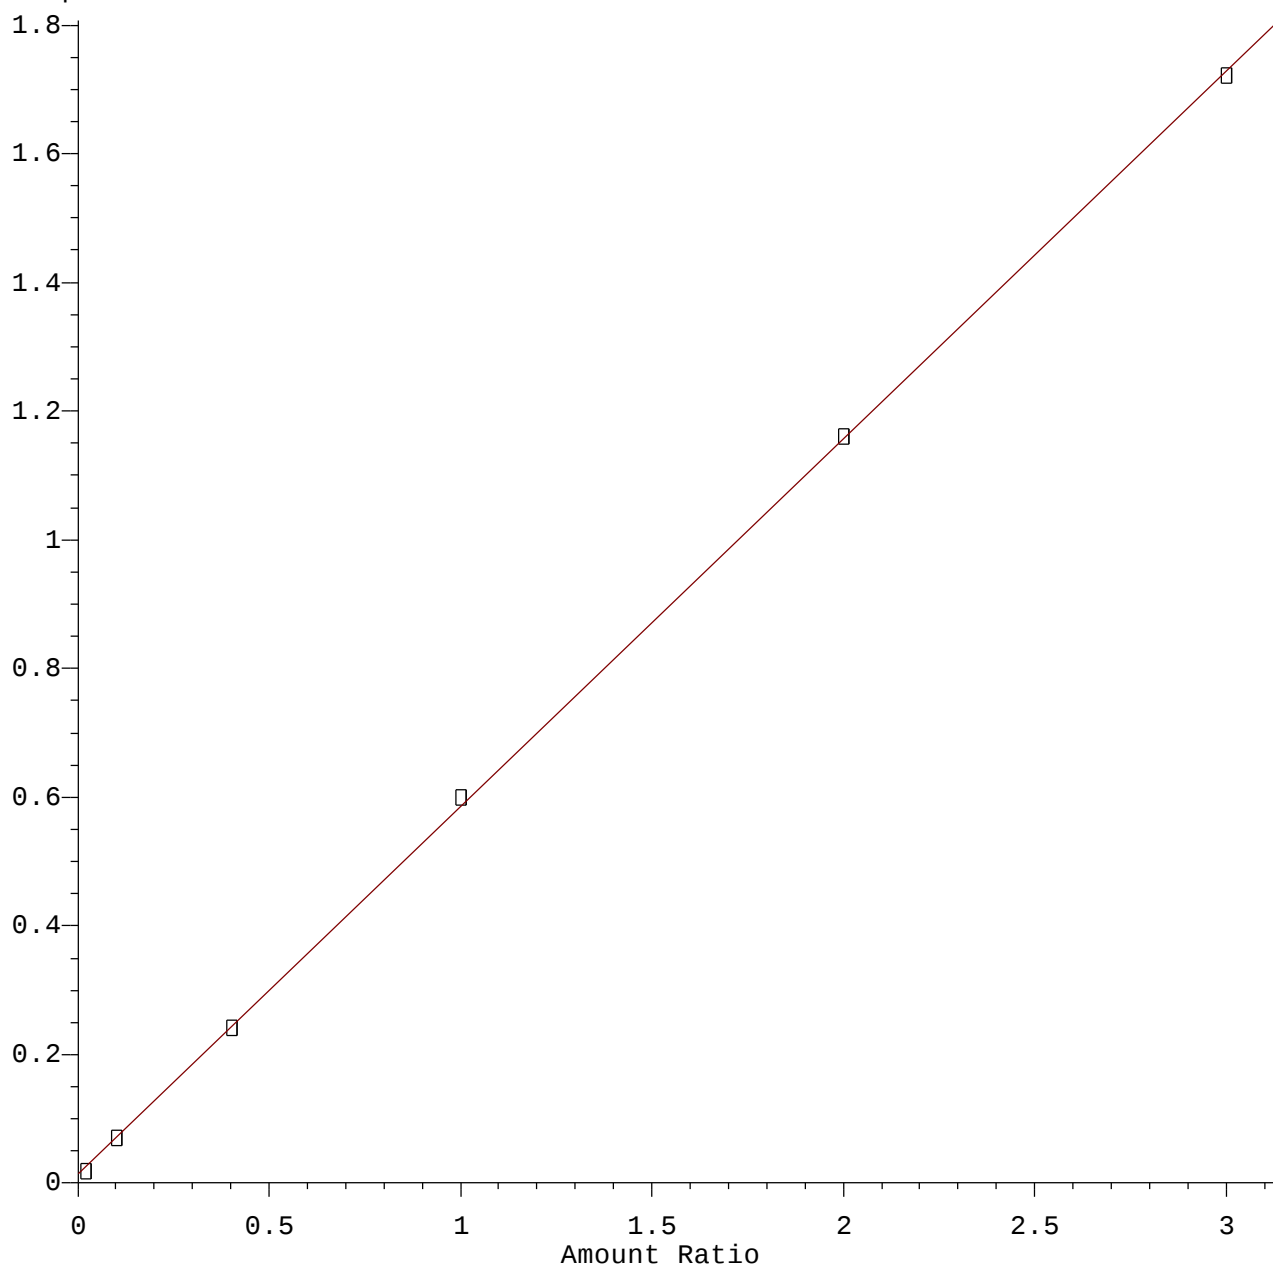

Resp Ratio = 5.71e-001 * Amt + 1.40e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Calibration Table Last Updated: Tue Dec 03 16:37:42 2019

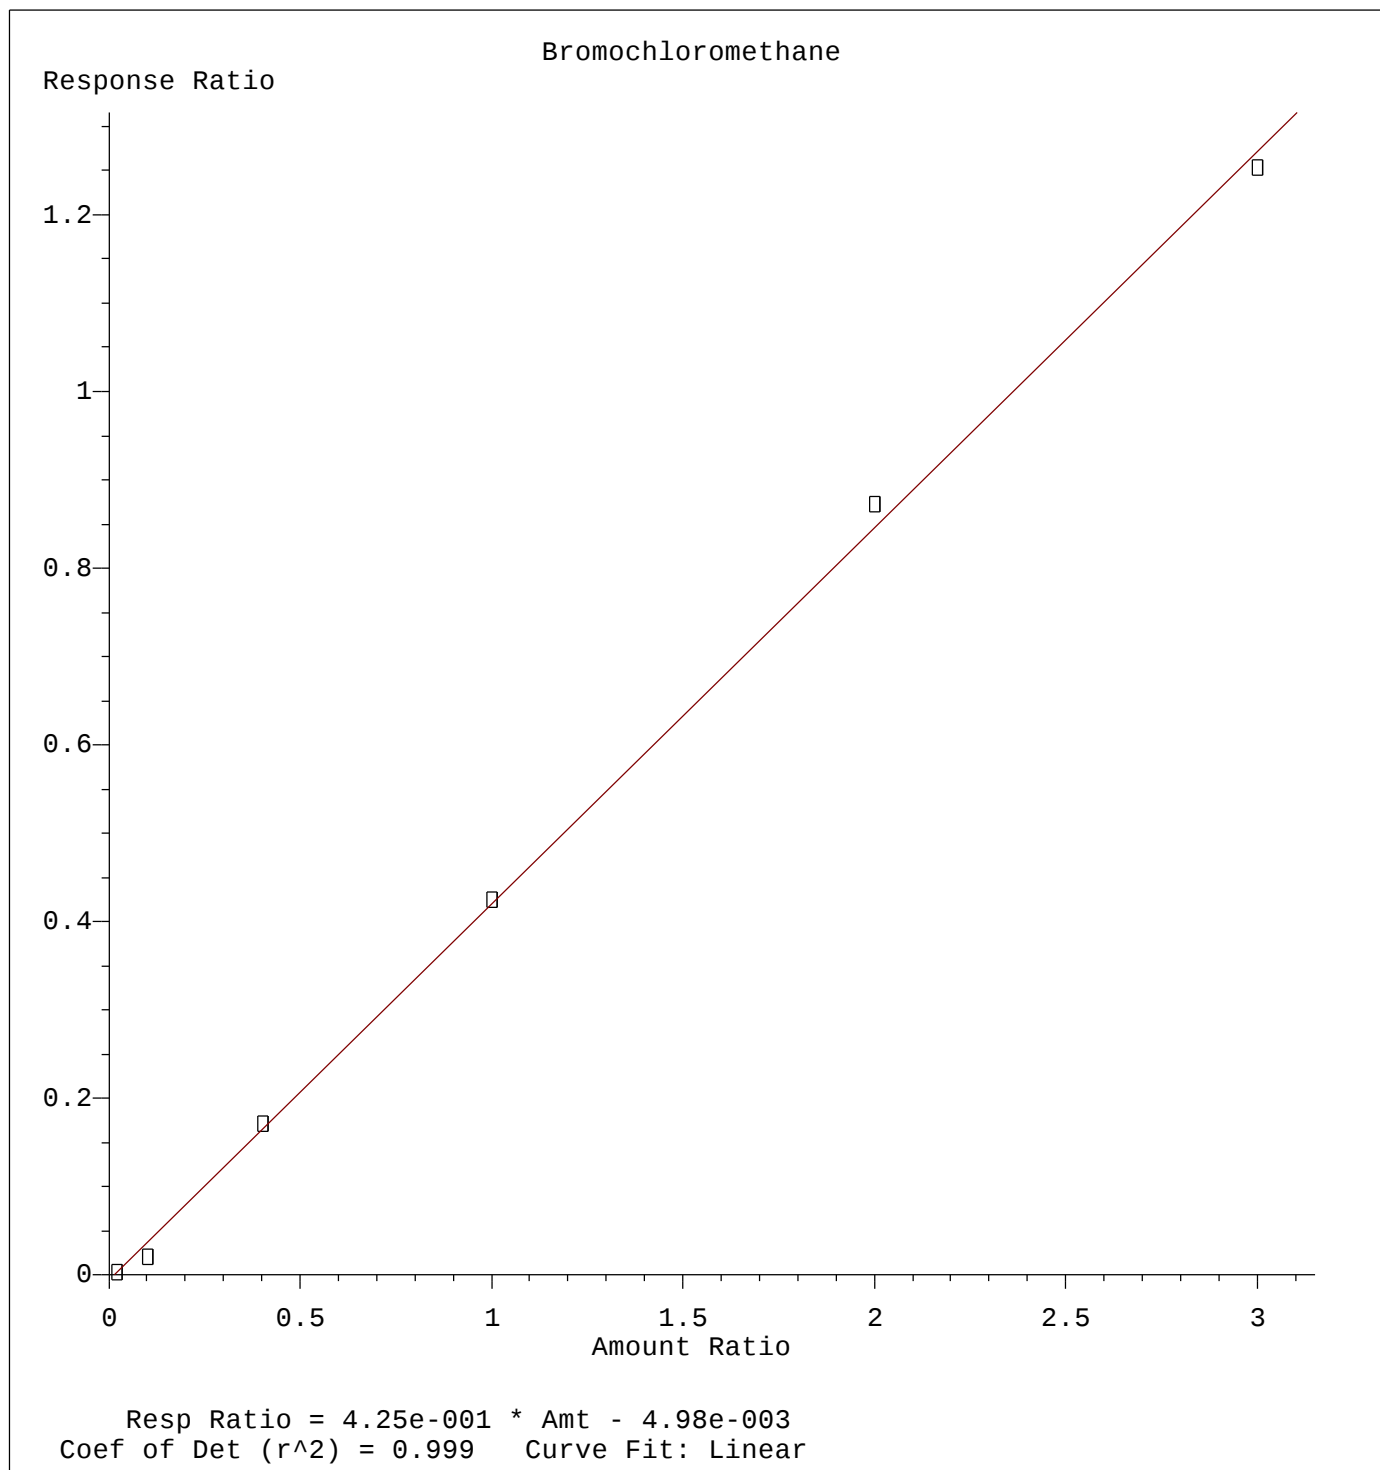

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Calibration Table Last Updated: Tue Dec 03 16:37:42 2019

Ethyl methacrylate

Response Ratio

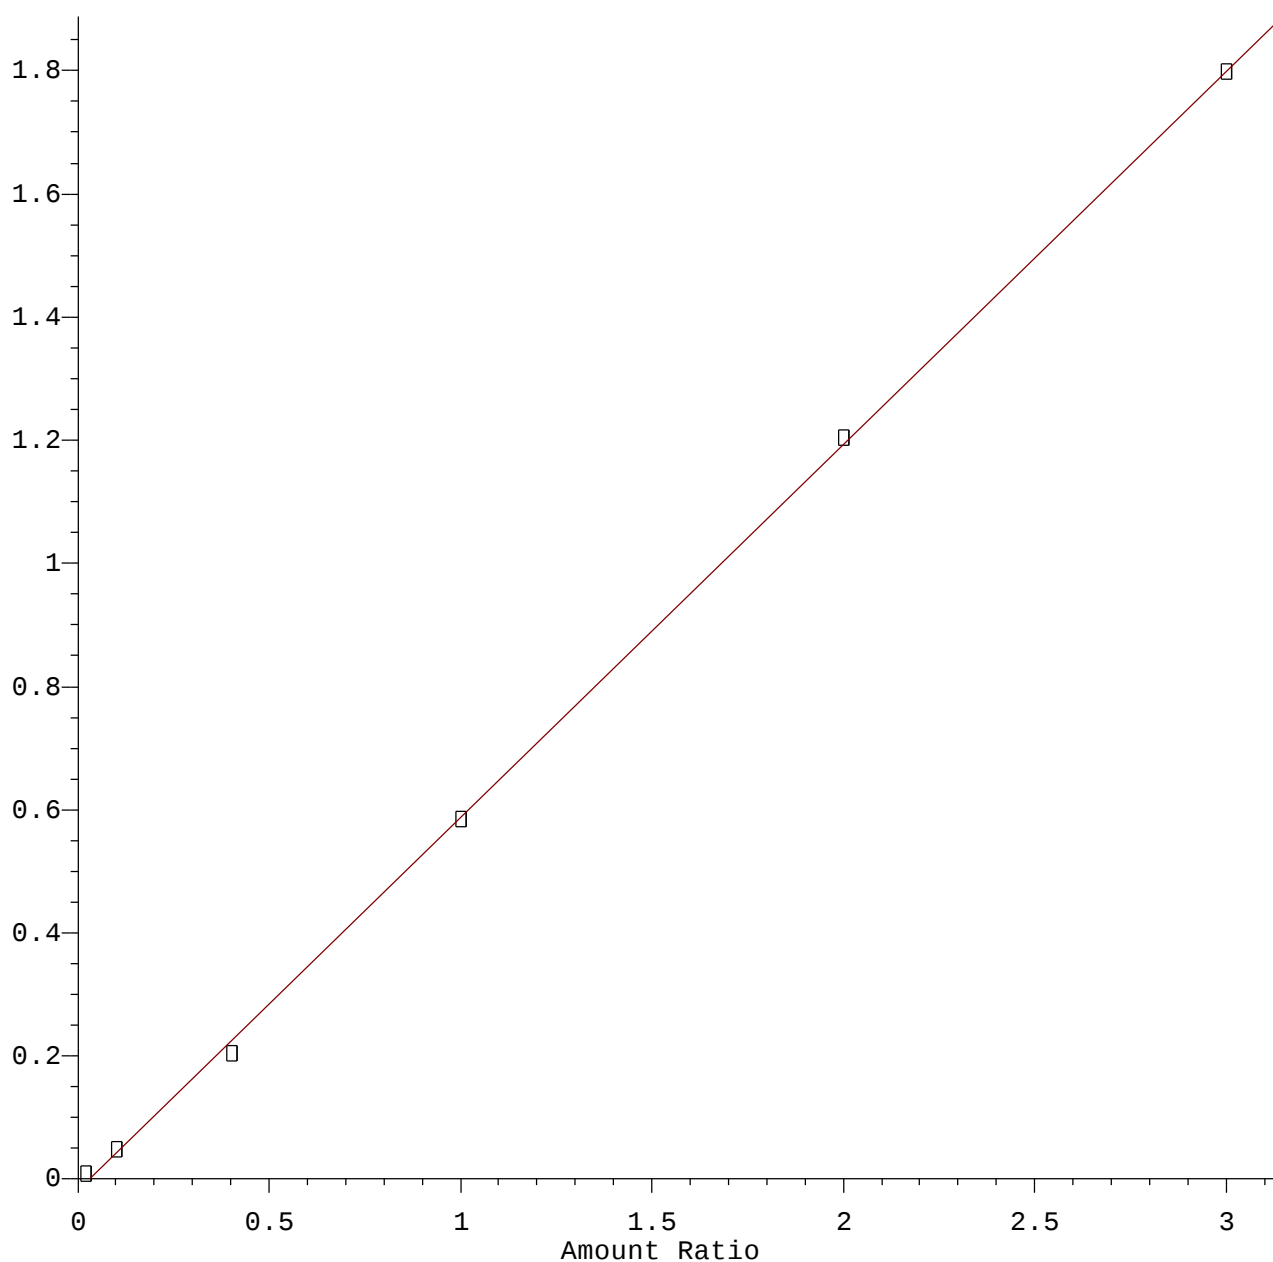


Resp Ratio = 6.06e-001 * Amt - 1.76e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Calibration Table Last Updated: Tue Dec 03 16:37:42 2019

2-Chloroethyl Vinyl ether

Response Ratio

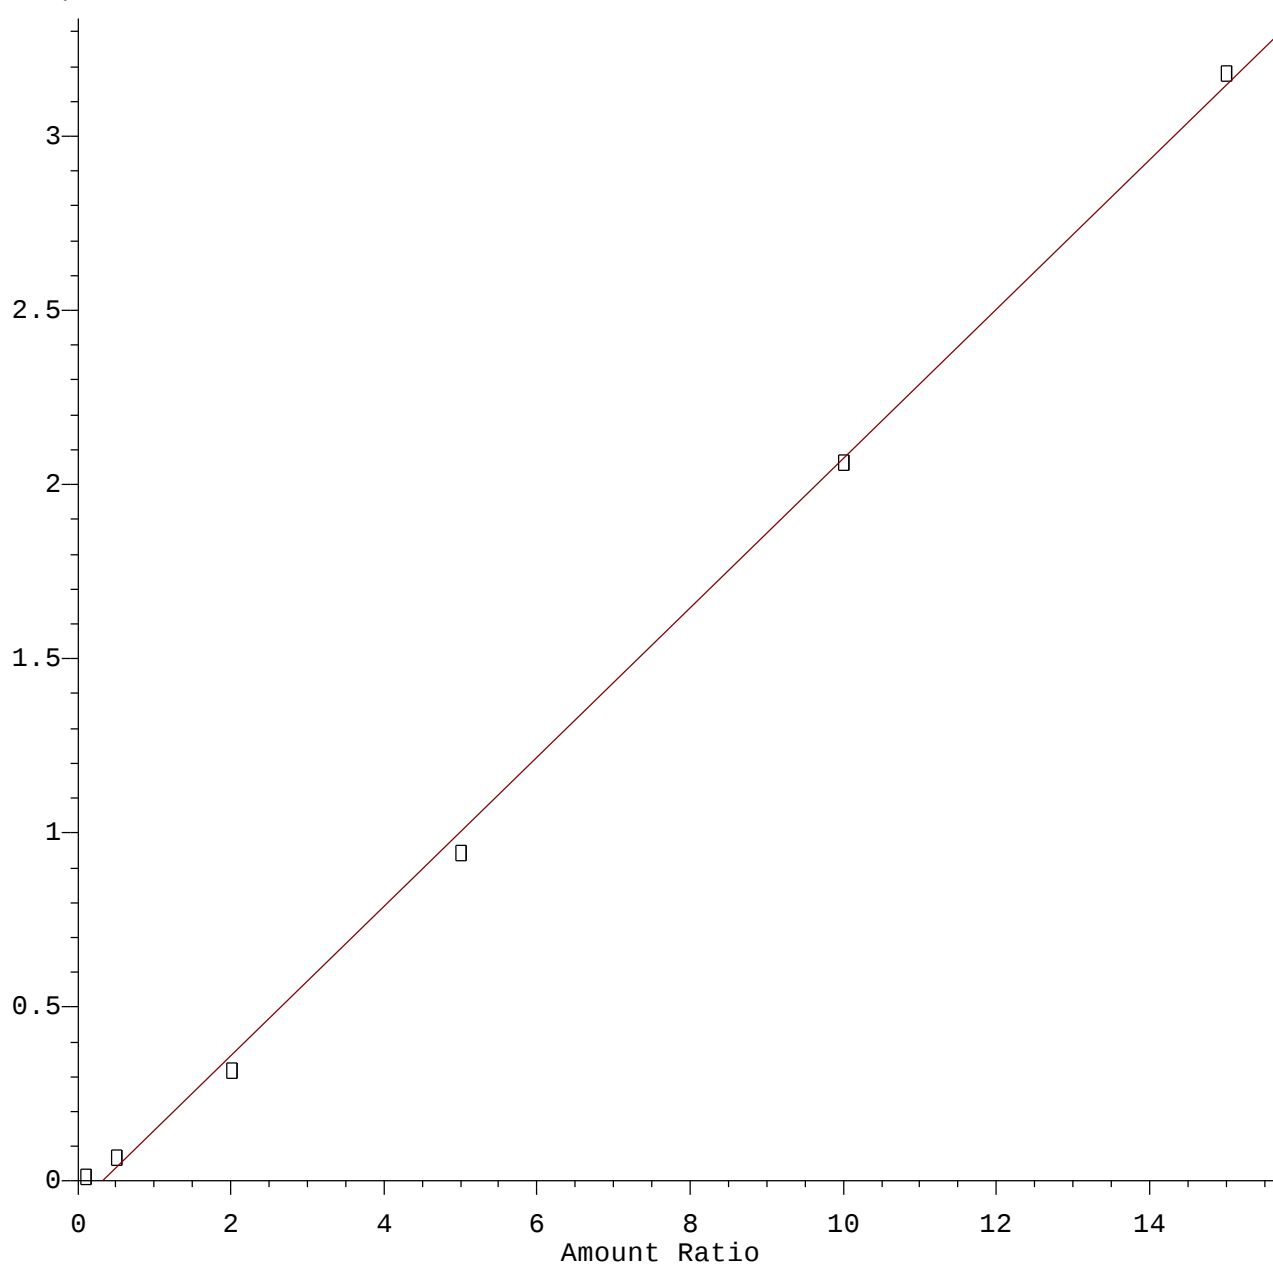


Resp Ratio = $2.14 \times 10^{-1} \times \text{Amt} - 6.77 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Calibration Table Last Updated: Tue Dec 03 16:37:42 2019


1,2-Dibromo-3-Chloropropane

Response Ratio

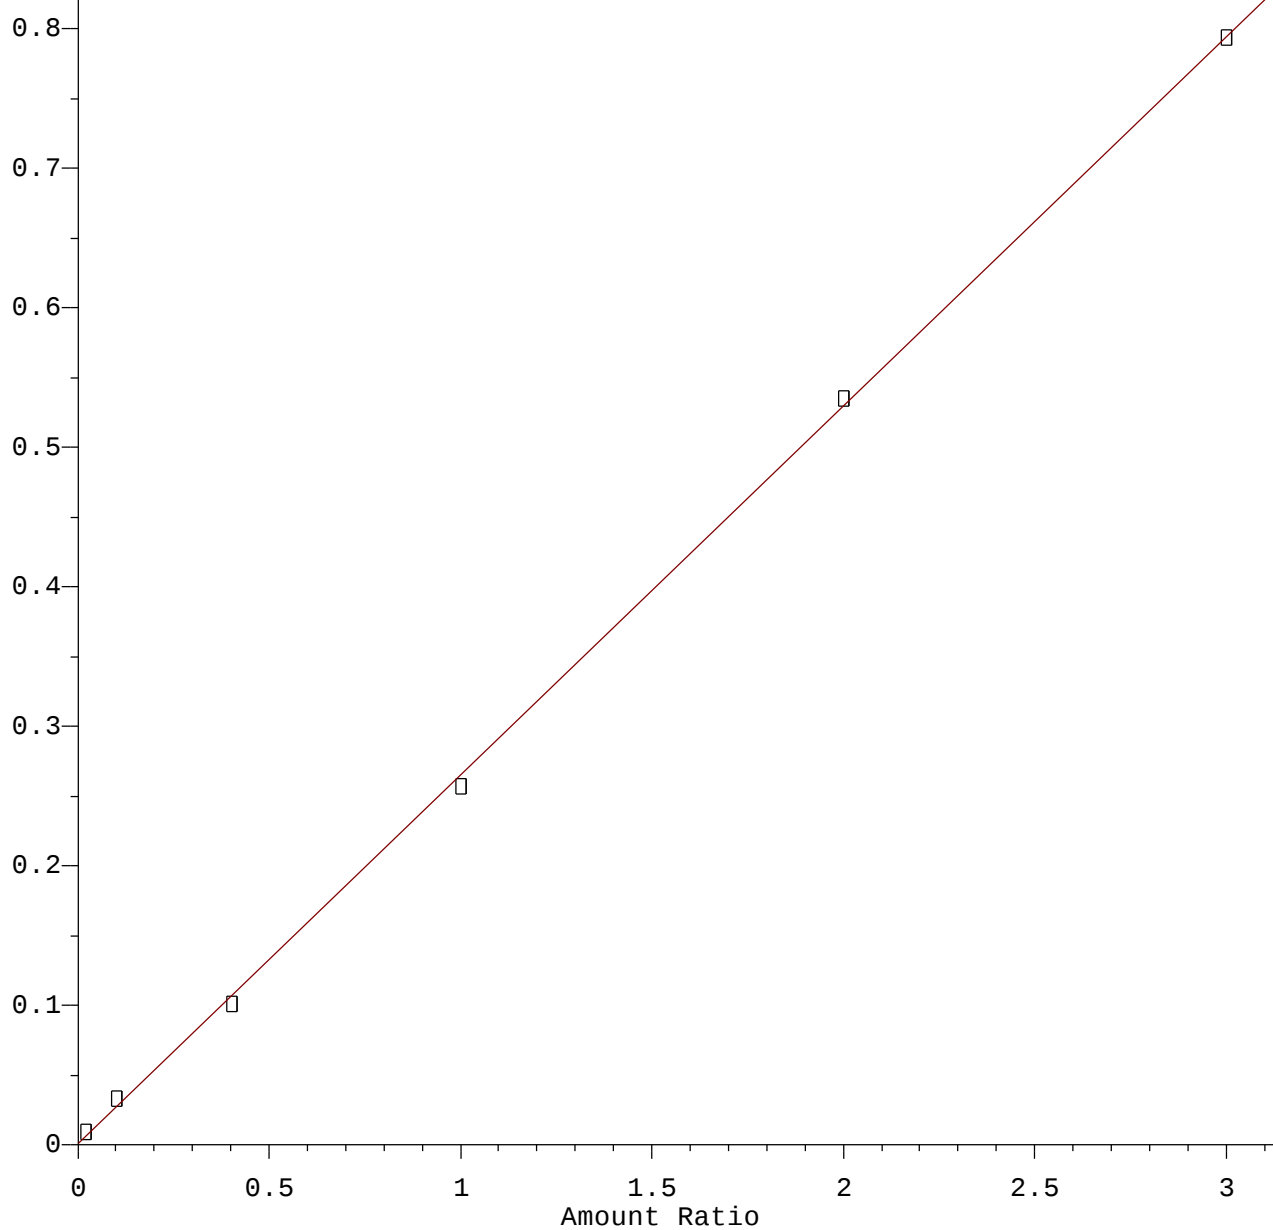


Resp Ratio = $2.65 \times 10^{-1} \times \text{Amt} + 6.96 \times 10^{-4}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Calibration Table Last Updated: Tue Dec 03 16:37:42 2019

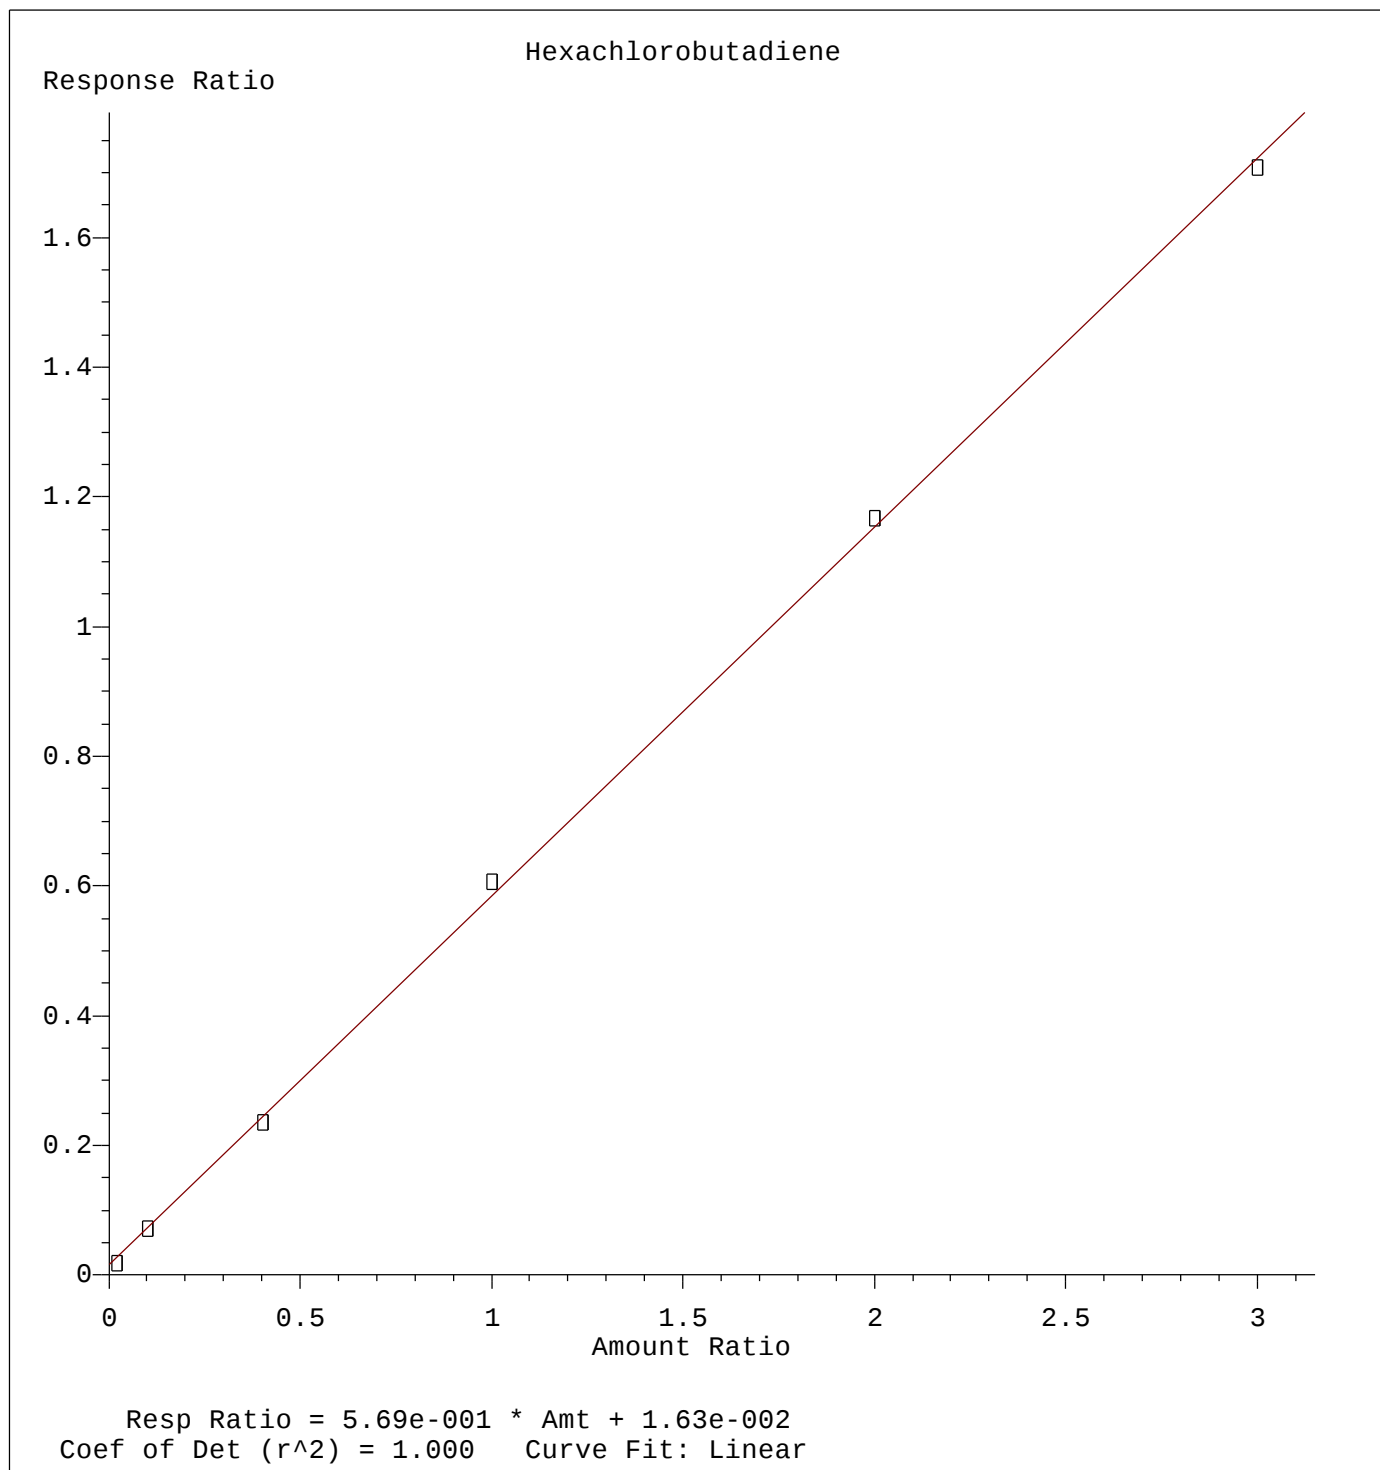


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Calibration Table Last Updated: Tue Dec 03 16:37:42 2019

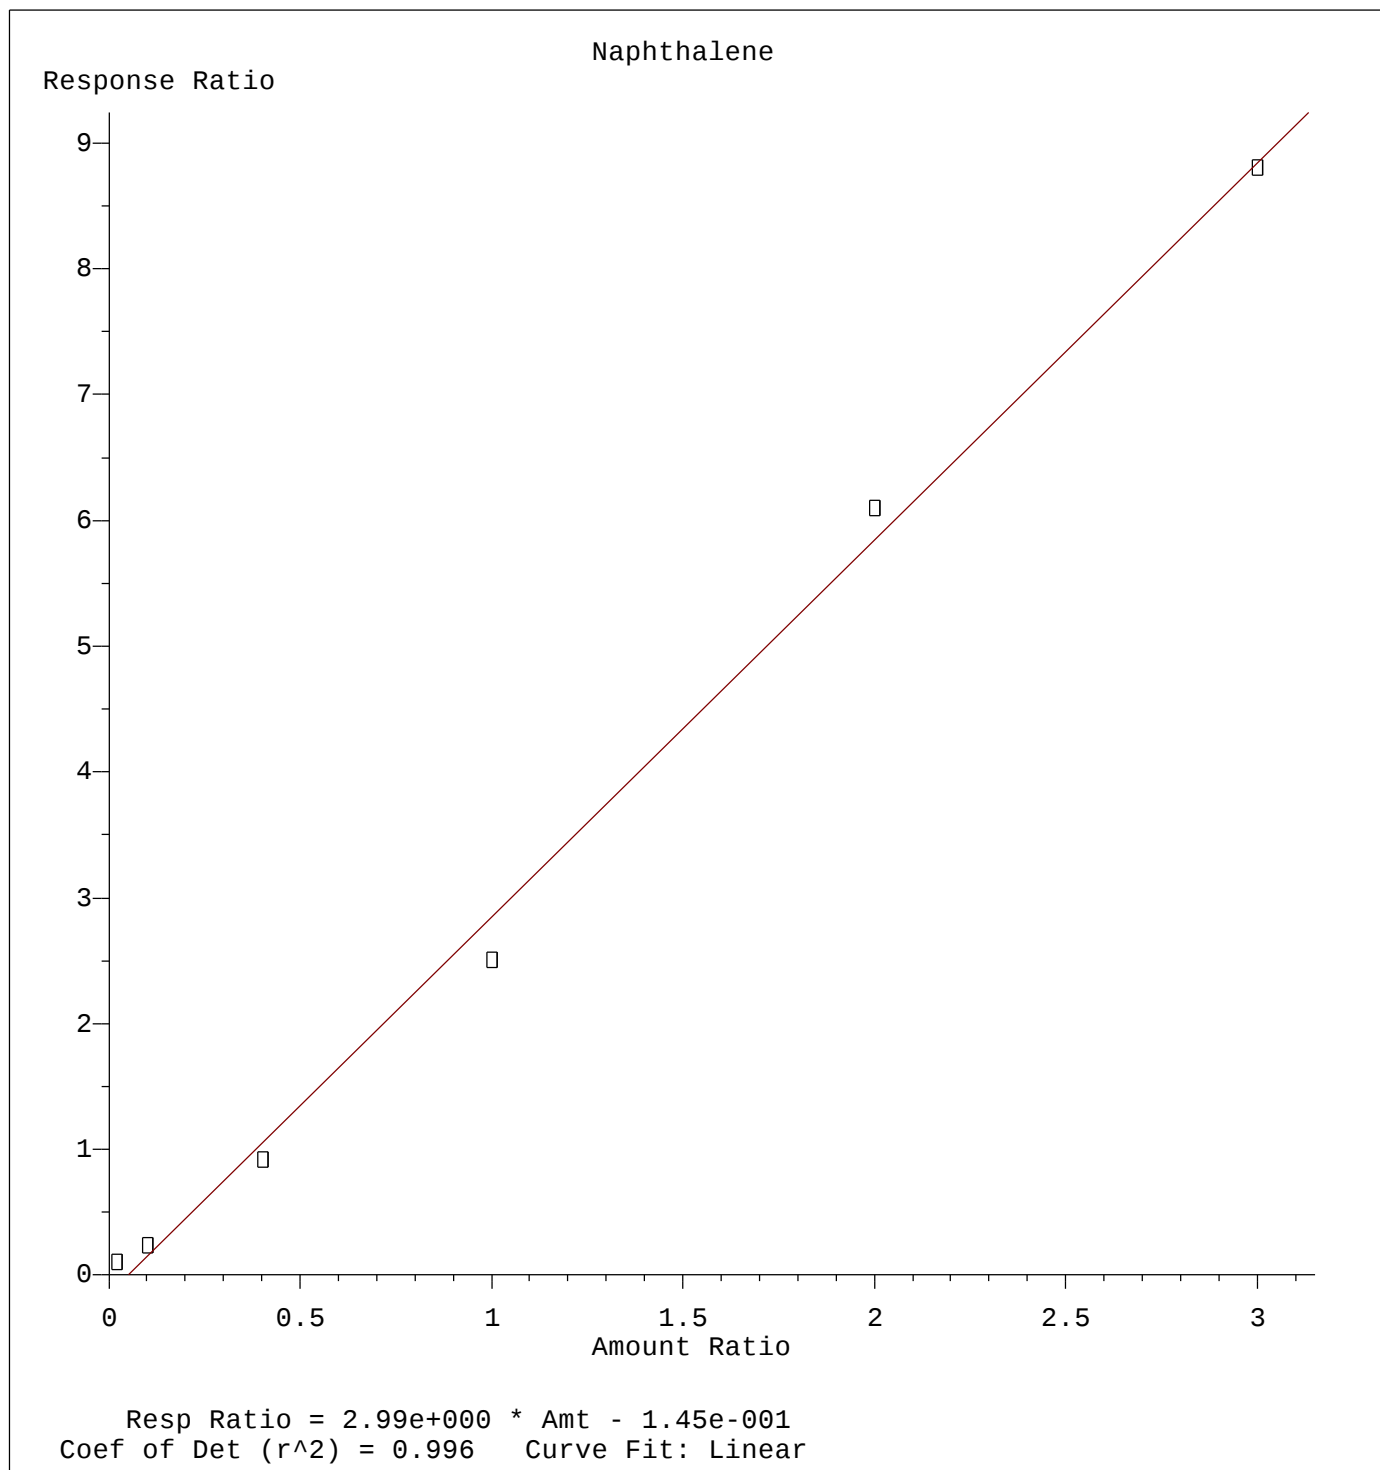

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Calibration Table Last Updated: Tue Dec 03 16:37:42 2019


1,2,3-Trichlorobenzene

Response Ratio

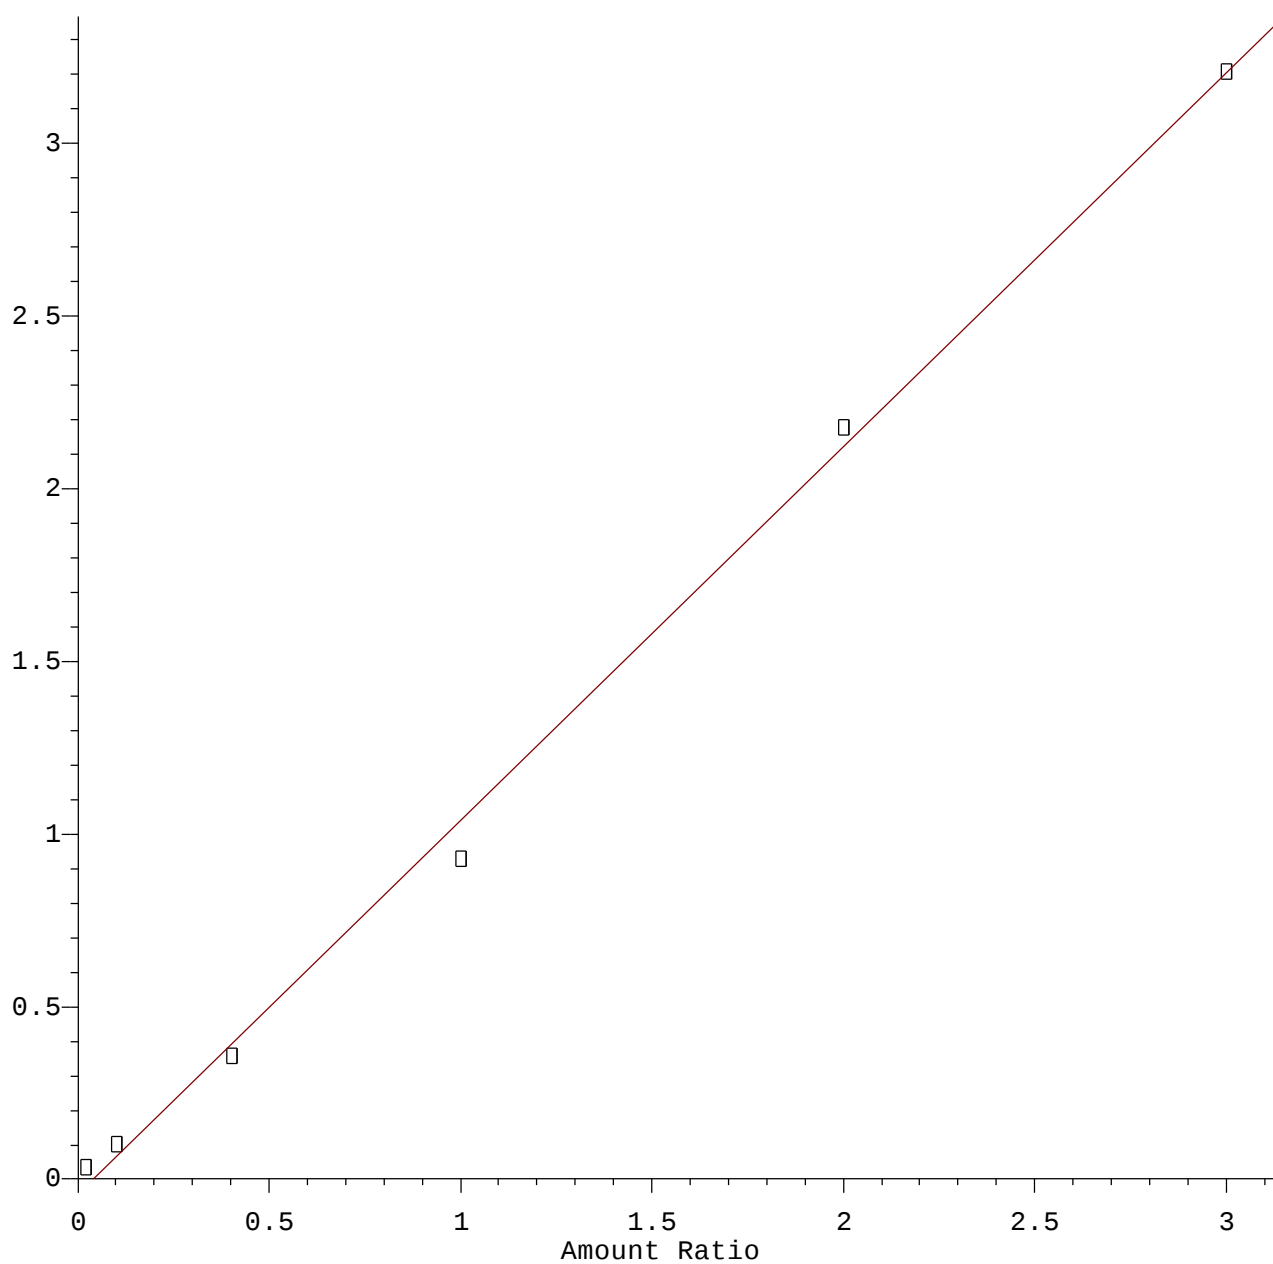

Resp Ratio = 1.08×10^0 * Amt - 4.25×10^{-2}
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Calibration Table Last Updated: Tue Dec 03 16:37:42 2019

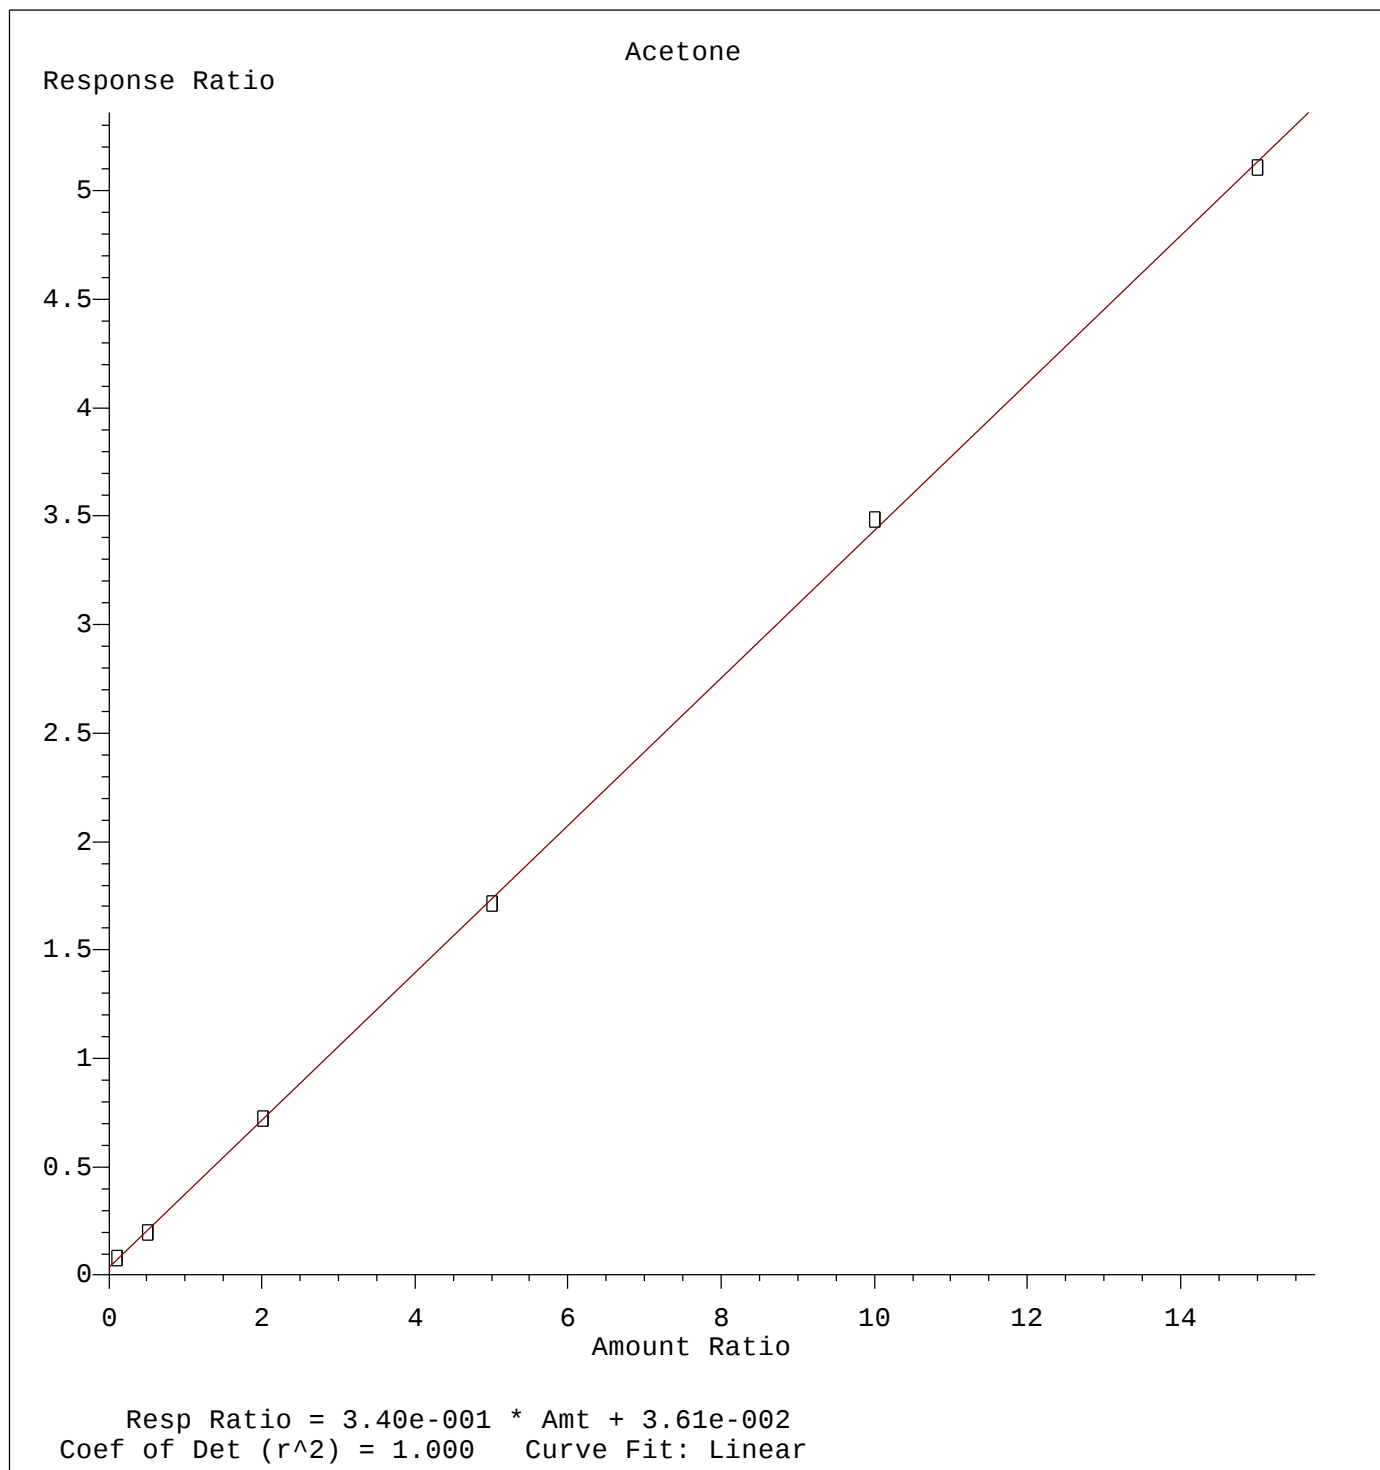

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Calibration Table Last Updated: Tue Dec 03 16:37:42 2019