


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN120320\
Data File : VN064888.D
Acq On : 3 Dec 2020 9:54
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Title : SW846 8260
Last Update : Mon Nov 23 13:54:12 2020

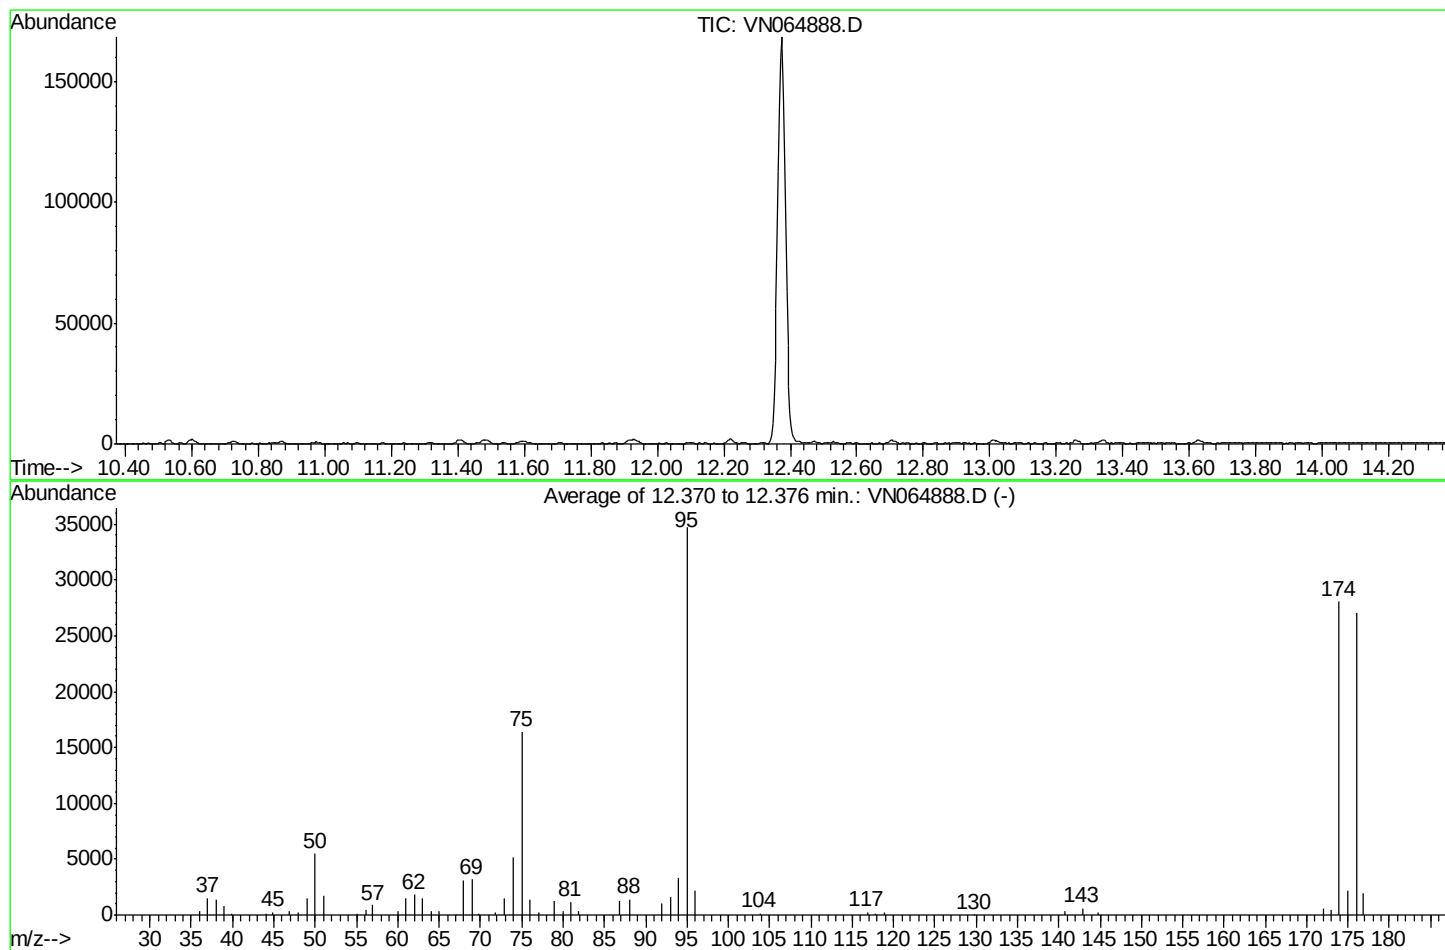

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	5499	PASS
75	95	30	60	47.4	16450	PASS
95	95	100	100	100.0	34712	PASS
96	95	5	9	6.4	2218	PASS
173	174	0.00	2	1.7	479	PASS
174	95	50	100	80.9	28072	PASS
175	174	5	9	7.7	2153	PASS
176	174	95	101	96.2	27013	PASS
177	176	5	9	7.1	1910	PASS