

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120321\
 Data File : VN069749.D
 Acq On : 4 Dec 2021 5:13
 Operator : JC/MD
 Sample : PB141141TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB141141TB

Quant Time: Dec 04 07:09:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	1409812	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2537603	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2692485	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	1067800	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	1100126	50.540	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 101.080%			
35) Dibromofluoromethane	8.024	113	762691	47.983	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 95.960%			
50) Toluene-d8	10.441	98	3296975	51.658	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 103.320%			
62) 4-Bromofluorobenzene	12.731	95	1274576	55.124	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 110.240%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.301	50	6667	0.324	ug/l #	64
8) Diethyl Ether	3.832	74	12413	1.296	ug/l	81
11) Tert butyl alcohol	5.361	59	4723	1.148	ug/l #	89
16) Acetone	4.296	43	188487	14.395	ug/l	94
18) Methyl Acetate	4.862	43	10665	0.270	ug/l #	62
20) Methylene Chloride	5.095	84	76155	4.375	ug/l	86
25) 2-Butanone	7.346	43	74276	4.175	ug/l	93
29) Tetrahydrofuran	7.686	42	2609	0.242	ug/l #	80
31) Cyclohexane	8.088	56	37677	1.244	ug/l #	29
36) 1,1-Dichloropropene	8.083	75	123080	5.095	ug/l #	49
37) Ethyl Acetate	7.346	43	74276	2.066	ug/l #	69
38) Carbon Tetrachloride	8.086	117	147463	6.225	ug/l #	16
43) Isopropyl Acetate	8.560	43	123730	2.325	ug/l #	85
45) 1,2-Dichloropropane	9.625	63	7094	0.358	ug/l #	44
48) Methyl methacrylate	9.545	41	35194	1.417	ug/l #	8
51) 4-Methyl-2-Pentanone	10.336	43	19146	0.555	ug/l #	80
53) t-1,3-Dichloropropene	10.639	75	88	2.797	ug/l #	1
54) cis-1,3-Dichloropropene	10.242	75	162162	7.007	ug/l #	74
56) Ethyl methacrylate	10.875	69	1387	2.318	ug/l #	1
57) 1,3-Dichloropropane	11.090	76	95810	2.992	ug/l #	43
58) 2-Chloroethyl Vinyl ether	10.054	63	30	18.392	ug/l #	45
59) 2-Hexanone	11.090	43	1761981	67.480	ug/l #	48
60) Dibromochloromethane	11.497	129	732	2.412	ug/l #	11
71) Bromoform	12.709	173	343	2.751	ug/l #	29
74) N-amyl acetate	12.363	43	10125	0.241	ug/l #	45
76) 1,2,3-Trichloropropane	12.731	75	718311	23.457	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	718311	74.598	ug/l #	5
93) 1,2,4-Trichlorobenzene	15.263	180	368	2.898	ug/l #	56
95) Naphthalene	15.504	128	2103	4.022	ug/l #	73
96) 1,2,3-Trichlorobenzene	15.697	180	484	2.463	ug/l #	36

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120321\
Data File : VN069749.D
Acq On : 4 Dec 2021 5:13
Operator : JC/MD
Sample : PB141141TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB141141TB

Quant Time: Dec 04 07:09:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 03 08:46:47 2021
Response via : Initial Calibration




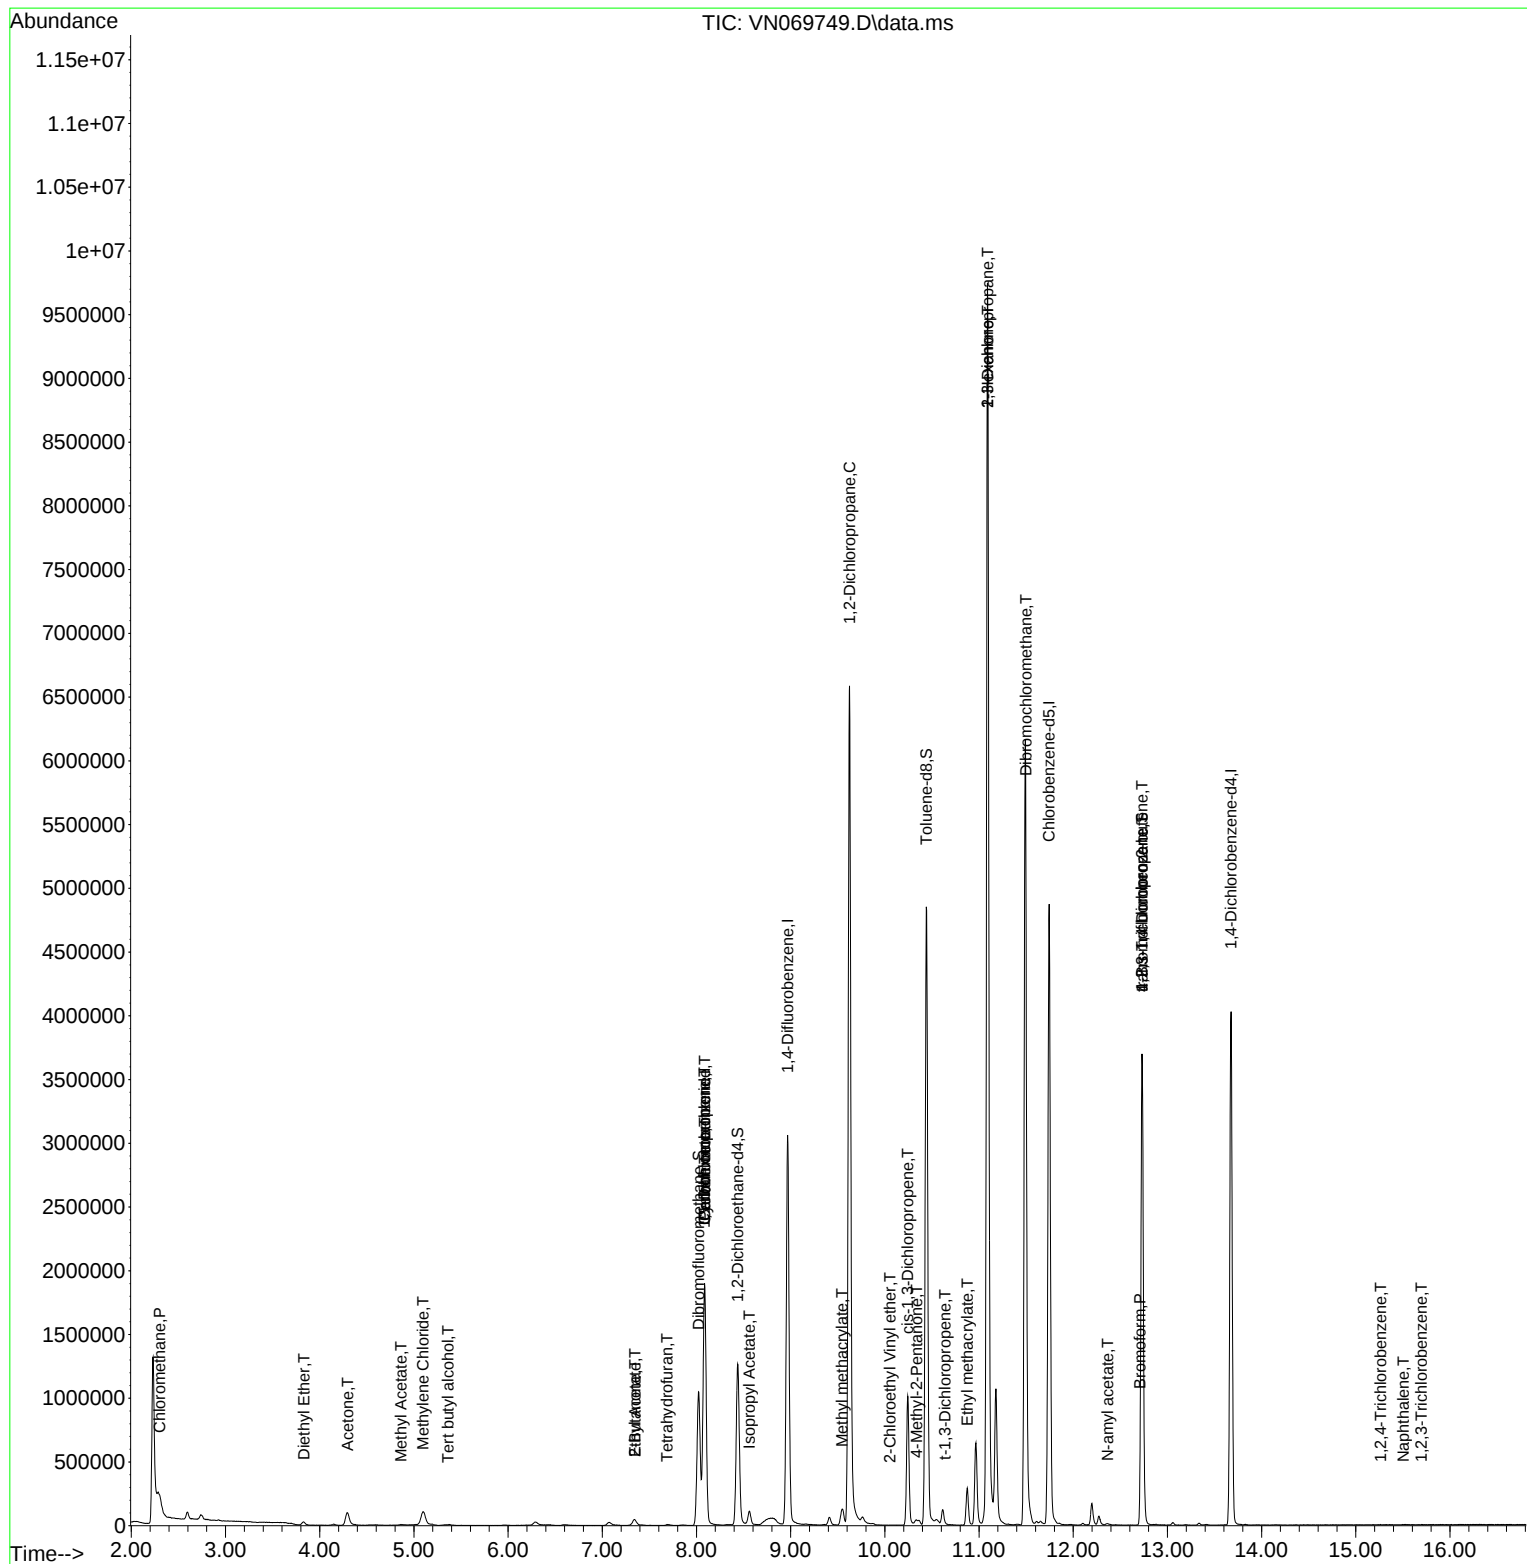




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13




Instrument :
MSVOA_N
ClientSampleId :
PB141141TB


Tgt Ion:168 Resp: 1409812
Ion Ratio Lower Upper
168 100
99 61.7 41.3 61.9

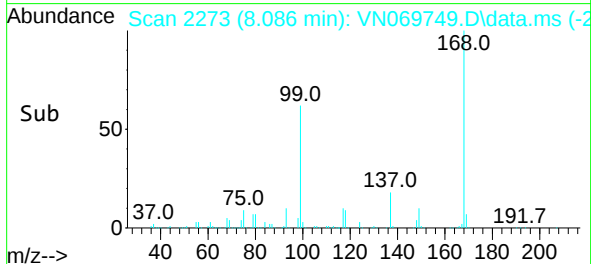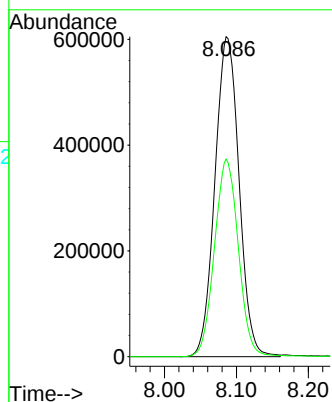

#3
Chloromethane
Concen: 0.324 ug/l
RT: 2.301 min Scan# 116
Delta R.T. -0.002 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion: 50 Resp: 6667
Ion Ratio Lower Upper
50 100
52 11.8 25.4 38.0#


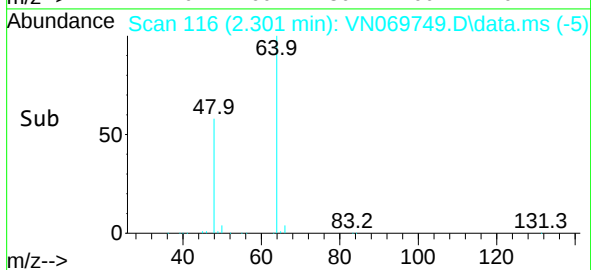
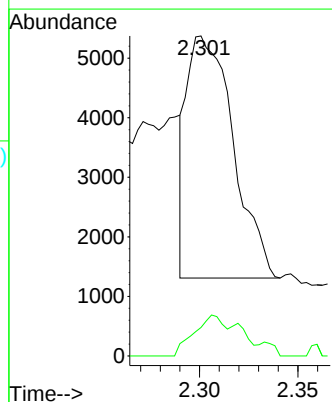
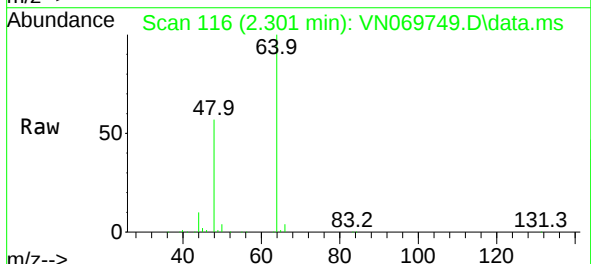




#8
Diethyl Ether
Concen: 1.296 ug/l
RT: 3.832 min Scan# 61
Delta R.T. 0.011 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13




Instrument :
MSVOA_N
ClientSampleId :
PB141141TB


Tgt Ion: 74 Resp: 12413
Ion Ratio Lower Upper
74 100
45 112.4 47.0 141.2

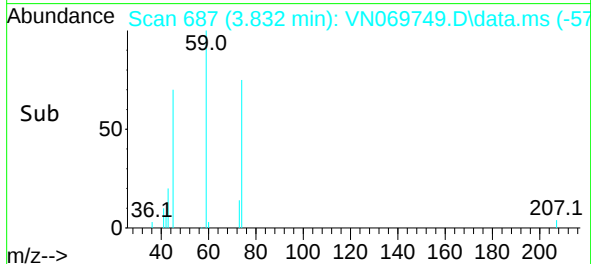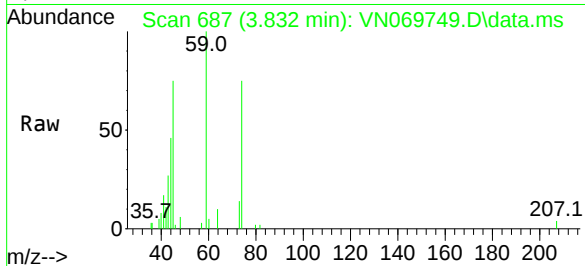

#11
Tert butyl alcohol
Concen: 1.148 ug/l
RT: 5.361 min Scan# 1257
Delta R.T. -0.029 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion: 59 Resp: 4723
Ion Ratio Lower Upper
59 100
57 6.6 8.7 13.1#


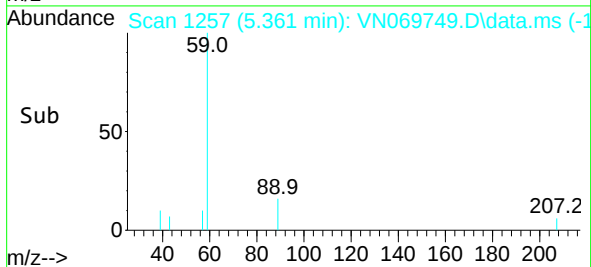

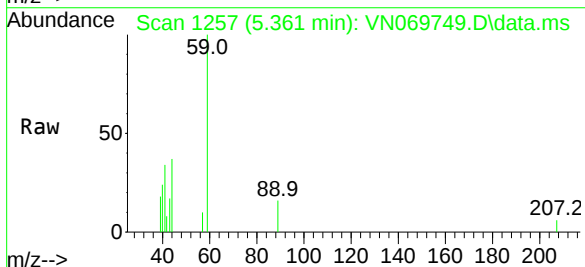




#16
Acetone
Concen: 14.395 ug/l
RT: 4.296 min Scan# 80
Delta R.T. 0.006 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13




Instrument :
MSVOA_N
ClientSampleId :
PB141141TB


Tgt Ion: 43 Resp: 188487
Ion Ratio Lower Upper
43 100
58 25.8 23.1 34.7

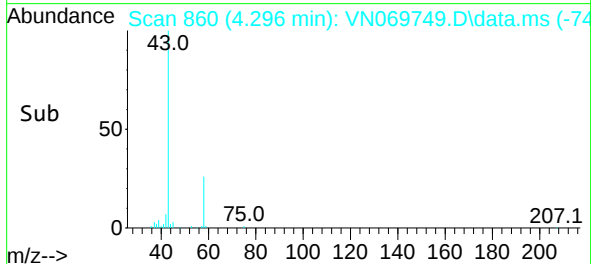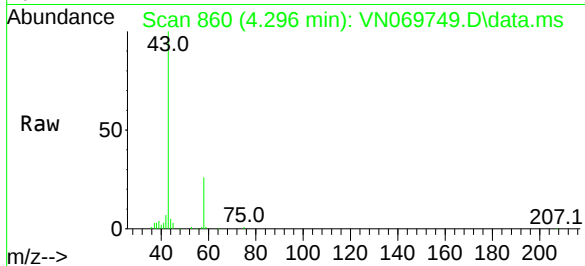

#18
Methyl Acetate
Concen: 0.270 ug/l
RT: 4.862 min Scan# 1071
Delta R.T. 0.006 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13


Tgt Ion: 43 Resp: 10665
Ion Ratio Lower Upper
43 100
74 5.3 19.4 29.2#

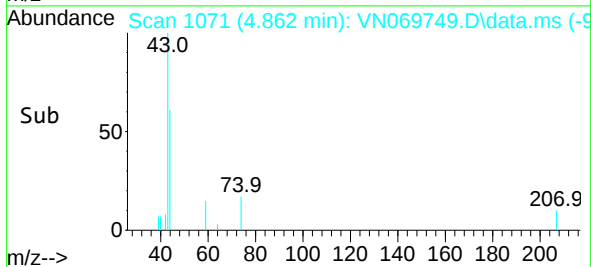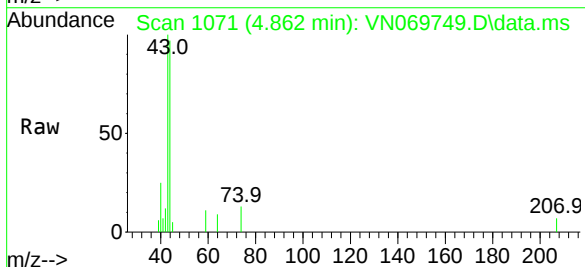

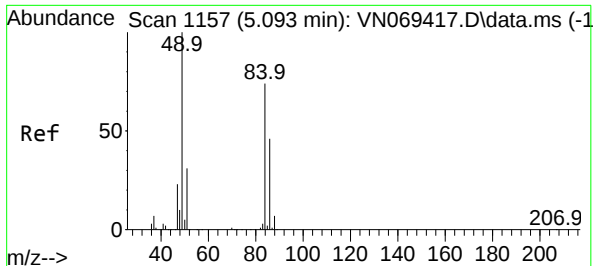




#20
Methylene Chloride
Concen: 4.375 ug/l
RT: 5.095 min Scan# 1157
Delta R.T. 0.003 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Instrument :
MSVOA_N
ClientSampleId :
PB141141TB

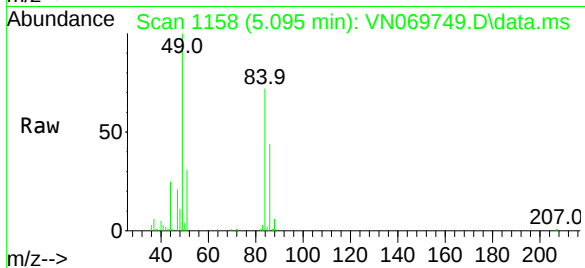

Tgt Ion: 84 Resp: 76155




Ion	Ratio	Lower	Upper
84	100		
49	139.0	93.5	140.3
51	42.6	29.4	44.2
86	61.1	53.0	79.4

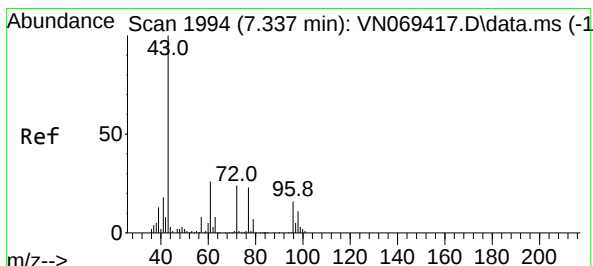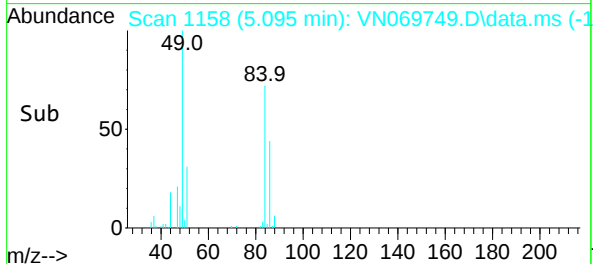


#25
2-Butanone
Concen: 4.175 ug/l
RT: 7.346 min Scan# 1997
Delta R.T. 0.008 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion: 43 Resp: 74276

Ion	Ratio	Lower	Upper
43	100		
72	23.4	21.7	32.5

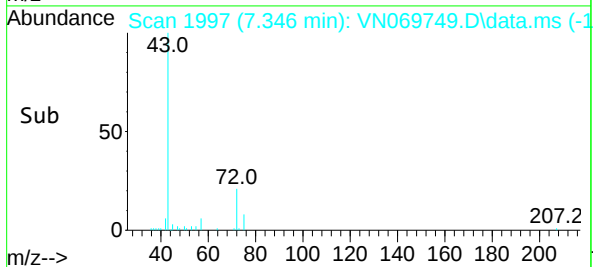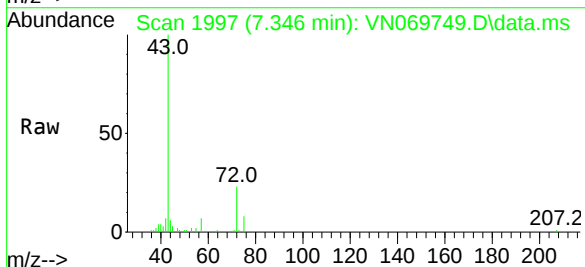



#29

Tetrahydrofuran

Concen: 0.242 ug/l

RT: 7.686 min Scan# 21

Delta R.T. 0.000 min

Lab File: VN069749.D

Acq: 4 Dec 2021 5:13

Instrument :

MSVOA_N

ClientSampleId :

PB141141TB





Tgt Ion: 42 Resp: 2609

Ion Ratio Lower Upper

42 100

72 27.2 36.3 54.5#

71 51.1 34.7 52.1

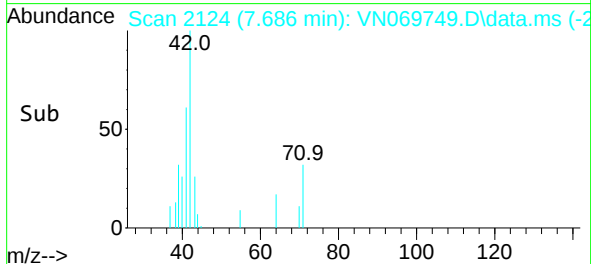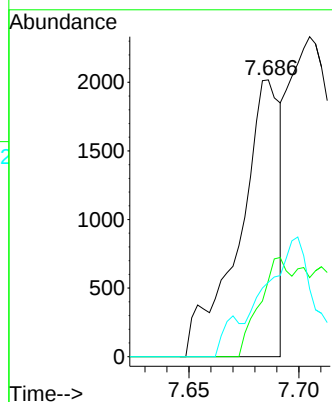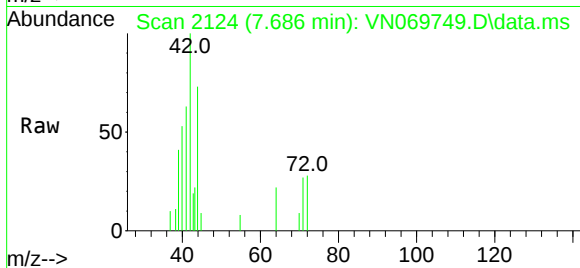

#31

Cyclohexane

Concen: 1.244 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. -0.005 min

Lab File: VN069749.D

Acq: 4 Dec 2021 5:13




Tgt Ion: 56 Resp: 37677


Ion Ratio Lower Upper

56 100

69 150.7 27.1 40.7#

84 112.2 73.4 110.0#

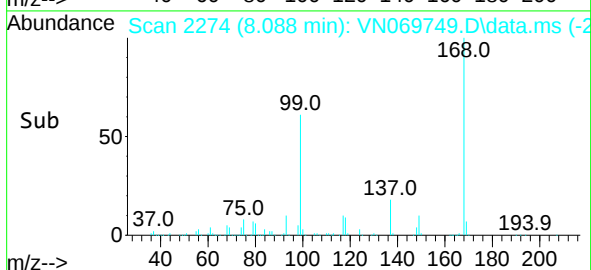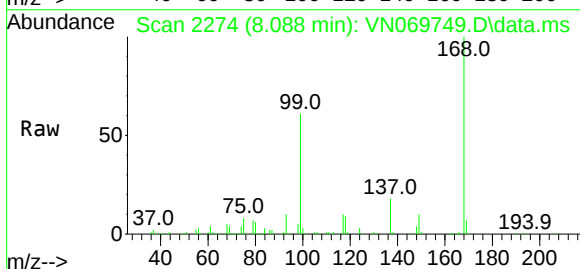



#33

1,2-Dichloroethane-d4

Concen: 50.540 ug/l

RT: 8.437 min Scan# 2405

Delta R.T. 0.000 min

Lab File: VN069749.D

Acq: 4 Dec 2021 5:13

Instrument :

MSVOA_N

ClientSampleId :





PB141141TB

Tgt Ion: 65 Resp: 1100126

Ion Ratio Lower Upper

65 100

67 50.6 0.0 103.0

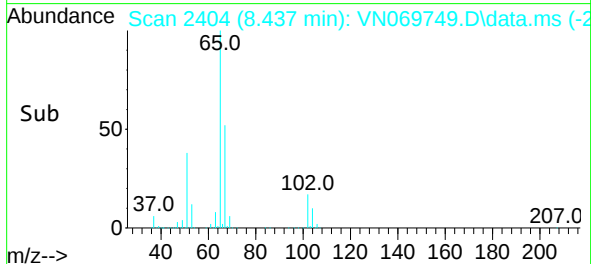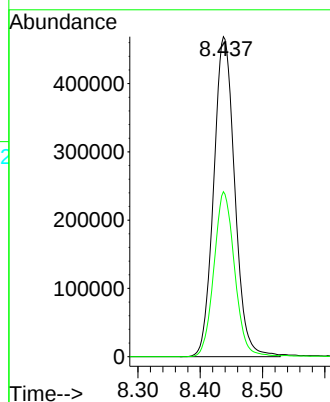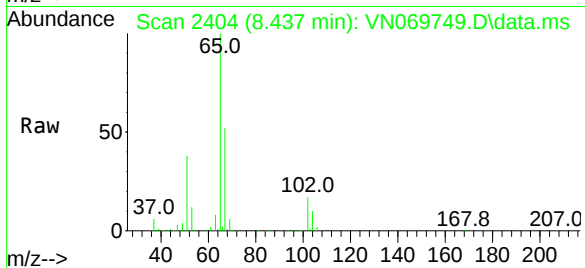

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.968 min Scan# 2602

Delta R.T. 0.000 min

Lab File: VN069749.D

Acq: 4 Dec 2021 5:13




Tgt Ion: 114 Resp: 2537603


Ion Ratio Lower Upper

114 100

63 23.6 0.0 37.8

88 16.3 0.0 27.4


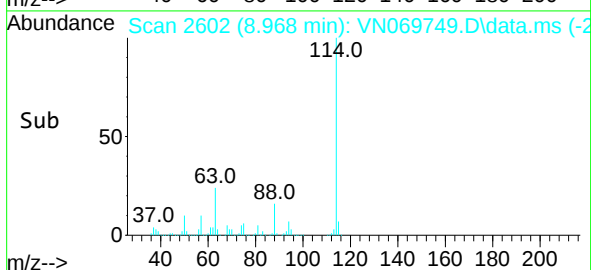

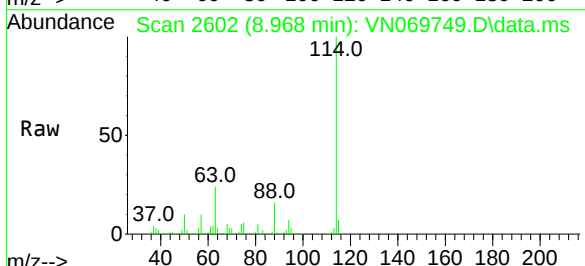




#35
Dibromofluoromethane
Concen: 47.983 ug/l
RT: 8.024 min Scan# 211
Delta R.T. 0.000 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13




Instrument :
MSVOA_N
ClientSampleId :
PB141141TB


Tgt Ion:113 Resp: 762691
Ion Ratio Lower Upper
113 100
111 102.4 82.2 123.2
192 18.7 16.9 25.3

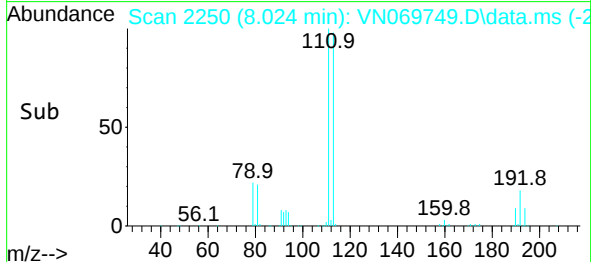

#36
1,1-Dichloropropene
Concen: 5.095 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.139 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13


Tgt Ion: 75 Resp: 123080
Ion Ratio Lower Upper
75 100
110 8.8 18.4 55.2#
77 0.0 24.4 36.6#

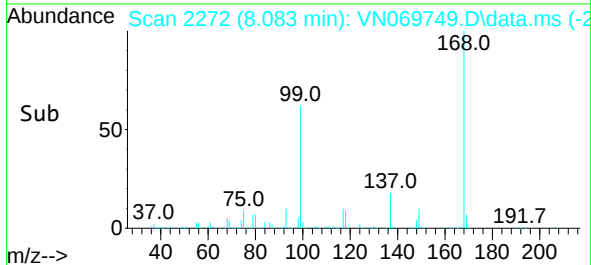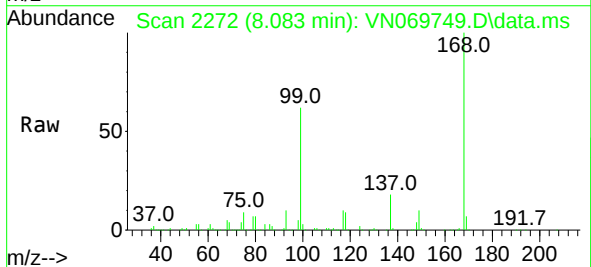






#37
Ethyl Acetate
Concen: 2.066 ug/l
RT: 7.346 min Scan# 1997
Delta R.T. -0.070 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Instrument :
MSVOA_N
ClientSampleId :
PB141141TB



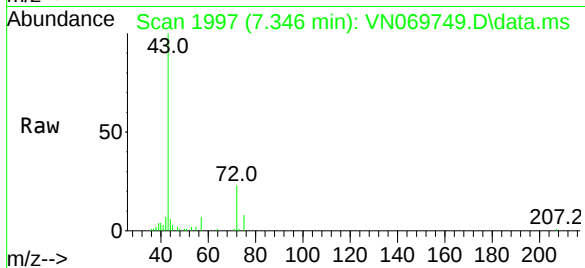



Tgt Ion: 43 Resp: 74276
Ion Ratio Lower Upper
43 100
61 0.2 11.5 17.3#
70 0.1 7.9 11.9#

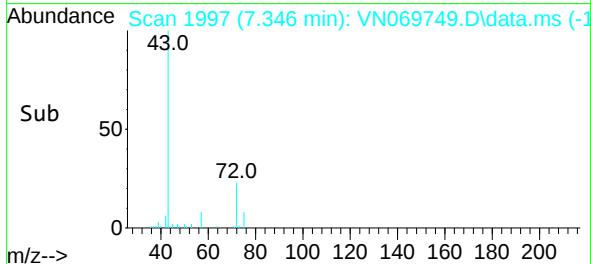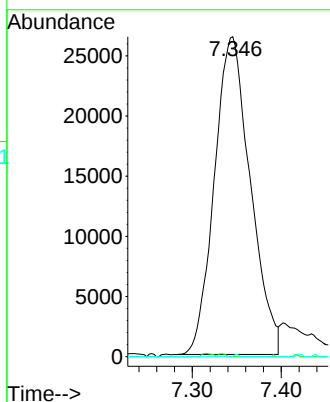

#38
Carbon Tetrachloride
Concen: 6.225 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.120 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion: 117 Resp: 147463
Ion Ratio Lower Upper
117 100
119 4.6 76.1 114.1#
121 0.0 24.2 36.2#


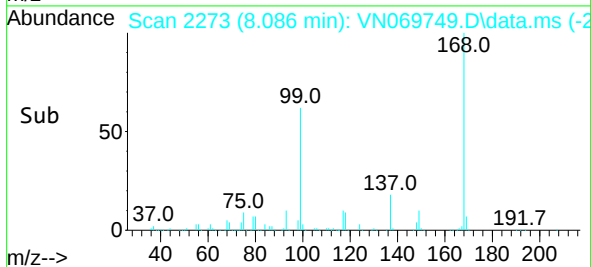

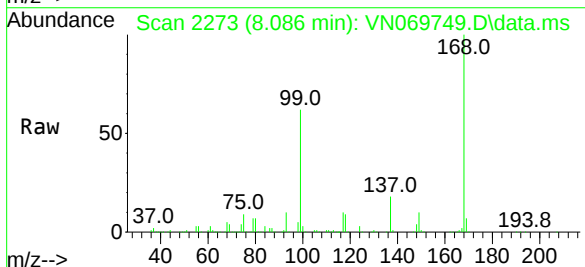




#43
Isopropyl Acetate
Concen: 2.325 ug/l
RT: 8.560 min Scan# 2451
Delta R.T. -0.002 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13




Instrument :
MSVOA_N
ClientSampleId :
PB141141TB


Tgt Ion: 43 Resp: 123730
Ion Ratio Lower Upper
43 100
61 15.7 20.4 30.6#
87 10.7 11.2 16.8#

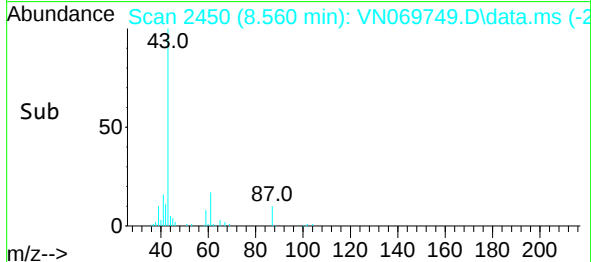

#45
1,2-Dichloropropane
Concen: 0.358 ug/l
RT: 9.625 min Scan# 2847
Delta R.T. 0.134 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion: 63 Resp: 7094
Ion Ratio Lower Upper
63 100
65 0.0 24.7 37.1#


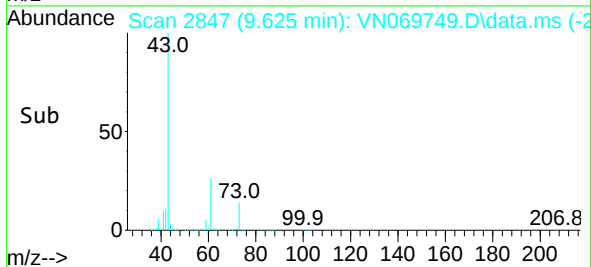

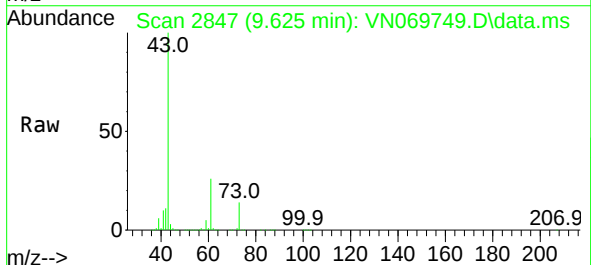




#48
Methyl methacrylate
Concen: 1.417 ug/l
RT: 9.545 min Scan# 21
Delta R.T. -0.016 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13




Instrument :
MSVOA_N
ClientSampleId :
PB141141TB


Tgt Ion: 41 Resp: 35194
Ion Ratio Lower Upper
41 100
69 0.3 72.4 108.6#
39 0.0 58.4 87.6#

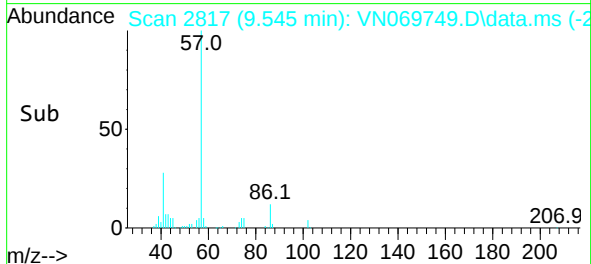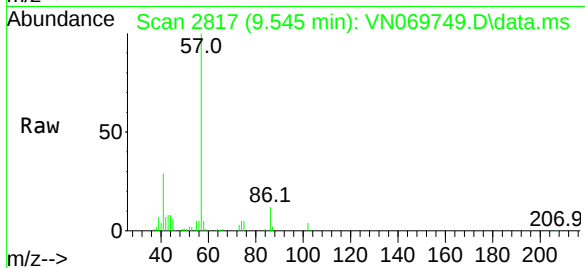

#50
Toluene-d8
Concen: 51.658 ug/l
RT: 10.441 min Scan# 3151
Delta R.T. -0.002 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion: 98 Resp: 3296975
Ion Ratio Lower Upper
98 100
100 63.8 50.4 75.6

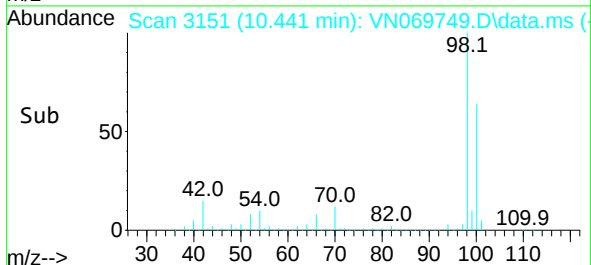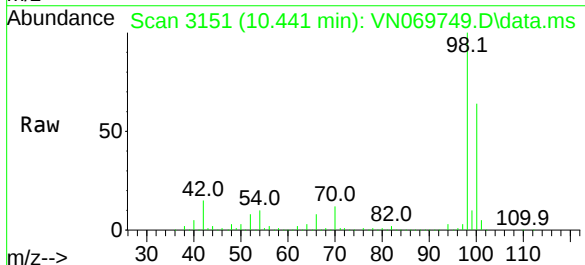

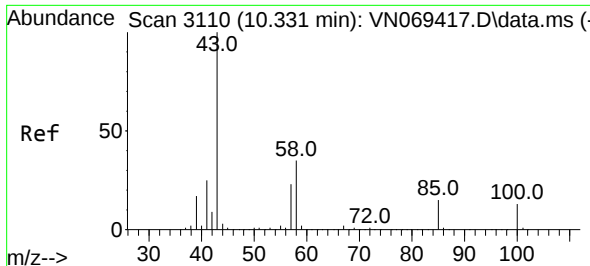

#51

4-Methyl-2-Pentanone

Concen: 0.555 ug/l

RT: 10.336 min Scan# 3110

Delta R.T. 0.003 min

Lab File: VN069749.D

Acq: 4 Dec 2021 5:13

Instrument :

MSVOA_N

ClientSampleId :





PB141141TB

Tgt Ion: 43 Resp: 19146

Ion Ratio Lower Upper

43 100

58 50.3 30.4 45.6#

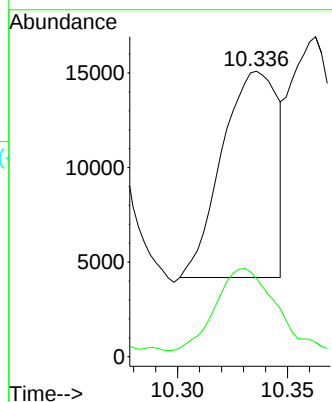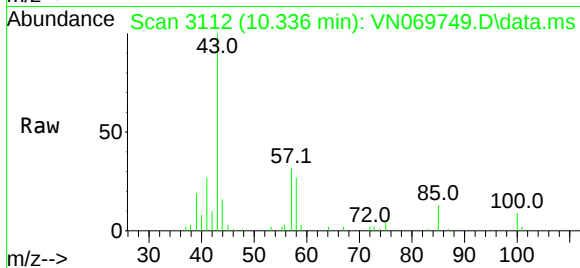

#53

t-1,3-Dichloropropene

Concen: 2.797 ug/l

RT: 10.639 min Scan# 3225

Delta R.T. -0.080 min

Lab File: VN069749.D




Acq: 4 Dec 2021 5:13


Tgt Ion: 75 Resp: 88

Ion Ratio Lower Upper

75 100

77 420.6 25.6 38.4#


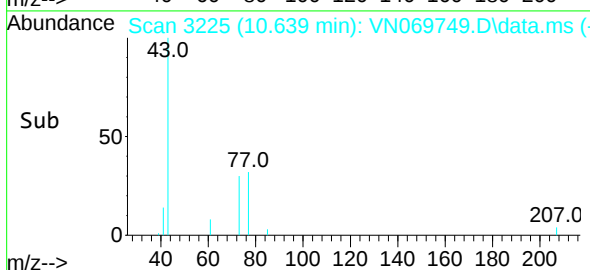

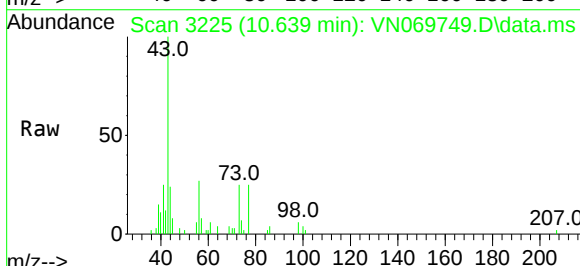




#54
 cis-1,3-Dichloropropene
 Concen: 7.007 ug/l
 RT: 10.242 min Scan# 3057
 Delta R.T. 0.051 min
 Lab File: VN069749.D
 Acq: 4 Dec 2021 5:13




Instrument :
 MSVOA_N
 ClientSampleId :
 PB141141TB


Tgt Ion: 75 Resp: 162162
 Ion Ratio Lower Upper
 75 100
 77 0.4 26.4 39.6#
 39 48.2 42.5 63.7

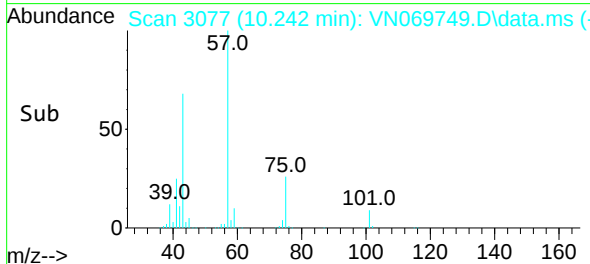

#56
 Ethyl methacrylate
 Concen: 2.318 ug/l
 RT: 10.875 min Scan# 3313
 Delta R.T. 0.113 min
 Lab File: VN069749.D
 Acq: 4 Dec 2021 5:13

Tgt Ion: 69 Resp: 1387
 Ion Ratio Lower Upper
 69 100
 41 4736.3 51.4 77.0#
 39 2277.2 34.6 52.0#

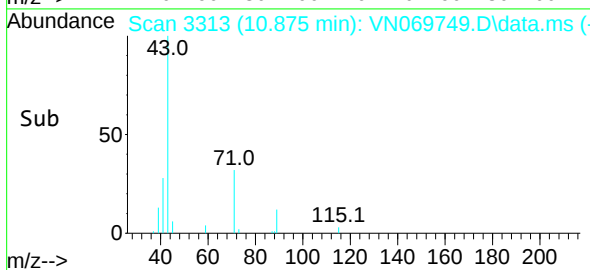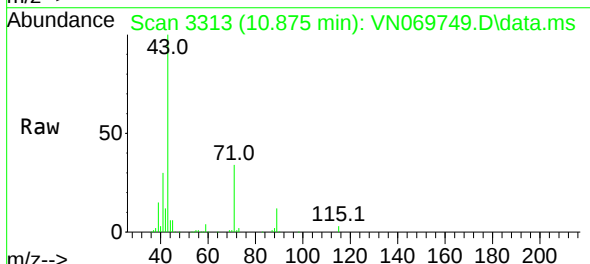

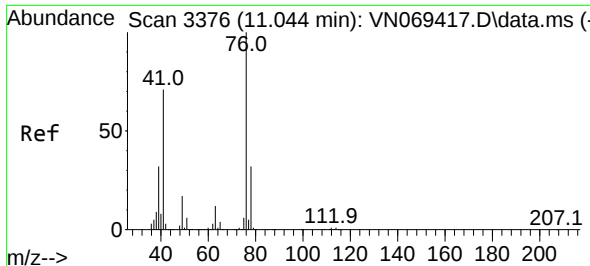

#57

1,3-Dichloropropane

Concen: 2.992 ug/l

RT: 11.090 min Scan# 31

Delta R.T. 0.043 min

Lab File: VN069749.D

Acq: 4 Dec 2021 5:13

Instrument :

MSVOA_N

ClientSampleId :





PB141141TB

Tgt Ion: 76 Resp: 95810

Ion Ratio Lower Upper

76 100

78 0.5 25.7 38.5#

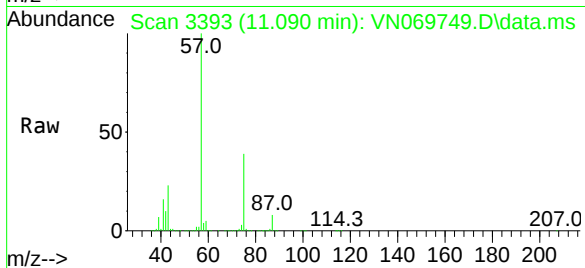

#58

2-Chloroethyl Vinyl ether

Concen: 18.392 ug/l

RT: 10.054 min Scan# 3007

Delta R.T. 0.011 min

Lab File: VN069749.D




Acq: 4 Dec 2021 5:13


Tgt Ion: 63 Resp: 30

Ion Ratio Lower Upper

63 100

106 0.0 23.9 35.9#


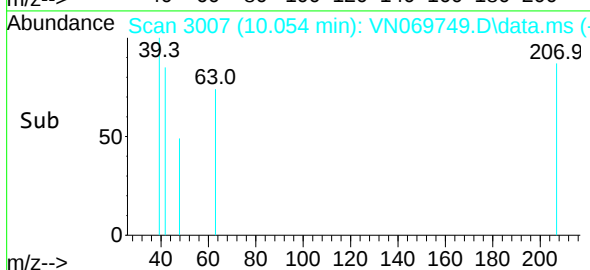

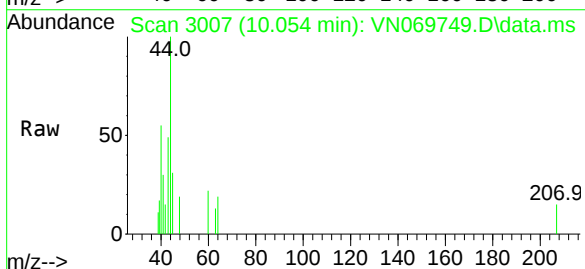




#59
2-Hexanone
Concen: 67.480 ug/l
RT: 11.090 min Scan# 31
Delta R.T. 0.003 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13




Instrument :
MSVOA_N
ClientSampleId :
PB141141TB


Tgt Ion: 43 Resp: 1761981
Ion Ratio Lower Upper
43 100
58 16.6 26.9 80.7#

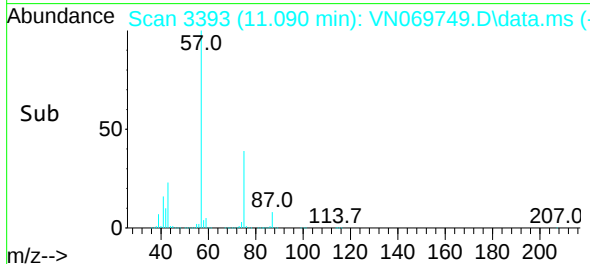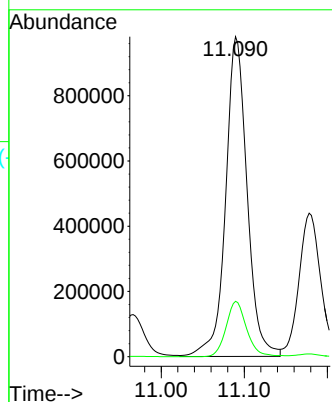

#60
Dibromochloromethane
Concen: 2.412 ug/l
RT: 11.497 min Scan# 3545
Delta R.T. 0.257 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion: 129 Resp: 732
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#




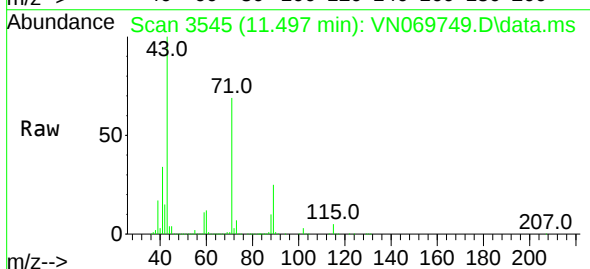


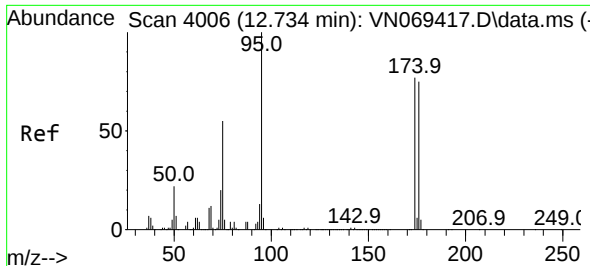

#62
4-Bromofluorobenzene
Concen: 55.124 ug/l
RT: 12.731 min Scan# 4006
Delta R.T. -0.000 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13




Instrument :
MSVOA_N
ClientSampleId :
PB141141TB


Tgt Ion: 95 Resp: 1274576
Ion Ratio Lower Upper
95 100
174 75.8 0.0 187.2
176 72.7 0.0 181.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.002 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion: 117 Resp: 2692485
Ion Ratio Lower Upper
117 100
82 58.6 42.4 63.6
119 32.2 25.4 38.2


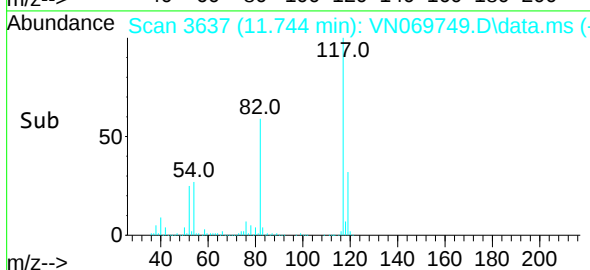






#71
Bromoform
Concen: 2.751 ug/l
RT: 12.709 min Scan# 3904
Delta R.T. 0.249 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13




Instrument :
MSVOA_N
ClientSampleId :
PB141141TB


Tgt Ion:173 Resp: 343
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0

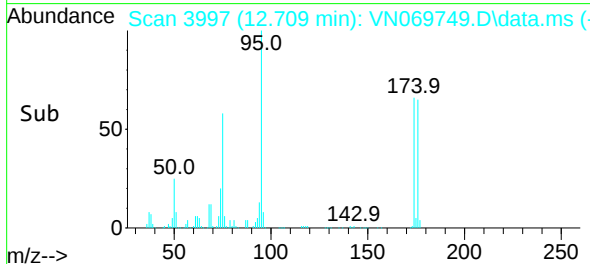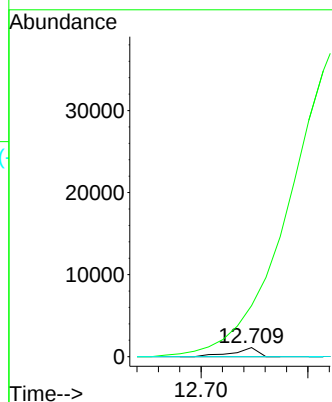

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.002 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13


Tgt Ion:152 Resp: 1067800
Ion Ratio Lower Upper
152 100
115 60.9 27.5 82.5
150 157.2 0.0 344.4

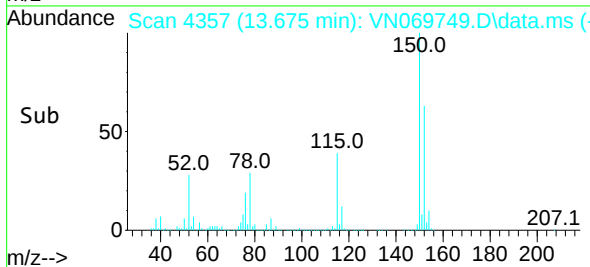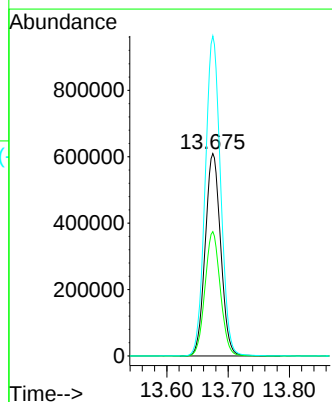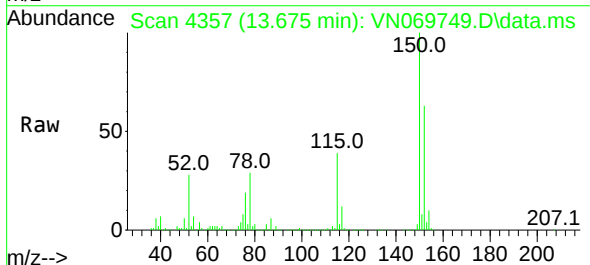






#74
N-amy1 acetate
Concen: 0.241 ug/l
RT: 12.363 min Scan# 31
Delta R.T. -0.024 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Instrument :
MSVOA_N
ClientSampleId :
PB141141TB







Tgt Ion:	43	Resp:	10125
Ion Ratio	Lower	Upper	
43	100		
70	0.8	33.4	50.0#
55	1.5	19.3	28.9#
61	0.0	18.5	27.7#

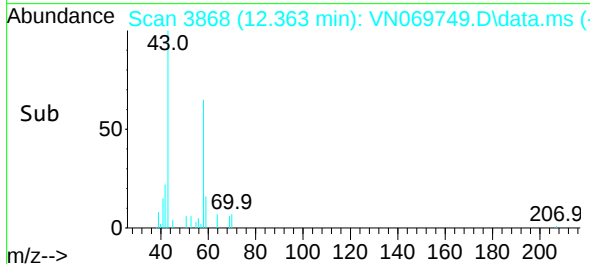

#76
1,2,3-Trichloropropane
Concen: 23.457 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.150 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion:	75	Resp:	718311
Ion Ratio	Lower	Upper	
75	100		
77	1.0	82.6	247.8#


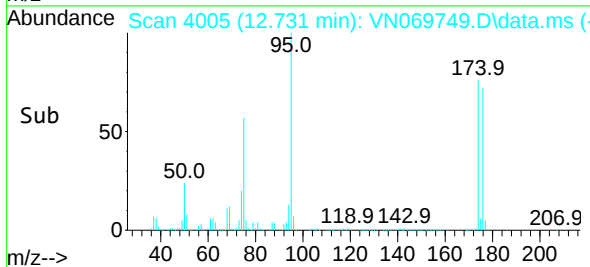

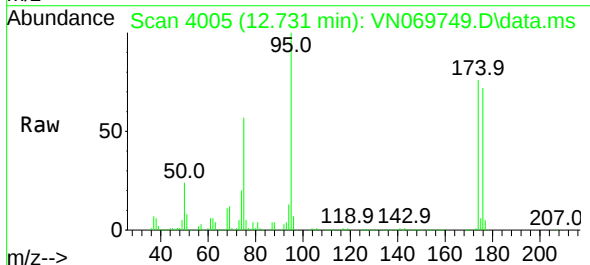




#81
trans-1,4-Dichloro-2-butene
Concen: 74.598 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13




Instrument :
MSVOA_N
ClientSampleId :
PB141141TB


Tgt Ion: 75 Resp: 718311
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

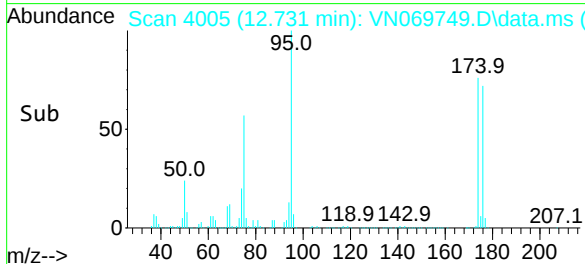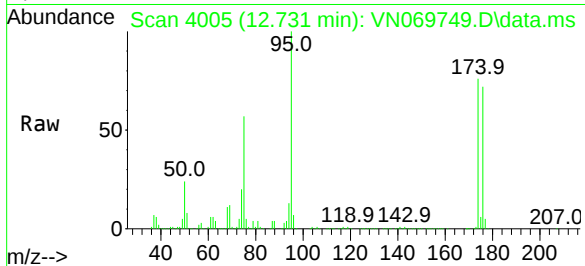

#93
1,2,4-Trichlorobenzene
Concen: 2.898 ug/l
RT: 15.263 min Scan# 4949
Delta R.T. -0.002 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion:180 Resp: 368
Ion Ratio Lower Upper
180 100
182 56.8 48.3 144.9
145 0.0 14.5 43.5#


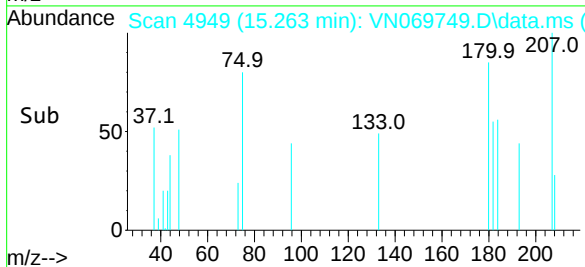

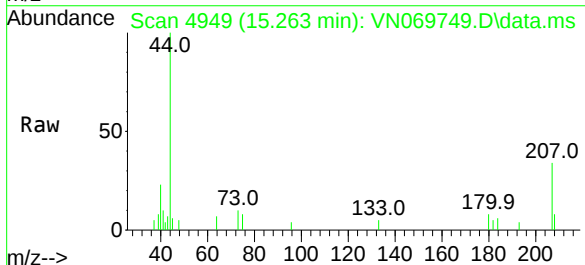




#95
Naphthalene
Concen: 4.022 ug/l
RT: 15.504 min Scan# 5040
Delta R.T. -0.003 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Instrument :
MSVOA_N
ClientSampleId :
PB141141TB

Tgt Ion:128 Resp: 2103
Ion Ratio Lower Upper
128 100
127 0.0 10.5 15.7#
129 3.0 8.7 13.1#

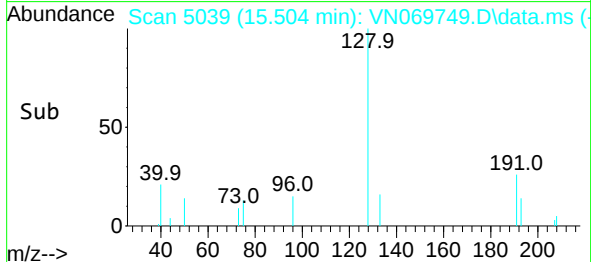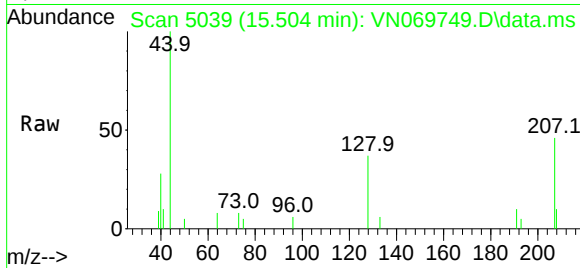

#96
1,2,3-Trichlorobenzene
Concen: 2.463 ug/l
RT: 15.697 min Scan# 5111
Delta R.T. -0.005 min
Lab File: VN069749.D
Acq: 4 Dec 2021 5:13

Tgt Ion:180 Resp: 484
Ion Ratio Lower Upper
180 100
182 30.6 47.4 142.2#
145 0.0 15.0 45.1#

