


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120321\
Data File : VN069732.D
Acq On : 3 Dec 2021 21:35
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Title : SW846 8260
Last Update : Fri Dec 03 08:46:47 2021

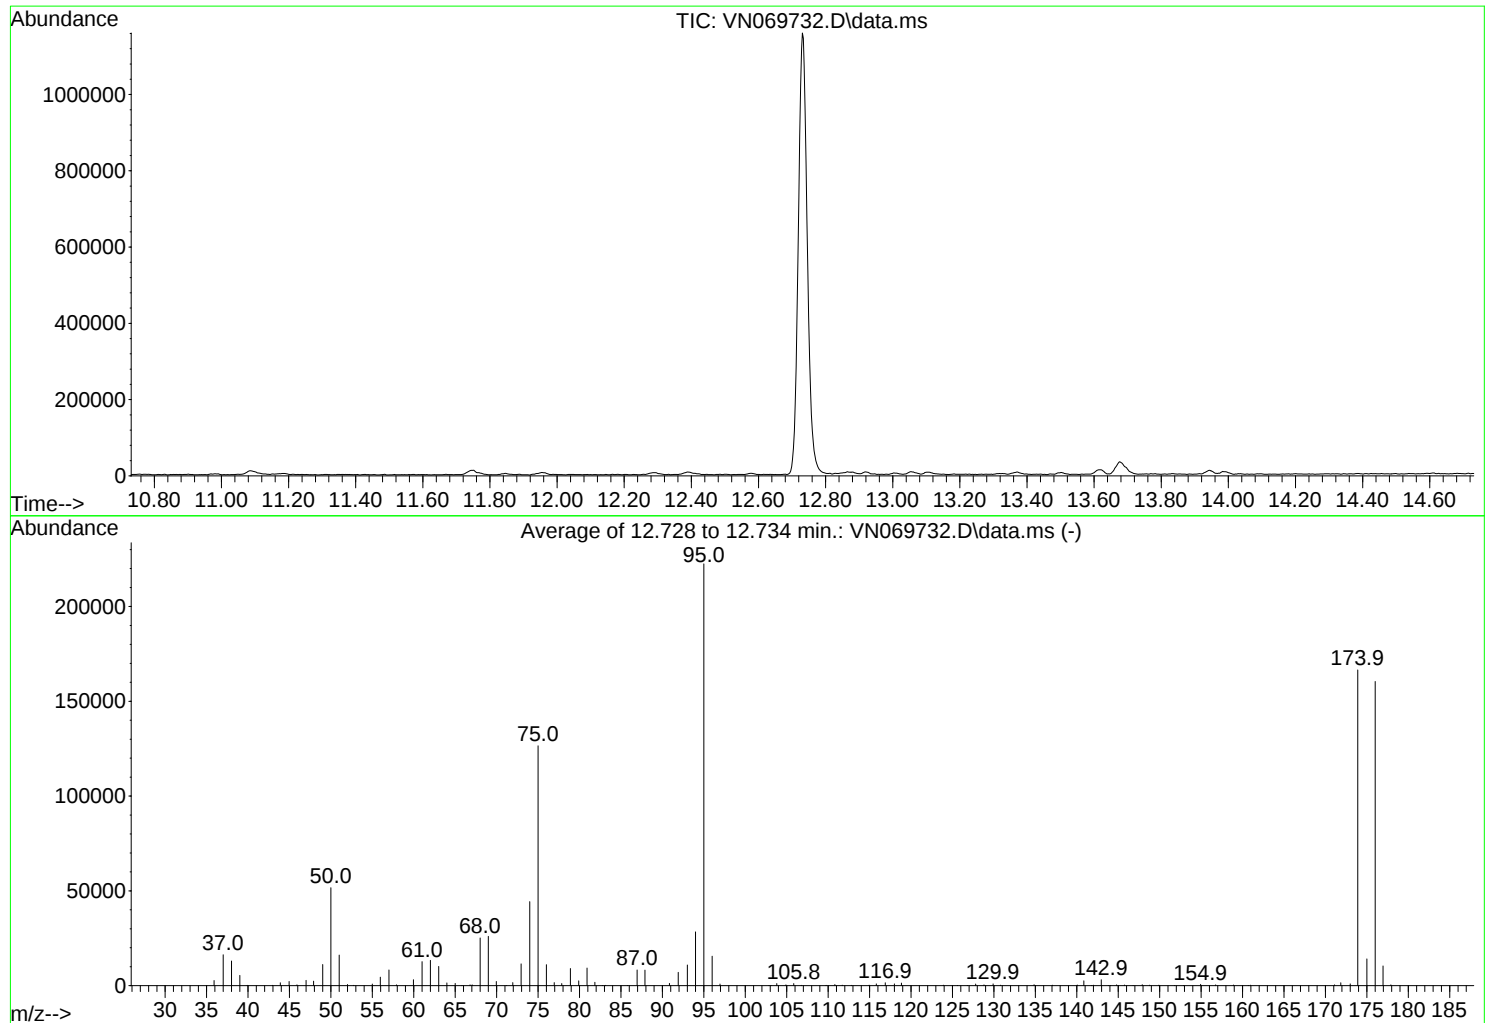

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.2	51635	PASS
75	95	30	60	56.9	126536	PASS
95	95	100	100	100.0	222485	PASS
96	95	5	9	7.0	15574	PASS
173	174	0.00	2	0.6	957	PASS
174	95	50	100	74.9	166549	PASS
175	174	5	9	8.4	14071	PASS
176	174	95	101	96.3	160405	PASS
177	176	5	9	6.5	10392	PASS