
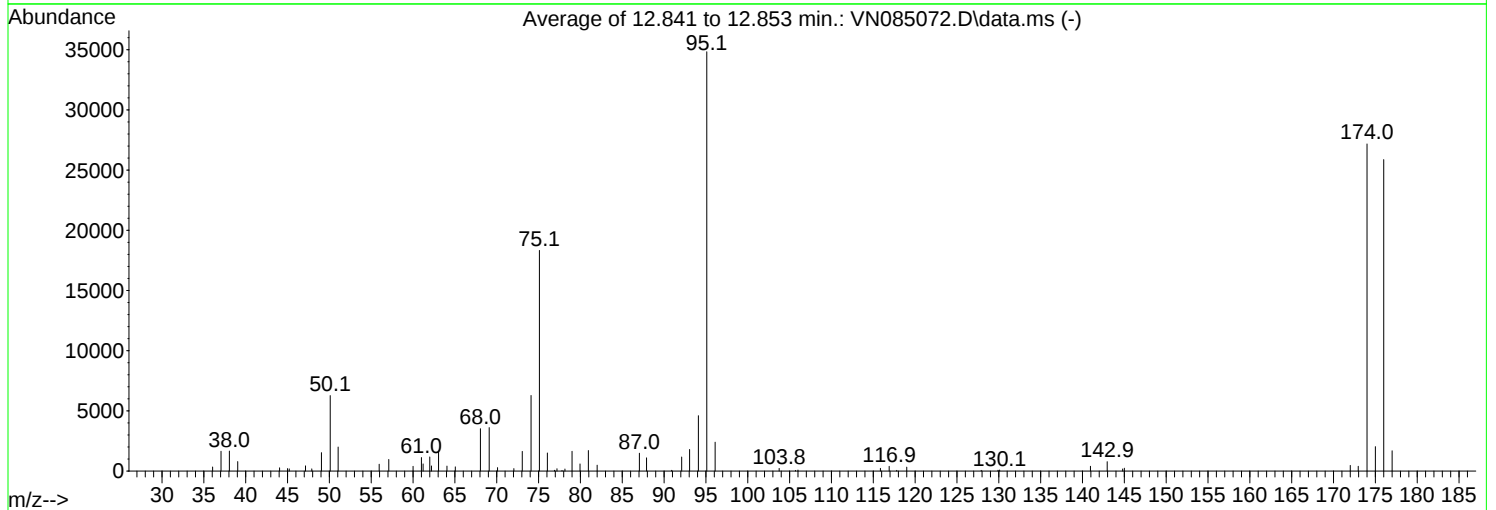


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120324\
Data File : VN085072.D
Acq On : 03 Dec 2024 08:50
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

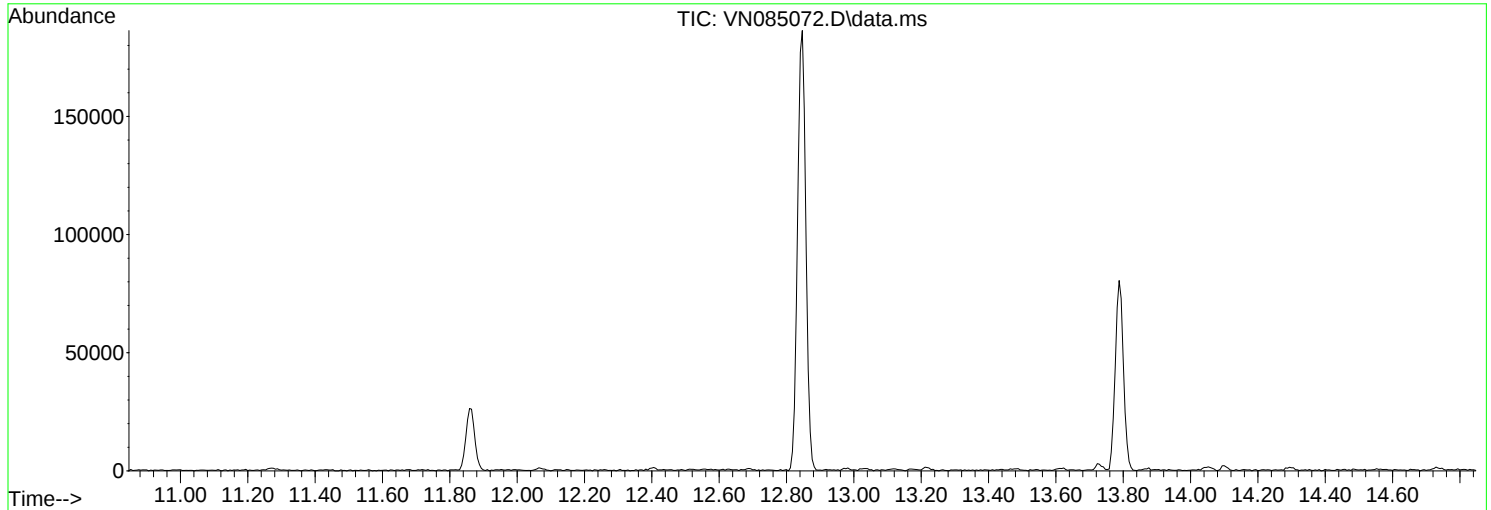

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	6273	PASS
75	95	30	60	52.6	18330	PASS
95	95	100	100	100.0	34835	PASS
96	95	5	9	6.9	2401	PASS
173	174	0.00	2	1.5	401	PASS
174	95	50	100	78.0	27173	PASS
175	174	5	9	7.5	2030	PASS
176	174	95	101	95.2	25877	PASS
177	176	5	9	6.5	1687	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	338	51.05	1996	68.05	3522	78.15	173
37.05	1647	55.95	572	69.10	3612	79.00	1645
38.05	1663	57.10	966	70.10	288	79.95	592
39.05	788	60.00	395	72.05	209	80.95	1708
44.05	271	61.00	1124	73.05	1636	82.00	493
45.00	208	61.20	594	74.10	6280	87.05	1484
45.20	184	62.00	1174	75.10	18330	87.90	1102
47.15	436	62.20	426	76.05	1504	90.90	62
47.90	183	63.05	1654	76.90	69	92.10	1170
49.05	1531	64.05	417	77.20	197	93.05	1795
50.10	6273	65.05	351	77.80	52	94.10	4602

Average of 12.841 to 12.853 min.: VN085072.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.10	34835	130.10	87				
96.10	2401	140.95	399				
103.75	224	142.95	780				
105.70	54	144.80	177				
106.00	89	145.00	238				
115.85	229	172.00	470				
116.90	396	172.95	401				
117.80	60	174.00	27173				
119.00	326	175.00	2030				
127.90	59	176.00	25877				
129.90	70	177.00	1687				

Instrument :

MSVOA_N

ClientSampleId :

BFB