

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120325\
 Data File : VN088417.D
 Acq On : 03 Dec 2025 10:43
 Operator : JC\MD
 Sample : VN1203MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1203MBL01

Quant Time: Dec 04 00:14:31 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 25 01:34:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	157196	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	366654	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.841	117	360665	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	162391	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	195853	66.138	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	132.280%#
35) Dibromofluoromethane	8.147	113	140865	55.439	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	110.880%
50) Toluene-d8	10.547	98	483810	51.175	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.340%
62) 4-Bromofluorobenzene	12.829	95	167218	51.549	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	103.100%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120325\
Data File : VN088417.D
Acq On : 03 Dec 2025 10:43
Operator : JC\MD
Sample : VN1203MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1203MBL01

Quant Time: Dec 04 00:14:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 25 01:34:52 2025
Response via : Initial Calibration




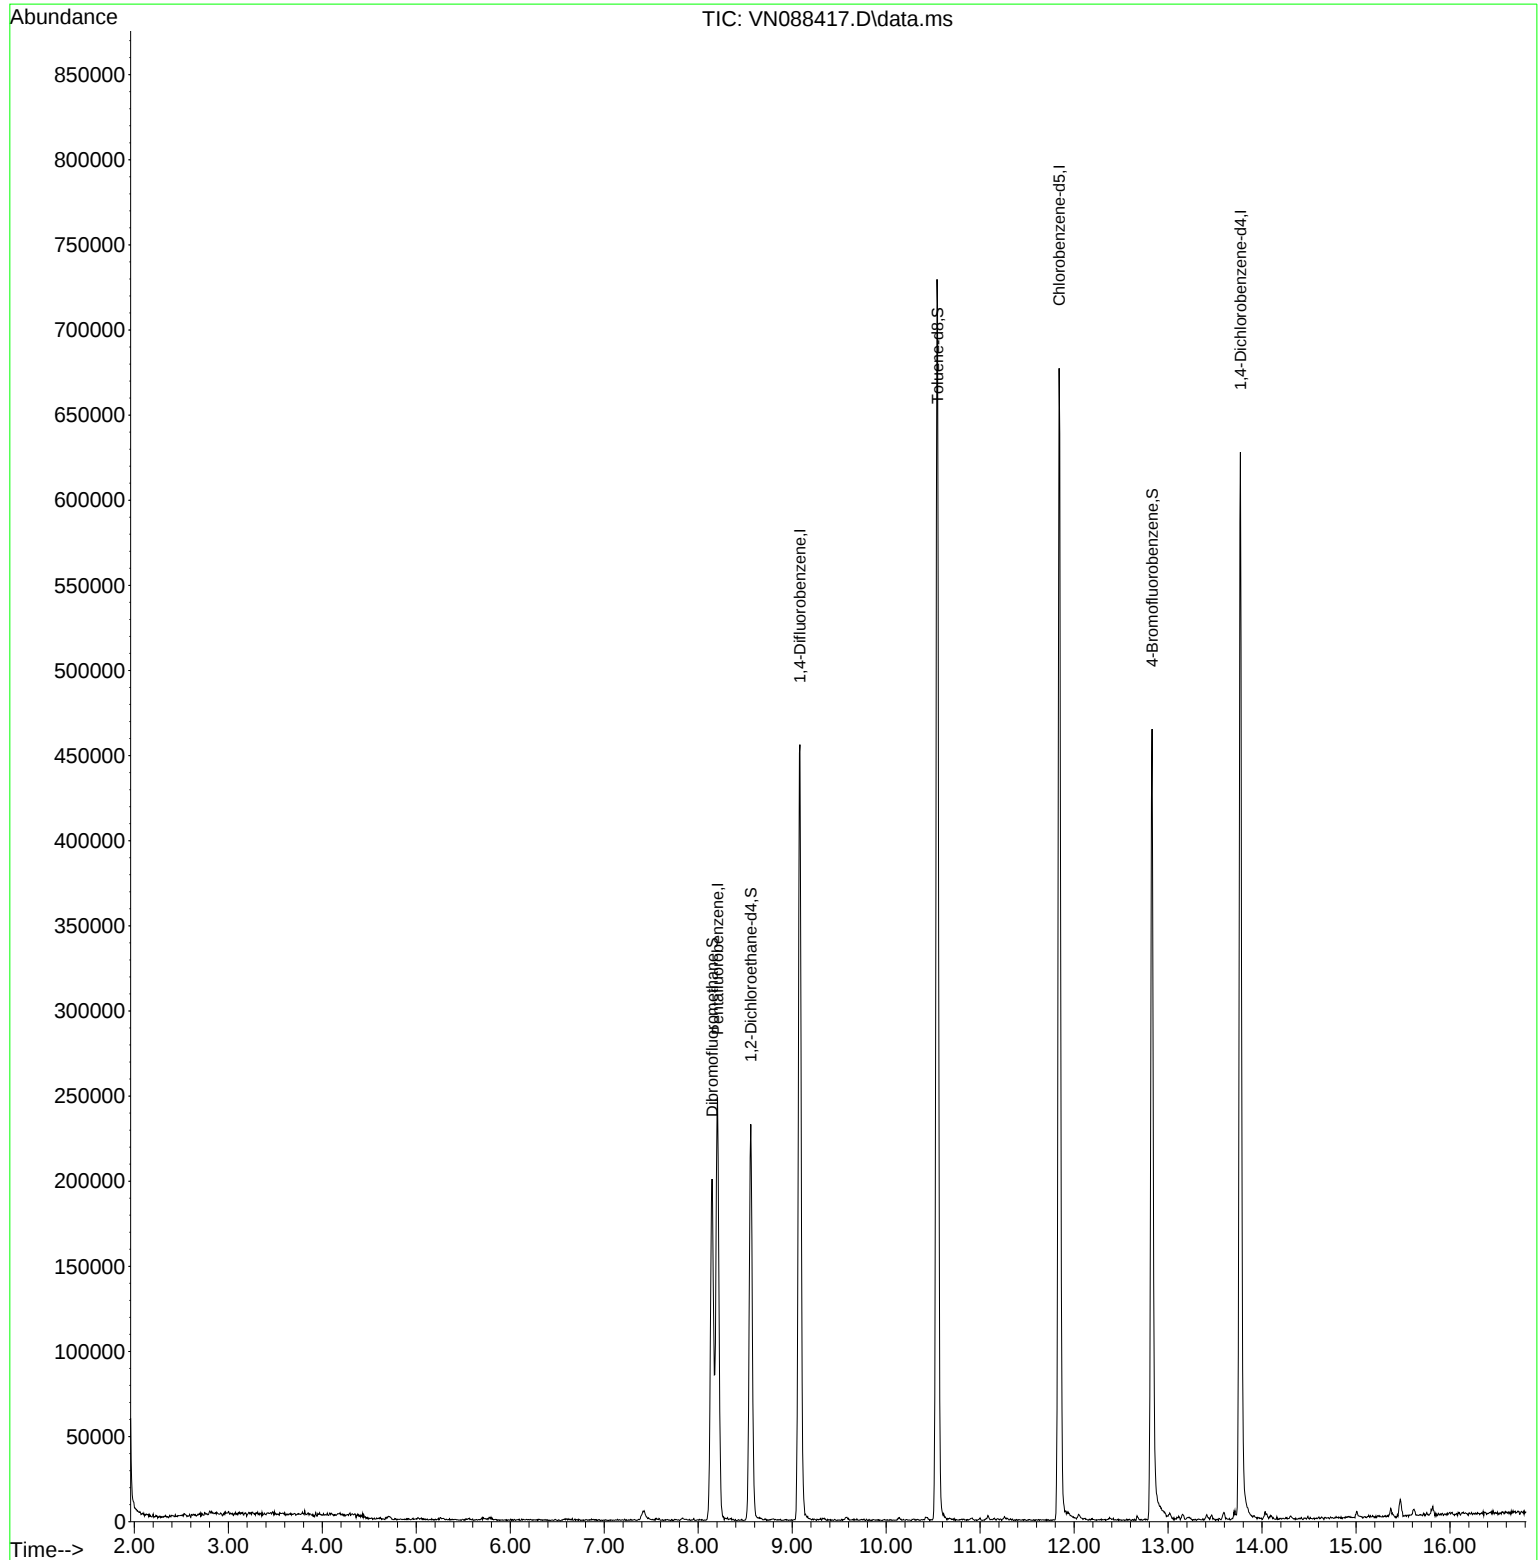


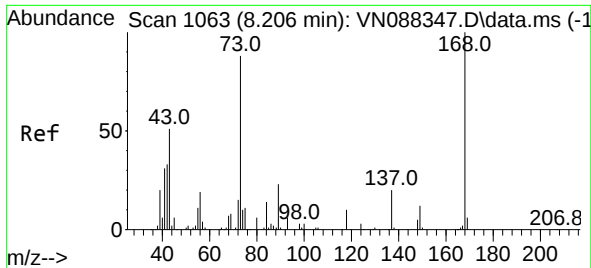

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1063
Delta R.T. 0.000 min
Lab File: VN088417.D
Acq: 03 Dec 2025 10:43




Instrument :
MSVOA_N
ClientSampleId :
VN1203MBL01


Tgt Ion:168 Resp: 157196
Ion Ratio Lower Upper
168 100
99 72.9 57.1 85.7

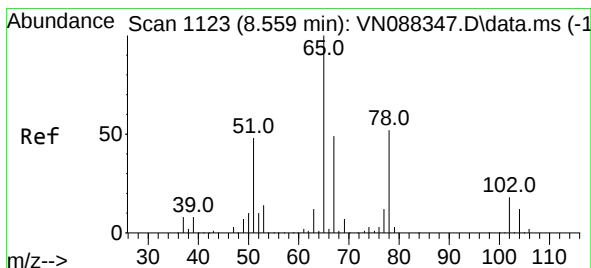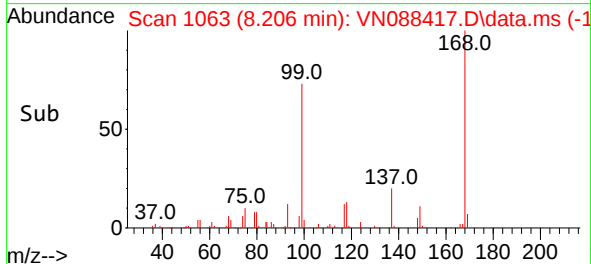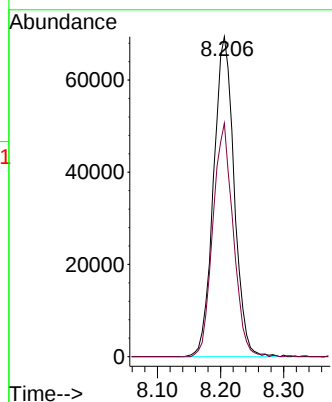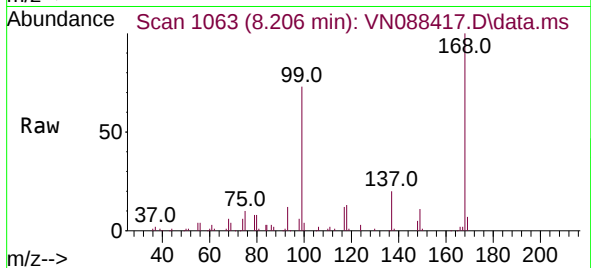

#33
1,2-Dichloroethane-d4
Concen: 66.138 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. 0.000 min
Lab File: VN088417.D
Acq: 03 Dec 2025 10:43

Tgt Ion: 65 Resp: 195853
Ion Ratio Lower Upper
65 100
67 49.5 0.0 100.8

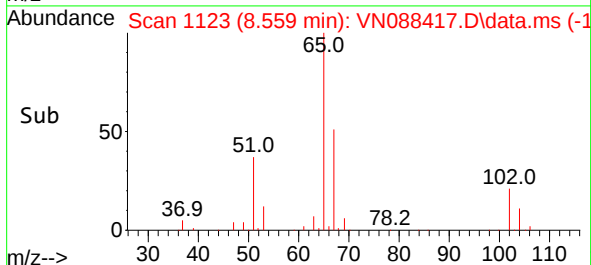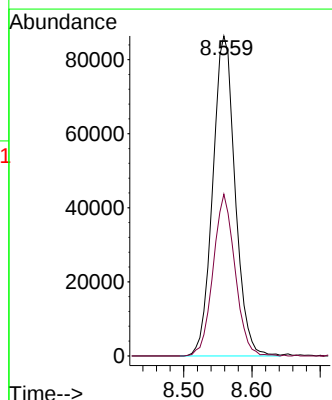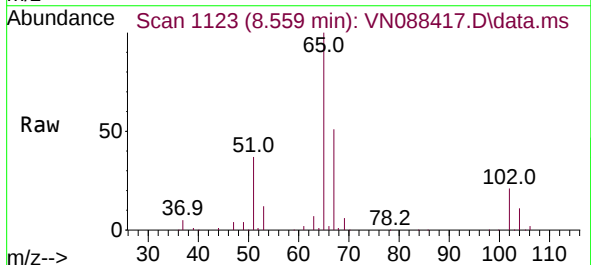

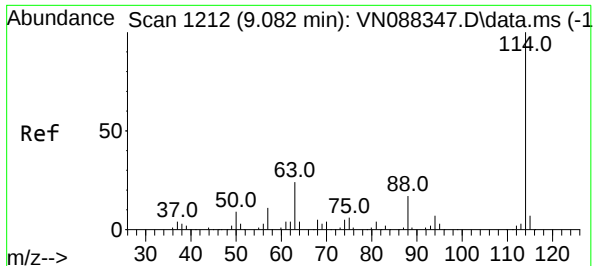

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.082 min Scan# 11

Delta R.T. 0.000 min

Lab File: VN088417.D

Acq: 03 Dec 2025 10:43

Instrument :

MSVOA_N

ClientSampleId :

VN1203MBL01





Tgt Ion:114 Resp: 366654

Ion Ratio Lower Upper

114 100

63 21.5 0.0 49.0

88 16.2 0.0 34.0

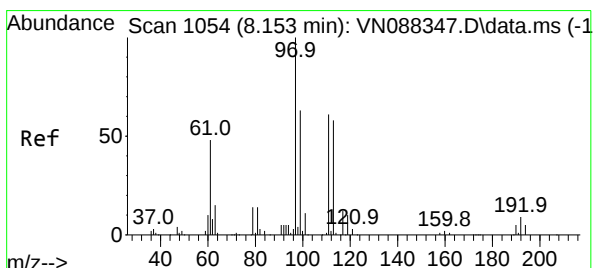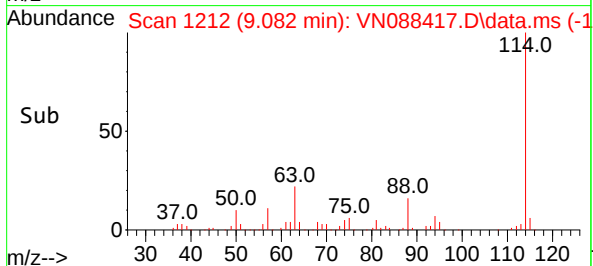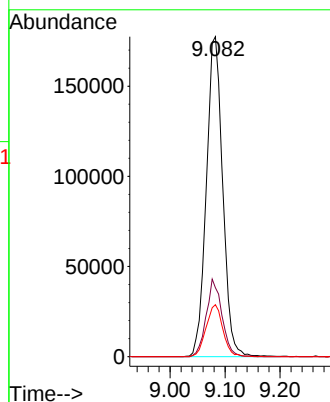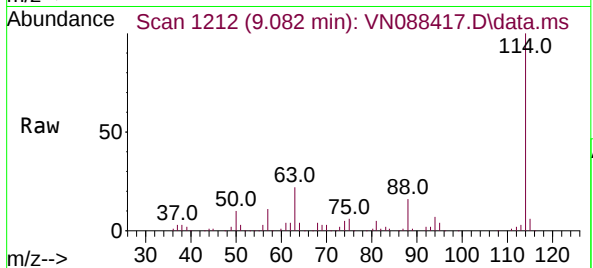

#35

Dibromofluoromethane

Concen: 55.439 ug/l

RT: 8.147 min Scan# 1053

Delta R.T. -0.006 min

Lab File: VN088417.D

Acq: 03 Dec 2025 10:43




Tgt Ion:113 Resp: 140865


Ion Ratio Lower Upper

113 100

111 103.1 82.5 123.7

192 15.6 12.8 19.2


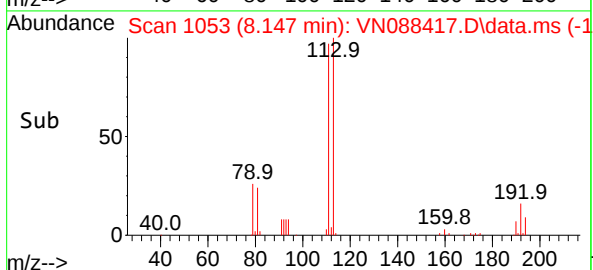
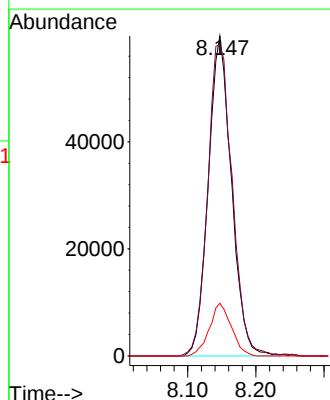
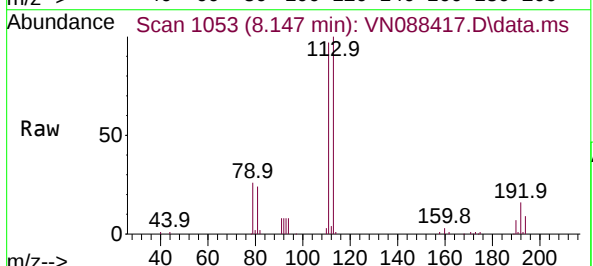


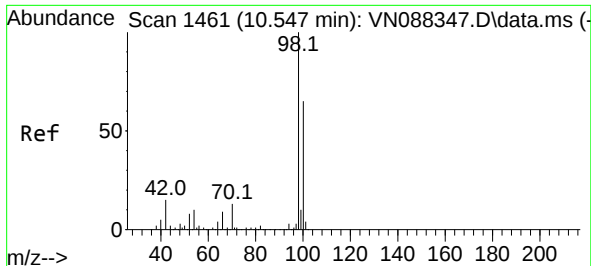

#50
Toluene-d8
Concen: 51.175 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. 0.000 min
Lab File: VN088417.D
Acq: 03 Dec 2025 10:43




Instrument :
MSVOA_N
ClientSampleId :
VN1203MBL01


Tgt Ion: 98 Resp: 483810
Ion Ratio Lower Upper
98 100
100 64.2 52.2 78.2

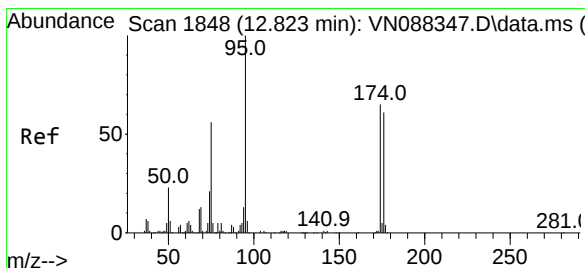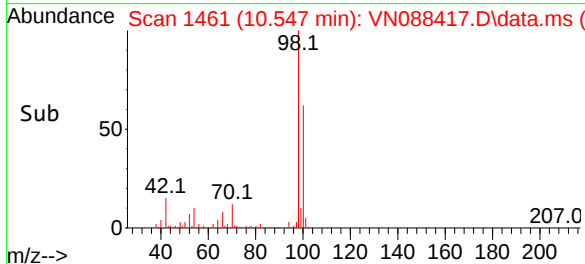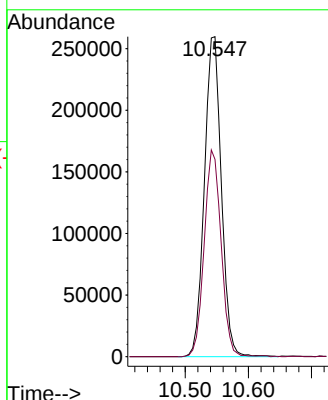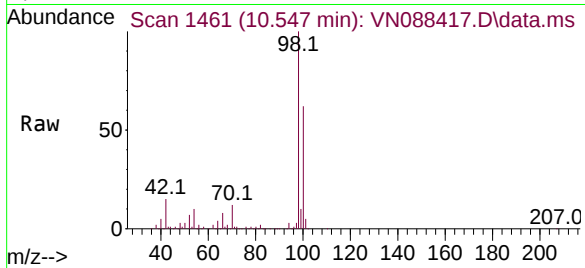

#62
4-Bromofluorobenzene
Concen: 51.549 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN088417.D
Acq: 03 Dec 2025 10:43

Tgt Ion: 95 Resp: 167218
Ion Ratio Lower Upper
95 100
174 70.6 0.0 139.0
176 65.4 0.0 132.4


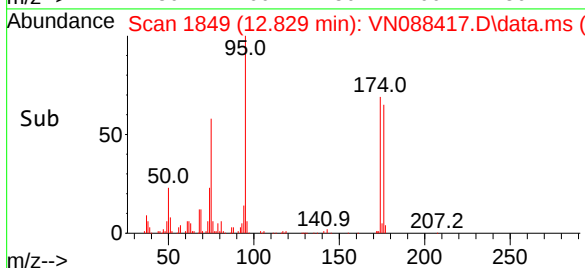
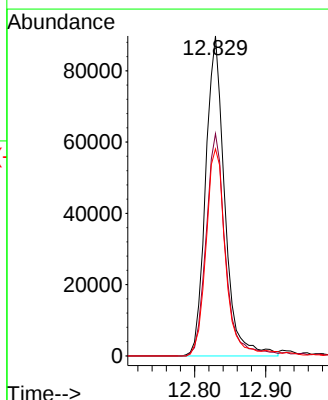
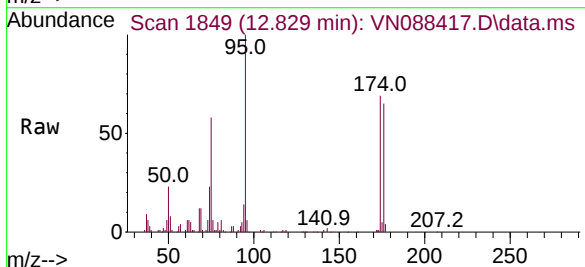


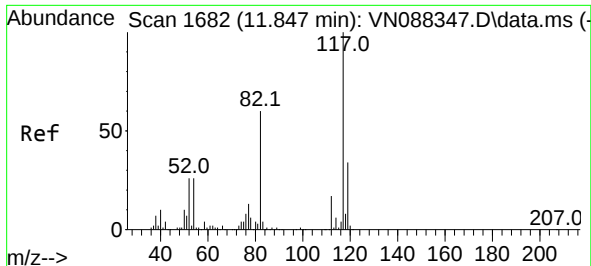

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.841 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN088417.D
Acq: 03 Dec 2025 10:43

Instrument :
MSVOA_N
ClientSampleId :
VN1203MBL01

Tgt Ion:117 Resp: 360665
Ion Ratio Lower Upper
117 100
82 61.1 47.8 71.8
119 31.7 26.9 40.3

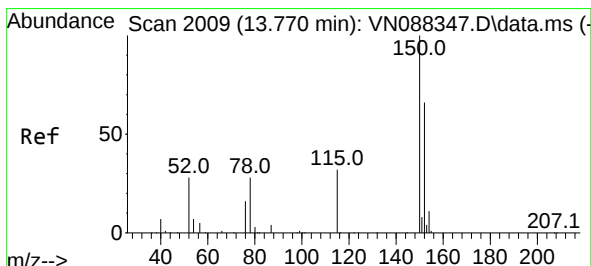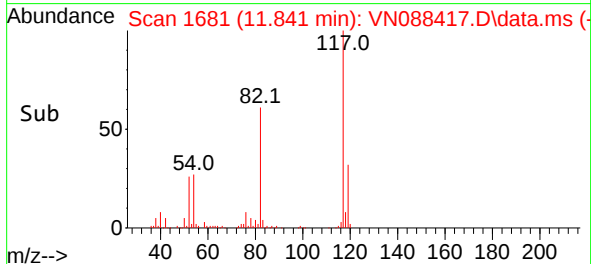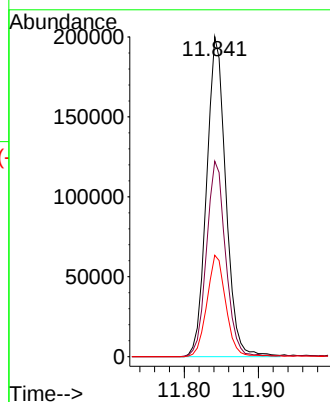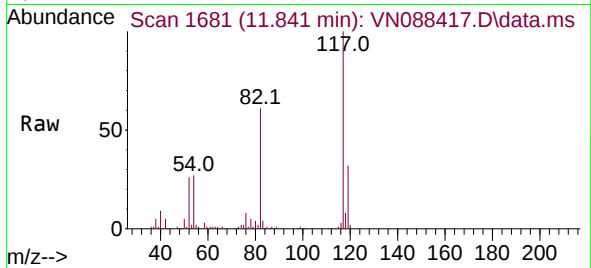

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.000 min
Lab File: VN088417.D
Acq: 03 Dec 2025 10:43

Tgt Ion:152 Resp: 162391
Ion Ratio Lower Upper
152 100
115 67.3 33.0 98.9
150 160.2 0.0 349.0

