
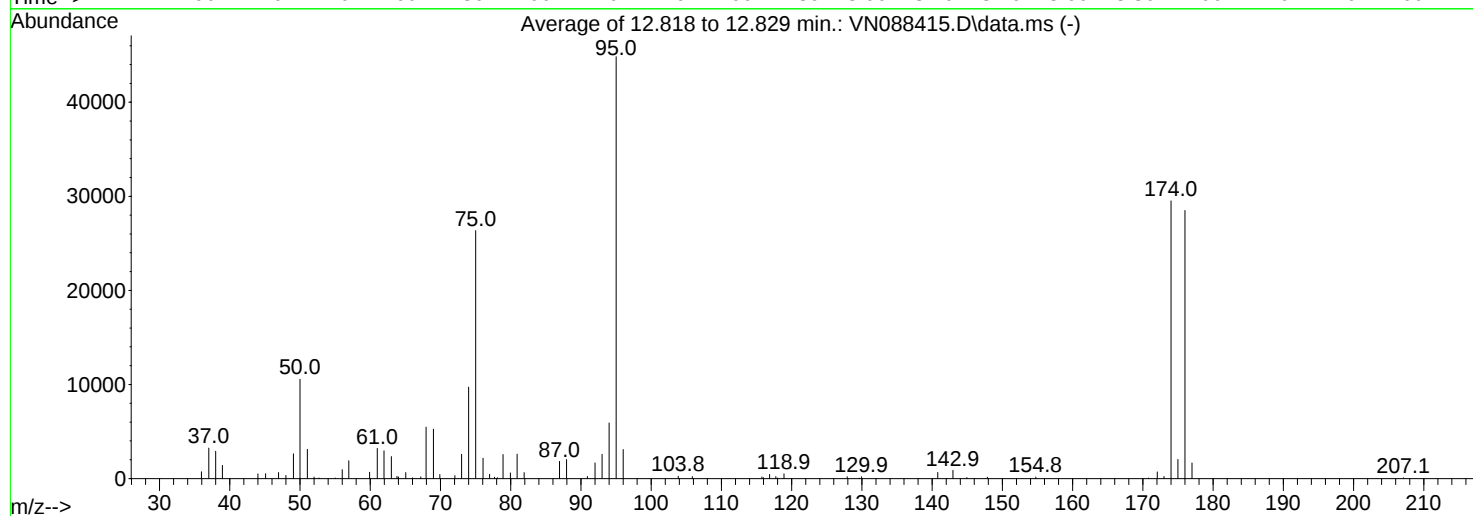


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120325\
Data File : VN088415.D
Acq On : 03 Dec 2025 09:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Title : SW846 8260
Last Update : Tue Nov 25 01:34:52 2025

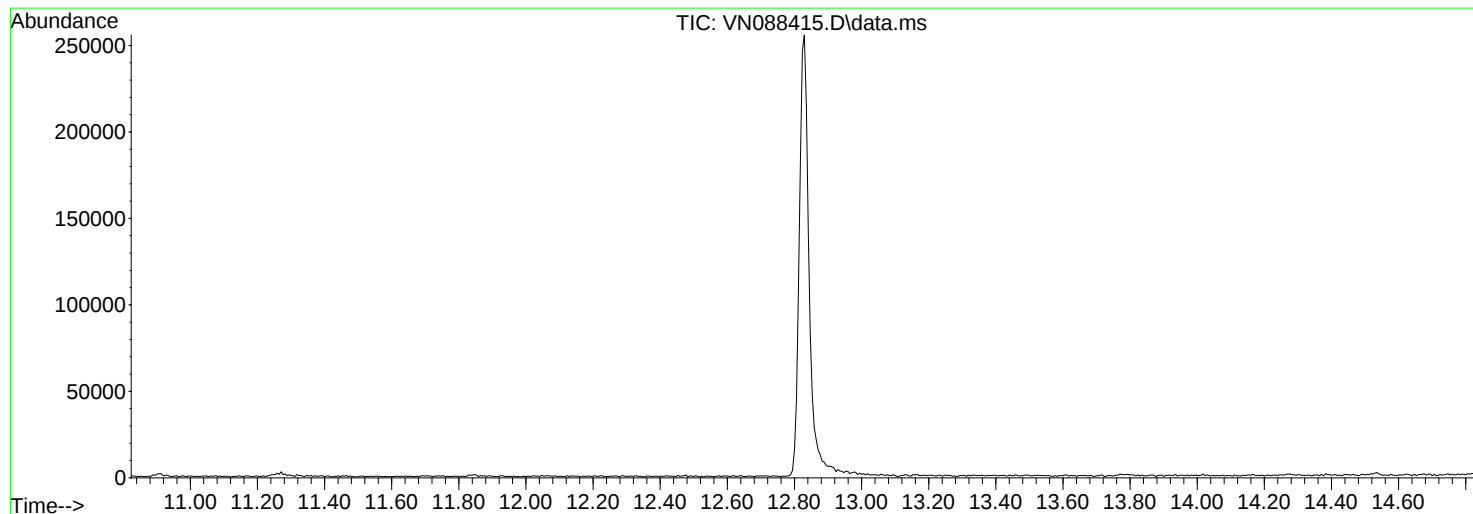

AutoFind: Scans 1847, 1848, 1849; Background Corrected with Scan 1839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	10550	PASS
75	95	30	60	58.8	26344	PASS
95	95	100	100	100.0	44832	PASS
96	95	5	9	6.9	3081	PASS
173	174	0.00	2	0.8	227	PASS
174	95	50	100	65.8	29515	PASS
175	174	5	9	6.9	2028	PASS
176	174	95	101	96.5	28493	PASS
177	176	5	9	5.9	1667	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	718	52.00	171	65.05	636	77.00	457
37.00	3234	52.70	61	66.00	75	77.70	142
38.00	2905	55.00	66	67.20	178	78.10	100
38.95	1396	56.00	952	67.95	5462	78.90	2567
44.00	503	56.95	1893	69.00	5246	79.95	607
45.10	516	59.90	681	69.90	428	80.90	2593
46.95	634	61.00	3199	72.05	309	81.90	636
48.00	340	61.95	2948	73.00	2576	86.95	1823
49.05	2636	63.00	2346	74.00	9727	87.95	2017
50.00	10550	63.80	226	75.00	26344	90.90	235
51.05	3098	64.00	173	76.05	2168	92.00	1665

Average of 12.818 to 12.829 min.: VN088415.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	2581	118.90	507	173.00	227		
94.00	5904	127.90	201	174.00	29515		
95.00	44832	129.60	50	175.00	2028		
96.00	3081	129.95	204	176.00	28493		
103.85	254	140.80	662	177.00	1667		
105.85	210	142.95	872	207.10	82		
115.75	179	144.95	110				
116.00	96	147.85	147				
116.85	441	154.75	165				
117.75	209	170.80	63				
118.00	54	172.05	714				

Instrument :

MSVOA_N

ClientSampleId :

BFB