

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN120418\
 Data File : VN052656.D
 Acq On : 4 Dec 2018 16:00
 Operator : MD\SY
 Sample : PB115293ZHE#02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 PB115293ZHE#02

Quant Time: Dec 05 04:00:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 03 03:24:02 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1137207	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1742371	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1491673	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	494714	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	587927	47.48	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.96%	
35) Dibromofluoromethane	7.59	113	538107	50.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.20%	
50) Toluene-d8	10.09	98	2123761	50.79	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.58%	
62) 4-Bromofluorobenzene	12.40	95	621141	44.21	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.42%	
Target Compounds						
16) Acetone	3.82	43	14966	4.582	ug/l	98
20) Methylene Chloride	4.55	84	83777	6.555	ug/l	98
43) Isopropyl Acetate	8.17	43	58047	3.416	ug/l #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN120418\
Data File : VN052656.D
Acq On : 4 Dec 2018 16:00
Operator : MD\SY
Sample : PB115293ZHE#02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
PB115293ZHE#02

Quant Time: Dec 05 04:00:16 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 03 03:24:02 2018
Response via : Initial Calibration

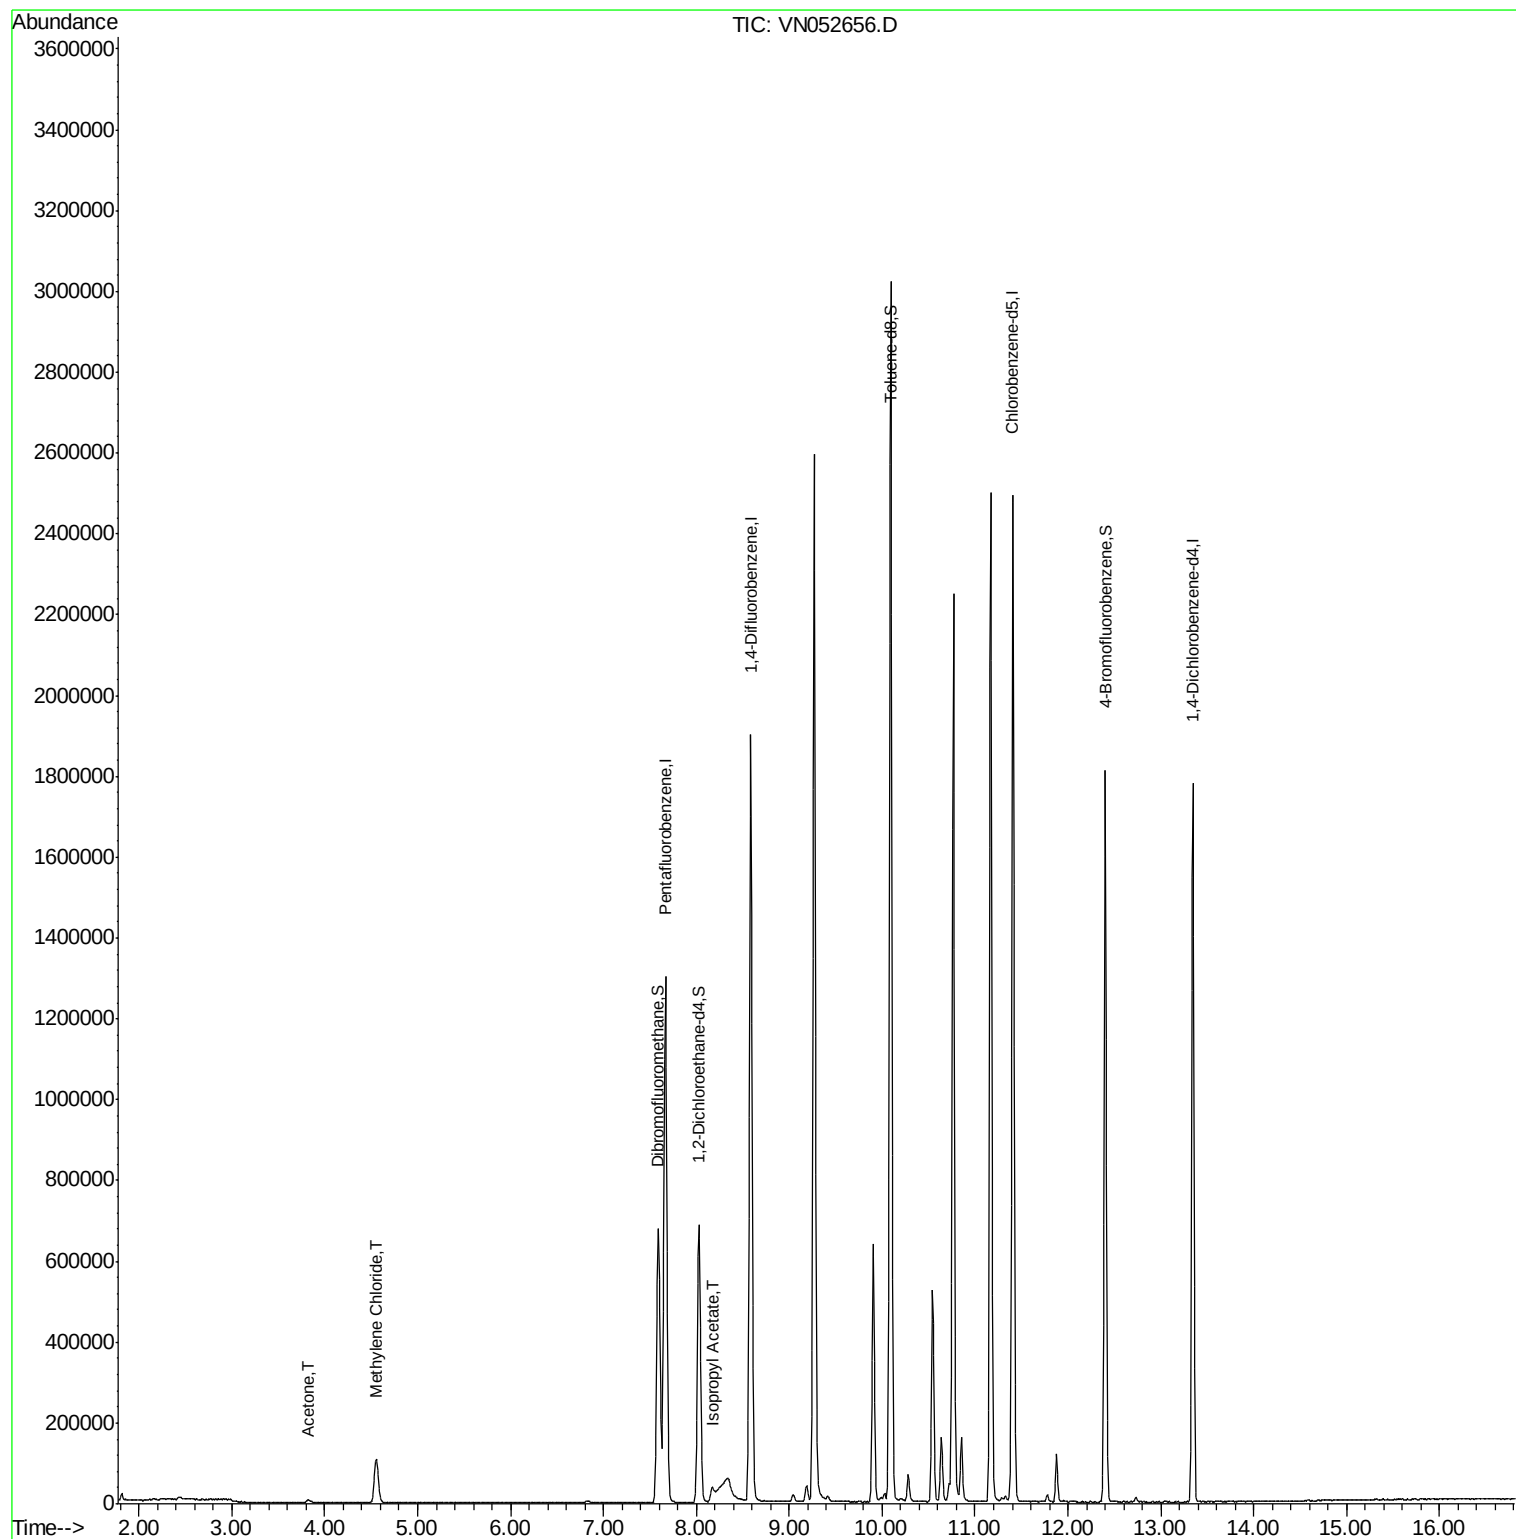

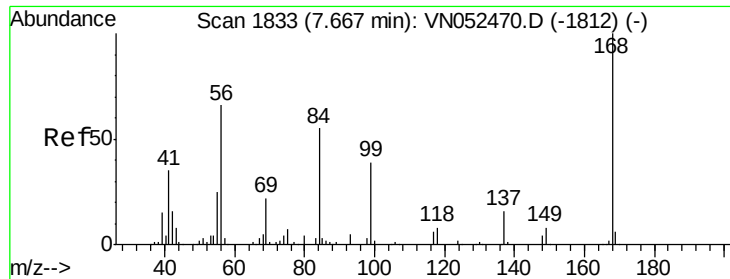

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN052656.D

Acq: 4 Dec 2018 16:00

Instrument :

MSVOA_N

ClientSampleId :


PB115293ZHE#02

Tgt Ion:168 Resp: 1137207

Ion Ratio Lower Upper

168 100

99 51.9 41.7 62.5

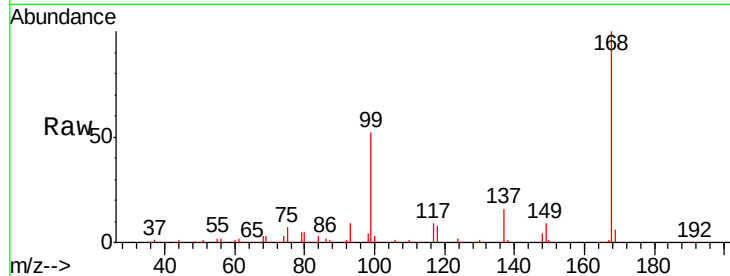

Abundance Ion 167.90 (167.60 to 168.60): VN052470.D

Ion 98.90 (98.60 to 99.60): VN052470.D

7.67

500000

400000



300000

200000

100000

0

Time-->

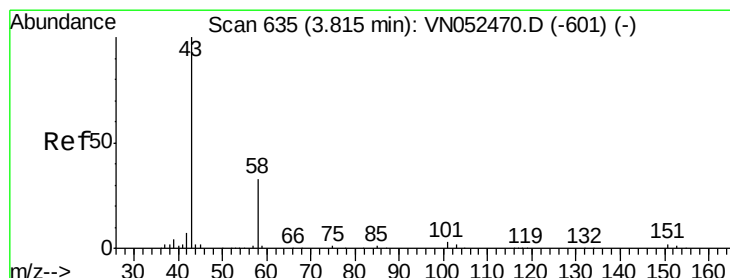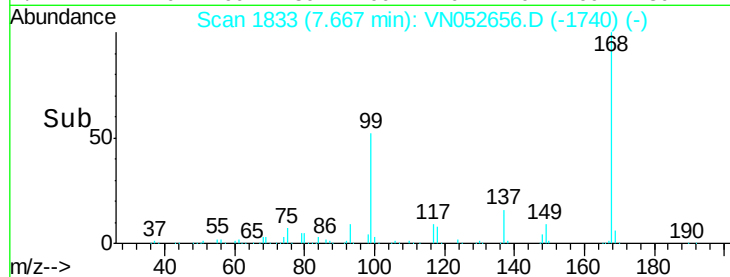

#16

Acetone

Concen: 4.582 ug/l

RT: 3.82 min Scan# 638

Delta R.T. 0.01 min

Lab File: VN052656.D


Acq: 4 Dec 2018 16:00

Tgt Ion: 43 Resp: 14966

Ion Ratio Lower Upper

43 100

58 33.5 26.0 39.0

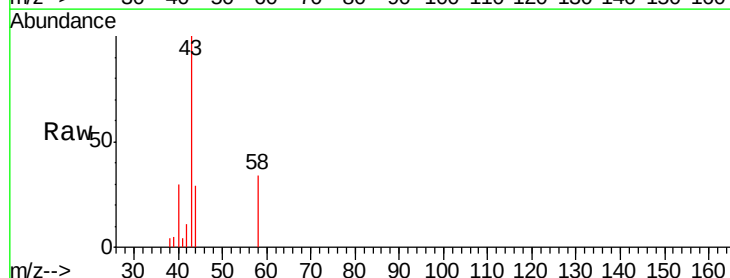

Abundance Ion 43.00 (42.70 to 43.70): VN052470.D

Ion 58.00 (57.70 to 58.70): VN052470.D

3.82

6000

5000

4000


3000


2000

1000

0

Time-->

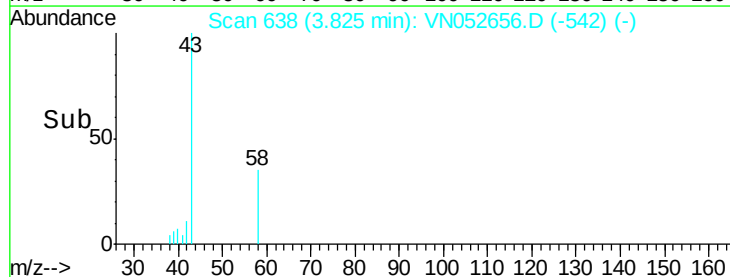

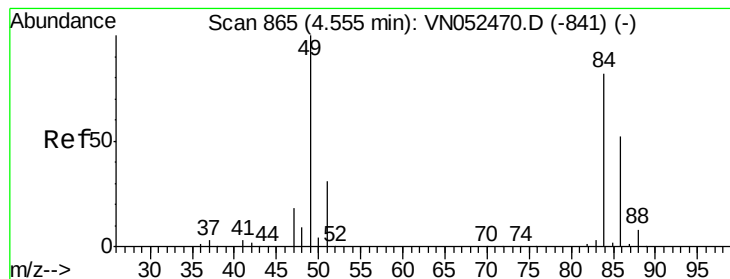

#20

Methylene Chloride

Concen: 6.555 ug/l

RT: 4.55 min Scan# 865

Delta R.T. -0.00 min

Lab File: VN052656.D

Acq: 4 Dec 2018 16:00

Instrument :

MSVOA_N

ClientSampleId :

PB115293ZHE#02

Tgt Ion: 84 Resp: 83777


Ion Ratio Lower Upper

84 100

49 125.1 98.0 147.0

51 38.1 30.1 45.1

86 62.0 50.7 76.1



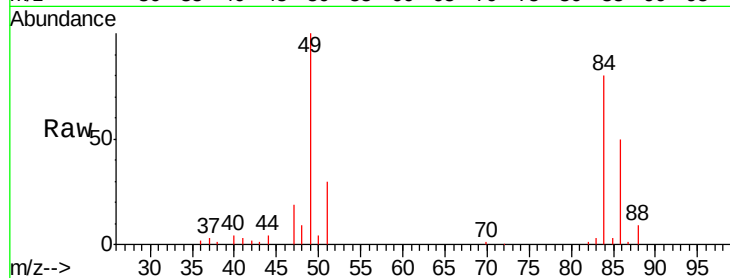


Abundance Ion 83.90 (83.60 to 84.60): VN0

Ion 48.90 (48.60 to 49.60): VN0

Ion 50.90 (50.60 to 51.60): VN0

Ion 85.90 (85.60 to 86.60): VN0

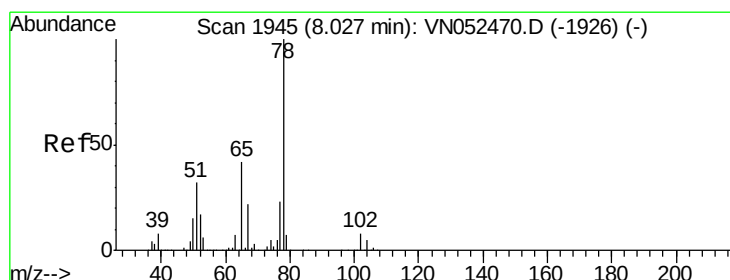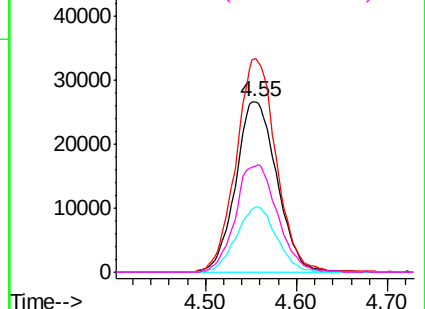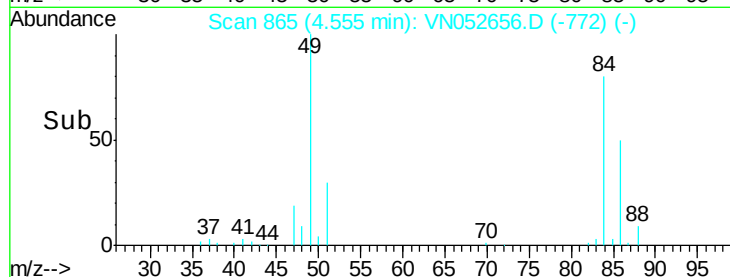

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 8.03 min Scan# 1945

Delta R.T. -0.00 min

Lab File: VN052656.D


Acq: 4 Dec 2018 16:00

Tgt Ion: 65 Resp: 587927

Ion Ratio Lower Upper



65 100


67 54.3 0.0 109.8

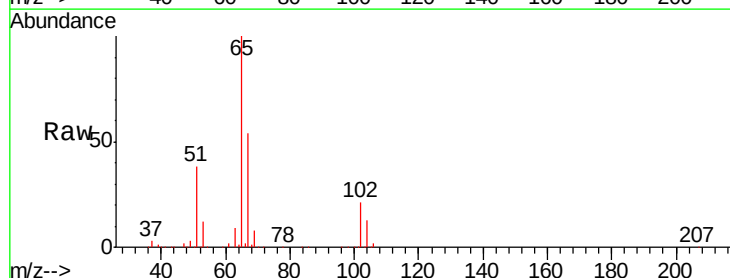

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0



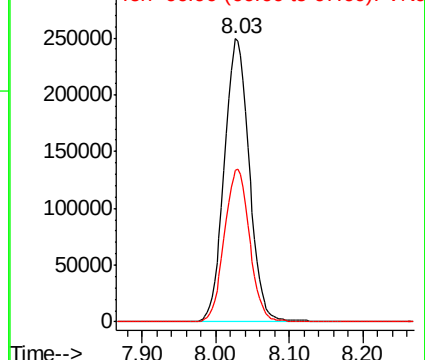
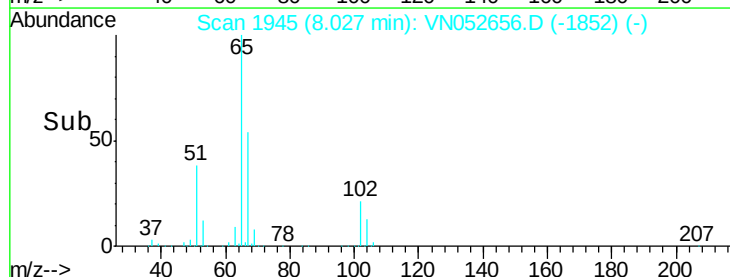


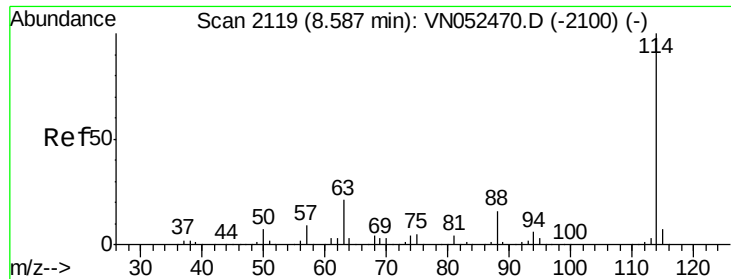

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.59 min Scan# 2119
Delta R.T. -0.00 min
Lab File: VN052656.D
Acq: 4 Dec 2018 16:00




Instrument :
MSVOA_N
ClientSampleId :
PB115293ZHE#02


Tgt Ion:114 Resp: 1742371
Ion Ratio Lower Upper
114 100
63 20.4 0.0 41.8
88 15.5 0.0 31.6

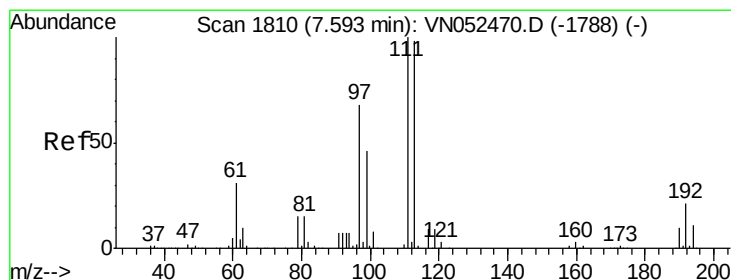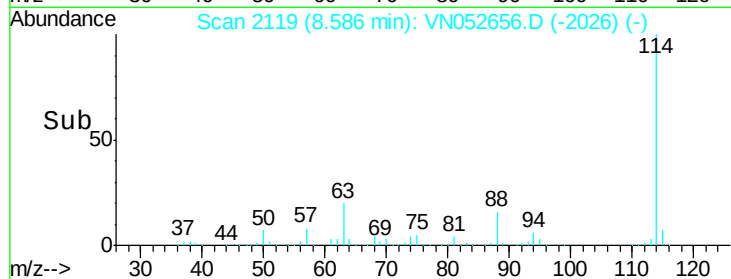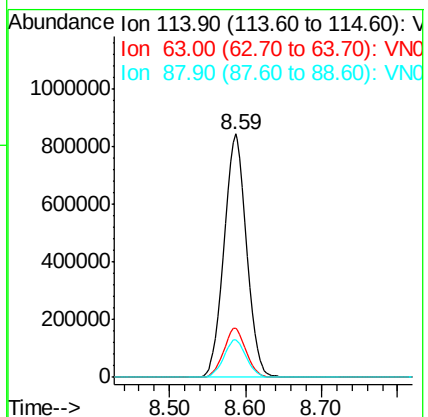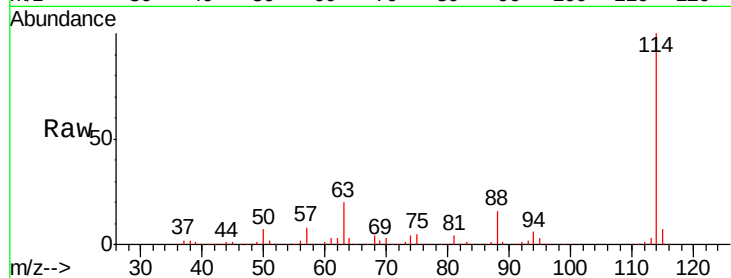

#35
Dibromofluoromethane
Concen: 50.000 ug/l
RT: 7.59 min Scan# 1809
Delta R.T. -0.00 min
Lab File: VN052656.D
Acq: 4 Dec 2018 16:00

Tgt Ion:113 Resp: 538107
Ion Ratio Lower Upper
113 100
111 102.3 82.0 123.0
192 21.6 17.0 25.6

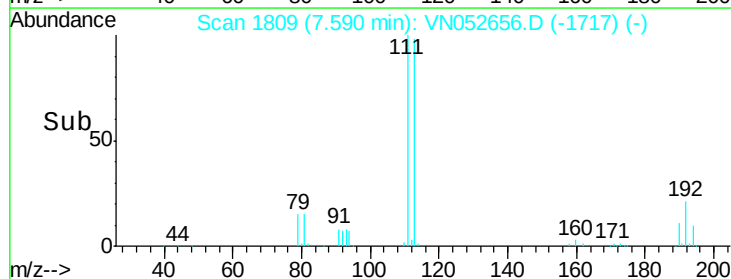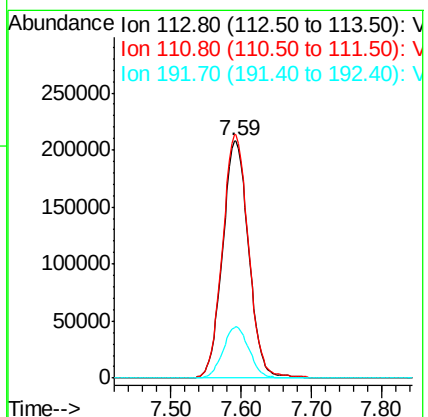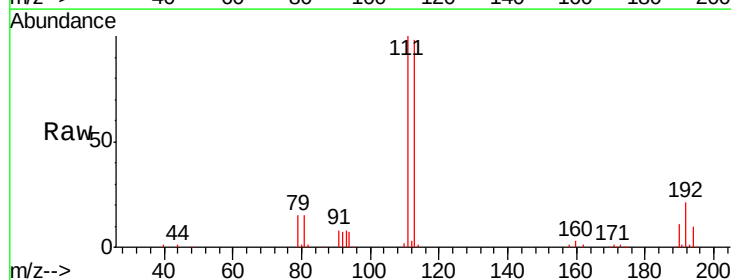

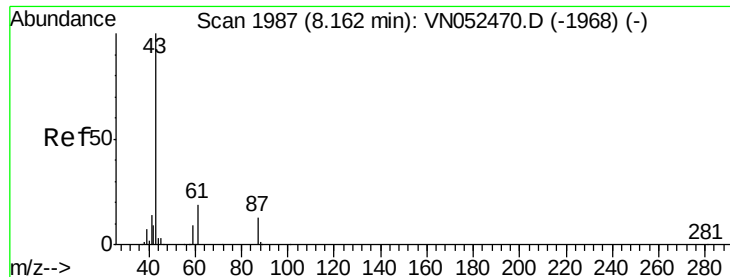

#43

Isopropyl Acetate

Concen: 3.416 ug/l

RT: 8.17 min Scan# 1989

Delta R.T. 0.01 min

Lab File: VN052656.D

Acq: 4 Dec 2018 16:00

Instrument :

MSVOA_N

ClientSampleId :

PB115293ZHE#02


Tgt Ion: 43 Resp: 58047

Ion Ratio Lower Upper

43 100

61 15.7 24.1 36.1#




87 8.5 10.6 15.8#

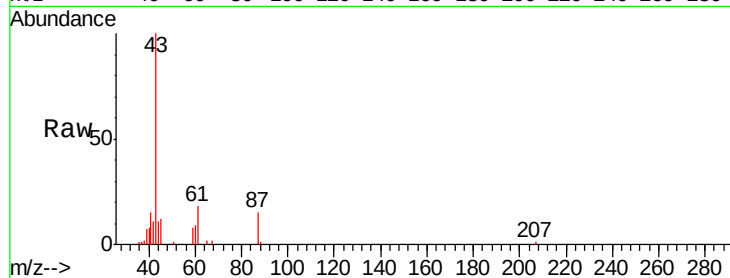

Abundance Ion 43.00 (42.70 to 43.70): VN052470.D (-1968) (-)

Ion 61.00 (60.70 to 61.70): VN052470.D (-1968) (-)

Ion 87.00 (86.70 to 87.70): VN052470.D (-1968) (-)

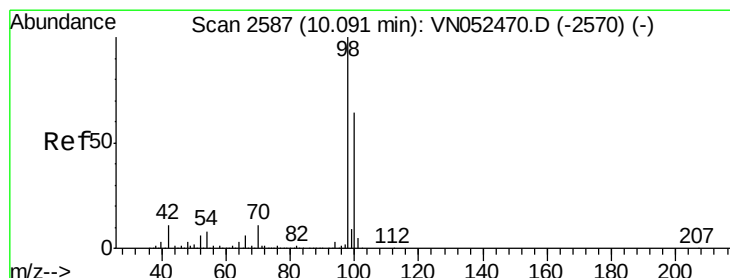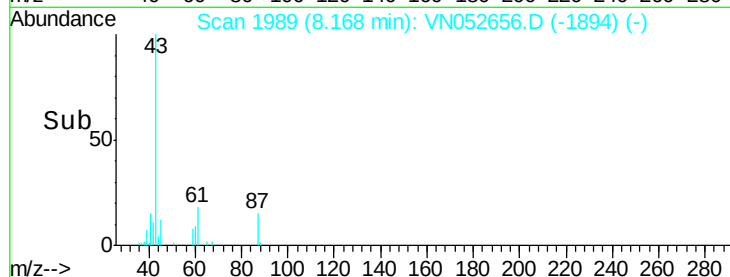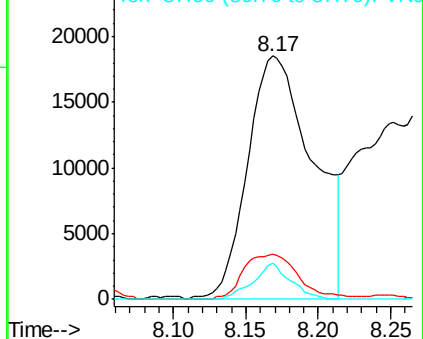

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN052656.D


Acq: 4 Dec 2018 16:00

Tgt Ion: 98 Resp: 2123761

Ion Ratio Lower Upper



98 100


100 64.2 51.3 76.9

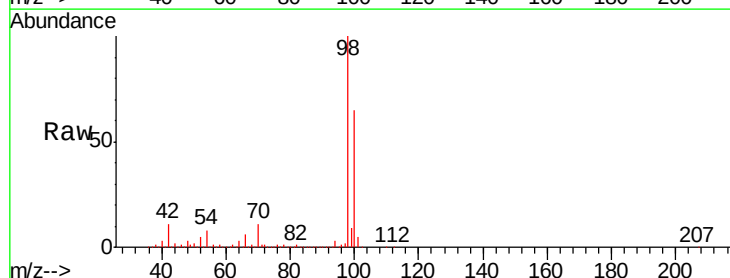

Abundance Ion 98.00 (97.70 to 98.70): VN052470.D (-2570) (-)

Ion 100.00 (99.70 to 100.70): VN052470.D (-2570) (-)

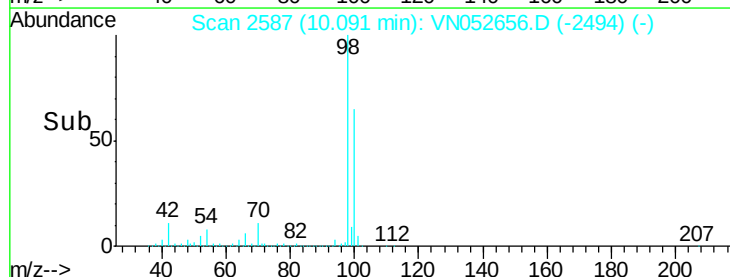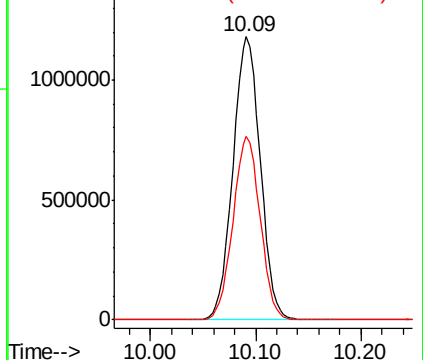

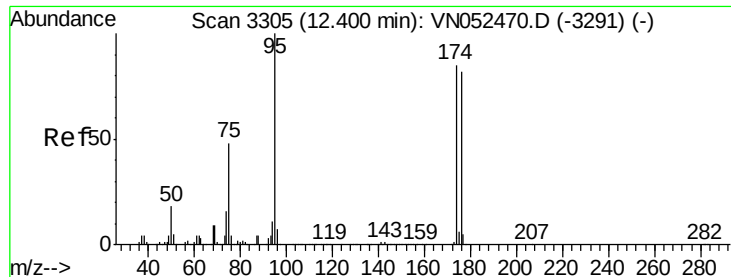

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN052656.D

Acq: 4 Dec 2018 16:00

Instrument :

MSVOA_N

ClientSampleId :

PB115293ZHE#02





Tgt Ion: 95 Resp: 621141

Ion Ratio Lower Upper

95 100

174 87.9 0.0 173.0

176 85.1 0.0 166.2

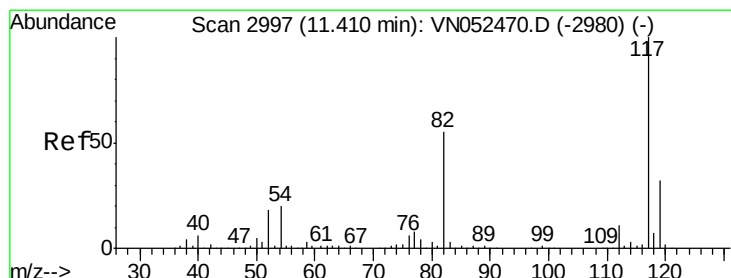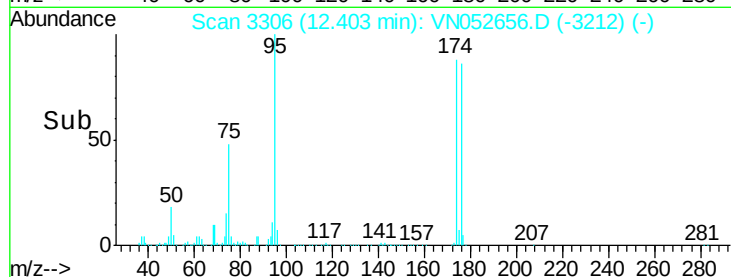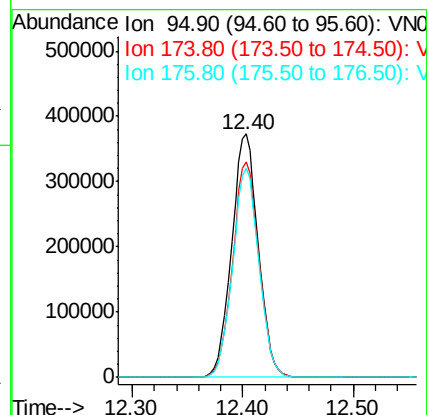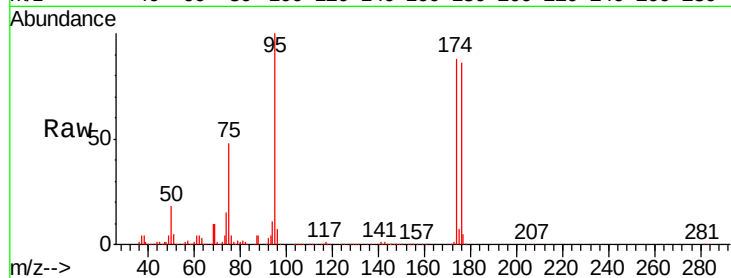

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. -0.00 min

Lab File: VN052656.D

Acq: 4 Dec 2018 16:00




Tgt Ion: 117 Resp: 1491673


Ion Ratio Lower Upper

117 100

82 54.1 43.6 65.4

119 32.0 25.4 38.2

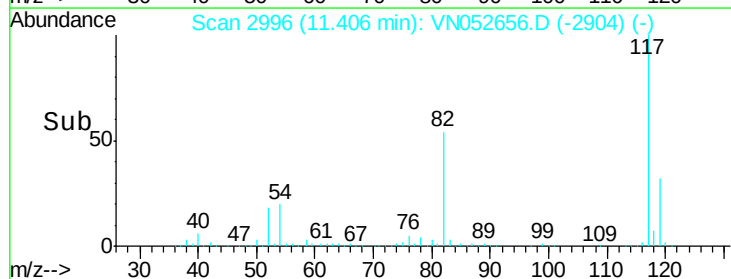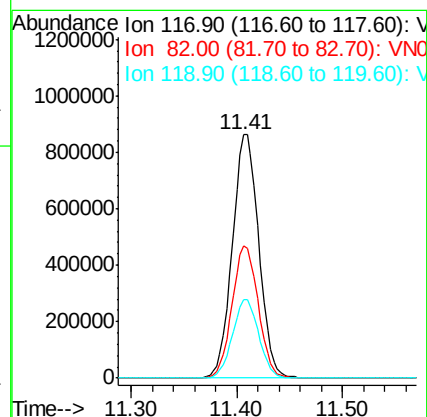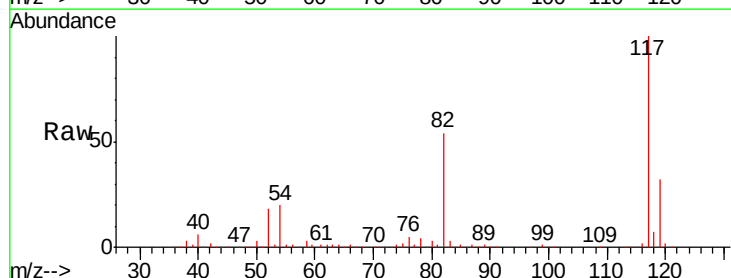

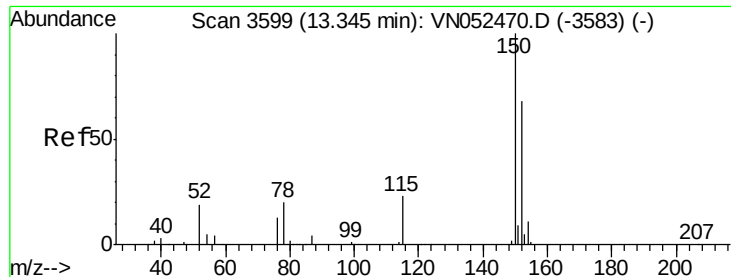

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3599

Delta R.T. -0.00 min

Lab File: VN052656.D


Acq: 4 Dec 2018 16:00

Instrument :

MSVOA_N

ClientSampleId :

PB115293ZHE#02

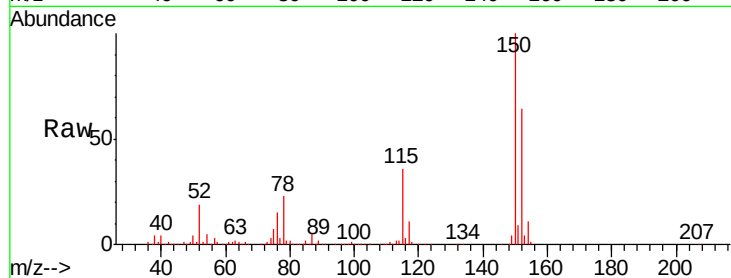


Tgt Ion:152 Resp: 494714

Ion Ratio Lower Upper

152 100

115 56.6 28.4 85.2

150 157.5 0.0 346.0

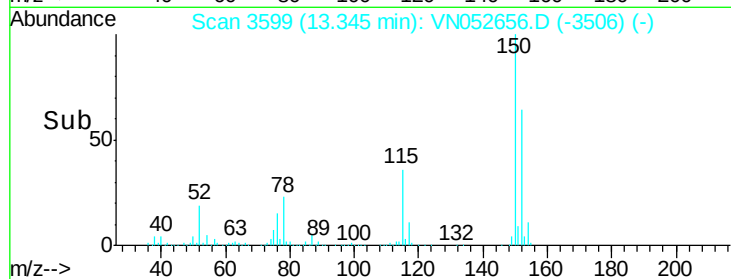

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

