


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120418\
 Data File : VN052644.D
 Acq On : 4 Dec 2018 9:38
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
 Title : SW846 8260
 Last Update : Mon Dec 03 03:24:02 2018

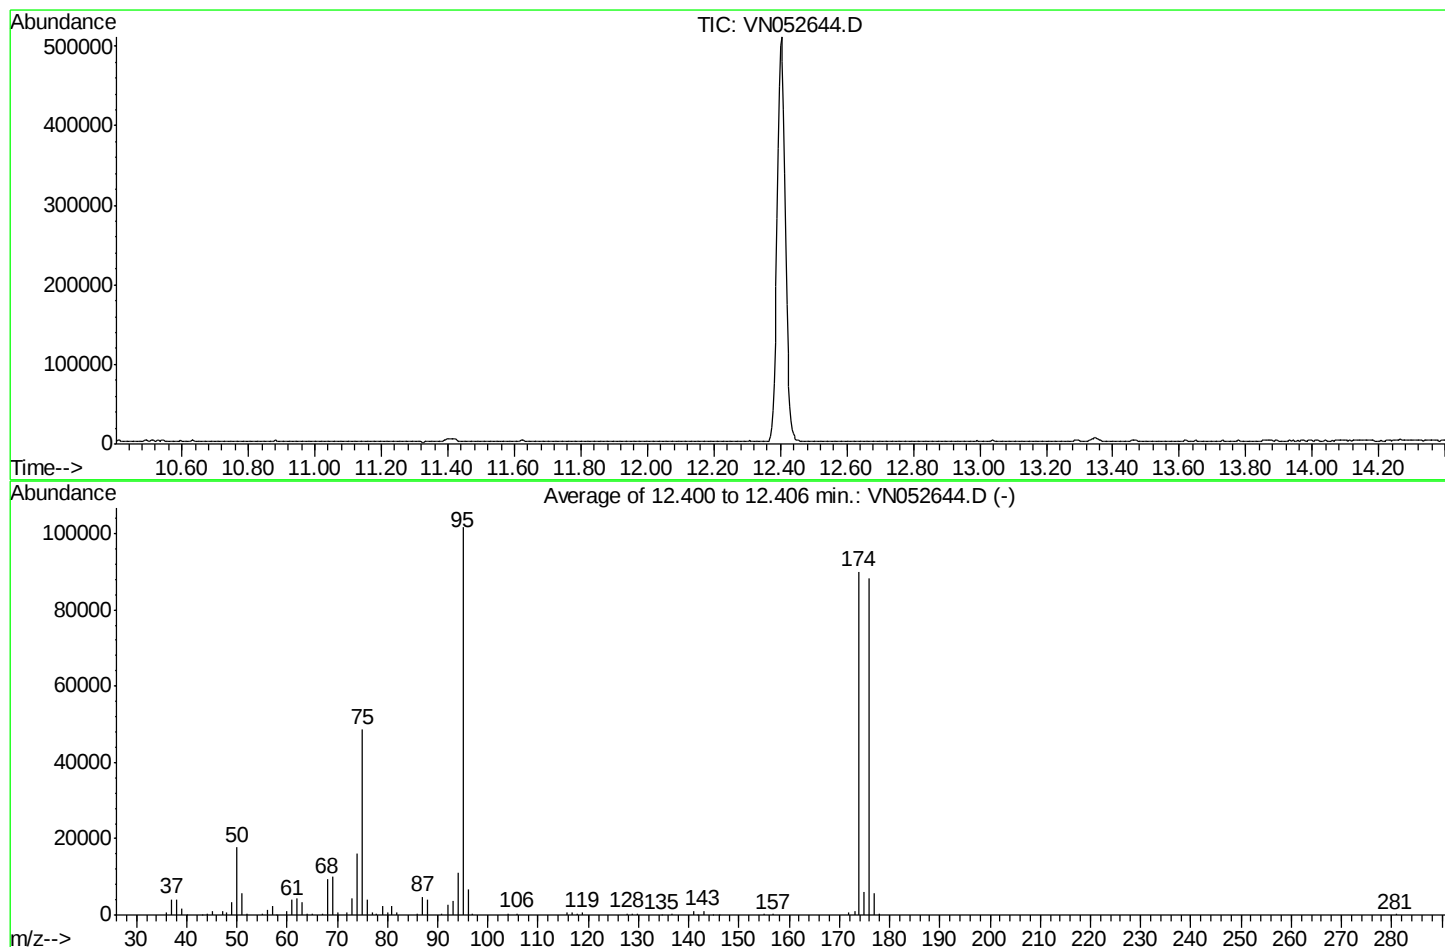

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	17650	PASS
75	95	30	60	47.7	48525	PASS
95	95	100	100	100.0	101645	PASS
96	95	5	9	6.5	6578	PASS
173	174	0.00	2	1.0	943	PASS
174	95	50	100	88.6	90042	PASS
175	174	5	9	6.8	6112	PASS
176	174	95	101	98.0	88253	PASS
177	176	5	9	6.3	5568	PASS