

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120420\
 Data File : VN064927.D
 Acq On : 4 Dec 2020 18:30
 Operator : JC/MD
 Sample : L4954-10
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SS013-13-6714-120120

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.029	694	712	734	rBV	8248	24127	2.33%	0.311%
2	4.473	834	850	851	rBV4	7378	11232	1.09%	0.145%
3	4.997	995	1013	1034	rBV6	13273	45791	4.43%	0.591%
4	6.576	1489	1504	1505	rBV4	6798	10701	1.04%	0.138%
5	6.782	1553	1568	1586	rVB5	4120	12490	1.21%	0.161%
6	7.341	1729	1742	1761	rVB5	6176	17547	1.70%	0.226%
7	7.550	1788	1807	1818	rBV2	124238	312829	30.27%	4.037%
8	7.624	1818	1830	1845	rVV	211590	512532	49.59%	6.614%
9	7.704	1846	1855	1872	rVB4	24394	58516	5.66%	0.755%
10	7.840	1883	1897	1904	rBV6	7966	18695	1.81%	0.241%
11	7.894	1905	1914	1927	rVB5	9528	22743	2.20%	0.293%
12	7.991	1927	1944	1969	rBV3	150056	381049	36.87%	4.917%
13	8.119	1969	1984	1996	rBV5	19907	47527	4.60%	0.613%
14	8.193	1996	2007	2019	rVV6	11914	26311	2.55%	0.340%
15	8.261	2020	2028	2042	rVB7	6491	14402	1.39%	0.186%
16	8.550	2098	2118	2139	rBV	329316	684446	66.22%	8.833%
17	9.013	2248	2262	2268	rBV5	19412	43198	4.18%	0.557%
18	9.331	2340	2361	2373	rVB5	18074	41528	4.02%	0.536%
19	9.479	2394	2407	2420	rVB4	26457	51658	5.00%	0.667%
20	9.630	2443	2454	2461	rBV4	6446	12350	1.19%	0.159%
21	9.810	2499	2510	2521	rBV5	20117	44691	4.32%	0.577%
22	9.865	2522	2527	2541	rVB4	5322	10722	1.04%	0.138%
23	10.058	2571	2587	2612	rBV	560352	1033632	100.00%	13.339%
24	10.222	2616	2638	2657	rVB4	38429	95897	9.28%	1.238%
25	10.402	2680	2694	2707	rVB2	77385	146790	14.20%	1.894%
26	10.502	2707	2725	2734	rBV5	29347	58501	5.66%	0.755%
27	10.891	2829	2846	2852	rBV5	20693	42465	4.11%	0.548%
28	10.978	2863	2873	2883	rVV2	56461	97048	9.39%	1.252%
29	11.032	2883	2890	2897	rVB5	8761	12088	1.17%	0.156%
30	11.081	2897	2905	2917	rVB8	6686	13092	1.27%	0.169%
31	11.183	2927	2937	2957	rVB4	14130	27136	2.63%	0.350%
32	11.380	2984	2998	3014	rBV	530885	916828	88.70%	11.831%
33	11.470	3016	3026	3034	rVV4	22909	44732	4.33%	0.577%
34	11.515	3034	3040	3048	rVB4	10606	16990	1.64%	0.219%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120420\
 Data File : VN064927.D
 Acq On : 4 Dec 2020 18:30
 Operator : JC/MD
 Sample : L4954-10
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SS013-13-6714-120120

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
 Title : SW846 8260

35	11.627	3063	3075	3097	rVB9	31164	91158	8.82%	1.176%
36	11.788	3116	3125	3133	rBV3	10550	18026	1.74%	0.233%
37	11.891	3144	3157	3167	rBV7	16700	39237	3.80%	0.506%
38	11.945	3167	3174	3181	rVB4	8096	13828	1.34%	0.178%
39	12.090	3212	3219	3228	rVB5	19612	33112	3.20%	0.427%
40	12.222	3250	3260	3270	rVB	47627	82715	8.00%	1.067%
41	12.376	3295	3308	3321	rBV	429994	719254	69.59%	9.282%
42	12.447	3323	3330	3340	rVB6	9583	14148	1.37%	0.183%
43	12.537	3351	3358	3364	rBV7	13911	21349	2.07%	0.276%
44	12.698	3400	3408	3417	rVV10	5502	10652	1.03%	0.137%
45	12.933	3471	3481	3488	rBV9	14720	29502	2.85%	0.381%
46	13.142	3534	3546	3555	rBV3	36261	72281	6.99%	0.933%
47	13.190	3556	3561	3574	rVB10	6309	14023	1.36%	0.181%
48	13.315	3588	3600	3620	rBV	513149	919164	88.93%	11.862%
49	13.418	3625	3632	3639	rBV2	8144	10889	1.05%	0.141%
50	13.486	3645	3653	3659	rBV	25320	39897	3.86%	0.515%
51	13.518	3659	3663	3670	rVB2	17825	22625	2.19%	0.292%
52	13.566	3670	3678	3691	rVB3	19228	30929	2.99%	0.399%
53	13.640	3691	3701	3711	rVB6	19780	35619	3.45%	0.460%
54	13.714	3711	3724	3732	rBV	19211	30987	3.00%	0.400%
55	13.775	3733	3743	3747	rBV9	7790	13671	1.32%	0.176%
56	13.807	3747	3753	3761	rVB4	10867	15450	1.49%	0.199%
57	13.862	3763	3770	3778	rVB4	14304	20524	1.99%	0.265%
58	13.920	3778	3788	3794	rBV	18207	31362	3.03%	0.405%
59	13.965	3795	3802	3811	rVB3	30586	48812	4.72%	0.630%
60	14.100	3834	3844	3853	rBV5	26119	42059	4.07%	0.543%
61	14.219	3877	3881	3890	rVB	13070	16827	1.63%	0.217%
62	14.267	3890	3896	3901	rBV3	8724	12868	1.24%	0.166%
63	14.299	3903	3906	3912	rVV6	11269	13006	1.26%	0.168%
64	14.402	3926	3938	3945	rVB5	12938	24590	2.38%	0.317%
65	14.457	3945	3955	3963	rBV6	17657	32477	3.14%	0.419%
66	14.498	3963	3968	3976	rVB5	8623	12403	1.20%	0.160%
67	14.563	3976	3988	4001	rBV4	37887	94562	9.15%	1.220%
68	14.630	4001	4009	4018	rVB8	8034	13935	1.35%	0.180%
69	14.823	4063	4069	4074	rBV5	12206	16886	1.63%	0.218%
70	14.859	4075	4080	4086	rVB3	7500	10890	1.05%	0.141%
71	14.929	4092	4102	4112	rVB3	38983	80445	7.78%	1.038%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120420\
Data File : VN064927.D
Acq On : 4 Dec 2020 18:30
Operator : JC/MD
Sample : L4954-10
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SS013-13-6714-120120

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Title : SW846 8260

72	15.016	4122	4129	4135	rBV2	9678	11221	1.09%	0.145%
73	15.225	4183	4194	4197	rBV9	11409	19856	1.92%	0.256%
74	15.447	4255	4263	4276	rVB9	8542	17204	1.66%	0.222%
75	15.871	4383	4395	4407	rBV4	11457	21920	2.12%	0.283%
76	16.309	4519	4531	4544	rBV4	7627	18488	1.79%	0.239%


Sum of corrected areas: 7749135

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN120420\
Data File : VN064927.D
Acq On : 4 Dec 2020 18:30
Operator : JC/MD
Sample : L4954-10
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SS013-13-6714-120120

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

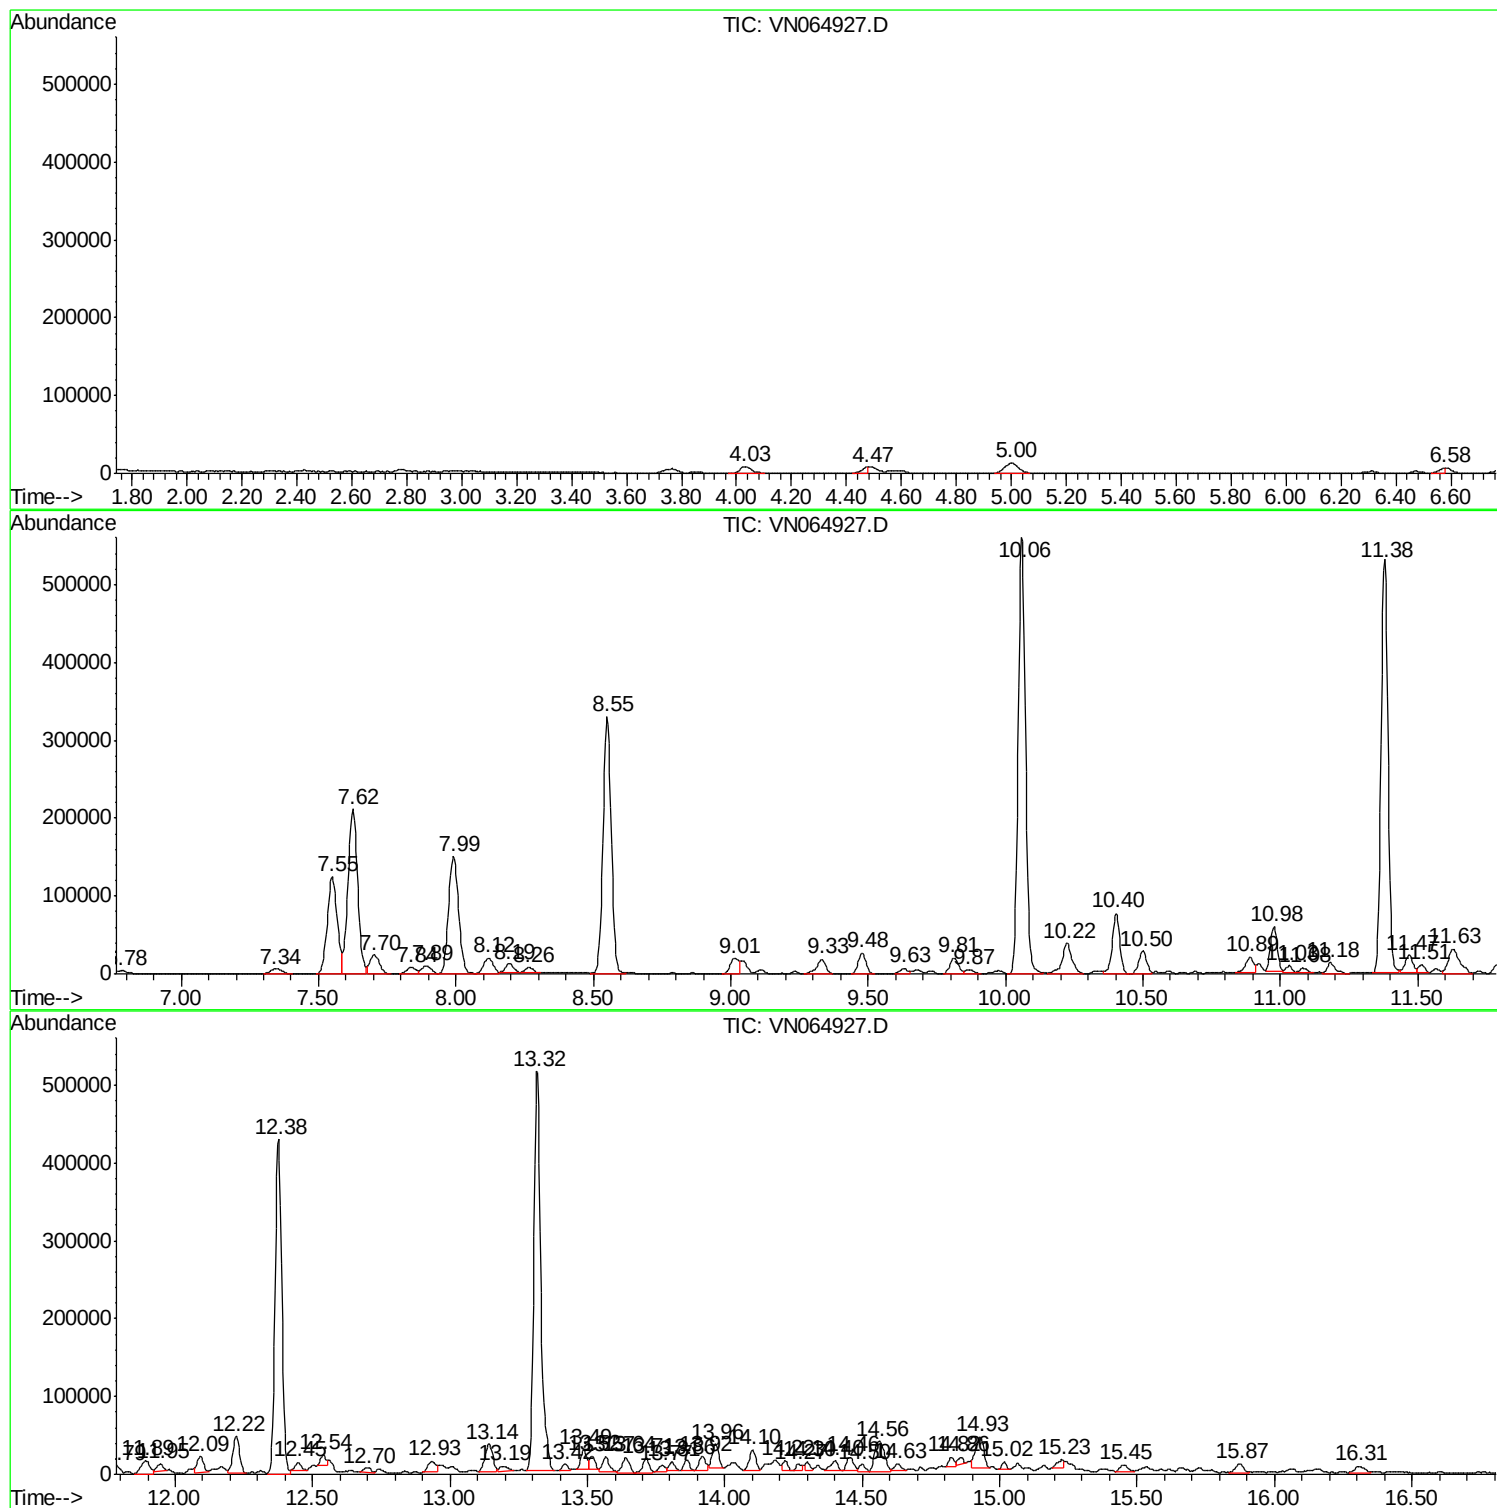

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN120420\
Data File : VN064927.D
Acq On : 4 Dec 2020 18:30
Operator : JC/MD
Sample : L4954-10
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SS013-13-6714-120120

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN120420\
Data File : VN064927.D
Acq On : 4 Dec 2020 18:30
Operator : JC/MD
Sample : L4954-10
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SS013-13-6714-120120

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc