

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120420\
 Data File : VN064928.D
 Acq On : 4 Dec 2020 18:54
 Operator : JC/MD
 Sample : L4954-11
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SS013-13-6712-120120

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.775	306	322	343	rBV	463224	956548	5.88%	0.895%
2	3.107	409	425	444	rBV	308469	660205	4.06%	0.618%
3	3.756	606	627	651	rBV3	106450	325116	2.00%	0.304%
4	4.486	832	854	856	rBV3	157677	365458	2.25%	0.342%
5	4.576	862	882	923	rVB4	522571	2683792	16.50%	2.512%
6	5.000	985	1014	1061	rBV	528499	1910009	11.75%	1.788%
7	5.518	1154	1175	1200	rVB2	74454	233735	1.44%	0.219%
8	6.579	1484	1505	1547	rVB	1015851	3222753	19.82%	3.017%
9	7.344	1727	1743	1768	rVB3	65050	188667	1.16%	0.177%
10	7.614	1784	1827	1844	rBV7	1193975	3873833	23.82%	3.627%
11	7.701	1844	1854	1875	rVB2	191162	497329	3.06%	0.466%
12	7.836	1877	1896	1907	rBV	313583	774454	4.76%	0.725%
13	7.987	1929	1943	1965	rVB	128358	306921	1.89%	0.287%
14	8.119	1965	1984	1997	rBV4	252139	643584	3.96%	0.603%
15	8.193	1997	2007	2018	rVV	199638	468217	2.88%	0.438%
16	8.264	2018	2029	2050	rVB2	301599	722439	4.44%	0.676%
17	8.550	2101	2118	2137	rBV	359353	770556	4.74%	0.721%
18	9.045	2246	2272	2286	rBV	1206008	2923316	17.98%	2.737%
19	9.235	2311	2331	2344	rBV	168237	328427	2.02%	0.307%
20	9.331	2344	2361	2374	rVB3	70849	170082	1.05%	0.159%
21	9.476	2394	2406	2422	rVB4	90715	189699	1.17%	0.178%
22	9.836	2497	2518	2540	rBV4	122032	427383	2.63%	0.400%
23	10.058	2572	2587	2615	rBV2	860592	1888678	11.61%	1.768%
24	10.225	2630	2639	2660	rVB6	165718	461930	2.84%	0.432%
25	10.402	2681	2694	2709	rVB2	269317	523141	3.22%	0.490%
26	10.499	2709	2724	2736	rBV3	153826	311568	1.92%	0.292%
27	10.923	2849	2856	2864	rVB	212142	325022	2.00%	0.304%
28	10.974	2864	2872	2883	rVB	206836	355970	2.19%	0.333%
29	11.180	2917	2936	2953	rVB7	64338	188213	1.16%	0.176%
30	11.380	2985	2998	3014	rVV	552774	979947	6.03%	0.917%
31	11.482	3014	3030	3048	rVV	5490367	9425909	57.97%	8.824%
32	11.589	3048	3063	3097	rVB	822204	1938006	11.92%	1.814%
33	11.920	3144	3166	3182	rBV5	123953	397262	2.44%	0.372%
34	12.222	3249	3260	3273	rVB	1121376	1804772	11.10%	1.690%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120420\
 Data File : VN064928.D
 Acq On : 4 Dec 2020 18:54
 Operator : JC/MD
 Sample : L4954-11
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SS013-13-6712-120120

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
 Title : SW846 8260

35	12.373	3296	3307	3320	rBV	467007	793347	4.88%	0.743%
36	12.563	3351	3366	3378	rVB	1234694	2038972	12.54%	1.909%
37	12.627	3378	3386	3393	rBV	145401	236959	1.46%	0.222%
38	12.708	3401	3411	3435	rVB	688100	1200986	7.39%	1.124%
39	12.865	3445	3460	3473	rBV	3015631	4948802	30.43%	4.633%
40	12.933	3473	3481	3490	rVV7	93151	224697	1.38%	0.210%
41	13.013	3493	3506	3533	rVV	9771215	16260883	100.00%	15.223%
42	13.142	3534	3546	3555	rVV3	197476	404336	2.49%	0.379%
43	13.203	3557	3565	3574	rVV3	113775	227532	1.40%	0.213%
44	13.261	3574	3583	3591	rVV	256779	419298	2.58%	0.393%
45	13.347	3591	3610	3623	rVV	5147816	9251293	56.89%	8.661%
46	13.515	3642	3662	3671	rBV	2514264	4825672	29.68%	4.518%
47	13.560	3672	3676	3693	rVB4	402582	787407	4.84%	0.737%
48	13.646	3693	3703	3712	rBV	228669	367138	2.26%	0.344%
49	13.711	3712	3723	3733	rBV	584413	918861	5.65%	0.860%
50	13.775	3733	3743	3747	rVV	631903	965865	5.94%	0.904%
51	13.804	3748	3752	3761	rVV	687805	958464	5.89%	0.897%
52	13.862	3761	3770	3779	rVV	888896	1314358	8.08%	1.230%
53	13.920	3779	3788	3794	rVV	253421	406804	2.50%	0.381%
54	13.968	3794	3803	3813	rVB2	923270	1538047	9.46%	1.440%
55	14.100	3834	3844	3854	rBV2	504661	798686	4.91%	0.748%
56	14.183	3854	3870	3875	rVV	552133	933610	5.74%	0.874%
57	14.222	3875	3882	3890	rVV	884547	1345038	8.27%	1.259%
58	14.267	3890	3896	3903	rVB2	131568	171600	1.06%	0.161%
59	14.399	3925	3937	3944	rBV5	98717	195282	1.20%	0.183%
60	14.447	3944	3952	3961	rVV2	436432	718530	4.42%	0.673%
61	14.495	3962	3967	3975	rVV2	158591	224345	1.38%	0.210%
62	14.556	3975	3986	4001	rVV4	1660497	3453679	21.24%	3.233%
63	14.711	4024	4034	4045	rBV	811580	1278712	7.86%	1.197%
64	14.823	4060	4069	4075	rBV4	198593	356171	2.19%	0.333%
65	14.926	4092	4101	4112	rVB3	237151	499998	3.07%	0.468%
66	15.100	4135	4155	4167	rBV	2519504	4503039	27.69%	4.216%
67	15.209	4181	4189	4200	rBV3	90463	231130	1.42%	0.216%
68	15.579	4298	4304	4320	rVB	165950	299312	1.84%	0.280%
69	15.875	4382	4396	4411	rBV2	164455	350805	2.16%	0.328%
70	16.119	4460	4472	4497	rVB	574007	1212498	7.46%	1.135%
71	16.309	4516	4531	4546	rBV	416877	913789	5.62%	0.855%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120420\
Data File : VN064928.D
Acq On : 4 Dec 2020 18:54
Operator : JC/MD
Sample : L4954-11
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SS013-13-6712-120120

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Title : SW846 8260


Sum of corrected areas: 106818886

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN120420\
Data File : VN064928.D
Acq On : 4 Dec 2020 18:54
Operator : JC/MD
Sample : L4954-11
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SS013-13-6712-120120

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

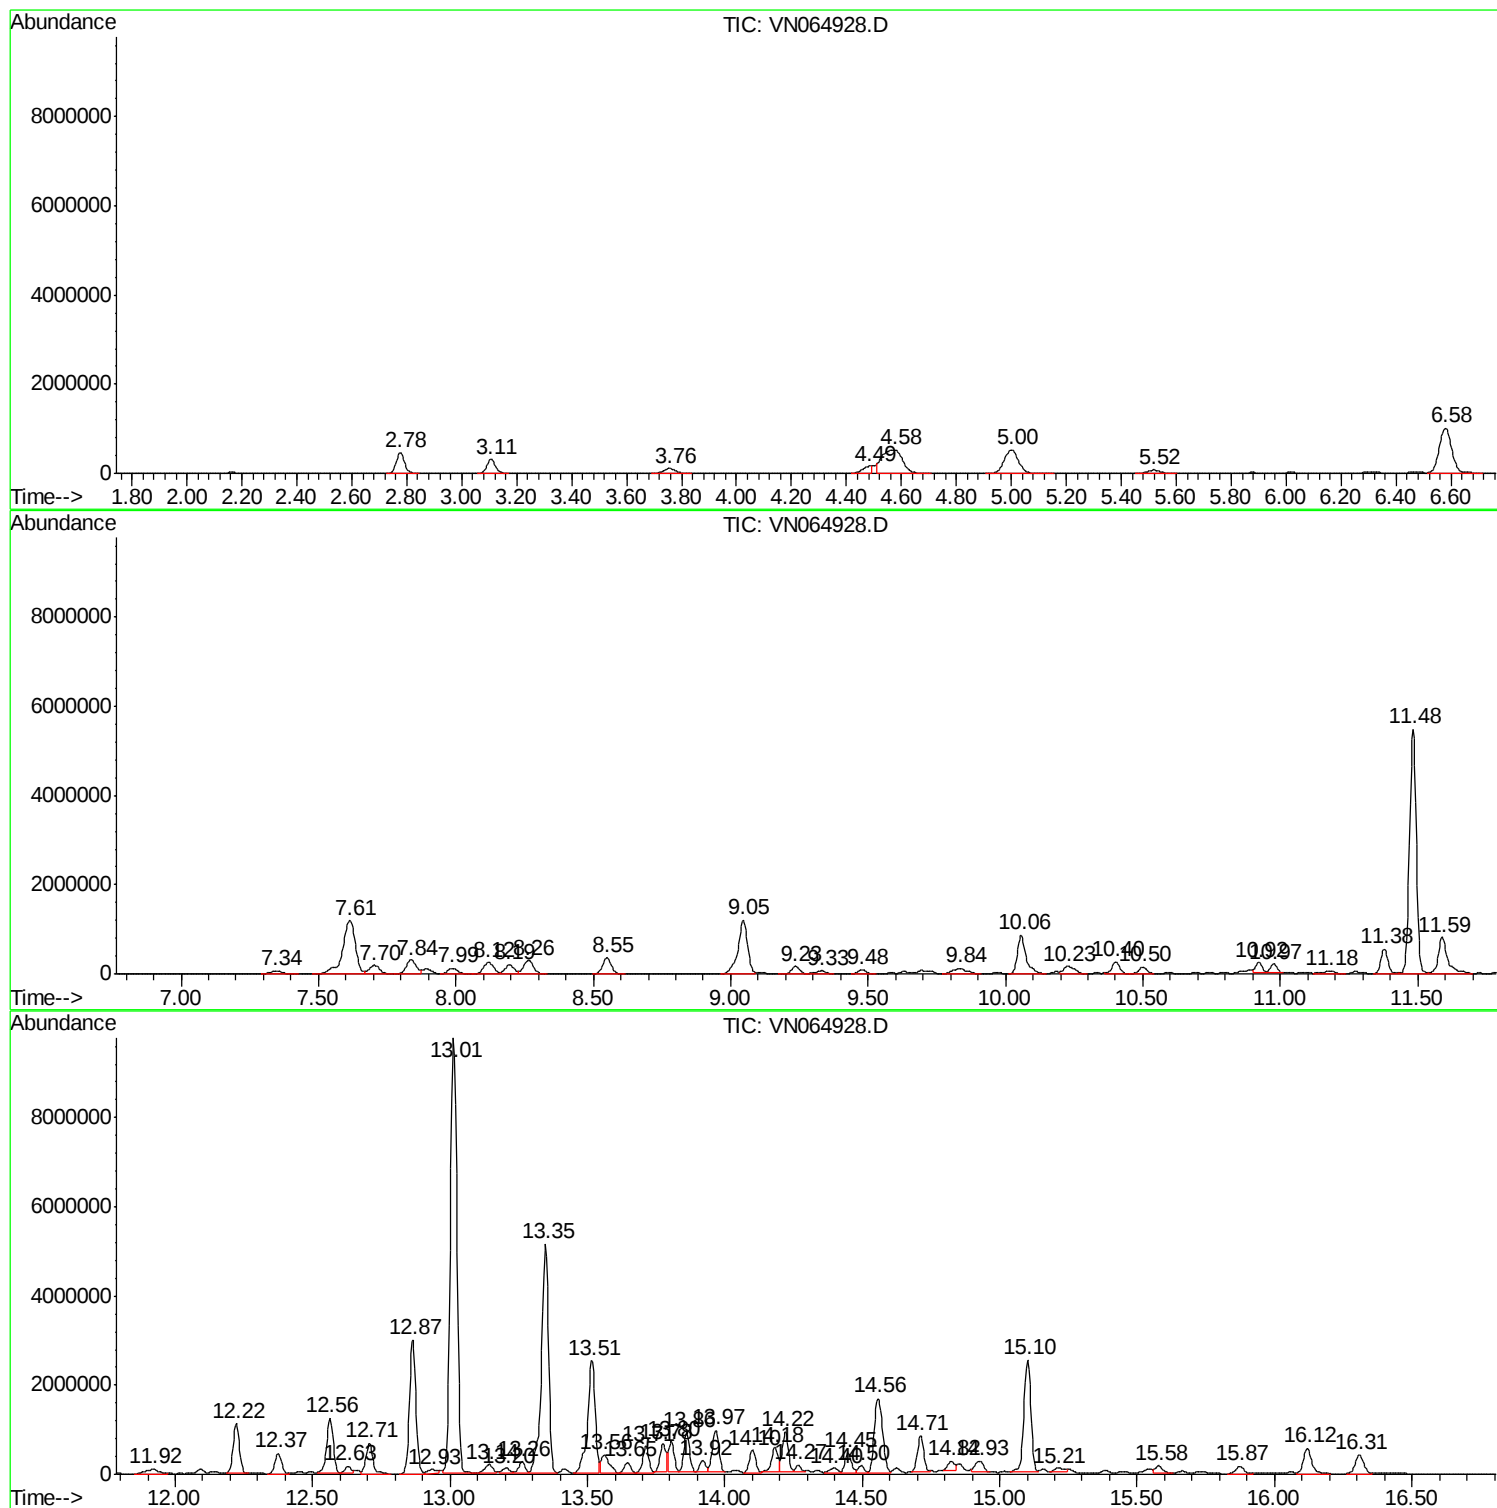

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN120420\
Data File : VN064928.D
Acq On : 4 Dec 2020 18:54
Operator : JC/MD
Sample : L4954-11
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SS013-13-6712-120120

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN120420\
Data File : VN064928.D
Acq On : 4 Dec 2020 18:54
Operator : JC/MD
Sample : L4954-11
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SS013-13-6712-120120

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc