


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120421\
Data File : VN069757.D
Acq On : 4 Dec 2021 10:22
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Title : SW846 8260
Last Update : Fri Dec 03 08:46:47 2021

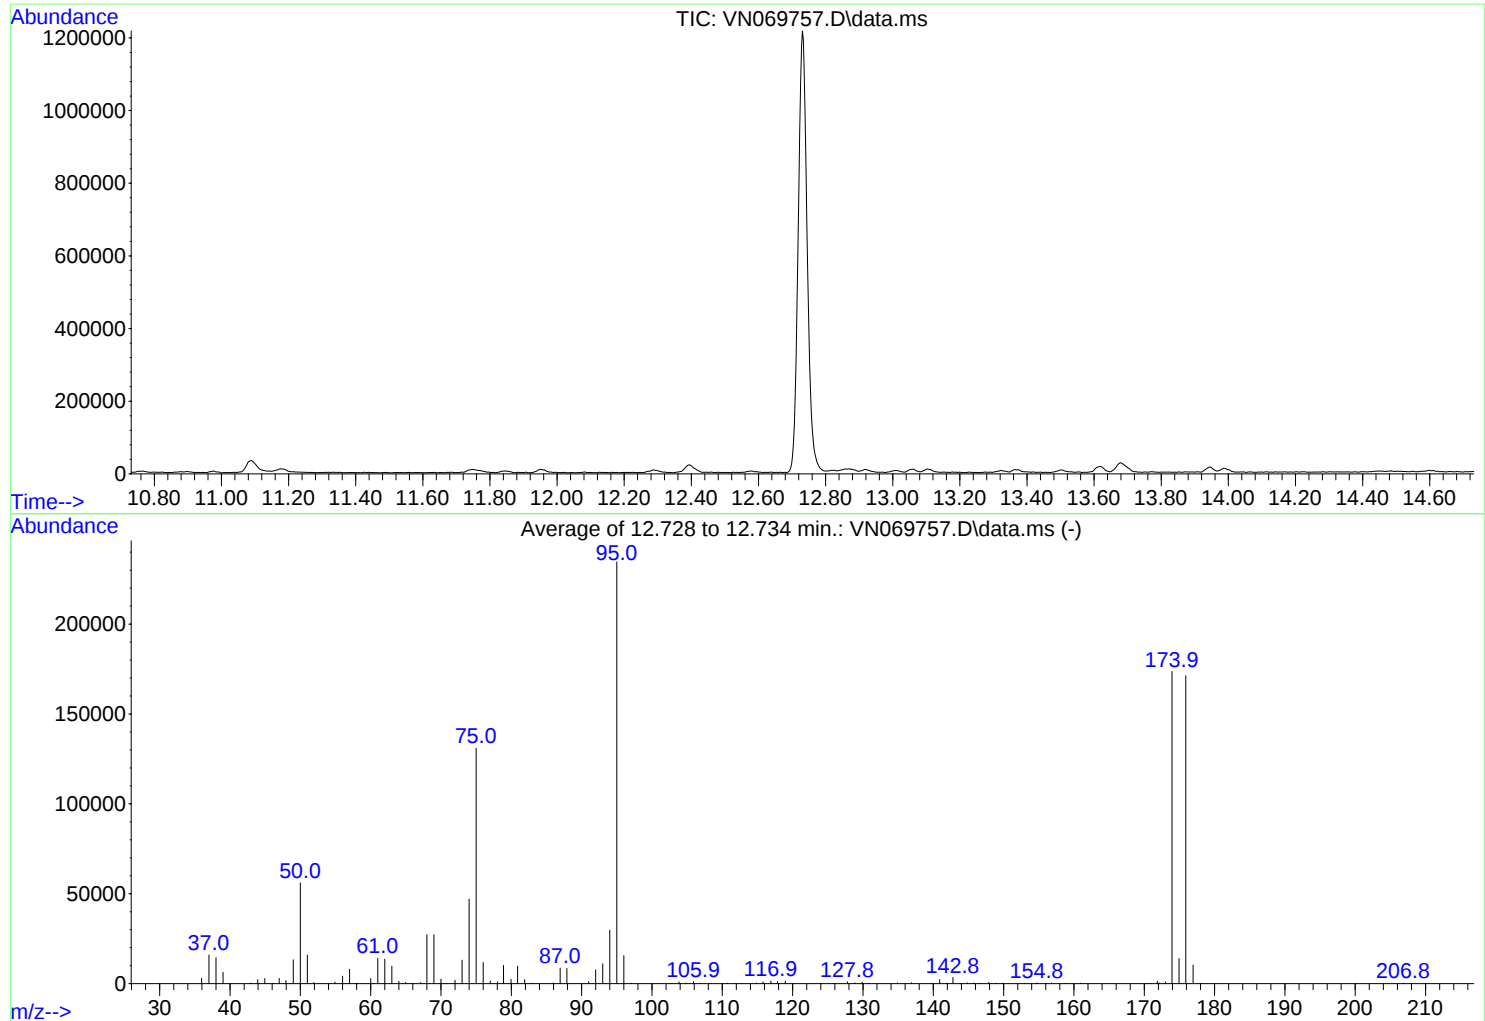

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	56045	PASS
75	95	30	60	55.8	130907	PASS
95	95	100	100	100.0	234624	PASS
96	95	5	9	6.7	15607	PASS
173	174	0.00	2	0.5	940	PASS
174	95	50	100	74.0	173675	PASS
175	174	5	9	8.1	14000	PASS
176	174	95	101	98.6	171328	PASS
177	176	5	9	6.0	10296	PASS