
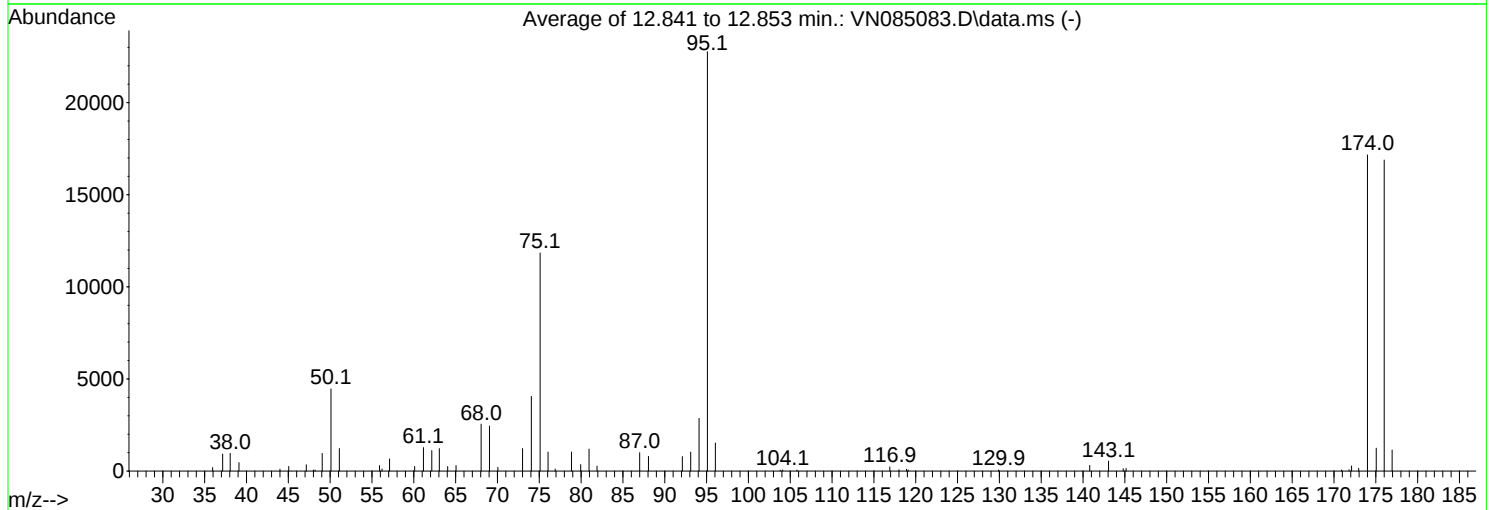


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120424\
Data File : VN085083.D
Acq On : 04 Dec 2024 09:00
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

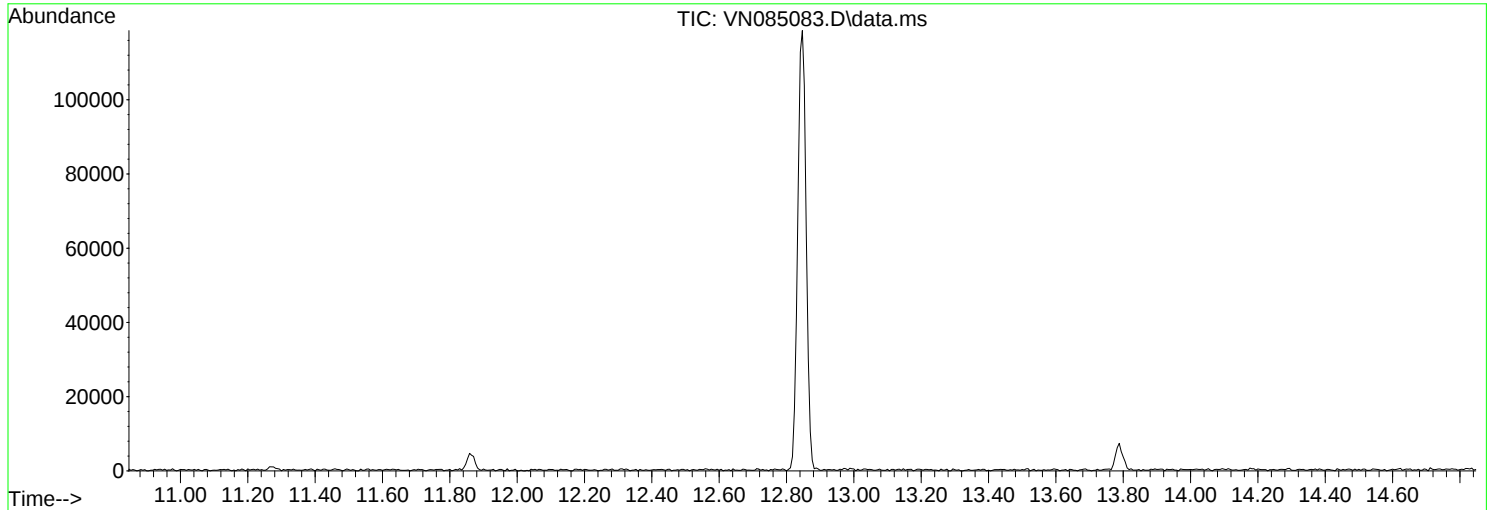

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	4460	PASS
75	95	30	60	52.0	11839	PASS
95	95	100	100	100.0	22763	PASS
96	95	5	9	6.7	1525	PASS
173	174	0.00	2	0.9	152	PASS
174	95	50	100	75.4	17162	PASS
175	174	5	9	7.2	1243	PASS
176	174	95	101	98.4	16884	PASS
177	176	5	9	6.8	1145	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	190	51.10	1225	69.05	2446	87.00	997
37.15	925	55.90	299	70.05	201	88.05	798
38.05	969	56.20	115	73.00	1222	92.10	788
39.10	460	57.10	659	74.05	4051	93.10	1035
44.00	104	60.10	255	75.10	11839	94.10	2860
45.05	253	61.15	1277	76.05	1031	95.10	22763
47.15	344	62.15	1113	76.90	118	96.05	1525
48.00	57	63.05	1219	78.85	1035	103.80	53
48.20	57	64.05	247	79.95	353	104.10	62
49.05	958	65.05	303	80.95	1197	105.80	60
50.10	4460	68.05	2552	81.90	274	116.90	231

Average of 12.841 to 12.853 min.: VN085083.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.00	72	172.95	152				
118.90	101	174.00	17162				
119.10	63	175.05	1243				
129.90	63	176.00	16884				
140.80	309	176.95	1145				
143.05	543						
144.80	134						
145.15	149						
170.90	58						
171.80	75						
172.10	276						

Instrument :

MSVOA_N

ClientSampleId :

BFB