

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120425\
 Data File : VN088455.D
 Acq On : 04 Dec 2025 18:31
 Operator : JC\MD
 Sample : Q3757-09 100X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 OW-05B-72-120325

Quant Time: Dec 05 00:19:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 25 01:34:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	191523	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	444923	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.841	117	435700	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	202473	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	203059	56.282	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	112.560%
35) Dibromofluoromethane	8.147	113	142965	46.368	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.740%
50) Toluene-d8	10.541	98	508334	44.310	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	88.620%
62) 4-Bromofluorobenzene	12.829	95	193168	49.073	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	98.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120425\
Data File : VN088455.D
Acq On : 04 Dec 2025 18:31
Operator : JC\MD
Sample : Q3757-09 100X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
OW-05B-72-120325

Quant Time: Dec 05 00:19:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 25 01:34:52 2025
Response via : Initial Calibration




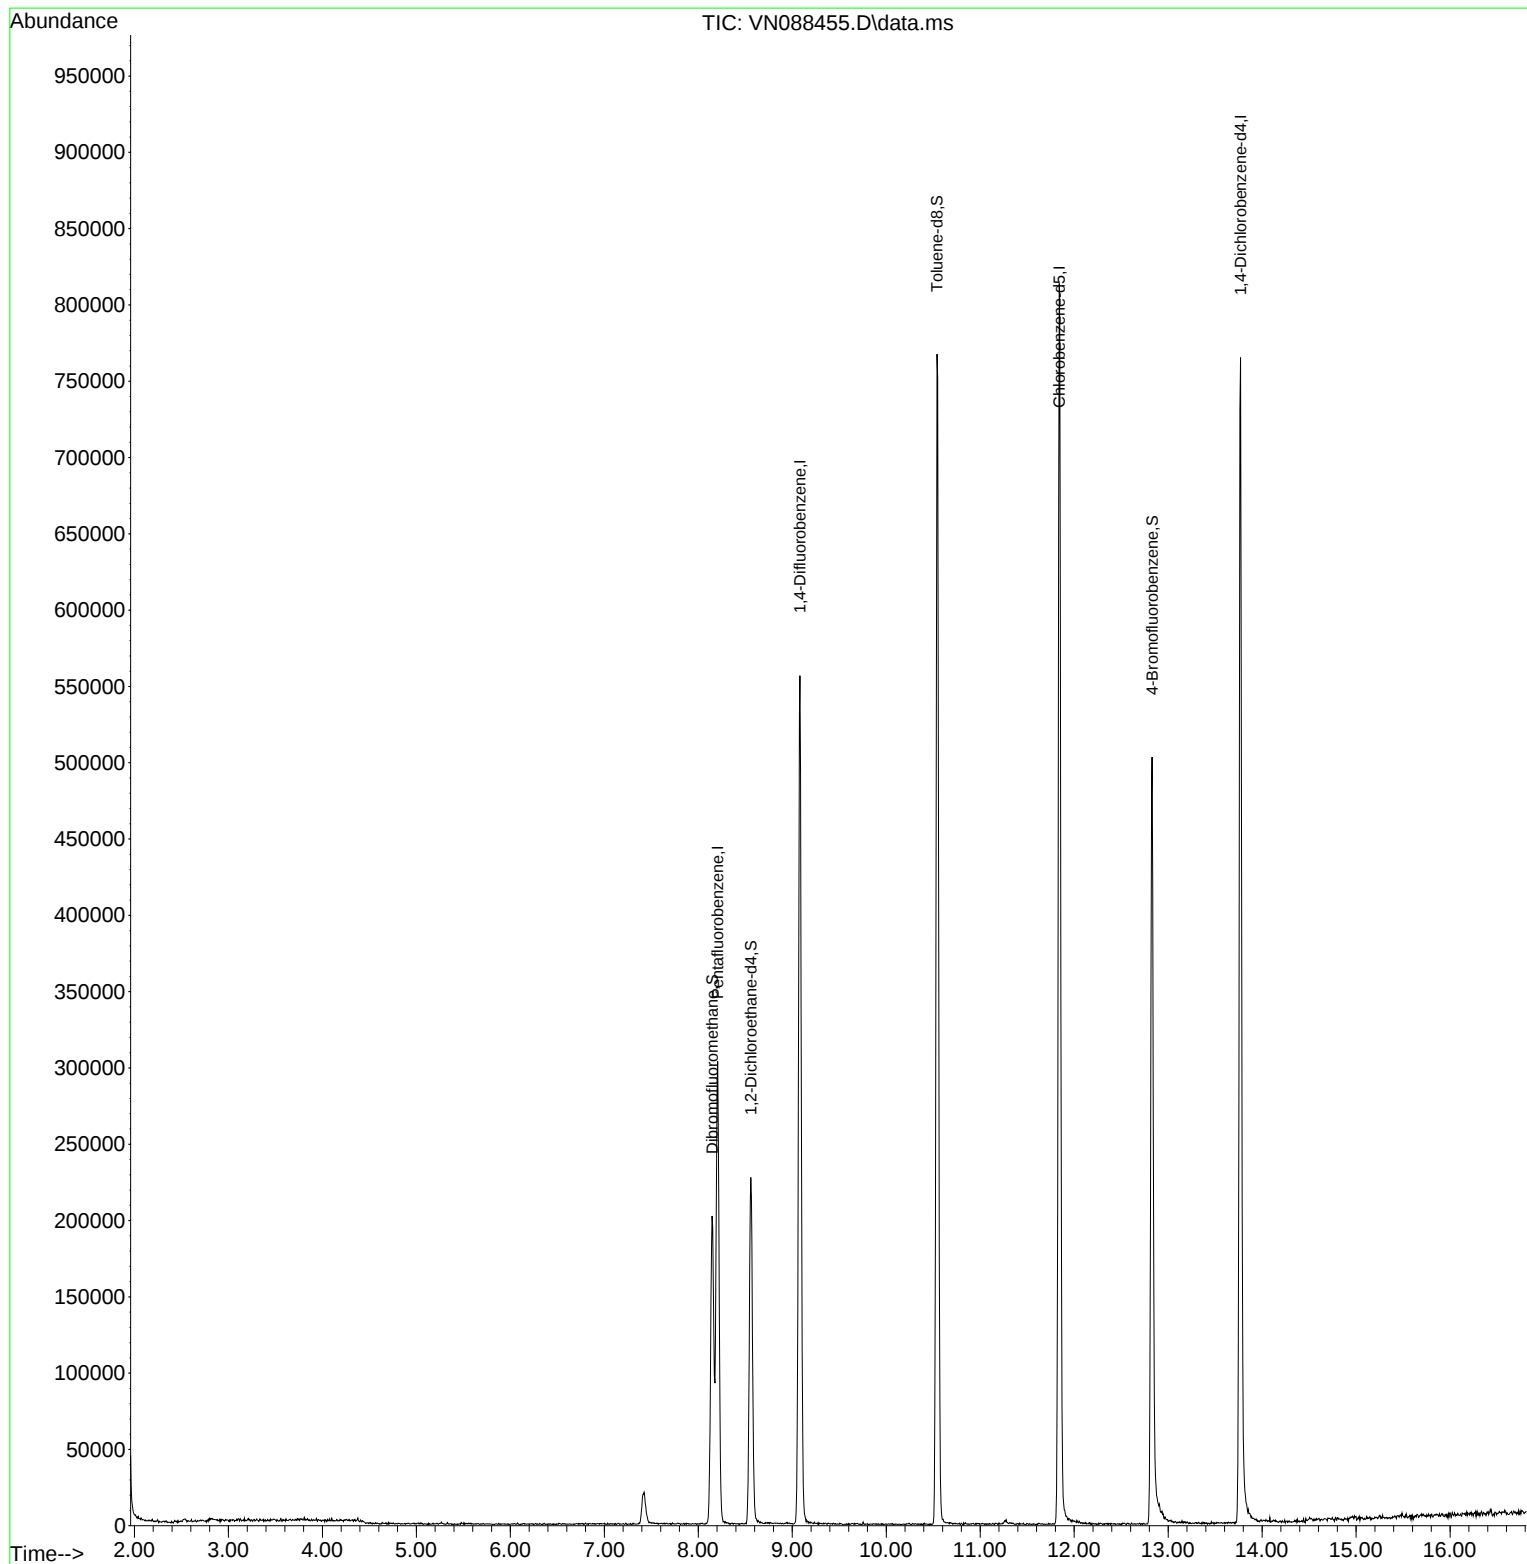


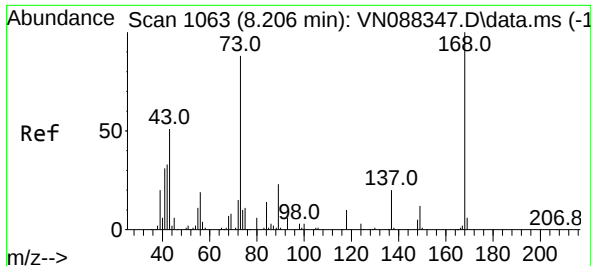

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1063
Delta R.T. 0.000 min
Lab File: VN088455.D
Acq: 04 Dec 2025 18:31




Instrument :
MSVOA_N
ClientSampleId :
OW-05B-72-120325


Tgt Ion:168 Resp: 191523
Ion Ratio Lower Upper
168 100
99 72.9 57.1 85.7

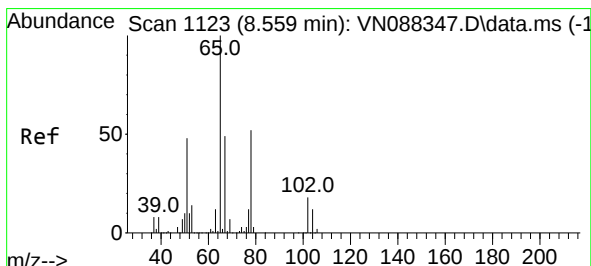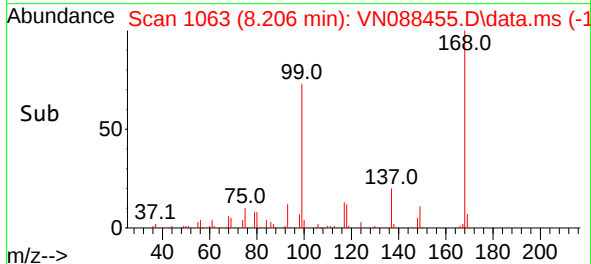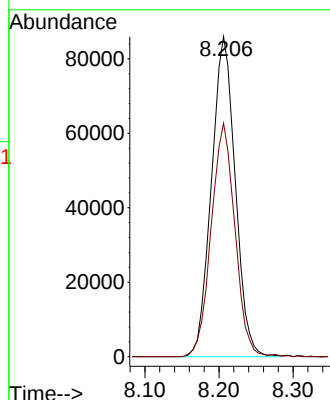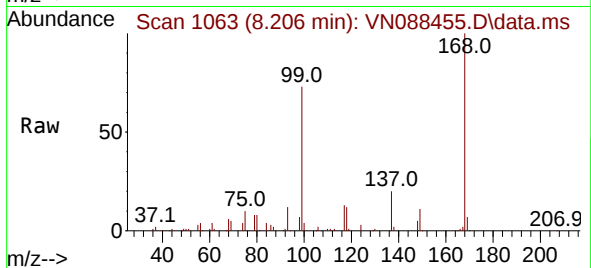

#33
1,2-Dichloroethane-d4
Concen: 56.282 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. 0.000 min
Lab File: VN088455.D
Acq: 04 Dec 2025 18:31

Tgt Ion: 65 Resp: 203059
Ion Ratio Lower Upper
65 100
67 49.2 0.0 100.8

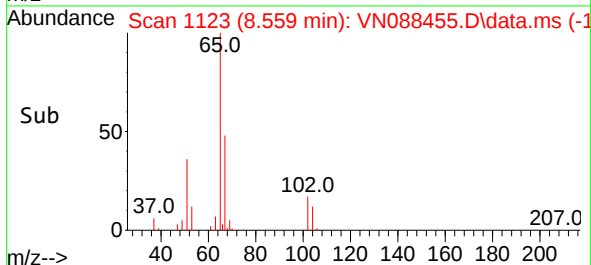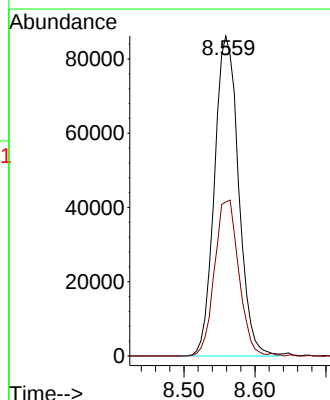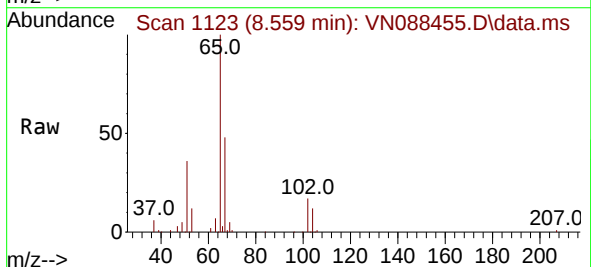

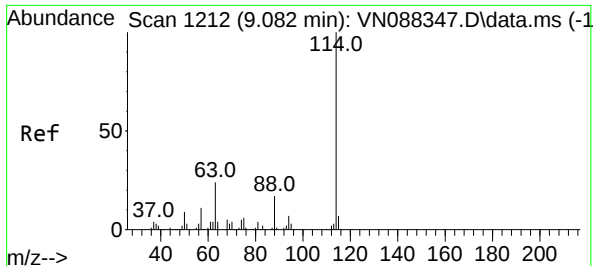

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.082 min Scan# 11

Delta R.T. 0.000 min

Lab File: VN088455.D

Acq: 04 Dec 2025 18:31

Instrument :

MSVOA_N

ClientSampleId :

OW-05B-72-120325





Tgt Ion:114 Resp: 444923

Ion Ratio Lower Upper

114 100

63 25.0 0.0 49.0

88 17.2 0.0 34.0

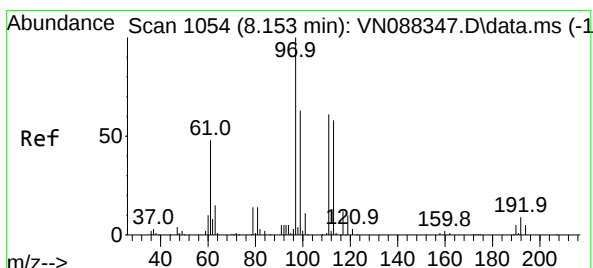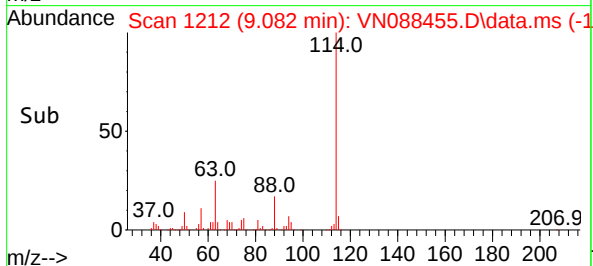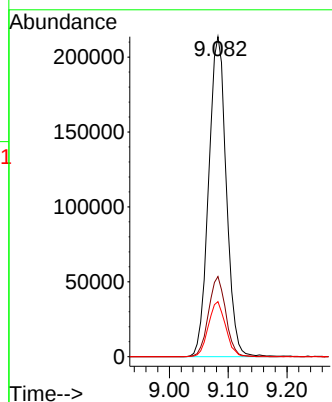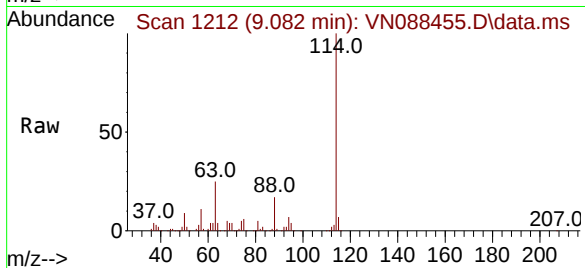

#35

Dibromofluoromethane

Concen: 46.368 ug/l

RT: 8.147 min Scan# 1053

Delta R.T. -0.006 min

Lab File: VN088455.D

Acq: 04 Dec 2025 18:31




Tgt Ion:113 Resp: 142965


Ion Ratio Lower Upper

113 100

111 105.5 82.5 123.7

192 16.1 12.8 19.2


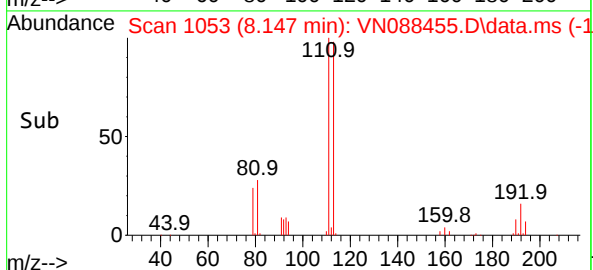
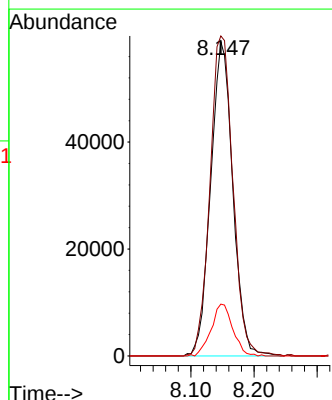
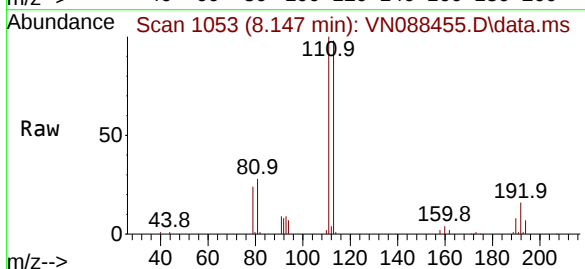


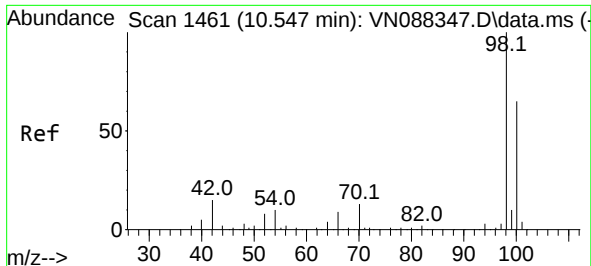

#50
Toluene-d8
Concen: 44.310 ug/l
RT: 10.541 min Scan# 1460
Delta R.T. -0.006 min
Lab File: VN088455.D
Acq: 04 Dec 2025 18:31




Instrument :
MSVOA_N
ClientSampleId :
OW-05B-72-120325


Tgt Ion: 98 Resp: 508334
Ion Ratio Lower Upper
98 100
100 63.9 52.2 78.2

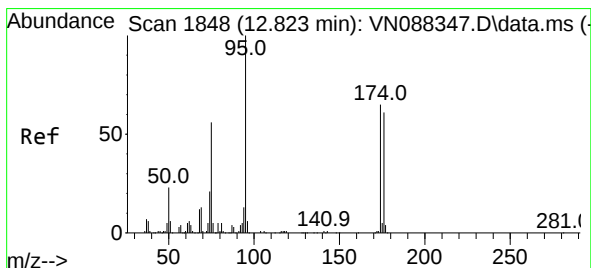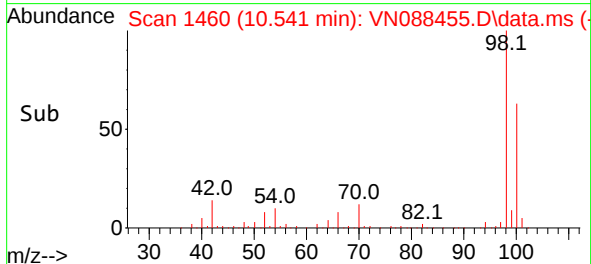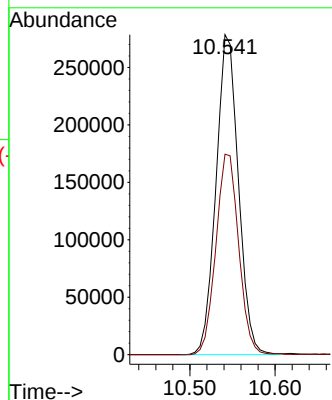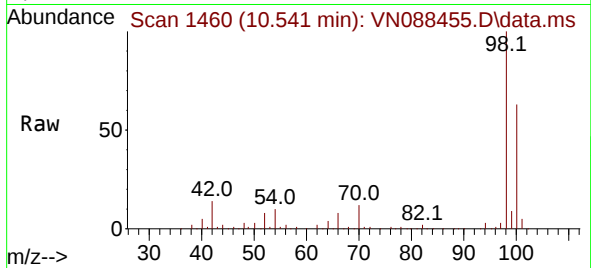

#62
4-Bromofluorobenzene
Concen: 49.073 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN088455.D
Acq: 04 Dec 2025 18:31

Tgt Ion: 95 Resp: 193168
Ion Ratio Lower Upper
95 100
174 66.3 0.0 139.0
176 64.8 0.0 132.4


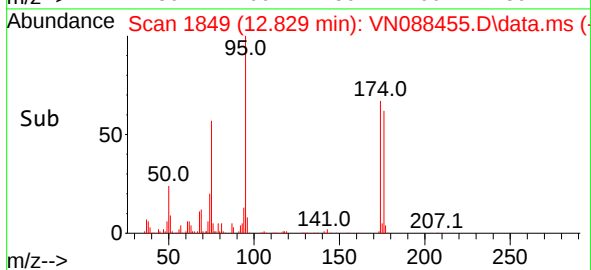
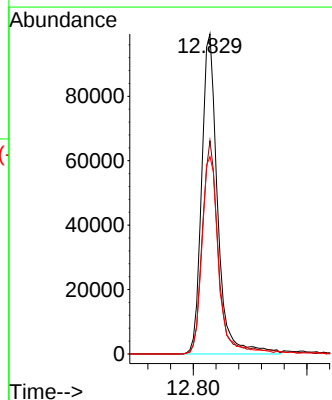
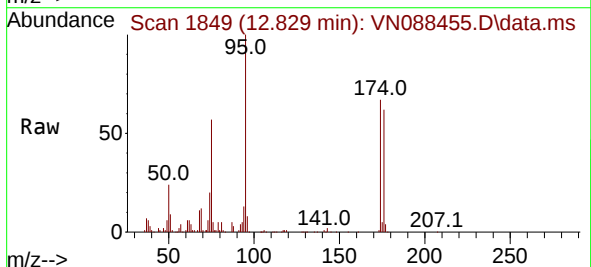


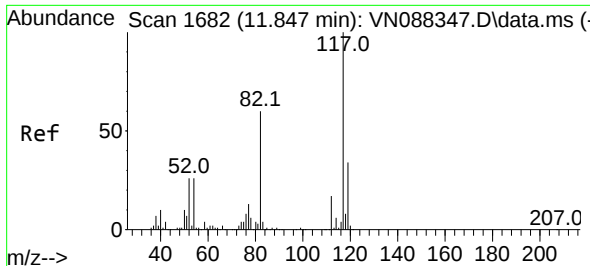

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.841 min Scan# 1170
Delta R.T. -0.006 min
Lab File: VN088455.D
Acq: 04 Dec 2025 18:31

Instrument :
MSVOA_N
ClientSampleId :
OW-05B-72-120325

Tgt Ion:117 Resp: 435700
Ion Ratio Lower Upper
117 100
82 60.6 47.8 71.8
119 30.6 26.9 40.3

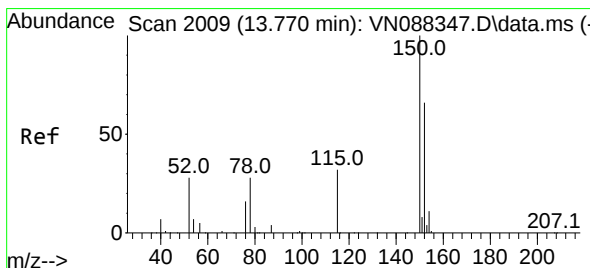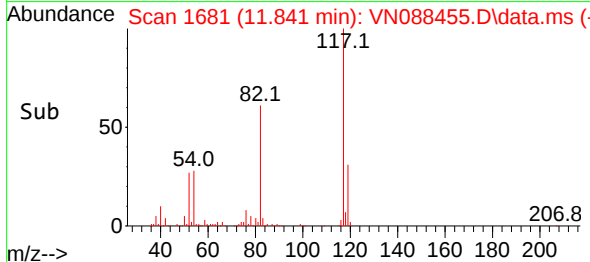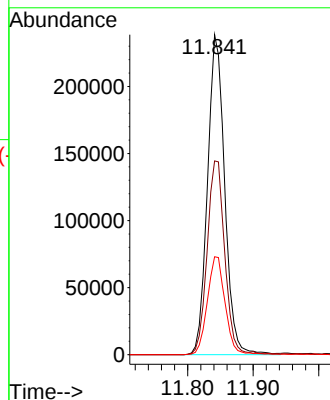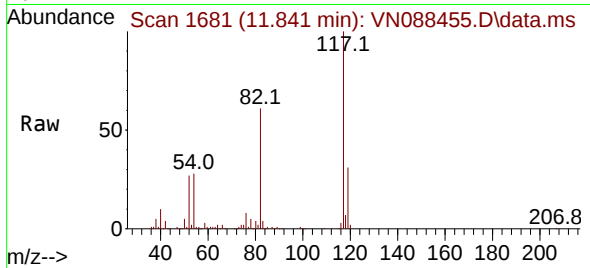

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.000 min
Lab File: VN088455.D
Acq: 04 Dec 2025 18:31

Tgt Ion:152 Resp: 202473
Ion Ratio Lower Upper
152 100
115 66.7 33.0 98.9
150 160.0 0.0 349.0

