

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120518\
 Data File : VN052674.D
 Acq On : 5 Dec 2018 14:13
 Operator : MD\SY
 Sample : PB115330ZHE#05
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 11 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 PB115330ZHE#05

Quant Time: Dec 06 05:01:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 03 03:24:02 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1226886	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1913076	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1712939	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	647809	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	655051	49.04	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.08%	
35) Dibromofluoromethane	7.59	113	586683	49.74	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.48%	
50) Toluene-d8	10.09	98	2344981	51.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.16%	
62) 4-Bromofluorobenzene	12.40	95	750635	48.66	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.32%	
Target Compounds						
16) Acetone	3.82	43	16114	4.573	ug/l	97
20) Methylene Chloride	4.55	84	85993	6.237	ug/l	97
43) Isopropyl Acetate	8.17	43	61164	3.278	ug/l #	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN120518\
Data File : VN052674.D
Acq On : 5 Dec 2018 14:13
Operator : MD\SY
Sample : PB115330ZHE#05
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 11 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
PB115330ZHE#05

Quant Time: Dec 06 05:01:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 03 03:24:02 2018
Response via : Initial Calibration

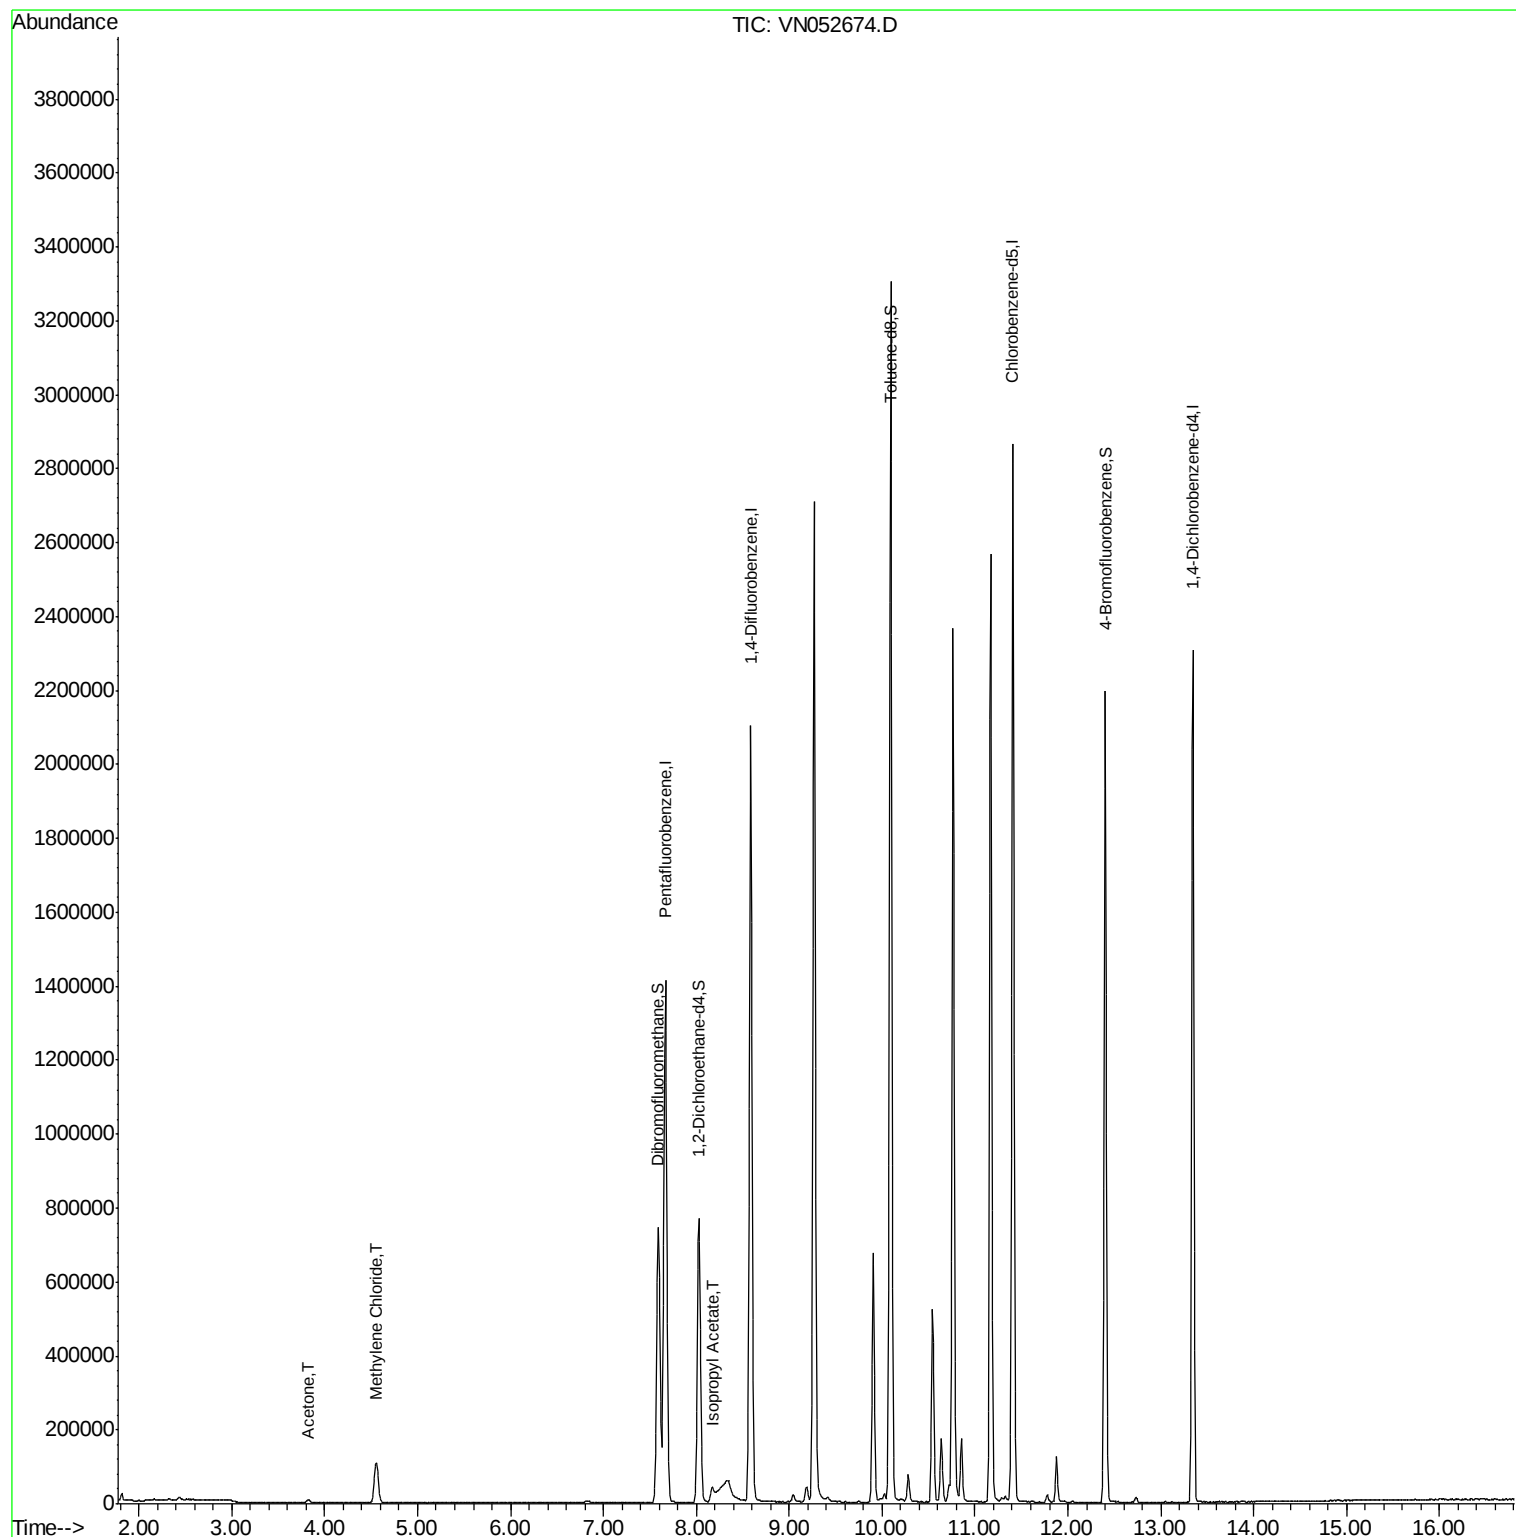

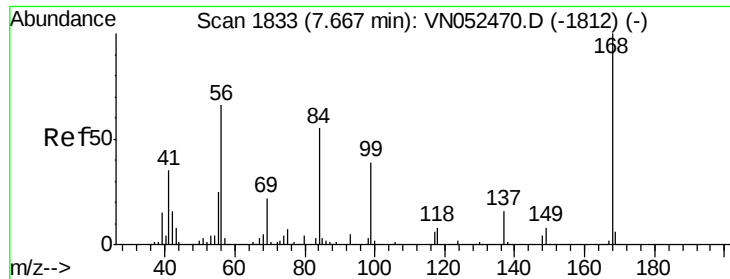

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN052674.D

Acq: 5 Dec 2018 14:13

Instrument :

MSVOA_N

ClientSampleId :


PB115330ZHE#05

Tot Ion:168 Resp: 1226886

Ion Ratio Lower Upper

168 100

99 51.3 41.7 62.5

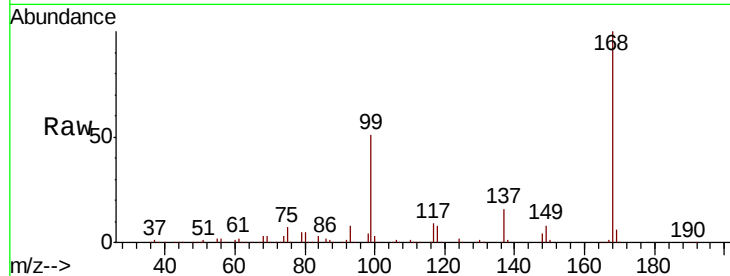

Abundance Ion 167.90 (167.60 to 168.60): VN052470.D (-1812) (-)

Ion 98.90 (98.60 to 99.60): VN052470.D (-1812) (-)

7.67

600000

500000

400000



300000

200000

100000

0

Time-->

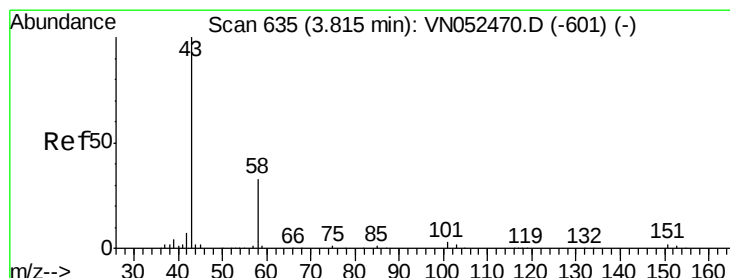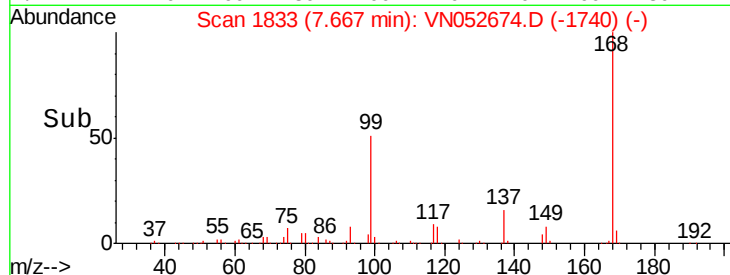

#16

Acetone

Concen: 4.573 ug/l

RT: 3.82 min Scan# 638

Delta R.T. 0.01 min

Lab File: VN052674.D


Acq: 5 Dec 2018 14:13

Tgt Ion: 43 Resp: 16114

Ion Ratio Lower Upper

43 100

58 33.9 26.0 39.0

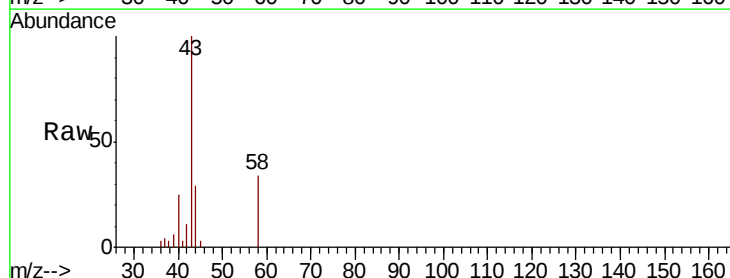

Abundance Ion 43.00 (42.70 to 43.70): VN052470.D (-601) (-)

Ion 58.00 (57.70 to 58.70): VN052470.D (-601) (-)

3.82

6000

5000

4000


3000


2000

1000

0

Time-->




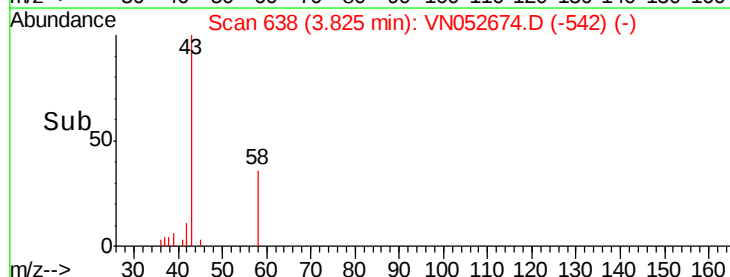


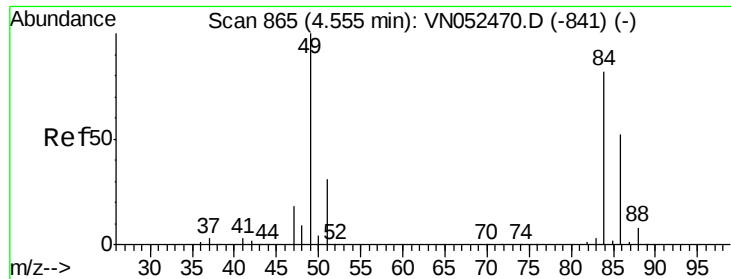

#20
Methylene Chloride
Concen: 6.237 ug/l
RT: 4.55 min Scan# 865
Delta R.T. -0.00 min
Lab File: VN052674.D
Acq: 5 Dec 2018 14:13




Instrument :
MSVOA_N
ClientSampleId :
PB115330ZHE#05


Tot Ion: 84 Resp: 85993
Ion Ratio Lower Upper
84 100
49 118.4 98.0 147.0
51 34.4 30.1 45.1
86 63.3 50.7 76.1

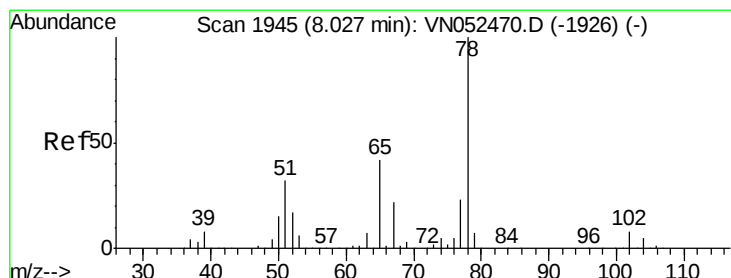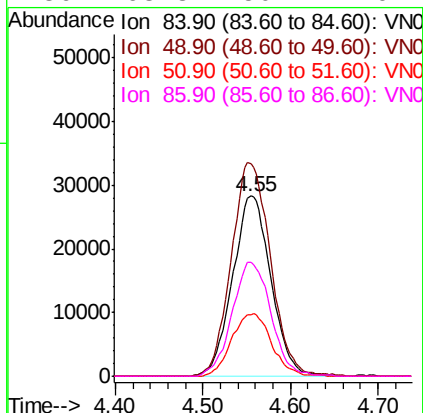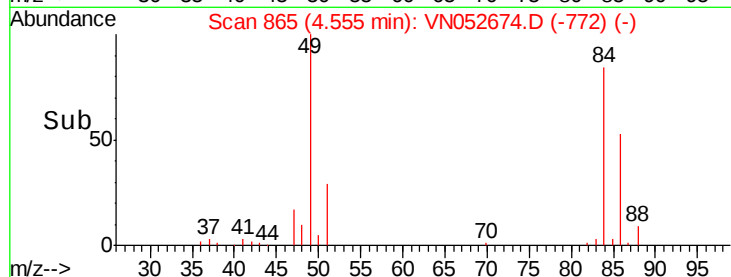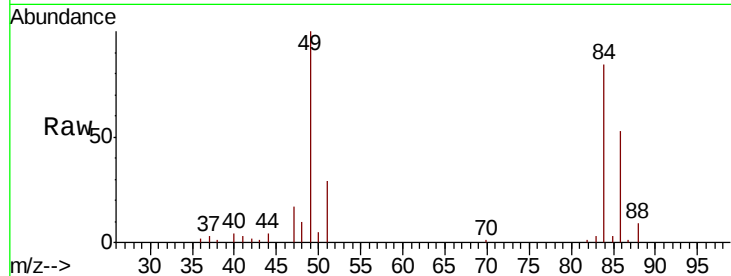

#33
1,2-Dichloroethane-d4
Concen: Below ug/l
RT: 8.03 min Scan# 1945
Delta R.T. -0.00 min
Lab File: VN052674.D
Acq: 5 Dec 2018 14:13

Tgt Ion: 65 Resp: 655051
Ion Ratio Lower Upper
65 100
67 54.8 0.0 109.8

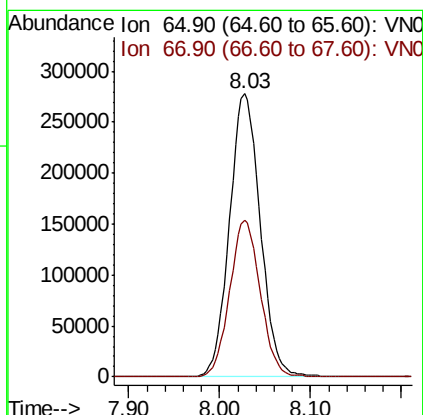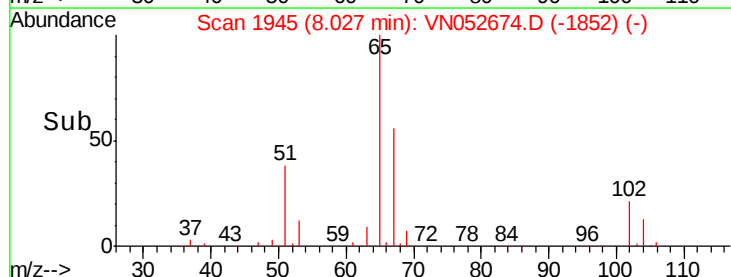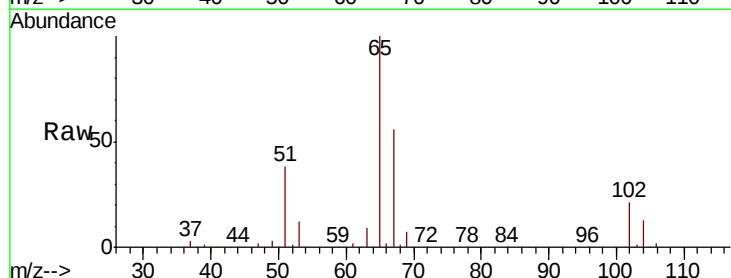

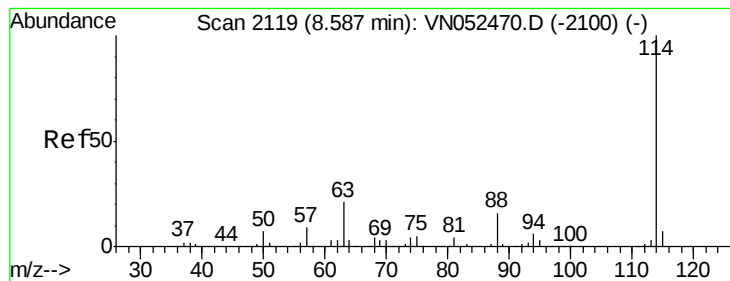

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. -0.00 min

Lab File: VN052674.D

Acq: 5 Dec 2018 14:13

Instrument :

MSVOA_N

ClientSampleId :

PB115330ZHE#05


Tot Ion:114 Resp: 1913076

Ion Ratio Lower Upper

114 100

63 20.2 0.0 41.8




88 15.6 0.0 31.6

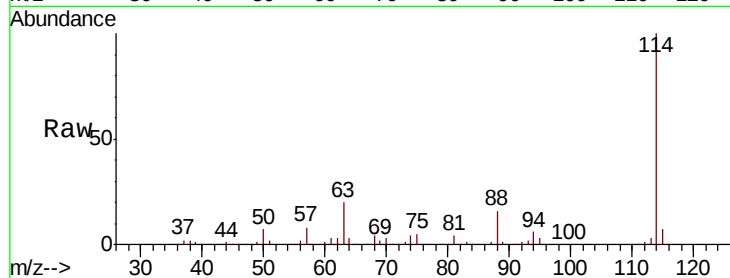

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

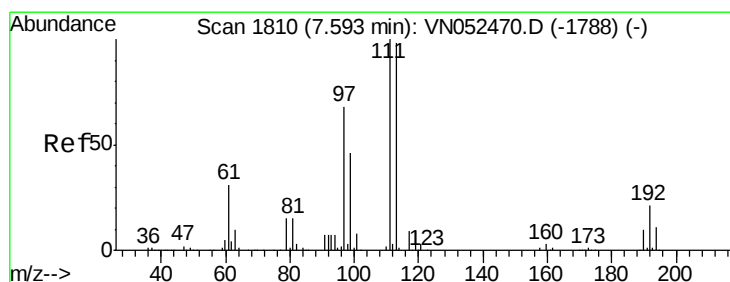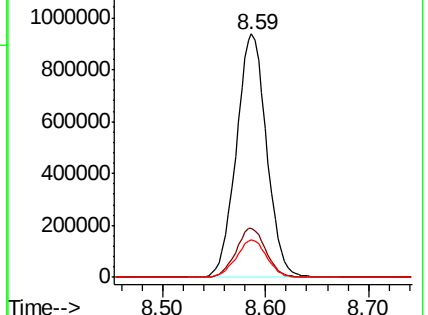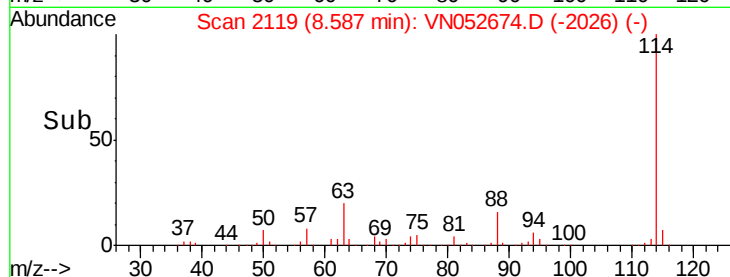

#35

Dibromofluoromethane

Concen: 50.000 ug/l

RT: 7.59 min Scan# 1809

Delta R.T. -0.00 min

Lab File: VN052674.D

Acq: 5 Dec 2018 14:13


Tgt Ion:113 Resp: 586683

Ion Ratio Lower Upper

113 100

111 103.2 82.0 123.0



192 22.0 17.0 25.6

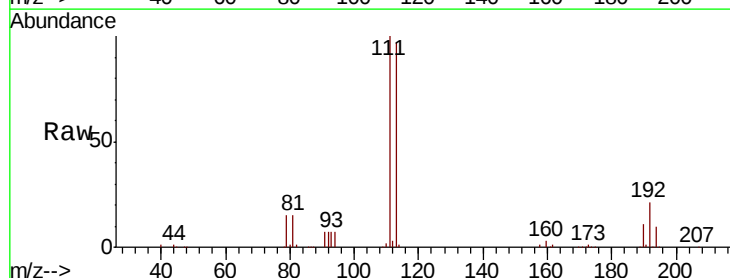


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

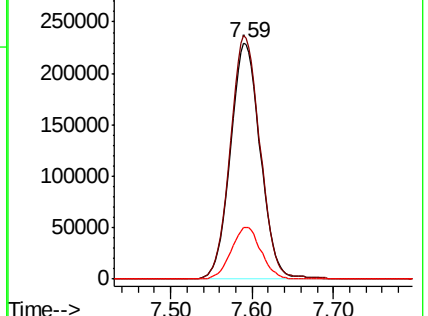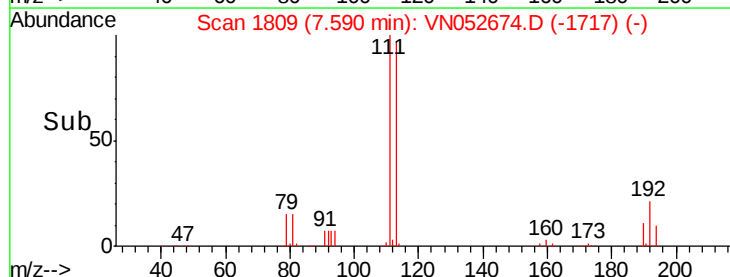

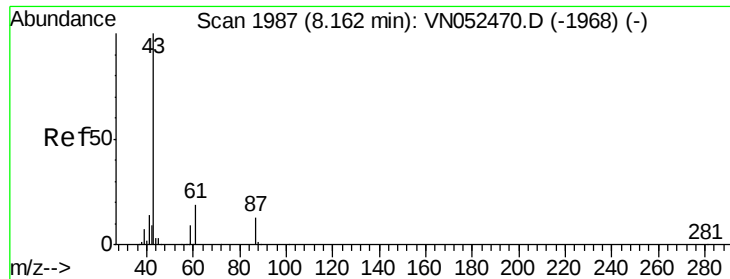

#43

Isopropyl Acetate

Concen: 3.278 ug/l

RT: 8.17 min Scan# 1988

Delta R.T. 0.00 min

Lab File: VN052674.D

Acq: 5 Dec 2018 14:13

Instrument :

MSVOA_N

ClientSampleId :

PB115330ZHE#05


Tot Ion: 43 Resp: 61164

Ion Ratio Lower Upper

43 100

61 14.2 24.1 36.1#




87 8.6 10.6 15.8#

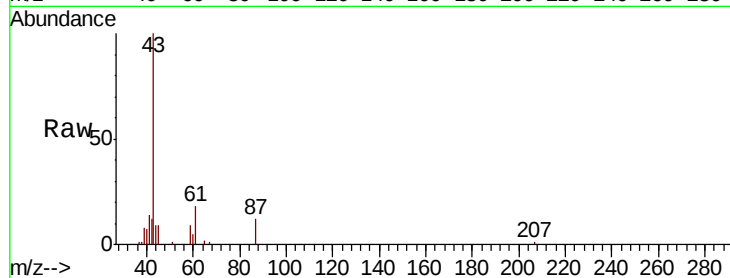

Abundance Ion 43.00 (42.70 to 43.70): VN052470.D (-1968) (-)

Ion 61.00 (60.70 to 61.70): VN052470.D (-1968) (-)

Ion 87.00 (86.70 to 87.70): VN052470.D (-1968) (-)

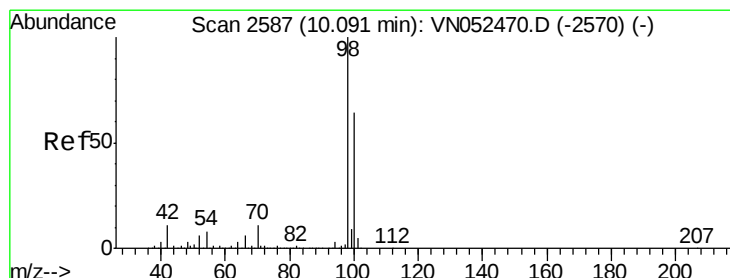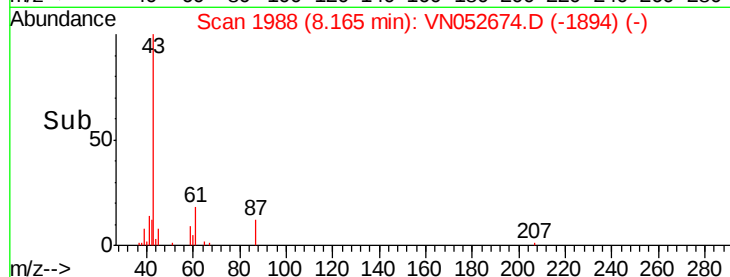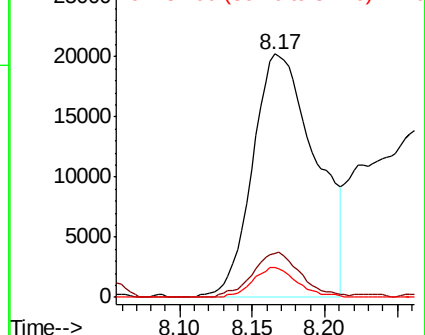

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN052674.D


Acq: 5 Dec 2018 14:13

Tgt Ion: 98 Resp: 2344981

Ion Ratio Lower Upper



98 100


100 64.0 51.3 76.9

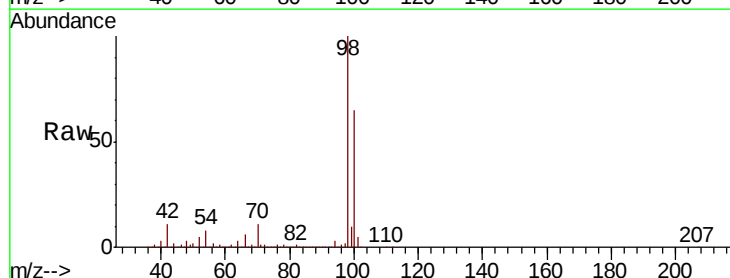

Abundance Ion 98.00 (97.70 to 98.70): VN052470.D (-2570) (-)

Ion 100.00 (99.70 to 100.70): VN052470.D (-2570) (-)

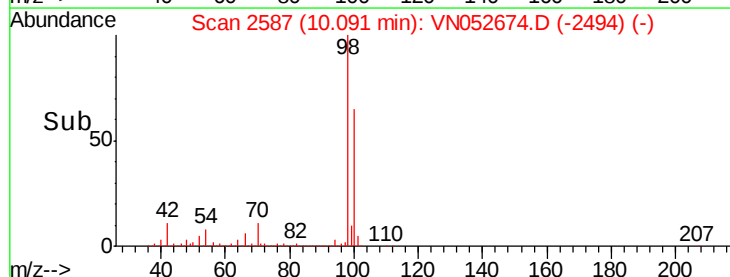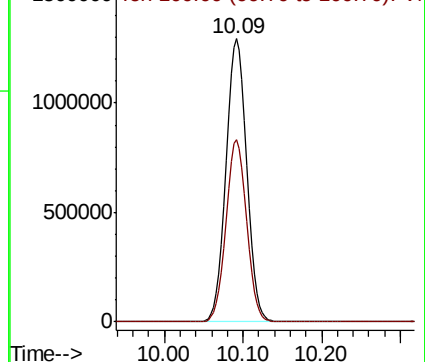

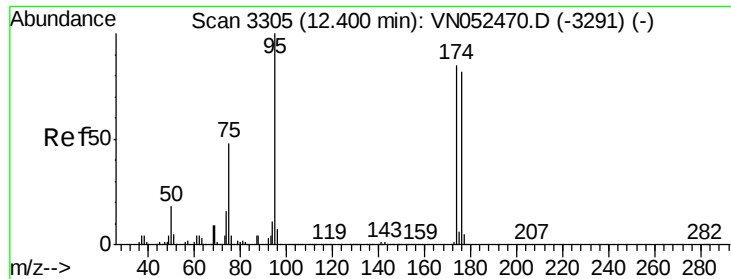

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN052674.D

Acq: 5 Dec 2018 14:13

Instrument :

MSVOA_N

ClientSampleId :

PB115330ZHE#05


Tot Ion: 95 Resp: 750635

Ion Ratio Lower Upper

95 100

174 88.0 0.0 173.0

176 85.7 0.0 166.2

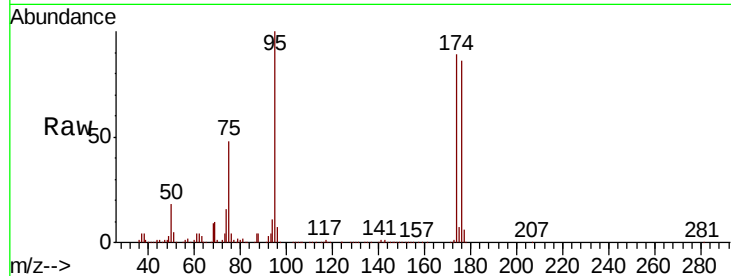



Abundance Ion 94.90 (94.60 to 95.60): VN052470.D (-3291) (-)

Ion 173.80 (173.50 to 174.50): VN052470.D (-3291) (-)

Ion 175.80 (175.50 to 176.50): VN052470.D (-3291) (-)

12.40

Time--> 12.30 12.40 12.50

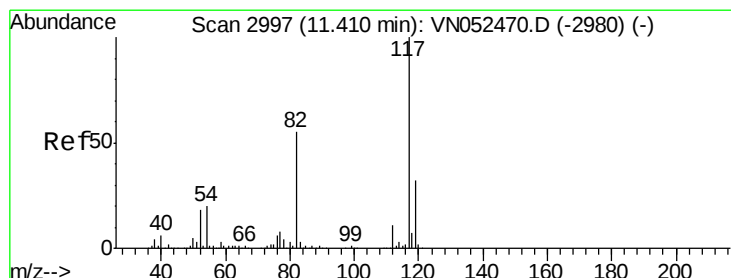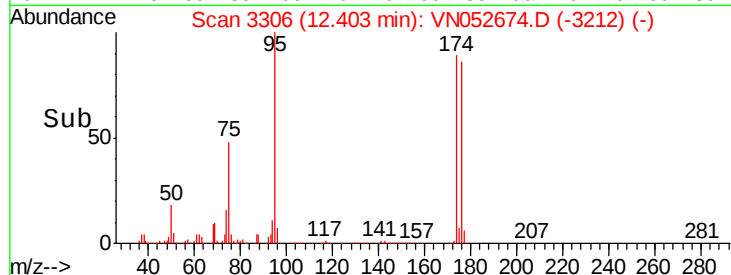

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. -0.00 min

Lab File: VN052674.D

Acq: 5 Dec 2018 14:13


Tgt Ion: 117 Resp: 1712939

Ion Ratio Lower Upper

117 100

82 54.1 43.6 65.4

119 32.5 25.4 38.2

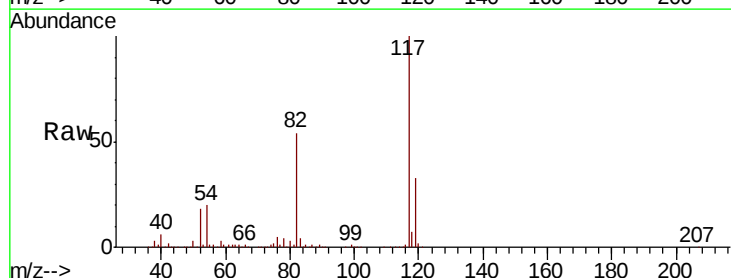


Abundance Ion 116.90 (116.60 to 117.60): VN052470.D (-2980) (-)


Ion 82.00 (81.70 to 82.70): VN052470.D (-2980) (-)

Ion 118.90 (118.60 to 119.60): VN052470.D (-2980) (-)

11.41

Time--> 11.30 11.40 11.50

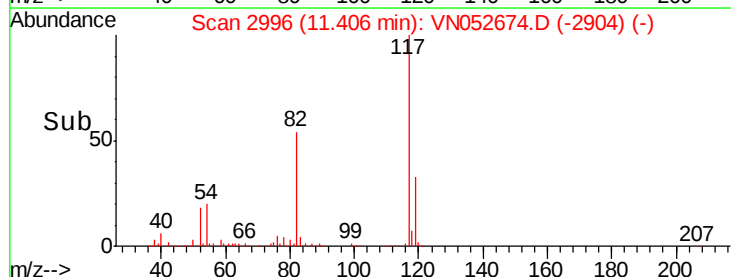

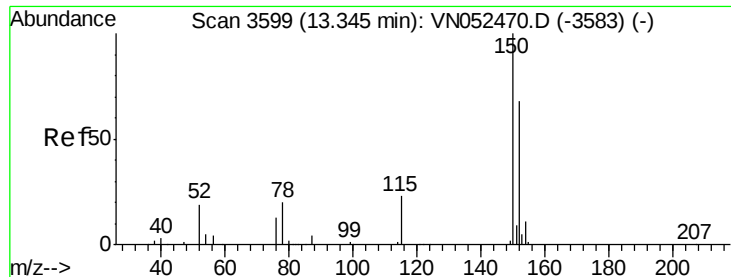

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3599

Delta R.T. -0.00 min

Lab File: VN052674.D

Acq: 5 Dec 2018 14:13

Instrument :

MSVOA_N

ClientSampleId :

PB115330ZHE#05


Tot Ion:152 Resp: 647809

Ion Ratio Lower Upper

152 100

115 56.2 28.4 85.2

150 156.5 0.0 346.0

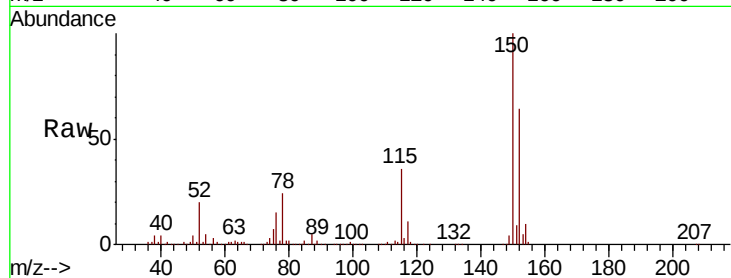

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

