


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN120518\
Data File : VN052664.D
Acq On : 5 Dec 2018 8:49
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Title : SW846 8260
Last Update : Mon Dec 03 03:24:02 2018

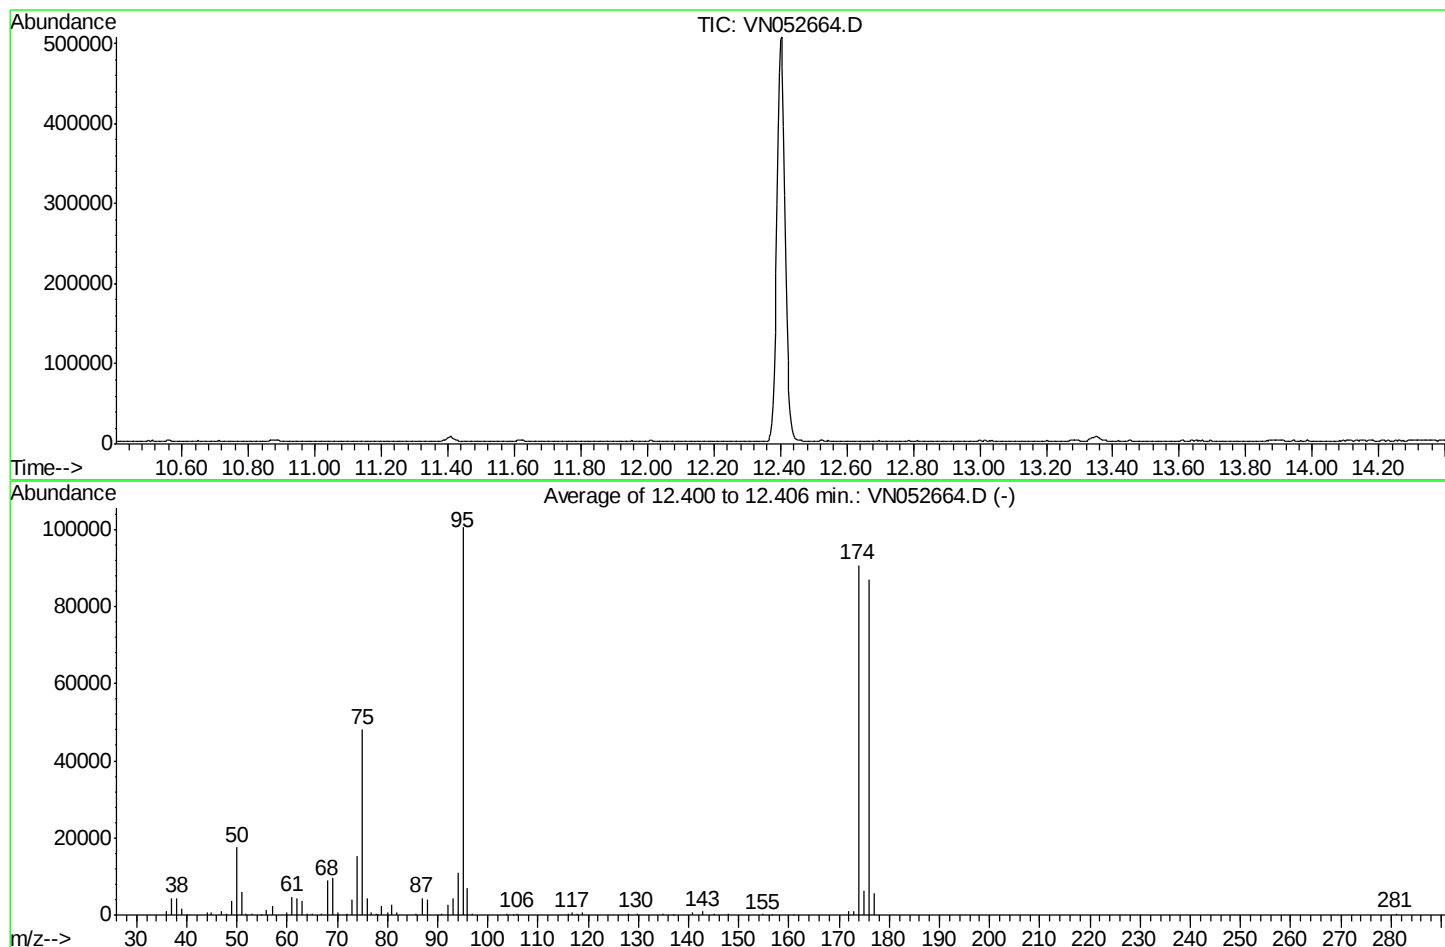

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	17448	PASS
75	95	30	60	47.7	48002	PASS
95	95	100	100	100.0	100533	PASS
96	95	5	9	6.9	6950	PASS
173	174	0.00	2	1.0	908	PASS
174	95	50	100	90.3	90797	PASS
175	174	5	9	7.0	6332	PASS
176	174	95	101	95.6	86821	PASS
177	176	5	9	6.6	5695	PASS