


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN120519\
Data File : VN059490.D
Acq On : 5 Dec 2019 9:21
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Title : SW846 8260
Last Update : Tue Dec 03 16:37:42 2019

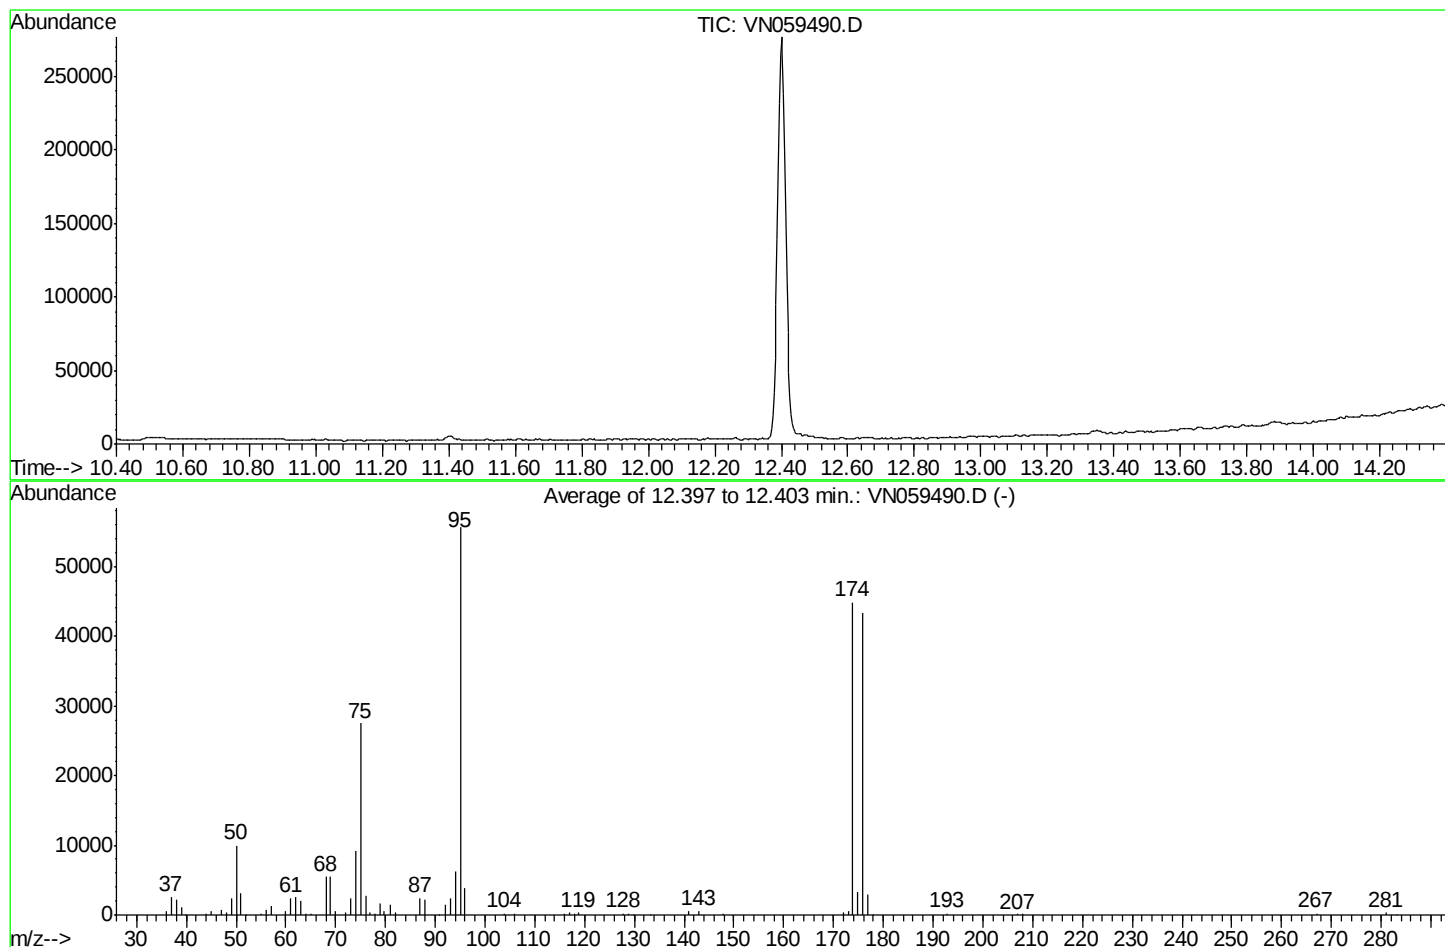

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	9946	PASS
75	95	30	60	49.4	27493	PASS
95	95	100	100	100.0	55610	PASS
96	95	5	9	6.9	3854	PASS
173	174	0.00	2	1.1	502	PASS
174	95	50	100	80.7	44872	PASS
175	174	5	9	7.5	3372	PASS
176	174	95	101	96.7	43413	PASS
177	176	5	9	6.6	2878	PASS