

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120523\
 Data File : VN080360.D
 Acq On : 05 Dec 2023 12:48
 Operator : JC\MD
 Sample : 05612-01 40X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Dec 06 00:50:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 17 01:19:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	171779	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	311125	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	328633	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	164236	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	148094	52.213	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 104.420%			
35) Dibromofluoromethane	8.165	113	118228	51.500	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 103.000%			
50) Toluene-d8	10.570	98	412650	49.864	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 99.720%			
62) 4-Bromofluorobenzene	12.853	95	177725	56.857	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 113.720%			
Target Compounds					Qvalue	
5) Bromomethane	2.971	94	545	0.394	ug/l #	74
6) Chloroethane	3.118	64	440	Below Cal	#	43
13) Acrolein	4.177	56	63	0.228	ug/l #	16
16) Acetone	4.453	43	218	0.229	ug/l #	40
18) Methyl Acetate	5.036	43	882	0.288	ug/l #	42
31) Cyclohexane	8.235	56	4355	1.412	ug/l #	54
36) 1,1-Dichloropropene	8.224	75	14253	4.288	ug/l #	51
38) Carbon Tetrachloride	8.229	117	20097	4.765	ug/l #	14
40) Benzene	8.606	78	239982	25.405	ug/l	99
42) 1,2-Dichloroethane	8.612	62	2619	0.678	ug/l #	73
43) Isopropyl Acetate	8.729	43	2269	0.506	ug/l #	49
52) Toluene	10.629	92	4490	0.760	ug/l	97
67) Ethyl Benzene	11.965	91	536316	40.474	ug/l	96
68) m/p-Xylenes	12.070	106	35238	7.294	ug/l	91
69) o-Xylene	12.400	106	46784	10.275	ug/l	91
70) Styrene	12.406	104	4756	0.702	ug/l #	1
71) Bromoform	12.853	173	927	0.433	ug/l #	1
73) Isopropylbenzene	12.694	105	15517	1.216	ug/l	97
76) 1,2,3-Trichloropropane	12.853	75	99089	24.624	ug/l #	1
78) n-propylbenzene	13.035	91	4645	0.325	ug/l	99
80) 1,3,5-Trimethylbenzene	13.176	105	12386	1.115	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.853	75	99089	83.195	ug/l #	15
83) tert-Butylbenzene	13.482	119	6485	0.728	ug/l #	53
84) 1,2,4-Trimethylbenzene	13.482	105	47404	4.333	ug/l	97
85) sec-Butylbenzene	13.482	105	47404	4.206	ug/l #	57
86) p-Isopropyltoluene	13.735	119	2269	0.225	ug/l #	72
89) n-Butylbenzene	14.000	91	104595	12.412	ug/l #	43
90) Hexachloroethane	14.329	117	1532	0.781	ug/l #	21
93) 1,2,4-Trichlorobenzene	15.400	180	835	0.259	ug/l	77
95) Naphthalene	15.641	128	2048402	218.935	ug/l	99
96) 1,2,3-Trichlorobenzene	15.847	180	1334	0.441	ug/l #	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120523\
Data File : VN080360.D
Acq On : 05 Dec 2023 12:48
Operator : JC\MD
Sample : 05612-01 40X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Dec 06 00:50:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 17 01:19:32 2023
Response via : Initial Calibration

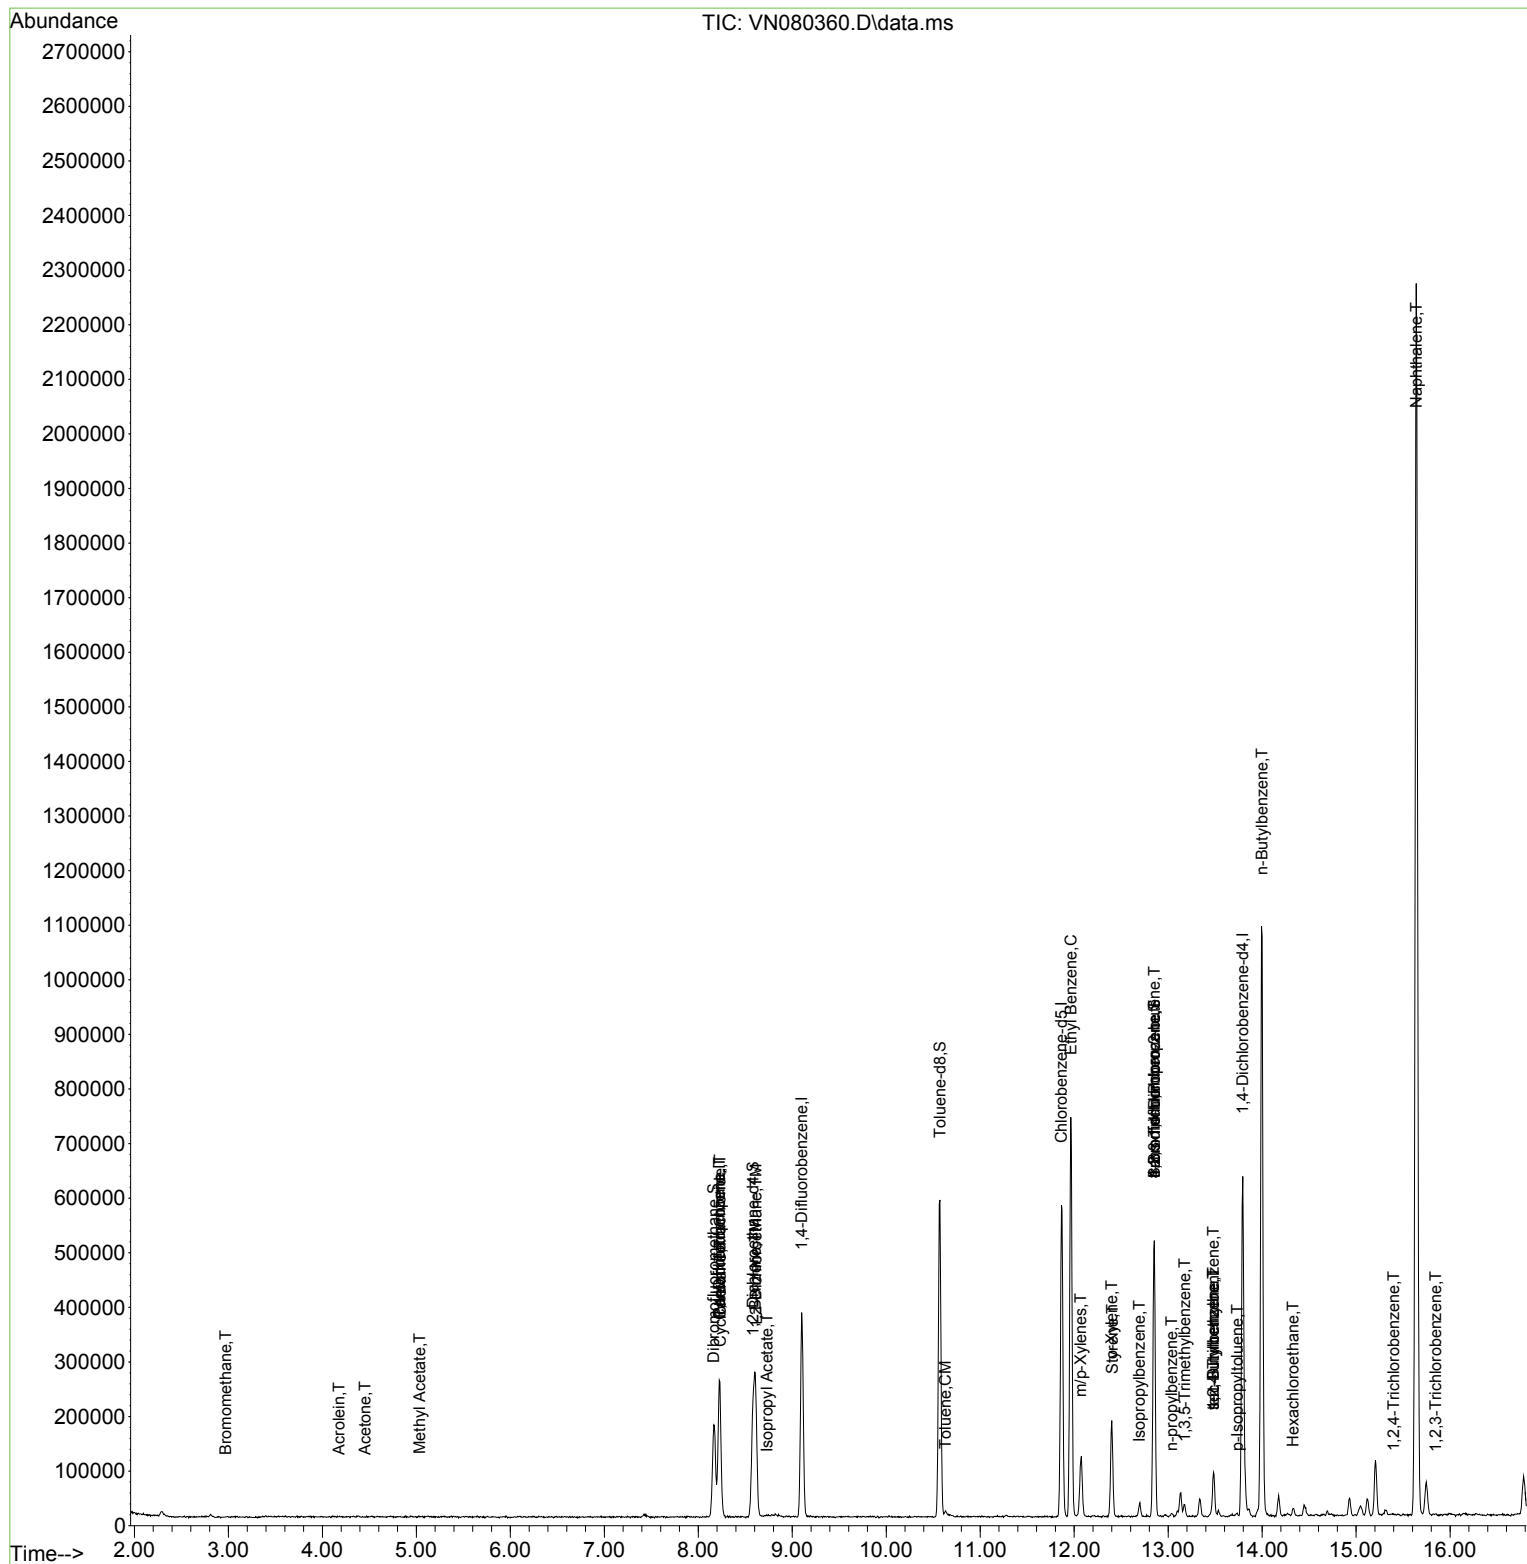






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 171779
Ion Ratio Lower Upper
168 100
99 63.9 53.0 79.6

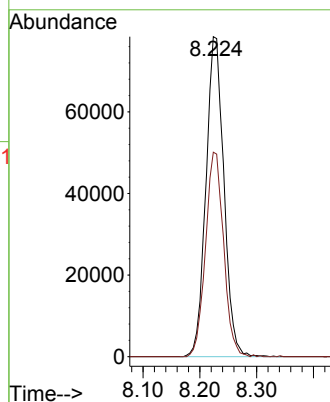

#5
Bromomethane
Concen: 0.394 ug/l
RT: 2.971 min Scan# 173
Delta R.T. 0.023 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Tgt Ion: 94 Resp: 545
Ion Ratio Lower Upper
94 100
96 66.6 73.1 109.7#



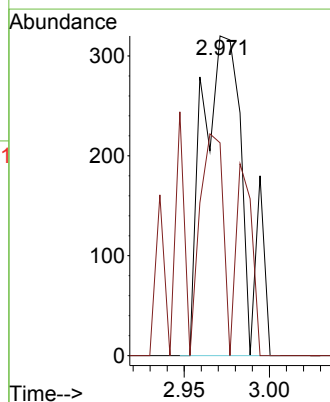
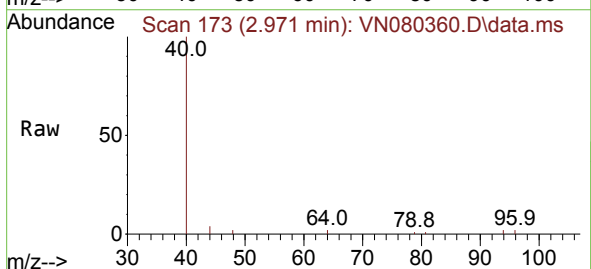




#6
Chloroethane
Concen: Below Cal
RT: 3.118 min Scan# 198
Delta R.T. 0.000 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 64 Resp: 440
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#



#13
Acrolein
Concen: 0.228 ug/l
RT: 4.177 min Scan# 378
Delta R.T. -0.000 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Tgt Ion: 56 Resp: 63
Ion Ratio Lower Upper
56 100
55 0.0 54.5 81.7#







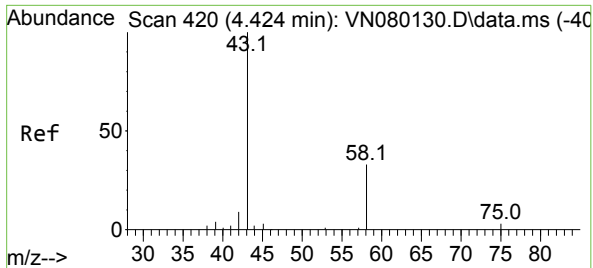

#16
Acetone
Concen: 0.229 ug/l
RT: 4.453 min Scan# 41
Delta R.T. 0.029 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 218
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#

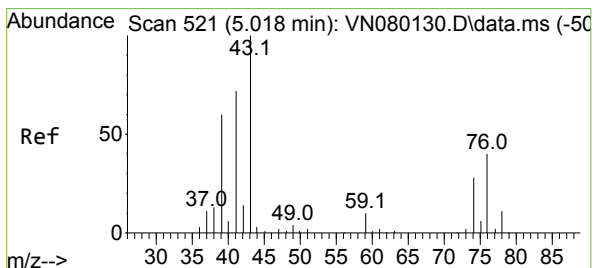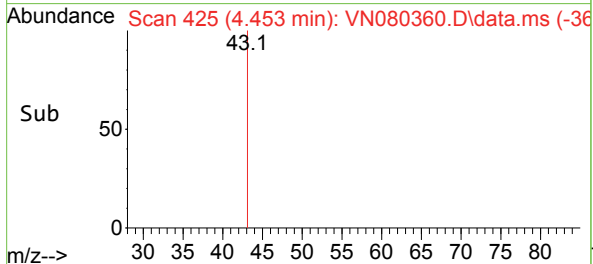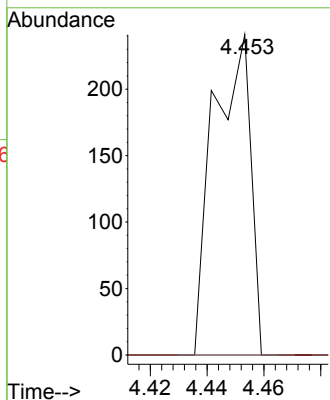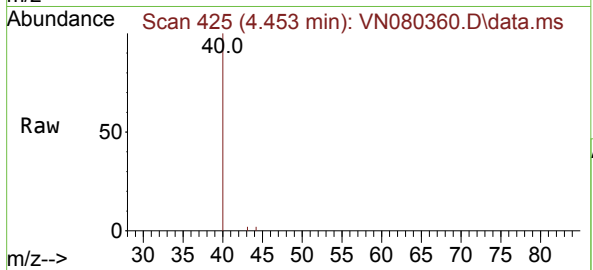

#18
Methyl Acetate
Concen: 0.288 ug/l
RT: 5.036 min Scan# 524
Delta R.T. 0.017 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48


Tgt Ion: 43 Resp: 882
Ion Ratio Lower Upper
43 100
74 0.0 26.2 39.4#

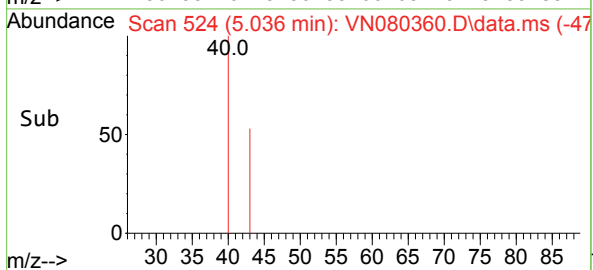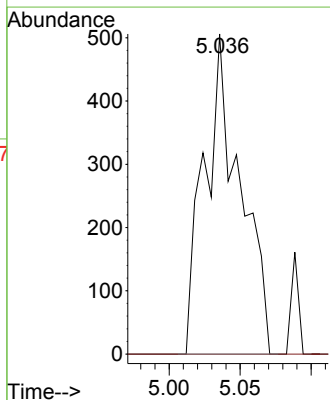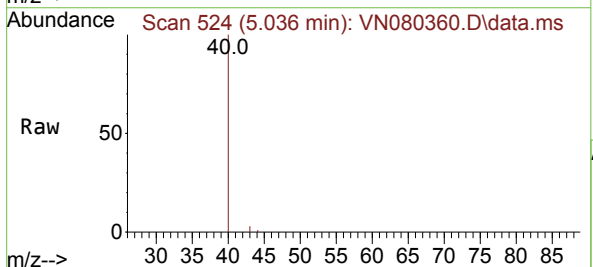






#31
Cyclohexane
Concen: 1.412 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. -0.024 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 4355
Ion Ratio Lower Upper
56 100
69 128.1 26.8 40.2#
84 95.4 81.8 122.6



#33
1,2-Dichloroethane-d4
Concen: 52.213 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Tgt Ion: 65 Resp: 148094
Ion Ratio Lower Upper
65 100
67 47.3 0.0 106.6

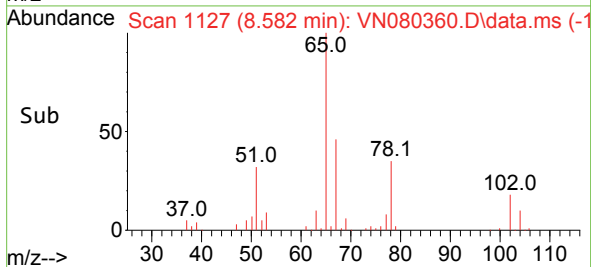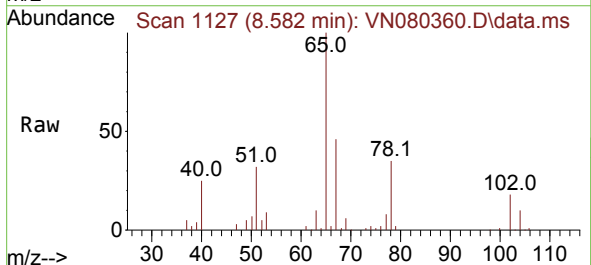



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. -0.006 min

Lab File: VN080360.D

Acq: 05 Dec 2023 12:48

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 311125

Ion Ratio Lower Upper

114 100

63 22.2 0.0 36.4

88 18.8 0.0 30.6

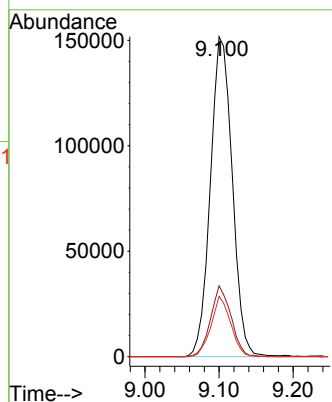

#35

Dibromofluoromethane

Concen: 51.500 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN080360.D

Acq: 05 Dec 2023 12:48




Tgt Ion:113 Resp: 118228


Ion Ratio Lower Upper

113 100

111 102.9 82.6 123.8

192 19.5 12.7 19.1#





#36

1,1-Dichloropropene

Concen: 4.288 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.153 min


Lab File: VN080360.D

Acq: 05 Dec 2023 12:48




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	75	Resp:	14253
Ion Ratio	100	Lower	Upper
75	100		
110	12.4	19.1	57.3#
77	0.0	25.0	37.4#

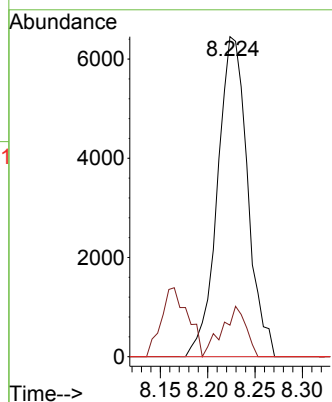

#38

Carbon Tetrachloride

Concen: 4.765 ug/l




RT: 8.229 min Scan# 1067


Delta R.T. -0.136 min

Lab File: VN080360.D

Acq: 05 Dec 2023 12:48

Tgt Ion:	117	Resp:	20097
Ion Ratio	100	Lower	Upper
117	100		
119	3.4	77.3	115.9#
121	0.0	23.3	34.9#









#40
Benzene
Concen: 25.405 ug/l
RT: 8.606 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 78 Resp: 239982
Ion Ratio Lower Upper
78 100
77 23.2 19.0 28.6

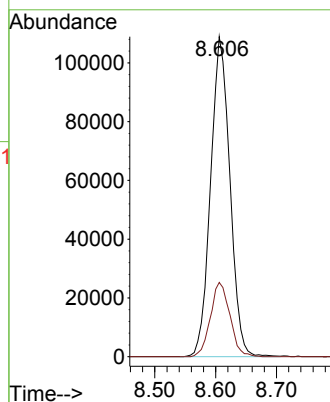

#42
1,2-Dichloroethane
Concen: 0.678 ug/l
RT: 8.612 min Scan# 1132
Delta R.T. -0.059 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Tgt Ion: 62 Resp: 2619
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.8


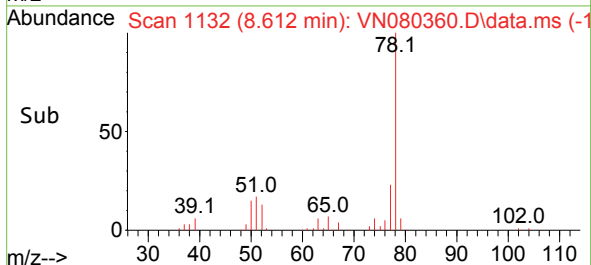
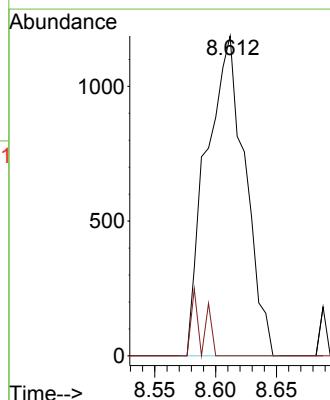
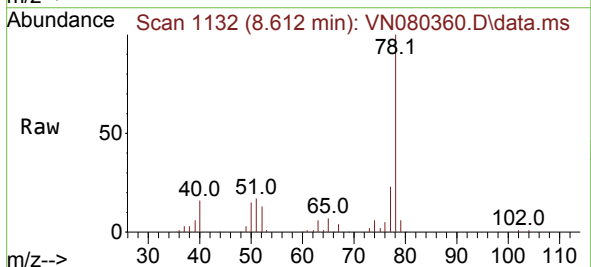




#43
Isopropyl Acetate
Concen: 0.506 ug/l
RT: 8.729 min Scan# 1152
Delta R.T. 0.041 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2269
Ion Ratio Lower Upper
43 100
61 0.0 24.7 37.1#
87 0.0 14.6 21.8#



#50
Toluene-d8
Concen: 49.864 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. 0.006 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Tgt Ion: 98 Resp: 412650
Ion Ratio Lower Upper
98 100
100 64.5 52.0 78.0

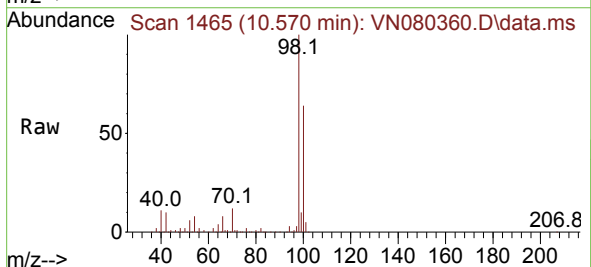



#52

Toluene

Concen: 0.760 ug/l

RT: 10.629 min Scan# 1475

Delta R.T. -0.000 min

Lab File: VN080360.D

Acq: 05 Dec 2023 12:48

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 92 Resp: 4490

Ion Ratio Lower Upper

92 100

91 176.3 137.4 206.0

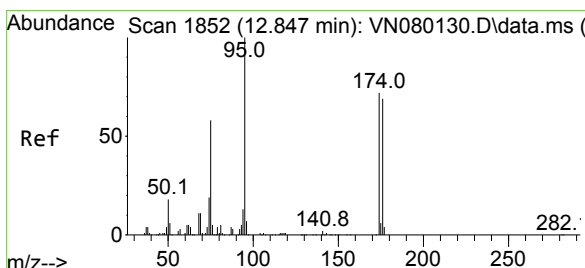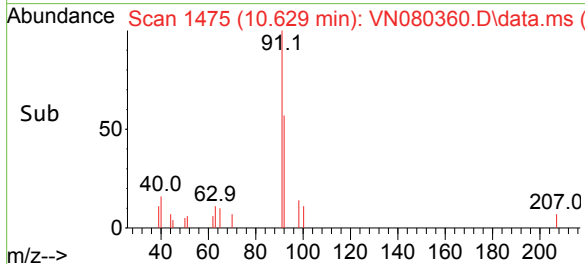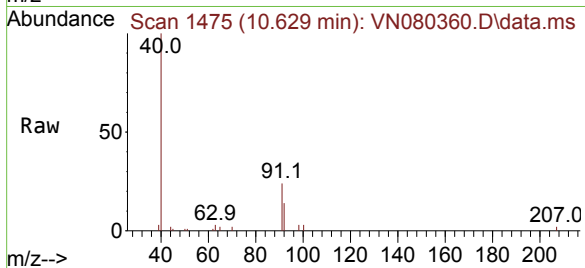

#62

4-Bromofluorobenzene

Concen: 56.857 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.006 min

Lab File: VN080360.D

Acq: 05 Dec 2023 12:48




Tgt Ion: 95 Resp: 177725


Ion Ratio Lower Upper

95 100

174 77.1 0.0 143.8

176 72.9 0.0 135.8


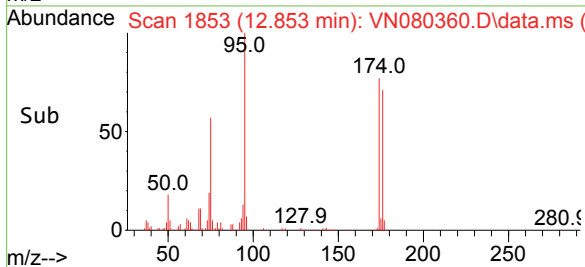

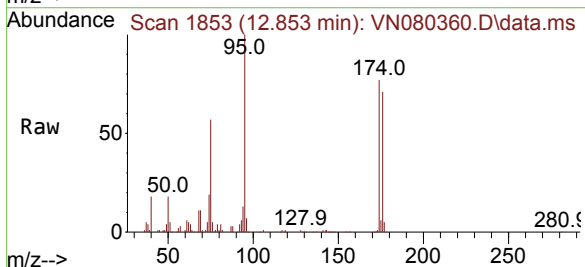




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 328633
Ion Ratio Lower Upper
117 100
82 58.8 44.0 66.0
119 31.8 25.6 38.4



#67
Ethyl Benzene
Concen: 40.474 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. -0.000 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Tgt Ion: 91 Resp: 536316
Ion Ratio Lower Upper
91 100
106 29.9 25.6 38.4




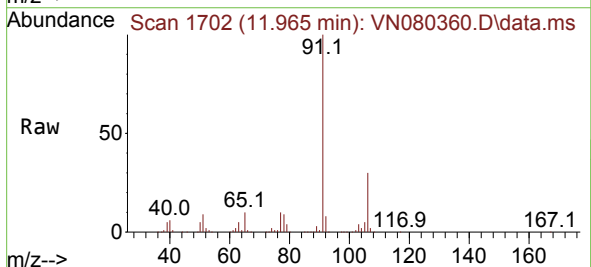




#68
m/p-Xylenes
Concen: 7.294 ug/l
RT: 12.070 min Scan# 1720
Delta R.T. -0.000 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 35238
Ion Ratio Lower Upper
106 100
91 212.9 159.6 239.4

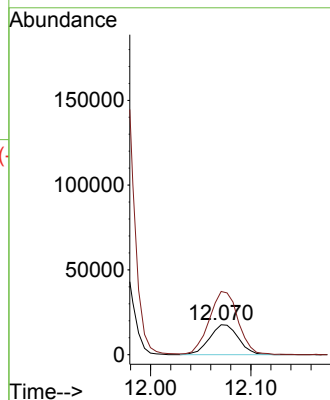

#69
o-Xylene
Concen: 10.275 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. -0.000 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Tgt Ion:106 Resp: 46784
Ion Ratio Lower Upper
106 100
91 224.7 105.2 315.5



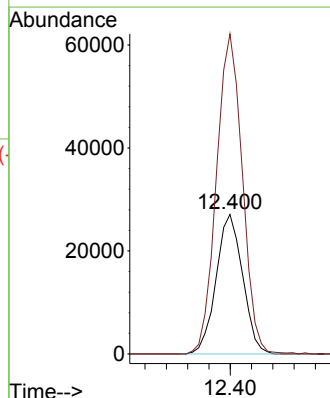
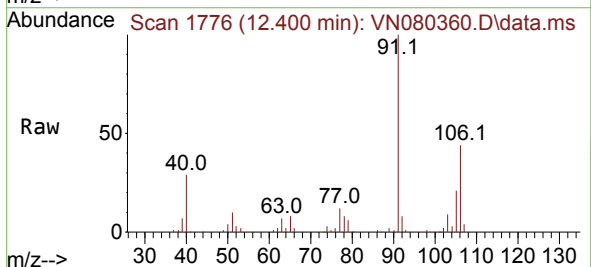




#70
Styrene
Concen: 0.702 ug/l
RT: 12.406 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:104 Resp: 4756
Ion Ratio Lower Upper
104 100
78 198.7 39.5 59.3#
103 181.8 43.2 64.8#

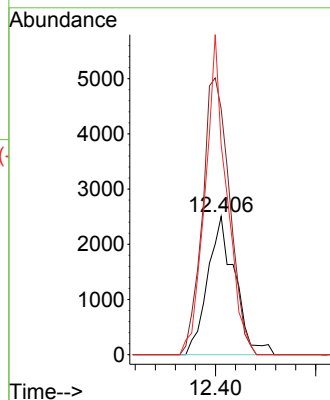

#71
Bromoform
Concen: 0.433 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.270 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Tgt Ion:173 Resp: 927
Ion Ratio Lower Upper
173 100
175 877.1 24.3 73.0#
254 0.0 0.0 0.0

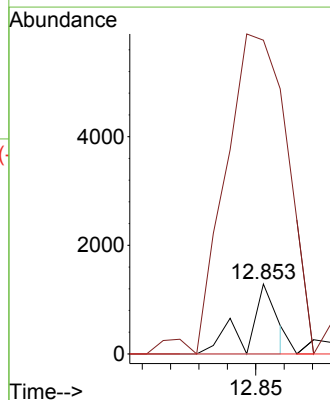



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.000 min


Lab File: VN080360.D

Acq: 05 Dec 2023 12:48

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:152 Resp: 164236

Ion Ratio Lower Upper

152 100

115 65.8 32.3 96.8

150 157.0 0.0 355.8

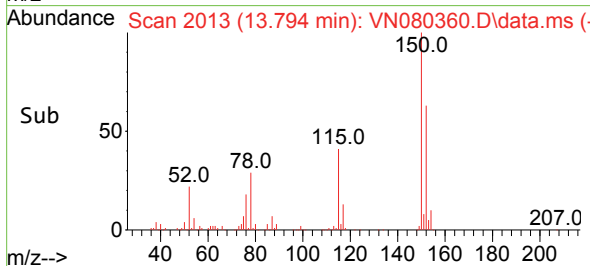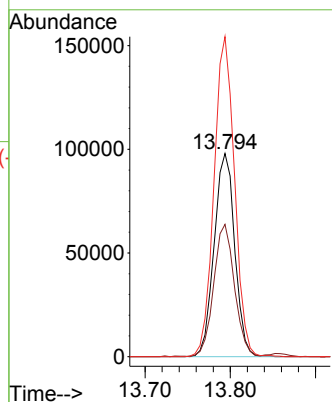

#73

Isopropylbenzene

Concen: 1.216 ug/l

RT: 12.694 min Scan# 1826

Delta R.T. -0.006 min

Lab File: VN080360.D




Acq: 05 Dec 2023 12:48


Tgt Ion:105 Resp: 15517

Ion Ratio Lower Upper

105 100

120 24.5 13.1 39.1


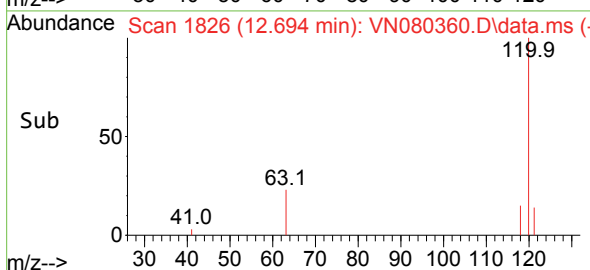

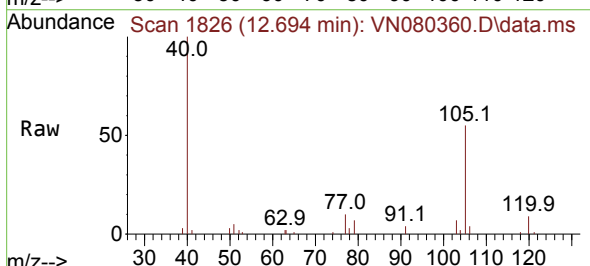




#76
1,2,3-Trichloropropane
Concen: 24.624 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.141 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 99089
Ion Ratio Lower Upper
75 100
77 1.0 84.5 253.5#

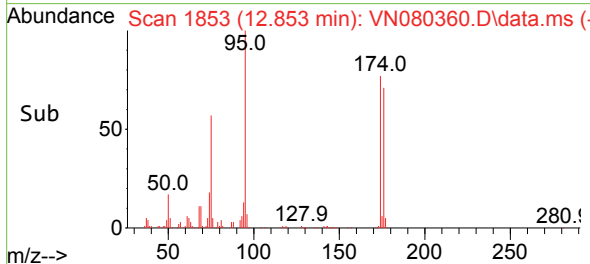

#78
n-propylbenzene
Concen: 0.325 ug/l
RT: 13.035 min Scan# 1884
Delta R.T. -0.000 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Tgt Ion: 91 Resp: 4645
Ion Ratio Lower Upper
91 100
120 23.3 11.5 34.4

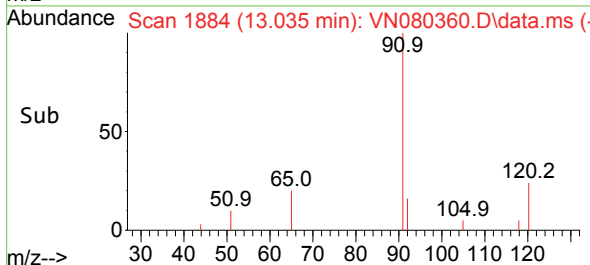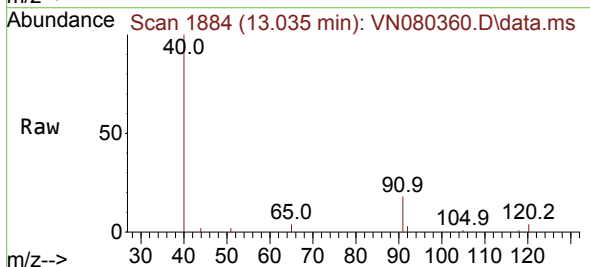



#80

1,3,5-Trimethylbenzene

Concen: 1.115 ug/l

RT: 13.176 min Scan# 1908

Delta R.T. -0.000 min MSVOA_N

Lab File: VN080360.D

Acq: 05 Dec 2023 12:48

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 12386

Ion Ratio Lower Upper

105 100

120 49.0 24.1 72.3

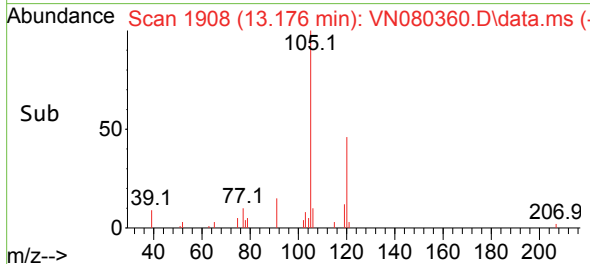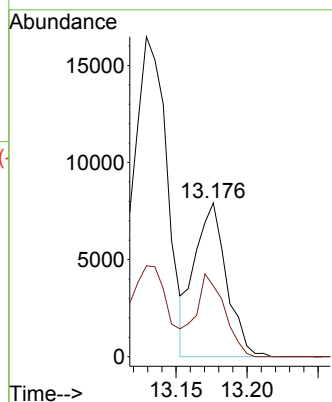

#81

trans-1,4-Dichloro-2-butene

Concen: 83.195 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN080360.D

Acq: 05 Dec 2023 12:48




Tgt Ion: 75 Resp: 99089


Ion Ratio Lower Upper

75 100

53 0.0 67.4 101.2#

89 0.0 38.8 58.2#


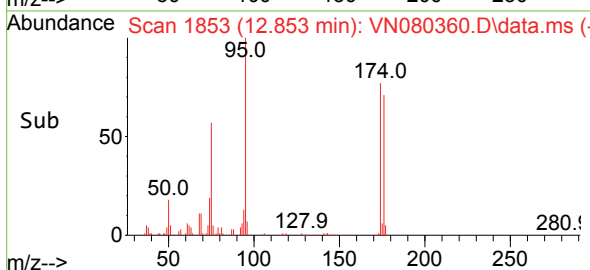

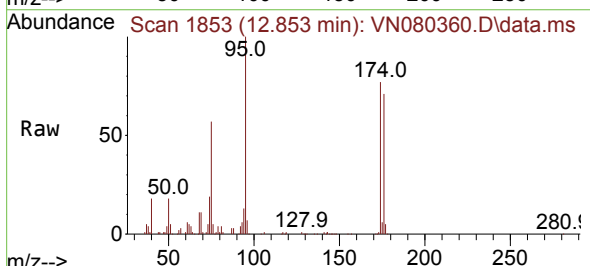




#83
 tert-Butylbenzene
 Concen: 0.728 ug/l
 RT: 13.482 min Scan# 1960
 Delta R.T. 0.041 min
 Lab File: VN080360.D
 Acq: 05 Dec 2023 12:48




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:119 Resp: 6485
 Ion Ratio Lower Upper
 119 100
 91 104.1 33.9 101.7#
 134 0.0 13.2 39.6#



#84
 1,2,4-Trimethylbenzene
 Concen: 4.333 ug/l
 RT: 13.482 min Scan# 1960
 Delta R.T. -0.000 min
 Lab File: VN080360.D
 Acq: 05 Dec 2023 12:48

Tgt Ion:105 Resp: 47404
 Ion Ratio Lower Upper
 105 100
 120 42.0 22.0 66.0




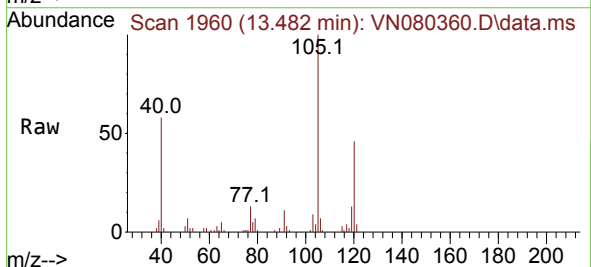




#85
 sec-Butylbenzene
 Concen: 4.206 ug/l
 RT: 13.482 min Scan# 1983
 Delta R.T. -0.136 min
 Lab File: VN080360.D
 Acq: 05 Dec 2023 12:48




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:105 Resp: 47404
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.3#

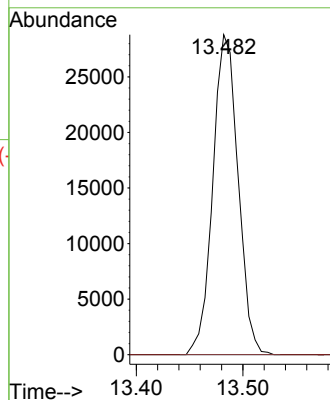

#86
 p-Isopropyltoluene
 Concen: 0.225 ug/l
 RT: 13.735 min Scan# 2003
 Delta R.T. 0.006 min
 Lab File: VN080360.D
 Acq: 05 Dec 2023 12:48

Tgt Ion:119 Resp: 2269
 Ion Ratio Lower Upper
 119 100
 134 28.3 12.6 37.8
 91 0.0 12.4 37.2#



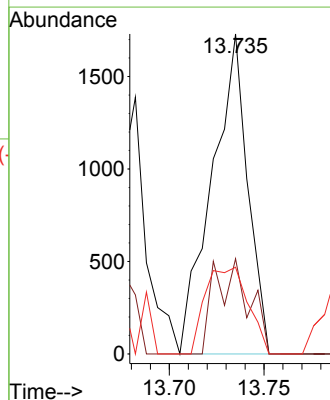
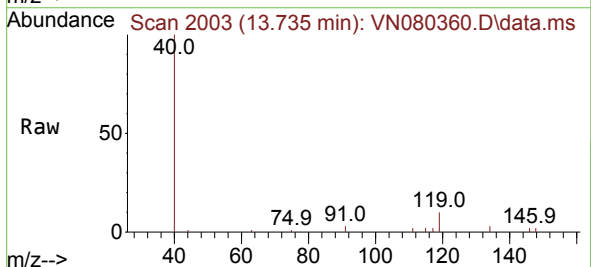


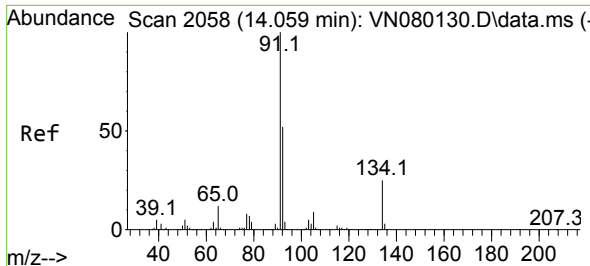

#89
n-Butylbenzene
Concen: 12.412 ug/l
RT: 14.000 min Scan# 2058
Delta R.T. -0.059 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 104595
Ion Ratio Lower Upper
91 100
92 10.1 26.4 79.0#
134 0.0 12.6 37.6#

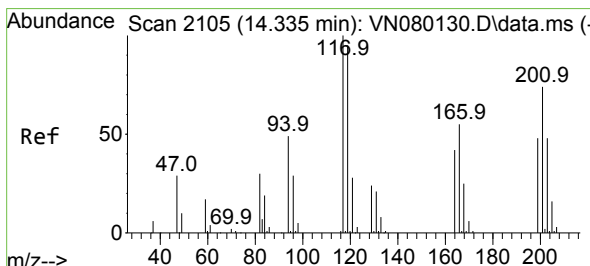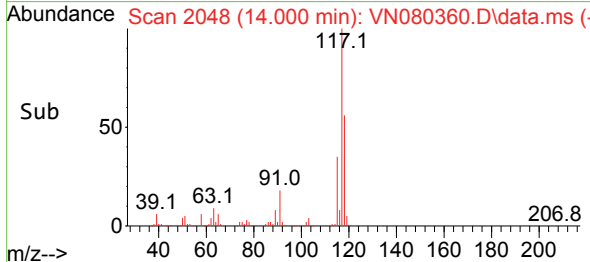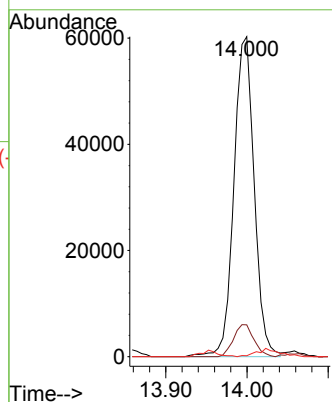

#90
Hexachloroethane
Concen: 0.781 ug/l
RT: 14.329 min Scan# 2104
Delta R.T. -0.006 min
Lab File: VN080360.D
Acq: 05 Dec 2023 12:48

Tgt Ion: 117 Resp: 1532
Ion Ratio Lower Upper
117 100
201 0.0 29.3 88.0#

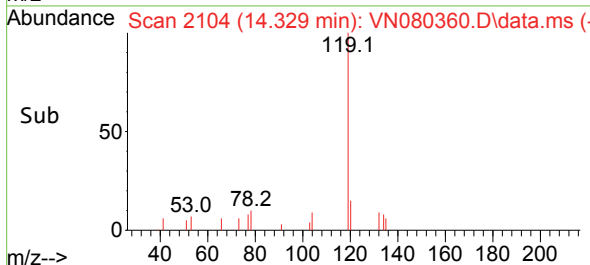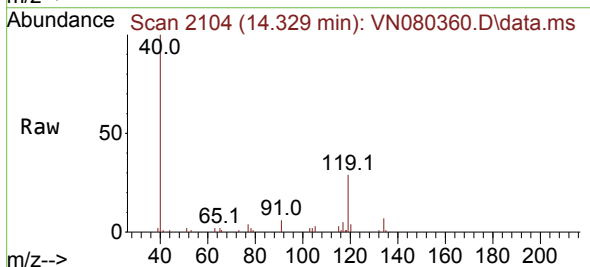



#93

1,2,4-Trichlorobenzene

Concen: 0.259 ug/l

RT: 15.400 min Scan# 21

Delta R.T. 0.006 min


Lab File: VN080360.D

Acq: 05 Dec 2023 12:48

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:180 Resp: 835

Ion Ratio Lower Upper

180 100

182 112.9 46.1 138.2

145 47.1 16.6 49.8

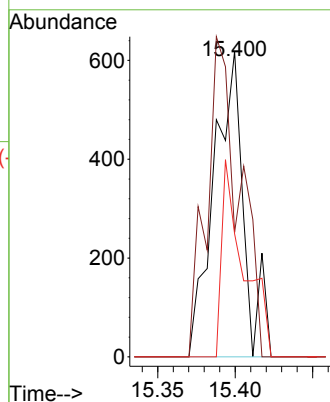

#95

Naphthalene

Concen: 218.935 ug/l

RT: 15.641 min Scan# 2327

Delta R.T. -0.000 min

Lab File: VN080360.D

Acq: 05 Dec 2023 12:48




Tgt Ion:128 Resp: 2048402


Ion Ratio Lower Upper

128 100

127 12.9 10.0 15.0


129 10.7 8.7 13.1

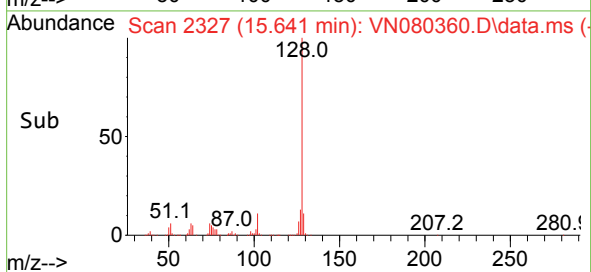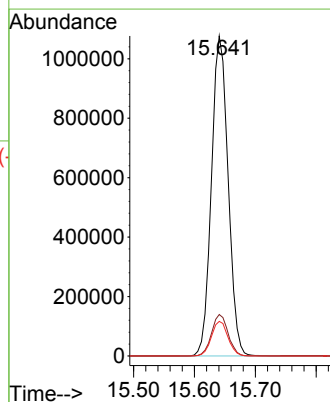



#96
 1,2,3-Trichlorobenzene
 Concen: 0.441 ug/l
 RT: 15.847 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN080360.D
 Acq: 05 Dec 2023 12:48

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion	Ratio	Lower	Upper
180	100		
182	36.4	46.2	138.6#
145	9.3	17.5	52.6#

