

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN120523\  
 Data File : VN080367.D  
 Acq On : 05 Dec 2023 15:34  
 Operator : JC\MD  
 Sample : 05616-03  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :

Quant Time: Dec 06 00:53:00 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N111623W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Nov 17 01:19:32 2023  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response            | Conc      | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|-----------|--------|----------|
| -----                         |                |      |                     |           |        |          |
| Internal Standards            |                |      |                     |           |        |          |
| 1) Pentafluorobenzene         | 8.229          | 168  | 165825              | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 9.100          | 114  | 296446              | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.865         | 117  | 317533              | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.794         | 152  | 164813              | 50.000    | ug/l   | 0.00     |
|                               |                |      |                     |           |        |          |
| System Monitoring Compounds   |                |      |                     |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.577          | 65   | 146294              | 53.430    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = 106.860% |           |        |          |
| 35) Dibromofluoromethane      | 8.165          | 113  | 118069              | 53.977    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 107.960% |           |        |          |
| 50) Toluene-d8                | 10.571         | 98   | 394168              | 49.989    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = 99.980%  |           |        |          |
| 62) 4-Bromofluorobenzene      | 12.847         | 95   | 164678              | 55.292    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = 110.580% |           |        |          |
|                               |                |      |                     |           |        |          |
| Target Compounds              |                |      |                     |           | Qvalue |          |
| 6) Chloroethane               | 3.112          | 64   | 402                 | Below Cal | #      | 43       |
| 11) Tert butyl alcohol        | 5.518          | 59   | 4825                | 16.025    | ug/l # | 92       |
| 16) Acetone                   | 4.430          | 43   | 29865               | 32.475    | ug/l   | 89       |
| 18) Methyl Acetate            | 5.030          | 43   | 1035                | 0.350     | ug/l # | 76       |
| 20) Methylene Chloride        | 5.289          | 84   | 391                 | 0.203     | ug/l # | 13       |
| 25) 2-Butanone                | 7.488          | 43   | 8079                | 7.394     | ug/l # | 80       |
| 31) Cyclohexane               | 8.218          | 56   | 3647                | 1.225     | ug/l # | 49       |
| 36) 1,1-Dichloropropene       | 8.218          | 75   | 13359               | 4.218     | ug/l # | 48       |
| 37) Ethyl Acetate             | 7.488          | 43   | 8079                | 3.678     | ug/l # | 63       |
| 38) Carbon Tetrachloride      | 8.224          | 117  | 18978               | 4.722     | ug/l # | 16       |
| 40) Benzene                   | 8.606          | 78   | 18506               | 2.056     | ug/l   | 97       |
| 43) Isopropyl Acetate         | 8.741          | 43   | 1382                | 0.323     | ug/l # | 49       |
| 48) Methyl methacrylate       | 9.659          | 41   | 7102                | 3.224     | ug/l # | 30       |
| 49) 1,4-Dioxane               | 9.706          | 88   | 55                  | 1.501     | ug/l # | 30       |
| 51) 4-Methyl-2-Pentanone      | 10.447         | 43   | 1187                | 0.536     | ug/l   | 94       |
| 52) Toluene                   | 10.635         | 92   | 22466               | 3.988     | ug/l   | 98       |
| 59) 2-Hexanone                | 11.194         | 43   | 2220                | 1.248     | ug/l   | 87       |
| 67) Ethyl Benzene             | 11.965         | 91   | 7700                | 0.601     | ug/l   | 99       |
| 68) m/p-Xylenes               | 12.070         | 106  | 11570               | 2.478     | ug/l   | 89       |
| 69) o-Xylene                  | 12.394         | 106  | 5308                | 1.207     | ug/l   | 80       |
| 71) Bromoform                 | 12.853         | 173  | 833                 | 0.402     | ug/l # | 1        |
| 74) N-amyl acetate            | 12.459         | 43   | 3178                | 0.796     | ug/l # | 40       |
| 76) 1,2,3-Trichloropropane    | 12.853         | 75   | 92163               | 22.823    | ug/l # | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.853         | 75   | 92163               | 77.109    | ug/l # | 15       |
| 84) 1,2,4-Trimethylbenzene    | 13.482         | 105  | 5340                | 0.486     | ug/l   | 97       |
| 95) Naphthalene               | 15.647         | 128  | 12791               | 1.362     | ug/l # | 94       |
| -----                         |                |      |                     |           |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN120523\  
Data File : VN080367.D  
Acq On : 05 Dec 2023 15:34  
Operator : JC\MD  
Sample : 05616-03  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :

Quant Time: Dec 06 00:53:00 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N111623W.M  
Quant Title : SW846 8260  
QLast Update : Fri Nov 17 01:19:32 2023  
Response via : Initial Calibration




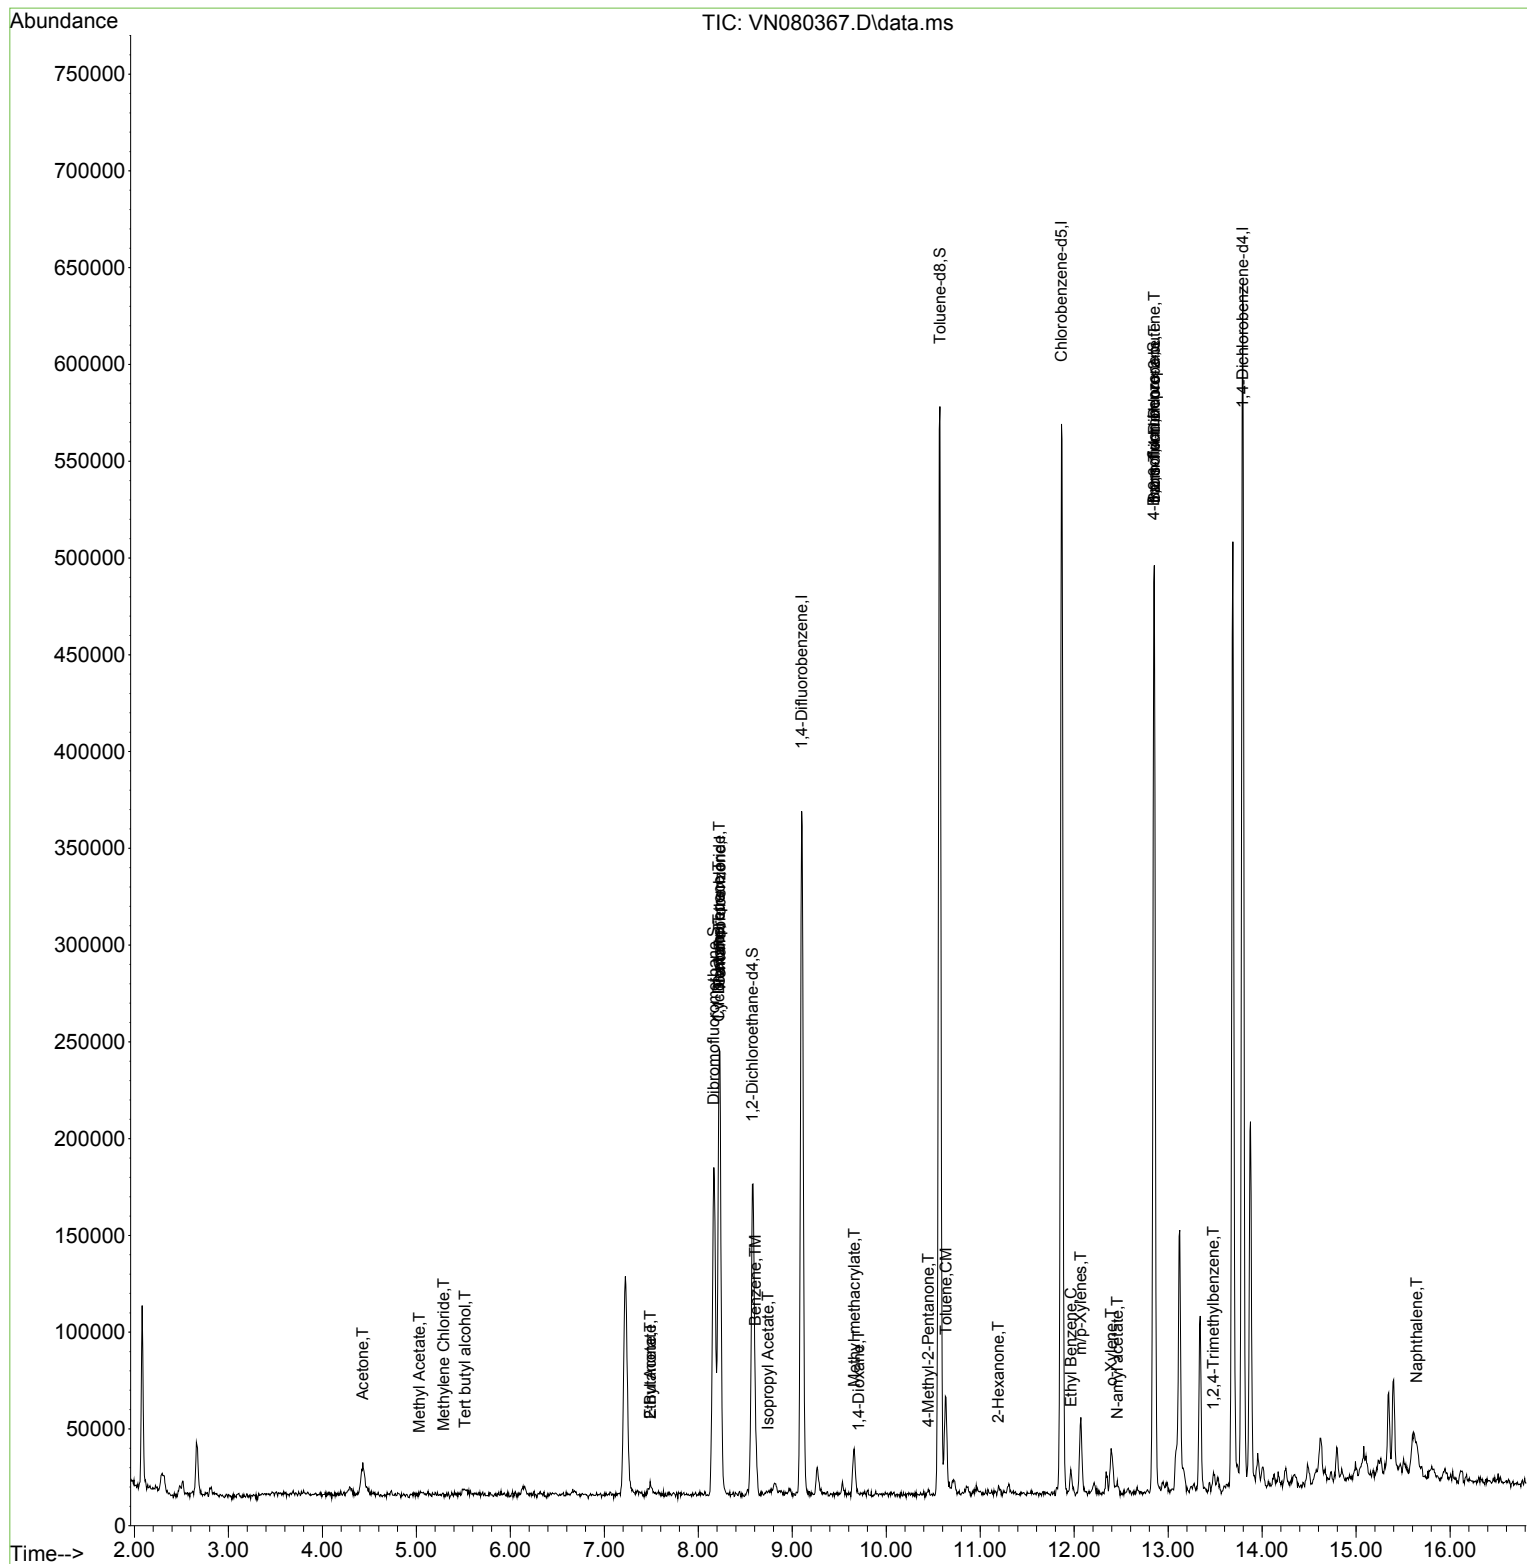




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.229 min Scan# 1066  
Delta R.T. 0.005 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion:168 Resp: 165825  
Ion Ratio Lower Upper  
168 100  
99 60.1 53.0 79.6

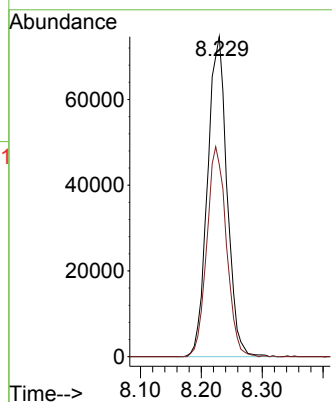

#6  
Chloroethane  
Concen: Below Cal  
RT: 3.112 min Scan# 197  
Delta R.T. -0.006 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion: 64 Resp: 402  
Ion Ratio Lower Upper  
64 100  
66 0.0 25.4 38.2#


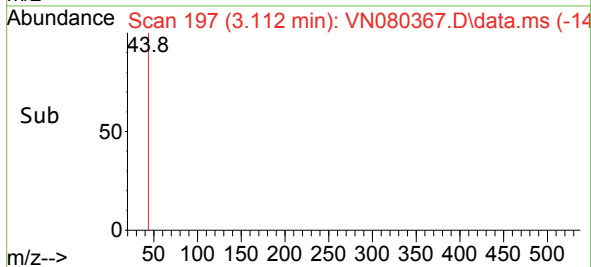
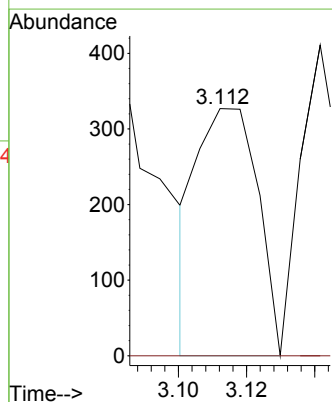
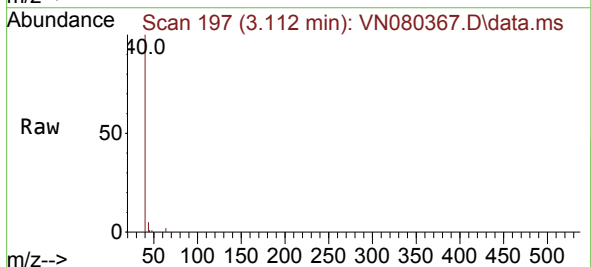




#11  
Tert butyl alcohol  
Concen: 16.025 ug/l  
RT: 5.518 min Scan# 606  
Delta R.T. -0.000 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 59 Resp: 4825  
Ion Ratio Lower Upper  
59 100  
57 7.3 8.2 12.4#



#16  
Acetone  
Concen: 32.475 ug/l  
RT: 4.430 min Scan# 421  
Delta R.T. 0.006 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion: 43 Resp: 29865  
Ion Ratio Lower Upper  
43 100  
58 28.5 28.0 42.0


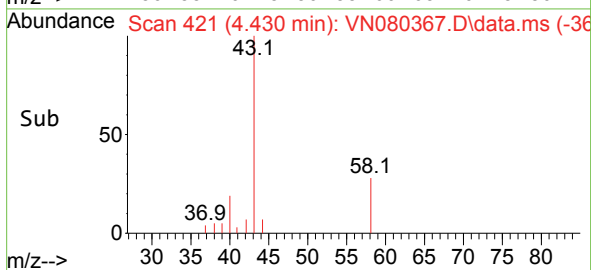






#18  
Methyl Acetate  
Concen: 0.350 ug/l  
RT: 5.030 min Scan# 51  
Delta R.T. 0.012 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 1035  
Ion Ratio Lower Upper  
43 100  
74 19.4 26.2 39.4#

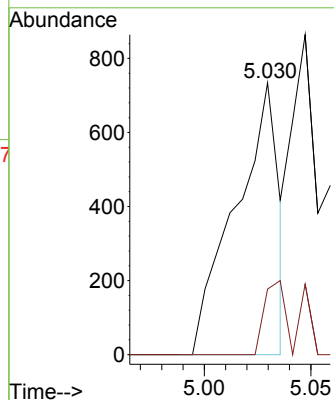

#20  
Methylene Chloride  
Concen: 0.203 ug/l  
RT: 5.289 min Scan# 567  
Delta R.T. 0.012 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion: 84 Resp: 391  
Ion Ratio Lower Upper  
84 100  
49 0.0 79.7 119.5#  
51 0.0 25.2 37.8#  
86 0.0 53.3 79.9#


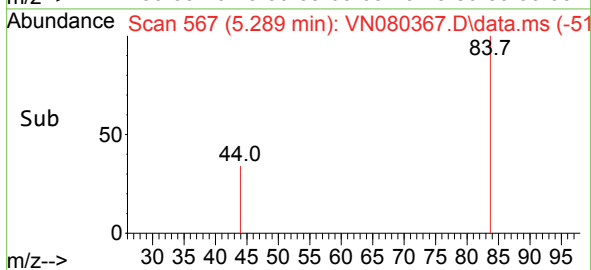
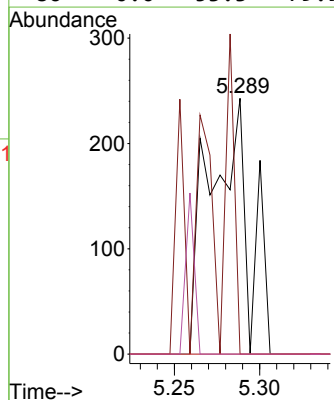



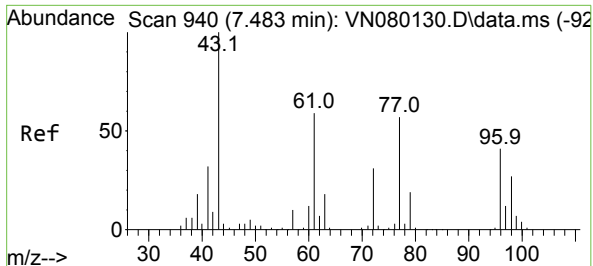

#25  
2-Butanone  
Concen: 7.394 ug/l  
RT: 7.488 min Scan# 941  
Delta R.T. 0.006 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 8079  
Ion Ratio Lower Upper  
43 100  
72 49.9 30.2 45.2#

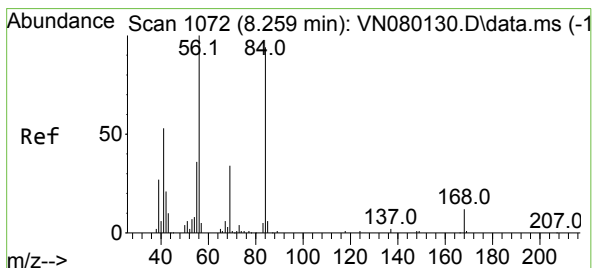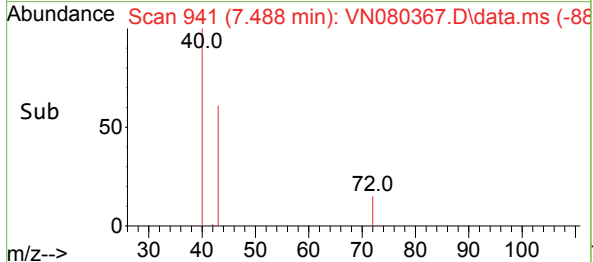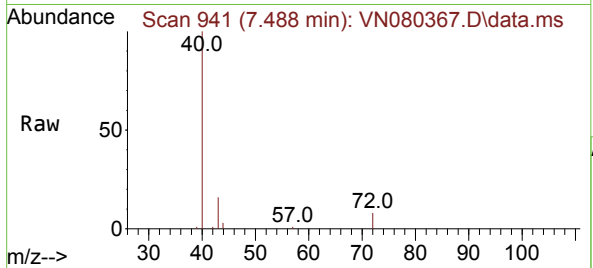

#31  
Cyclohexane  
Concen: 1.225 ug/l  
RT: 8.218 min Scan# 1065  
Delta R.T. -0.041 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion: 56 Resp: 3647  
Ion Ratio Lower Upper  
56 100  
69 135.2 26.8 40.2#  
84 93.1 81.8 122.6

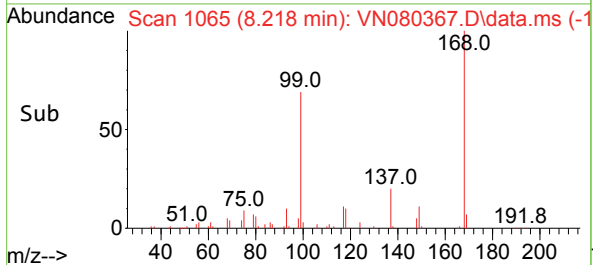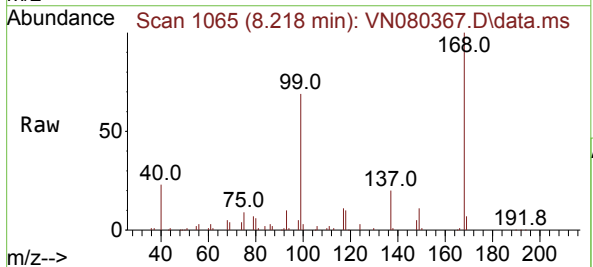



#33

1,2-Dichloroethane-d4

Concen: 53.430 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VN080367.D

Acq: 05 Dec 2023 15:34

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 65 Resp: 146294

Ion Ratio Lower Upper

65 100

67 47.0 0.0 106.6

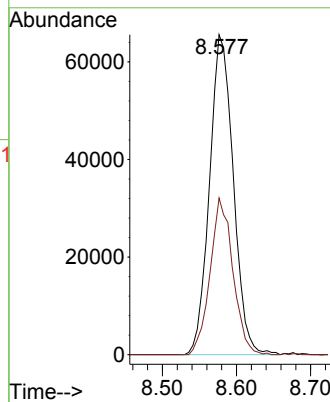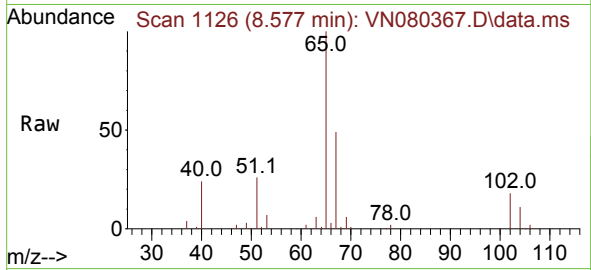

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. -0.006 min

Lab File: VN080367.D

Acq: 05 Dec 2023 15:34




Tgt Ion: 114 Resp: 296446


Ion Ratio Lower Upper

114 100

63 20.6 0.0 36.4


88 18.1 0.0 30.6

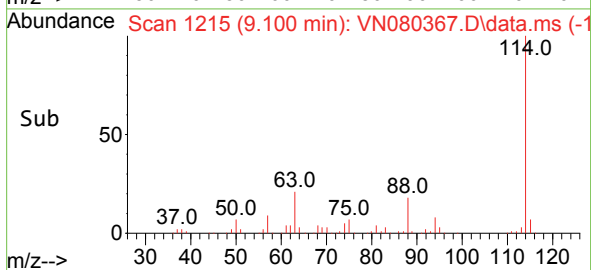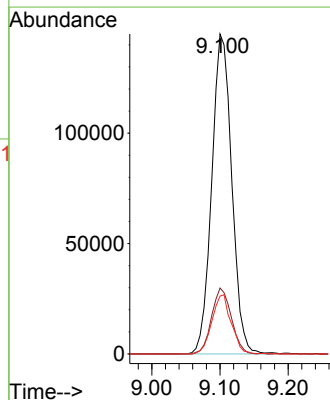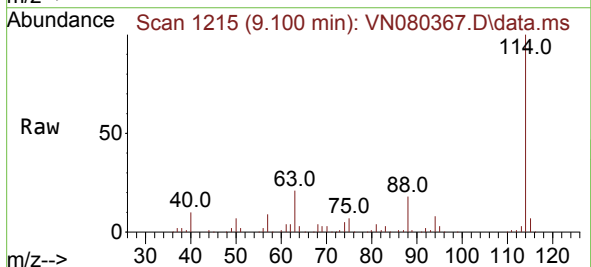






#35  
Dibromofluoromethane  
Concen: 53.977 ug/l  
RT: 8.165 min Scan# 1056  
Delta R.T. -0.000 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion:113 Resp: 118069  
Ion Ratio Lower Upper  
113 100  
111 101.9 82.6 123.8  
192 19.0 12.7 19.1

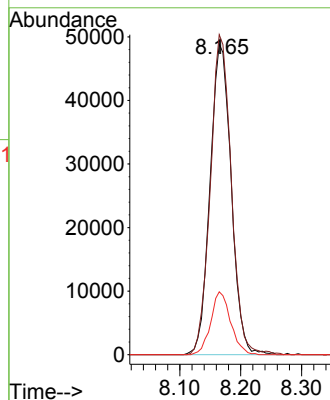

#36  
1,1-Dichloropropene  
Concen: 4.218 ug/l  
RT: 8.218 min Scan# 1065  
Delta R.T. -0.159 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34


Tgt Ion: 75 Resp: 13359  
Ion Ratio Lower Upper  
75 100  
110 9.3 19.1 57.3#  
77 0.0 25.0 37.4#

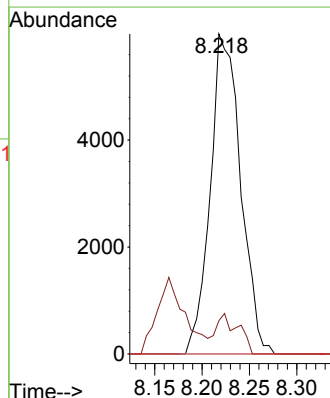






#37  
Ethyl Acetate  
Concen: 3.678 ug/l  
RT: 7.488 min Scan# 941  
Delta R.T. -0.071 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 43 Resp: 8079  
Ion Ratio Lower Upper  
43 100  
61 0.0 13.2 19.8#  
70 0.0 11.3 16.9#

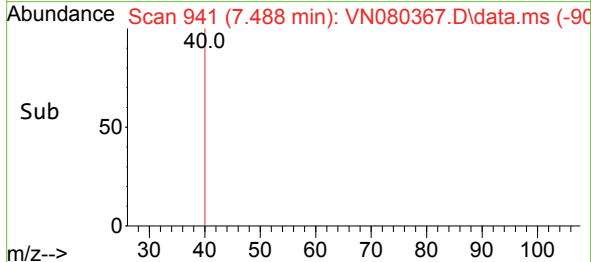

#38  
Carbon Tetrachloride  
Concen: 4.722 ug/l  
RT: 8.224 min Scan# 1066  
Delta R.T. -0.141 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion: 117 Resp: 18978  
Ion Ratio Lower Upper  
117 100  
119 5.1 77.3 115.9#  
121 0.0 23.3 34.9#


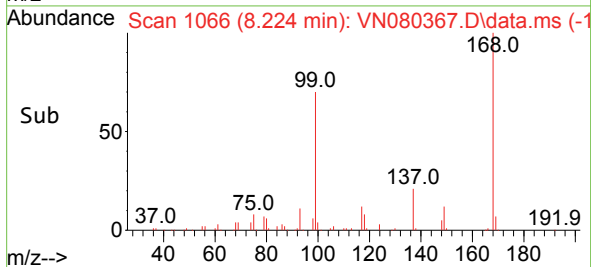

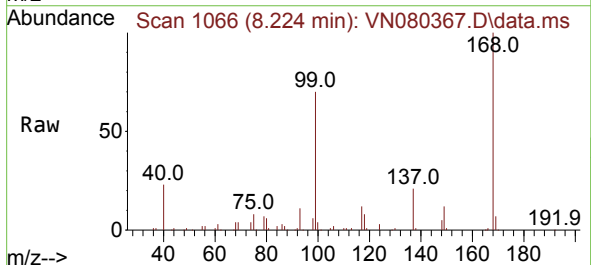




#40  
Benzene  
Concen: 2.056 ug/l  
RT: 8.606 min Scan# 1131  
Delta R.T. -0.000 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 78 Resp: 18506  
Ion Ratio Lower Upper  
78 100  
77 25.1 19.0 28.6

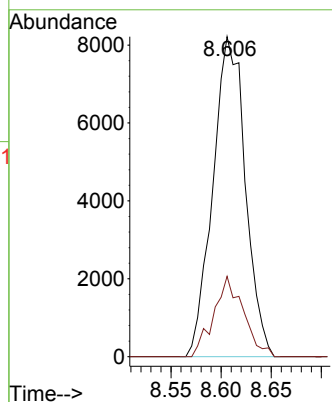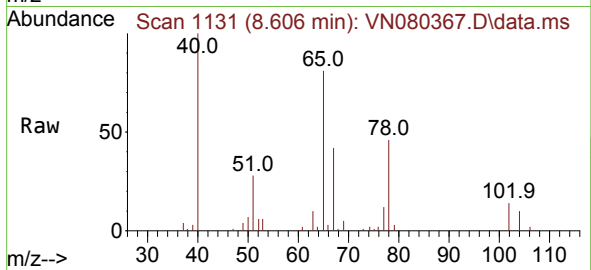

#43  
Isopropyl Acetate  
Concen: 0.323 ug/l  
RT: 8.741 min Scan# 1154  
Delta R.T. 0.053 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion: 43 Resp: 1382  
Ion Ratio Lower Upper  
43 100  
61 0.0 24.7 37.1#  
87 0.0 14.6 21.8#

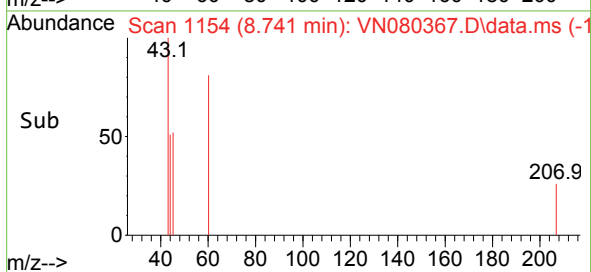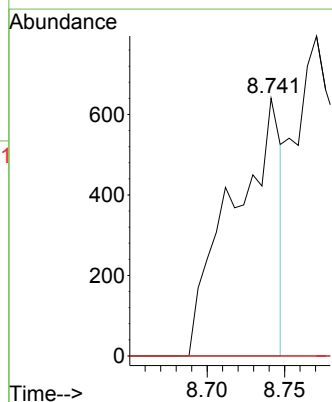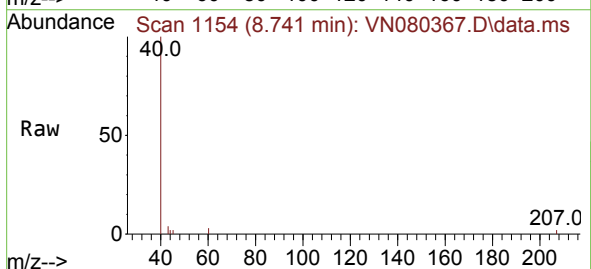



#48

Methyl methacrylate

Concen: 3.224 ug/l

RT: 9.659 min Scan# 1310

Delta R.T. -0.024 min

Lab File: VN080367.D

Acq: 05 Dec 2023 15:34

Instrument :

MSVOA\_N

ClientSampleId :





Tgt Ion: 41 Resp: 7102

Ion Ratio Lower Upper

41 100

69 0.0 90.4 135.6#

39 59.0 54.6 81.8

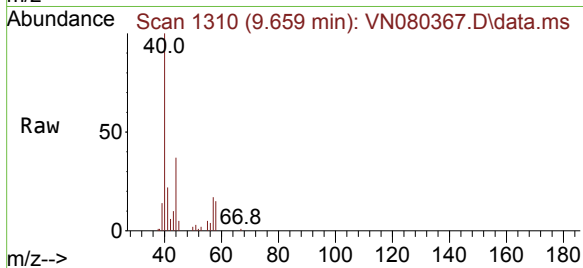

#49

1,4-Dioxane

Concen: 1.501 ug/l

RT: 9.706 min Scan# 1318

Delta R.T. 0.012 min

Lab File: VN080367.D

Acq: 05 Dec 2023 15:34




Tgt Ion: 88 Resp: 55


Ion Ratio Lower Upper

88 100

43 0.0 17.0 25.6#

58 0.0 47.0 70.4#


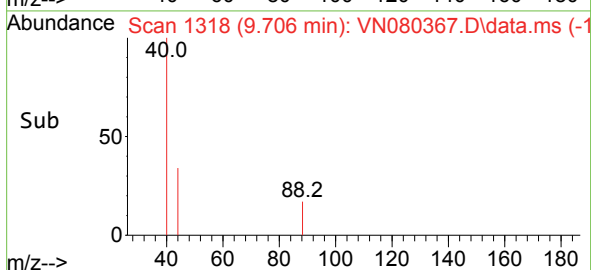

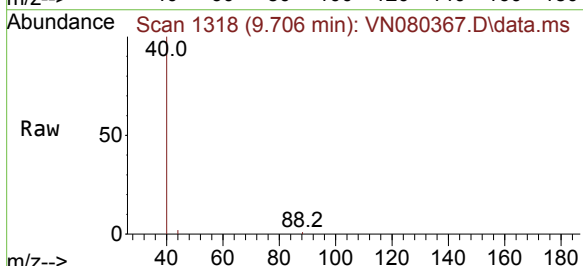


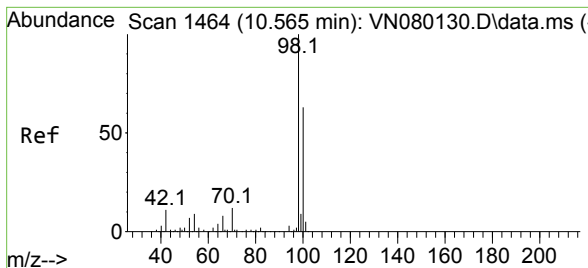

#50  
Toluene-d8  
Concen: 49.989 ug/l  
RT: 10.571 min Scan# 1465  
Delta R.T. 0.006 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 98 Resp: 394168  
Ion Ratio Lower Upper  
98 100  
100 64.4 52.0 78.0

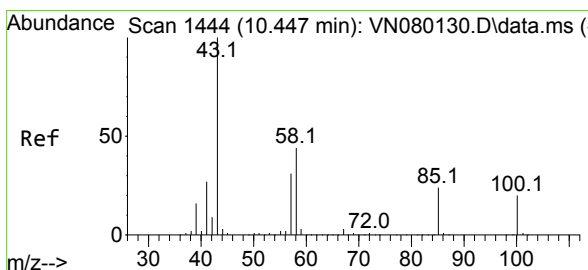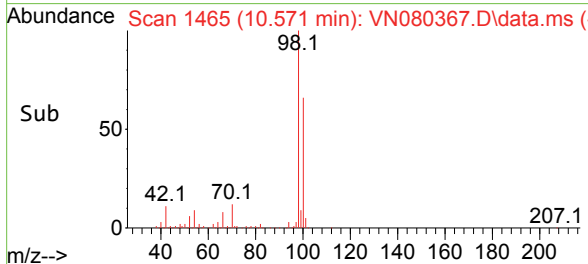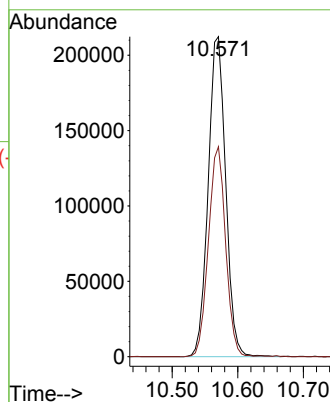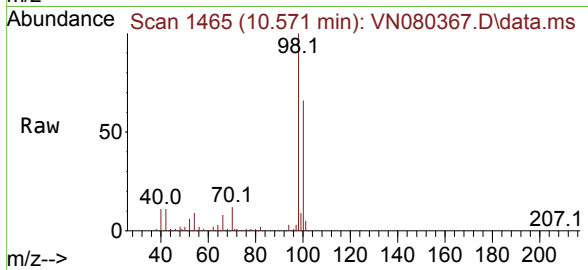

#51  
4-Methyl-2-Pentanone  
Concen: 0.536 ug/l  
RT: 10.447 min Scan# 1444  
Delta R.T. -0.000 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion: 43 Resp: 1187  
Ion Ratio Lower Upper  
43 100  
58 41.7 36.6 54.8


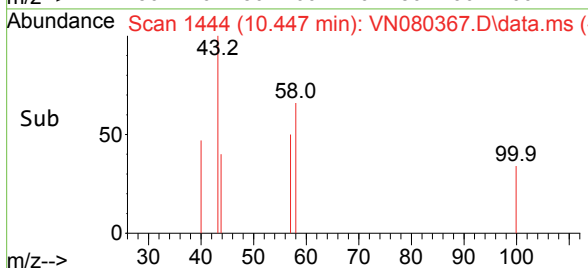
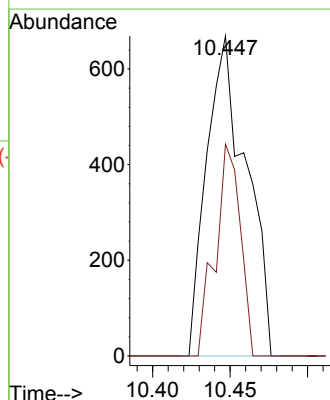
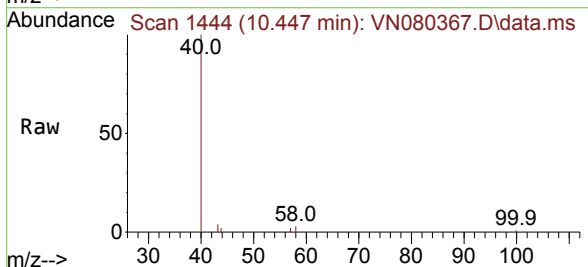


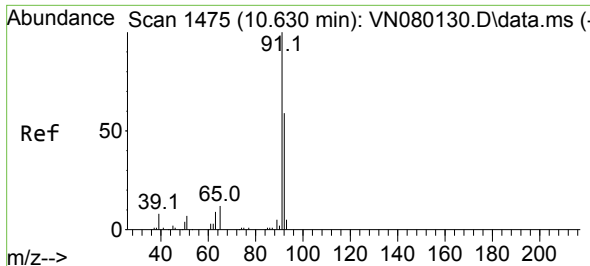

#52  
Toluene  
Concen: 3.988 ug/l  
RT: 10.635 min Scan# 1475  
Delta R.T. 0.006 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 92 Resp: 22466  
Ion Ratio Lower Upper  
92 100  
91 174.1 137.4 206.0

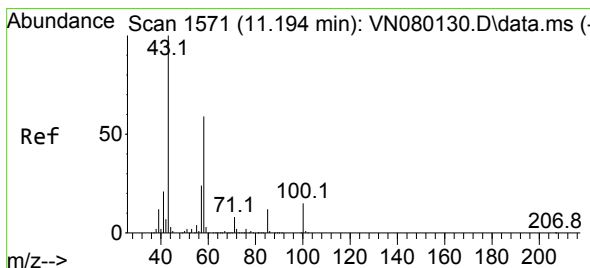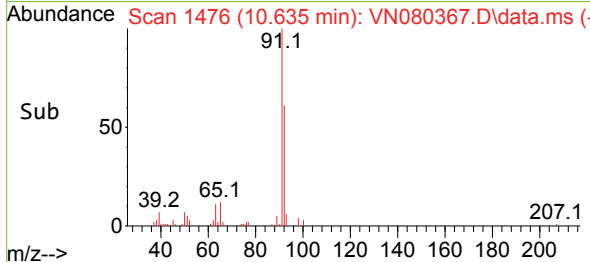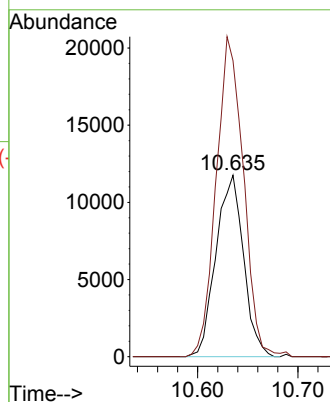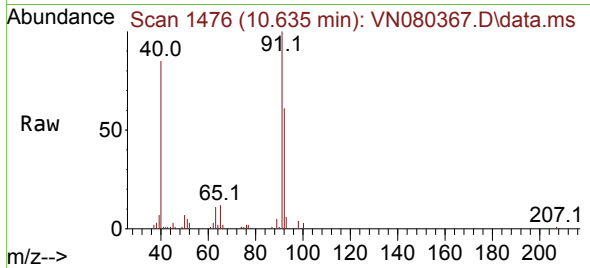

#59  
2-Hexanone  
Concen: 1.248 ug/l  
RT: 11.194 min Scan# 1571  
Delta R.T. -0.000 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion: 43 Resp: 2220  
Ion Ratio Lower Upper  
43 100  
58 53.4 31.7 95.1


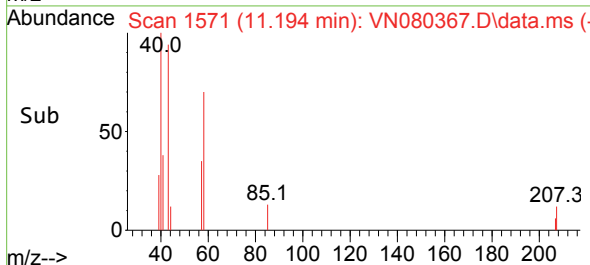
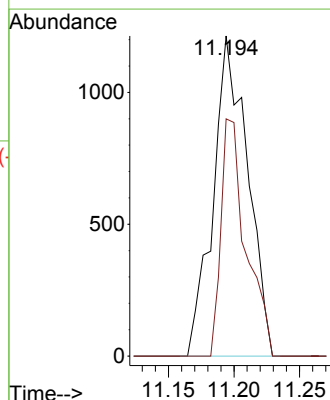
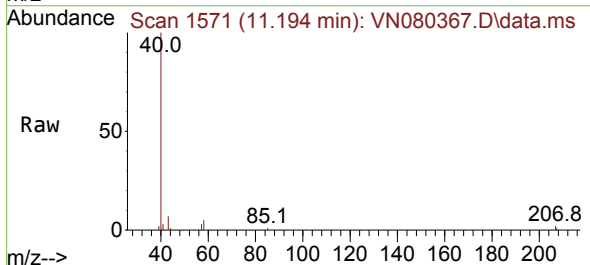


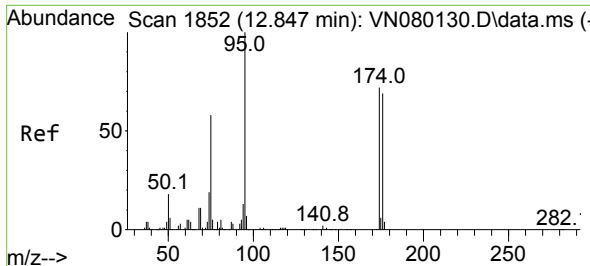

#62  
4-Bromofluorobenzene  
Concen: 55.292 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. -0.000 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 95 Resp: 164678  
Ion Ratio Lower Upper  
95 100  
174 77.8 0.0 143.8  
176 75.1 0.0 135.8

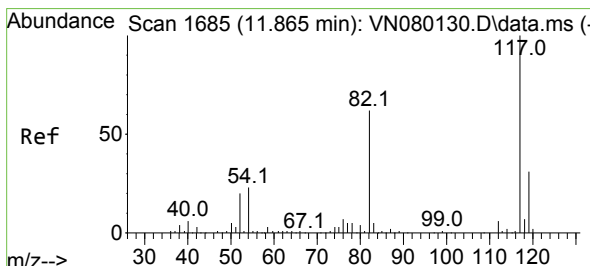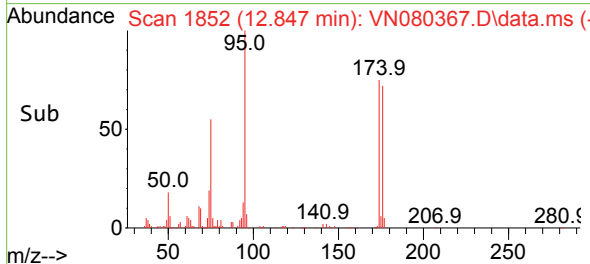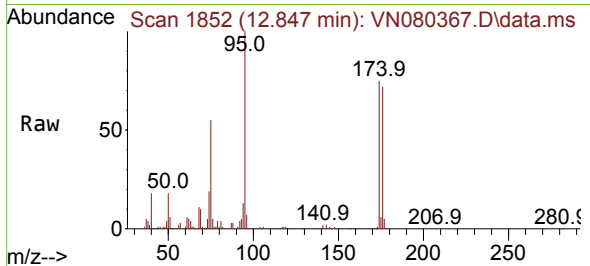

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.865 min Scan# 1685  
Delta R.T. -0.000 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion: 117 Resp: 317533  
Ion Ratio Lower Upper  
117 100  
82 62.5 44.0 66.0  
119 32.0 25.6 38.4


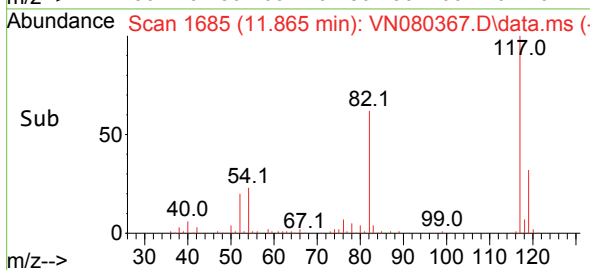

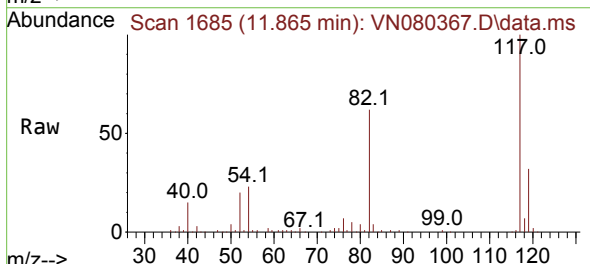




#67  
Ethyl Benzene  
Concen: 0.601 ug/l  
RT: 11.965 min Scan# 1702  
Delta R.T. -0.000 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 91 Resp: 7700  
Ion Ratio Lower Upper  
91 100  
106 32.4 25.6 38.4

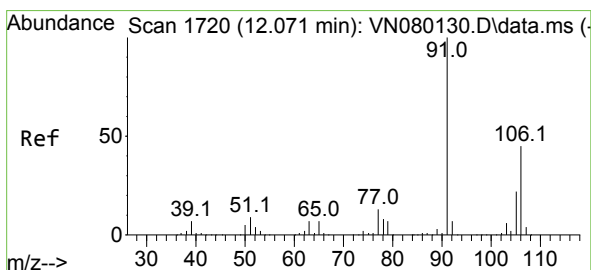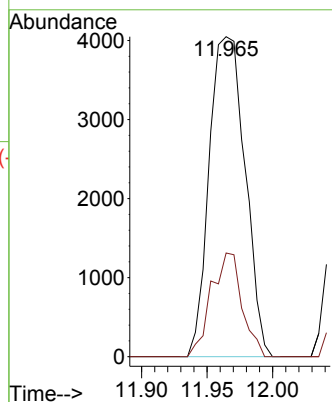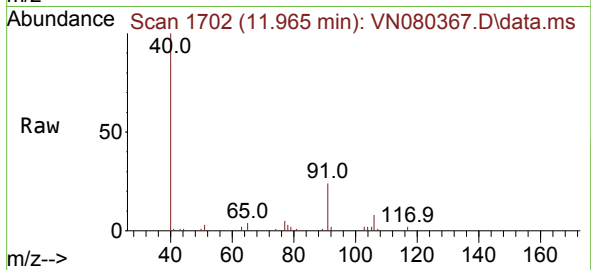

#68  
m/p-Xylenes  
Concen: 2.478 ug/l  
RT: 12.070 min Scan# 1720  
Delta R.T. -0.000 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion:106 Resp: 11570  
Ion Ratio Lower Upper  
106 100  
91 216.5 159.6 239.4


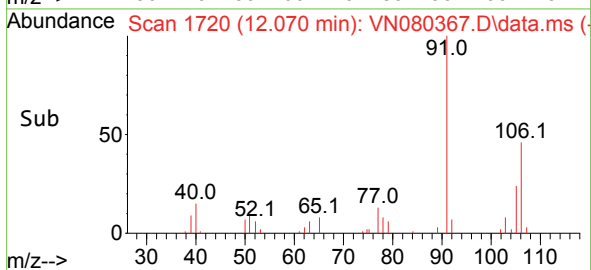
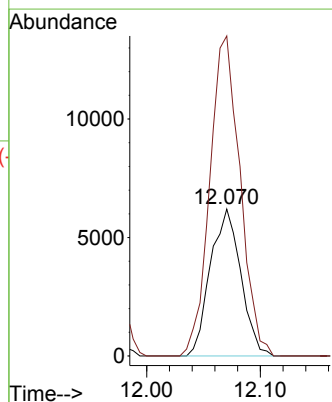
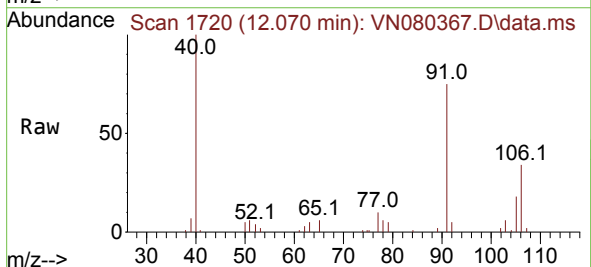




#69  
o-Xylene  
Concen: 1.207 ug/l  
RT: 12.394 min Scan# 11  
Delta R.T. -0.006 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion:106 Resp: 5308  
Ion Ratio Lower Upper  
106 100  
91 241.2 105.2 315.5

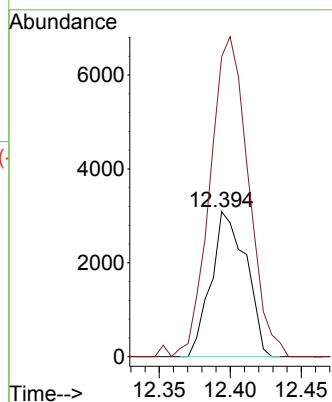

#71  
Bromoform  
Concen: 0.402 ug/l  
RT: 12.853 min Scan# 1853  
Delta R.T. 0.270 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34


Tgt Ion:173 Resp: 833  
Ion Ratio Lower Upper  
173 100  
175 1032.2 24.3 73.0#  
254 0.0 0.0 0.0

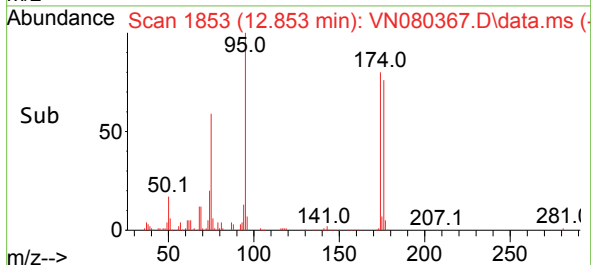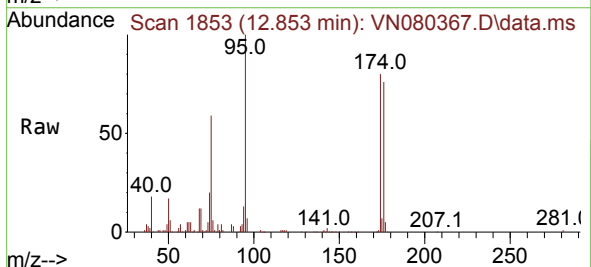



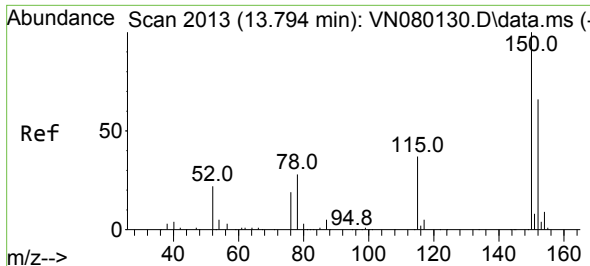


#72  
 1,4-Dichlorobenzene-d4  
 Concen: 50.000 ug/l  
 RT: 13.794 min Scan# 20  
 Delta R.T. -0.000 min  
 Lab File: VN080367.D  
 Acq: 05 Dec 2023 15:34


Instrument :  
 MSVOA\_N  
 ClientSampleId :

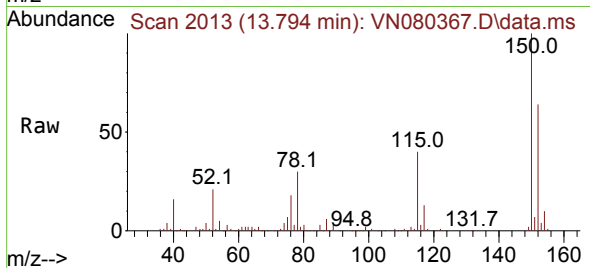



Tgt Ion:152 Resp: 164813  
 Ion Ratio Lower Upper  
 152 100  
 115 66.6 32.3 96.8  
 150 157.2 0.0 355.8

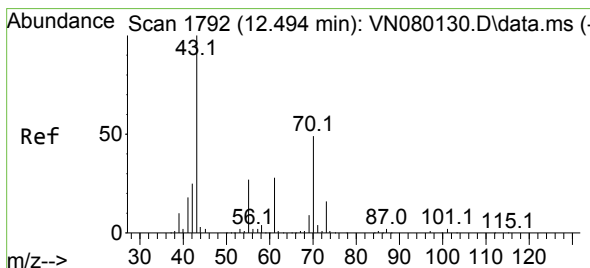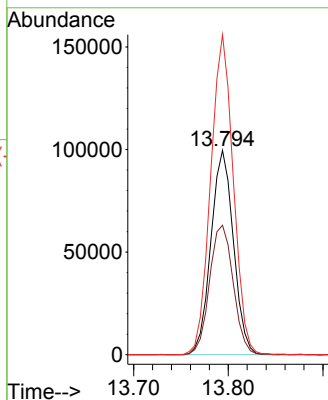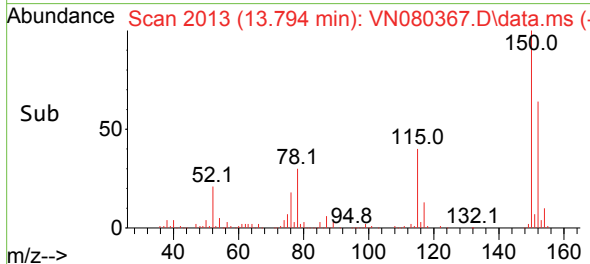


#74  
 N-ethyl acetate  
 Concen: 0.796 ug/l  
 RT: 12.459 min Scan# 1786  
 Delta R.T. -0.035 min  
 Lab File: VN080367.D  
 Acq: 05 Dec 2023 15:34

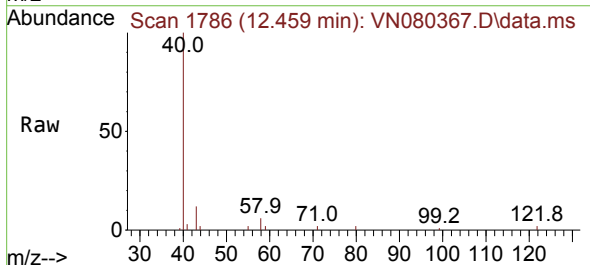

Tgt Ion: 43 Resp: 3178  
 Ion Ratio Lower Upper  
 43 100  
 70 0.0 43.4 65.2#  
 55 9.2 21.4 32.0#  
 61 0.0 22.8 34.2#



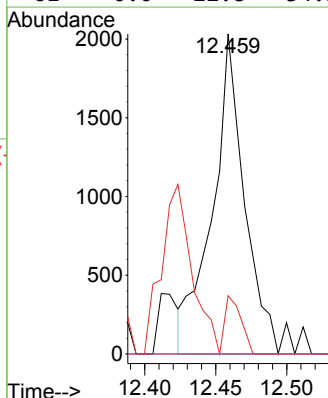
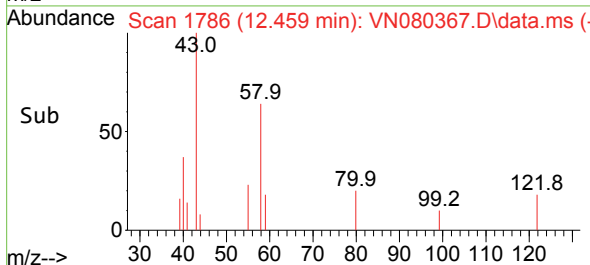




#76  
1,2,3-Trichloropropane  
Concen: 22.823 ug/l  
RT: 12.853 min Scan# 1853  
Delta R.T. -0.141 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 75 Resp: 92163  
Ion Ratio Lower Upper  
75 100  
77 1.5 84.5 253.5#

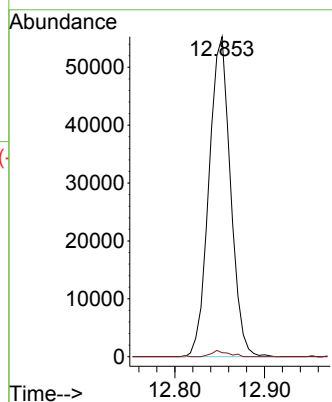

#81  
trans-1,4-Dichloro-2-butene  
Concen: 77.109 ug/l  
RT: 12.853 min Scan# 1853  
Delta R.T. 0.112 min  
Lab File: VN080367.D  
Acq: 05 Dec 2023 15:34

Tgt Ion: 75 Resp: 92163  
Ion Ratio Lower Upper  
75 100  
53 0.1 67.4 101.2#  
89 0.0 38.8 58.2#


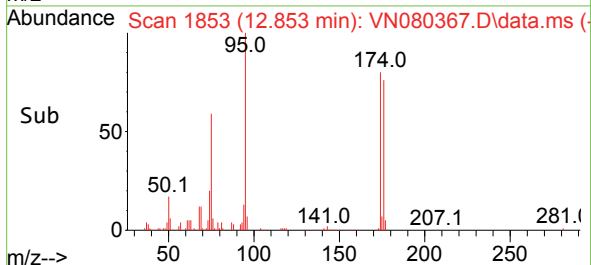

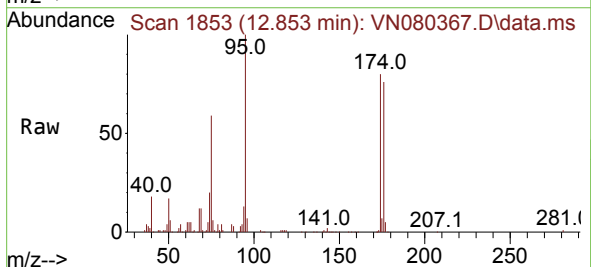


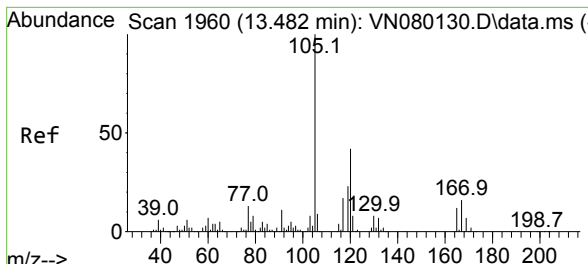

#84  
 1,2,4-Trimethylbenzene  
 Concen: 0.486 ug/l  
 RT: 13.482 min Scan# 1960  
 Delta R.T. -0.000 min  
 Lab File: VN080367.D  
 Acq: 05 Dec 2023 15:34

Instrument :  
 MSVOA\_N  
 ClientSampleId :

Tgt Ion:105 Resp: 5340  
 Ion Ratio Lower Upper  
 105 100  
 120 42.2 22.0 66.0

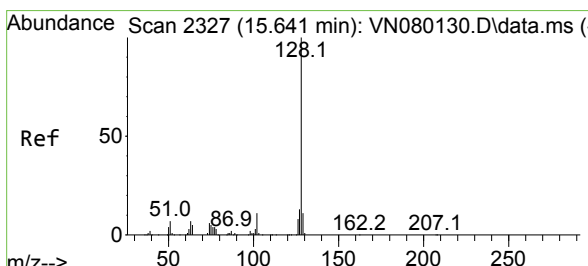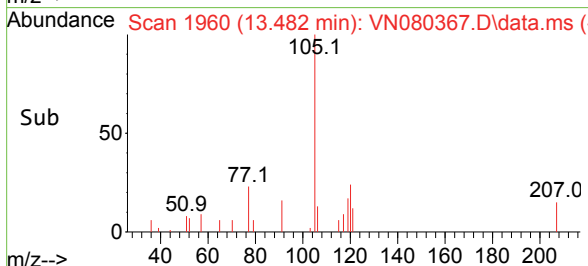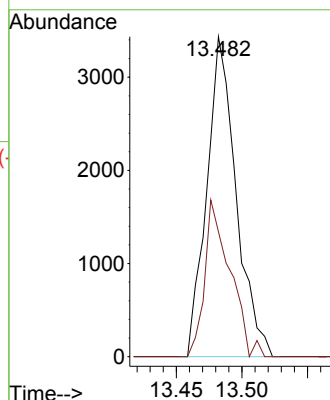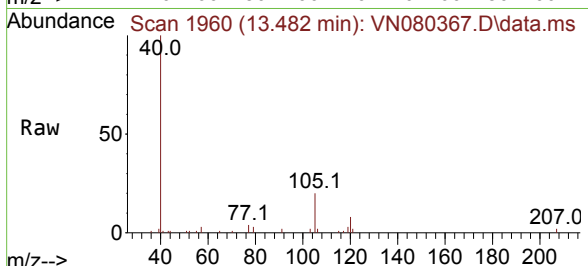

#95  
 Naphthalene  
 Concen: 1.362 ug/l  
 RT: 15.647 min Scan# 2328  
 Delta R.T. 0.006 min  
 Lab File: VN080367.D  
 Acq: 05 Dec 2023 15:34

Tgt Ion:128 Resp: 12791  
 Ion Ratio Lower Upper  
 128 100  
 127 15.0 10.0 15.0  
 129 13.3 8.7 13.1#

