

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120523\
 Data File : VN080366.D
 Acq On : 05 Dec 2023 15:11
 Operator : JC\MD
 Sample : 05620-01 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 OILY-WATER-TOTE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
 Title : SW846 8260

Signal : TIC: VN080366.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.289	53	57	68	rVB4	11851	27980	2.74%	0.424%
2	2.665	112	121	130	rBV	210217	380025	37.27%	5.762%
3	3.789	300	312	322	rBV2	76285	213083	20.90%	3.231%
4	4.424	409	420	430	rBV	48650	147735	14.49%	2.240%
5	4.712	462	469	479	rVB3	8858	25343	2.49%	0.384%
6	8.165	1046	1056	1061	rBV	165463	399807	39.21%	6.062%
7	8.224	1061	1066	1075	rVB	228930	516821	50.69%	7.836%
8	8.400	1089	1096	1105	rVB2	9192	26052	2.56%	0.395%
9	8.577	1118	1126	1136	rBV	156822	355042	34.82%	5.383%
10	9.100	1206	1215	1227	rBV	350390	721740	70.78%	10.943%
11	10.571	1457	1465	1474	rBV	546083	1019631	100.00%	15.460%
12	11.865	1678	1685	1695	rVB	541147	960733	94.22%	14.567%
13	12.853	1844	1853	1861	rBV	459100	802183	78.67%	12.163%
14	13.429	1947	1951	1955	rVB4	7338	13792	1.35%	0.209%
15	13.647	1981	1988	1992	rVB3	12828	19907	1.95%	0.302%
16	13.794	2004	2013	2019	rBV	545301	920295	90.26%	13.954%
17	13.994	2041	2047	2055	rVB7	8763	21324	2.09%	0.323%
18	14.106	2061	2066	2069	rBV4	9886	13621	1.34%	0.207%
19	15.635	2321	2326	2328	rBV4	7190	10279	1.01%	0.156%




Sum of corrected areas: 6595393

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120523\
Data File : VN080366.D
Acq On : 05 Dec 2023 15:11
Operator : JC\MD
Sample : 05620-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-TOTE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

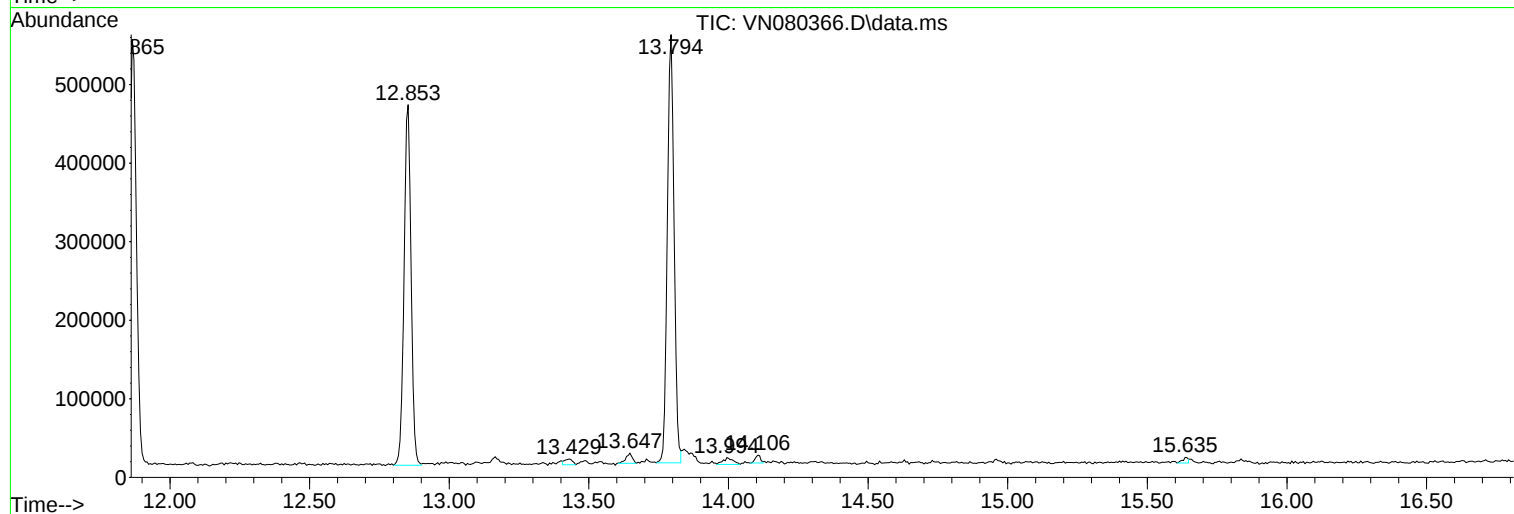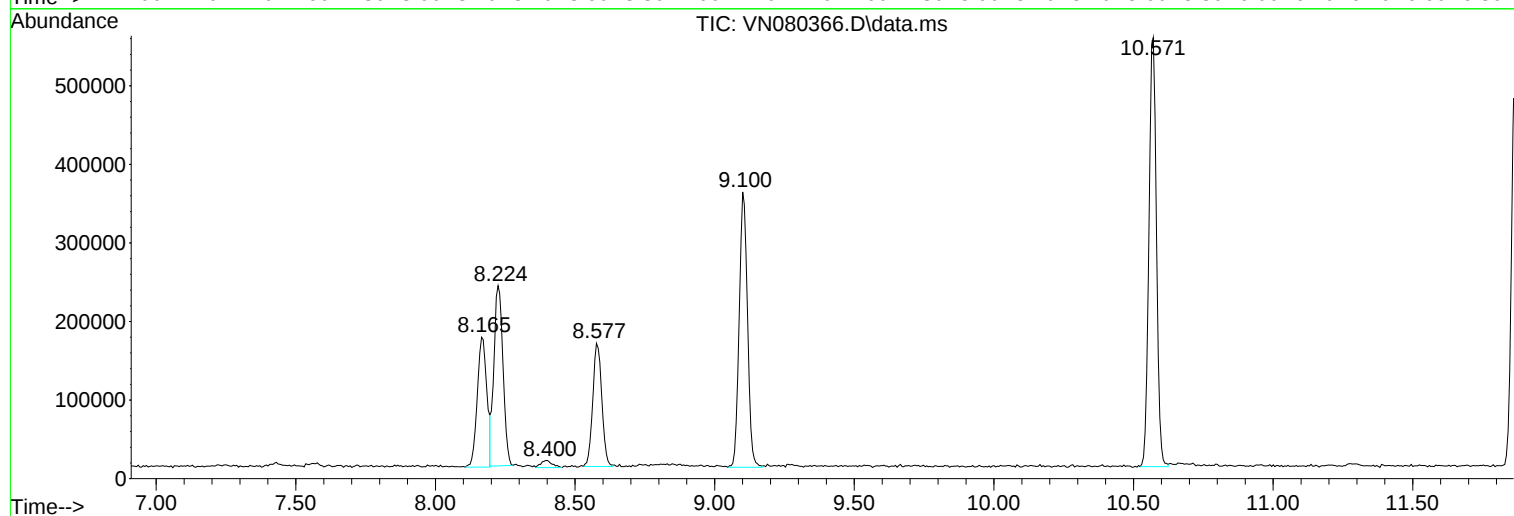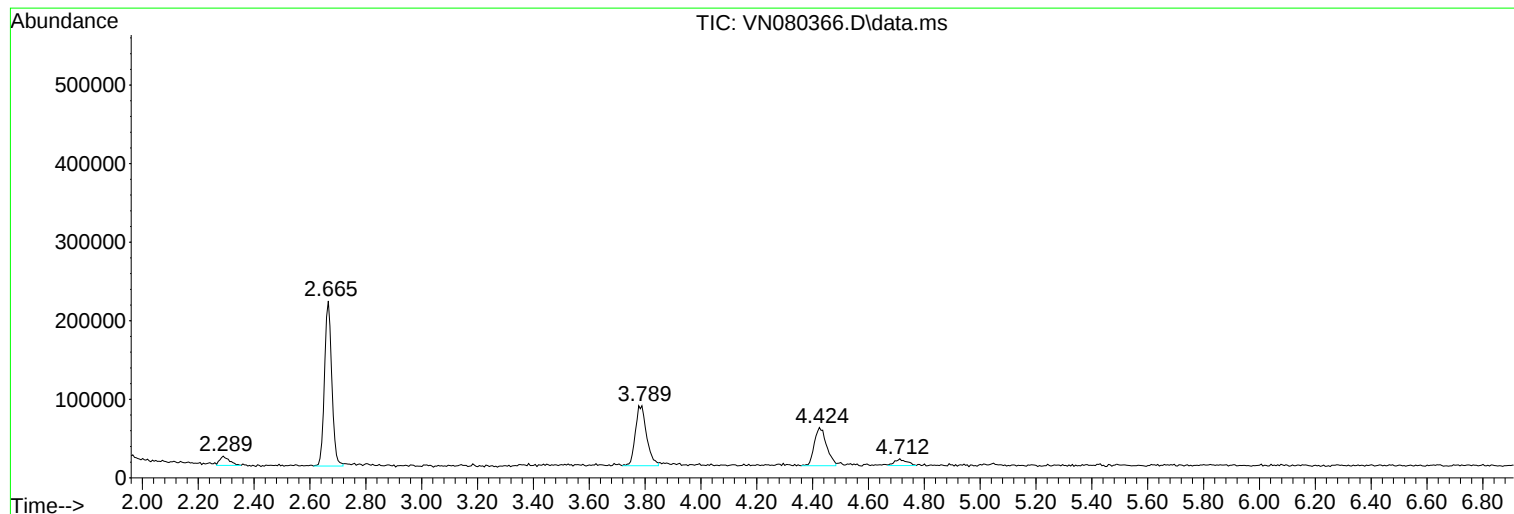

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120523\
Data File : VN080366.D
Acq On : 05 Dec 2023 15:11
Operator : JC\MD
Sample : 05620-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-TOTE










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethanol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.789	20.61 ug/l	213083	Pentafluorobenzene	8.224

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Ethanol			46	C2H6O	000064-17-5	74
2	Dimethyl ether			46	C2H6O	000115-10-6	9
3	Methane, nitroso-			45	CH3NO	000865-40-7	4
4	Formic acid			46	CH2O2	000064-18-6	4
5	Oxalic acid			90	C2H2O4	000144-62-7	4

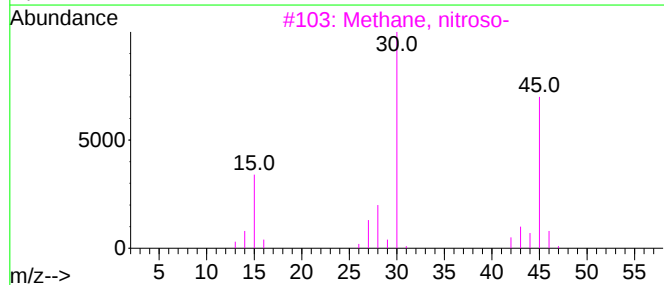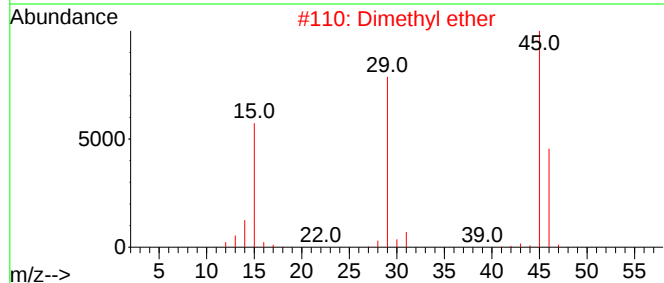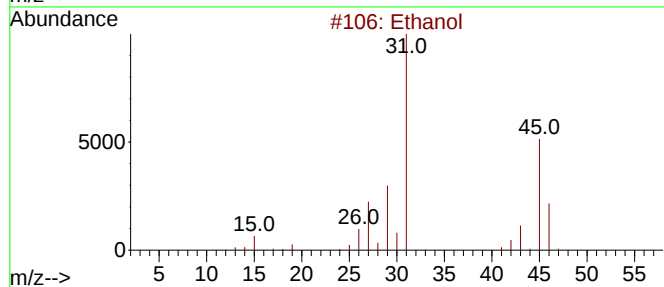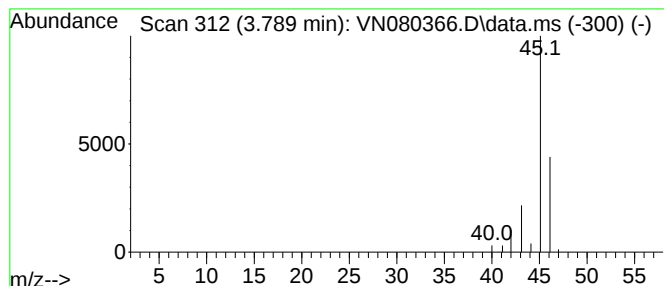

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120523\
Data File : VN080366.D
Acq On : 05 Dec 2023 15:11
Operator : JC\MD
Sample : 05620-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-TOTE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol	3.789	20.6	ug/l	213083	1	8.224	516821	50.0