


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120523\
Data File : VN080353.D
Acq On : 05 Dec 2023 09:32
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

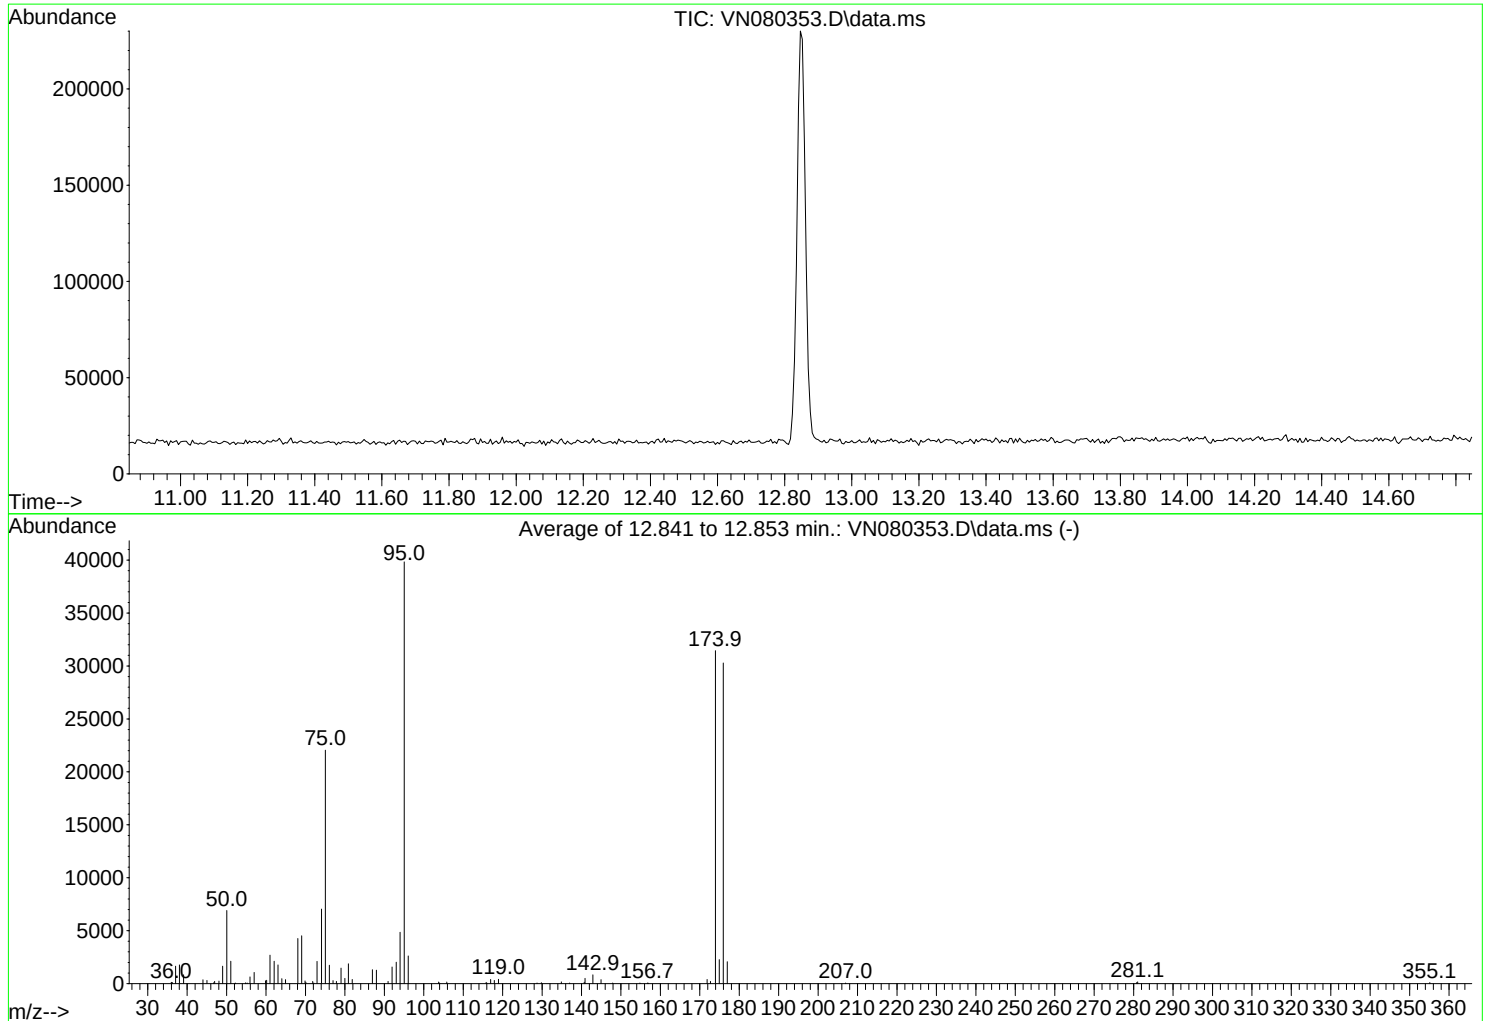

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	6902	PASS
75	95	30	60	55.4	22051	PASS
95	95	100	100	100.0	39835	PASS
96	95	5	9	6.6	2620	PASS
173	174	0.00	2	0.7	210	PASS
174	95	50	100	79.0	31451	PASS
175	174	5	9	7.2	2272	PASS
176	174	95	101	96.3	30277	PASS
177	176	5	9	6.8	2069	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	119	49.00	1650	62.05	2121	74.05	704
36.10	118	50.05	6902	63.05	1772	75.05	2205
36.30	84	51.05	2121	64.00	477	76.05	173
37.05	1651	52.20	55	64.95	375	77.00	29
38.05	1764	54.80	83	68.05	4257	77.85	219
39.10	835	55.20	62	69.05	4521	79.00	1467
44.00	359	55.95	635	69.90	260	80.00	493
45.00	296	57.00	1057	70.10	141	80.90	1874
46.70	76	59.85	269	71.85	217	81.85	397
46.95	215	60.15	319	72.10	69	86.95	1322
48.05	236	61.00	2695	72.95	2108	88.00	1265

Average of 12.841 to 12.853 min.: VN080353.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.95	216	116.95	387	147.90	58	280.80	104
91.95	1569	117.90	297	154.80	57	281.05	174
93.00	2023	118.95	411	156.70	60	355.10	102
94.00	4848	128.70	60	156.90	51		
95.05	39835	129.80	92	171.85	389		
96.05	2620	134.90	175	172.70	210		
103.75	152	137.00	54	173.95	31451		
104.00	68	140.70	142	174.95	2272		
105.85	155	140.90	505	175.95	30277		
115.80	127	142.90	834	176.95	2069		
116.00	63	144.95	373	207.00	63		

Instrument :

MSVOA_N

ClientSampleId :

BFB