
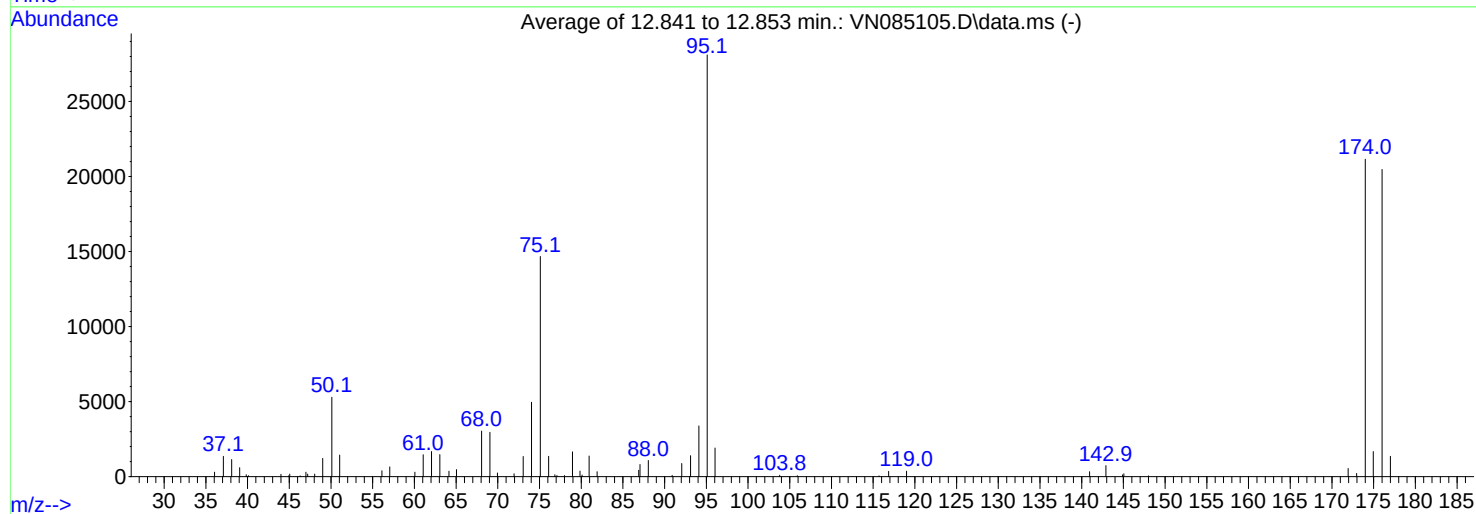


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120524\
Data File : VN085105.D
Acq On : 05 Dec 2024 08:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

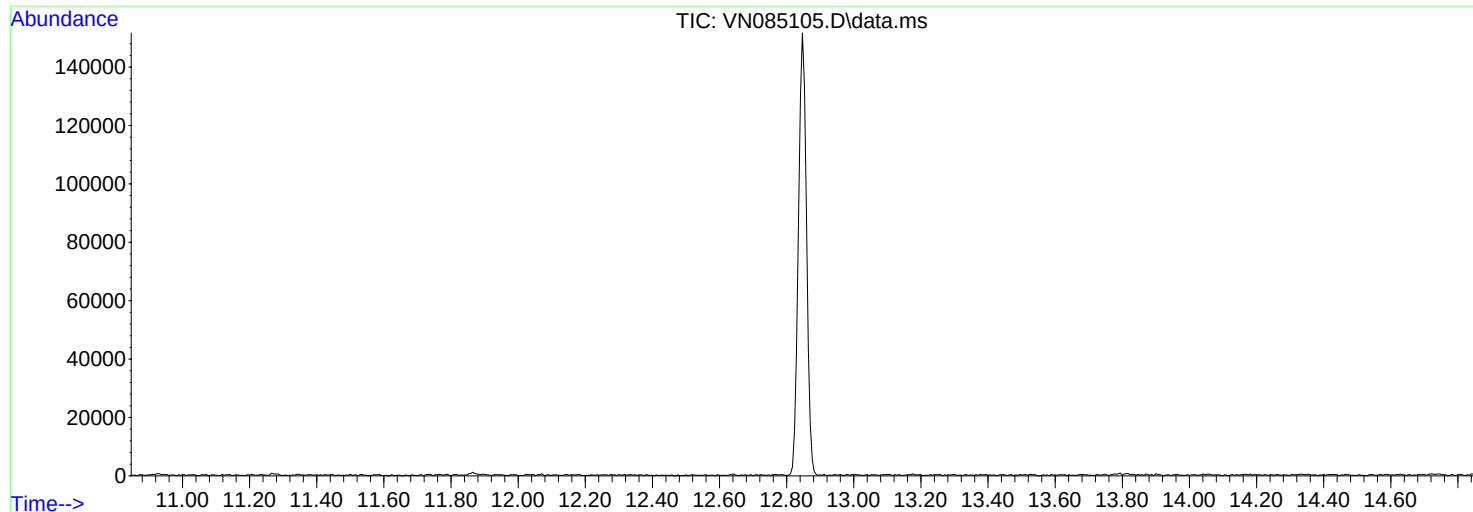

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	5290	PASS
75	95	30	60	52.2	14673	PASS
95	95	100	100	100.0	28109	PASS
96	95	5	9	6.8	1904	PASS
173	174	0.00	2	1.0	218	PASS
174	95	50	100	75.2	21152	PASS
175	174	5	9	7.9	1679	PASS
176	174	95	101	96.8	20475	PASS
177	176	5	9	6.6	1354	PASS

Average of 12.841 to 12.853 min.: VN085105.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	296	47.20	170	64.15	362	77.10	71
37.10	1356	48.05	172	65.05	474	78.00	71
38.10	1140	49.00	1211	68.05	3039	78.95	165
39.05	596	50.10	5290	69.05	2955	79.85	37
39.85	126	51.05	1436	69.95	246	80.10	107
40.10	67	56.10	390	71.95	194	80.95	1373
44.00	165	57.05	654	73.05	1348	81.90	327
44.90	50	60.05	304	74.05	4954	86.90	431
45.05	172	61.05	1461	75.10	14673	87.05	808
46.30	52	62.05	1672	76.10	1358	88.05	1079
47.00	298	63.05	1469	76.85	131	90.90	84

Average of 12.841 to 12.853 min.: VN085105.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.05	877	142.90	733				
93.10	1392	144.90	118				
94.10	3383	145.05	197				
95.10	28109	148.00	56				
96.05	1904	171.95	548				
103.80	92	172.95	218				
105.90	63	174.00	21152				
115.70	56	174.95	1679				
116.85	347	176.00	20475				
119.00	363	177.00	1354				
140.95	335						

Instrument :

MSVOA_N

ClientSampleId :

BFB