


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN120618\
Data File : VN052687.D
Acq On : 6 Dec 2018 8:48
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Title : SW846 8260
Last Update : Mon Dec 03 03:24:02 2018

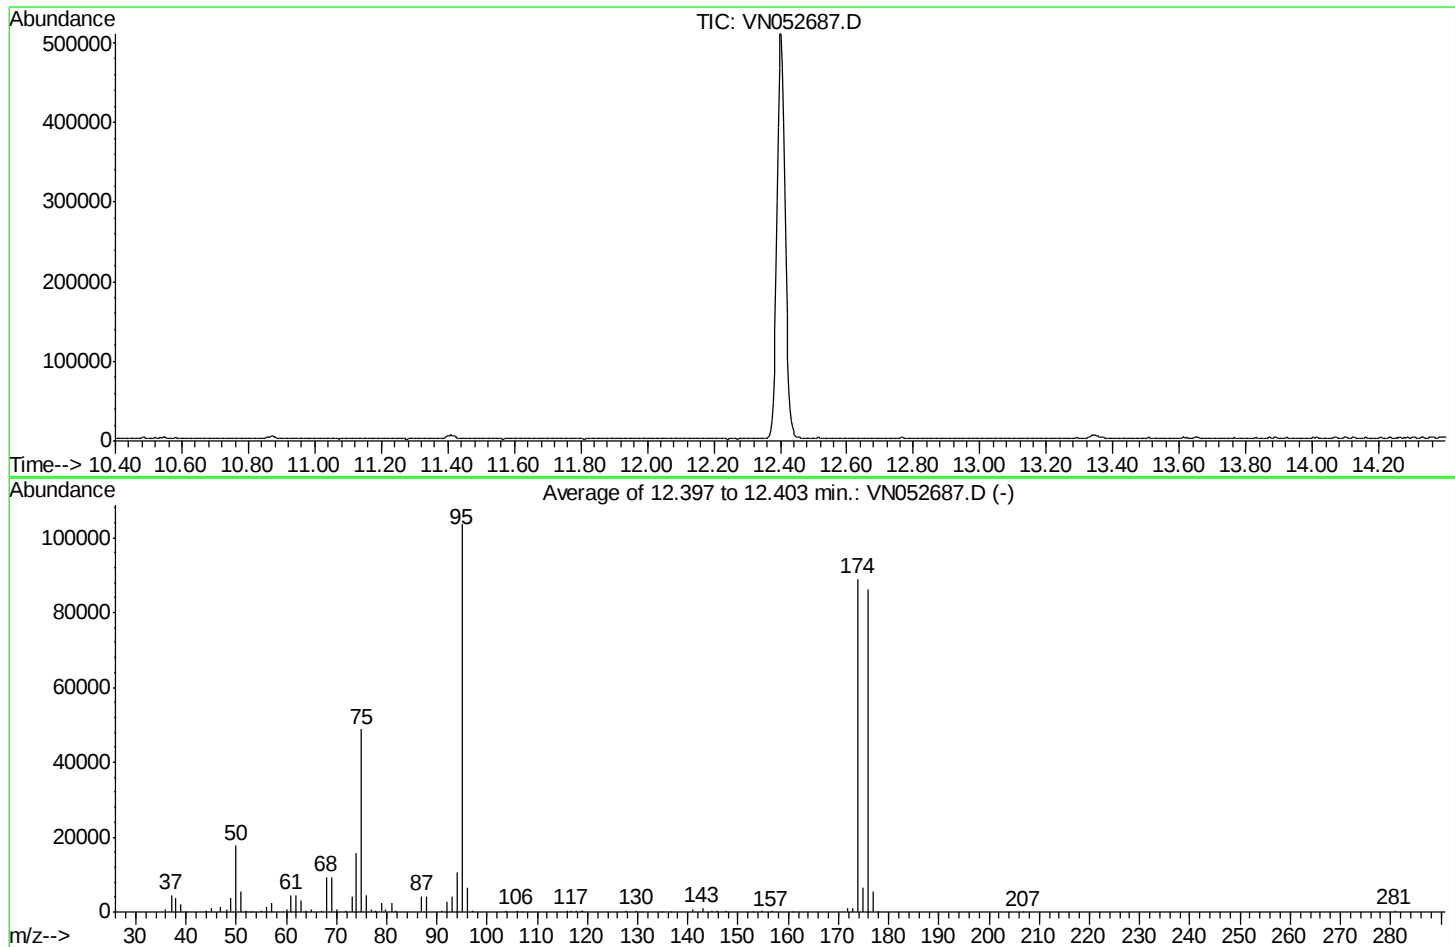

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	17664	PASS
75	95	30	60	47.2	48885	PASS
95	95	100	100	100.0	103552	PASS
96	95	5	9	6.4	6678	PASS
173	174	0.00	2	1.0	920	PASS
174	95	50	100	85.9	88968	PASS
175	174	5	9	7.4	6610	PASS
176	174	95	101	96.7	86053	PASS
177	176	5	9	6.4	5544	PASS