


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120618\
Data File : VN052708.D
Acq On : 6 Dec 2018 19:59
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 23 Sample Multiplier: 22

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N112618W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Nov 27 00:48:33 2018

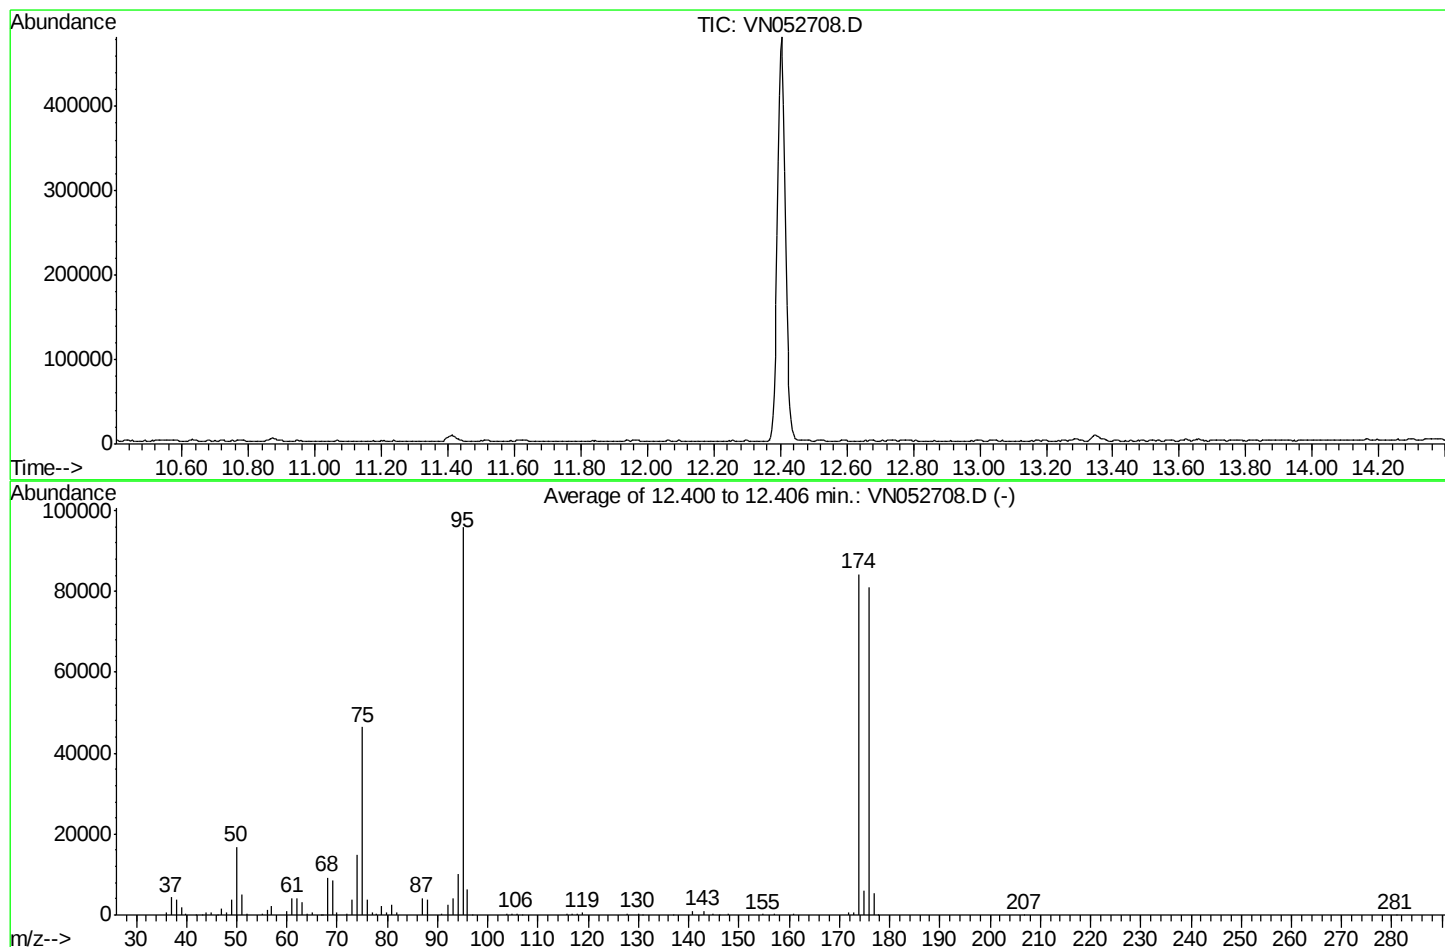

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	16891	PASS
75	95	30	60	48.4	46402	PASS
95	95	100	100	100.0	95845	PASS
96	95	5	9	6.5	6246	PASS
173	174	0.00	2	0.9	798	PASS
174	95	50	100	87.9	84285	PASS
175	174	5	9	7.1	6023	PASS
176	174	95	101	96.0	80901	PASS
177	176	5	9	6.6	5308	PASS