


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120619\
Data File : VN059503.D
Acq On : 6 Dec 2019 9:34
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N120319W.M
Title : SW846 8260
Last Update : Tue Dec 03 16:37:42 2019

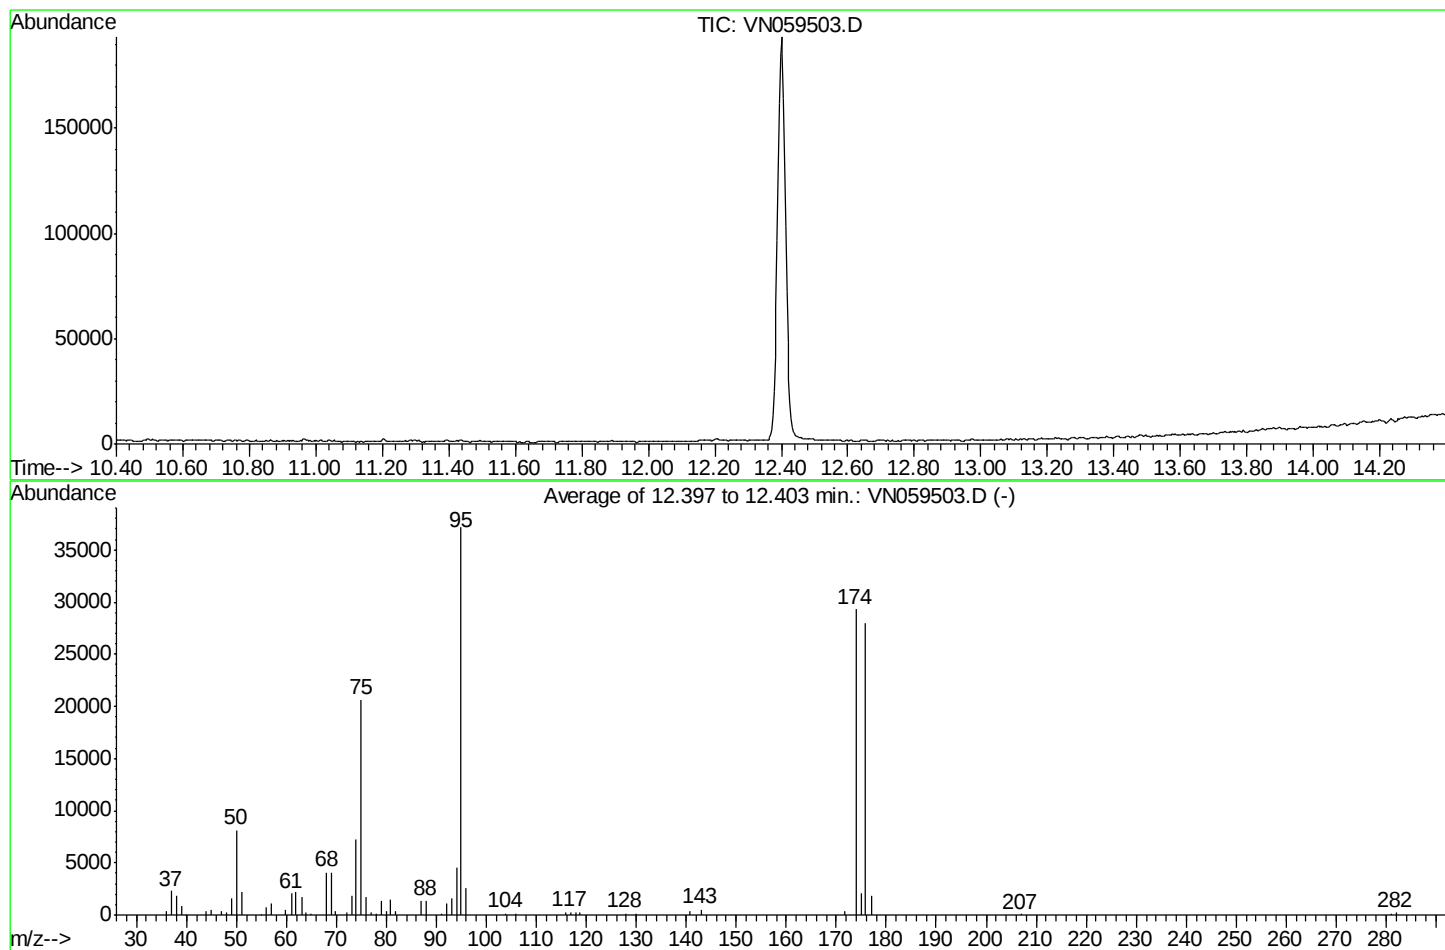

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	8104	PASS
75	95	30	60	55.6	20653	PASS
95	95	100	100	100.0	37160	PASS
96	95	5	9	6.9	2558	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.8	29298	PASS
175	174	5	9	7.3	2136	PASS
176	174	95	101	95.6	28013	PASS
177	176	5	9	6.7	1886	PASS