

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120621\
 Data File : VN069798.D
 Acq On : 6 Dec 2021 21:28
 Operator : JC/MD
 Sample : M4920-02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FDR-20211202-WC-S

Quant Time: Dec 07 03:51:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	1298740	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2341620	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	2502302	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	993876	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	992899	49.515	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	99.020%		
35) Dibromofluoromethane	8.024	113	681975	46.496	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	93.000%		
50) Toluene-d8	10.443	98	3025948	51.379	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	102.760%		
62) 4-Bromofluorobenzene	12.733	95	1184777	55.529	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	111.060%		
Target Compounds						Qvalue
11) Tert butyl alcohol	5.390	59	9768	2.577	ug/l	99
13) Acrolein	4.046	56	1676	0.519	ug/l #	73
16) Acetone	4.296	43	210358	17.439	ug/l	95
18) Methyl Acetate	4.875	43	35509	0.975	ug/l #	83
20) Methylene Chloride	5.095	84	73370	4.575	ug/l #	85
25) 2-Butanone	7.345	43	147204	8.982	ug/l	90
29) Tetrahydrofuran	7.697	42	9207	0.925	ug/l #	57
31) Cyclohexane	8.088	56	34234	1.227	ug/l #	24
36) 1,1-Dichloropropene	8.086	75	110339	4.950	ug/l #	49
37) Ethyl Acetate	7.345	43	147204	4.437	ug/l #	69
38) Carbon Tetrachloride	8.088	117	134220	6.140	ug/l #	16
43) Isopropyl Acetate	8.566	43	162267	3.305	ug/l #	83
48) Methyl methacrylate	9.545	41	45104	1.968	ug/l #	8
49) 1,4-Dioxane	9.630	88	1397	3.398	ug/l #	1
51) 4-Methyl-2-Pentanone	10.333	43	25003	0.785	ug/l	94
53) t-1,3-Dichloropropene	10.717	75	151	2.799	ug/l #	11
54) cis-1,3-Dichloropropene	10.245	75	173278	7.798	ug/l #	71
56) Ethyl methacrylate	10.706	69	2439	2.353	ug/l #	24
57) 1,3-Dichloropropane	11.092	76	99679	3.373	ug/l #	43
59) 2-Hexanone	11.092	43	1839691	76.353	ug/l #	49
60) Dibromochloromethane	11.494	129	863	2.422	ug/l #	11
71) Bromoform	12.725	173	1070	2.797	ug/l #	1
74) N-amyl acetate	12.355	43	16636	0.425	ug/l #	48
76) 1,2,3-Trichloropropane	12.733	75	658931	23.119	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.733	75	658931	73.580	ug/l #	5
82) 4-Chlorotoluene	13.323	91	51560	0.882	ug/l #	38
83) tert-Butylbenzene	13.326	119	72629	1.152	ug/l	92
90) Hexachloroethane	14.329	117	2807	0.239	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.265	180	462	2.905	ug/l #	77
95) Naphthalene	15.501	128	1374	4.011	ug/l #	64
96) 1,2,3-Trichlorobenzene	15.705	180	178	2.446	ug/l #	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120621\
Data File : VN069798.D
Acq On : 6 Dec 2021 21:28
Operator : JC/MD
Sample : M4920-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S

Quant Time: Dec 07 03:51:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 03 08:46:47 2021
Response via : Initial Calibration




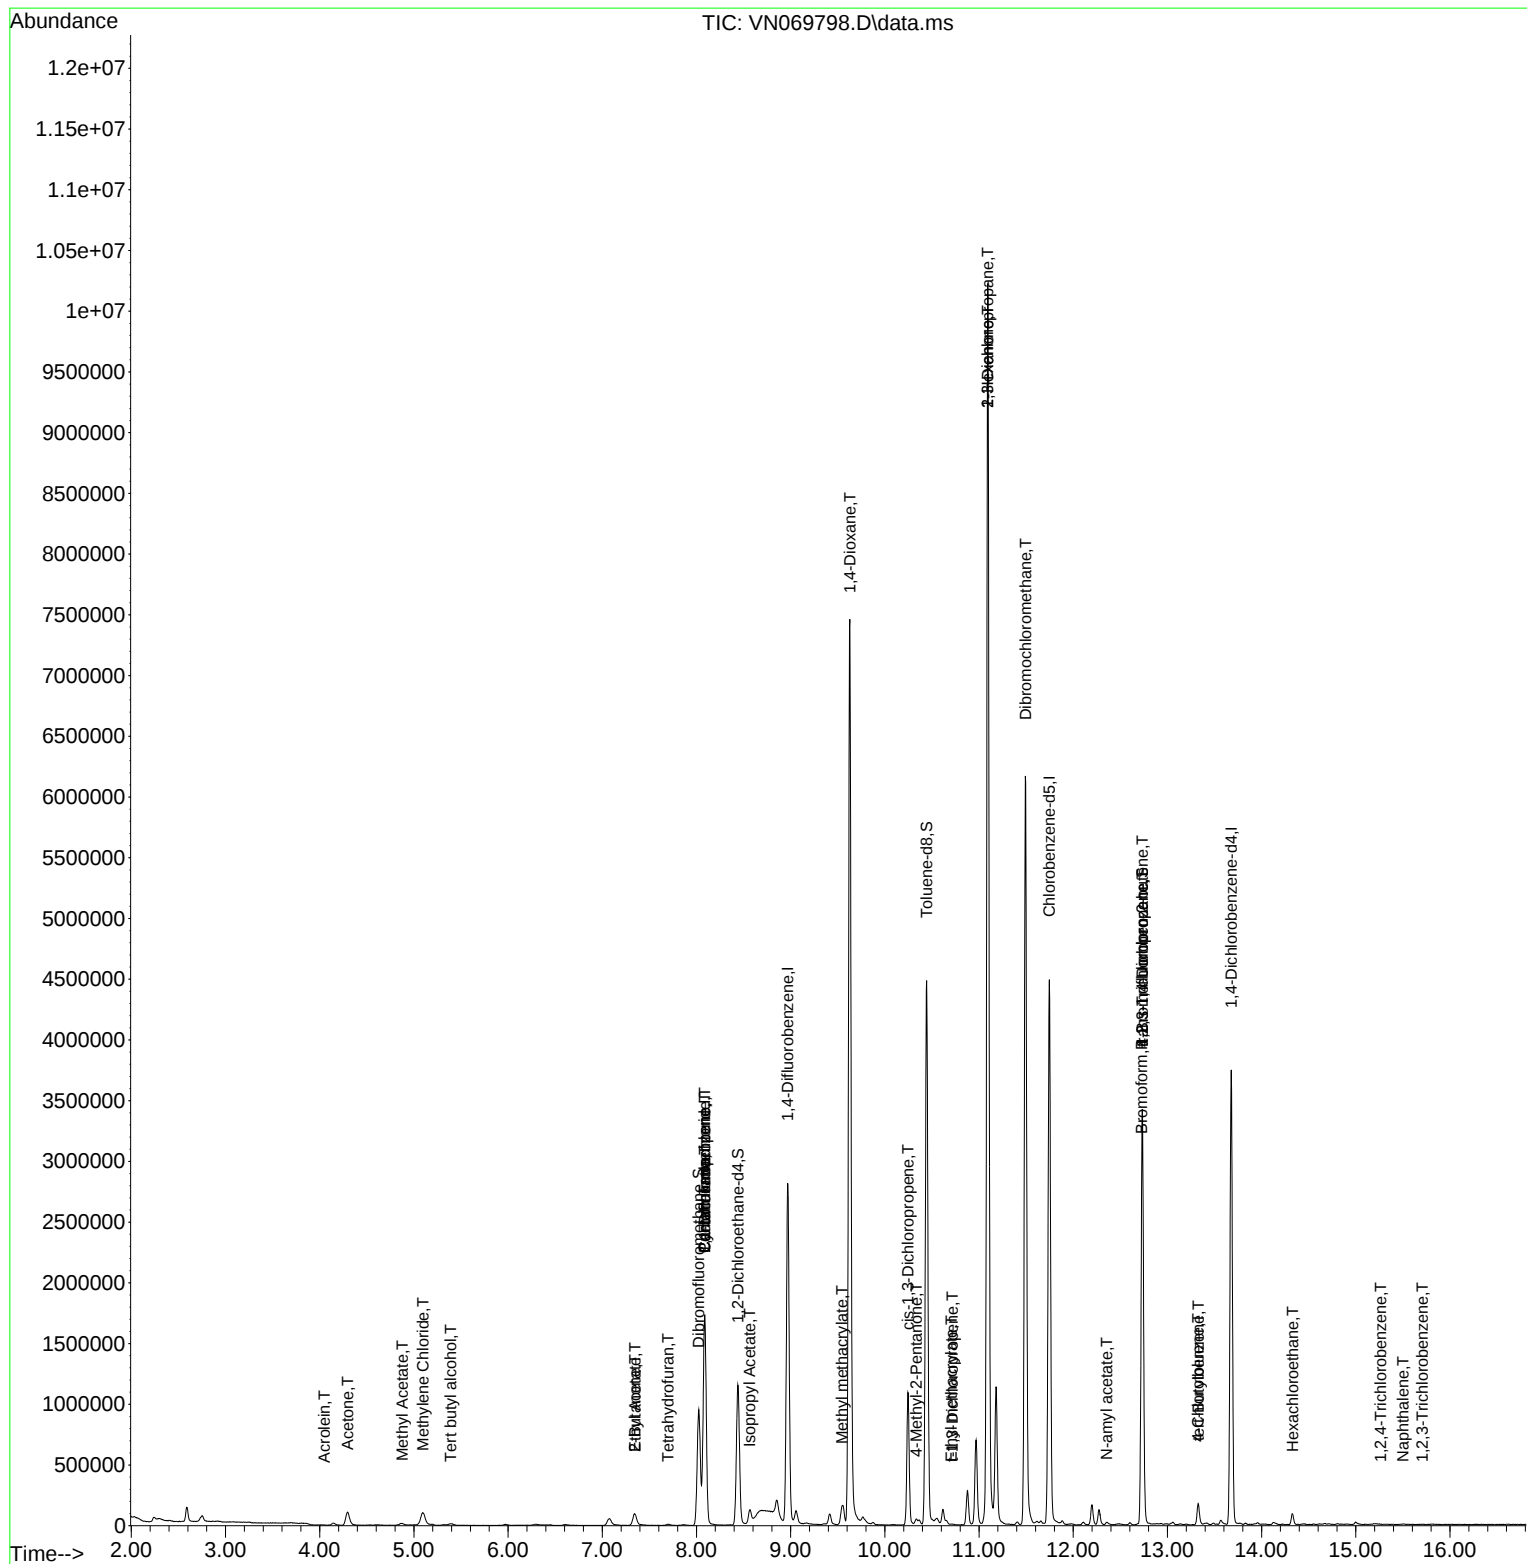




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion:168 Resp: 1298740
Ion Ratio Lower Upper
168 100
99 60.4 41.3 61.9

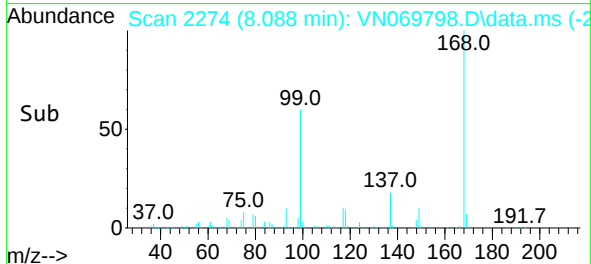

#11
Tert butyl alcohol
Concen: 2.577 ug/l
RT: 5.390 min Scan# 1268
Delta R.T. 0.000 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 59 Resp: 9768
Ion Ratio Lower Upper
59 100
57 10.7 8.7 13.1




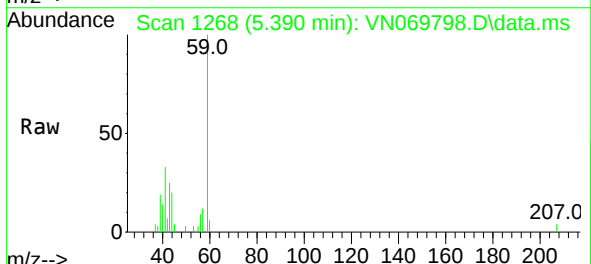




#13
Acrolein
Concen: 0.519 ug/l
RT: 4.046 min Scan# 765
Delta R.T. 0.008 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 56 Resp: 1676
Ion Ratio Lower Upper
56 100
55 48.3 56.6 85.0#

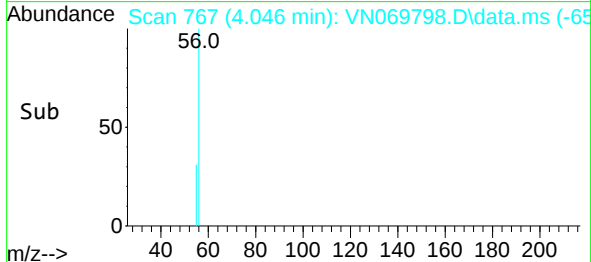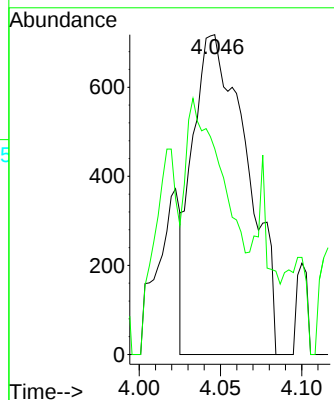

#16
Acetone
Concen: 17.439 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.005 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 43 Resp: 210358
Ion Ratio Lower Upper
43 100
58 26.1 23.1 34.7


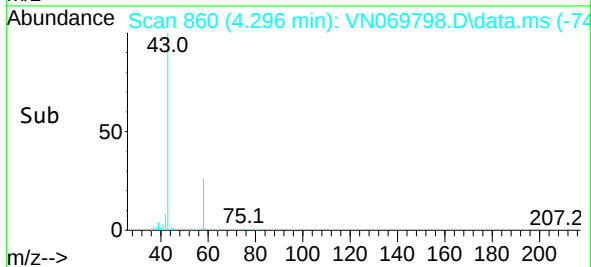
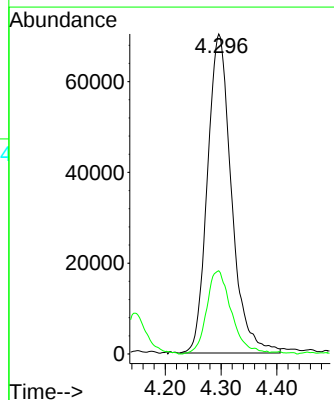
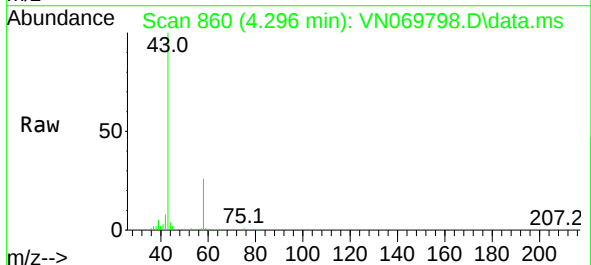


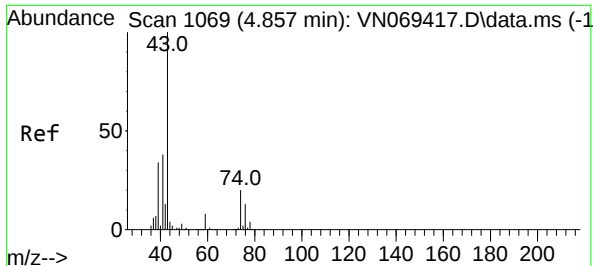

#18
Methyl Acetate
Concen: 0.975 ug/l
RT: 4.875 min Scan# 1069
Delta R.T. 0.019 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 43 Resp: 35509
Ion Ratio Lower Upper
43 100
74 15.6 19.4 29.2#

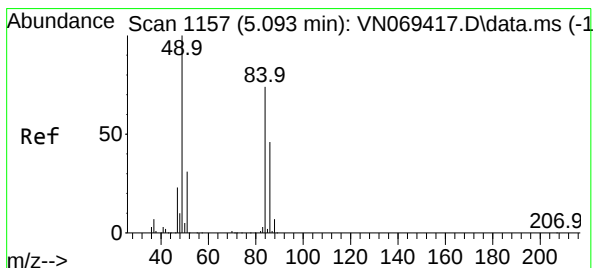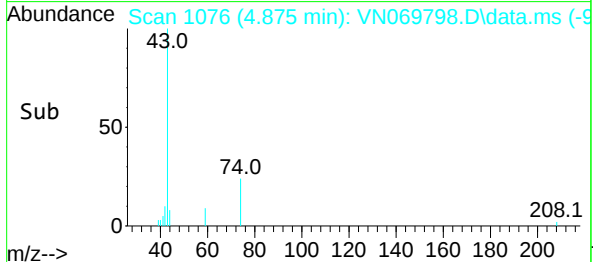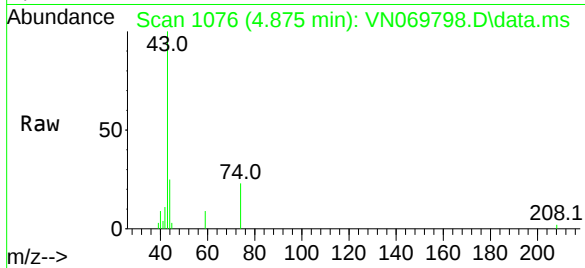

#20
Methylene Chloride
Concen: 4.575 ug/l
RT: 5.095 min Scan# 1158
Delta R.T. 0.003 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 84 Resp: 73370
Ion Ratio Lower Upper
84 100
49 140.8 93.5 140.3#
51 45.8 29.4 44.2#
86 65.1 53.0 79.4

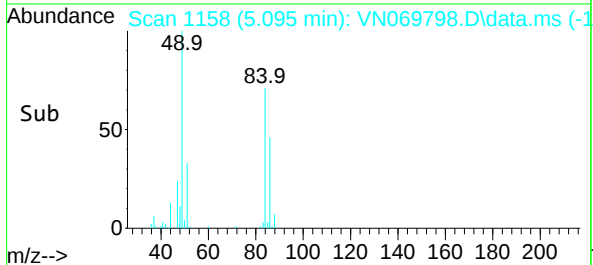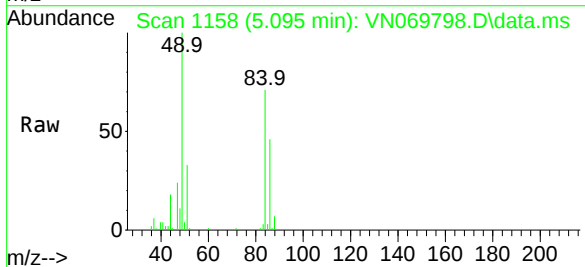

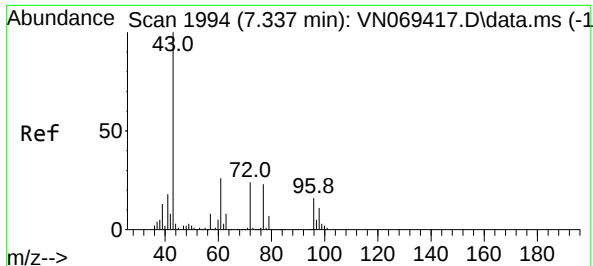

#25

2-Butanone

Concen: 8.982 ug/l

RT: 7.345 min Scan# 1994

Delta R.T. 0.008 min

Lab File: VN069798.D

Acq: 6 Dec 2021 21:28

Instrument :

MSVOA_N

ClientSampleId :





FDR-20211202-WC-S

Tgt Ion: 43 Resp: 147204

Ion Ratio Lower Upper

43 100

72 22.0 21.7 32.5

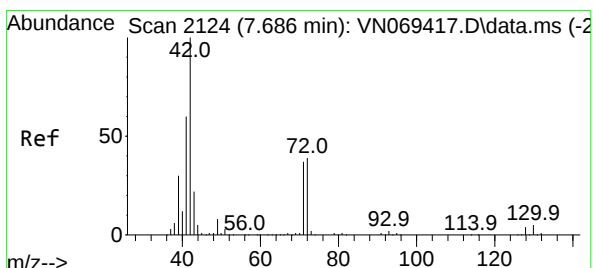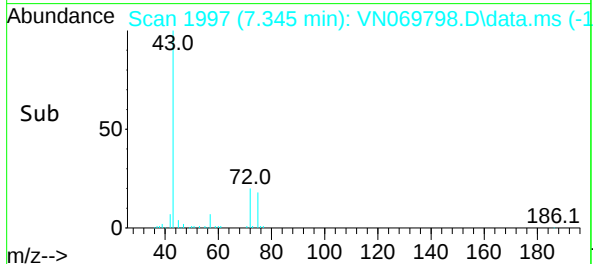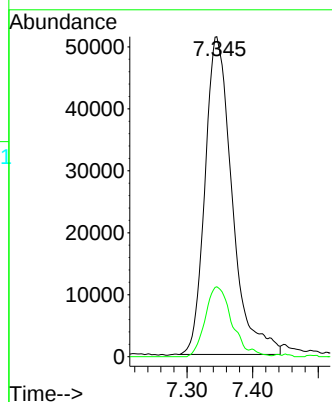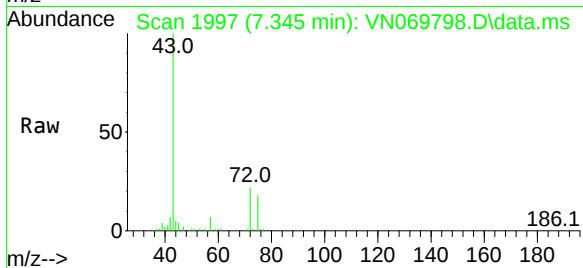

#29

Tetrahydrofuran

Concen: 0.925 ug/l

RT: 7.697 min Scan# 2128

Delta R.T. 0.011 min

Lab File: VN069798.D

Acq: 6 Dec 2021 21:28




Tgt Ion: 42 Resp: 9207


Ion Ratio Lower Upper

42 100

72 10.0 36.3 54.5#

71 23.2 34.7 52.1#


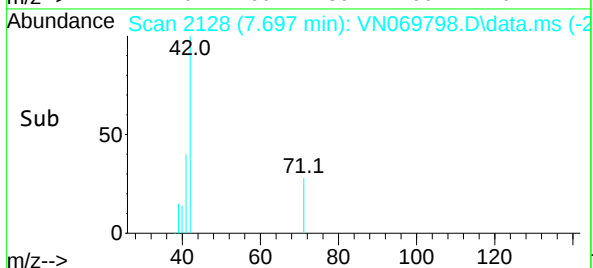

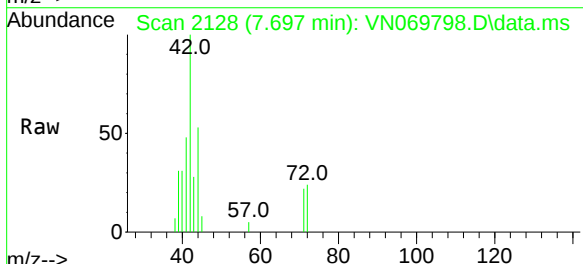




#31
Cyclohexane
Concen: 1.227 ug/l
RT: 8.088 min Scan# 21
Delta R.T. -0.005 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 56 Resp: 34234
Ion Ratio Lower Upper
56 100
69 155.6 27.1 40.7#
84 115.7 73.4 110.0#

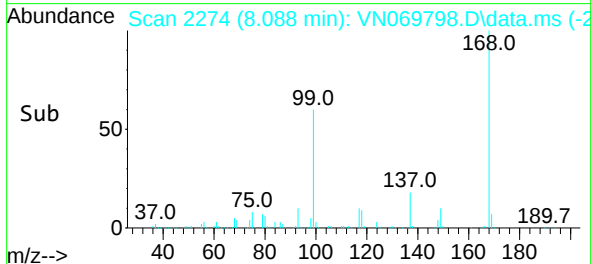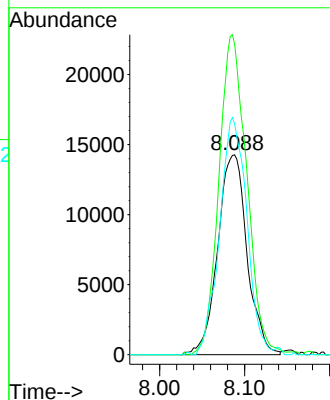

#33
1,2-Dichloroethane-d4
Concen: 49.515 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.003 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28


Tgt Ion: 65 Resp: 992899
Ion Ratio Lower Upper
65 100
67 51.1 0.0 103.0

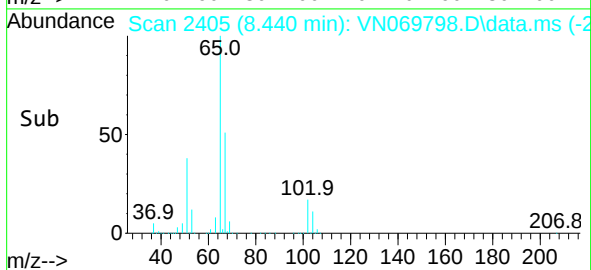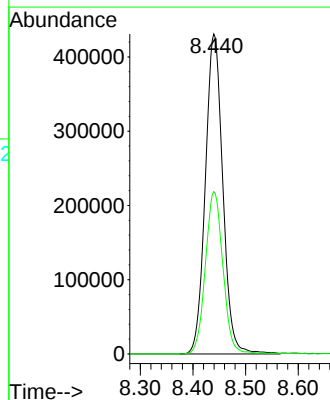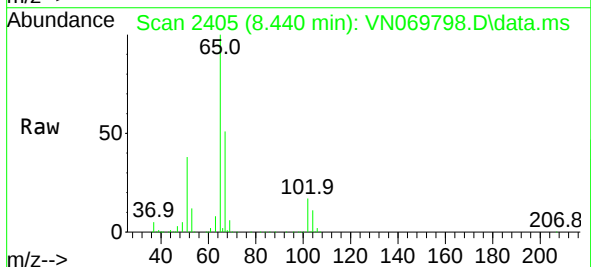






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S







Tgt Ion:114 Resp: 2341620
Ion Ratio Lower Upper
114 100
63 22.9 0.0 37.8
88 16.2 0.0 27.4

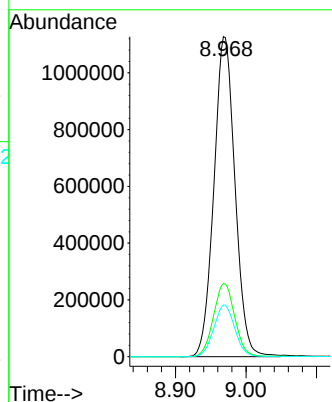

#35
Dibromofluoromethane
Concen: 46.496 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion:113 Resp: 681975
Ion Ratio Lower Upper
113 100
111 104.2 82.2 123.2
192 19.0 16.9 25.3



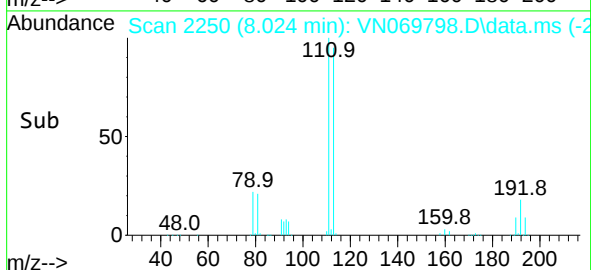





#36
1,1-Dichloropropene
Concen: 4.950 ug/l
RT: 8.086 min Scan# 211
Delta R.T. -0.137 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 75 Resp: 110339
Ion Ratio Lower Upper
75 100
110 8.4 18.4 55.2#
77 0.0 24.4 36.6#

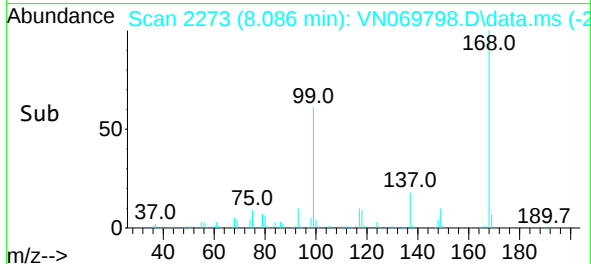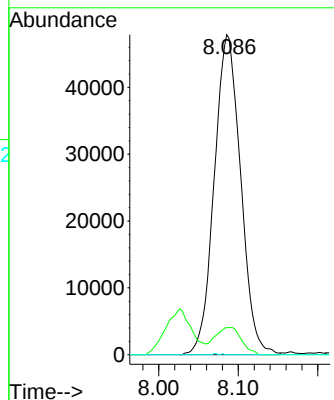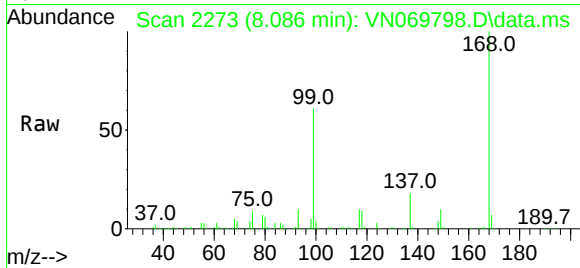

#37
Ethyl Acetate
Concen: 4.437 ug/l
RT: 7.345 min Scan# 1997
Delta R.T. -0.070 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 43 Resp: 147204
Ion Ratio Lower Upper
43 100
61 0.5 11.5 17.3#
70 0.0 7.9 11.9#


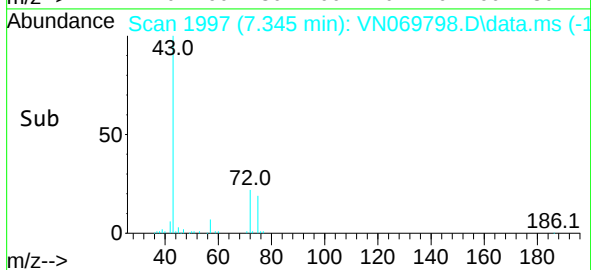
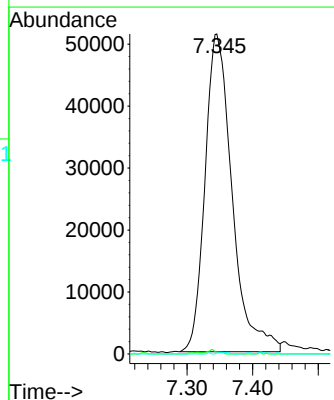
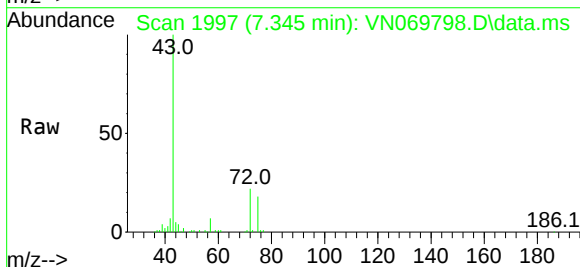




#38
Carbon Tetrachloride
Concen: 6.140 ug/l
RT: 8.088 min Scan# 211
Delta R.T. -0.118 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion:117 Resp: 134220
Ion Ratio Lower Upper
117 100
119 5.0 76.1 114.1#
121 0.0 24.2 36.2#

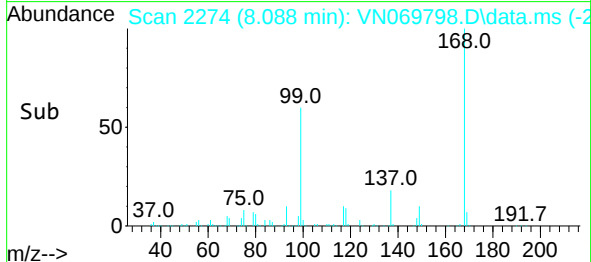

#43
Isopropyl Acetate
Concen: 3.305 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.003 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 43 Resp: 162267
Ion Ratio Lower Upper
43 100
61 15.5 20.4 30.6#
87 9.5 11.2 16.8#


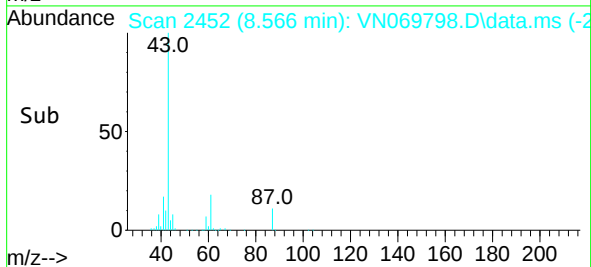

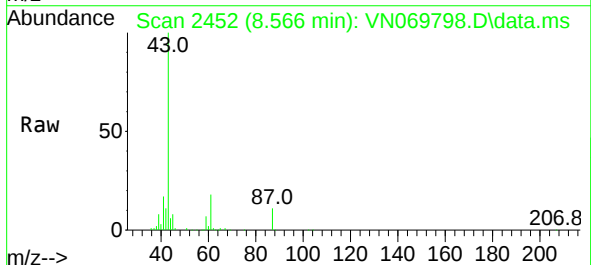




#48
Methyl methacrylate
Concen: 1.968 ug/l
RT: 9.545 min Scan# 2817
Delta R.T. -0.016 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 41 Resp: 45104
Ion Ratio Lower Upper
41 100
69 0.2 72.4 108.6#
39 0.0 58.4 87.6#

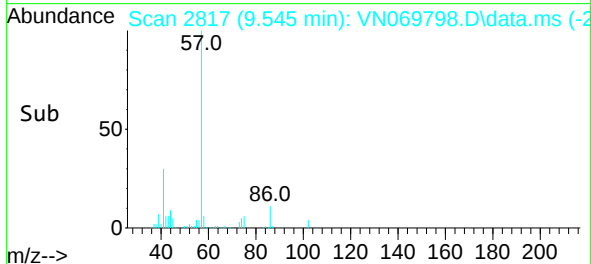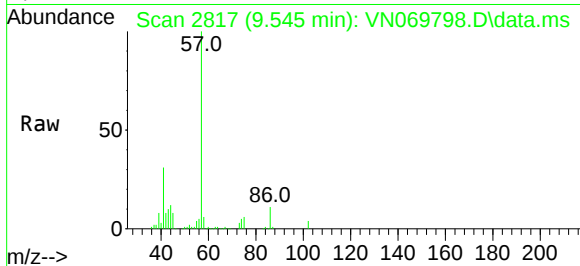

#49
1,4-Dioxane
Concen: 3.398 ug/l
RT: 9.630 min Scan# 2849
Delta R.T. 0.059 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 88 Resp: 1397
Ion Ratio Lower Upper
88 100
43 551313.7 23.4 35.2#
58 2195.8 50.6 75.8#


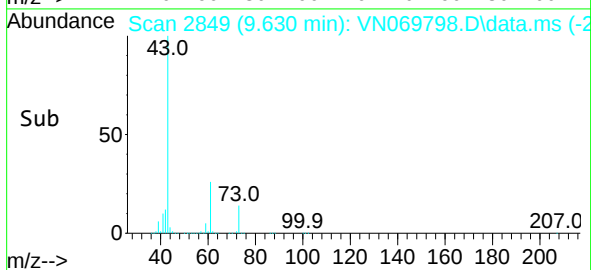

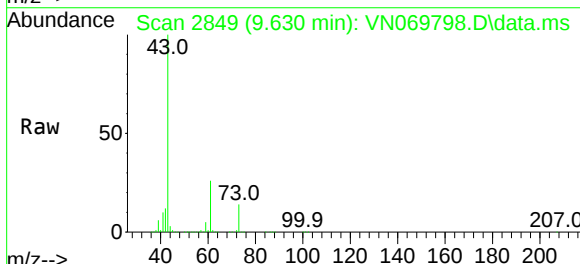




#50
Toluene-d8
Concen: 51.379 ug/l
RT: 10.443 min Scan# 3151
Delta R.T. 0.000 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 98 Resp: 3025948
Ion Ratio Lower Upper
98 100
100 64.0 50.4 75.6

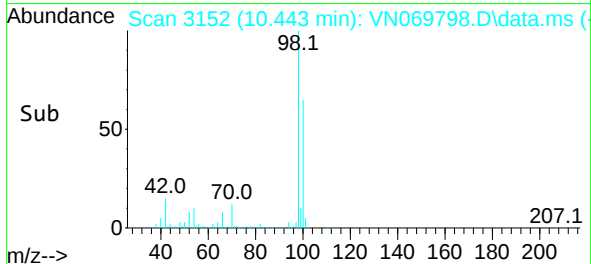

#51
4-Methyl-2-Pentanone
Concen: 0.785 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 43 Resp: 25003
Ion Ratio Lower Upper
43 100
58 41.4 30.4 45.6




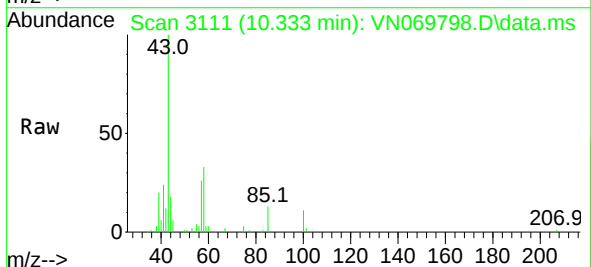




#53
t-1,3-Dichloropropene
Concen: 2.799 ug/l
RT: 10.717 min Scan# 31
Delta R.T. -0.002 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 75 Resp: 151
Ion Ratio Lower Upper
75 100
77 81.9 25.6 38.4#

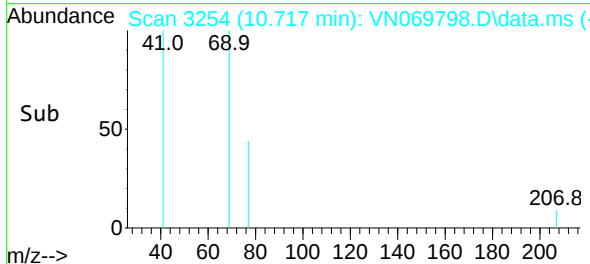

#54
cis-1,3-Dichloropropene
Concen: 7.798 ug/l
RT: 10.245 min Scan# 3078
Delta R.T. 0.054 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 75 Resp: 173278
Ion Ratio Lower Upper
75 100
77 0.4 26.4 39.6#
39 44.6 42.5 63.7


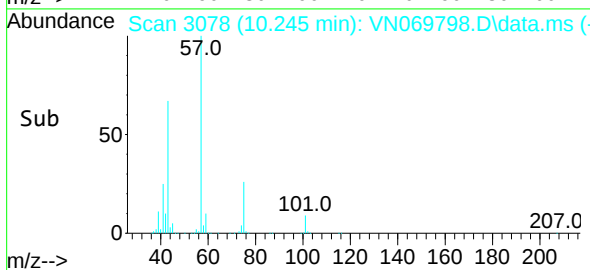

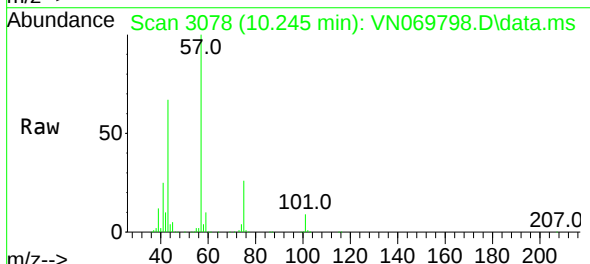




#56
Ethyl methacrylate
Concen: 2.353 ug/l
RT: 10.706 min Scan# 31
Delta R.T. -0.056 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 69 Resp: 2439
Ion Ratio Lower Upper
69 100
41 0.0 51.4 77.0#
39 0.0 34.6 52.0#

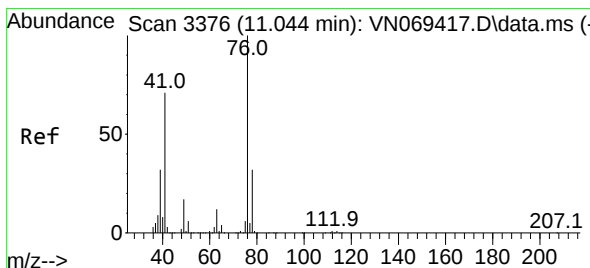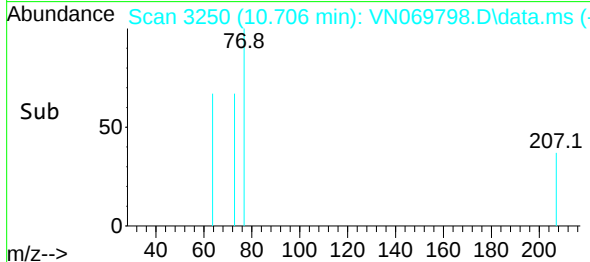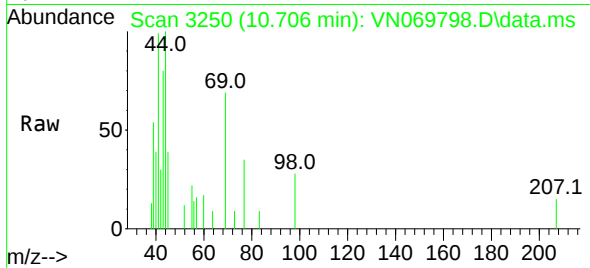

#57
1,3-Dichloropropane
Concen: 3.373 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.046 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 76 Resp: 99679
Ion Ratio Lower Upper
76 100
78 0.3 25.7 38.5#


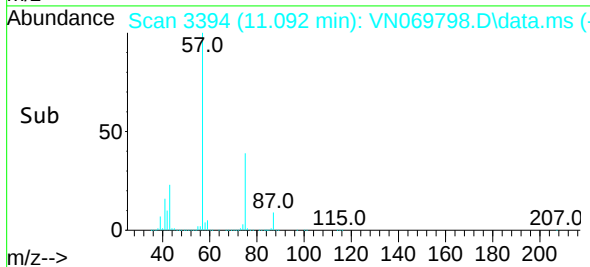

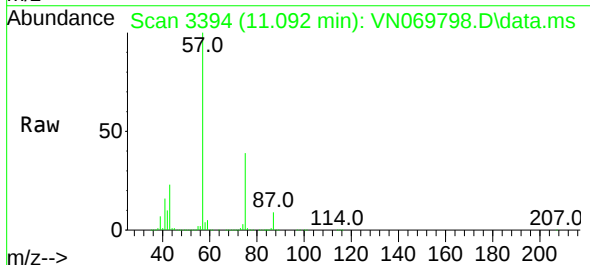




#59
2-Hexanone
Concen: 76.353 ug/l
RT: 11.092 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 43 Resp: 1839691
Ion Ratio Lower Upper
43 100
58 17.2 26.9 80.7#

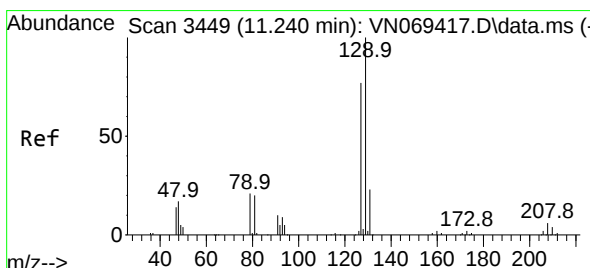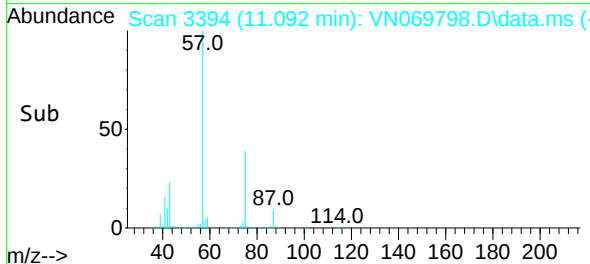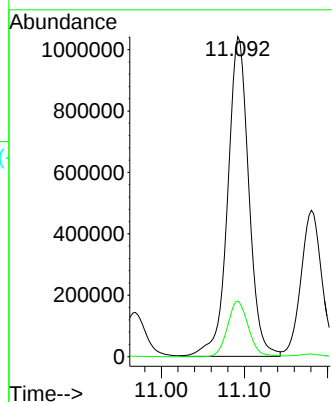

#60
Dibromochloromethane
Concen: 2.422 ug/l
RT: 11.494 min Scan# 3544
Delta R.T. 0.254 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion:129 Resp: 863
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#


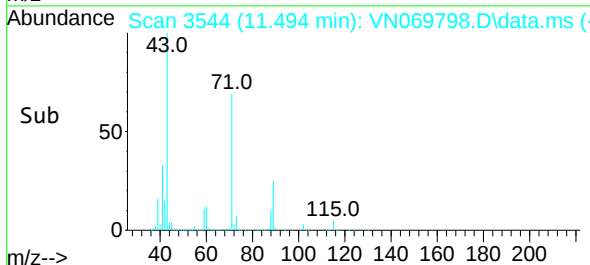

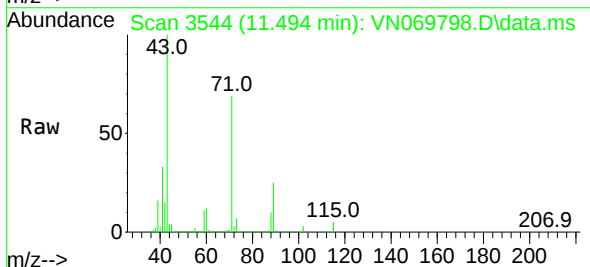




#62
4-Bromofluorobenzene
Concen: 55.529 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.002 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 95 Resp: 1184777
Ion Ratio Lower Upper
95 100
174 76.7 0.0 187.2
176 73.8 0.0 181.4

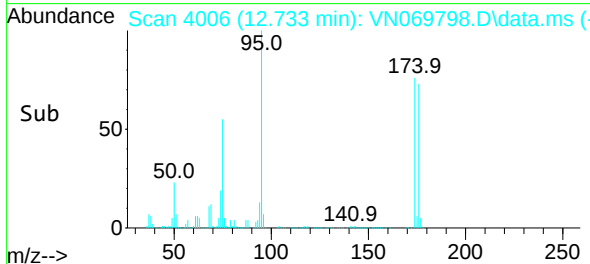

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 117 Resp: 2502302
Ion Ratio Lower Upper
117 100
82 58.4 42.4 63.6
119 32.2 25.4 38.2

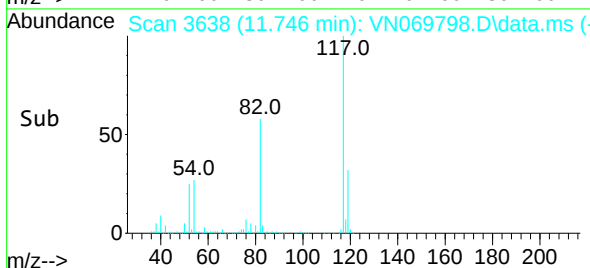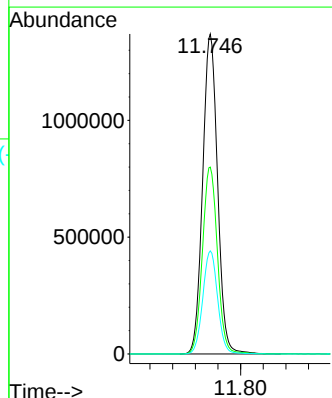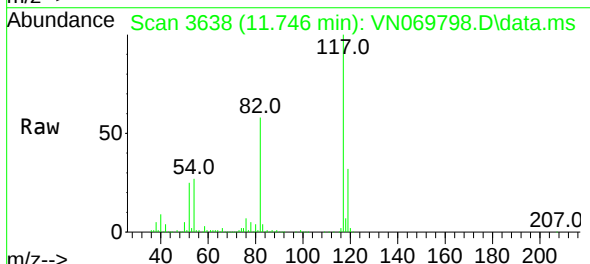

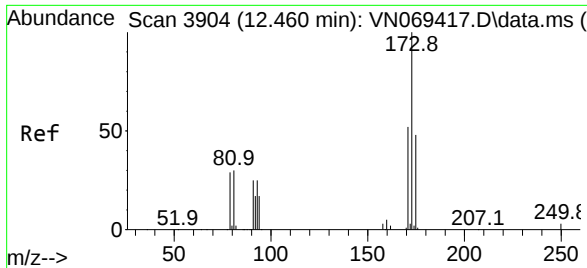

#71

Bromoform

Concen: 2.797 ug/l

RT: 12.725 min Scan# 4003

Delta R.T. 0.265 min

Lab File: VN069798.D

Acq: 6 Dec 2021 21:28

Instrument :





MSVOA_N

ClientSampleId :

FDR-20211202-WC-S

Tgt Ion:173 Resp: 1070

Ion	Ratio	Lower	Upper
173	100		
175	6129.0	24.2	72.6#
254	0.0	0.0	0.0

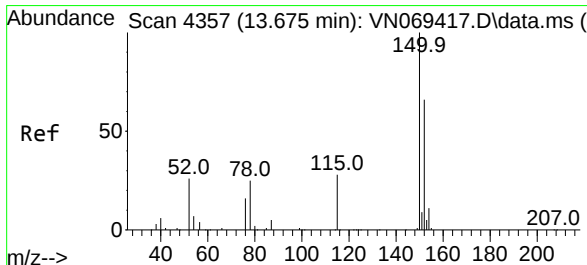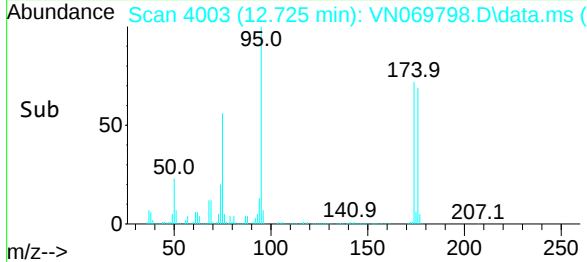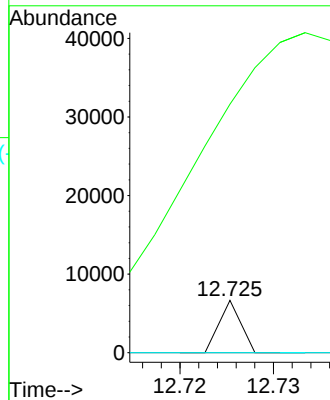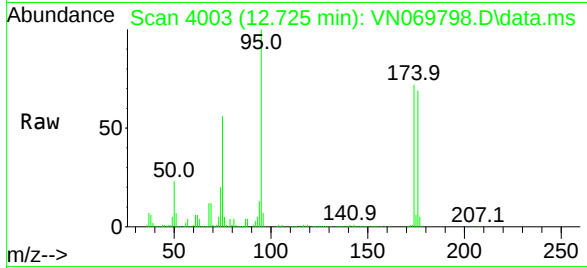

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.677 min Scan# 4358




Delta R.T. 0.000 min


Lab File: VN069798.D

Acq: 6 Dec 2021 21:28

Tgt Ion:152 Resp: 993876


Ion	Ratio	Lower	Upper
152	100		
115	60.6	27.5	82.5
150	156.3	0.0	344.4

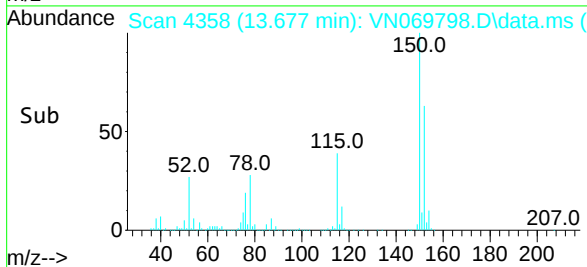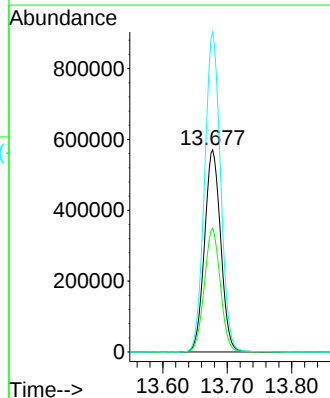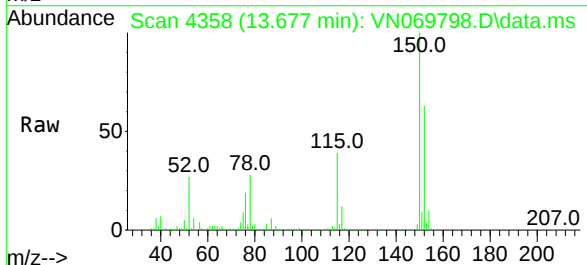






#74
N-amy1 acetate
Concen: 0.425 ug/l
RT: 12.355 min Scan# 31
Delta R.T. -0.032 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S



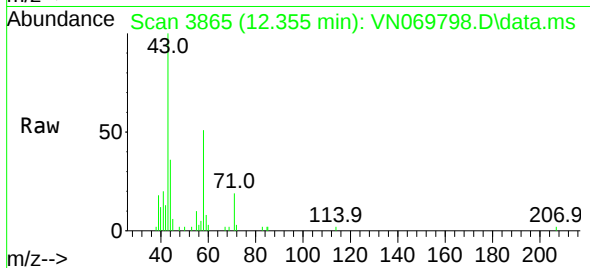



Tgt Ion: 43	Resp: 16636
Ion Ratio	Lower Upper
43 100	
70 1.4	33.4 50.0#
55 6.3	19.3 28.9#
61 0.0	18.5 27.7#

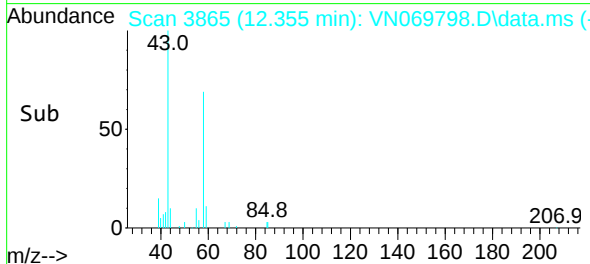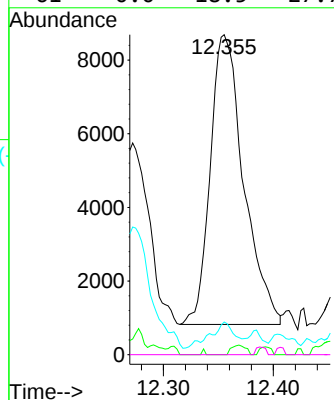

#76
1,2,3-Trichloropropane
Concen: 23.119 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.147 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 75	Resp: 658931
Ion Ratio	Lower Upper
75 100	
77 1.1	82.6 247.8#


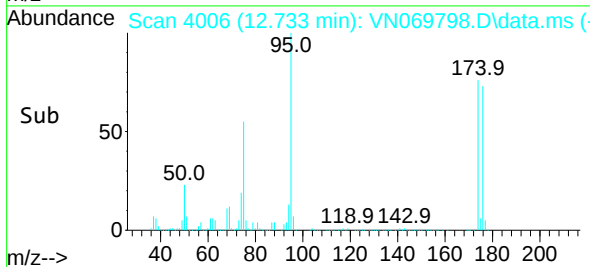
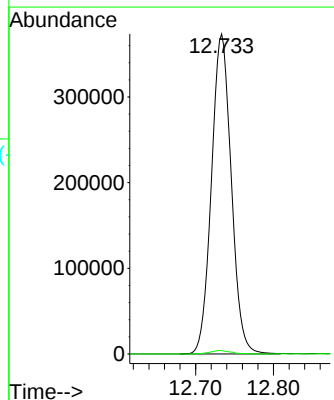
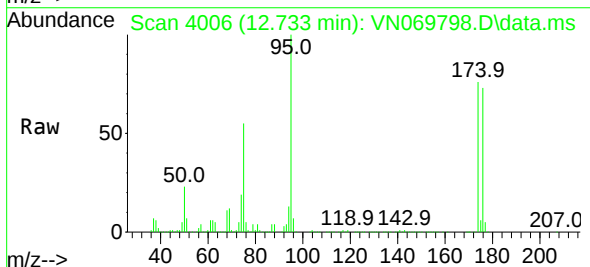




#81
trans-1,4-Dichloro-2-butene
Concen: 73.580 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.107 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion: 75 Resp: 658931
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

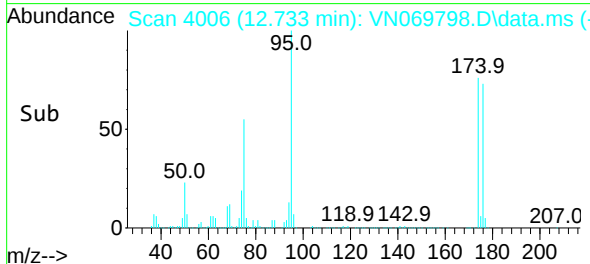

#82
4-Chlorotoluene
Concen: 0.882 ug/l
RT: 13.323 min Scan# 4226
Delta R.T. 0.217 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28

Tgt Ion: 91 Resp: 51560
Ion Ratio Lower Upper
91 100
126 0.0 18.2 54.6#


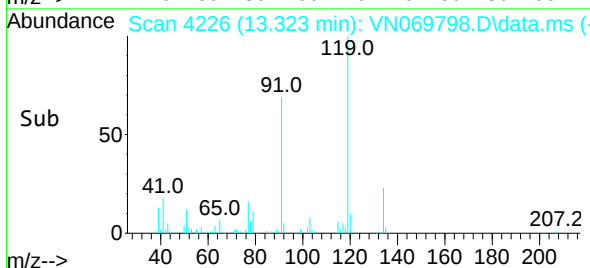
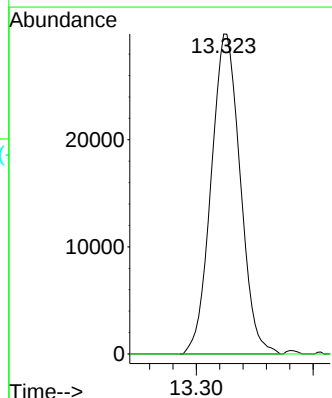
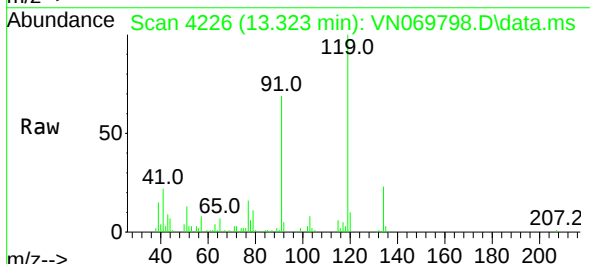


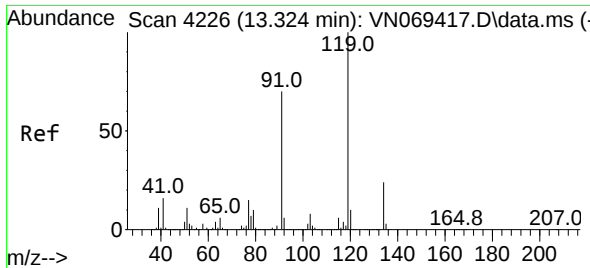

#83
 tert-Butylbenzene
 Concen: 1.152 ug/l
 RT: 13.326 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VN069798.D
 Acq: 6 Dec 2021 21:28




Instrument :
 MSVOA_N
 ClientSampleId :
 FDR-20211202-WC-S


Tgt Ion:119 Resp: 72629
 Ion Ratio Lower Upper
 119 100
 91 71.0 31.5 94.5
 134 23.6 12.4 37.4

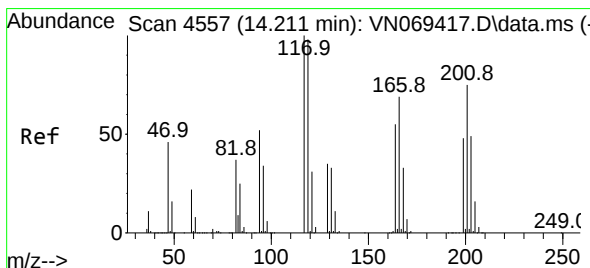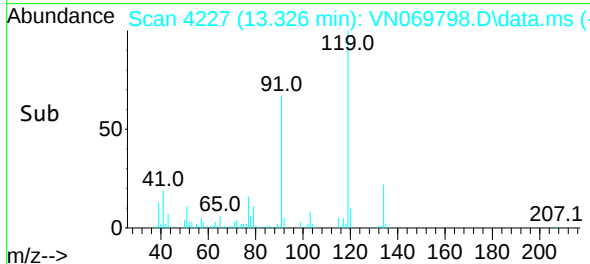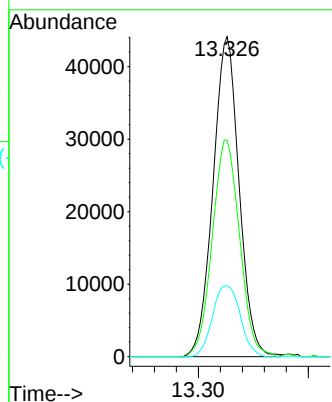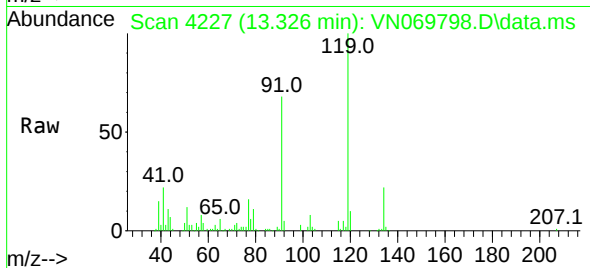

#90
 Hexachloroethane
 Concen: 0.239 ug/l
 RT: 14.329 min Scan# 4601
 Delta R.T. 0.118 min
 Lab File: VN069798.D
 Acq: 6 Dec 2021 21:28

Tgt Ion:117 Resp: 2807
 Ion Ratio Lower Upper
 117 100
 201 0.0 43.9 131.6#


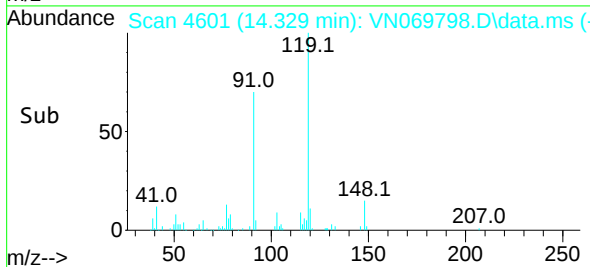
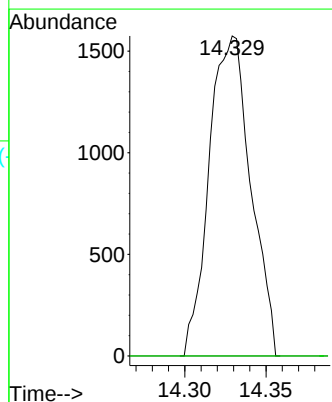
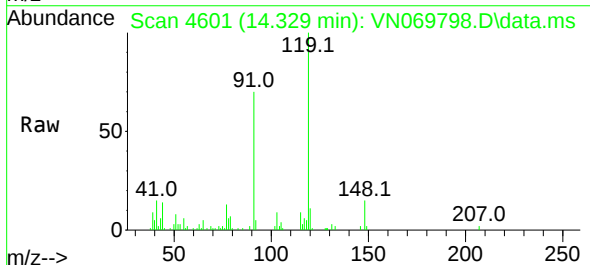




#93
1,2,4-Trichlorobenzene
Concen: 2.905 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28




Instrument :
MSVOA_N
ClientSampleId :
FDR-20211202-WC-S


Tgt Ion:180 Resp: 462
Ion Ratio Lower Upper
180 100
182 74.9 48.3 144.9
145 43.5 14.5 43.5#

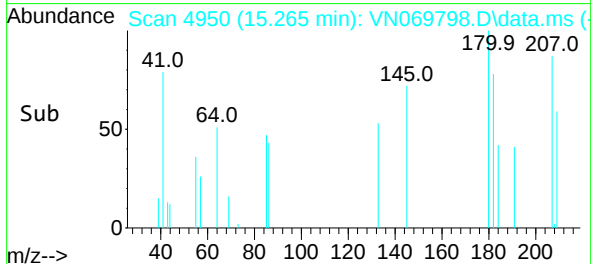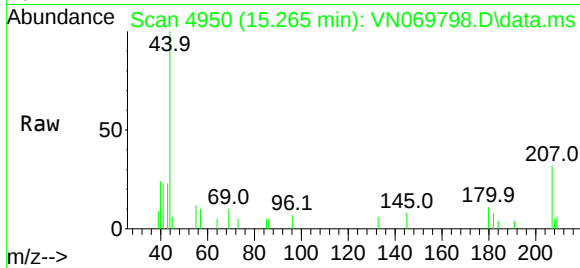

#95
Naphthalene
Concen: 4.011 ug/l
RT: 15.501 min Scan# 5038
Delta R.T. -0.006 min
Lab File: VN069798.D
Acq: 6 Dec 2021 21:28


Tgt Ion:128 Resp: 1374
Ion Ratio Lower Upper
128 100
127 34.1 10.5 15.7#
129 17.2 8.7 13.1#

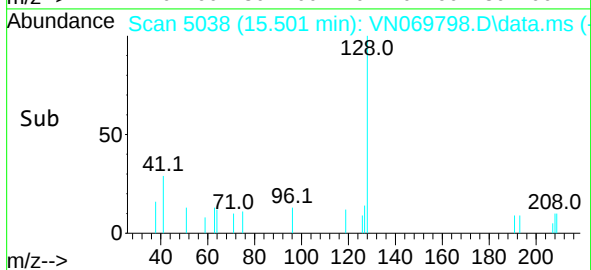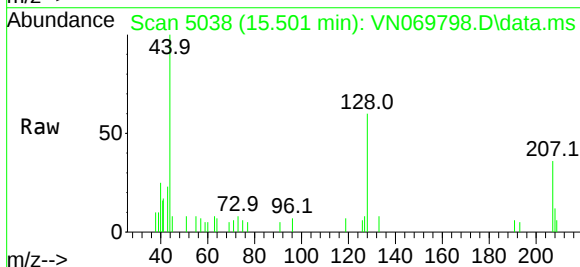



#96
 1,2,3-Trichlorobenzene
 Concen: 2.446 ug/l
 RT: 15.705 min Scan# 51
 Delta R.T. 0.003 min
 Lab File: VN069798.D
 Acq: 6 Dec 2021 21:28

Instrument :
 MSVOA_N
 ClientSampleId :
 FDR-20211202-WC-S



Tgt Ion:180 Resp: 178
 Ion Ratio Lower Upper
 180 100
 182 100.0 47.4 142.2
 145 0.0 15.0 45.1#

