


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120621\
Data File : VN069776.D
Acq On : 6 Dec 2021 10:59
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Title : SW846 8260
Last Update : Fri Dec 03 08:46:47 2021

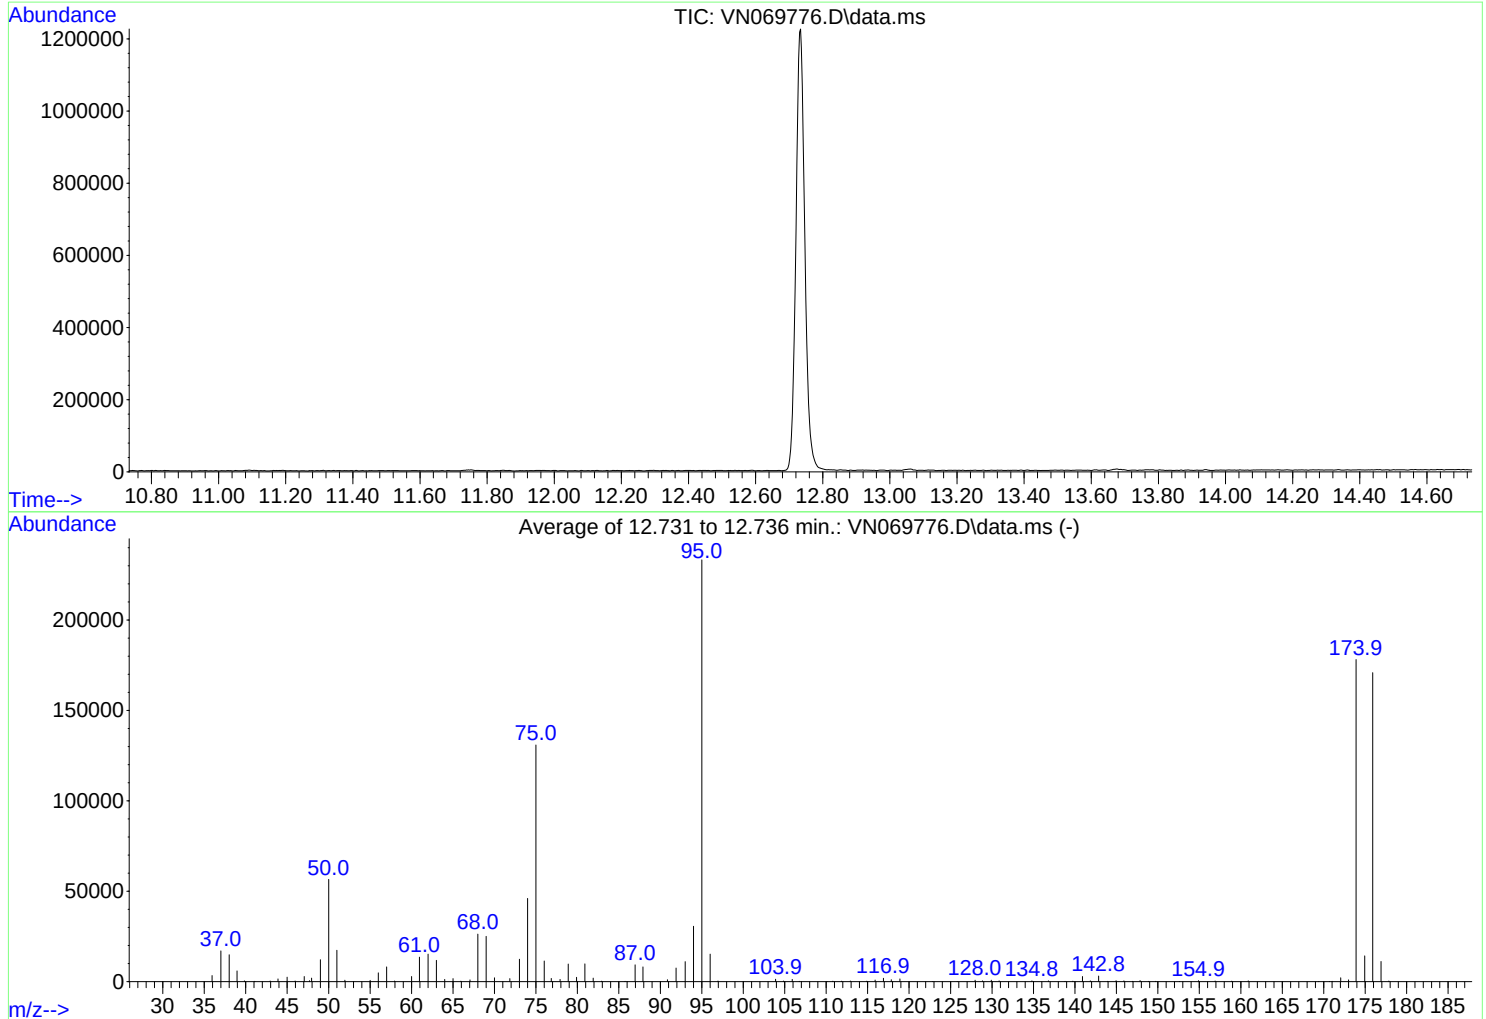

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3987

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.2	56509	PASS
75	95	30	60	56.1	130853	PASS
95	95	100	100	100.0	233259	PASS
96	95	5	9	6.5	15234	PASS
173	174	0.00	2	0.6	985	PASS
174	95	50	100	76.4	178155	PASS
175	174	5	9	8.0	14232	PASS
176	174	95	101	95.9	170880	PASS
177	176	5	9	6.5	11143	PASS