

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120623\
 Data File : VN080399.D
 Acq On : 06 Dec 2023 20:19
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Dec 07 01:07:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 17 01:19:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	206092	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	359417	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	379457	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	191450	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	161784	47.543	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	95.080%
35) Dibromofluoromethane	8.165	113	136329	51.406	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.820%
50) Toluene-d8	10.571	98	477783	49.977	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.960%
62) 4-Bromofluorobenzene	12.847	95	209311	57.965	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	115.940%
Target Compounds						
95) Naphthalene	15.641	128	355688	32.612	ug/l	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120623\
Data File : VN080399.D
Acq On : 06 Dec 2023 20:19
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Dec 07 01:07:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 17 01:19:32 2023
Response via : Initial Calibration




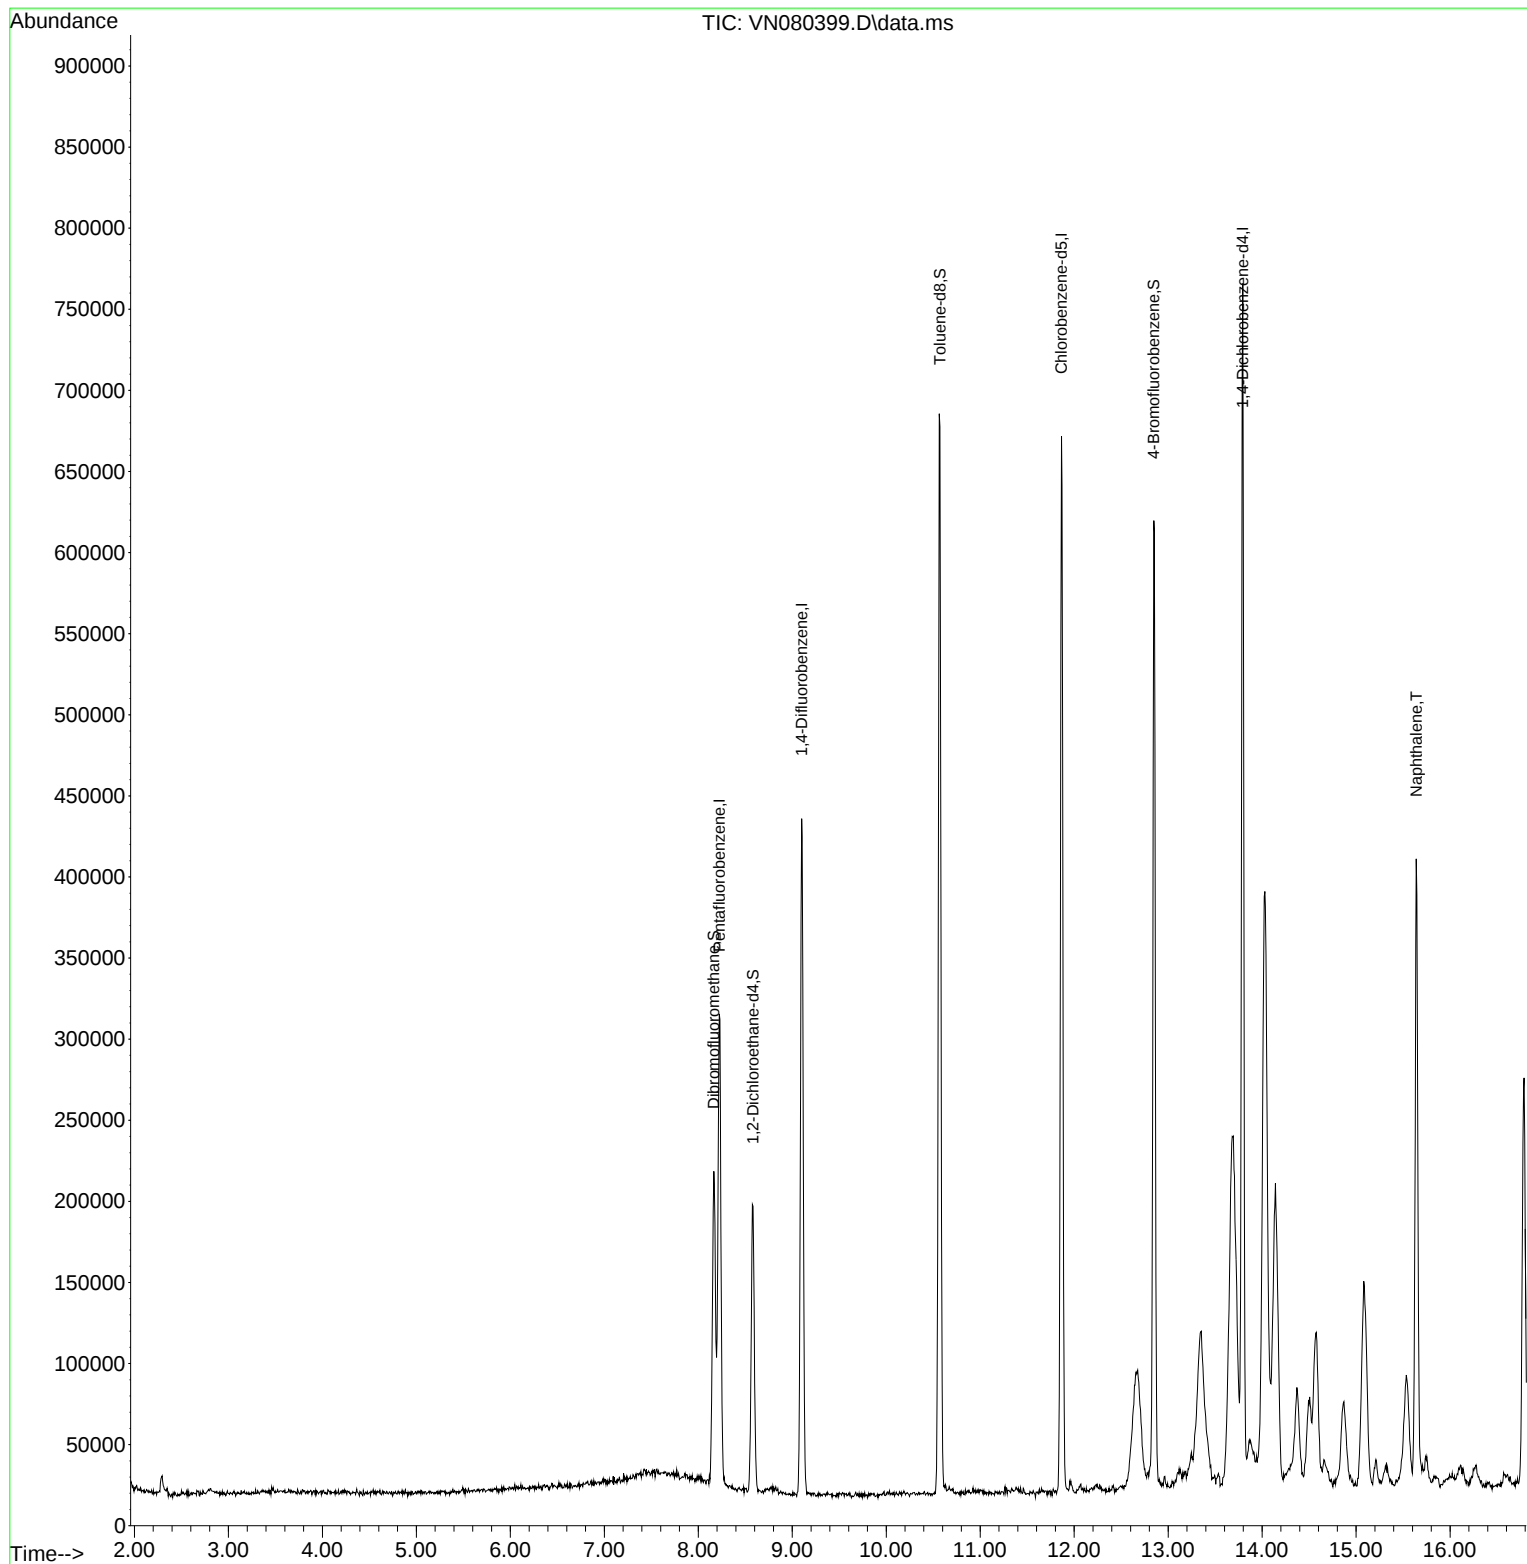


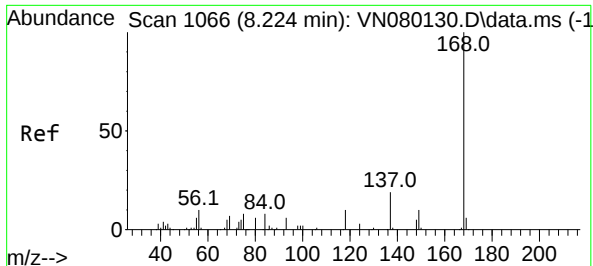

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN080399.D
Acq: 06 Dec 2023 20:19




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 206092
Ion Ratio Lower Upper
168 100
99 61.7 53.0 79.6

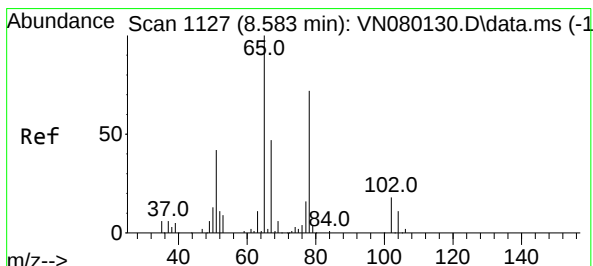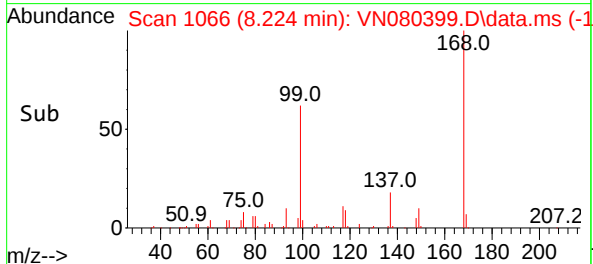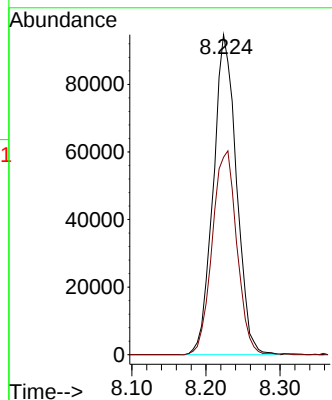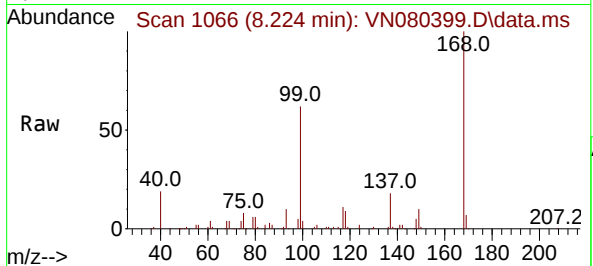

#33
1,2-Dichloroethane-d4
Concen: 47.543 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VN080399.D
Acq: 06 Dec 2023 20:19

Tgt Ion: 65 Resp: 161784
Ion Ratio Lower Upper
65 100
67 49.0 0.0 106.6

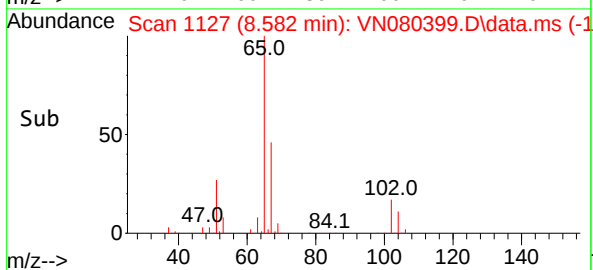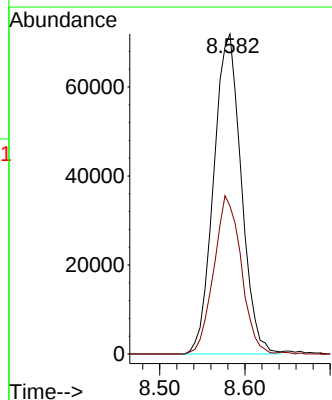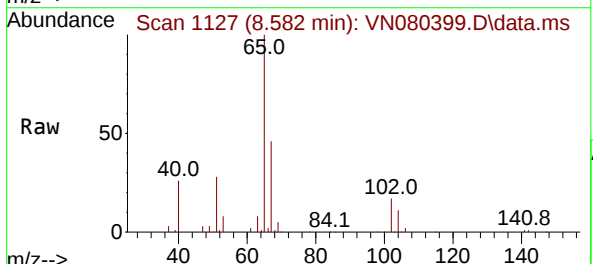

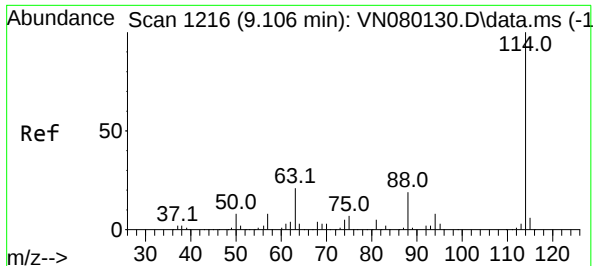

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.006 min

Lab File: VN080399.D

Acq: 06 Dec 2023 20:19

Instrument :

MSVOA_N

ClientSampleId :

IBLK




Tgt Ion:114 Resp: 359417

Ion Ratio Lower Upper

114 100

63 20.7 0.0 36.4

88 16.7 0.0 30.6

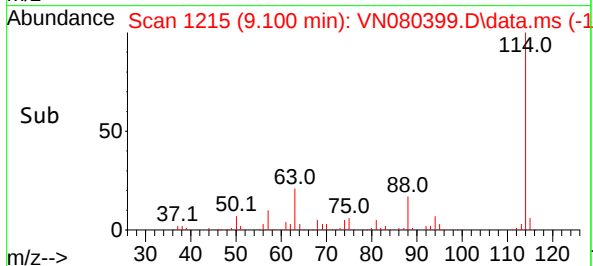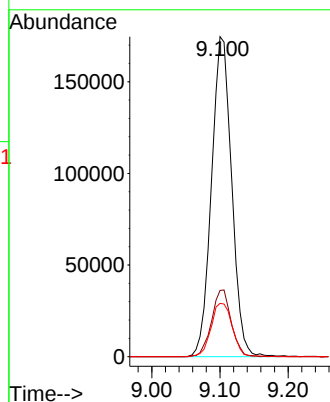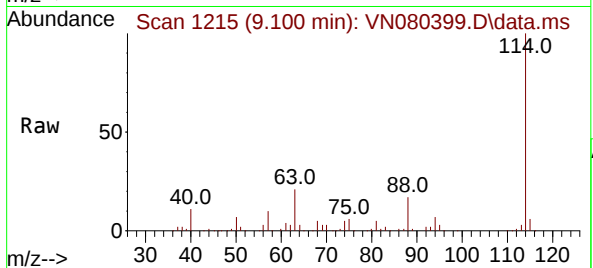

#35

Dibromofluoromethane

Concen: 51.406 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN080399.D

Acq: 06 Dec 2023 20:19




Tgt Ion:113 Resp: 136329


Ion Ratio Lower Upper

113 100

111 103.3 82.6 123.8

192 18.8 12.7 19.1


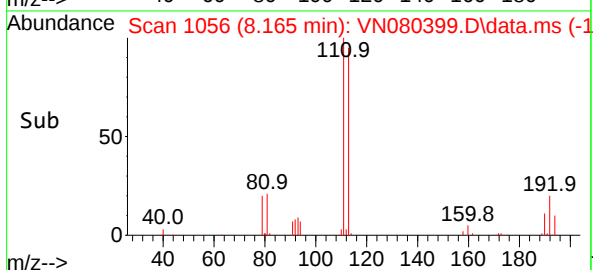
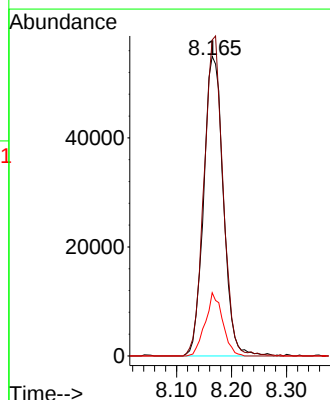
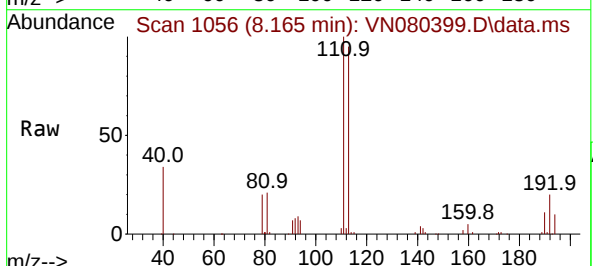


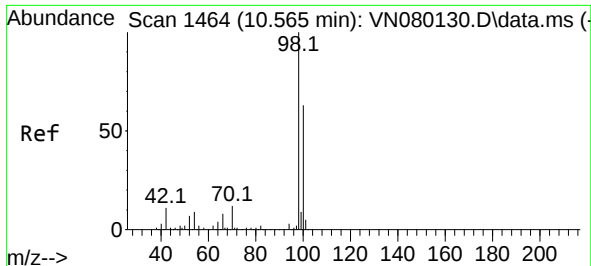

#50
Toluene-d8
Concen: 49.977 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.006 min
Lab File: VN080399.D
Acq: 06 Dec 2023 20:19




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 477783
Ion Ratio Lower Upper
98 100
100 64.6 52.0 78.0

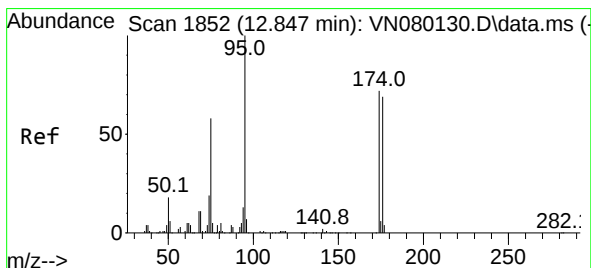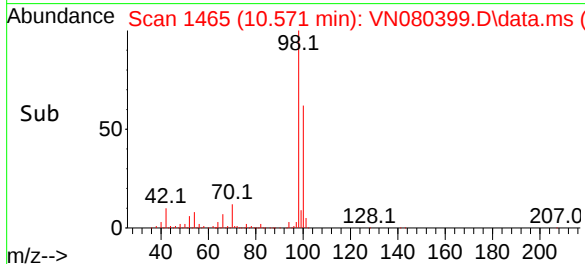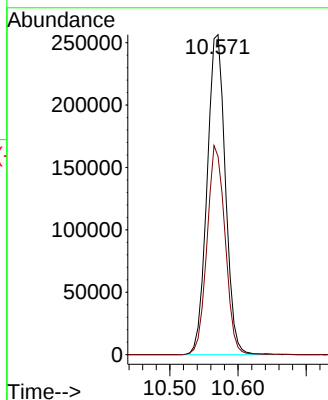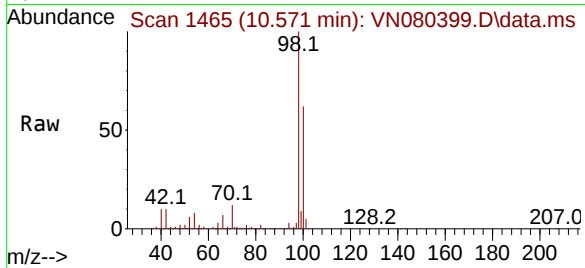

#62
4-Bromofluorobenzene
Concen: 57.965 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN080399.D
Acq: 06 Dec 2023 20:19

Tgt Ion: 95 Resp: 209311
Ion Ratio Lower Upper
95 100
174 75.6 0.0 143.8
176 73.1 0.0 135.8


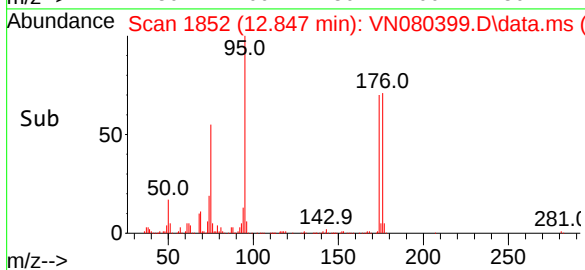
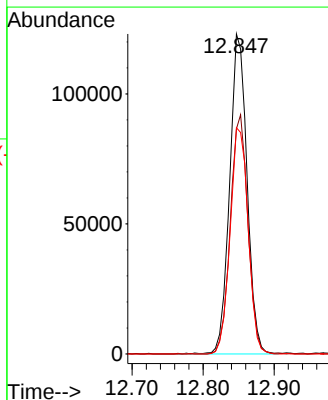
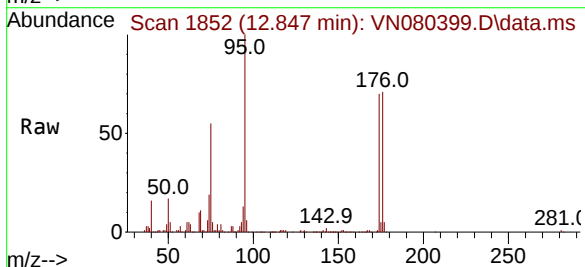


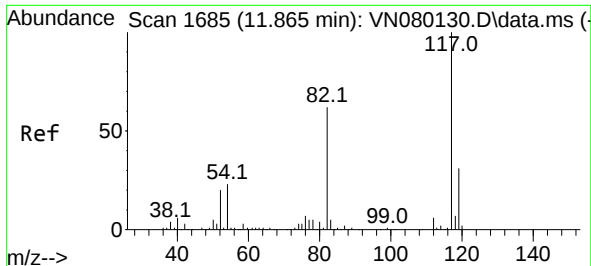

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VN080399.D
Acq: 06 Dec 2023 20:19




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:117 Resp: 379457
Ion Ratio Lower Upper
117 100
82 60.9 44.0 66.0
119 31.2 25.6 38.4

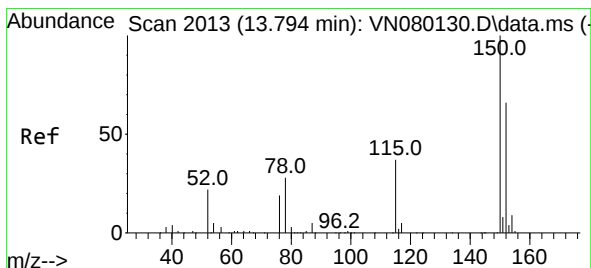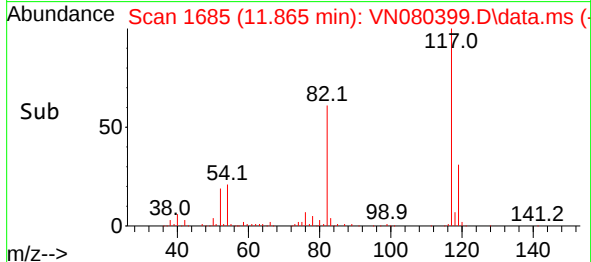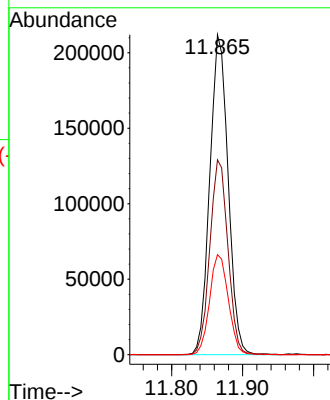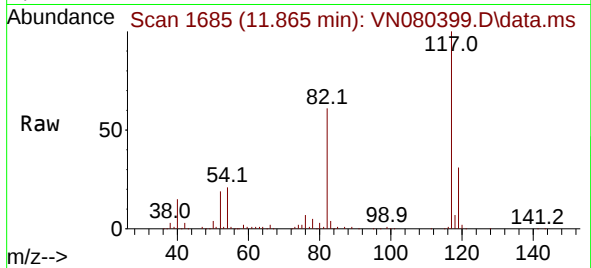

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN080399.D
Acq: 06 Dec 2023 20:19


Tgt Ion:152 Resp: 191450
Ion Ratio Lower Upper
152 100
115 67.4 32.3 96.8
150 158.3 0.0 355.8

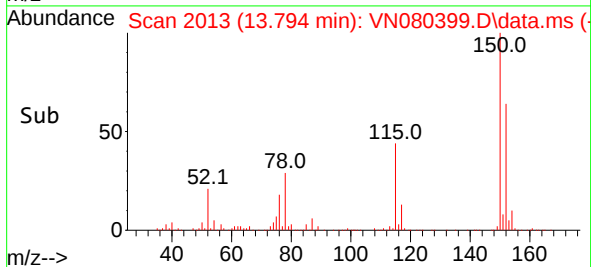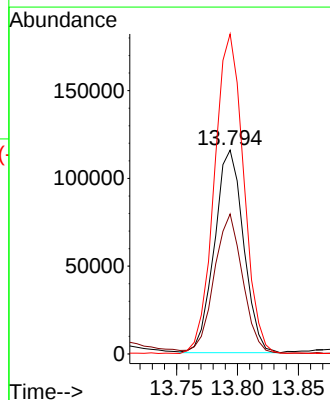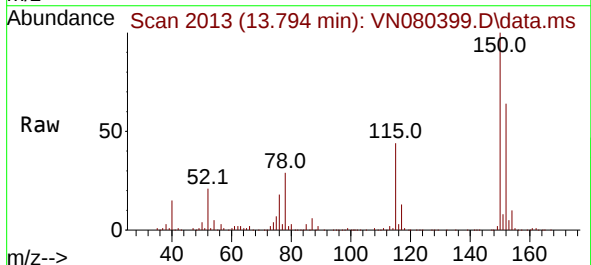

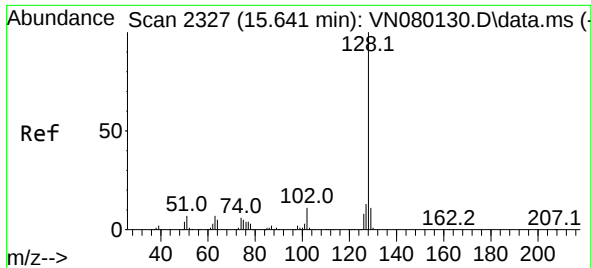

#95
Naphthalene
Concen: 32.612 ug/l
RT: 15.641 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN080399.D
Acq: 06 Dec 2023 20:19

Instrument :
MSVOA_N
ClientSampleId :
IBLK

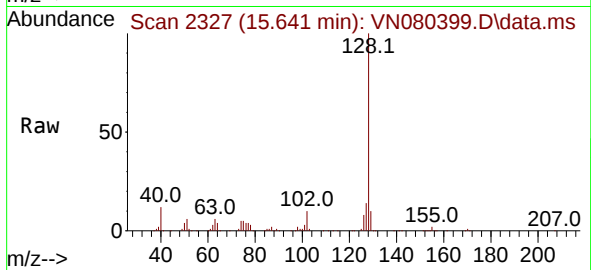

Tgt Ion:128 Resp: 355688
Ion Ratio Lower Upper
128 100
127 13.8 10.0 15.0
129 10.9 8.7 13.1

