

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120623\
 Data File : VN080394.D
 Acq On : 06 Dec 2023 18:20
 Operator : JC\MD
 Sample : 05650-01 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 50194

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
 Title : SW846 8260

Signal : TIC: VN080394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.295	51	58	61	rBV3	11317	24689	2.26%	0.322%
2	2.512	87	95	101	rBV2	35561	59746	5.47%	0.780%
3	3.254	213	221	227	rVB4	14584	30194	2.76%	0.394%
4	3.659	283	290	291	rBV5	6763	12127	1.11%	0.158%
5	3.783	305	311	320	rBV	21247	54553	4.99%	0.713%
6	4.148	364	373	380	rBV2	16564	43930	4.02%	0.574%
7	7.565	947	954	963	rBV3	11437	29731	2.72%	0.388%
8	8.165	1046	1056	1061	rBV	175199	412840	37.78%	5.392%
9	8.224	1061	1066	1077	rVB	252252	564293	51.64%	7.370%
10	8.600	1115	1130	1141	rBV3	227844	794490	72.70%	10.377%
11	9.106	1208	1216	1224	rBV	372381	750130	68.64%	9.798%
12	10.571	1456	1465	1470	rBV	580997	1092791	100.00%	14.273%
13	10.630	1470	1475	1484	rVB	412523	757618	69.33%	9.896%
14	11.865	1677	1685	1696	rBV	576457	1026634	93.95%	13.409%
15	11.965	1696	1702	1707	rVV	21907	40386	3.70%	0.527%
16	12.071	1713	1720	1727	rBV2	60222	117330	10.74%	1.532%
17	12.400	1770	1776	1782	rBV2	30222	54944	5.03%	0.718%
18	12.853	1844	1853	1861	rBV	482388	823471	75.35%	10.756%
19	13.488	1956	1961	1964	rBV3	8356	12576	1.15%	0.164%
20	13.794	2005	2013	2023	rBV	555677	936943	85.74%	12.238%
21	15.641	2323	2327	2333	rVB2	8596	16703	1.53%	0.218%




Sum of corrected areas: 7656119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120623\
Data File : VN080394.D
Acq On : 06 Dec 2023 18:20
Operator : JC\MD
Sample : 05650-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
50194

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

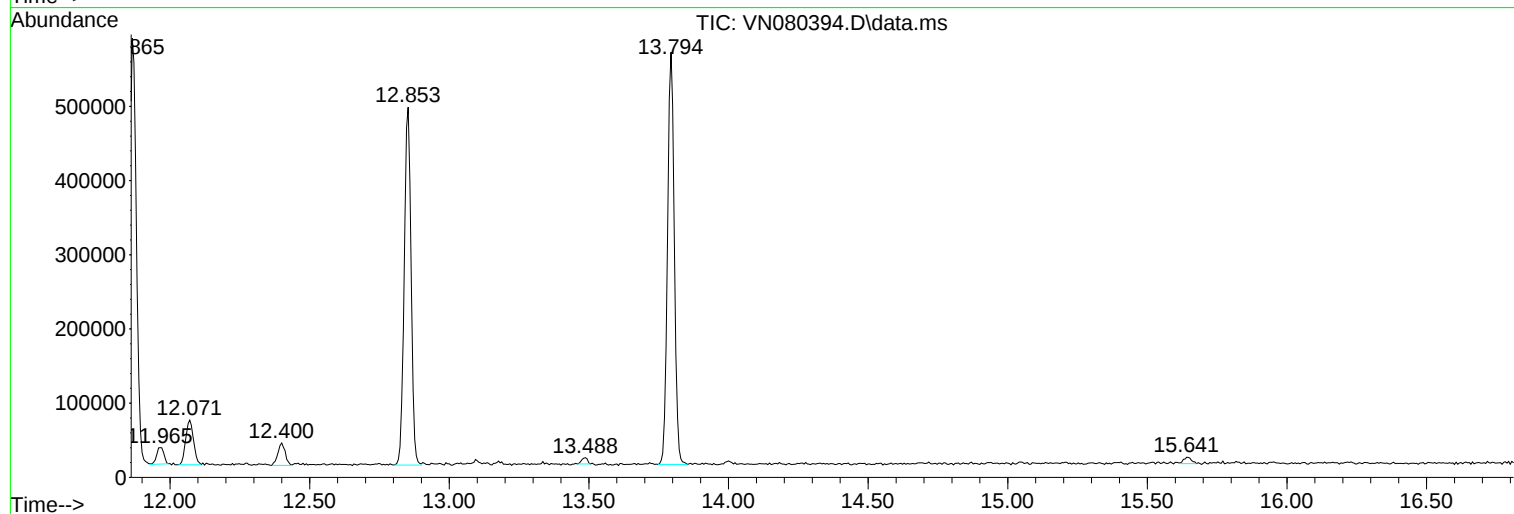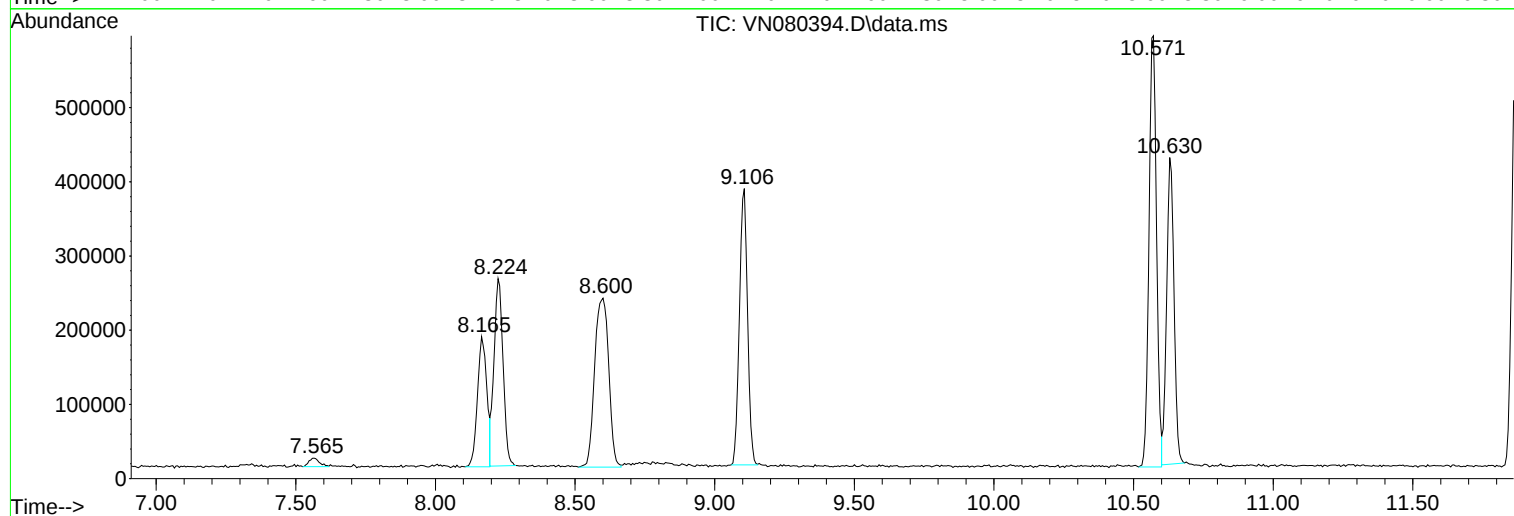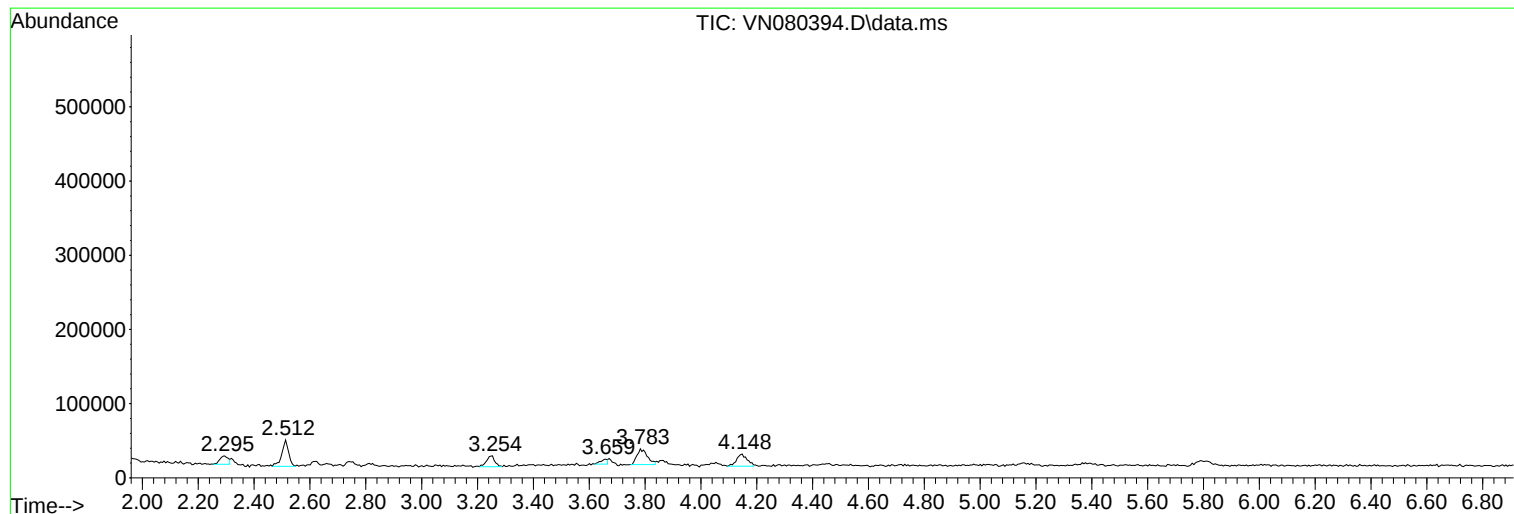

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120623\
Data File : VN080394.D
Acq On : 06 Dec 2023 18:20
Operator : JC\MD
Sample : 05650-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
50194










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.512 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.512	5.29 ug/l	59746	Pentafluorobenzene	8.224

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane	58	C4H10	000106-97-8	42
2			Isopropylsulfonyl chloride	142	C3H7ClO2S	010147-37-2	9
3			Formic acid, chloro-, (3,4,4-tri...	194	C7H11ClO4	107323-92-2	9
4			Acetone	58	C3H6O	000067-64-1	7
5			Hydrogen isocyanate	43	CHNO	000075-13-8	4

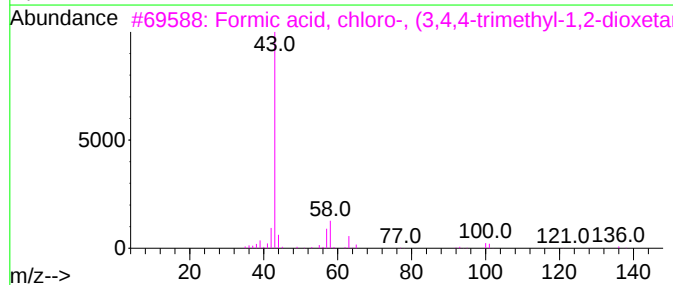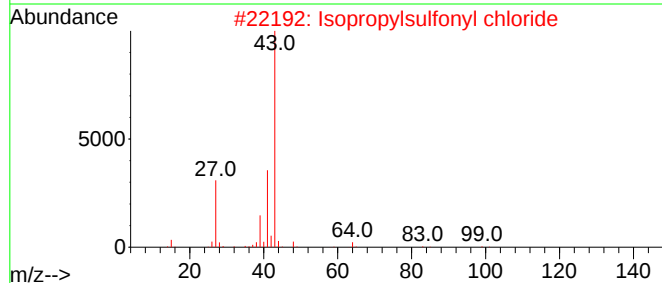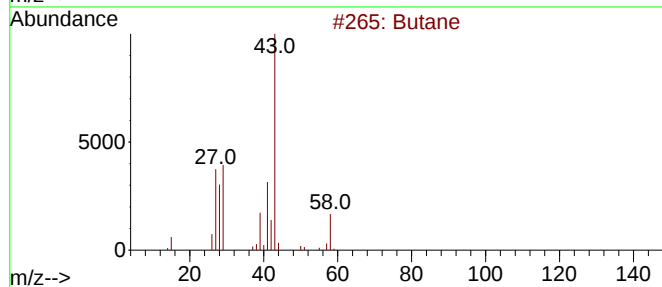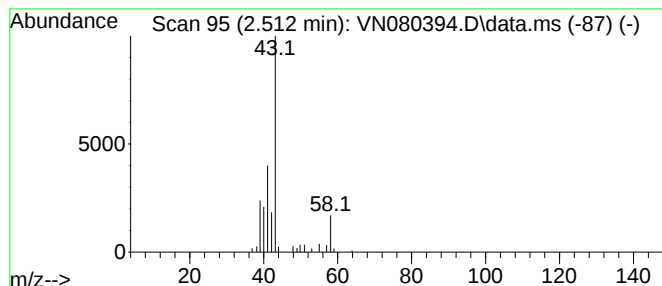

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120623\
Data File : VN080394.D
Acq On : 06 Dec 2023 18:20
Operator : JC\MD
Sample : 05650-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
50194

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.512	2.512	5.3	ug/l	59746	1	8.224	564293	50.0