

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN120718\
 Data File : VN052719.D
 Acq On : 7 Dec 2018 11:52
 Operator : MD\SY
 Sample : VN1207WBL02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1207WBL02

Quant Time: Dec 07 13:01:17 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 03 03:24:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1107918	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1727278	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1488958	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	535440	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	586992	48.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.32%	
35) Dibromofluoromethane	7.59	113	535569	50.29	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.58%	
50) Toluene-d8	10.09	98	2106982	50.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.66%	
62) 4-Bromofluorobenzene	12.40	95	636755	45.72	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.44%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN120718\
Data File : VN052719.D
Acq On : 7 Dec 2018 11:52
Operator : MD\SY
Sample : VN1207WBL02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
VN1207WBL02

Quant Time: Dec 07 13:01:17 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 03 03:24:02 2018
Response via : Initial Calibration

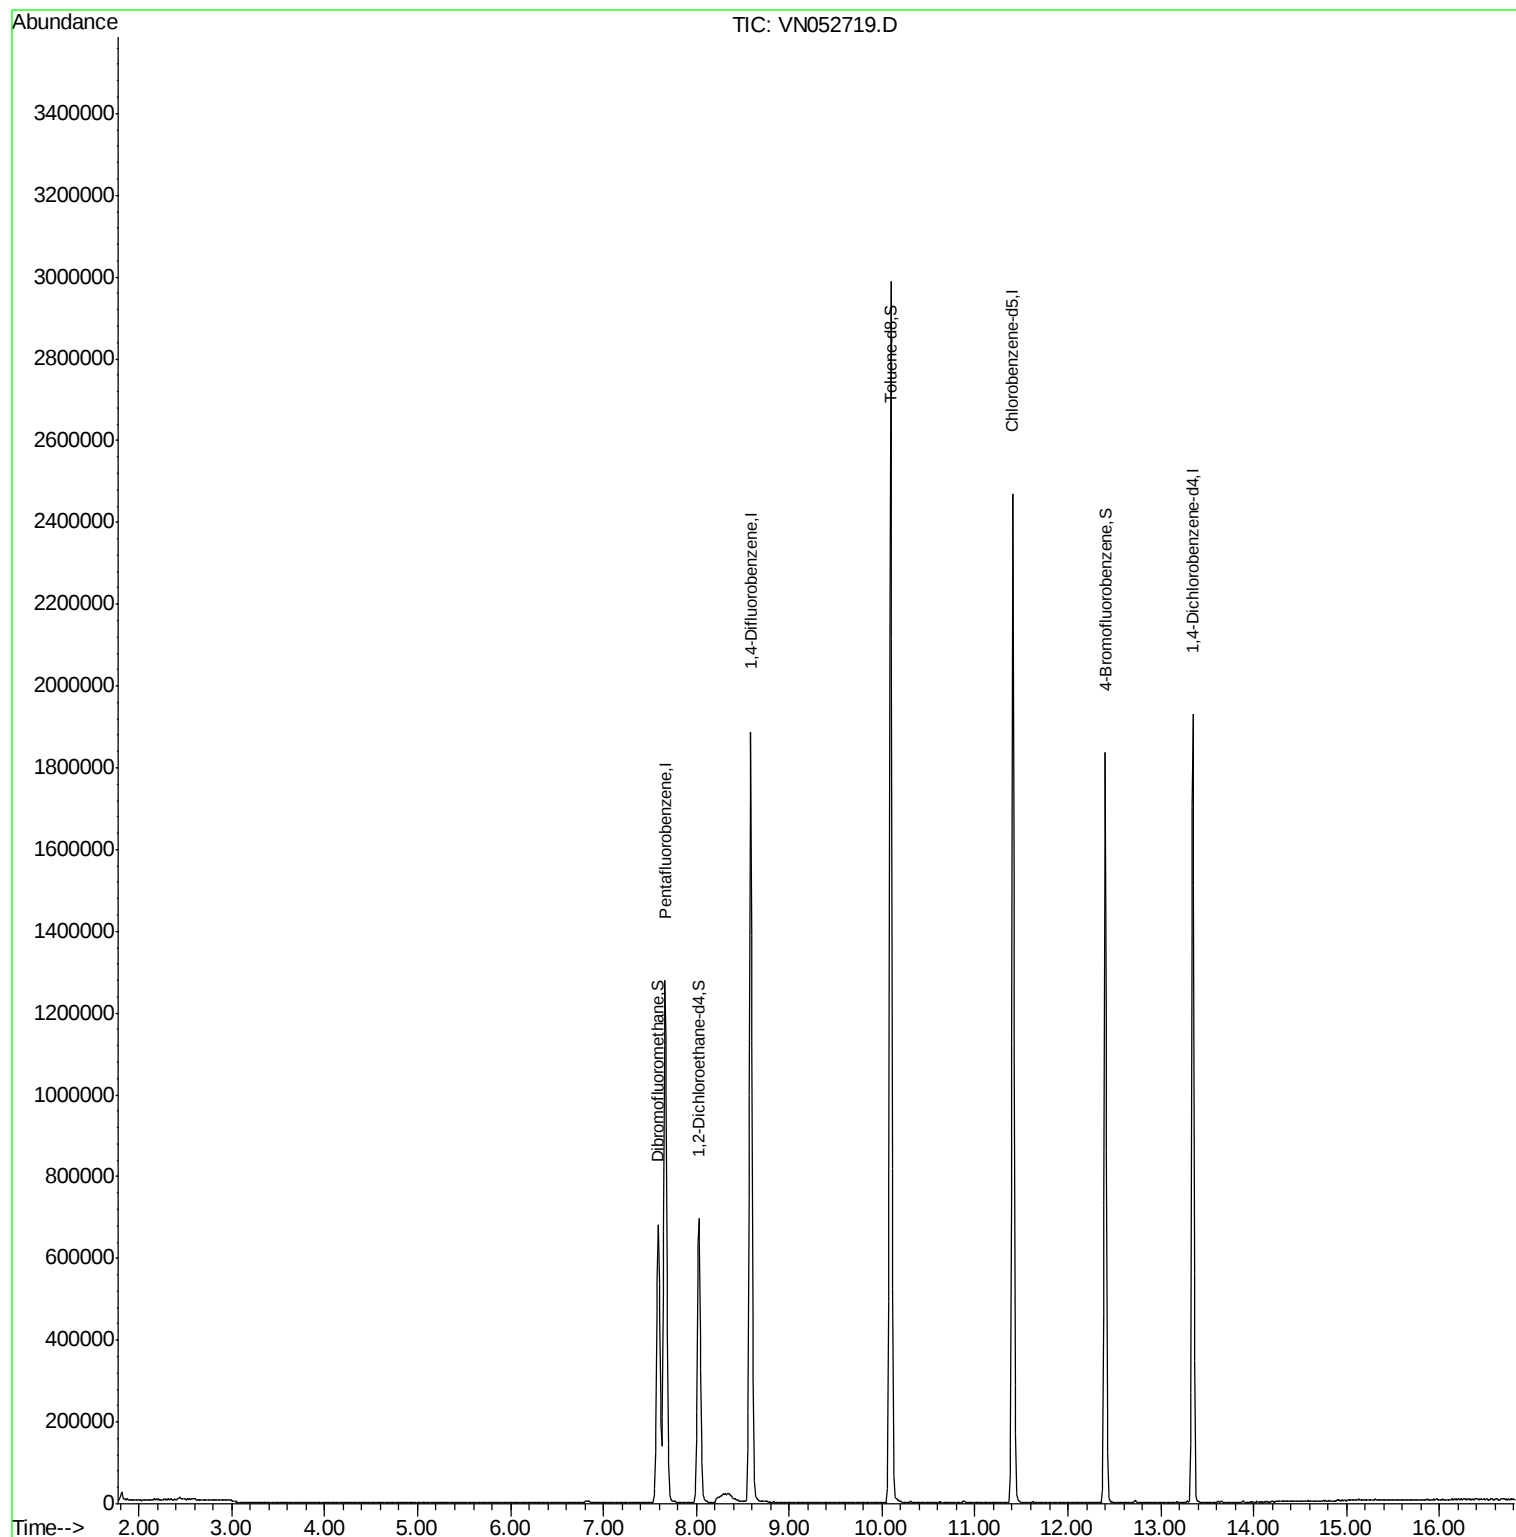

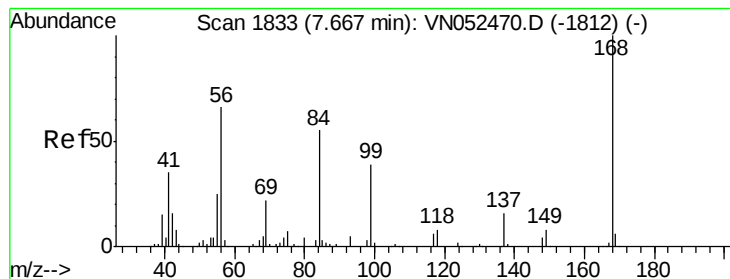

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN052719.D

Acq: 7 Dec 2018 11:52

Instrument :

MSVOA_N

ClientSampleId :


VN1207WBL02

Tgt Ion:168 Resp: 1107918

Ion Ratio Lower Upper

168 100

99 51.7 41.7 62.5

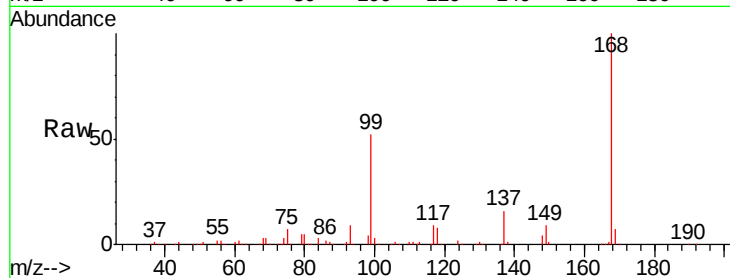

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.67

400000



300000

200000

100000

0

Time-->

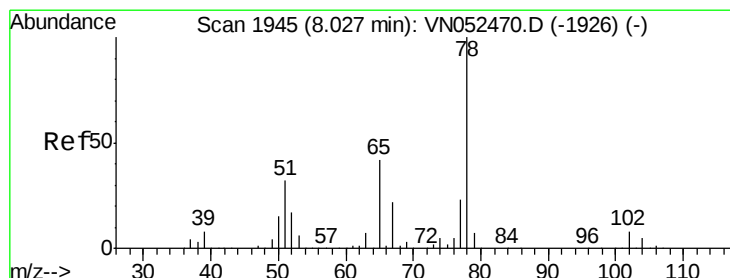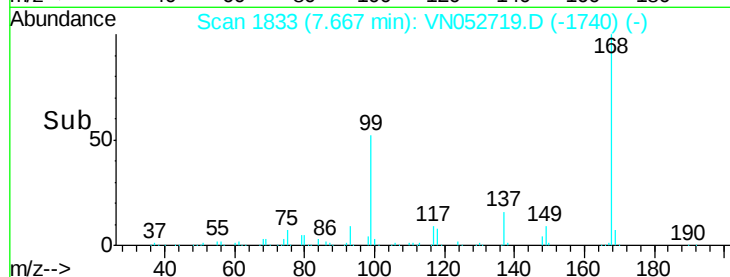

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 8.03 min Scan# 1945

Delta R.T. -0.00 min

Lab File: VN052719.D


Acq: 7 Dec 2018 11:52

Tgt Ion: 65 Resp: 586992

Ion Ratio Lower Upper

65 100

67 54.8 0.0 109.8

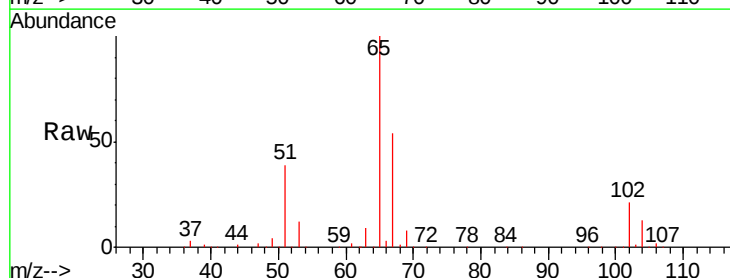

Abundance Ion 64.90 (64.60 to 65.60): VNO

Ion 66.90 (66.60 to 67.60): VNO

8.03

300000

250000

200000


150000


100000

50000

0

Time-->

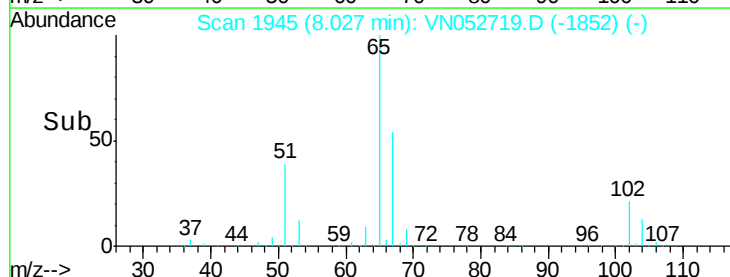


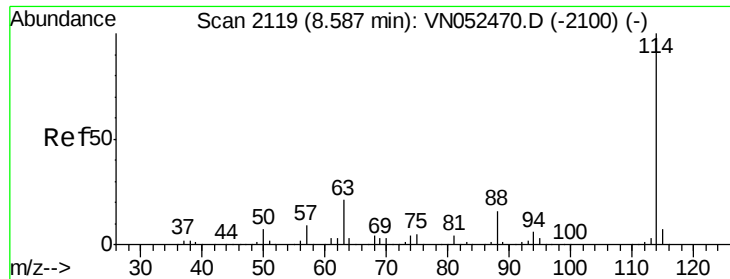




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN052719.D
 Acq: 7 Dec 2018 11:52

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1207WBL02

Tgt Ion:114 Resp: 1727278
 Ion Ratio Lower Upper
 114 100
 63 20.4 0.0 41.8
 88 15.4 0.0 31.6

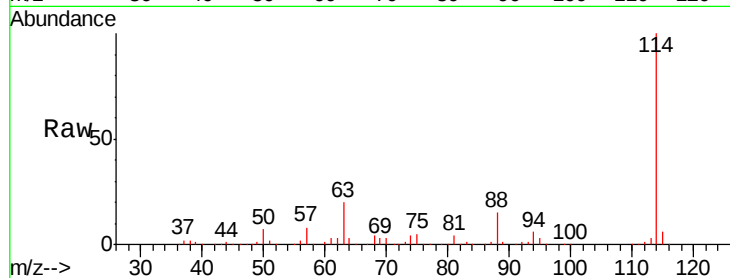


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN0
 Ion 87.90 (87.60 to 88.60): VN0

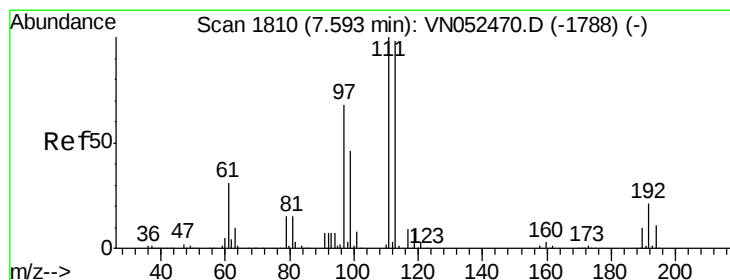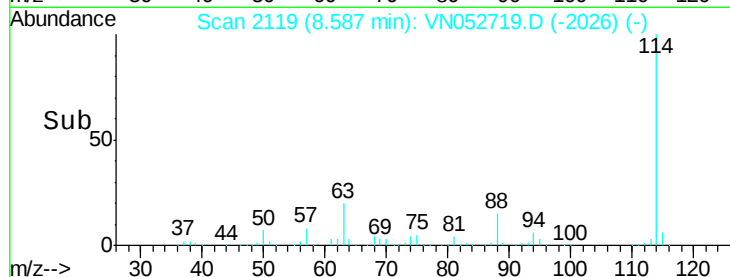
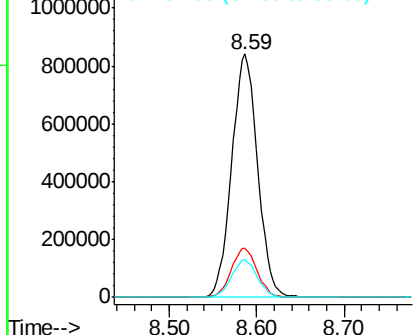



#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 7.59 min Scan# 1809
 Delta R.T. -0.00 min
 Lab File: VN052719.D
 Acq: 7 Dec 2018 11:52

Tgt Ion:113 Resp: 535569
 Ion Ratio Lower Upper
 113 100
 111 102.1 82.0 123.0
 192 21.9 17.0 25.6

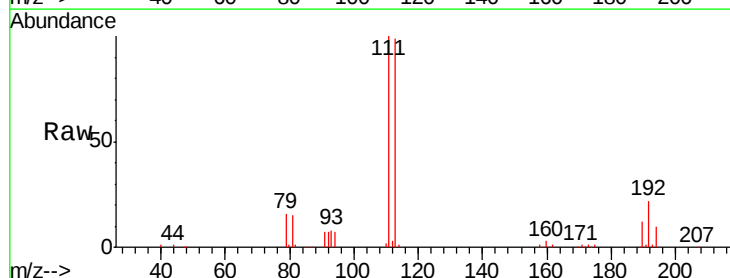

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

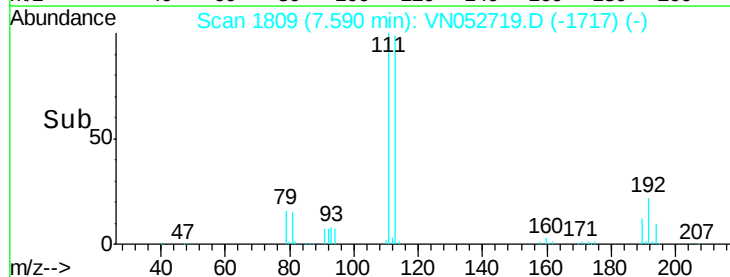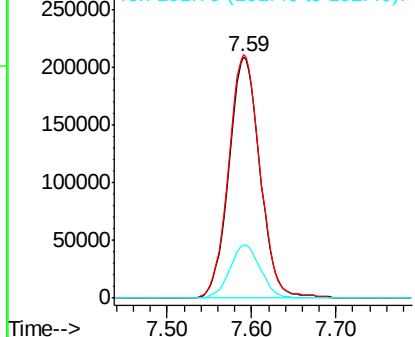

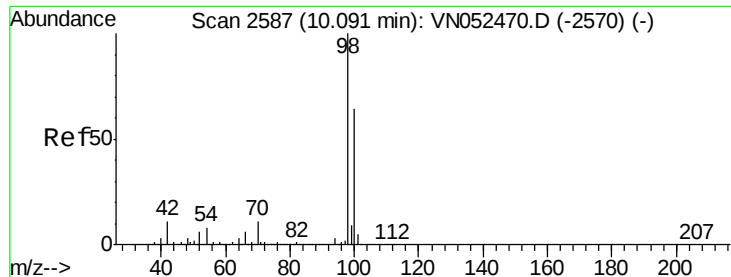

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN052719.D

Acq: 7 Dec 2018 11:52

Instrument :

MSVOA_N

ClientSampleId :


VN1207WBL02

Tgt Ion: 98 Resp: 2106982

Ion Ratio Lower Upper

98 100

100 64.2 51.3 76.9

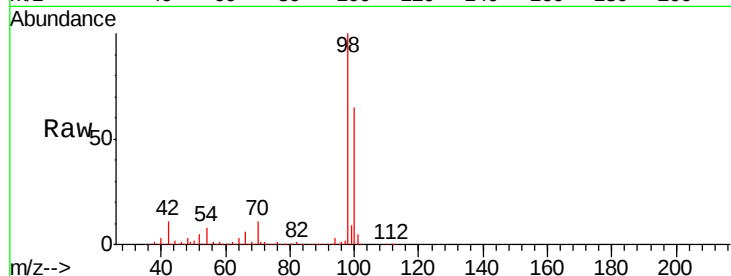

Abundance Ion 98.00 (97.70 to 98.70): VN052719.D (-2494) (-)

Ion 100.00 (99.70 to 100.70): VN052719.D (-2494) (-)

10.09



1000000

500000

0

Time-->

10.00 10.10 10.20

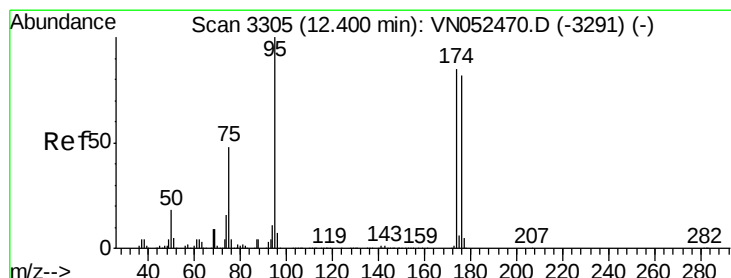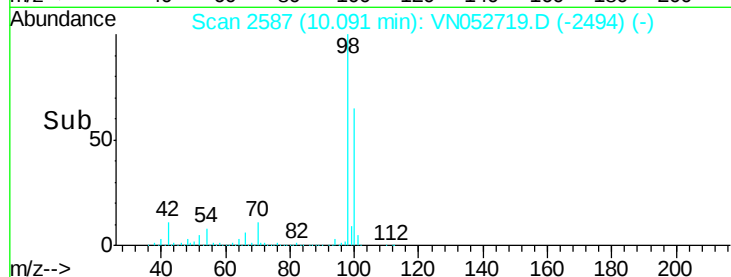

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN052719.D

Acq: 7 Dec 2018 11:52


Tgt Ion: 95 Resp: 636755

Ion Ratio Lower Upper

95 100

174 88.3 0.0 173.0

176 85.9 0.0 166.2

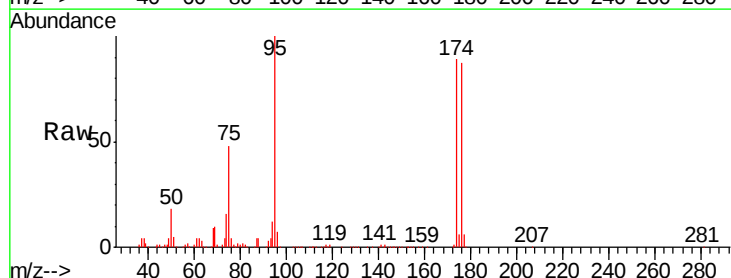

Abundance Ion 94.90 (94.60 to 95.60): VN052719.D (-3212) (-)

Ion 173.80 (173.50 to 174.50): VN052719.D (-3212) (-)

Ion 175.80 (175.50 to 176.50): VN052719.D (-3212) (-)

500000

400000

300000


200000


100000

0

Time-->

12.30 12.40 12.50




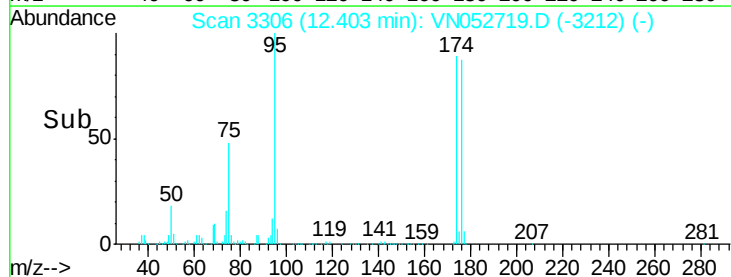


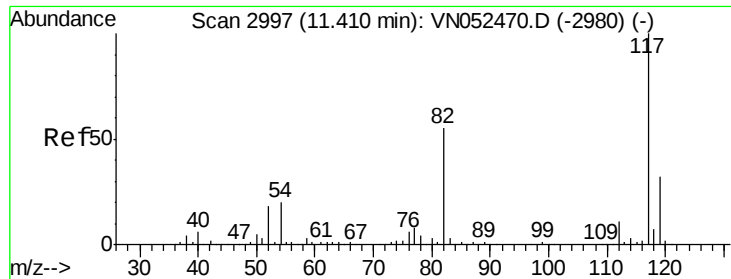

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. -0.00 min
Lab File: VN052719.D
Acq: 7 Dec 2018 11:52

Instrument :
MSVOA_N
ClientSampled :
VN1207WBL02

Tgt Ion:117 Resp: 1488958
Ion Ratio Lower Upper
117 100
82 54.3 43.6 65.4
119 32.5 25.4 38.2

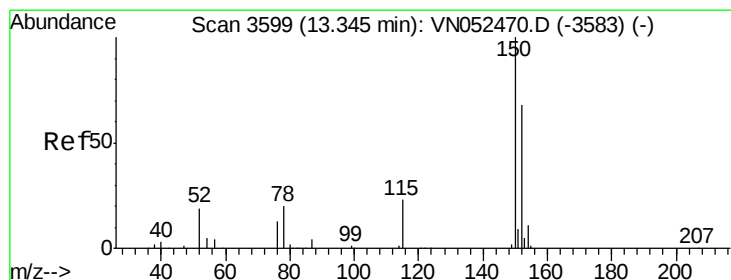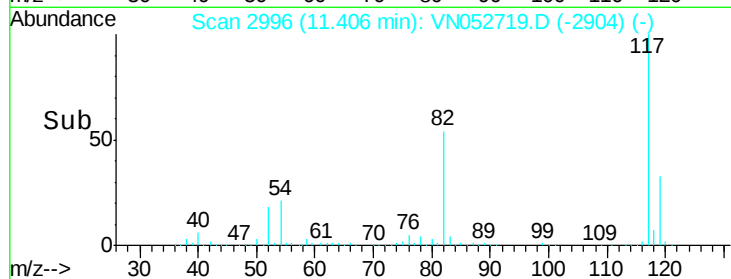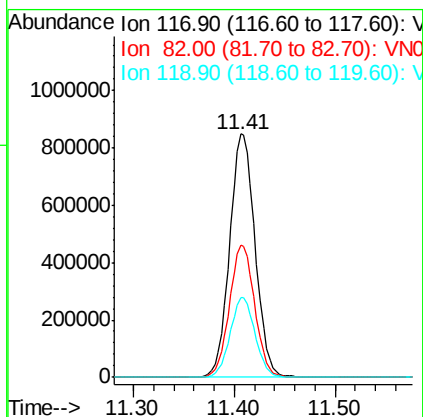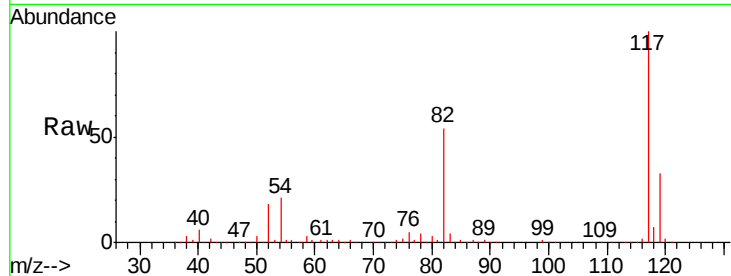

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. -0.00 min
Lab File: VN052719.D
Acq: 7 Dec 2018 11:52

Tgt Ion:152 Resp: 535440
Ion Ratio Lower Upper
152 100
115 56.6 28.4 85.2
150 157.5 0.0 346.0

