


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120718\
Data File : VN052715.D
Acq On : 7 Dec 2018 9:39
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112718W.M
Title : SW846 8260
Last Update : Mon Dec 03 03:24:02 2018

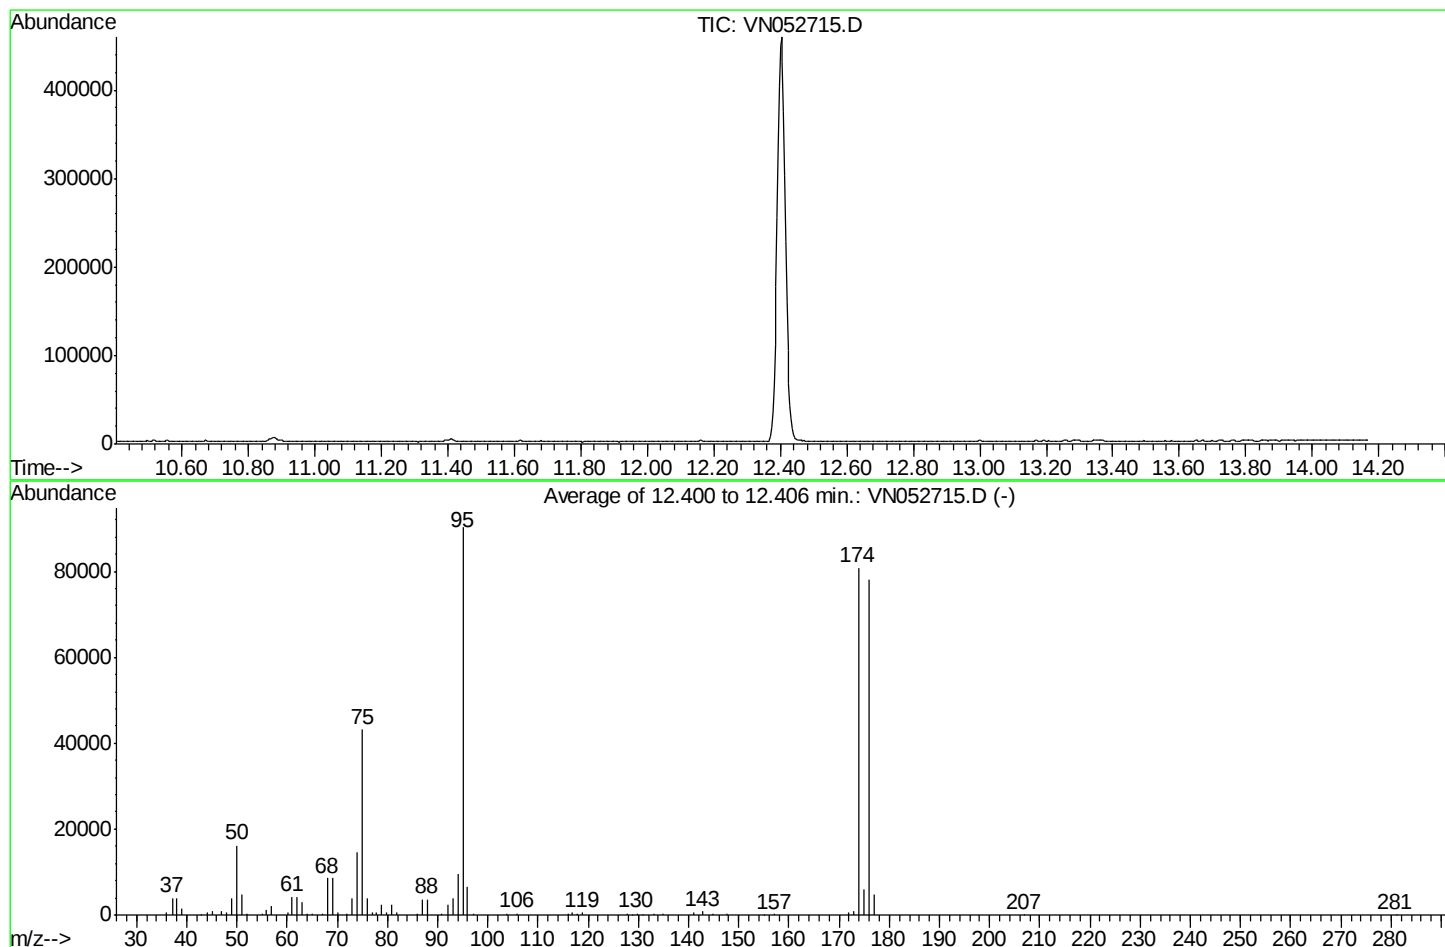

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	16234	PASS
75	95	30	60	47.7	43090	PASS
95	95	100	100	100.0	90253	PASS
96	95	5	9	7.1	6449	PASS
173	174	0.00	2	1.0	831	PASS
174	95	50	100	89.6	80832	PASS
175	174	5	9	7.2	5845	PASS
176	174	95	101	96.6	78064	PASS
177	176	5	9	6.3	4925	PASS