

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120721\
 Data File : VN069808.D
 Acq On : 7 Dec 2021 12:26
 Operator : JC/MD
 Sample : M4956-08 10X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RE137-20211204

Quant Time: Dec 08 04:33:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	1314353	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2323073	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2457640	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	958705	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	995661	49.06	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	98.12%		
35) Dibromofluoromethane	8.021	113	687748	47.26	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	94.52%		
50) Toluene-d8	10.440	98	3004657	51.42	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	102.84%		
62) 4-Bromofluorobenzene	12.731	95	1156984	54.66	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	109.32%		
Target Compounds						
					Qvalue	
9) 1,1,2-Trichlorotrifluo...	4.205	101	7200	0.55	ug/l #	6
11) Tert butyl alcohol	5.315	59	3748	0.98	ug/l #	71
12) 1,1-Dichloroethene	4.181	96	5467	0.44	ug/l	82
13) Acrolein	4.041	56	1167	0.36	ug/l #	80
16) Acetone	4.285	43	3328	0.27	ug/l #	83
18) Methyl Acetate	4.862	43	9156	0.25	ug/l #	85
25) 2-Butanone	7.340	43	5207	0.31	ug/l #	80
27) cis-1,2-Dichloroethene	7.327	96	5624	0.34	ug/l	62
29) Tetrahydrofuran	7.699	42	2329	0.23	ug/l #	82
31) Cyclohexane	8.080	56	34148	1.21	ug/l #	28
36) 1,1-Dichloropropene	8.083	75	112267	5.08	ug/l #	49
38) Carbon Tetrachloride	8.088	117	135927	6.27	ug/l #	16
44) Trichloroethene	9.217	130	1652148	102.40	ug/l	92
49) 1,4-Dioxane	9.569	88	848	2.08	ug/l #	78
51) 4-Methyl-2-Pentanone	10.336	43	8585	0.27	ug/l	94
53) t-1,3-Dichloropropene	10.714	75	333	2.81	ug/l #	43
54) cis-1,3-Dichloropropene	10.186	75	226	2.01	ug/l #	65
56) Ethyl methacrylate	10.768	69	1120	2.31	ug/l #	46
58) 2-Chloroethyl Vinyl ether	10.043	63	173	18.41	ug/l #	45
59) 2-Hexanone	11.087	43	18998	0.79	ug/l	86
60) Dibromochloromethane	11.237	129	206	2.39	ug/l	94
71) Bromoform	12.465	173	409	2.76	ug/l #	29
74) N-amyl acetate	12.390	43	11771	0.31	ug/l #	85
76) 1,2,3-Trichloropropane	12.731	75	656401	23.87	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	656401	75.85	ug/l #	5
89) n-Butylbenzene	13.946	91	14536	0.28	ug/l	96
92) 1,2-Dibromo-3-Chloropr...	14.608	75	1323	0.25	ug/l #	56
93) 1,2,4-Trichlorobenzene	15.263	180	9117	3.42	ug/l	94
95) Naphthalene	15.504	128	38615	4.74	ug/l #	92
96) 1,2,3-Trichlorobenzene	15.697	180	11711	3.16	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Dec 08 04:33:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 03 08:46:47 2021
Response via : Initial Calibration







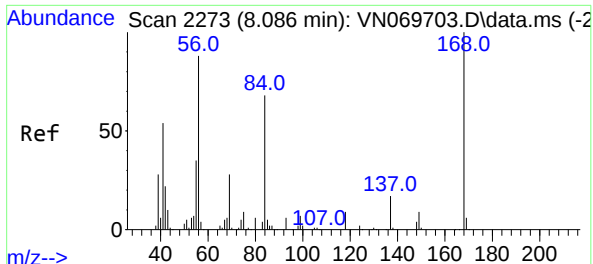

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion:168 Resp: 1314353
Ion Ratio Lower Upper
168 100
99 59.0 41.3 61.9

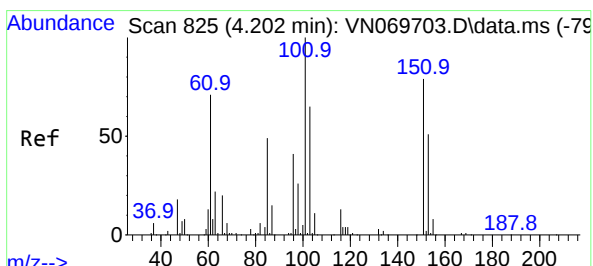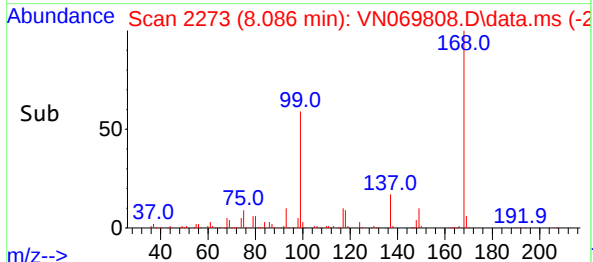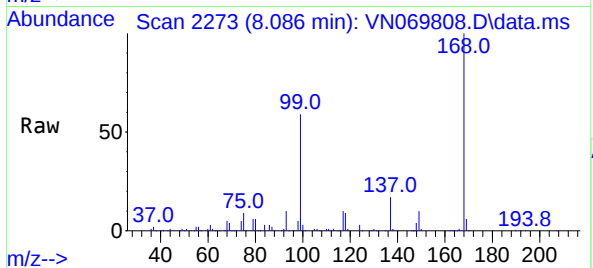

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.55 ug/l
RT: 4.205 min Scan# 826
Delta R.T. 0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion:101 Resp: 7200
Ion Ratio Lower Upper
101 100
85 102.7 37.2 55.8#
151 170.9 65.9 98.9#


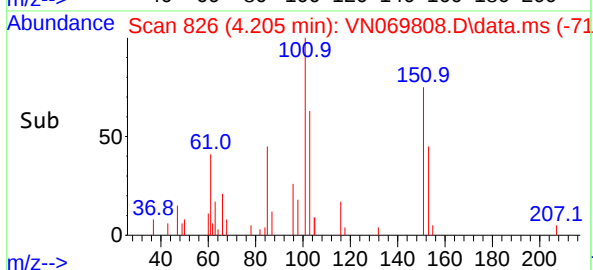

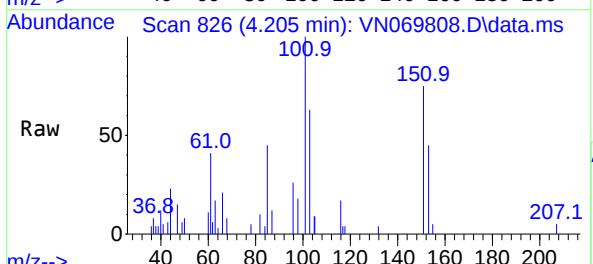




#11
Tert butyl alcohol
Concen: 0.98 ug/l
RT: 5.315 min Scan# 11
Delta R.T. -0.075 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 59 Resp: 3748
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

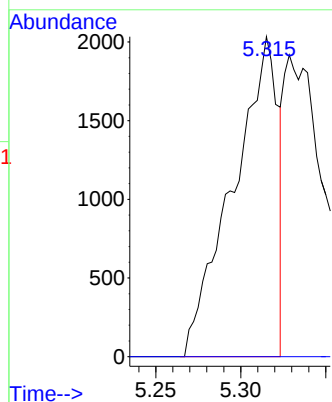

#12
1,1-Dichloroethene
Concen: 0.44 ug/l
RT: 4.181 min Scan# 817
Delta R.T. 0.005 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 96 Resp: 5467
Ion Ratio Lower Upper
96 100
61 136.3 131.0 196.6
98 54.9 52.4 78.6


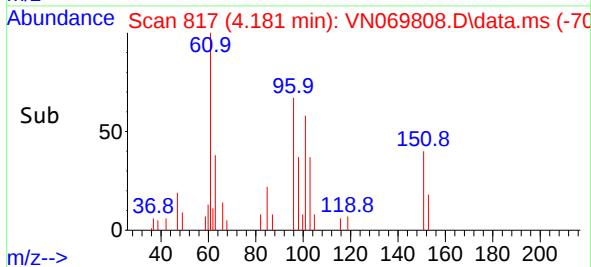

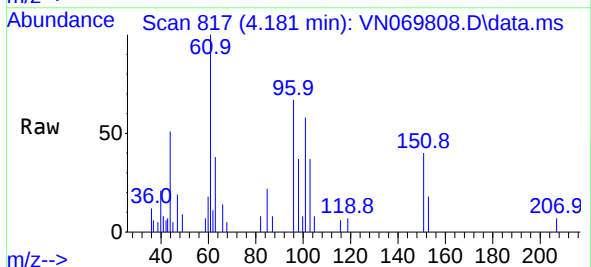




#13
Acrolein
Concen: 0.36 ug/l
RT: 4.041 min Scan# 764
Delta R.T. 0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 56 Resp: 1167
Ion Ratio Lower Upper
56 100
55 87.2 56.6 85.0#

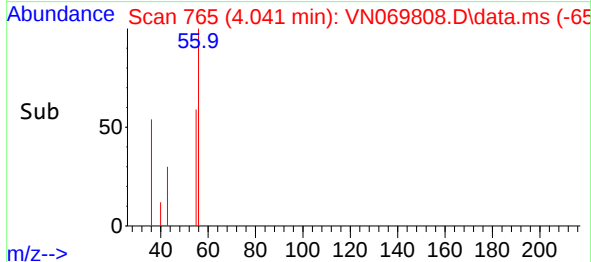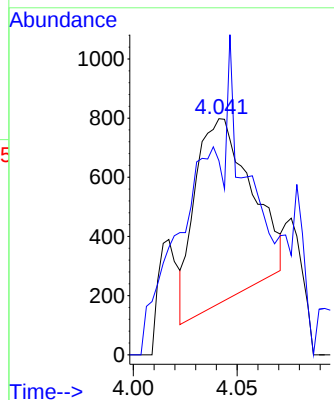

#16
Acetone
Concen: 0.27 ug/l
RT: 4.285 min Scan# 856
Delta R.T. -0.005 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 43 Resp: 3328
Ion Ratio Lower Upper
43 100
58 20.0 23.1 34.7#


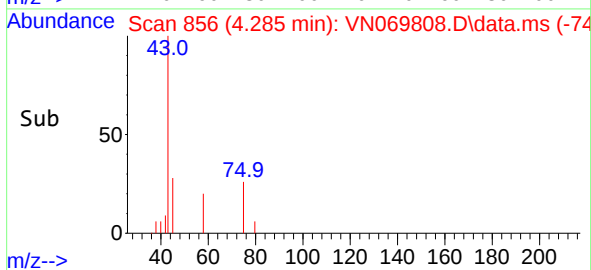
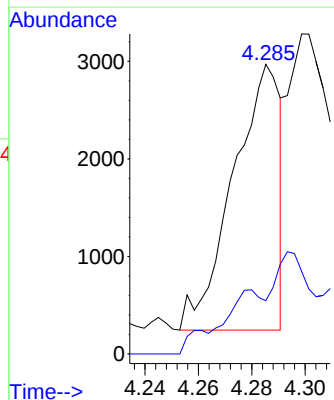



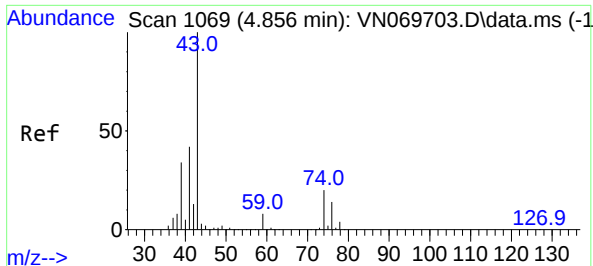

#18
Methyl Acetate
Concen: 0.25 ug/l
RT: 4.862 min Scan# 1069
Delta R.T. 0.005 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 43 Resp: 9156
Ion Ratio Lower Upper
43 100
74 16.7 19.4 29.2#

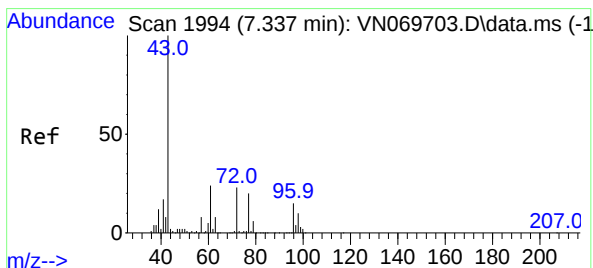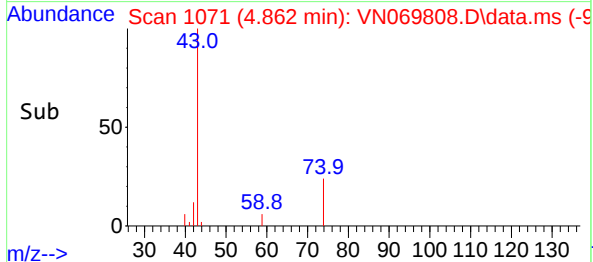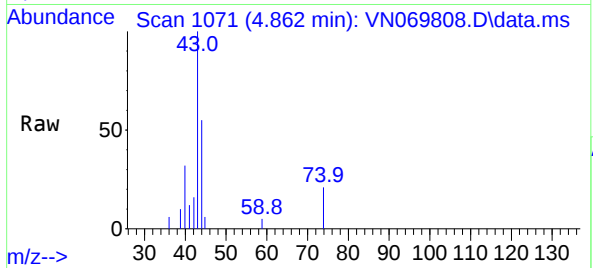

#25
2-Butanone
Concen: 0.31 ug/l
RT: 7.340 min Scan# 1995
Delta R.T. 0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 43 Resp: 5207
Ion Ratio Lower Upper
43 100
72 16.5 21.7 32.5#


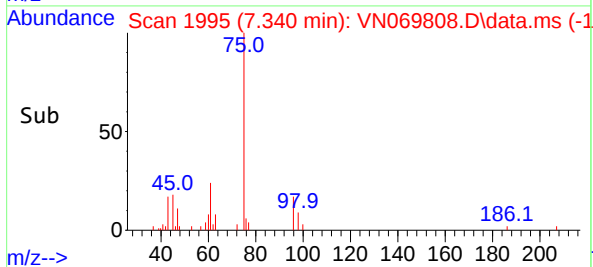

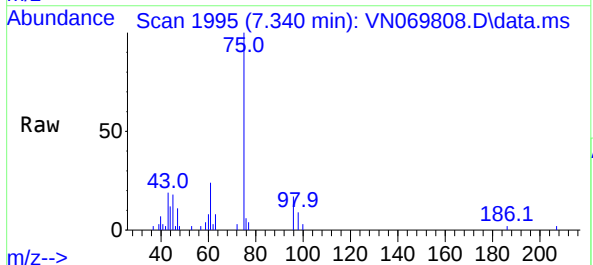


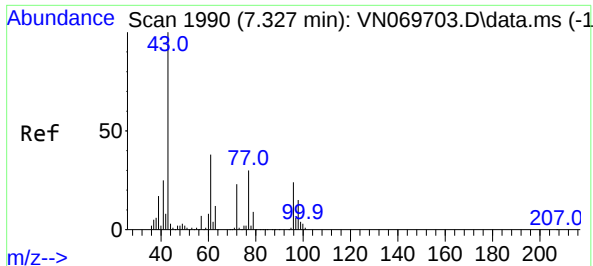

#27
cis-1,2-Dichloroethene
Concen: 0.34 ug/l
RT: 7.327 min Scan# 1990
Delta R.T. 0.000 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion:	96	Resp:	5624
Ion	Ratio	Lower	Upper
96	100		
61	178.3	0.0	275.0
98	28.1	0.0	129.6

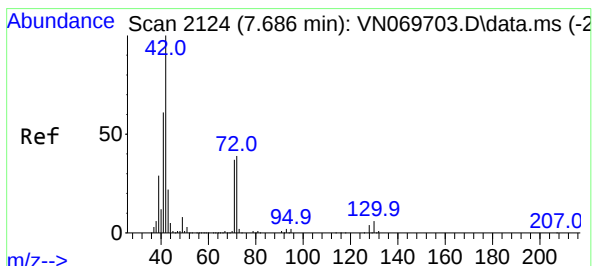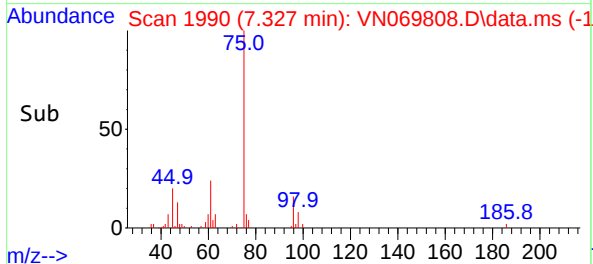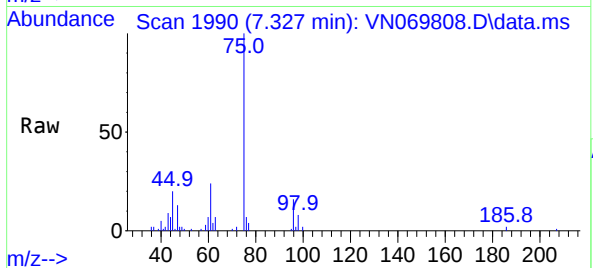

#29
Tetrahydrofuran
Concen: 0.23 ug/l
RT: 7.699 min Scan# 2129
Delta R.T. 0.013 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26


Tgt Ion:	42	Resp:	2329
Ion	Ratio	Lower	Upper
42	100		
72	36.8	36.3	54.5
71	28.6	34.7	52.1

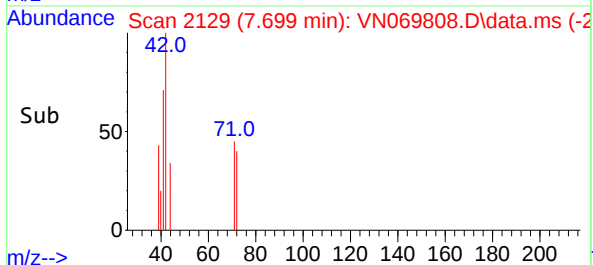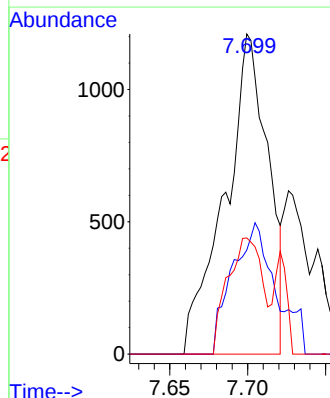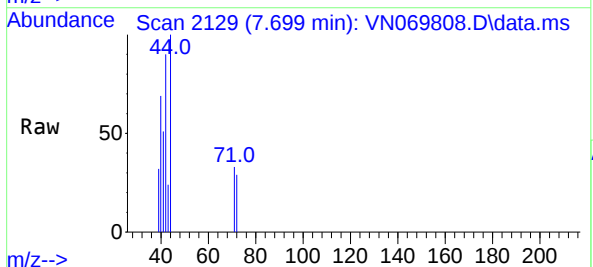






#31
Cyclohexane
Concen: 1.21 ug/l
RT: 8.080 min Scan# 21
Delta R.T. -0.013 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204







Tgt Ion: 56 Resp: 34148
Ion Ratio Lower Upper
56 100
69 146.6 27.1 40.7#
84 116.5 73.4 110.0#



#33
1,2-Dichloroethane-d4
Concen: 49.06 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. 0.000 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 65 Resp: 995661
Ion Ratio Lower Upper
65 100
67 50.8 0.0 103.0

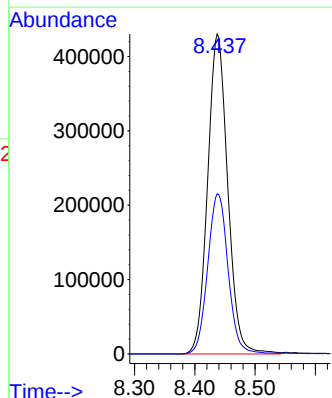



#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.968 min Scan# 2

Delta R.T. -0.000 min

Lab File: VN069808.D

Acq: 7 Dec 2021 12:26

Instrument :

MSVOA_N

ClientSampleId :

RE137-20211204





Tgt Ion:114 Resp: 2323073

Ion Ratio Lower Upper

114 100

63 23.9 0.0 37.8

88 16.0 0.0 27.4

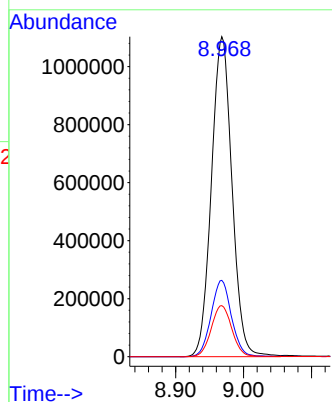

#35

Dibromofluoromethane

Concen: 47.26 ug/l

RT: 8.021 min Scan# 2249

Delta R.T. -0.003 min

Lab File: VN069808.D

Acq: 7 Dec 2021 12:26




Tgt Ion:113 Resp: 687748


Ion Ratio Lower Upper

113 100

111 103.6 82.2 123.2

192 18.7 16.9 25.3


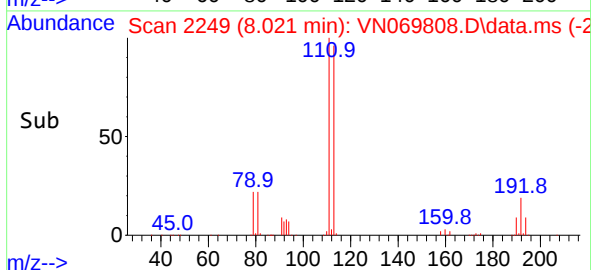






#36
1,1-Dichloropropene
Concen: 5.08 ug/l
RT: 8.083 min Scan# 211
Delta R.T. -0.139 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 75 Resp: 112267
Ion Ratio Lower Upper
75 100
110 9.1 18.4 55.2#
77 0.0 24.4 36.6#



#38
Carbon Tetrachloride
Concen: 6.27 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 117 Resp: 135927
Ion Ratio Lower Upper
117 100
119 5.1 76.1 114.1#
121 0.0 24.2 36.2#


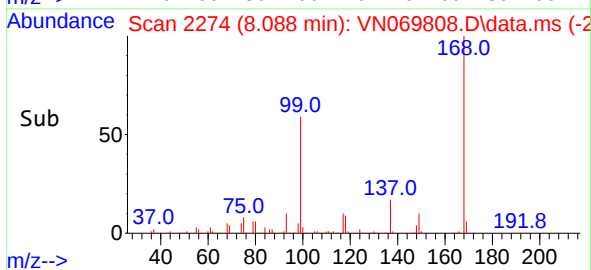






#44
Trichloroethene
Concen: 102.40 ug/l
RT: 9.217 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion:130 Resp: 1652148
Ion Ratio Lower Upper
130 100
95 103.6 0.0 191.2

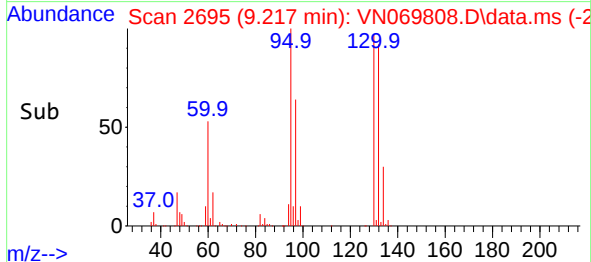

#49
1,4-Dioxane
Concen: 2.08 ug/l
RT: 9.569 min Scan# 2826
Delta R.T. -0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 88 Resp: 848
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 58.3 50.6 75.8


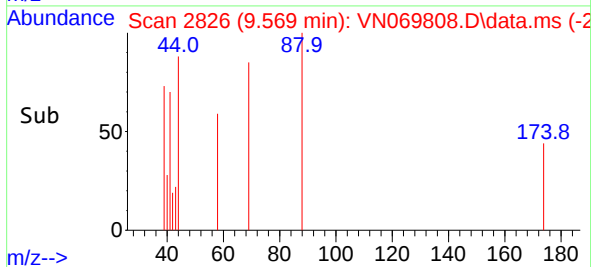

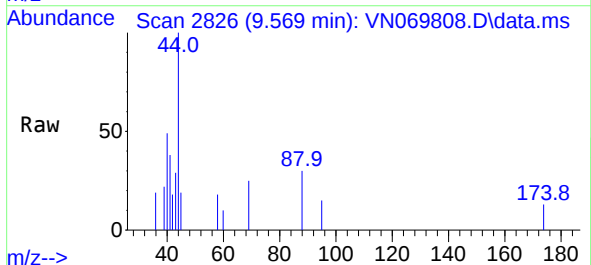


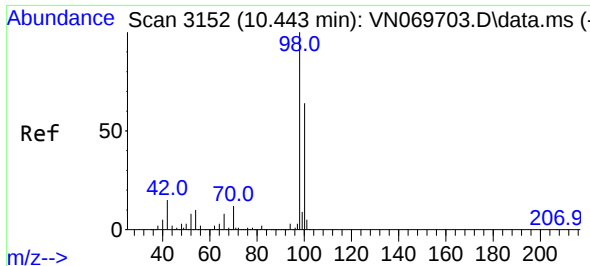

#50
Toluene-d8
Concen: 51.42 ug/l
RT: 10.440 min Scan# 3152
Delta R.T. -0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 98 Resp: 3004657
Ion Ratio Lower Upper
98 100
100 63.6 50.4 75.6

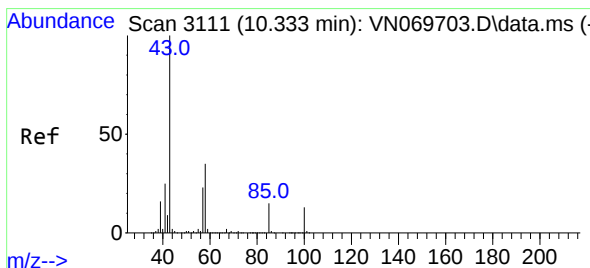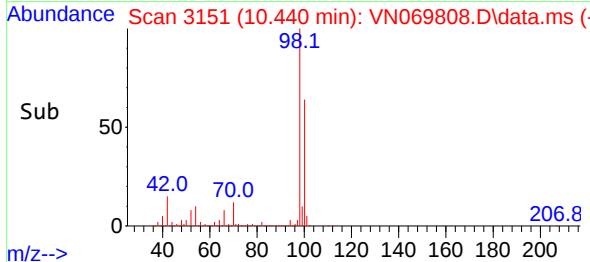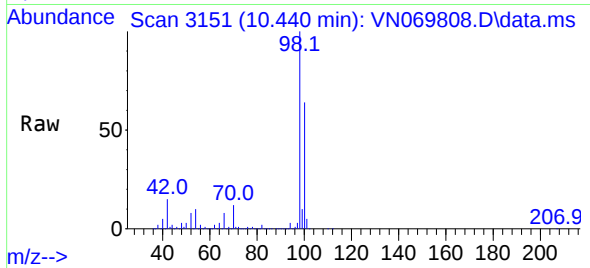

#51
4-Methyl-2-Pentanone
Concen: 0.27 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 43 Resp: 8585
Ion Ratio Lower Upper
43 100
58 41.7 30.4 45.6


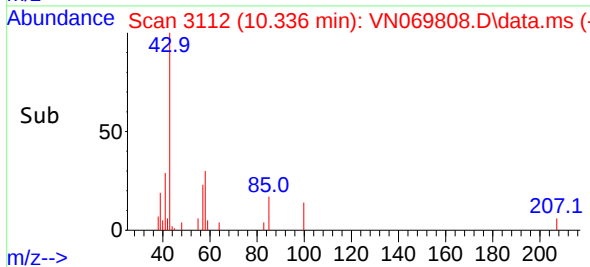

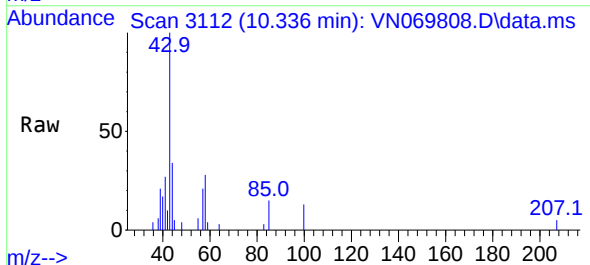


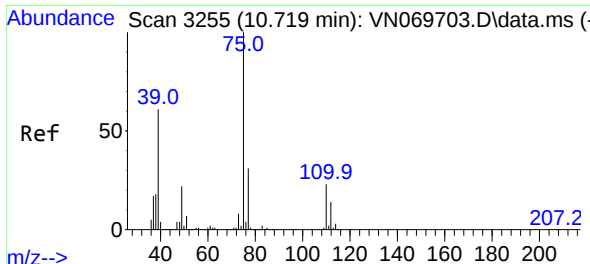

#53
t-1,3-Dichloropropene
Concen: 2.81 ug/l
RT: 10.714 min Scan# 31
Delta R.T. -0.005 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 75 Resp: 333
Ion Ratio Lower Upper
75 100
77 0.0 25.6 38.4#

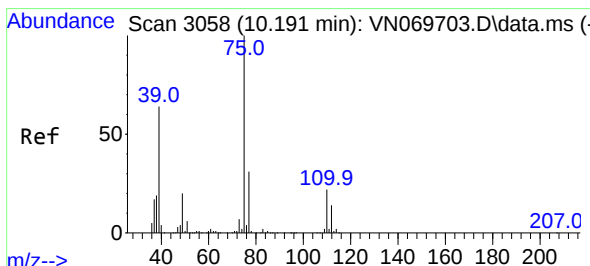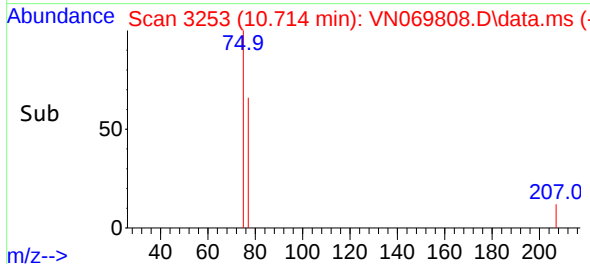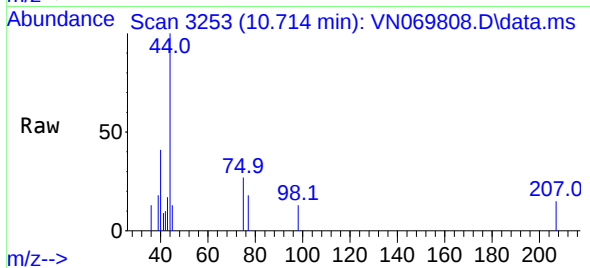

#54
cis-1,3-Dichloropropene
Concen: 2.01 ug/l
RT: 10.186 min Scan# 3056
Delta R.T. -0.005 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 75 Resp: 226
Ion Ratio Lower Upper
75 100
77 0.0 26.4 39.6#
39 38.1 42.5 63.7#


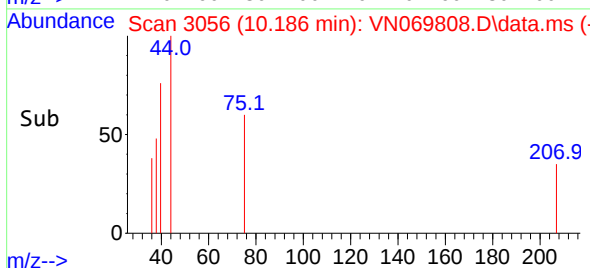
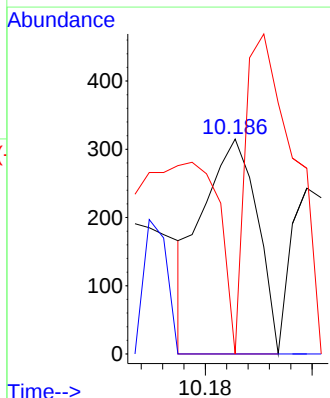
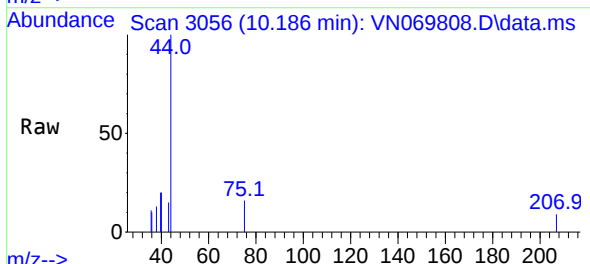




#56
Ethyl methacrylate
Concen: 2.31 ug/l
RT: 10.768 min Scan# 311
Delta R.T. 0.006 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 69 Resp: 1120
Ion Ratio Lower Upper
69 100
41 118.0 51.4 77.0#
39 63.7 34.6 52.0#

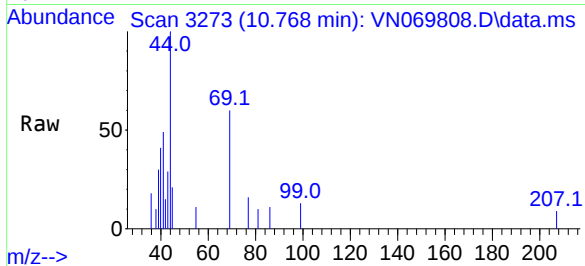

#58
2-Chloroethyl Vinyl ether
Concen: 18.41 ug/l
RT: 10.043 min Scan# 3003
Delta R.T. 0.000 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 63 Resp: 173
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#


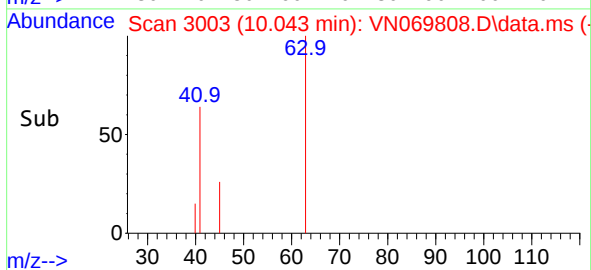

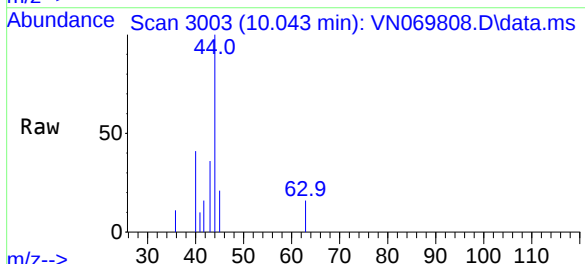




#59
2-Hexanone
Concen: 0.79 ug/l
RT: 11.087 min Scan# 31
Delta R.T. -0.000 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 43 Resp: 18998
Ion Ratio Lower Upper
43 100
58 44.1 26.9 80.7

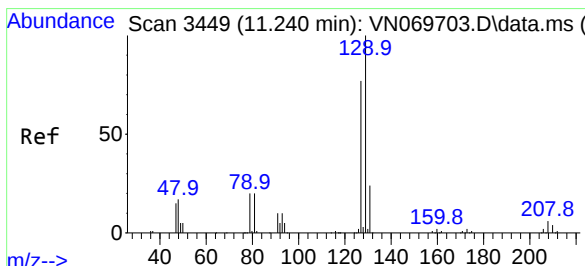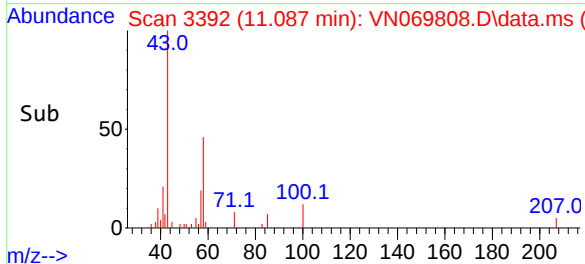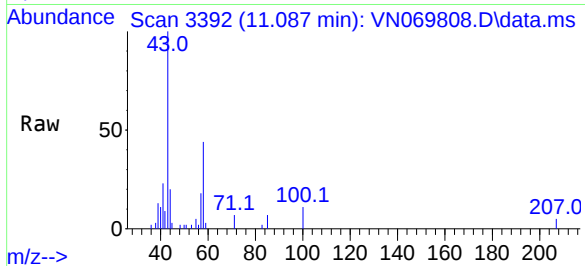

#60
Dibromochloromethane
Concen: 2.39 ug/l
RT: 11.237 min Scan# 3448
Delta R.T. -0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 129 Resp: 206
Ion Ratio Lower Upper
129 100
127 72.3 38.6 116.0


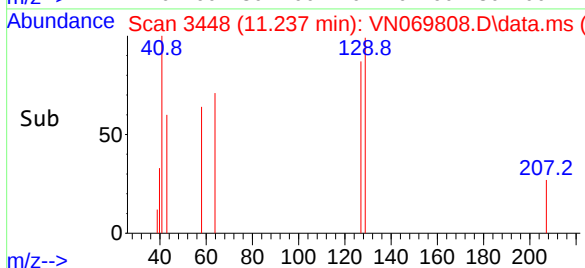
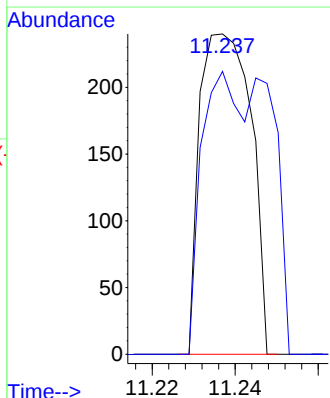
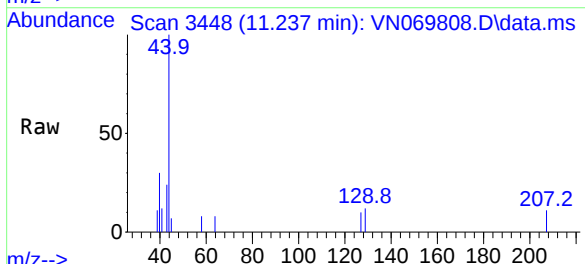




#62
4-Bromofluorobenzene
Concen: 54.66 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 95 Resp: 1156984
Ion Ratio Lower Upper
95 100
174 76.1 0.0 187.2
176 73.6 0.0 181.4

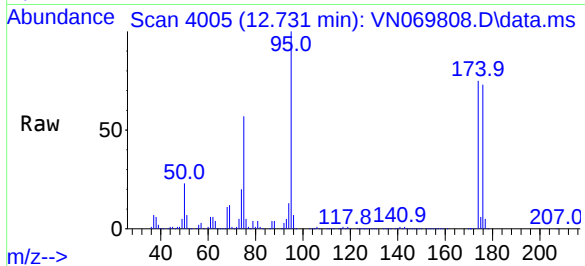

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.002 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 117 Resp: 2457640
Ion Ratio Lower Upper
117 100
82 59.4 42.4 63.6
119 32.2 25.4 38.2



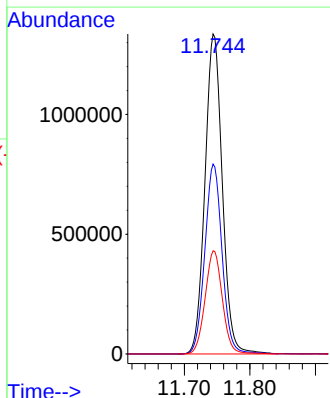
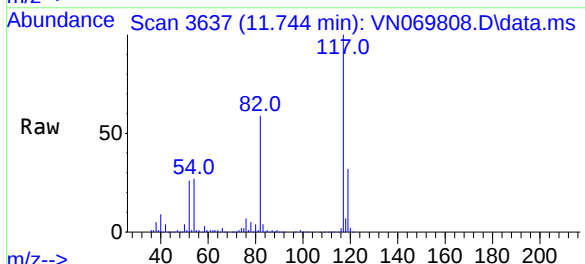


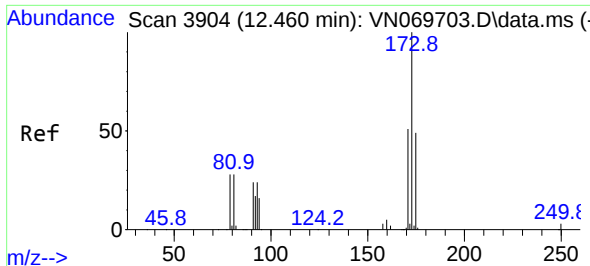

#71
Bromoform
Concen: 2.76 ug/l
RT: 12.465 min Scan# 3904
Delta R.T. 0.005 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion:173 Resp: 409
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0

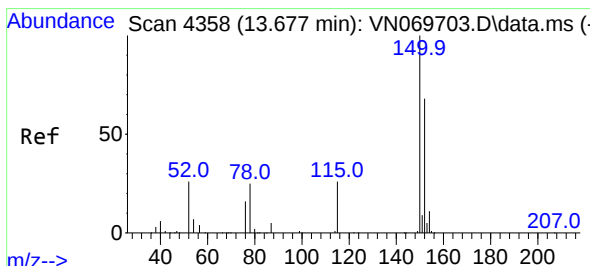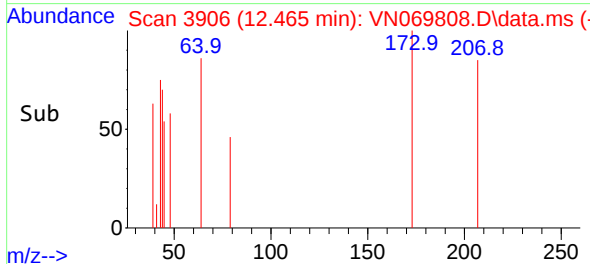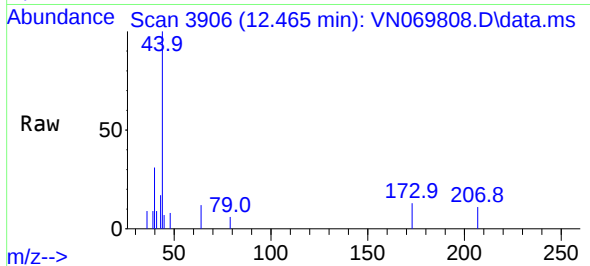

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion:152 Resp: 958705
Ion Ratio Lower Upper
152 100
115 60.0 27.5 82.5
150 157.0 0.0 344.4


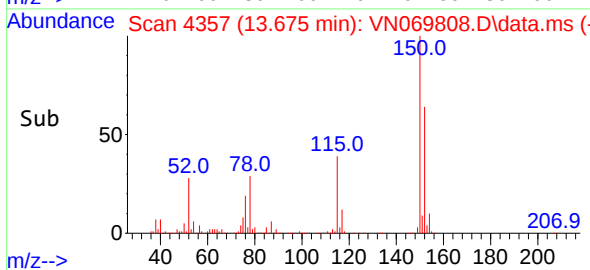

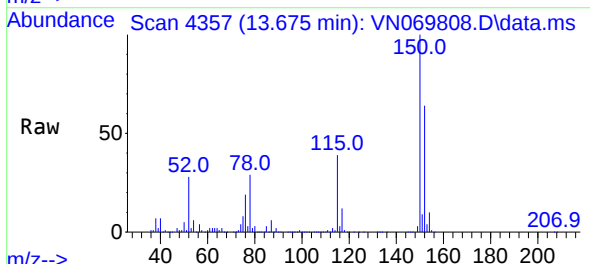




#74
N-amy1 acetate
Concen: 0.31 ug/l
RT: 12.390 min Scan# 31
Delta R.T. 0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion:	43	Resp:	11771
Ion	Ratio	Lower	Upper
43	100		
70	31.1	33.4	50.0#
55	15.9	19.3	28.9#
61	17.8	18.5	27.7#

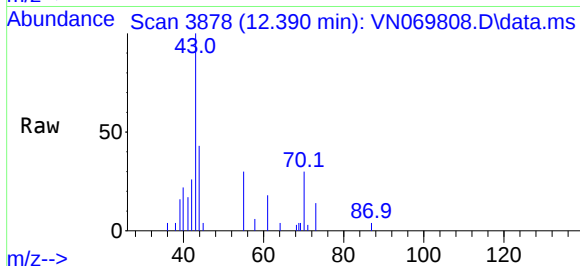

#76
1,2,3-Trichloropropane
Concen: 23.87 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.150 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion:	75	Resp:	656401
Ion	Ratio	Lower	Upper
75	100		
77	1.1	82.6	247.8#







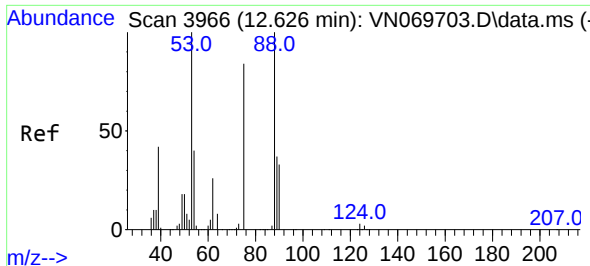

#81
trans-1,4-Dichloro-2-butene
Concen: 75.85 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 75 Resp: 656401
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

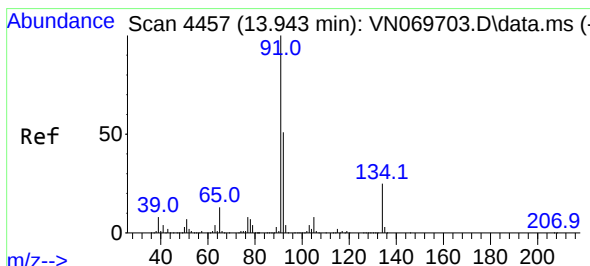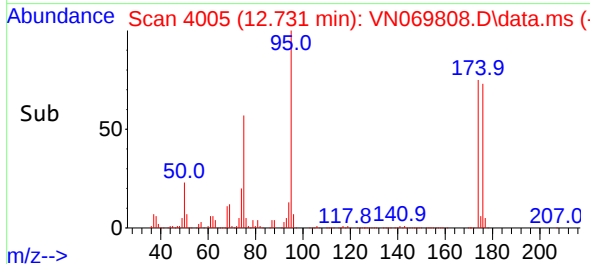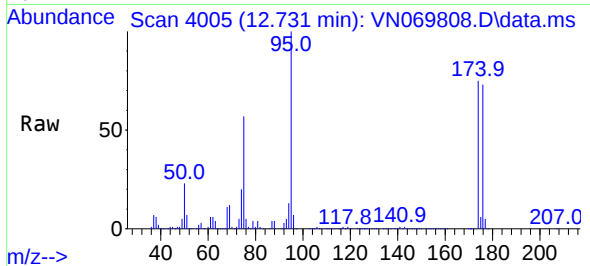

#89
n-Butylbenzene
Concen: 0.28 ug/l
RT: 13.946 min Scan# 4458
Delta R.T. 0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 91 Resp: 14536
Ion Ratio Lower Upper
91 100
92 49.3 25.4 76.0
134 22.7 13.6 40.8


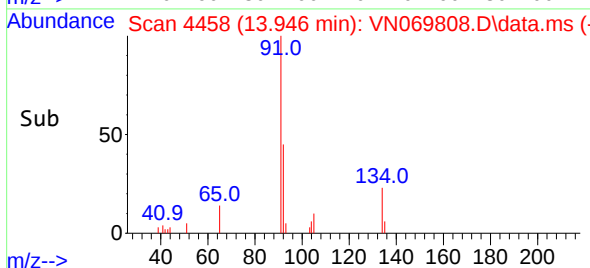
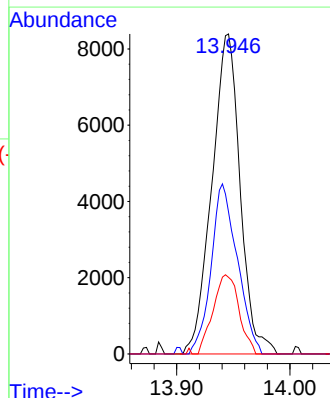
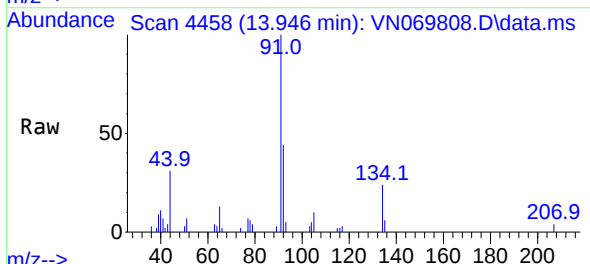




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.25 ug/l
RT: 14.608 min Scan# 41
Delta R.T. 0.005 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26




Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204


Tgt Ion: 75 Resp: 1323
Ion Ratio Lower Upper
75 100
155 44.2 46.9 140.7#
157 78.5 60.6 181.7

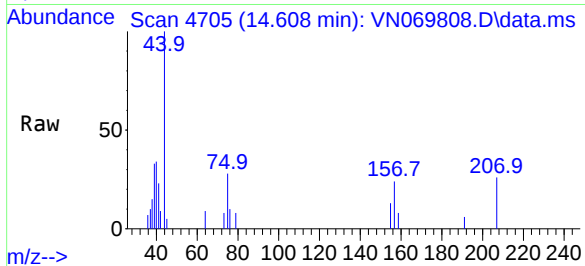

#93
1,2,4-Trichlorobenzene
Concen: 3.42 ug/l
RT: 15.263 min Scan# 4949
Delta R.T. -0.002 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion: 180 Resp: 9117
Ion Ratio Lower Upper
180 100
182 101.7 48.3 144.9
145 34.6 14.5 43.5


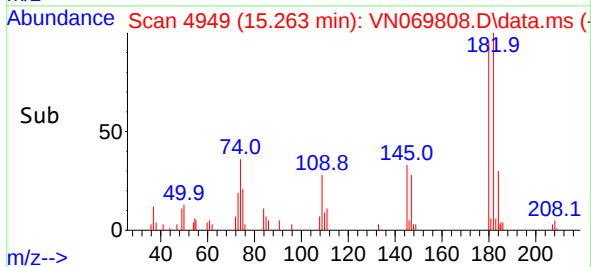

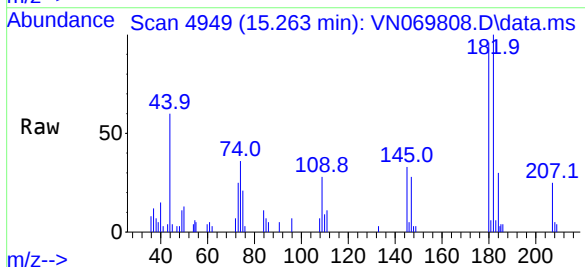




#95
Naphthalene
Concen: 4.74 ug/l
RT: 15.504 min Scan# 5040
Delta R.T. -0.003 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Instrument :
MSVOA_N
ClientSampleId :
RE137-20211204

Tgt Ion:	128	Resp:	38615
Ion Ratio	Lower	Upper	
128	100		
127	13.7	10.5	15.7
129	5.1	8.7	13.1#

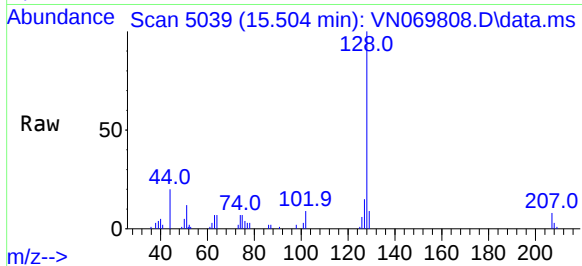

#96
1,2,3-Trichlorobenzene
Concen: 3.16 ug/l
RT: 15.697 min Scan# 5111
Delta R.T. -0.005 min
Lab File: VN069808.D
Acq: 7 Dec 2021 12:26

Tgt Ion:	180	Resp:	11711
Ion Ratio	Lower	Upper	
180	100		
182	93.9	47.4	142.2
145	32.9	15.0	45.1

