

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120721\
 Data File : VN069835.D
 Acq On : 8 Dec 2021 1:09
 Operator : JC/MD
 Sample : M4957-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW17811-20211206

Quant Time: Dec 08 06:36:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	1375278	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2462822	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2598359	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	968709	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	1052084	49.55	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	99.10%		
35) Dibromofluoromethane	8.024	113	724305	46.95	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	93.90%		
50) Toluene-d8	10.441	98	3141248	50.71	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	101.42%		
62) 4-Bromofluorobenzene	12.731	95	1205530	53.72	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	107.44%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.306	50	4026	0.20	ug/l	92
5) Bromomethane	2.885	94	4095	0.41	ug/l	98
11) Tert butyl alcohol	5.315	59	2893	0.72	ug/l #	71
12) 1,1-Dichloroethene	4.191	96	35461	2.71	ug/l	95
14) Allyl chloride	4.580	41	20892	0.71	ug/l #	74
16) Acetone	4.301	43	18199	1.42	ug/l	98
24) 1,1-Dichloroethane	6.391	63	29327	0.98	ug/l	97
27) cis-1,2-Dichloroethene	7.329	96	670745	39.02	ug/l	97
30) Chloroform	7.818	83	7876	0.26	ug/l	93
31) Cyclohexane	8.083	56	35433	1.20	ug/l #	24
36) 1,1-Dichloropropene	8.088	75	117938	5.03	ug/l #	49
38) Carbon Tetrachloride	8.086	117	142259	6.19	ug/l #	16
42) 1,2-Dichloroethane	8.528	62	10222	0.35	ug/l	90
44) Trichloroethene	9.215	130	6647913	388.66	ug/l	90
45) 1,2-Dichloropropane	9.491	63	405948	21.09	ug/l	99
48) Methyl methacrylate	9.491	41	282806	11.74	ug/l #	42
49) 1,4-Dioxane	9.574	88	910	2.10	ug/l #	80
53) t-1,3-Dichloropropene	10.725	75	412	2.81	ug/l #	74
54) cis-1,3-Dichloropropene	10.188	75	222	2.01	ug/l #	75
55) 1,1,2-Trichloroethane	10.894	97	7548	0.43	ug/l	97
56) Ethyl methacrylate	10.760	69	274	2.29	ug/l #	28
58) 2-Chloroethyl Vinyl ether	10.213	63	25	18.39	ug/l #	45
60) Dibromochloromethane	10.977	129	301924	17.58	ug/l #	11
64) Tetrachloroethene	10.977	164	317203	18.00	ug/l	95
71) Bromoform	12.709	173	473	2.76	ug/l #	29
76) 1,2,3-Trichloropropane	12.881	75	51869	1.87	ug/l #	3
81) trans-1,4-Dichloro-2-b...	12.731	75	671776	76.78	ug/l #	5
93) 1,2,4-Trichlorobenzene	15.268	180	2360	3.02	ug/l	98
95) Naphthalene	15.507	128	10675	4.19	ug/l #	91
96) 1,2,3-Trichlorobenzene	15.700	180	2720	2.60	ug/l	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120721\
Data File : VN069835.D
Acq On : 8 Dec 2021 1:09
Operator : JC/MD
Sample : M4957-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206

Quant Time: Dec 08 06:36:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 03 08:46:47 2021
Response via : Initial Calibration




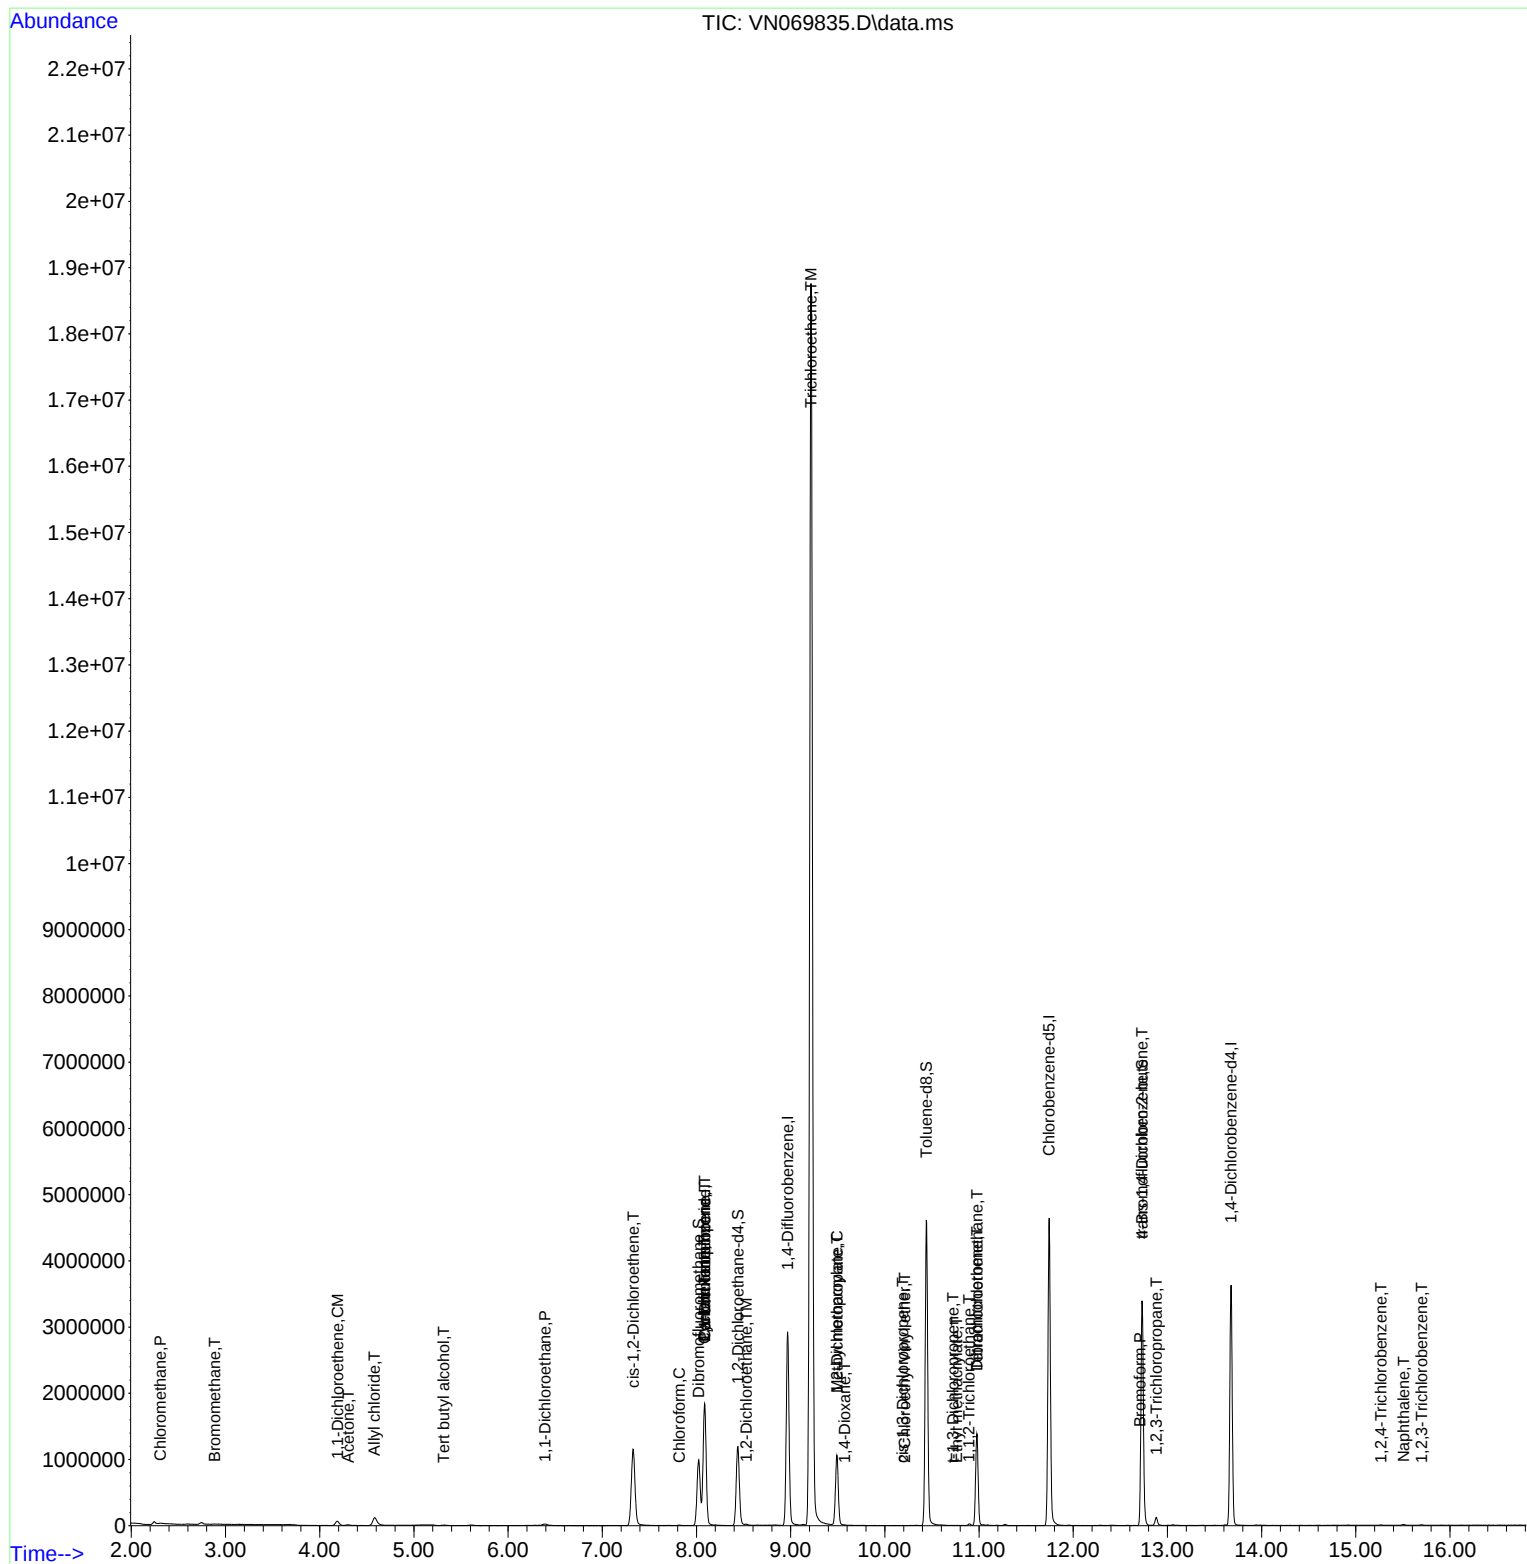


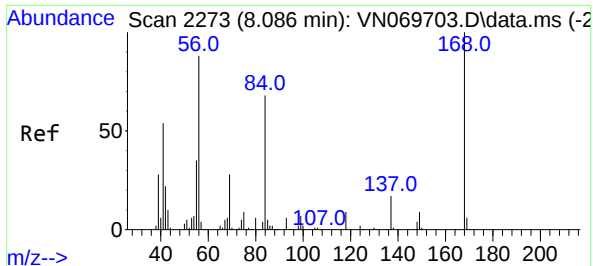

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09




Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206


Tgt Ion:168 Resp: 1375278
Ion Ratio Lower Upper
168 100
99 59.4 41.3 61.9

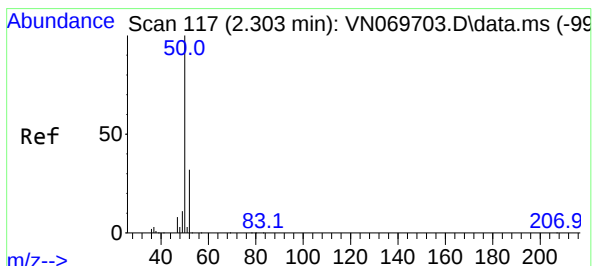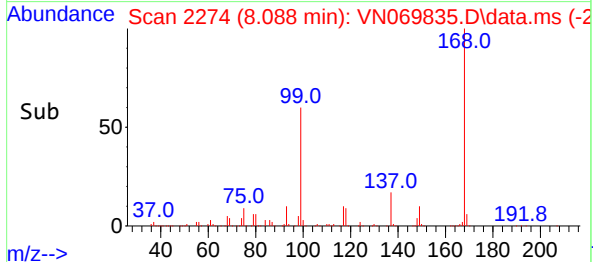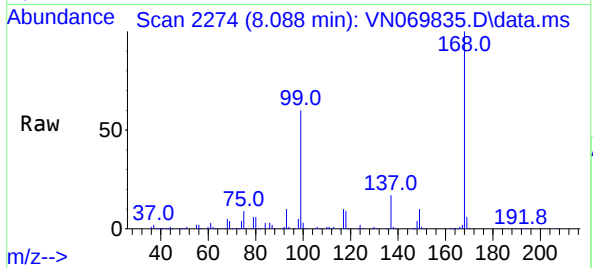

#3
Chloromethane
Concen: 0.20 ug/l
RT: 2.306 min Scan# 118
Delta R.T. 0.003 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Tgt Ion: 50 Resp: 4026
Ion Ratio Lower Upper
50 100
52 36.0 25.4 38.0


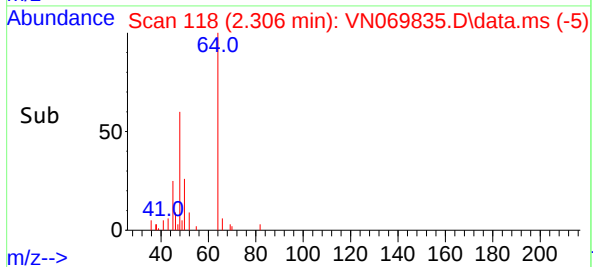

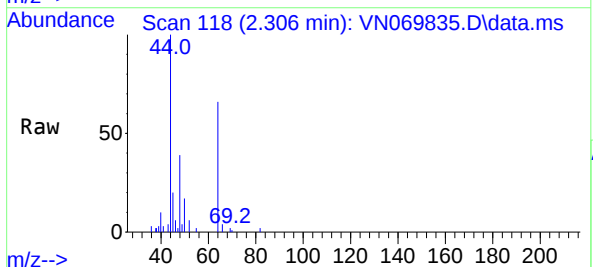




#5
Bromomethane
Concen: 0.41 ug/l
RT: 2.885 min Scan# 31
Delta R.T. 0.048 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09




Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206


Tgt Ion: 94 Resp: 4095
Ion Ratio Lower Upper
94 100
96 90.9 73.8 110.8



#11
Tert butyl alcohol
Concen: 0.72 ug/l
RT: 5.315 min Scan# 1240
Delta R.T. -0.075 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Tgt Ion: 59 Resp: 2893
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#









#12
1,1-Dichloroethene
Concen: 2.71 ug/l
RT: 4.191 min Scan# 815
Delta R.T. 0.016 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09




Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206


Tgt Ion: 96 Resp: 35461
Ion Ratio Lower Upper
96 100
61 156.9 131.0 196.6
98 62.5 52.4 78.6

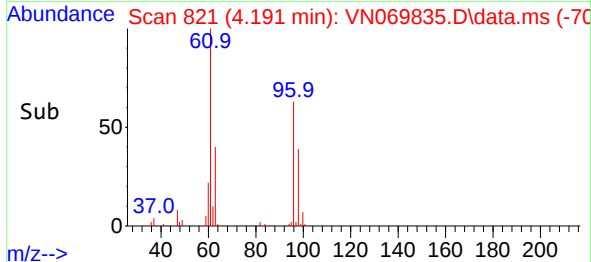

#14
Allyl chloride
Concen: 0.71 ug/l
RT: 4.580 min Scan# 966
Delta R.T. -0.257 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Tgt Ion: 41 Resp: 20892
Ion Ratio Lower Upper
41 100
39 86.9 61.2 91.8
76 0.0 26.0 39.0#


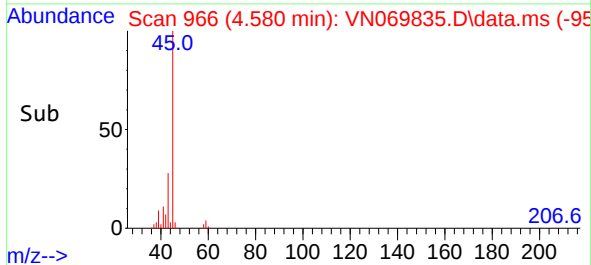

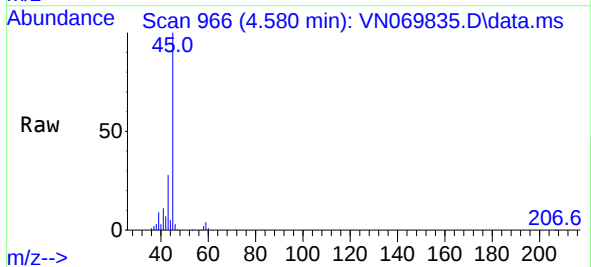




#16
Acetone
Concen: 1.42 ug/l
RT: 4.301 min Scan# 80
Delta R.T. 0.011 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09




Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206


Tgt Ion: 43 Resp: 18199
Ion Ratio Lower Upper
43 100
58 28.0 23.1 34.7

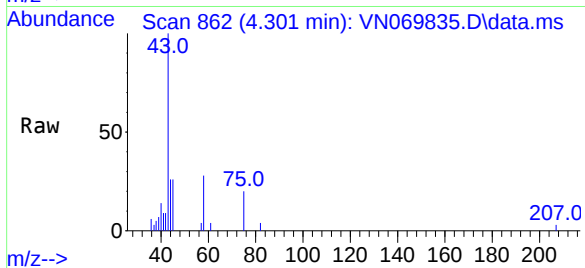

#24
1,1-Dichloroethane
Concen: 0.98 ug/l
RT: 6.391 min Scan# 1641
Delta R.T. 0.003 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09


Tgt Ion: 63 Resp: 29327
Ion Ratio Lower Upper
63 100
98 5.9 3.3 9.9
100 3.0 2.1 6.5

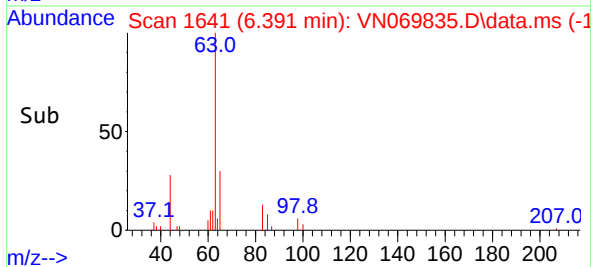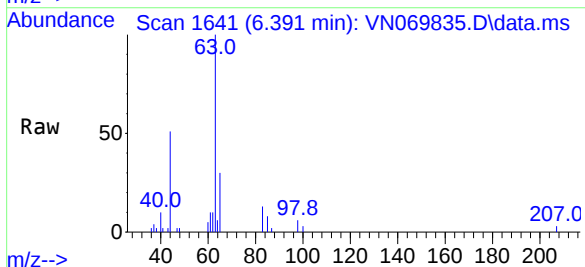



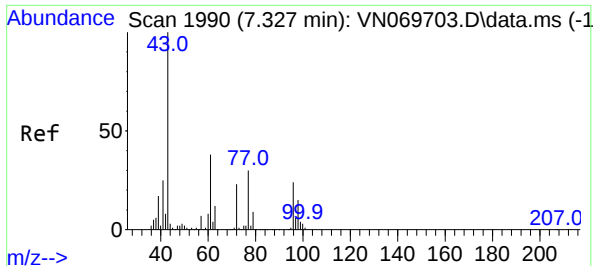


#27
cis-1,2-Dichloroethene
Concen: 39.02 ug/l
RT: 7.329 min Scan# 1990
Delta R.T. 0.003 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206



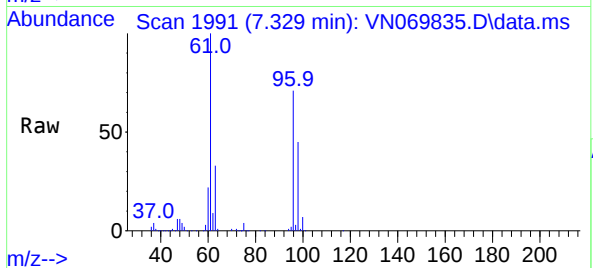



Tgt Ion: 96 Resp: 670745
Ion Ratio Lower Upper
96 100
61 142.3 0.0 275.0
98 63.3 0.0 129.6

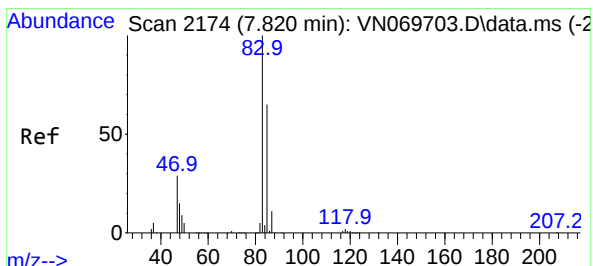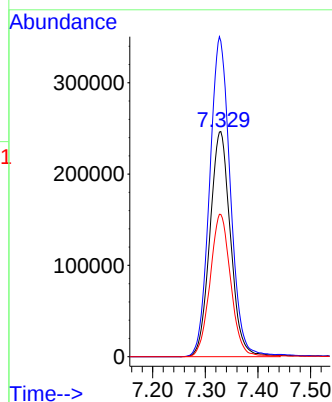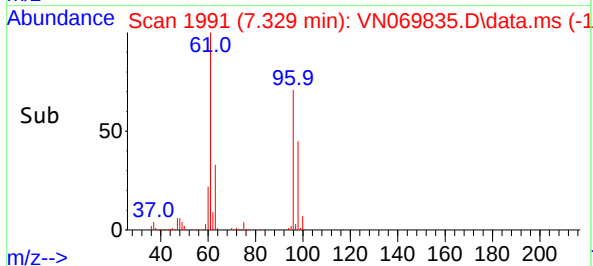

#30
Chloroform
Concen: 0.26 ug/l
RT: 7.818 min Scan# 2173
Delta R.T. -0.002 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09


Tgt Ion: 83 Resp: 7876
Ion Ratio Lower Upper
83 100
85 59.2 51.9 77.9

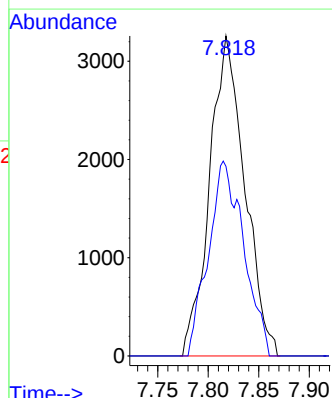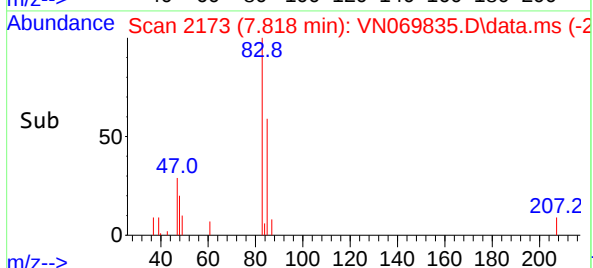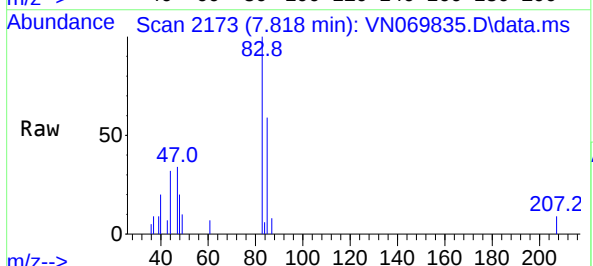






#31
Cyclohexane
Concen: 1.20 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.011 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206



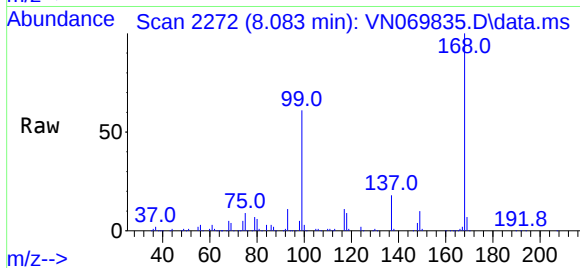



Tgt Ion: 56 Resp: 35433
Ion Ratio Lower Upper
56 100
69 152.1 27.1 40.7#
84 117.5 73.4 110.0#



#33
1,2-Dichloroethane-d4
Concen: 49.55 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.003 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09


Tgt Ion: 65 Resp: 1052084
Ion Ratio Lower Upper
65 100
67 51.1 0.0 103.0

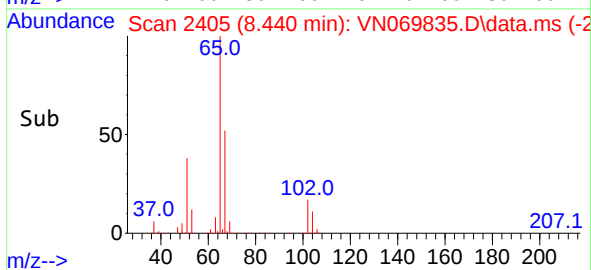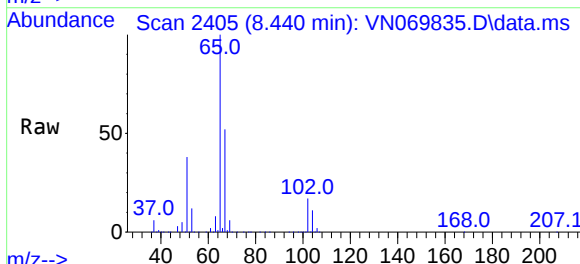






#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.968 min Scan# 2062
Delta R.T. 0.000 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206



Tgt Ion:114 Resp: 2462822




Ion	Ratio	Lower	Upper
114	100		
63	23.2	0.0	37.8
88	16.0	0.0	27.4




#35
Dibromofluoromethane
Concen: 46.95 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Tgt Ion:113 Resp: 724305

Ion	Ratio	Lower	Upper
113	100		
111	102.8	82.2	123.2
192	18.8	16.9	25.3


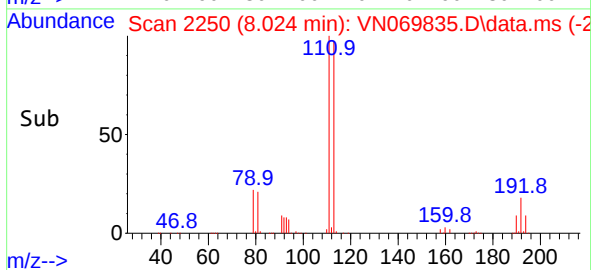






#36
1,1-Dichloropropene
Concen: 5.03 ug/l
RT: 8.088 min Scan# 211
Delta R.T. -0.134 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09




Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206


Tgt Ion: 75 Resp: 117938
Ion Ratio Lower Upper
75 100
110 8.4 18.4 55.2#
77 0.0 24.4 36.6#



#38
Carbon Tetrachloride
Concen: 6.19 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.120 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Tgt Ion: 117 Resp: 142259
Ion Ratio Lower Upper
117 100
119 4.8 76.1 114.1#
121 0.0 24.2 36.2#

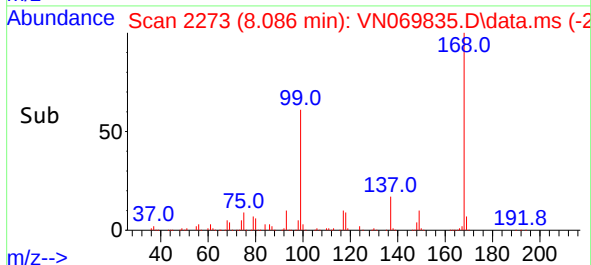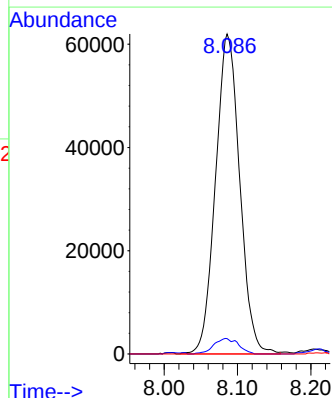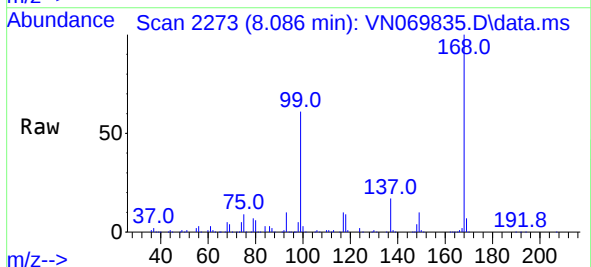



#42

1,2-Dichloroethane

Concen: 0.35 ug/l

RT: 8.528 min Scan# 2439

Delta R.T. -0.002 min

Lab File: VN069835.D

Acq: 8 Dec 2021 1:09

Instrument :

MSVOA_N

ClientSampleId :





MW17811-20211206

Tgt Ion: 62 Resp: 10222

Ion Ratio Lower Upper

62 100

98 5.3 0.0 17.6



#44

Trichloroethene

Concen: 388.66 ug/l

RT: 9.215 min Scan# 2694

Delta R.T. -0.002 min

Lab File: VN069835.D




Acq: 8 Dec 2021 1:09


Tgt Ion:130 Resp: 6647913

Ion Ratio Lower Upper

130 100

95 105.4 0.0 191.2

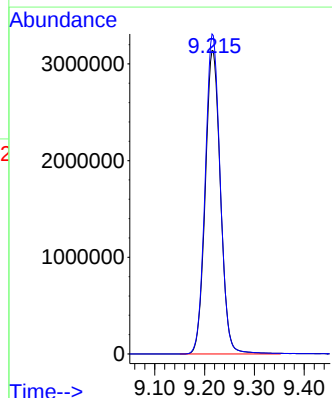



#45

1,2-Dichloropropane

Concen: 21.09 ug/l

RT: 9.491 min Scan# 2797

Delta R.T. 0.000 min

Lab File: VN069835.D

Acq: 8 Dec 2021 1:09

Instrument :

MSVOA_N

ClientSampleId :





MW17811-20211206

Tgt Ion: 63 Resp: 405948

Ion Ratio Lower Upper

63 100

65 30.5 24.7 37.1

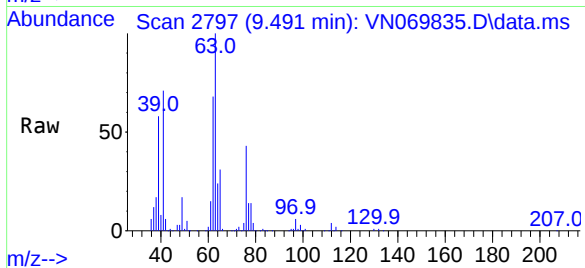

#48

Methyl methacrylate

Concen: 11.74 ug/l

RT: 9.491 min Scan# 2797

Delta R.T. -0.070 min

Lab File: VN069835.D

Acq: 8 Dec 2021 1:09




Tgt Ion: 41 Resp: 282806


Ion Ratio Lower Upper

41 100

69 0.0 72.4 108.6

39 82.1 58.4 87.6


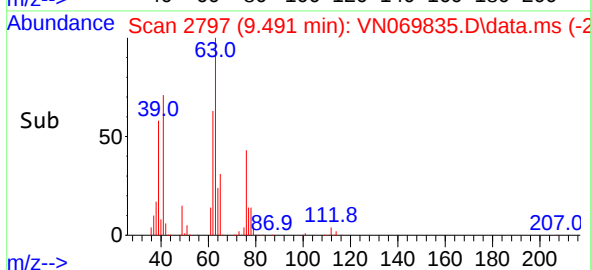

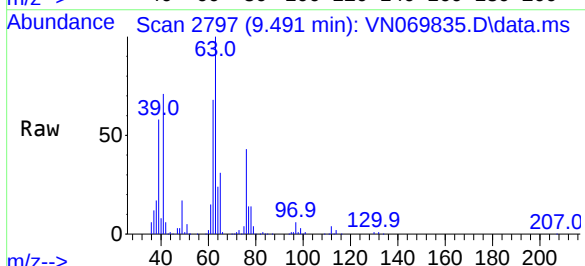


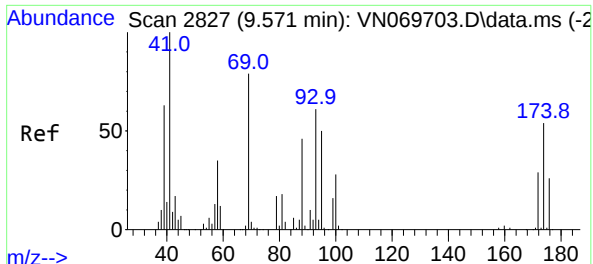

#49
1,4-Dioxane
Concen: 2.10 ug/l
RT: 9.574 min Scan# 21
Delta R.T. 0.003 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09




Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206


Tgt Ion: 88 Resp: 910
Ion Ratio Lower Upper
88 100
43 11.8 23.4 35.2#
58 52.1 50.6 75.8

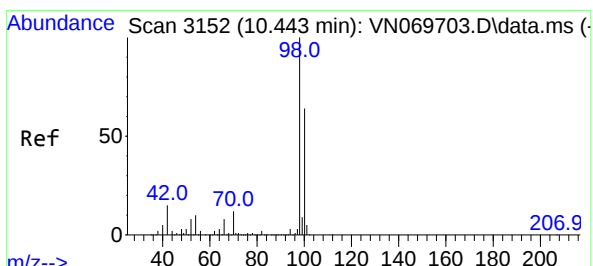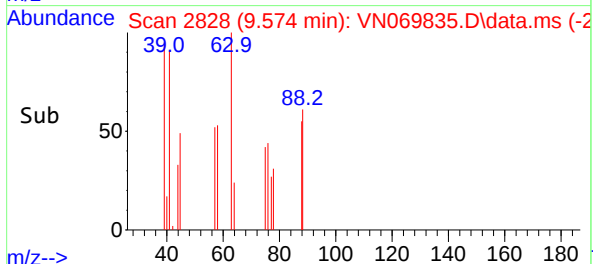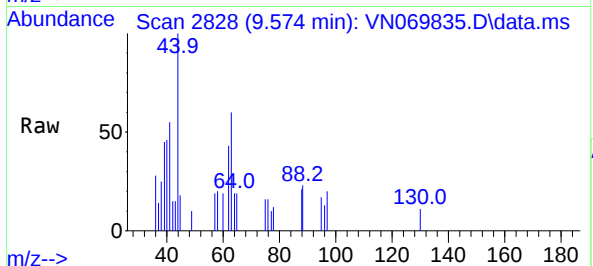

#50
Toluene-d8
Concen: 50.71 ug/l
RT: 10.441 min Scan# 3151
Delta R.T. -0.002 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Tgt Ion: 98 Resp: 3141248
Ion Ratio Lower Upper
98 100
100 64.4 50.4 75.6


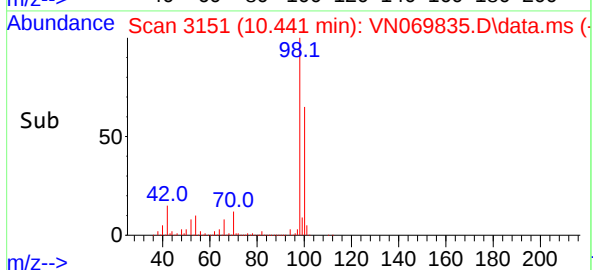

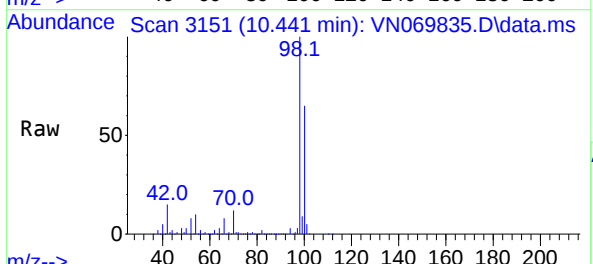




#53
t-1,3-Dichloropropene
Concen: 2.81 ug/l
RT: 10.725 min Scan# 31
Delta R.T. 0.006 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09




Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206


Tgt Ion: 75 Resp: 412
Ion Ratio Lower Upper
75 100
77 17.6 25.6 38.4#

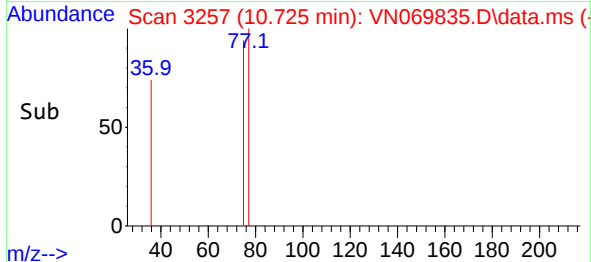

#54
cis-1,3-Dichloropropene
Concen: 2.01 ug/l
RT: 10.188 min Scan# 3057
Delta R.T. -0.003 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09


Tgt Ion: 75 Resp: 222
Ion Ratio Lower Upper
75 100
77 0.0 26.4 39.6#
39 50.6 42.5 63.7

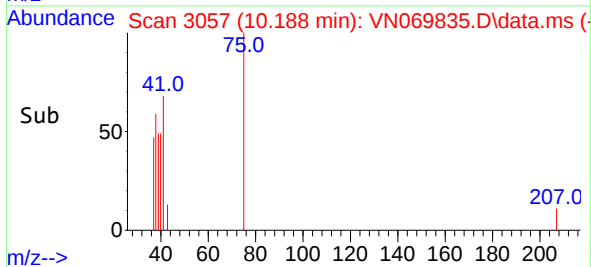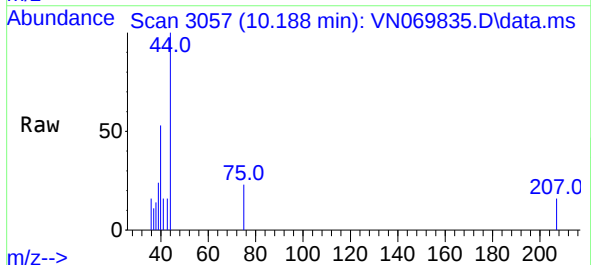






#55
1,1,2-Trichloroethane
Concen: 0.43 ug/l
RT: 10.894 min Scan# 31
Delta R.T. -0.005 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206



Tgt Ion: 97 Resp: 7548




Ion	Ratio	Lower	Upper
97	100		
83	81.8	67.8	101.6
85	57.0	45.4	68.2
99	65.9	49.4	74.0

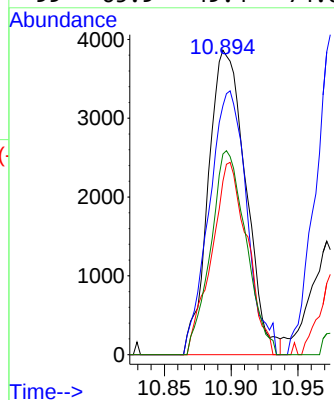


#56
Ethyl methacrylate
Concen: 2.29 ug/l
RT: 10.760 min Scan# 3270
Delta R.T. -0.002 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Tgt Ion: 69 Resp: 274

Ion	Ratio	Lower	Upper
69	100		
41	123.4	51.4	77.0#
39	0.0	34.6	52.0#


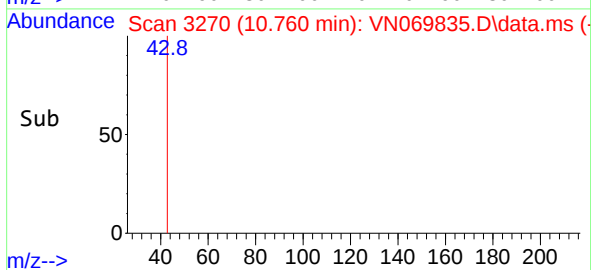
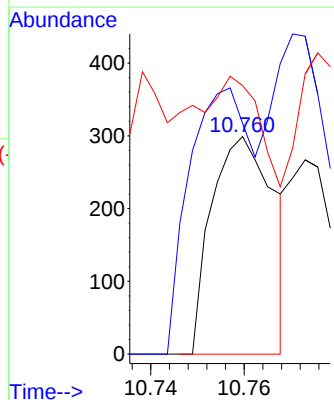





#58
2-Chloroethyl Vinyl ether
Concen: 18.39 ug/l
RT: 10.213 min Scan# 3003
Delta R.T. 0.170 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09




Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206


Tgt Ion: 63 Resp: 25
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#



#60
Dibromochloromethane
Concen: 17.58 ug/l
RT: 10.977 min Scan# 3351
Delta R.T. -0.263 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Tgt Ion: 129 Resp: 301924
Ion Ratio Lower Upper
129 100
127 0.1 38.6 116.0#



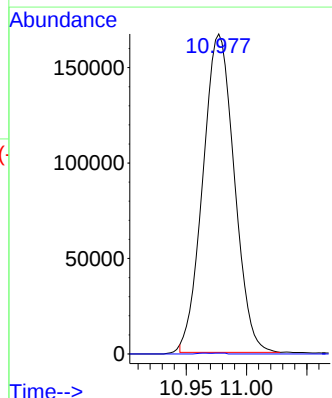





#62
4-Bromofluorobenzene
Concen: 53.72 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09




Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206


Tgt Ion: 95 Resp: 1205530
Ion Ratio Lower Upper
95 100
174 75.5 0.0 187.2
176 73.1 0.0 181.4

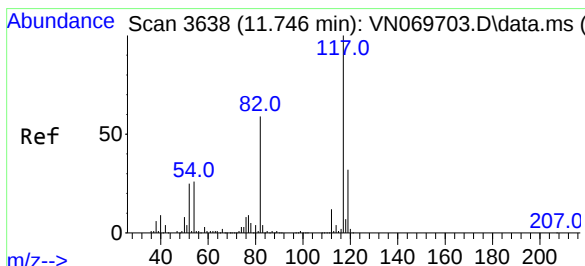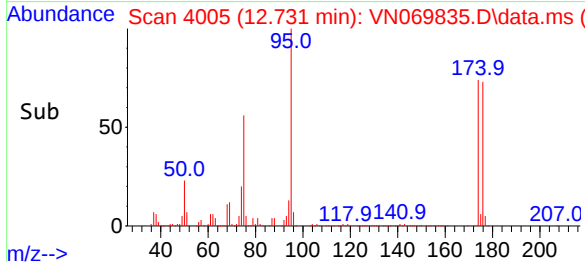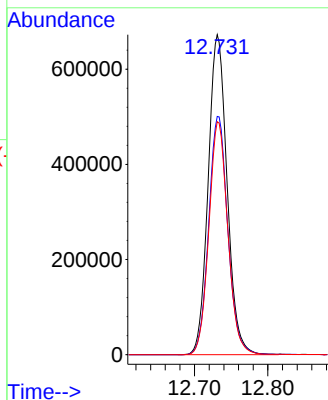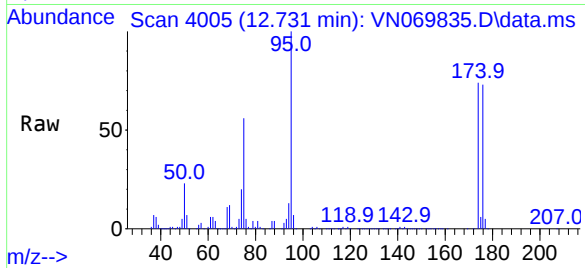

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.002 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09


Tgt Ion: 117 Resp: 2598359
Ion Ratio Lower Upper
117 100
82 59.2 42.4 63.6
119 32.1 25.4 38.2

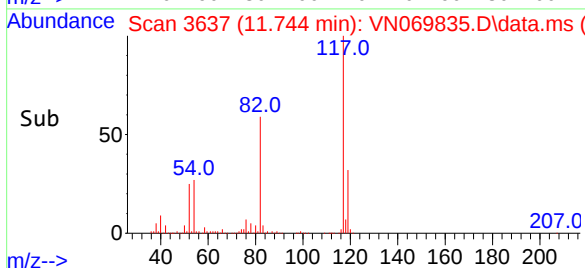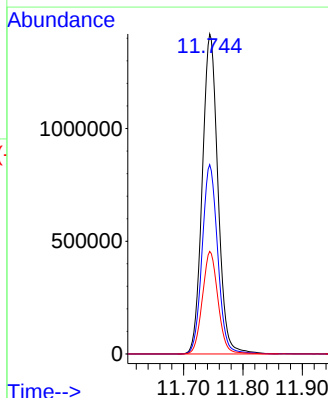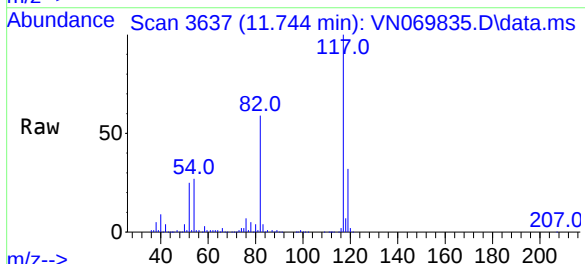






#64
Tetrachloroethene
Concen: 18.00 ug/l
RT: 10.977 min Scan# 31
Delta R.T. -0.002 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206



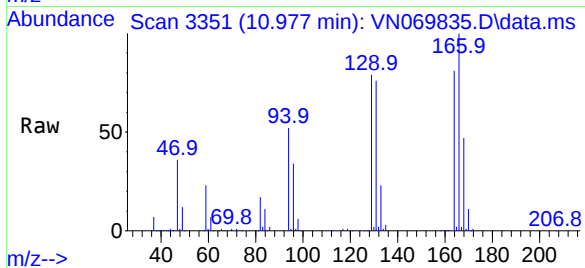



Tgt Ion:164 Resp: 317203
Ion Ratio Lower Upper
164 100
166 123.7 101.9 152.9
129 97.3 72.0 108.0
131 93.8 70.9 106.3

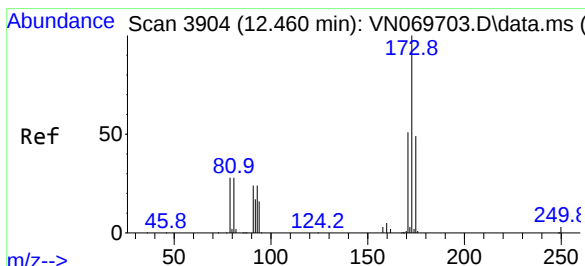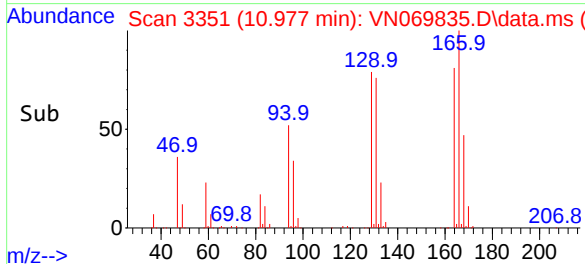

#71
Bromoform
Concen: 2.76 ug/l
RT: 12.709 min Scan# 3997
Delta R.T. 0.249 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09


Tgt Ion:173 Resp: 473
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0

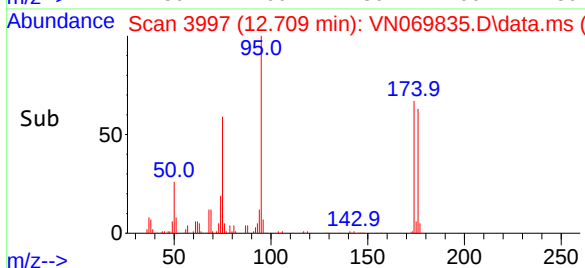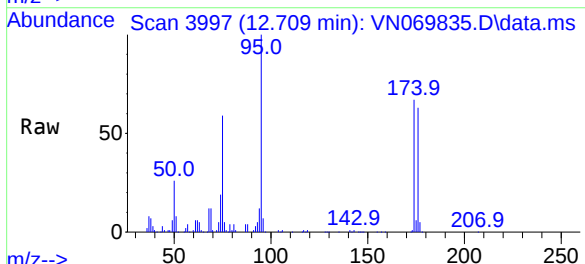






#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.675 min Scan# 41
Delta R.T. -0.002 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09


Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206

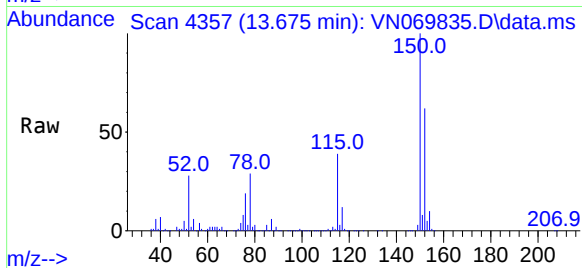



Tgt Ion:152 Resp: 968709
Ion Ratio Lower Upper
152 100
115 61.4 27.5 82.5
150 158.0 0.0 344.4




#76
1,2,3-Trichloropropane
Concen: 1.87 ug/l
RT: 12.881 min Scan# 4061
Delta R.T. 0.000 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

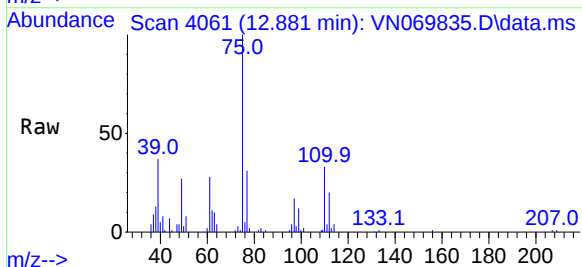

Tgt Ion: 75 Resp: 51869
Ion Ratio Lower Upper
75 100
77 34.4 82.6 247.8#



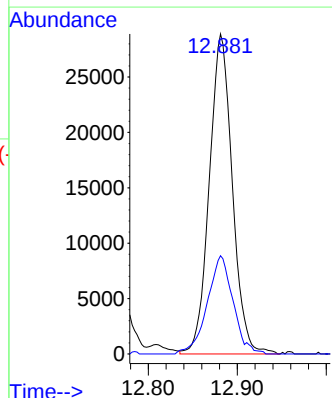
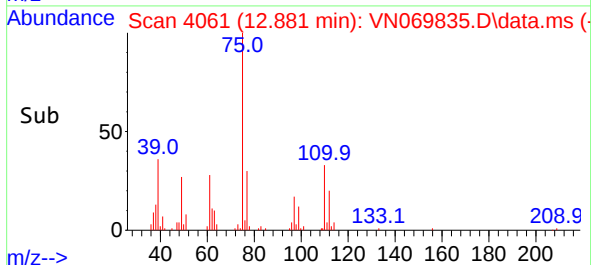




#81
trans-1,4-Dichloro-2-butene
Concen: 76.78 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09




Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206


Tgt Ion: 75 Resp: 671776
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#

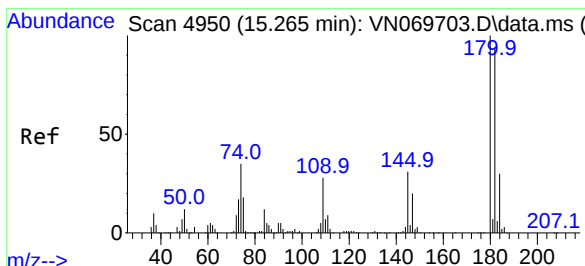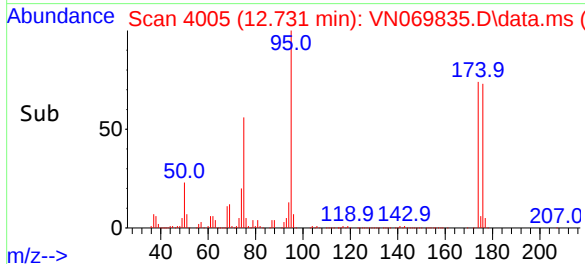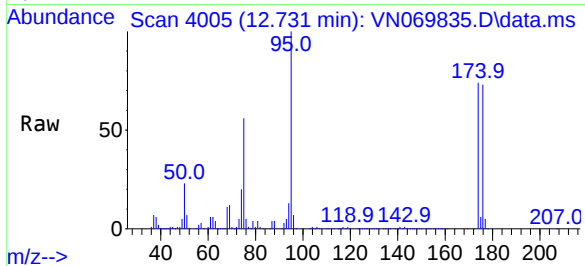

#93
1,2,4-Trichlorobenzene
Concen: 3.02 ug/l
RT: 15.268 min Scan# 4951
Delta R.T. 0.003 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Tgt Ion: 180 Resp: 2360
Ion Ratio Lower Upper
180 100
182 97.8 48.3 144.9
145 32.2 14.5 43.5


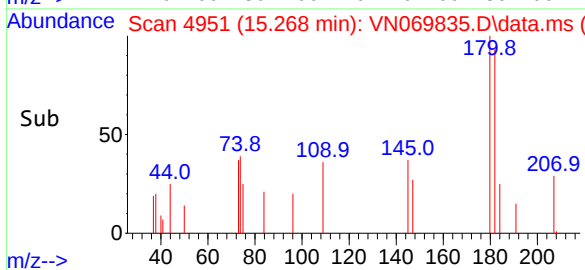

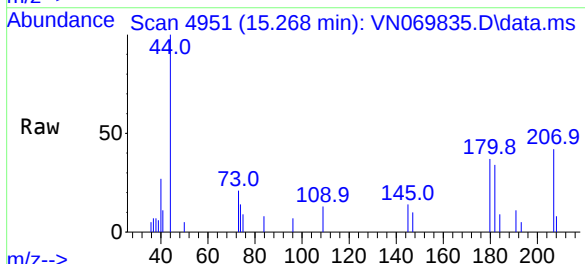




#95
Naphthalene
Concen: 4.19 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Instrument :
MSVOA_N
ClientSampleId :
MW17811-20211206

Tgt Ion:128 Resp: 10675
Ion Ratio Lower Upper
128 100
127 7.9 10.5 15.7#
129 12.6 8.7 13.1

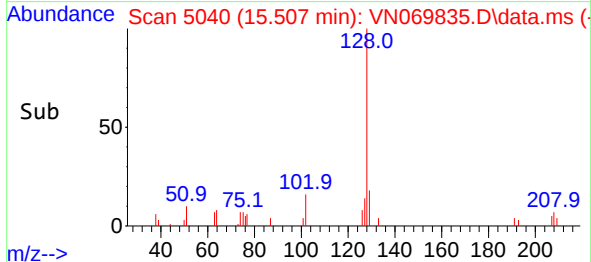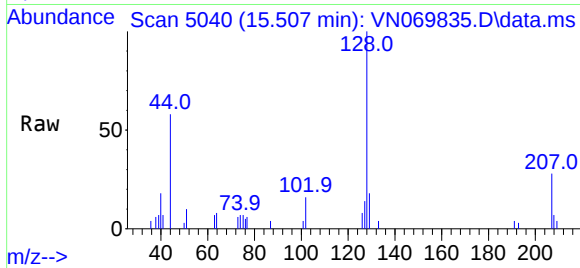

#96
1,2,3-Trichlorobenzene
Concen: 2.60 ug/l
RT: 15.700 min Scan# 5112
Delta R.T. -0.002 min
Lab File: VN069835.D
Acq: 8 Dec 2021 1:09

Tgt Ion:180 Resp: 2720
Ion Ratio Lower Upper
180 100
182 56.5 47.4 142.2
145 33.5 15.0 45.1

