

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN120820\
 Data File : VN064960.D
 Acq On : 8 Dec 2020 11:11
 Operator : JC/MD
 Sample : VN1208WBL01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1208WBL01

Quant Time: Dec 08 16:31:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 23 13:54:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.62	168	153937	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	271127	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	275977	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	119695	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.98	65	95147	53.17	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery	=	106.34%	
35) Dibromofluoromethane	7.54	113	88100	54.30	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery	=	108.60%	
50) Toluene-d8	10.06	98	342421	51.66	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery	=	103.32%	
62) 4-Bromofluorobenzene	12.37	95	125057	52.72	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery	=	105.44%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN120820\
Data File : VN064960.D
Acq On : 8 Dec 2020 11:11
Operator : JC/MD
Sample : VN1208WBL01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1208WBL01

Quant Time: Dec 08 16:31:16 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Quant Title : SW846 8260
QLast Update : Mon Nov 23 13:54:12 2020
Response via : Initial Calibration

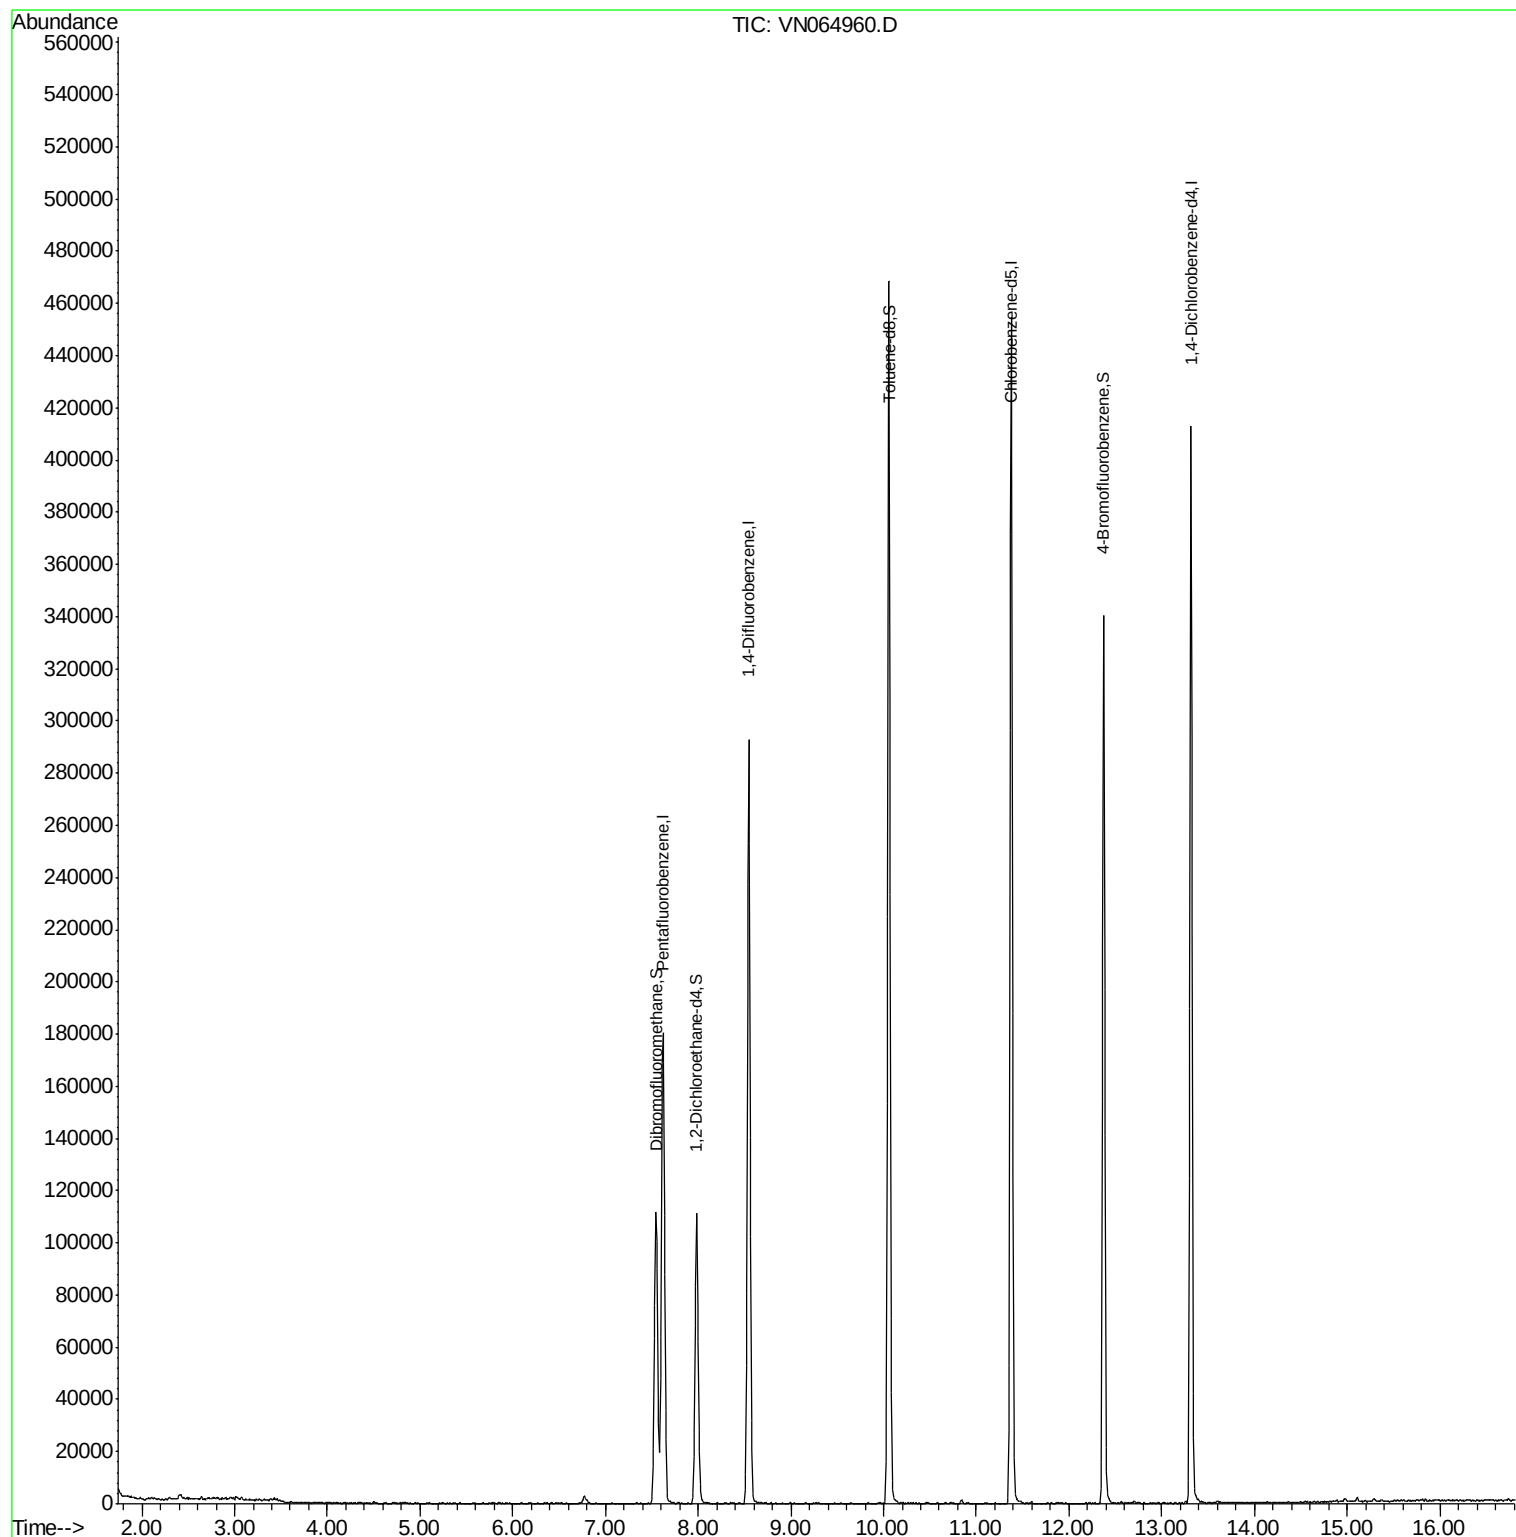

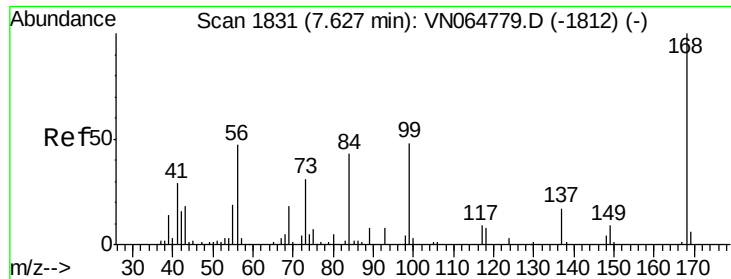

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.62 min Scan# 1829

Delta R.T. -0.01 min

Lab File: VN064960.D

Acq: 8 Dec 2020 11:11

Instrument :

MSVOA_N

ClientSampleId :


VN1208WBL01

Tot Ion:168 Resp: 153937

Ion Ratio Lower Upper




168 100

99 54.5 43.0 64.4

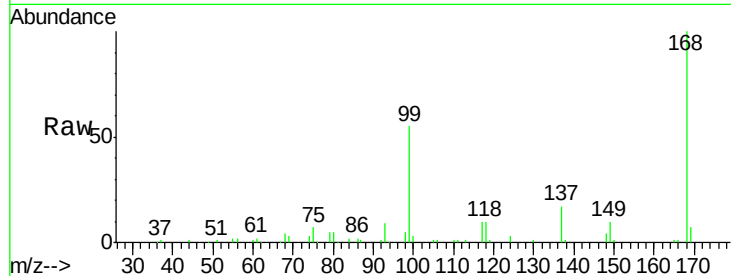

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

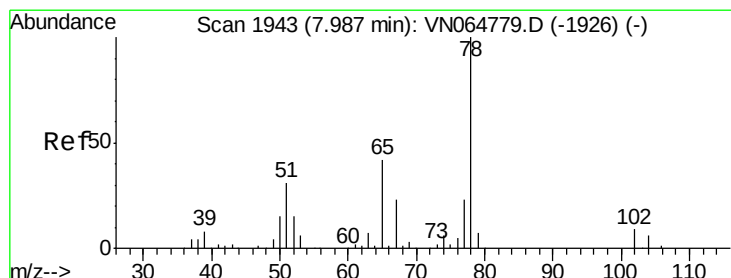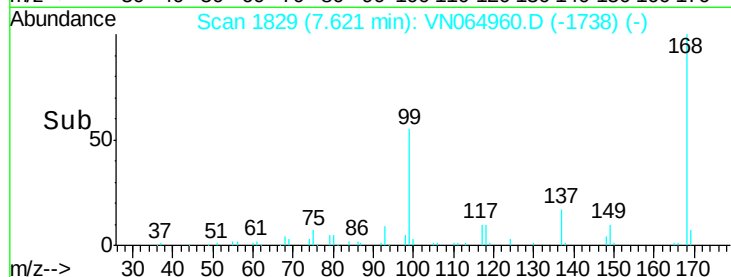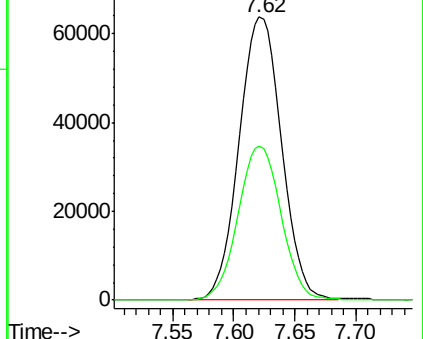

#33

1,2-Dichloroethane-d4

Concen: 53.166 ug/l

RT: 7.98 min Scan# 1942

Delta R.T. -0.00 min

Lab File: VN064960.D


Acq: 8 Dec 2020 11:11

Tgt Ion: 65 Resp: 95147

Ion Ratio Lower Upper



65 100


67 53.6 0.0 108.2

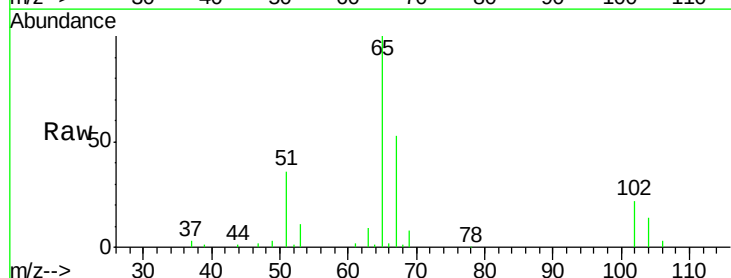

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

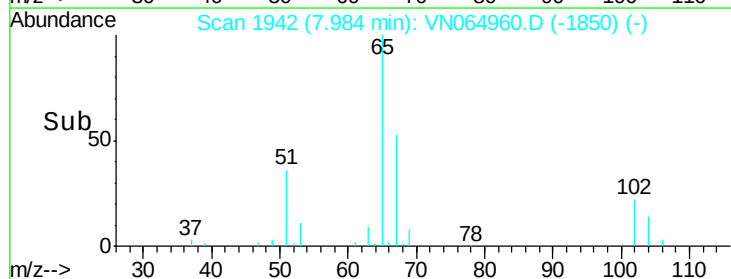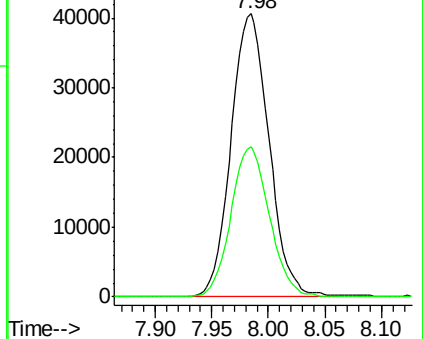


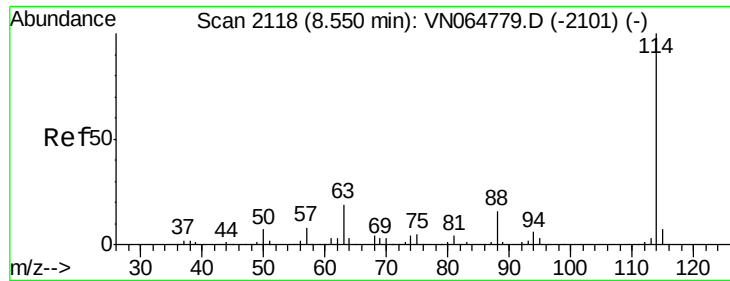




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2117
 Delta R.T. -0.00 min
 Lab File: VN064960.D
 Acq: 8 Dec 2020 11:11

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1208WBL01

Tot Ion:114 Resp: 271127
 Ion Ratio Lower Upper
 114 100
 63 19.9 0.0 38.6
 88 16.1 0.0 32.6

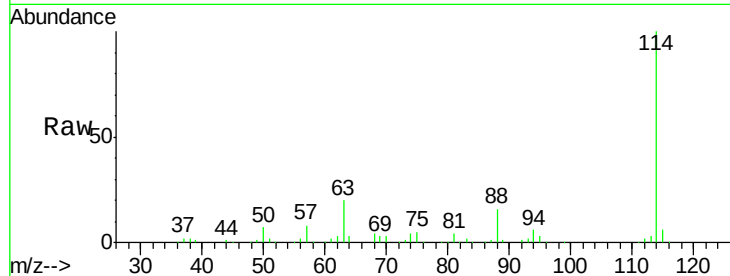


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

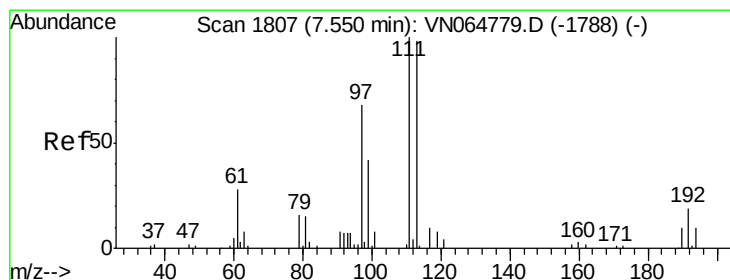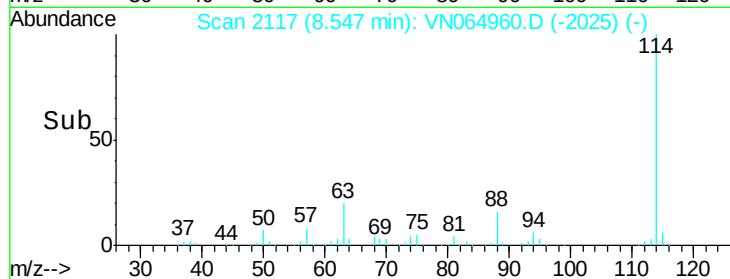
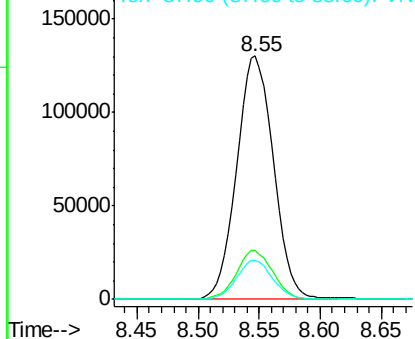



#35
 Dibromofluoromethane
 Concen: 54.304 ug/l
 RT: 7.54 min Scan# 1805
 Delta R.T. -0.01 min
 Lab File: VN064960.D
 Acq: 8 Dec 2020 11:11

Tgt Ion:113 Resp: 88100
 Ion Ratio Lower Upper
 113 100
 111 104.3 81.6 122.4
 192 20.0 16.2 24.2

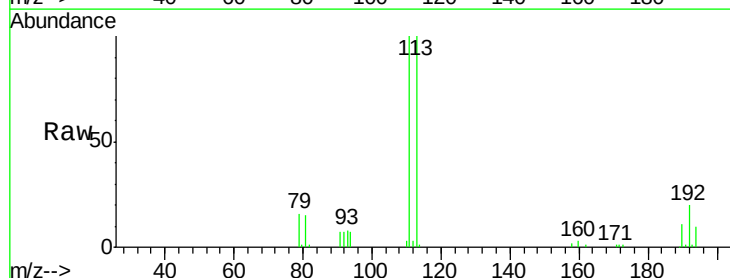

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

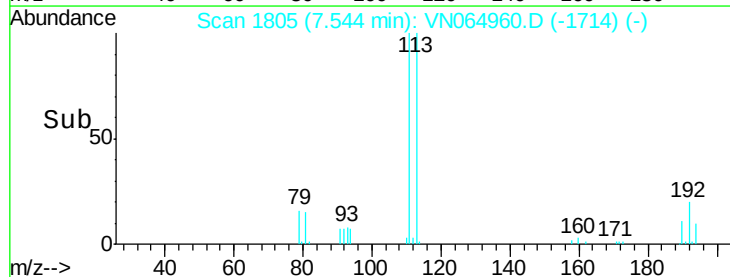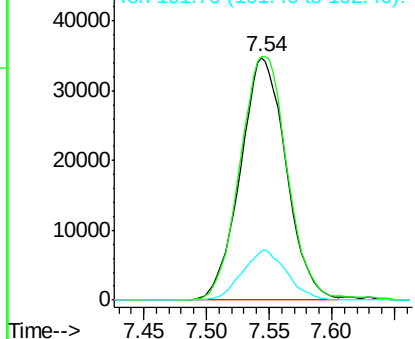

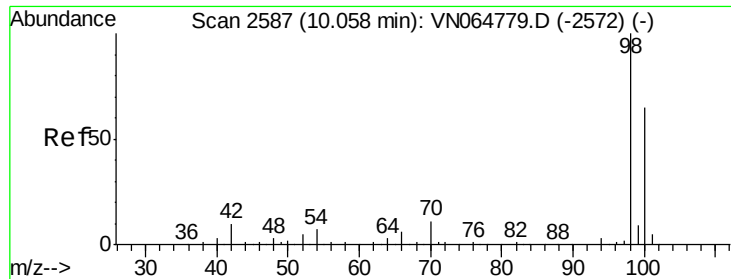

#50

Toluene-d8

Concen: 51.657 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN064960.D

Acq: 8 Dec 2020 11:11

Instrument :

MSVOA_N

ClientSampleId :


VN1208WBL01

Tot Ion: 98 Resp: 342421

Ion Ratio Lower Upper




98 100

100 64.1 51.7 77.5

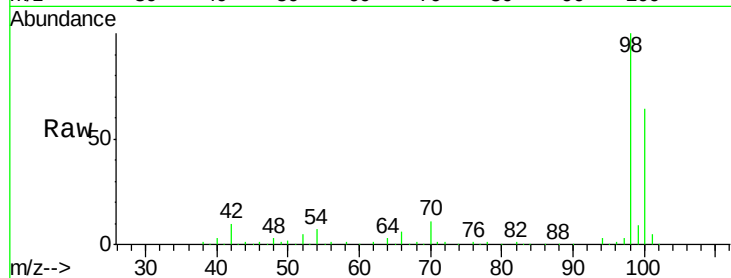

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

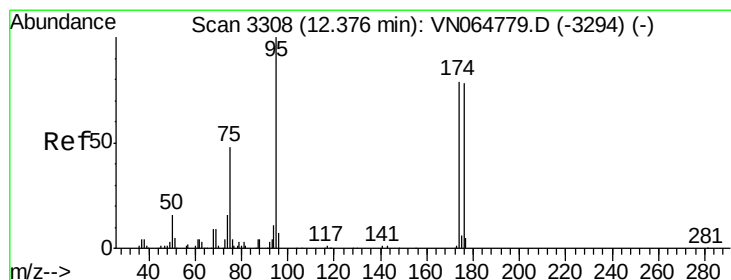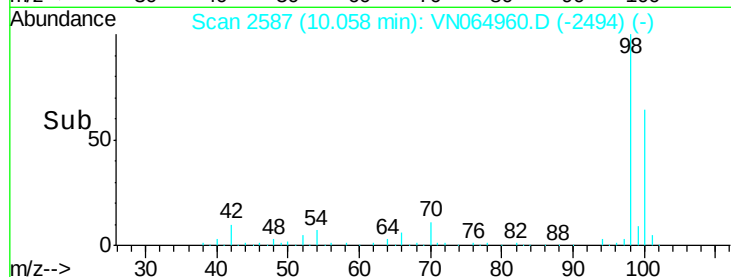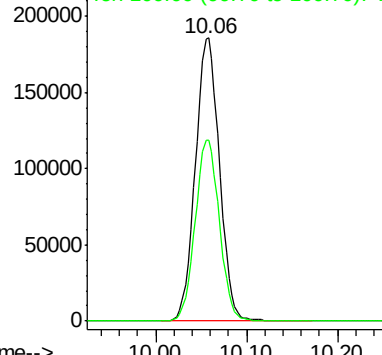

#62

4-Bromofluorobenzene

Concen: 52.716 ug/l

RT: 12.37 min Scan# 3307

Delta R.T. -0.00 min

Lab File: VN064960.D

Acq: 8 Dec 2020 11:11


Tgt Ion: 95 Resp: 125057

Ion Ratio Lower Upper

95 100

174 81.8 0.0 160.4



176 78.8 0.0 158.4

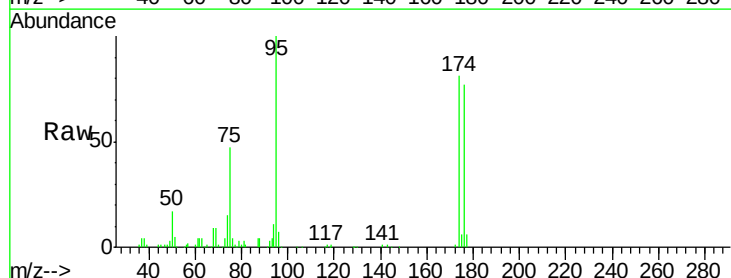


Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

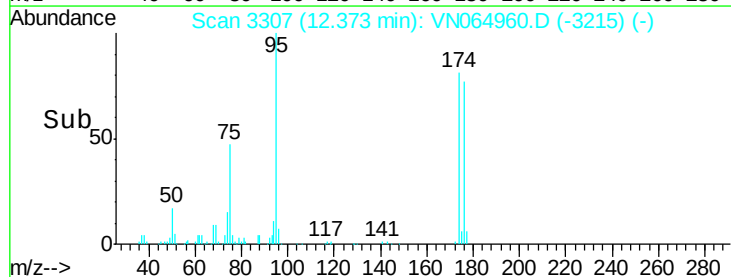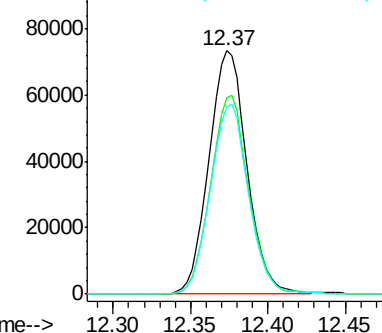

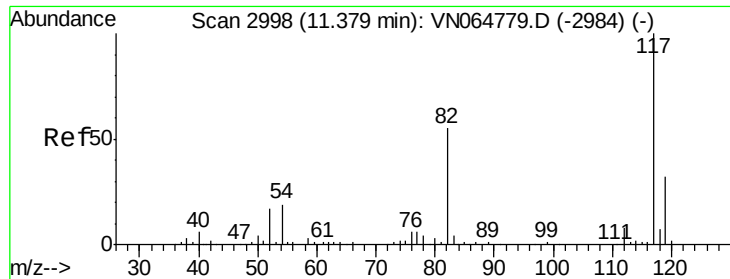

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2997

Delta R.T. -0.00 min

Lab File: VN064960.D

Acq: 8 Dec 2020 11:11

Instrument :

MSVOA_N

ClientSampleId :

VN1208WBL01


Tot Ion:117 Resp: 275977

Ion Ratio Lower Upper

117 100

82 55.8 44.2 66.2




119 32.6 25.8 38.6

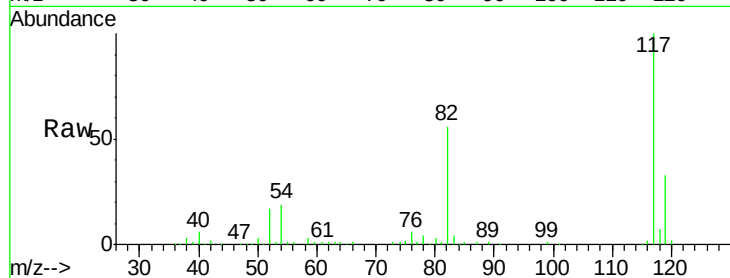

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VN0

Ion 118.90 (118.60 to 119.60): V

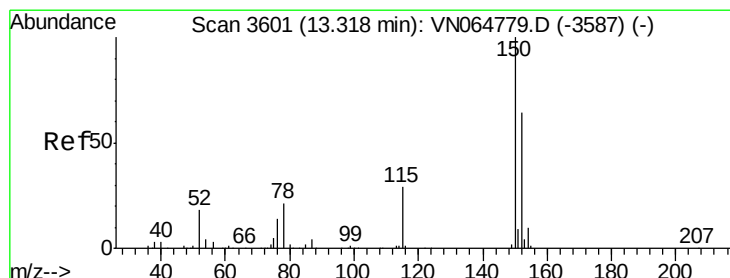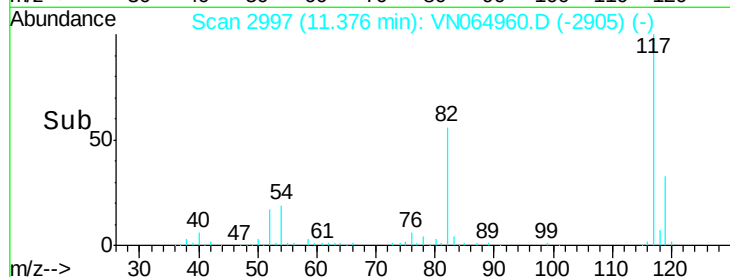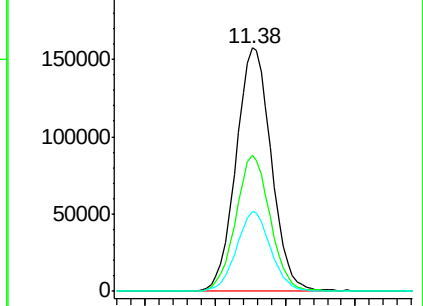

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3600

Delta R.T. -0.00 min

Lab File: VN064960.D

Acq: 8 Dec 2020 11:11


Tgt Ion:152 Resp: 119695

Ion Ratio Lower Upper

152 100

115 58.9 29.7 89.1

150 156.7 0.0 350.6

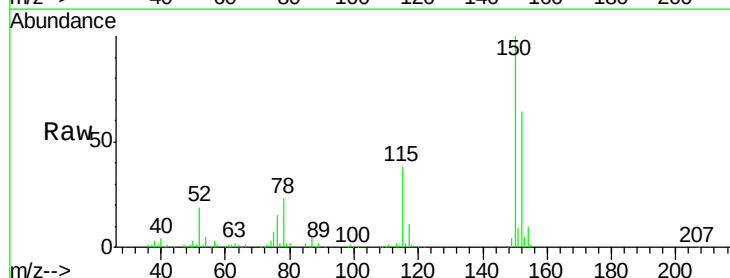

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

