


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN120820\
Data File : VN064958.D
Acq On : 8 Dec 2020 9:24
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112320W.M
Title : SW846 8260
Last Update : Mon Nov 23 13:54:12 2020

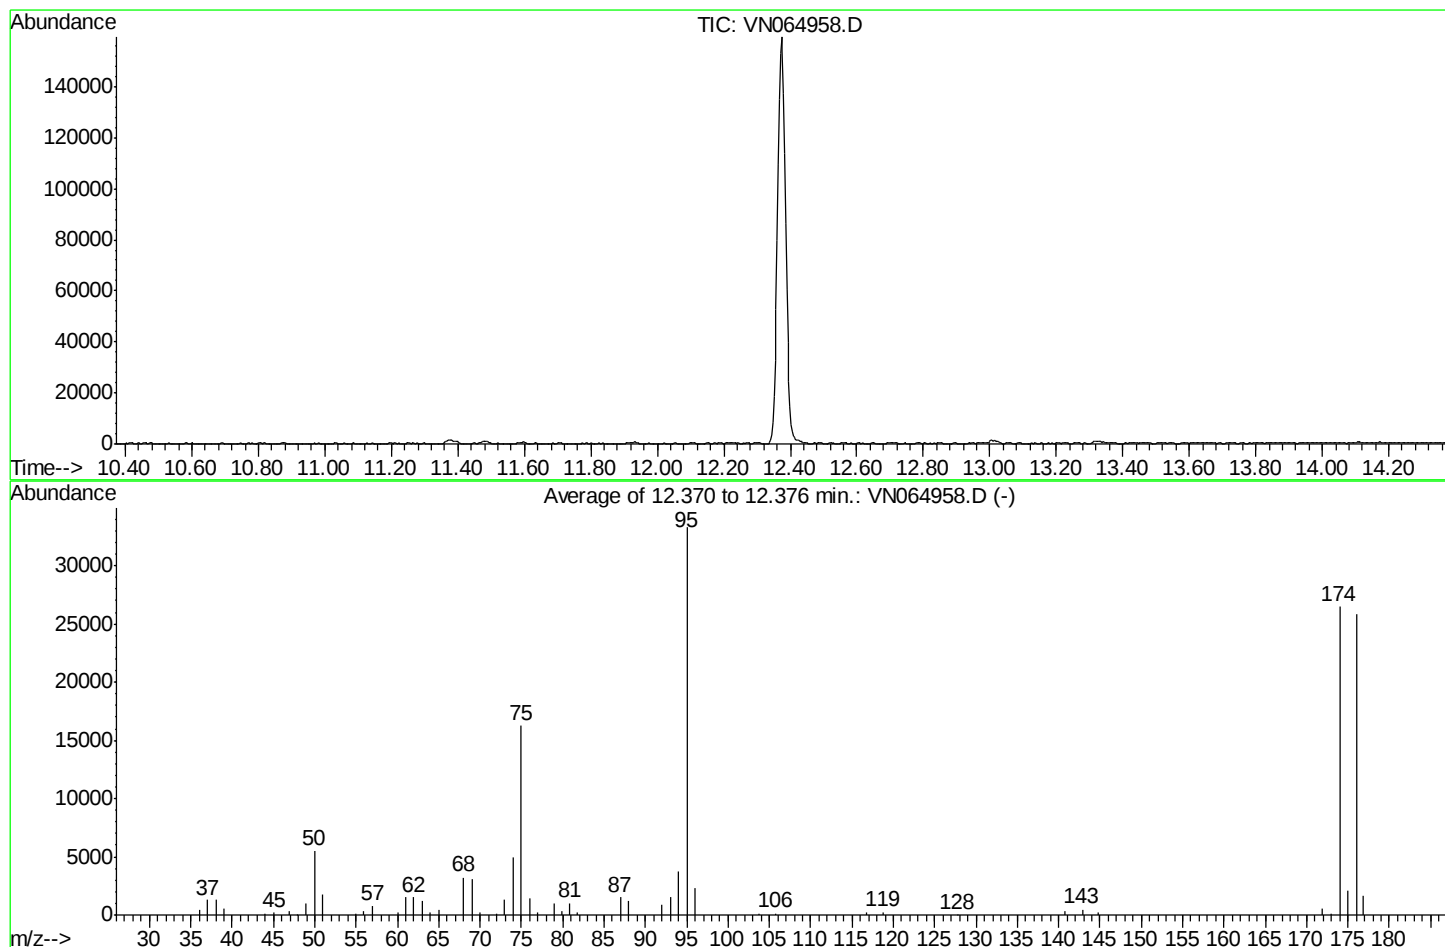

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	5512	PASS
75	95	30	60	48.7	16233	PASS
95	95	100	100	100.0	33301	PASS
96	95	5	9	6.8	2265	PASS
173	174	0.00	2	0.4	94	PASS
174	95	50	100	79.5	26477	PASS
175	174	5	9	7.9	2104	PASS
176	174	95	101	97.5	25824	PASS
177	176	5	9	6.3	1630	PASS