

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120821\
 Data File : VN069865.D
 Acq On : 8 Dec 2021 16:55
 Operator : JC/MD
 Sample : M4957-02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RE114D2-20211206

Quant Time: Dec 09 11:42:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	1243667	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2264883	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2454479	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	925871	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	968444	50.434	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 100.860%	
35) Dibromofluoromethane	8.024	113	672861	47.429	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 94.860%	
50) Toluene-d8	10.443	98	2944486	51.690	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 103.380%	
62) 4-Bromofluorobenzene	12.733	95	1142847	55.379	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 110.760%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.078	85	7310	0.504	ug/l	95
3) Chloromethane	2.311	50	3775	0.208	ug/l	90
7) Trichlorofluoromethane	3.381	101	7312	0.333	ug/l	92
9) 1,1,2-Trichlorotrifluo...	4.213	101	122732	9.984	ug/l	96
12) 1,1-Dichloroethene	4.183	96	8750	0.739	ug/l	90
16) Acetone	4.296	43	12345	1.069	ug/l	99
24) 1,1-Dichloroethane	6.383	63	6414	0.237	ug/l #	91
27) cis-1,2-Dichloroethene	7.327	96	14312	0.921	ug/l	99
30) Chloroform	7.825	83	9229	0.338	ug/l	95
31) Cyclohexane	8.088	56	33098	1.239	ug/l #	37
36) 1,1-Dichloropropene	8.086	75	106918	4.959	ug/l #	42
38) Carbon Tetrachloride	8.204	117	8337	0.394	ug/l	89
39) Methylcyclohexane	9.220	83	12649	0.493	ug/l #	1
44) Trichloroethene	9.217	130	959087	60.973	ug/l	90
49) 1,4-Dioxane	9.574	88	2639	6.636	ug/l #	76
51) 4-Methyl-2-Pentanone	10.440	43	16254	0.528	ug/l #	1
53) t-1,3-Dichloropropene	10.443	75	496	2.812	ug/l #	1
54) cis-1,3-Dichloropropene	10.430	75	286	2.009	ug/l #	1
55) 1,1,2-Trichloroethane	10.896	97	3712	0.229	ug/l	91
60) Dibromochloromethane	10.979	129	3714	2.580	ug/l #	11
64) Tetrachloroethene	10.977	164	3659	0.220	ug/l #	77
71) Bromoform	12.720	173	1433	2.821	ug/l #	1
76) 1,2,3-Trichloropropane	12.731	75	637000	23.991	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	637000	76.203	ug/l #	5
93) 1,2,4-Trichlorobenzene	15.265	180	216	2.891	ug/l #	1
95) Naphthalene	15.507	128	1623	4.018	ug/l #	77
96) 1,2,3-Trichlorobenzene	15.694	180	578	2.473	ug/l #	45

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206

The chromatogram displays a series of peaks corresponding to different chemical compounds. The y-axis represents Abundance, ranging from 0 to 5,200,000. The x-axis represents Time in minutes, ranging from 2.00 to 16.00. The following table lists the compounds identified in the chromatogram, along with their approximate retention times and relative abundances.





Compound	Retention Time (min)	Approximate Abundance
Dichlorodifluoromethane, T	2.1	100,000
Chloromethane, P	2.5	50,000
Trichlorofluoromethane, T	3.5	50,000
Acetone, T	4.2	200,000
1,1-Dichloroethane, T	4.5	100,000
1,1-Dichloroethane, P	6.5	100,000
cis-1,2-Dichloroethene, T	7.5	50,000
Chloroform, C	8.1	100,000
Dibromodifluoromethane, S	8.2	1,200,000
Carbon Tetrachloride, T	8.3	800,000
1,2-Dichloroethane-d4, S	8.5	1,100,000
1,4-Difluorobenzene, I	9.1	2,700,000
Methyldichloromethane, TM	9.3	2,700,000
1,4-Dioxane, T	9.8	100,000
cis-1,3-Dichloropropene, T	10.5	4,000,000
trans-1,3-Dichloropropene, T	10.6	4,000,000
Chlorobenzene-d5, I	11.8	4,000,000
Bromoform, P	12.8	2,000,000
1,2-Trichloroethane, T	13.0	3,300,000
1,4-Dichlorobenzene-d4, I	13.8	3,400,000
1,2,4-Trichlorobenzene, T	15.2	100,000
Naphthalene, T	15.5	100,000
1,2,3-Trichlorobenzene, T	15.8	100,000



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion:168 Resp: 1243667
Ion Ratio Lower Upper
168 100
99 59.8 41.3 61.9

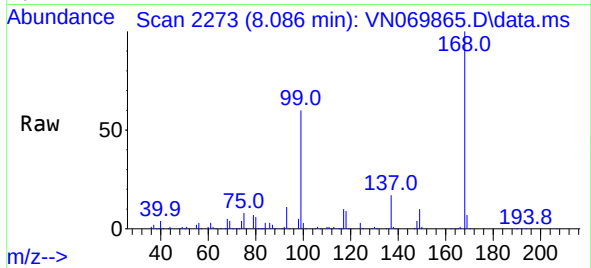

#2
Dichlorodifluoromethane
Concen: 0.504 ug/l
RT: 2.078 min Scan# 33
Delta R.T. 0.005 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion: 85 Resp: 7310
Ion Ratio Lower Upper
85 100
87 29.9 16.3 48.9


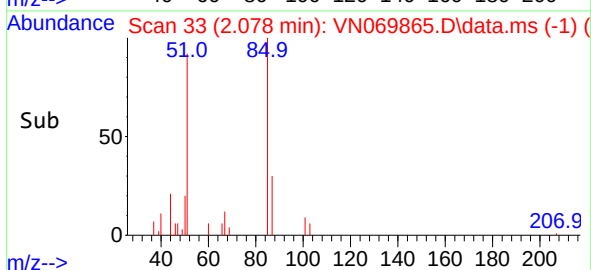






#3
Chloromethane
Concen: 0.208 ug/l
RT: 2.311 min Scan# 117
Delta R.T. 0.008 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion: 50 Resp: 3775
Ion Ratio Lower Upper
50 100
52 26.3 25.4 38.0

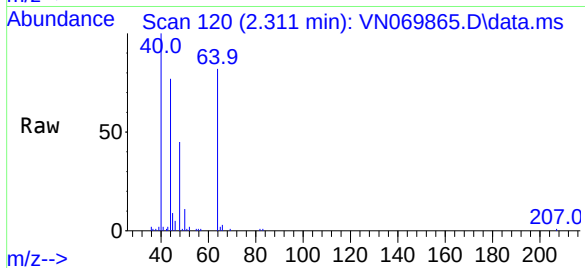

#7
Trichlorofluoromethane
Concen: 0.333 ug/l
RT: 3.381 min Scan# 519
Delta R.T. 0.013 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion: 101 Resp: 7312
Ion Ratio Lower Upper
101 100
103 68.6 50.1 75.1


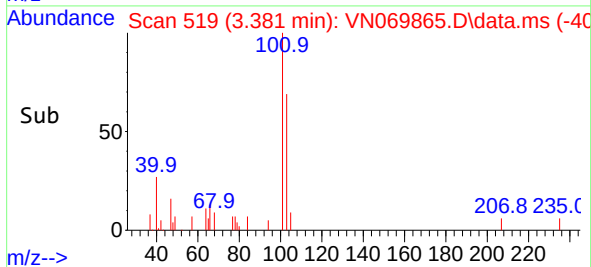

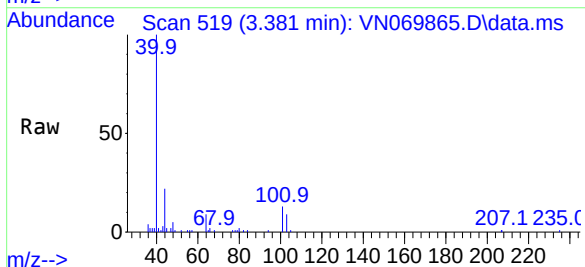




#9
1,1,2-Trichlorotrifluoroethane
Concen: 9.984 ug/l
RT: 4.213 min Scan# 81
Delta R.T. 0.011 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion:101 Resp: 122732
Ion Ratio Lower Upper
101 100
85 47.2 37.2 55.8
151 77.6 65.9 98.9

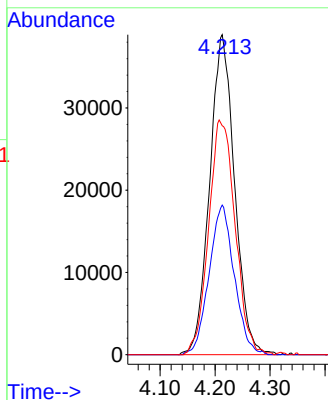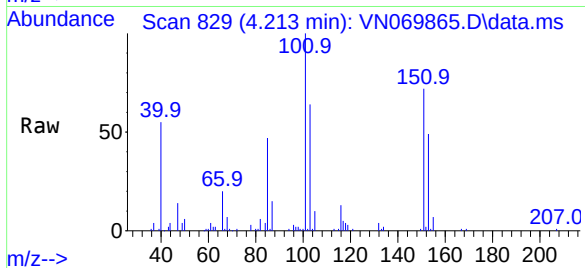

#12
1,1-Dichloroethene
Concen: 0.739 ug/l
RT: 4.183 min Scan# 818
Delta R.T. 0.008 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion: 96 Resp: 8750
Ion Ratio Lower Upper
96 100
61 179.9 131.0 196.6
98 69.3 52.4 78.6


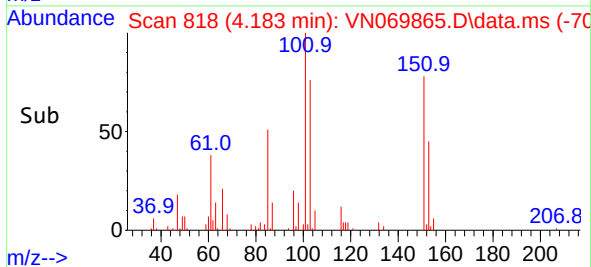
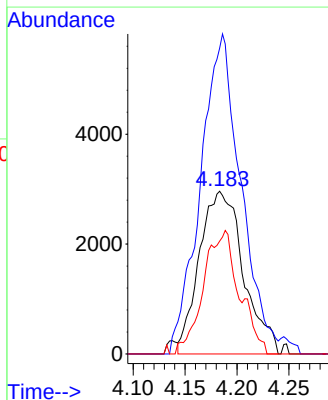
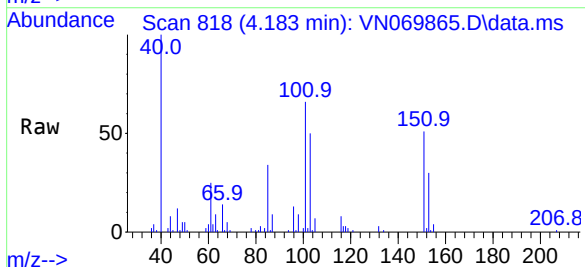




#16
Acetone
Concen: 1.069 ug/l
RT: 4.296 min Scan# 80
Delta R.T. 0.005 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion: 43 Resp: 12345
Ion Ratio Lower Upper
43 100
58 28.2 23.1 34.7

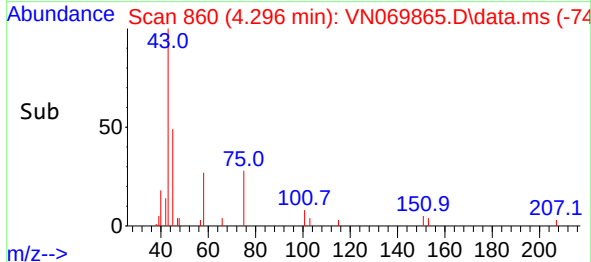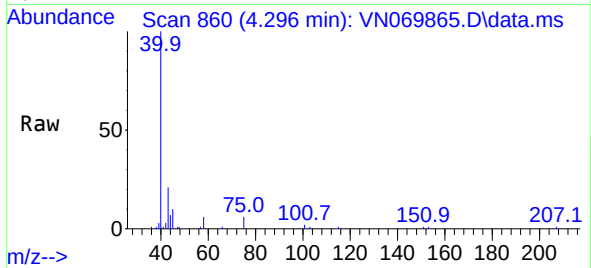

#24
1,1-Dichloroethane
Concen: 0.237 ug/l
RT: 6.383 min Scan# 1638
Delta R.T. -0.005 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion: 63 Resp: 6414
Ion Ratio Lower Upper
63 100
98 4.6 3.3 9.9
100 0.0 2.1 6.5#


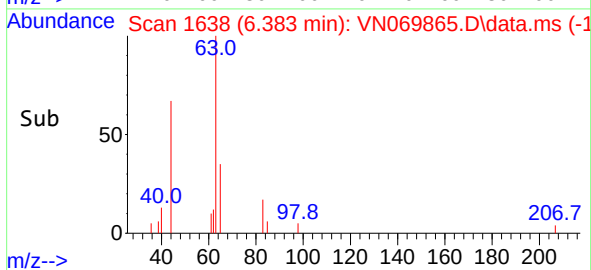




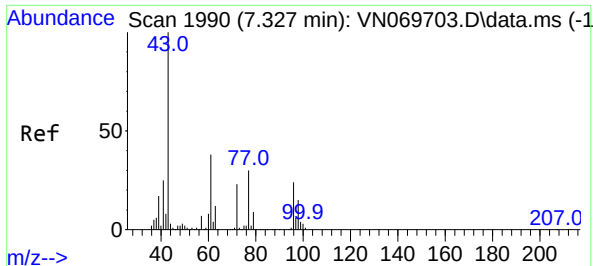

#27
 cis-1,2-Dichloroethene
 Concen: 0.921 ug/l
 RT: 7.327 min Scan# 1990
 Delta R.T. 0.000 min
 Lab File: VN069865.D
 Acq: 8 Dec 2021 16:55




Instrument :
 MSVOA_N
 ClientSampleId :
 RE114D2-20211206


Tgt Ion:	96	Resp:	14312
Ion	Ratio	Lower	Upper
96	100		
61	137.2	0.0	275.0
98	62.6	0.0	129.6

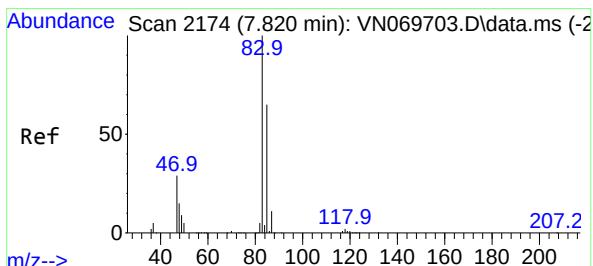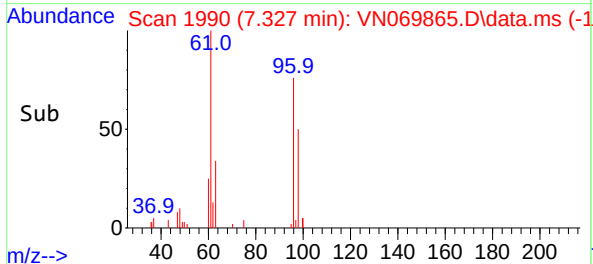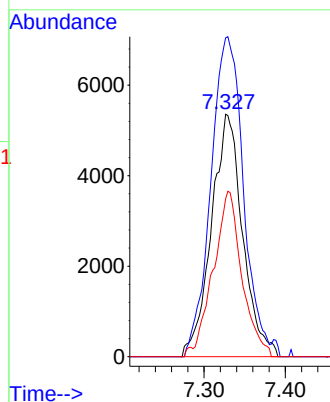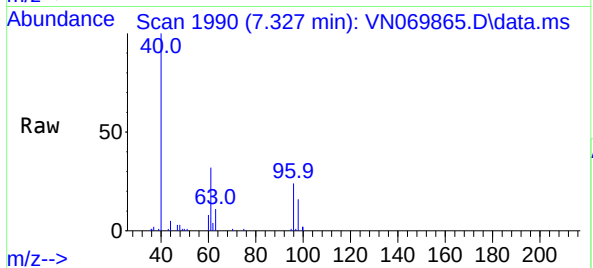

#30
 Chloroform
 Concen: 0.338 ug/l
 RT: 7.825 min Scan# 2176
 Delta R.T. 0.005 min
 Lab File: VN069865.D
 Acq: 8 Dec 2021 16:55

Tgt Ion:	83	Resp:	9229
Ion	Ratio	Lower	Upper
83	100		
85	60.9	51.9	77.9


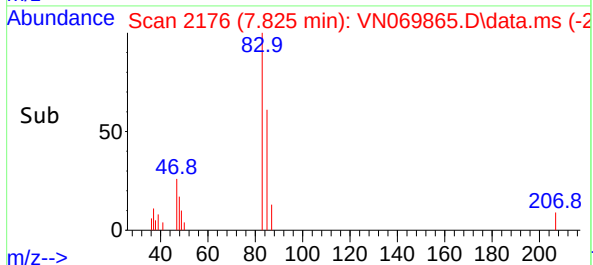

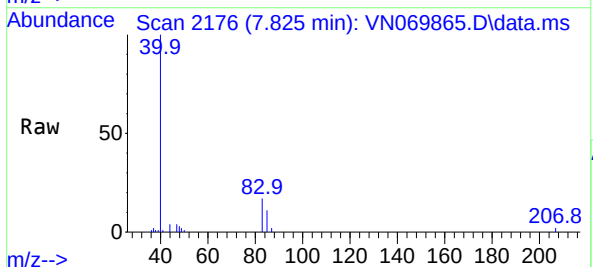




#31
Cyclohexane
Concen: 1.239 ug/l
RT: 8.088 min Scan# 21
Delta R.T. -0.005 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion: 56 Resp: 33098
Ion Ratio Lower Upper
56 100
69 140.0 27.1 40.7#
84 108.2 73.4 110.0

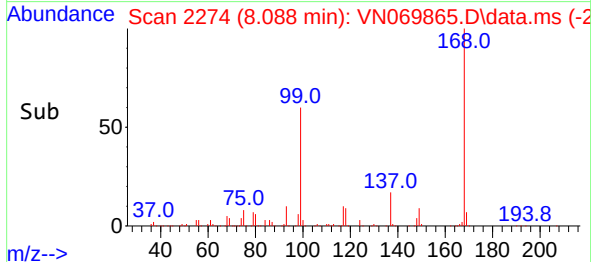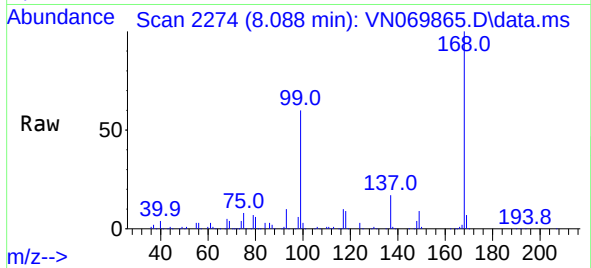

#33
1,2-Dichloroethane-d4
Concen: 50.434 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.003 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion: 65 Resp: 968444
Ion Ratio Lower Upper
65 100
67 50.9 0.0 103.0


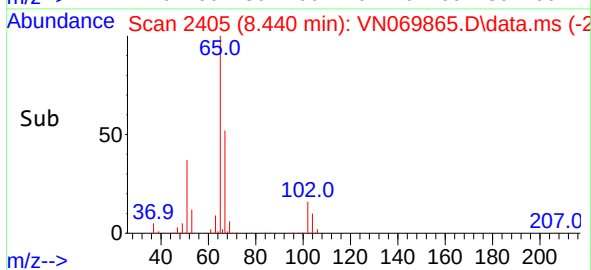






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. -0.000 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion:114 Resp: 2264883
Ion Ratio Lower Upper
114 100
63 22.9 0.0 37.8
88 15.9 0.0 27.4

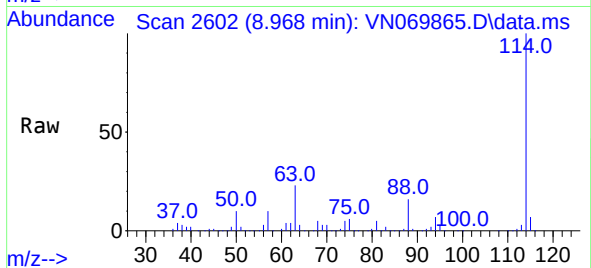

#35
Dibromofluoromethane
Concen: 47.429 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion:113 Resp: 672861
Ion Ratio Lower Upper
113 100
111 103.6 82.2 123.2
192 18.9 16.9 25.3


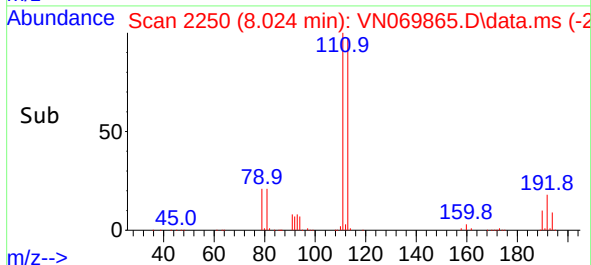
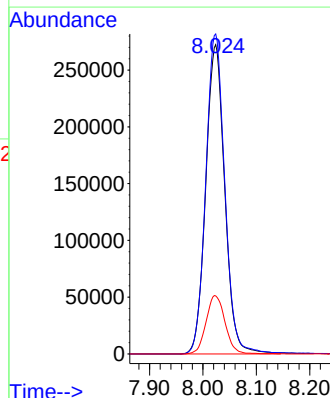
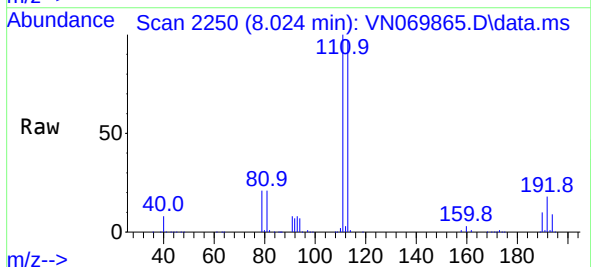




#36
1,1-Dichloropropene
Concen: 4.959 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.137 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion: 75 Resp: 106918
Ion Ratio Lower Upper
75 100
110 1.8 18.4 55.2#
77 0.0 24.4 36.6#

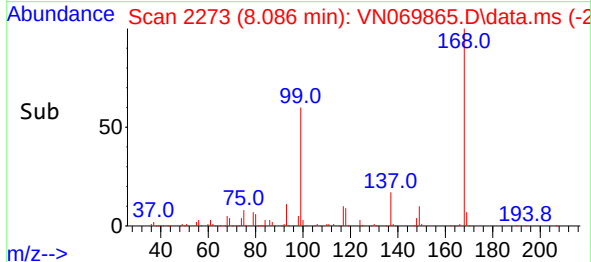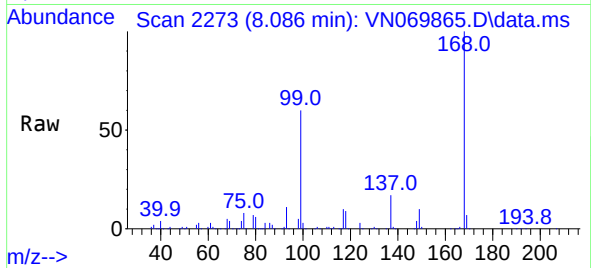

#38
Carbon Tetrachloride
Concen: 0.394 ug/l
RT: 8.204 min Scan# 2317
Delta R.T. -0.003 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion: 117 Resp: 8337
Ion Ratio Lower Upper
117 100
119 84.2 76.1 114.1
121 35.3 24.2 36.2

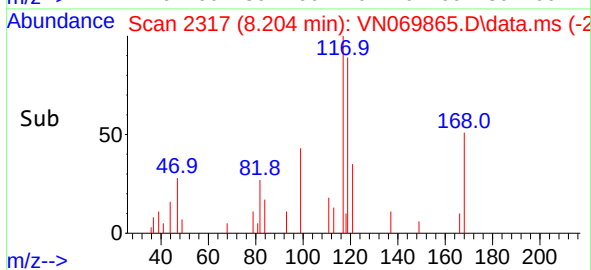



#39

Methylcyclohexane

Concen: 0.493 ug/l

RT: 9.220 min Scan# 2

Delta R.T. -0.241 min

Lab File: VN069865.D

Acq: 8 Dec 2021 16:55

Instrument :

MSVOA_N

ClientSampleId :

RE114D2-20211206





Tgt Ion: 83 Resp: 12649

Ion Ratio Lower Upper

83 100

55 0.0 58.1 87.1#

98 189.7 38.4 57.6#

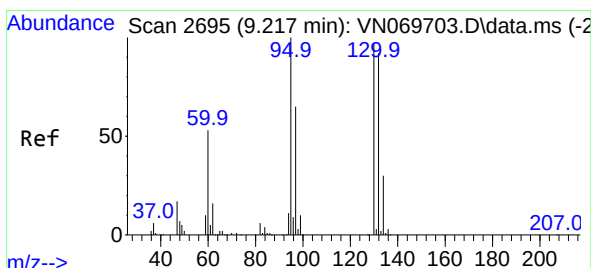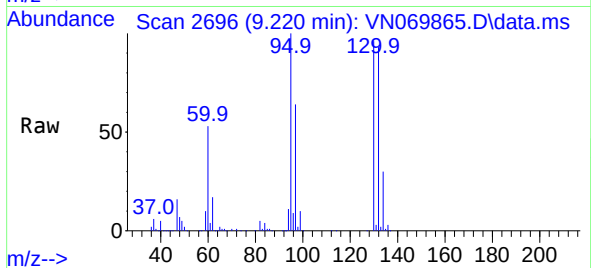

#44

Trichloroethene

Concen: 60.973 ug/l

RT: 9.217 min Scan# 2695

Delta R.T. 0.000 min

Lab File: VN069865.D




Acq: 8 Dec 2021 16:55


Tgt Ion:130 Resp: 959087

Ion Ratio Lower Upper

130 100

95 104.9 0.0 191.2


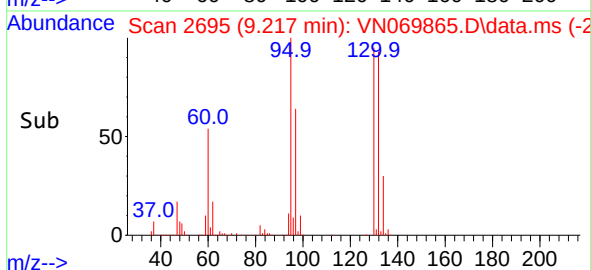




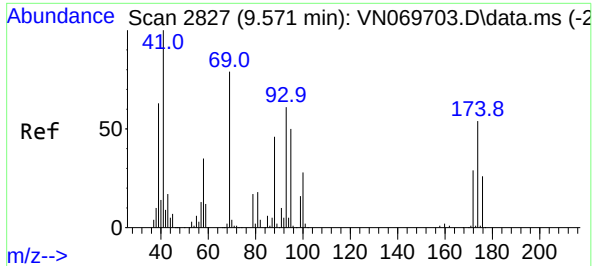

#49
1,4-Dioxane
Concen: 6.636 ug/l
RT: 9.574 min Scan# 21
Delta R.T. 0.003 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion: 88 Resp: 2639
Ion Ratio Lower Upper
88 100
43 3.9 23.4 35.2#
58 53.2 50.6 75.8

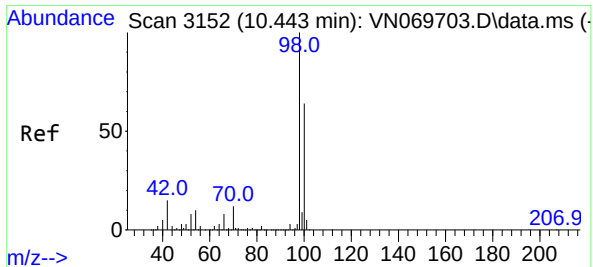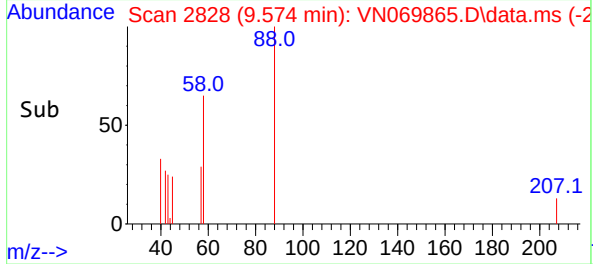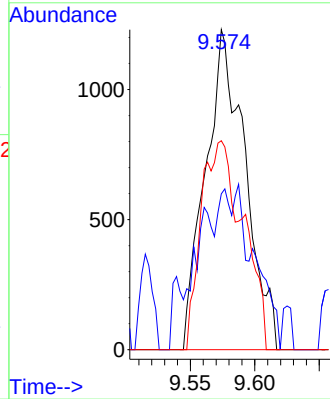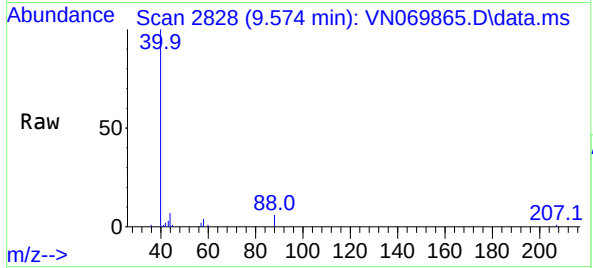

#50
Toluene-d8
Concen: 51.690 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion: 98 Resp: 2944486
Ion Ratio Lower Upper
98 100
100 63.4 50.4 75.6

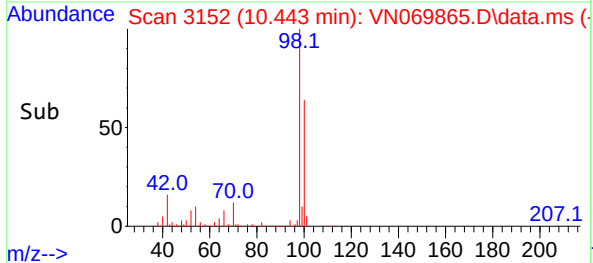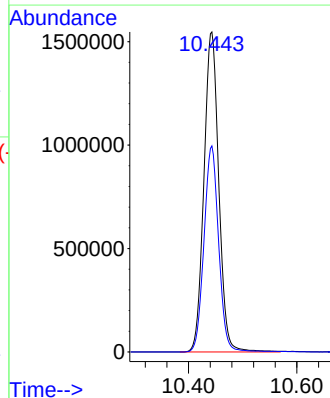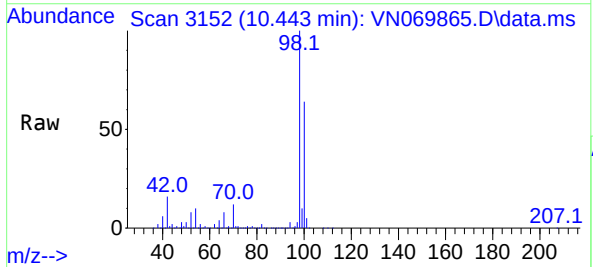



#51

4-Methyl-2-Pentanone

Concen: 0.528 ug/l

RT: 10.440 min Scan# 3111

Delta R.T. 0.107 min

Lab File: VN069865.D

Acq: 8 Dec 2021 16:55

Instrument :

MSVOA_N

ClientSampleId :





RE114D2-20211206

Tgt Ion: 43 Resp: 16254

Ion Ratio Lower Upper

43 100

58 172.9 30.4 45.6#

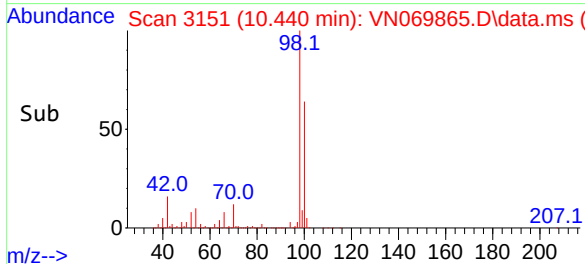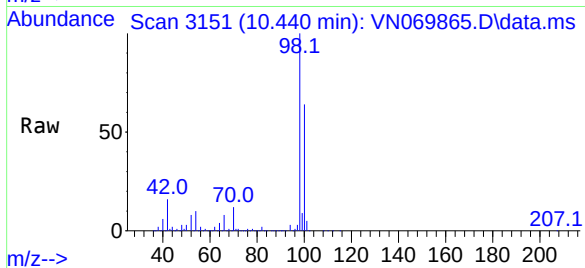

#53

t-1,3-Dichloropropene

Concen: 2.812 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. -0.276 min

Lab File: VN069865.D




Acq: 8 Dec 2021 16:55


Tgt Ion: 75 Resp: 496

Ion Ratio Lower Upper

75 100


77 314.8 25.6 38.4#

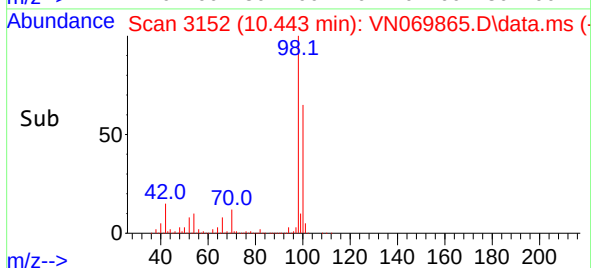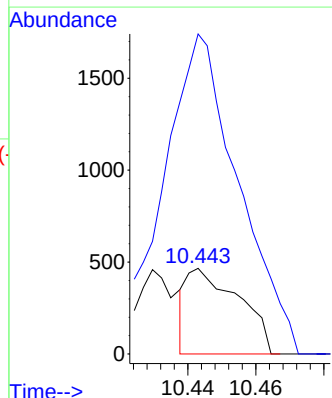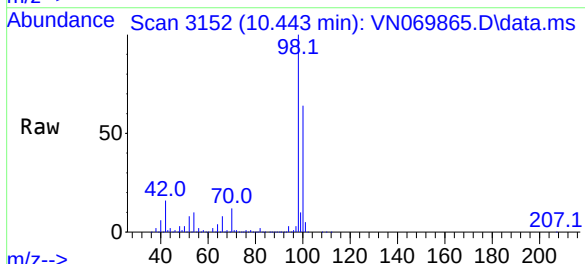

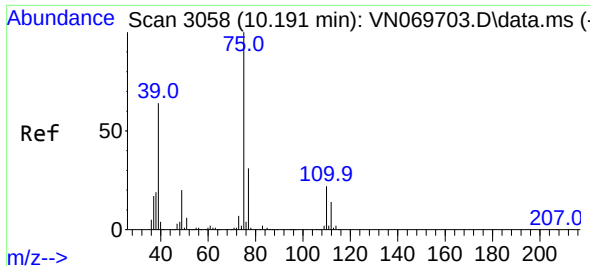




#54
cis-1,3-Dichloropropene
Concen: 2.009 ug/l
RT: 10.430 min Scan# 3147
Delta R.T. 0.239 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206

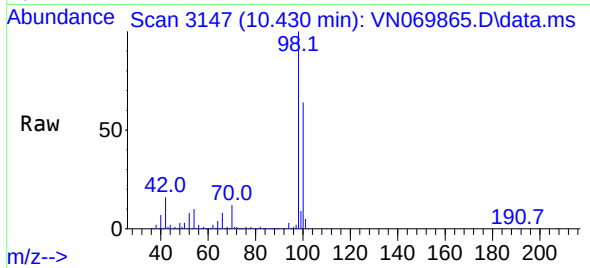

Tgt Ion: 75 Resp: 286




Ion	Ratio	Lower	Upper
75	100		
77	89.5	26.4	39.6#
39	179.1	42.5	63.7#

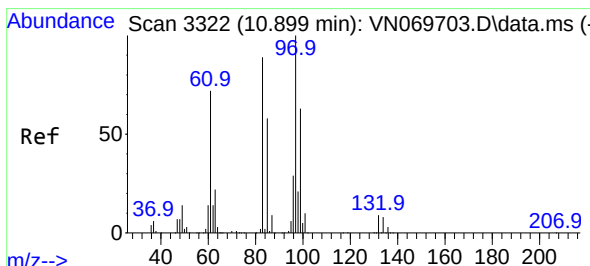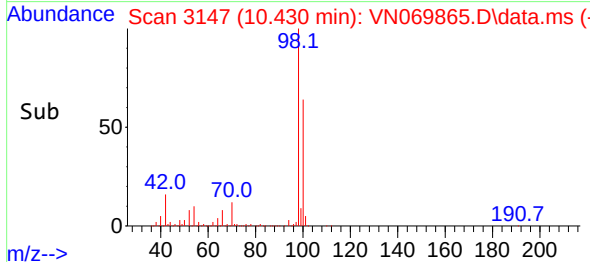


#55
1,1,2-Trichloroethane
Concen: 0.229 ug/l
RT: 10.896 min Scan# 3321
Delta R.T. -0.003 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion: 97 Resp: 3712

Ion	Ratio	Lower	Upper
97	100		
83	76.2	67.8	101.6
85	47.4	45.4	68.2
99	58.2	49.4	74.0


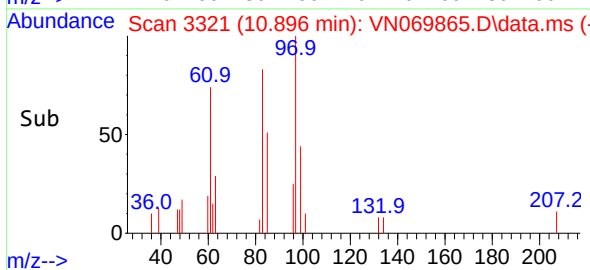
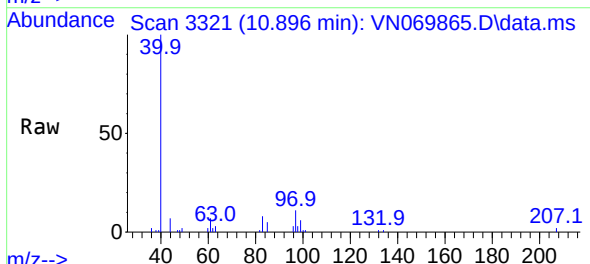
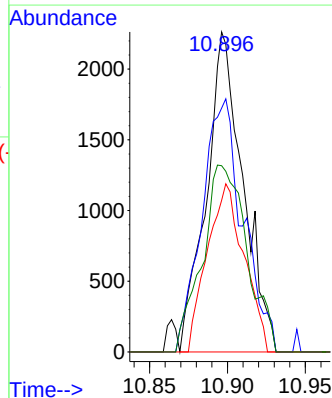


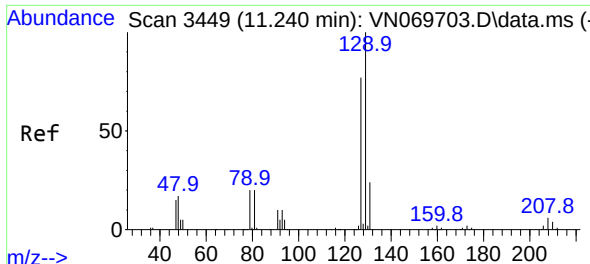

#60
Dibromochloromethane
Concen: 2.580 ug/l
RT: 10.979 min Scan# 31
Delta R.T. -0.261 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion:129 Resp: 3714
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#

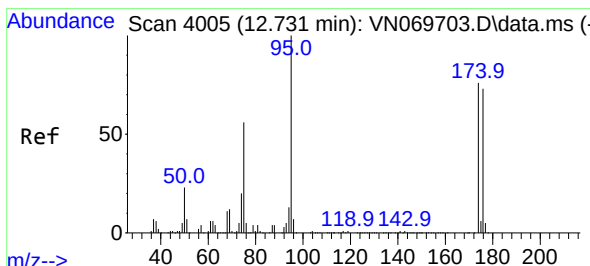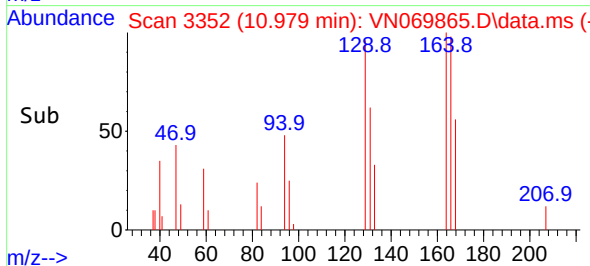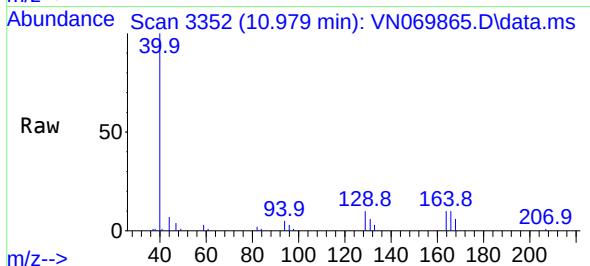

#62
4-Bromofluorobenzene
Concen: 55.379 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.002 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion: 95 Resp: 1142847
Ion Ratio Lower Upper
95 100
174 76.0 0.0 187.2
176 73.6 0.0 181.4

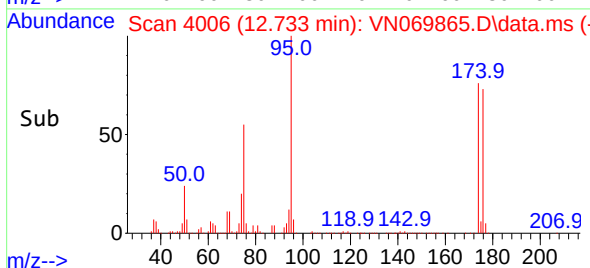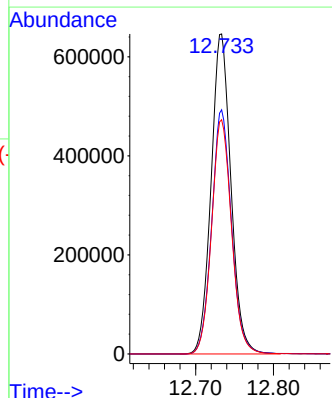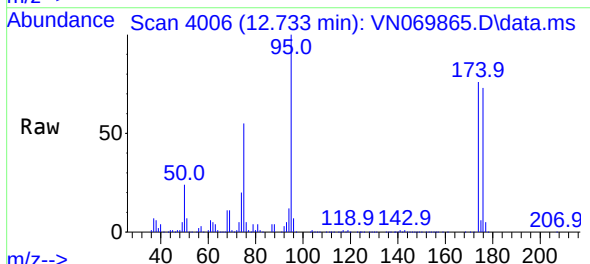







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3638
Delta R.T. -0.002 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206

Tgt Ion:117 Resp: 2454479




Ion	Ratio	Lower	Upper
117	100		
82	59.4	42.4	63.6
119	31.6	25.4	38.2

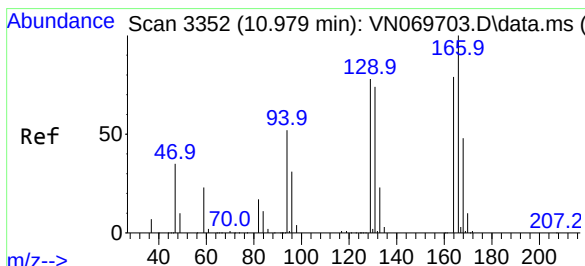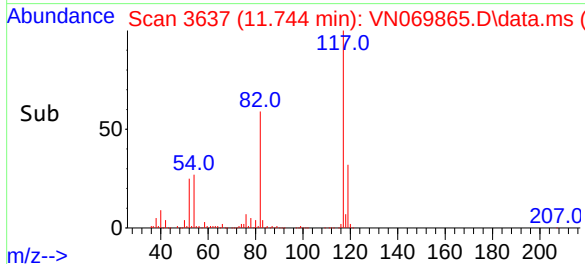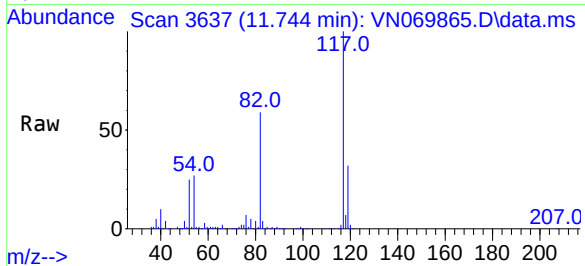


#64
Tetrachloroethene
Concen: 0.220 ug/l
RT: 10.977 min Scan# 3351
Delta R.T. -0.002 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion:164 Resp: 3659

Ion	Ratio	Lower	Upper
164	100		
166	87.6	101.9	152.9#
129	90.7	72.0	108.0
131	61.2	70.9	106.3#


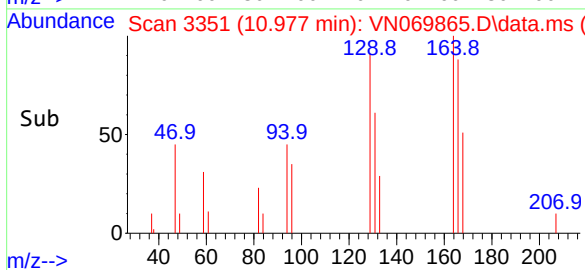

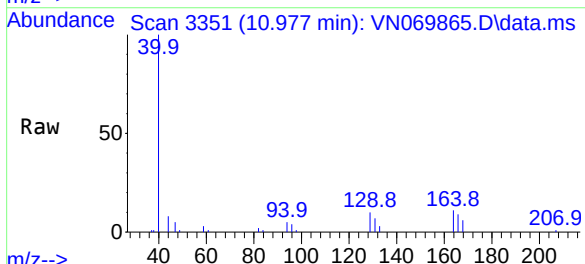


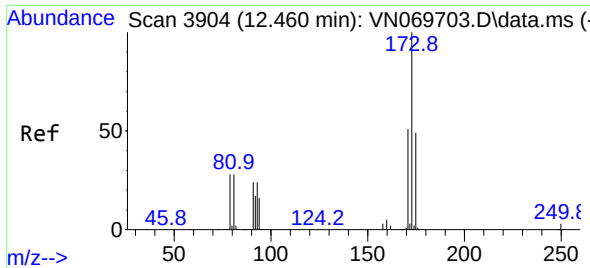

#71
Bromoform
Concen: 2.821 ug/l
RT: 12.720 min Scan# 4001
Delta R.T. 0.260 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion:173 Resp: 1433
Ion Ratio Lower Upper
173 100
175 4301.0 24.2 72.6#
254 0.0 0.0 0.0

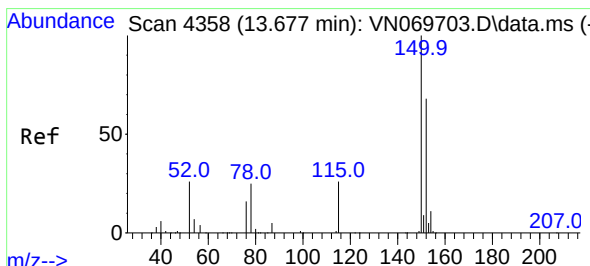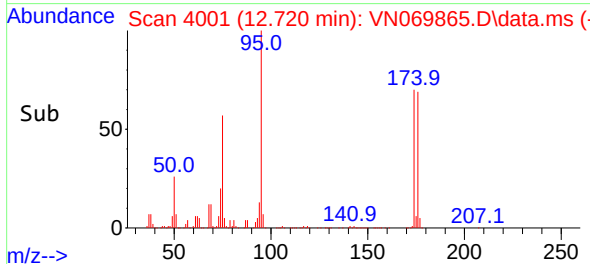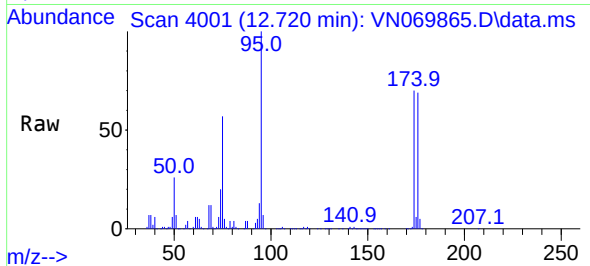

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Tgt Ion:152 Resp: 925871
Ion Ratio Lower Upper
152 100
115 61.3 27.5 82.5
150 158.2 0.0 344.4


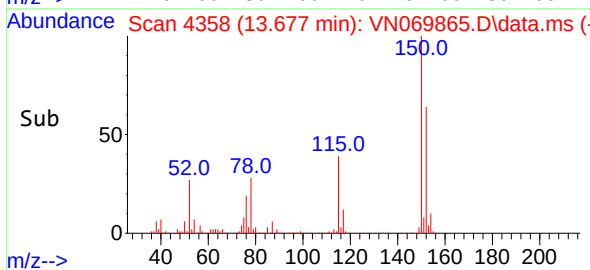

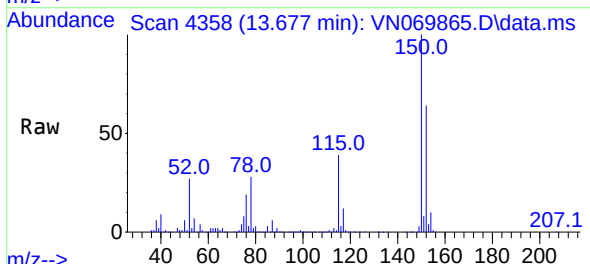




#76
1,2,3-Trichloropropane
Concen: 23.991 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.150 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55




Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206


Tgt Ion: 75 Resp: 637000
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#

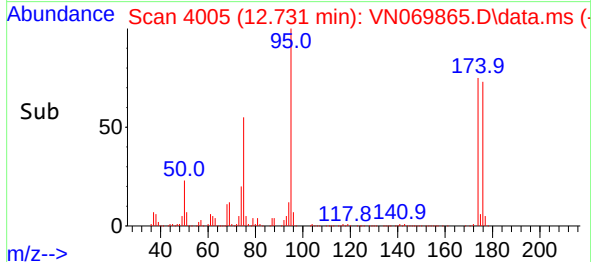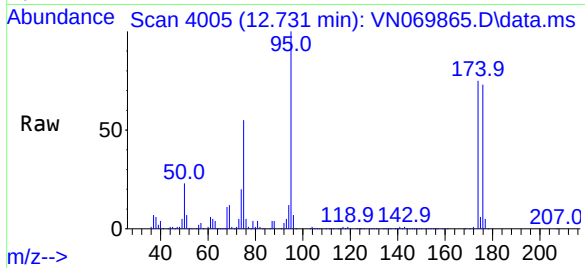

#81
trans-1,4-Dichloro-2-butene
Concen: 76.203 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55


Tgt Ion: 75 Resp: 637000
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#

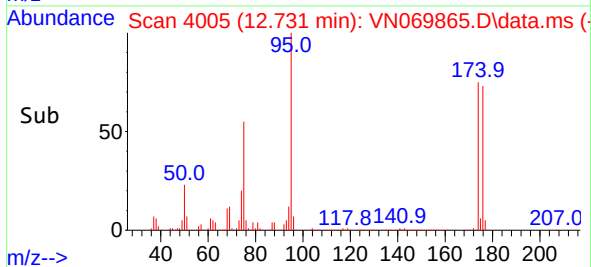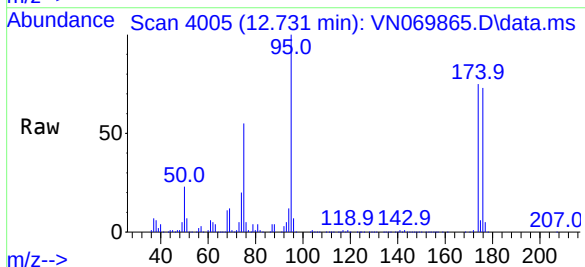






#93
1,2,4-Trichlorobenzene
Concen: 2.891 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206



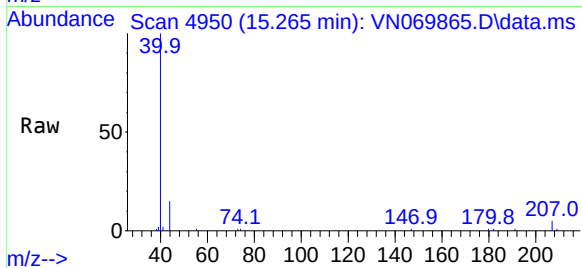



Tgt Ion:180 Resp: 216
Ion Ratio Lower Upper
180 100
182 215.3 48.3 144.9#
145 0.0 14.5 43.5#



#95
Naphthalene
Concen: 4.018 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55


Tgt Ion:128 Resp: 1623
Ion Ratio Lower Upper
128 100
127 5.5 10.5 15.7#
129 0.0 8.7 13.1#

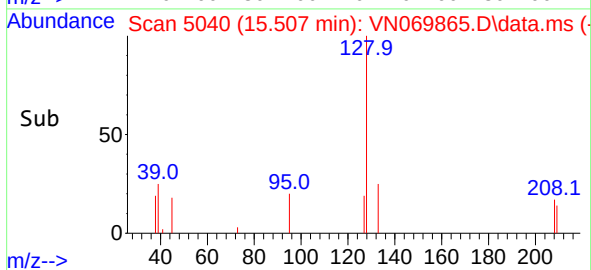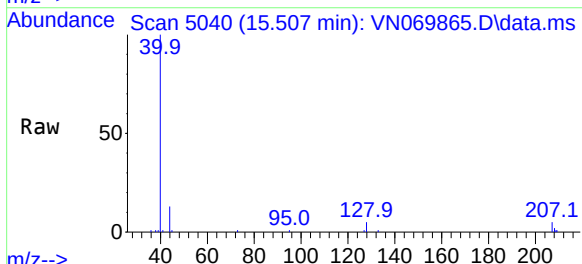



#96
1,2,3-Trichlorobenzene
Concen: 2.473 ug/l
RT: 15.694 min Scan# 51
Delta R.T. -0.008 min
Lab File: VN069865.D
Acq: 8 Dec 2021 16:55

Instrument :
MSVOA_N
ClientSampleId :
RE114D2-20211206

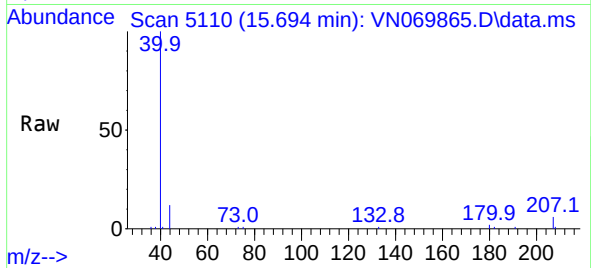

Tgt Ion:180 Resp: 578
Ion Ratio Lower Upper
180 100
182 42.2 47.4 142.2#
145 0.0 15.0 45.1#

