

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120821\
 Data File : VN069885.D
 Acq On : 9 Dec 2021 2:13
 Operator : JC/MD
 Sample : PB141231ZHE#10
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB141231ZHE#10

Quant Time: Dec 09 11:54:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	8.088	168	1378840	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2540855	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2815123	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	1110560	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	1064676	50.010	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 100.020%	
35) Dibromofluoromethane	8.024	113	746398	46.898	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 93.800%	
50) Toluene-d8	10.440	98	3329901	52.107	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 104.220%	
62) 4-Bromofluorobenzene	12.731	95	1336405	57.724	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 115.440%	
Target Compounds						Qvalue
11) Tert butyl alcohol	5.312	59	3647	0.906	ug/l	# 71
16) Acetone	4.291	43	86573	6.760	ug/l	98
18) Methyl Acetate	4.862	43	44562	1.153	ug/l	95
20) Methylene Chloride	5.101	84	44068	2.588	ug/l	91
25) 2-Butanone	7.348	43	19399	1.115	ug/l	92
29) Tetrahydrofuran	7.699	42	4307	0.408	ug/l	# 52
31) Cyclohexane	8.088	56	35767	1.207	ug/l	# 32
36) 1,1-Dichloropropene	8.086	75	117990	4.878	ug/l	# 49
37) Ethyl Acetate	7.348	43	19399	0.539	ug/l	# 70
38) Carbon Tetrachloride	8.088	117	140991	5.944	ug/l	# 16
43) Isopropyl Acetate	8.563	43	213144	4.001	ug/l	# 80
45) 1,2-Dichloropropane	9.625	63	9981	0.503	ug/l	# 44
48) Methyl methacrylate	9.545	41	42146	1.695	ug/l	# 8
49) 1,4-Dioxane	9.563	88	136	0.305	ug/l	# 1
51) 4-Methyl-2-Pentanone	10.330	43	35843	1.037	ug/l	90
53) t-1,3-Dichloropropene	10.714	75	102	2.797	ug/l	# 43
54) cis-1,3-Dichloropropene	10.245	75	232141	9.159	ug/l	# 71
56) Ethyl methacrylate	10.706	69	773	2.301	ug/l	# 24
57) 1,3-Dichloropropane	11.089	76	138588	4.322	ug/l	# 43
59) 2-Hexanone	11.089	43	2431640	93.007	ug/l	# 48
60) Dibromochloromethane	11.492	129	1658	2.457	ug/l	# 11
71) Bromoform	12.742	173	1122	2.793	ug/l	# 1
74) N-amyl acetate	12.197	43	98907	2.263	ug/l	# 52
76) 1,2,3-Trichloropropane	12.731	75	747326	23.465	ug/l	# 1
80) 1,3,5-Trimethylbenzene	13.055	105	24087	0.303	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.731	75	747326	74.622	ug/l	# 5
93) 1,2,4-Trichlorobenzene	15.265	180	1613	2.961	ug/l	90
95) Naphthalene	15.509	128	6638	4.098	ug/l	# 93
96) 1,2,3-Trichlorobenzene	15.692	180	818	2.479	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120821\
Data File : VN069885.D
Acq On : 9 Dec 2021 2:13
Operator : JC/MD
Sample : PB141231ZHE#10
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10

Quant Time: Dec 09 11:54:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 03 08:46:47 2021
Response via : Initial Calibration




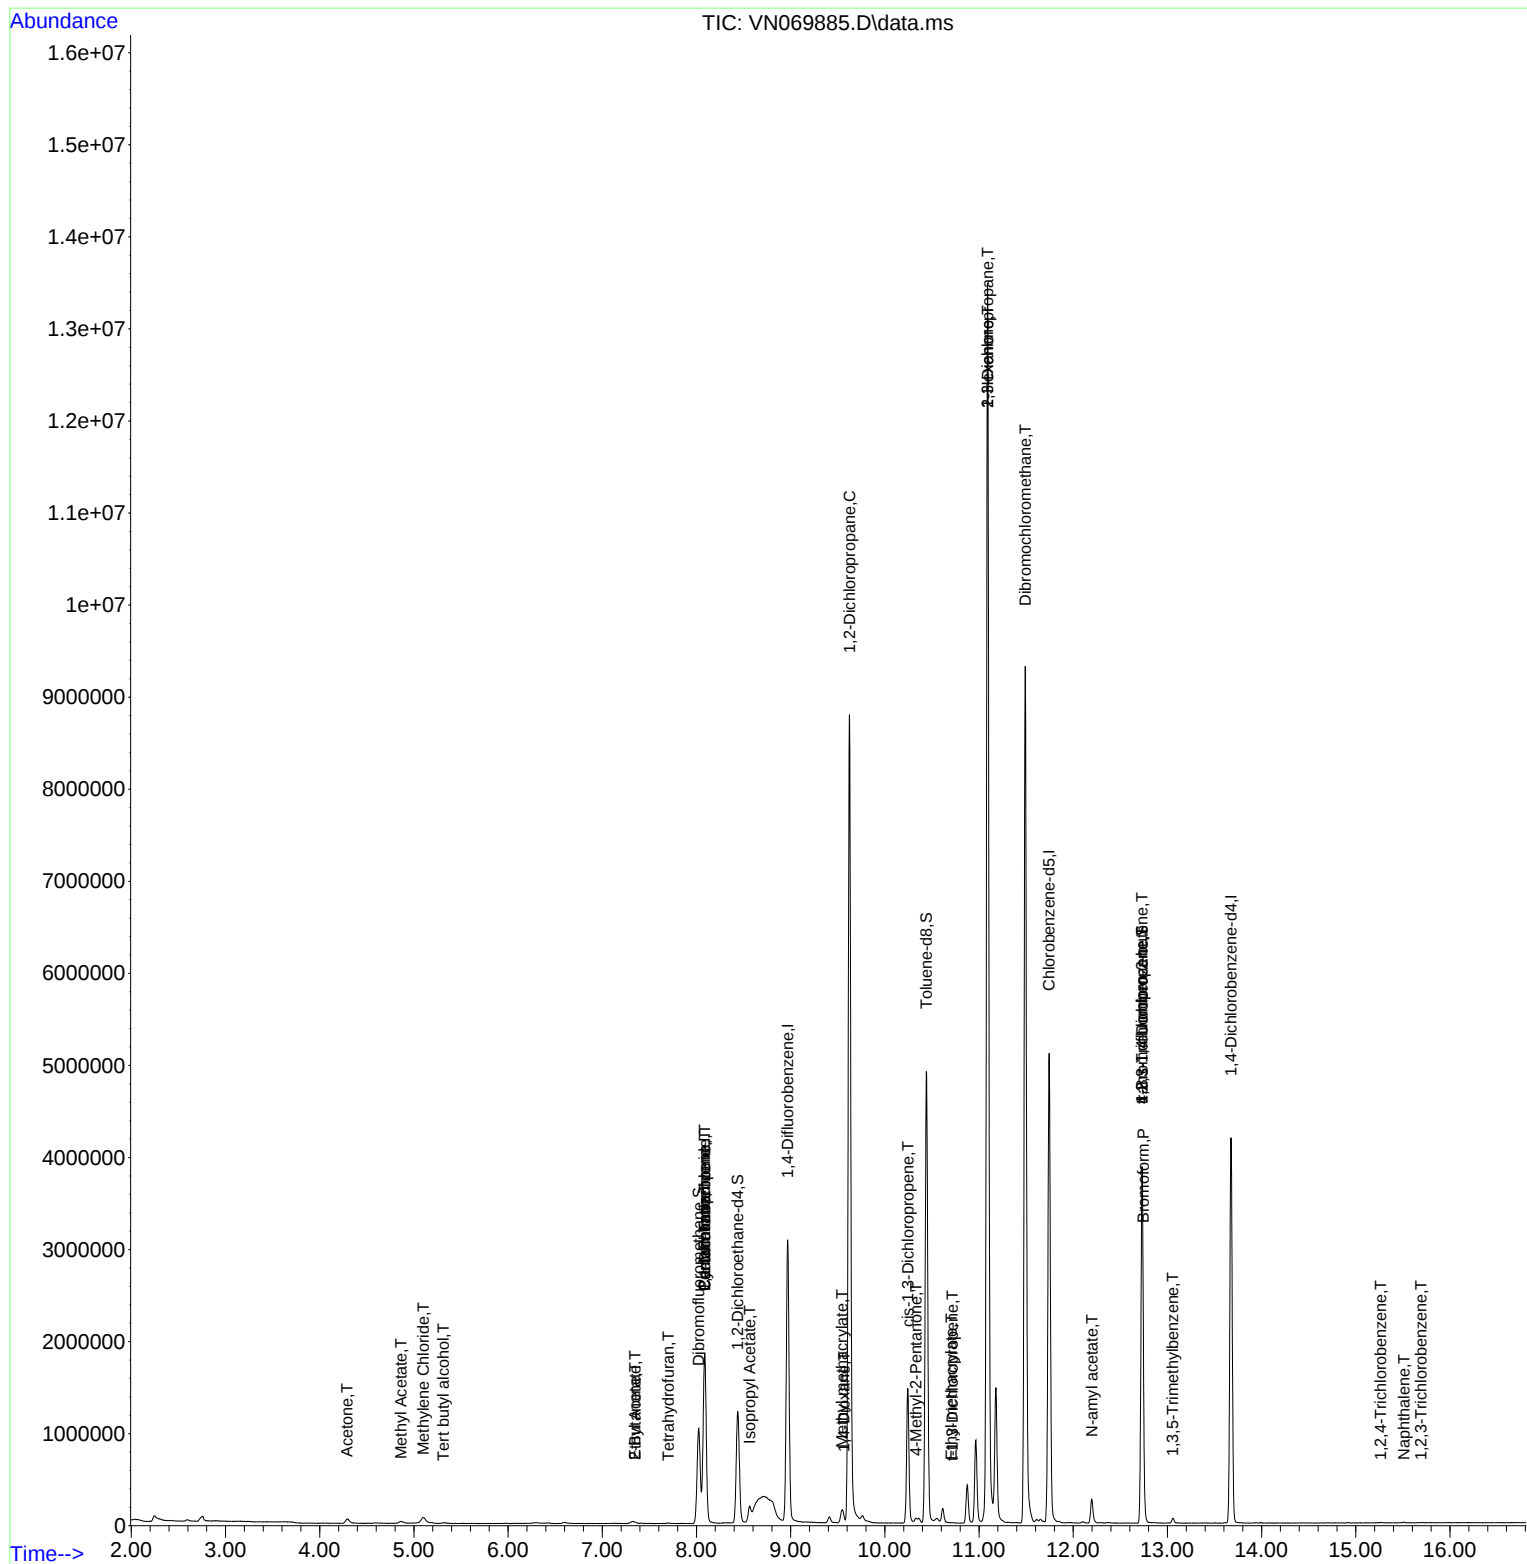




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion:168 Resp: 1378840
Ion Ratio Lower Upper
168 100
99 59.8 41.3 61.9

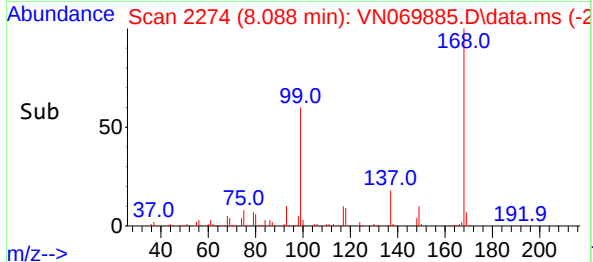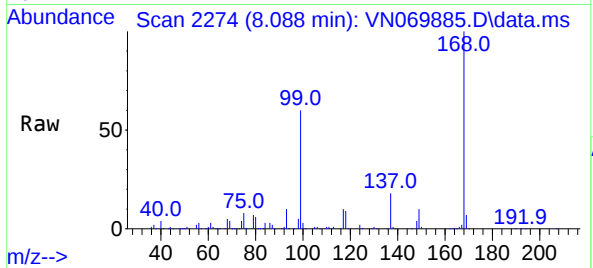

#11
Tert butyl alcohol
Concen: 0.906 ug/l
RT: 5.312 min Scan# 1239
Delta R.T. -0.078 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 59 Resp: 3647
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


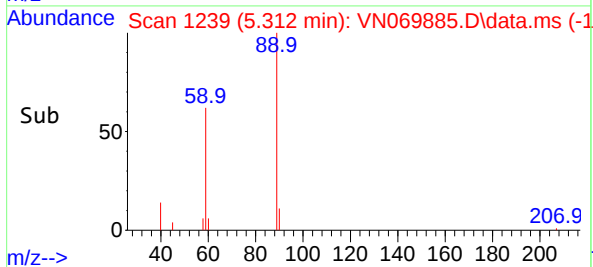

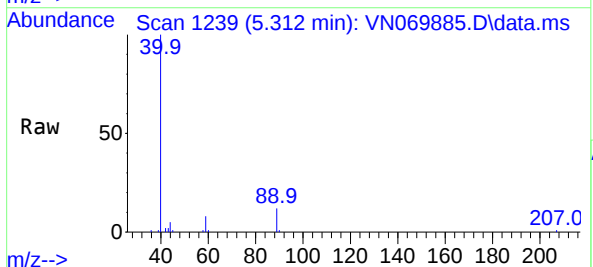




#16
Acetone
Concen: 6.760 ug/l
RT: 4.291 min Scan# 858
Delta R.T. 0.000 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion: 43 Resp: 86573
Ion Ratio Lower Upper
43 100
58 27.9 23.1 34.7

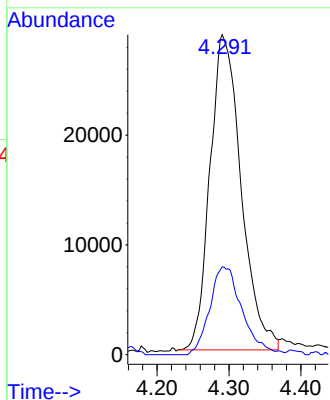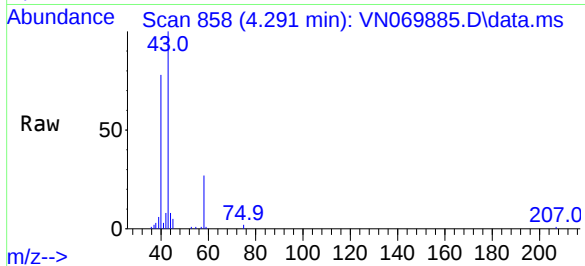

#18
Methyl Acetate
Concen: 1.153 ug/l
RT: 4.862 min Scan# 1071
Delta R.T. 0.005 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 43 Resp: 44562
Ion Ratio Lower Upper
43 100
74 21.6 19.4 29.2


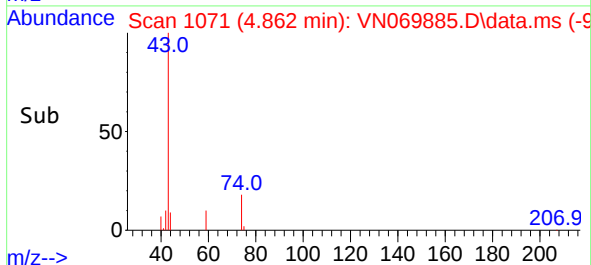
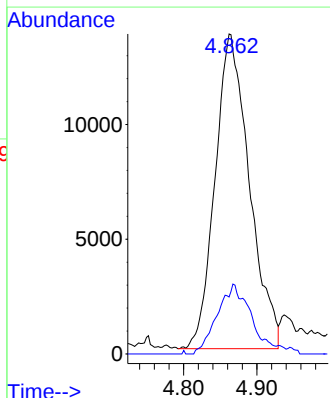
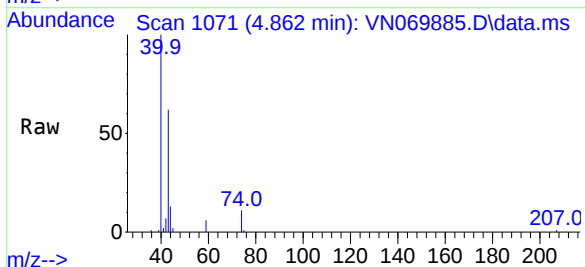


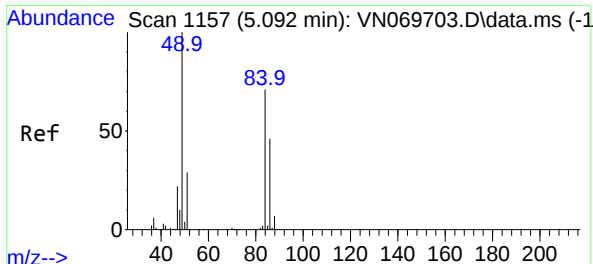

#20
Methylene Chloride
Concen: 2.588 ug/l
RT: 5.101 min Scan# 1157
Delta R.T. 0.008 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion:	84	Resp:	44068
Ion	Ratio	Lower	Upper
84	100		
49	132.3	93.5	140.3
51	37.7	29.4	44.2
86	61.8	53.0	79.4

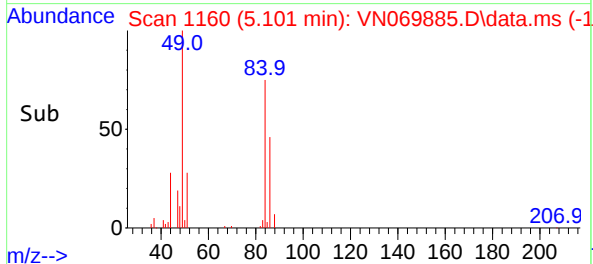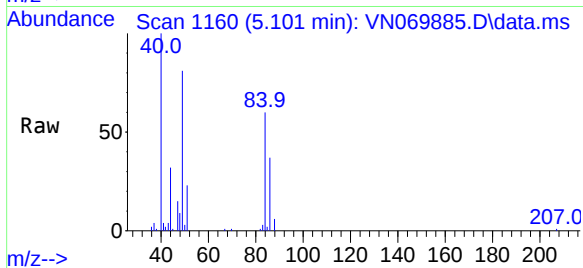

#25
2-Butanone
Concen: 1.115 ug/l
RT: 7.348 min Scan# 1998
Delta R.T. 0.011 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion:	43	Resp:	19399
Ion	Ratio	Lower	Upper
43	100		
72	23.0	21.7	32.5

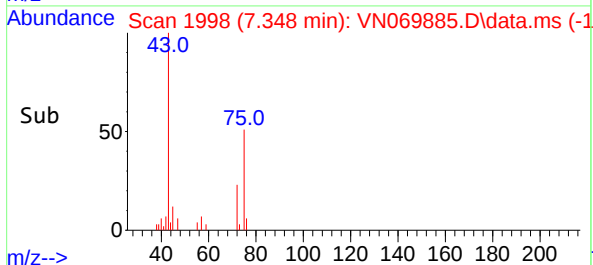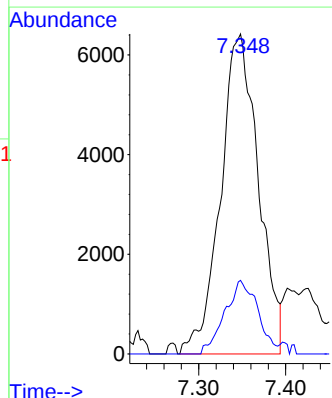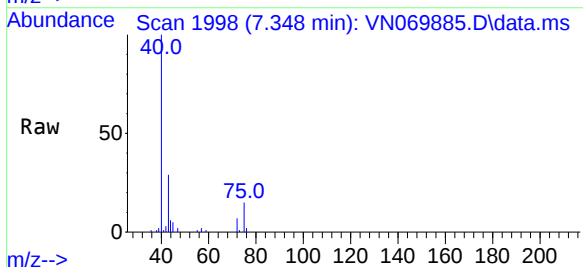



#29

Tetrahydrofuran

Concen: 0.408 ug/l

RT: 7.699 min Scan# 21

Delta R.T. 0.014 min

Lab File: VN069885.D

Acq: 9 Dec 2021 2:13

Instrument :

MSVOA_N

ClientSampleId :

PB141231ZHE#10





Tgt Ion: 42 Resp: 4307

Ion Ratio Lower Upper

42 100

72 14.0 36.3 54.5#

71 12.4 34.7 52.1#

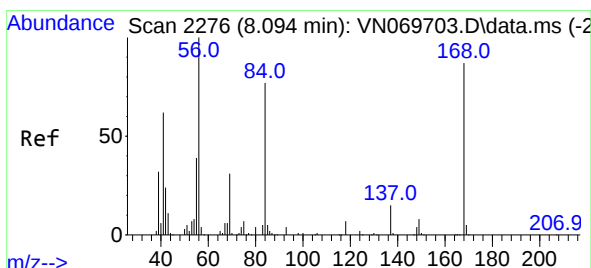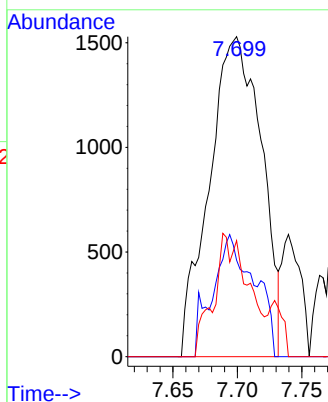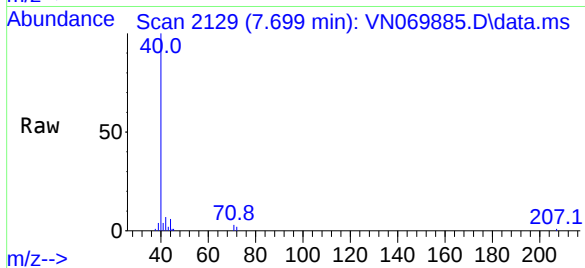

#31

Cyclohexane

Concen: 1.207 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. -0.005 min

Lab File: VN069885.D

Acq: 9 Dec 2021 2:13




Tgt Ion: 56 Resp: 35767


Ion Ratio Lower Upper

56 100

69 152.2 27.1 40.7#

84 107.1 73.4 110.0


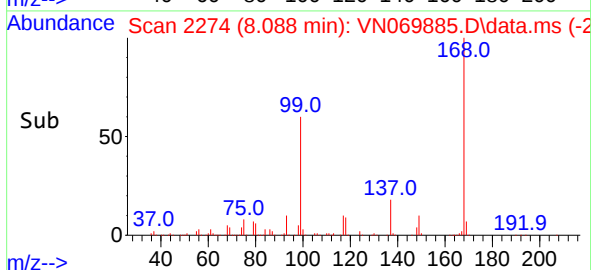
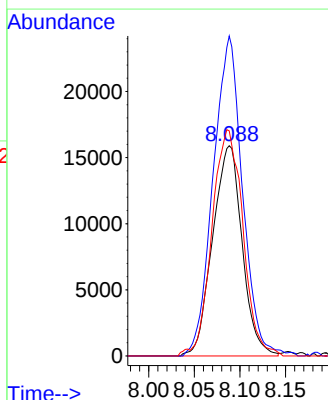
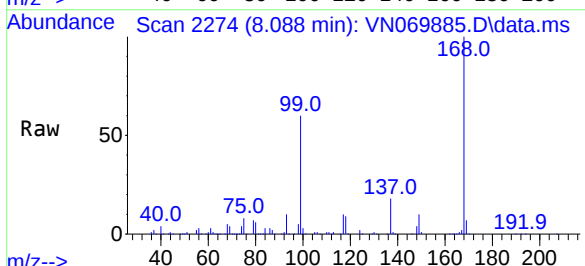




#33
1,2-Dichloroethane-d4
Concen: 50.010 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. 0.000 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion: 65 Resp: 1064676
Ion Ratio Lower Upper
65 100
67 51.0 0.0 103.0

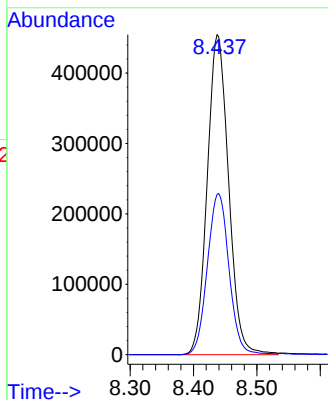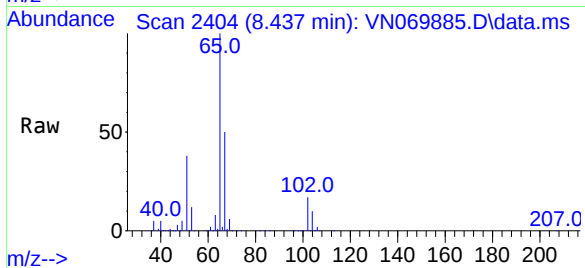

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. -0.000 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13


Tgt Ion: 114 Resp: 2540855
Ion Ratio Lower Upper
114 100
63 23.3 0.0 37.8
88 16.1 0.0 27.4

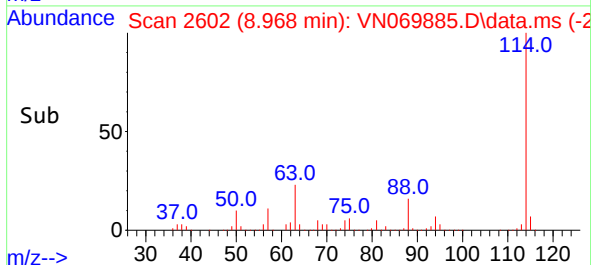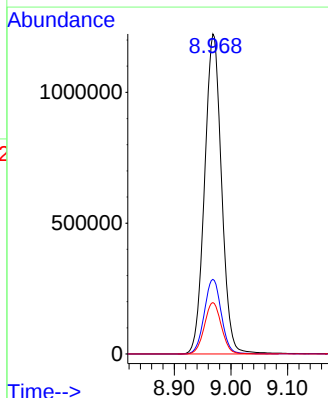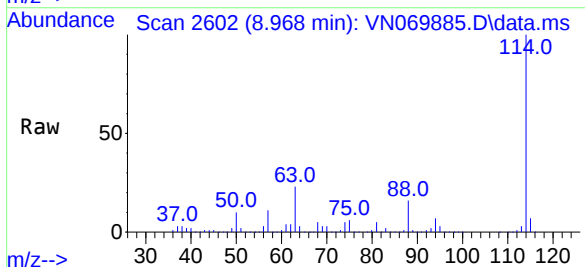






#35
Dibromofluoromethane
Concen: 46.898 ug/l
RT: 8.024 min Scan# 211
Delta R.T. 0.000 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10



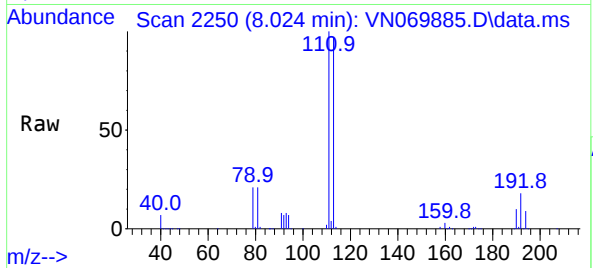



Tgt Ion:113 Resp: 746398
Ion Ratio Lower Upper
113 100
111 102.9 82.2 123.2
192 18.7 16.9 25.3

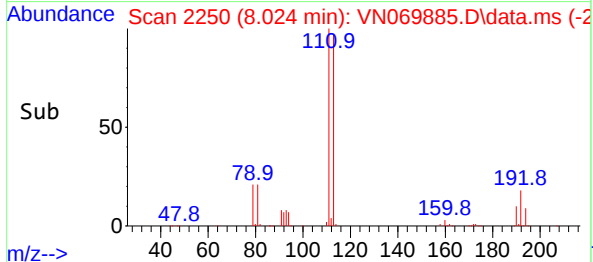

#36
1,1-Dichloropropene
Concen: 4.878 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.137 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 75 Resp: 117990
Ion Ratio Lower Upper
75 100
110 9.0 18.4 55.2#
77 0.0 24.4 36.6#

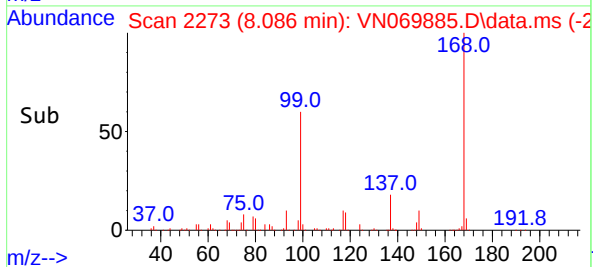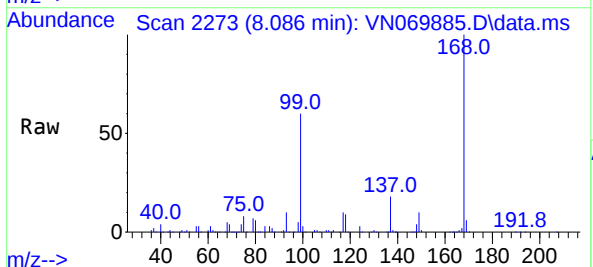




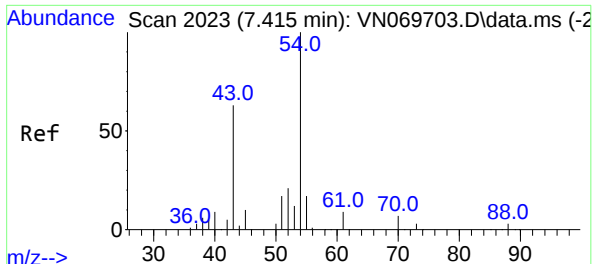


#37
Ethyl Acetate
Concen: 0.539 ug/l
RT: 7.348 min Scan# 1998
Delta R.T. -0.067 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Instrument : MSVOA_N
ClientSampleId : PB141231ZHE#10

Tgt Ion: 43 Resp: 19399




Ion	Ratio	Lower	Upper
43	100		
61	1.1	11.5	17.3#
70	0.0	7.9	11.9#

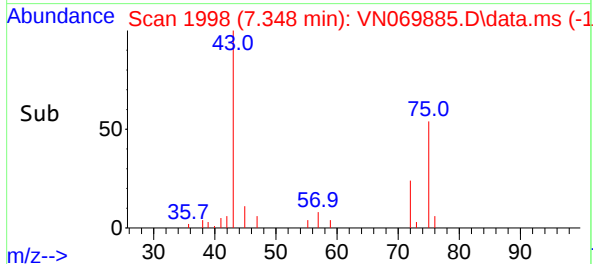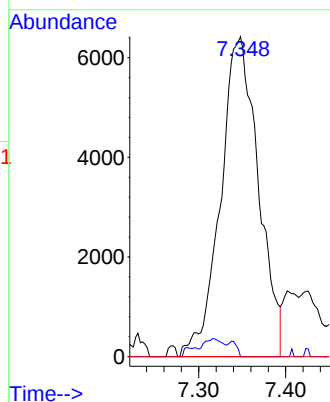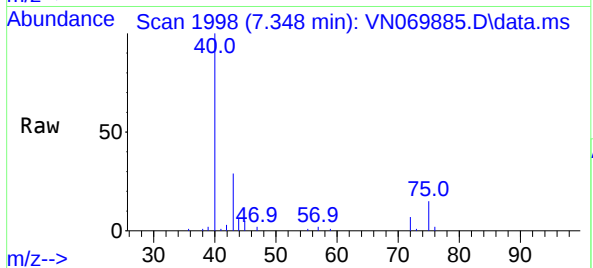


#38
Carbon Tetrachloride
Concen: 5.944 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 117 Resp: 140991

Ion	Ratio	Lower	Upper
117	100		
119	4.5	76.1	114.1#
121	0.0	24.2	36.2#


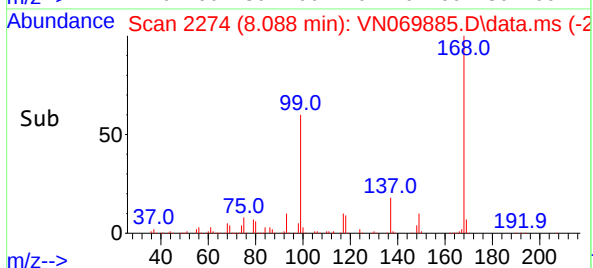
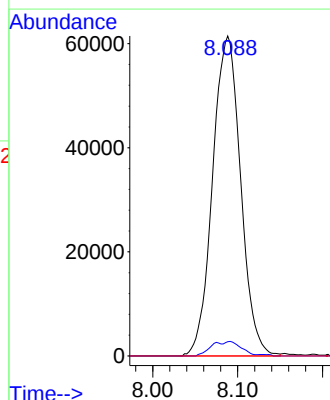
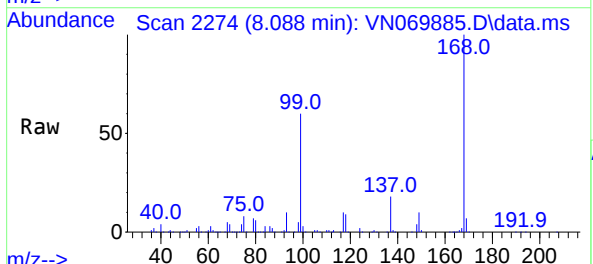




#43
Isopropyl Acetate
Concen: 4.001 ug/l
RT: 8.563 min Scan# 24
Delta R.T. 0.000 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion: 43 Resp: 213144
Ion Ratio Lower Upper
43 100
61 13.9 20.4 30.6#
87 8.0 11.2 16.8#

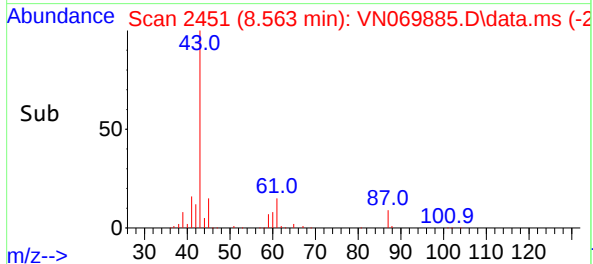

#45
1,2-Dichloropropane
Concen: 0.503 ug/l
RT: 9.625 min Scan# 2847
Delta R.T. 0.134 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 63 Resp: 9981
Ion Ratio Lower Upper
63 100
65 0.0 24.7 37.1#


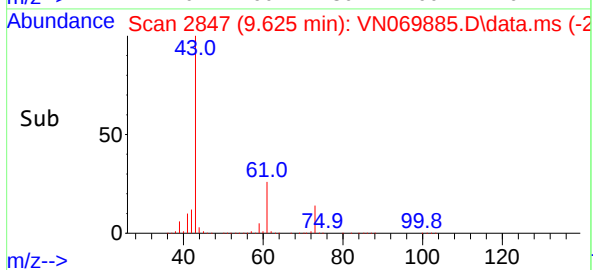

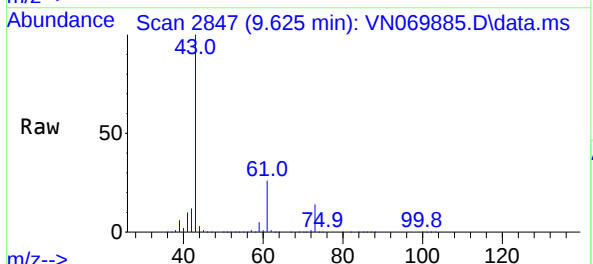




#48
Methyl methacrylate
Concen: 1.695 ug/l
RT: 9.545 min Scan# 21
Delta R.T. -0.016 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion: 41 Resp: 42146
Ion Ratio Lower Upper
41 100
69 0.2 72.4 108.6#
39 0.0 58.4 87.6#

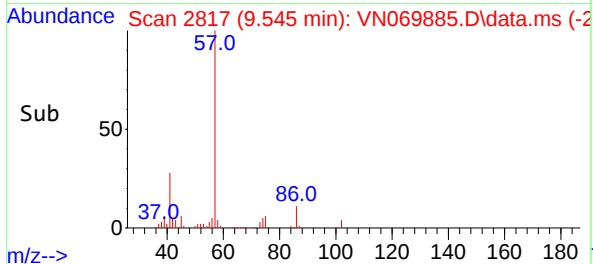

#49
1,4-Dioxane
Concen: 0.305 ug/l
RT: 9.563 min Scan# 2824
Delta R.T. -0.008 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 88 Resp: 136
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 4748.5 50.6 75.8#


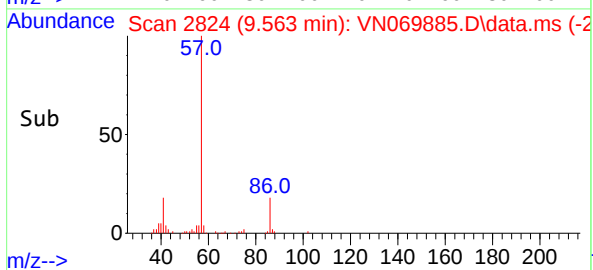

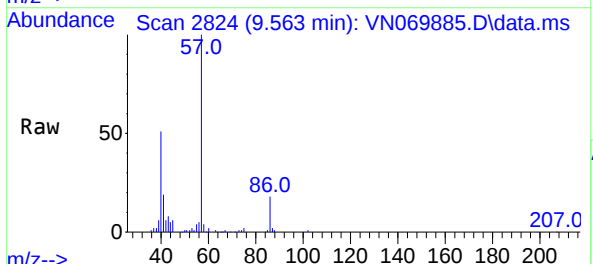




#50
Toluene-d8
Concen: 52.107 ug/l
RT: 10.440 min Scan# 3152
Delta R.T. -0.003 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion: 98 Resp: 3329901
Ion Ratio Lower Upper
98 100
100 64.0 50.4 75.6

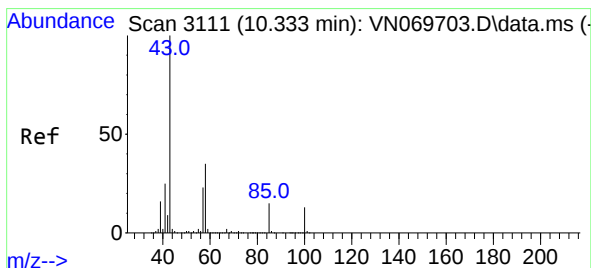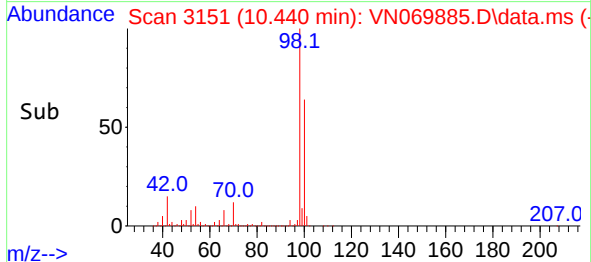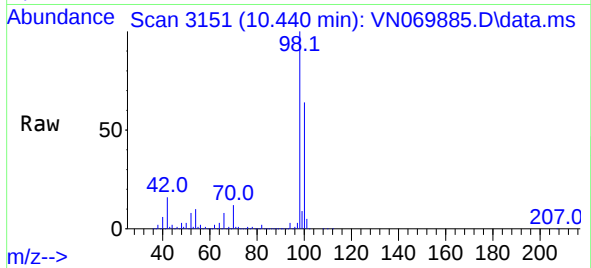

#51
4-Methyl-2-Pentanone
Concen: 1.037 ug/l
RT: 10.330 min Scan# 3110
Delta R.T. -0.003 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 43 Resp: 35843
Ion Ratio Lower Upper
43 100
58 31.9 30.4 45.6


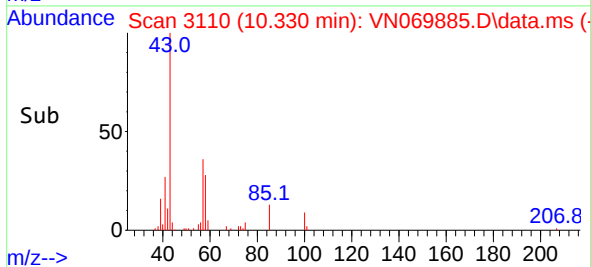

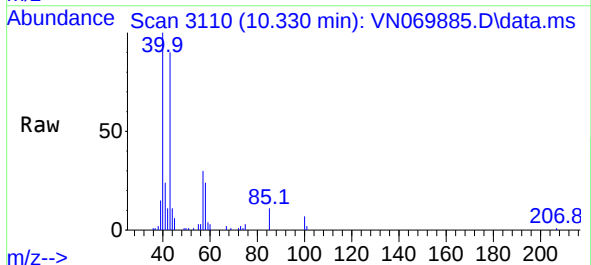




#53
t-1,3-Dichloropropene
Concen: 2.797 ug/l
RT: 10.714 min Scan# 31
Delta R.T. -0.005 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion: 75 Resp: 102
Ion Ratio Lower Upper
75 100
77 0.0 25.6 38.4#

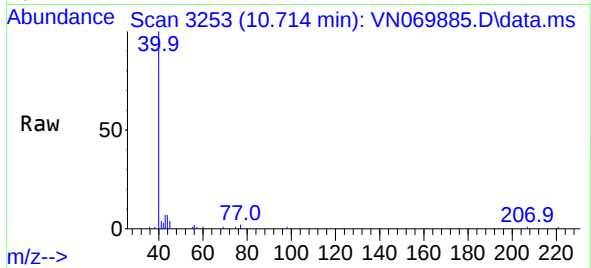

#54
cis-1,3-Dichloropropene
Concen: 9.159 ug/l
RT: 10.245 min Scan# 3078
Delta R.T. 0.054 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 75 Resp: 232141
Ion Ratio Lower Upper
75 100
77 0.7 26.4 39.6#
39 44.8 42.5 63.7


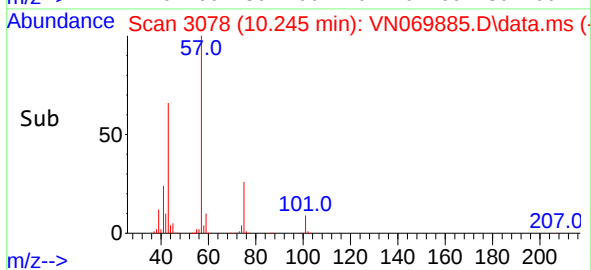

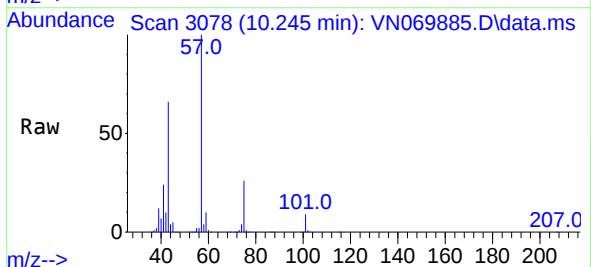




#56
Ethyl methacrylate
Concen: 2.301 ug/l
RT: 10.706 min Scan# 31
Delta R.T. -0.056 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion: 69 Resp: 773
Ion Ratio Lower Upper
69 100
41 0.0 51.4 77.0#
39 0.0 34.6 52.0#

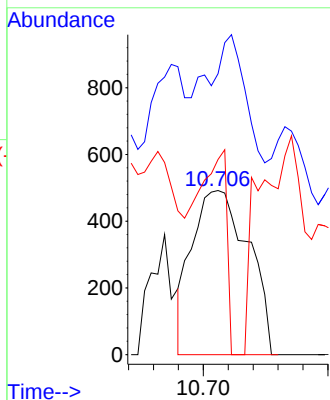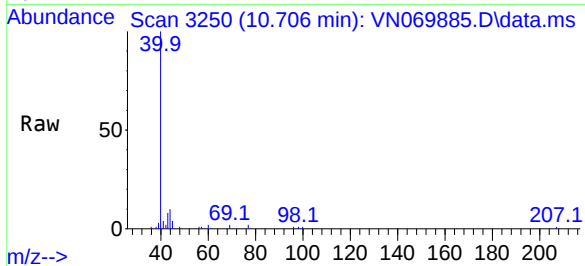

#57
1,3-Dichloropropane
Concen: 4.322 ug/l
RT: 11.089 min Scan# 3393
Delta R.T. 0.043 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 76 Resp: 138588
Ion Ratio Lower Upper
76 100
78 0.4 25.7 38.5#


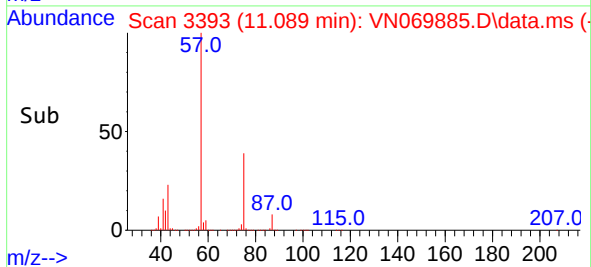
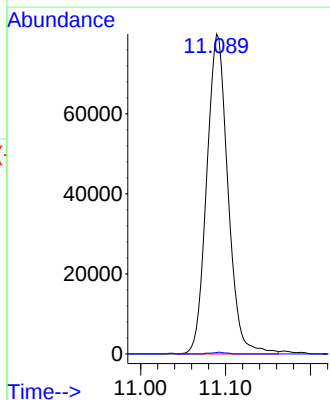
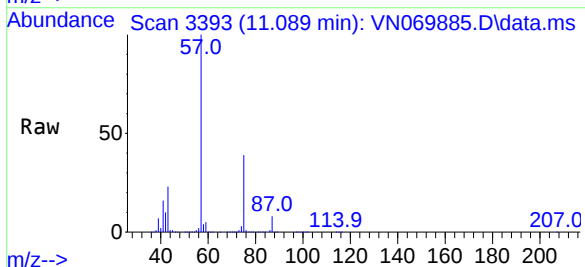




#59
2-Hexanone
Concen: 93.007 ug/l
RT: 11.089 min Scan# 31
Delta R.T. 0.002 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion: 43 Resp: 2431640
Ion Ratio Lower Upper
43 100
58 16.4 26.9 80.7#

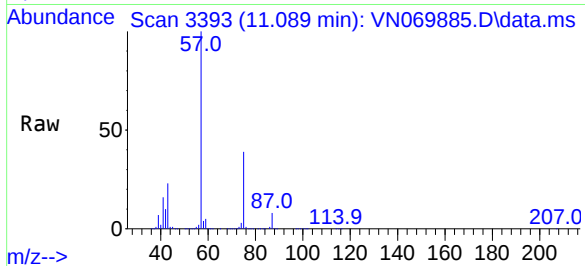

#60
Dibromochloromethane
Concen: 2.457 ug/l
RT: 11.492 min Scan# 3543
Delta R.T. 0.252 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion:129 Resp: 1658
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#


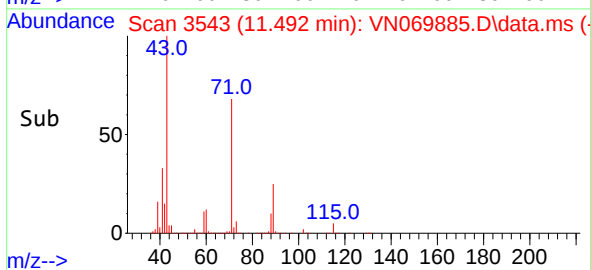

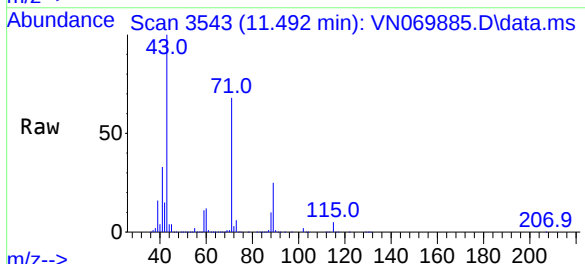




#62
4-Bromofluorobenzene
Concen: 57.724 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion: 95 Resp: 1336405
Ion Ratio Lower Upper
95 100
174 76.0 0.0 187.2
176 73.3 0.0 181.4

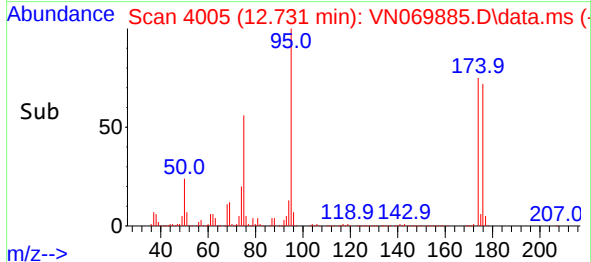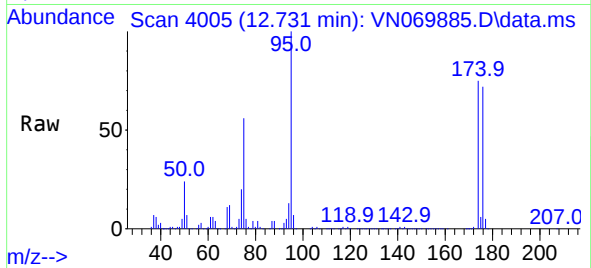

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.002 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 117 Resp: 2815123
Ion Ratio Lower Upper
117 100
82 60.0 42.4 63.6
119 32.2 25.4 38.2


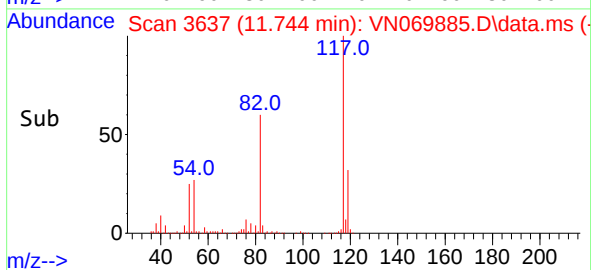




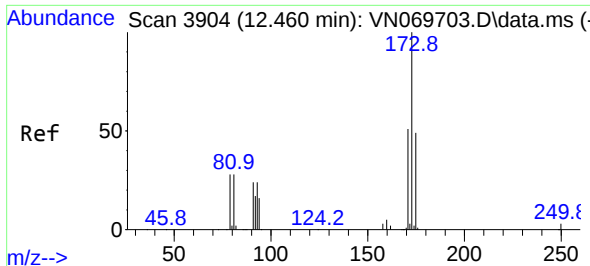

#71
Bromoform
Concen: 2.793 ug/l
RT: 12.742 min Scan# 4009
Delta R.T. 0.282 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion:173 Resp: 1122
Ion Ratio Lower Upper
173 100
175 6566.1 24.2 72.6#
254 0.0 0.0 0.0

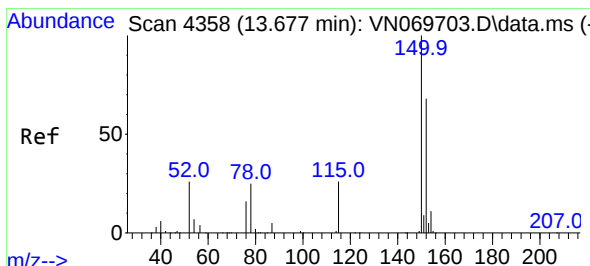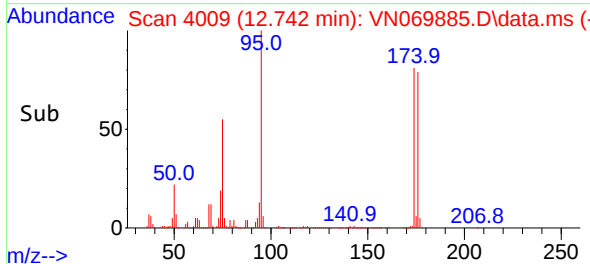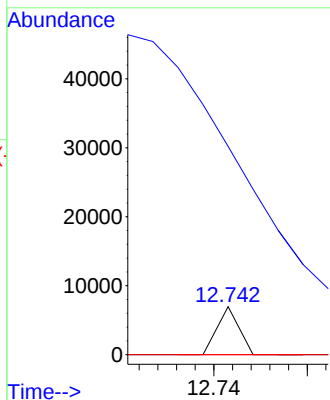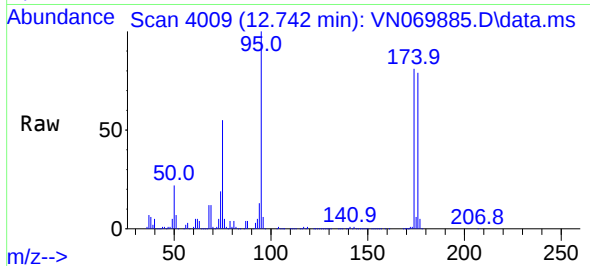

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.003 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion:152 Resp: 1110560
Ion Ratio Lower Upper
152 100
115 60.8 27.5 82.5
150 157.3 0.0 344.4


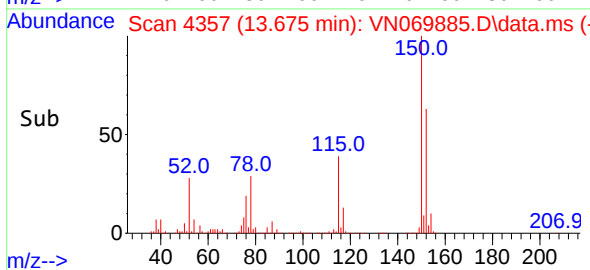
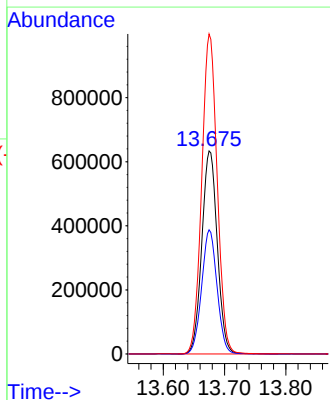
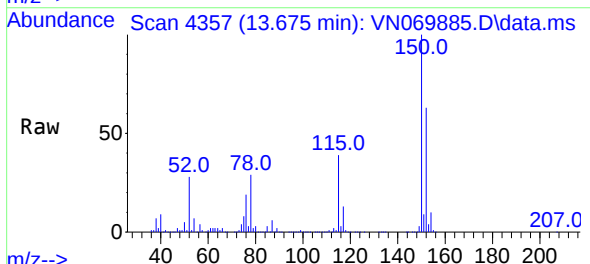




#74
N-amy1 acetate
Concen: 2.263 ug/l
RT: 12.197 min Scan# 31
Delta R.T. -0.190 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion: 43	Resp: 98907
Ion Ratio	Lower Upper
43 100	
70 2.2	33.4 50.0#
55 4.5	19.3 28.9#
61 8.5	18.5 27.7#

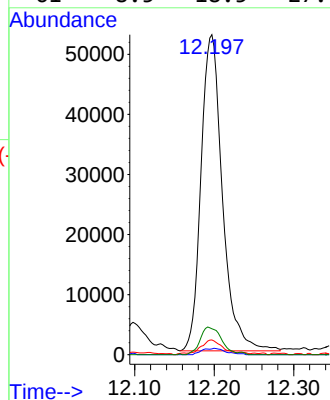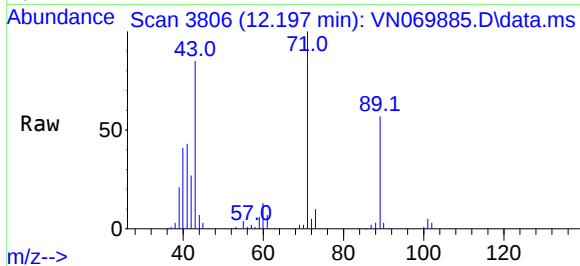

#76
1,2,3-Trichloropropane
Concen: 23.465 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.150 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Tgt Ion: 75	Resp: 747326
Ion Ratio	Lower Upper
75 100	
77 1.0	82.6 247.8#


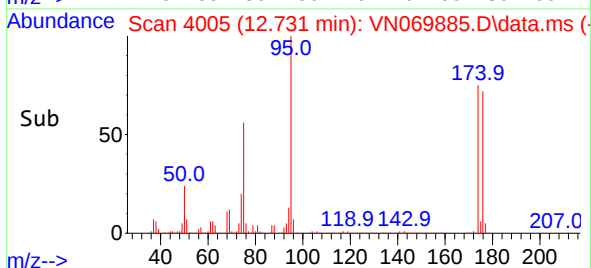
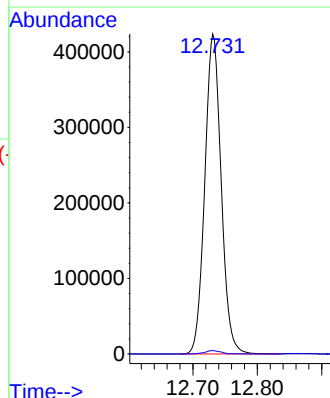
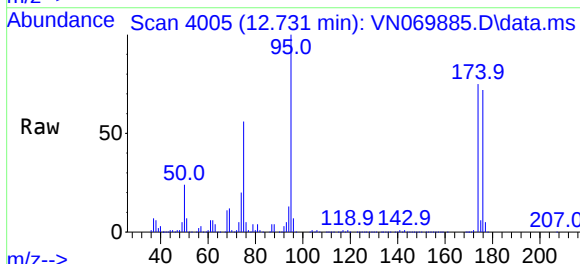




#80
1,3,5-Trimethylbenzene
Concen: 0.303 ug/l
RT: 13.055 min Scan# 41
Delta R.T. -0.005 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13




Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10


Tgt Ion:105 Resp: 24087
Ion Ratio Lower Upper
105 100
120 49.4 24.6 73.6

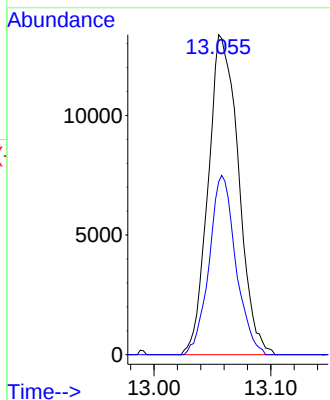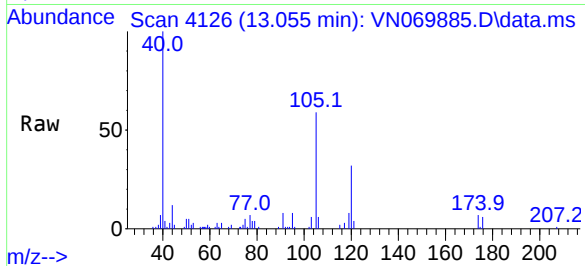

#81
trans-1,4-Dichloro-2-butene
Concen: 74.622 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13


Tgt Ion: 75 Resp: 747326
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#

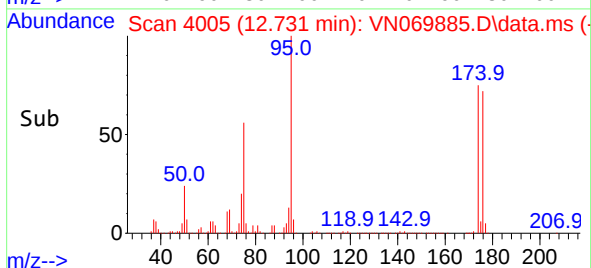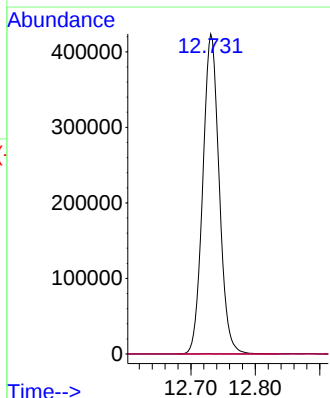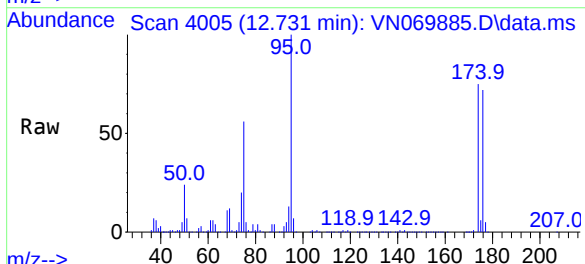






#93
1,2,4-Trichlorobenzene
Concen: 2.961 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13

Instrument :
MSVOA_N
ClientSampleId :
PB141231ZHE#10







Tgt Ion:180 Resp: 1613
Ion Ratio Lower Upper
180 100
182 90.4 48.3 144.9
145 16.9 14.5 43.5



#95
Naphthalene
Concen: 4.098 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN069885.D
Acq: 9 Dec 2021 2:13


Tgt Ion:128 Resp: 6638
Ion Ratio Lower Upper
128 100
127 11.6 10.5 15.7
129 7.2 8.7 13.1#

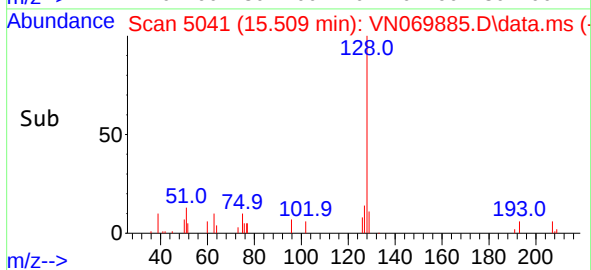



#96
 1,2,3-Trichlorobenzene
 Concen: 2.479 ug/l
 RT: 15.692 min Scan# 51
 Delta R.T. -0.010 min
 Lab File: VN069885.D
 Acq: 9 Dec 2021 2:13

Instrument :
 MSVOA_N
 ClientSampleId :
 PB141231ZHE#10

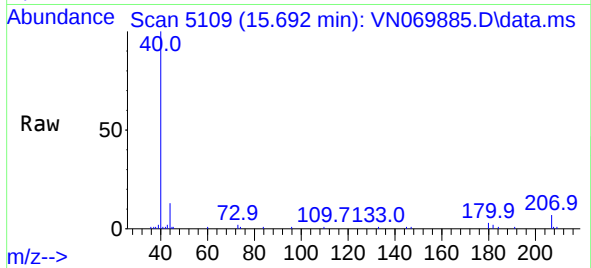

Tgt Ion:180 Resp: 818
 Ion Ratio Lower Upper
 180 100
 182 89.4 47.4 142.2
 145 17.2 15.0 45.1

