

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120821\
 Data File : VN069900.D
 Acq On : 9 Dec 2021 8:35
 Operator : JC/MD
 Sample : M4965-15
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BLUE-CONCRETE-COMP

Quant Time: Dec 09 12:03:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	1246425	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2338213	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2644833	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	1093657	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	1008931	52.426	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 104.860%			
35) Dibromofluoromethane	8.024	113	724693	49.480	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 98.960%			
50) Toluene-d8	10.440	98	3105956	52.815	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 105.620%			
62) 4-Bromofluorobenzene	12.731	95	1282300	60.187	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 120.380%			
Target Compounds					Qvalue	
11) Tert butyl alcohol	5.326	59	5022	1.381	ug/l #	71
16) Acetone	4.293	43	106163	9.170	ug/l	99
17) Carbon Disulfide	4.524	76	13088	0.427	ug/l	95
18) Methyl Acetate	4.867	43	43961	1.258	ug/l #	73
20) Methylene Chloride	5.100	84	42442	2.758	ug/l	87
25) 2-Butanone	7.345	43	18713	1.190	ug/l #	88
31) Cyclohexane	8.085	56	32360	1.208	ug/l #	33
36) 1,1-Dichloropropene	8.085	75	107627	4.835	ug/l #	49
38) Carbon Tetrachloride	8.085	117	126913	5.814	ug/l #	16
41) Methacrylonitrile	7.699	41	3306	0.213	ug/l #	35
43) Isopropyl Acetate	8.563	43	188956	3.854	ug/l #	82
48) Methyl methacrylate	9.544	41	52312	2.286	ug/l #	9
49) 1,4-Dioxane	9.625	88	1251	3.047	ug/l #	1
51) 4-Methyl-2-Pentanone	10.333	43	24682	0.776	ug/l #	85
53) t-1,3-Dichloropropene	10.725	75	91	2.797	ug/l	97
54) cis-1,3-Dichloropropene	10.242	75	204796	8.863	ug/l #	71
56) Ethyl methacrylate	10.703	69	555	2.296	ug/l #	24
57) 1,3-Dichloropropane	11.089	76	114356	3.875	ug/l #	43
59) 2-Hexanone	11.089	43	2050581	85.230	ug/l #	47
60) Dibromochloromethane	11.494	129	942	2.426	ug/l #	11
67) Ethyl Benzene	11.846	91	31989	0.328	ug/l #	86
68) m/p-Xylenes	11.945	106	36538	1.030	ug/l	90
69) o-Xylene	12.280	106	19258	0.539	ug/l	94
71) Bromoform	12.701	173	72	2.735	ug/l #	29
76) 1,2,3-Trichloropropane	12.731	75	723705	23.075	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	723705	73.448	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.396	105	35164	0.471	ug/l #	31
85) sec-Butylbenzene	13.396	105	35164	0.374	ug/l #	56
95) Naphthalene	15.504	128	737	3.998	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.708	180	146	2.444	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120821\
Data File : VN069900.D
Acq On : 9 Dec 2021 8:35
Operator : JC/MD
Sample : M4965-15
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP

Quant Time: Dec 09 12:03:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 03 08:46:47 2021
Response via : Initial Calibration




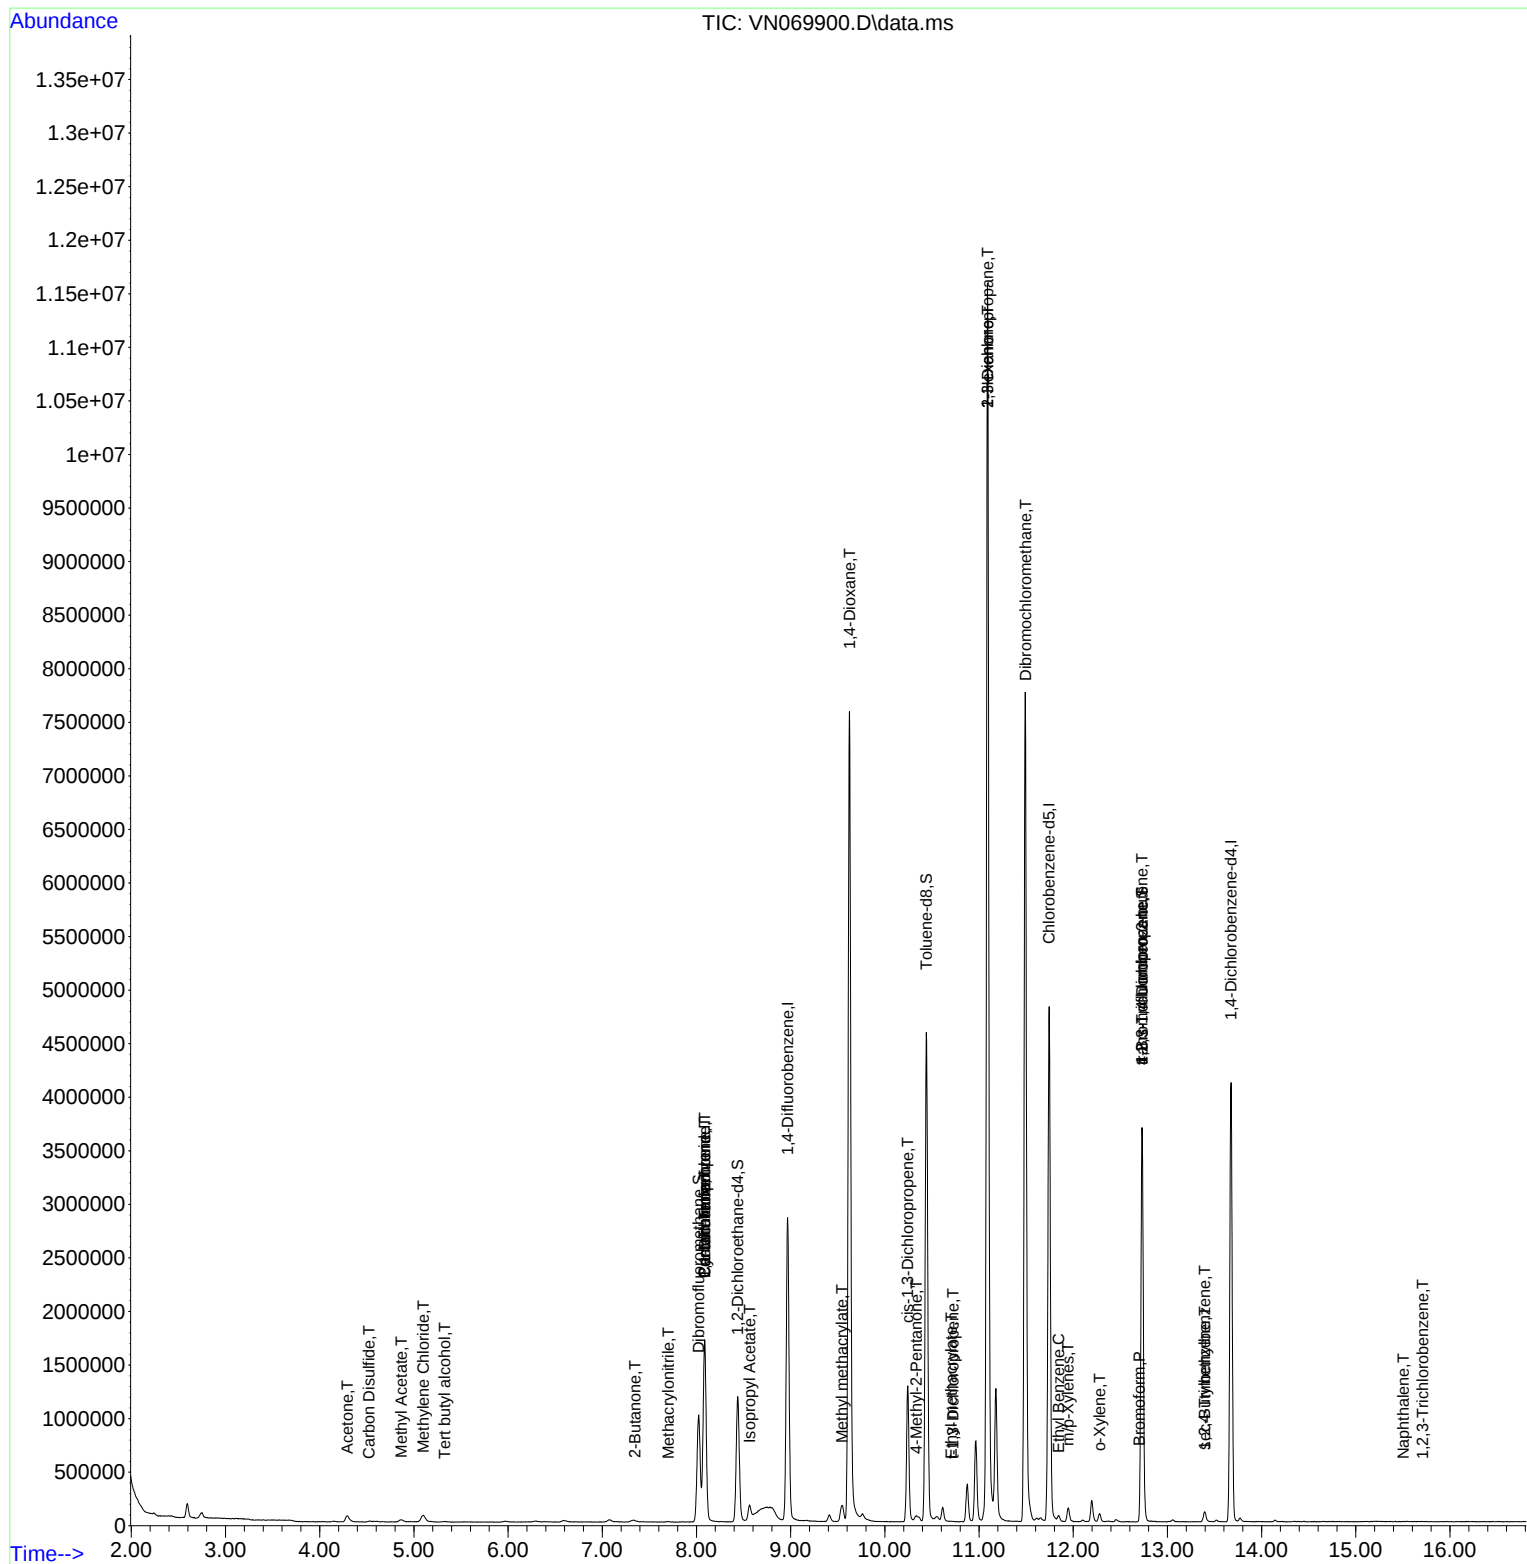


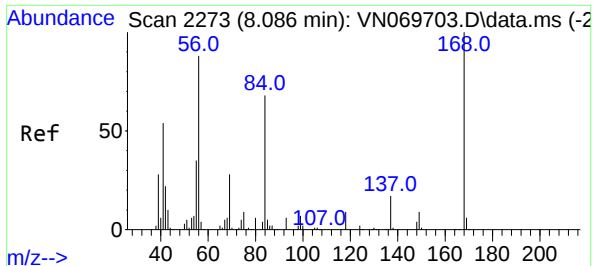

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion:168 Resp: 1246425
Ion Ratio Lower Upper
168 100
99 59.6 41.3 61.9

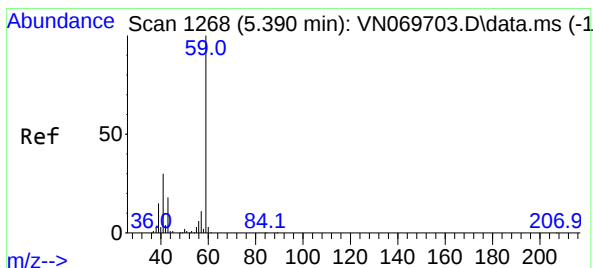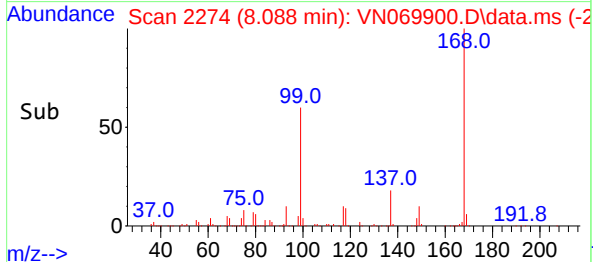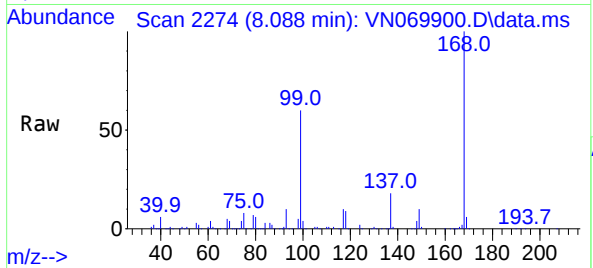

#11
Tert butyl alcohol
Concen: 1.381 ug/l
RT: 5.326 min Scan# 1244
Delta R.T. -0.064 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 59 Resp: 5022
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


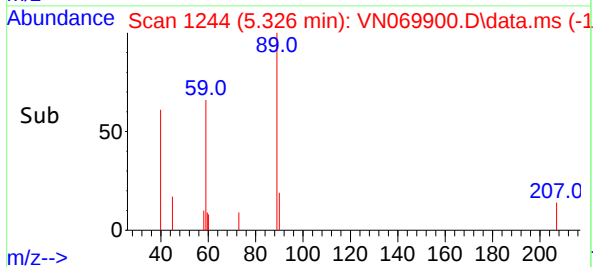

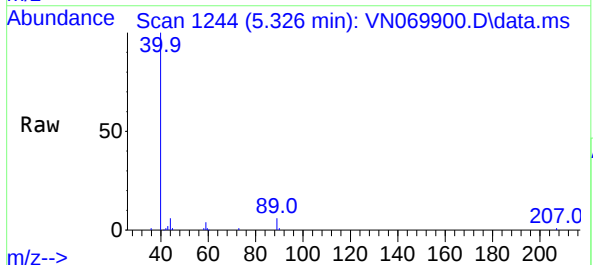




#16
Acetone
Concen: 9.170 ug/l
RT: 4.293 min Scan# 859
Delta R.T. 0.003 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion: 43 Resp: 106163
Ion Ratio Lower Upper
43 100
58 28.3 23.1 34.7

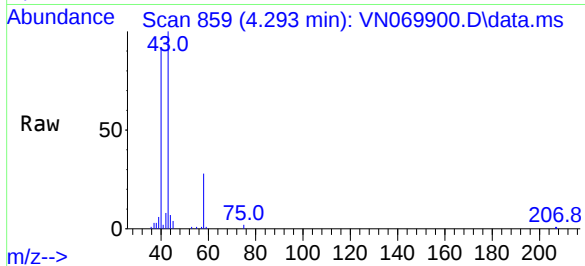

#17
Carbon Disulfide
Concen: 0.427 ug/l
RT: 4.524 min Scan# 945
Delta R.T. 0.000 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 76 Resp: 13088
Ion Ratio Lower Upper
76 100
78 7.6 7.5 11.3

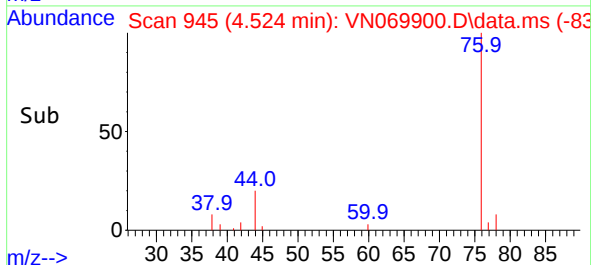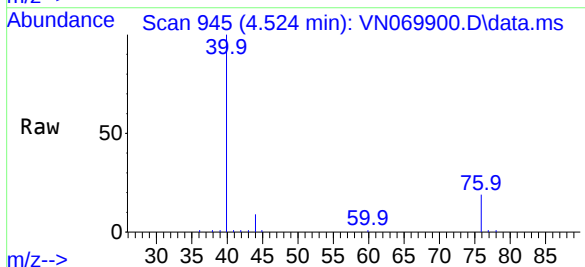

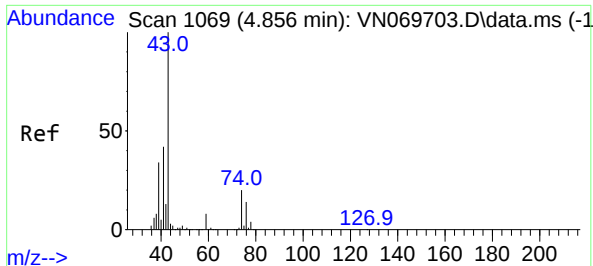

#18

Methyl Acetate

Concen: 1.258 ug/l

RT: 4.867 min Scan# 1160

Delta R.T. 0.011 min

Lab File: VN069900.D

Acq: 9 Dec 2021 8:35

Instrument :

MSVOA_N

ClientSampleId :





BLUE-CONCRETE-COMP

Tgt Ion: 43 Resp: 43961

Ion Ratio Lower Upper

43 100

74 11.0 19.4 29.2#

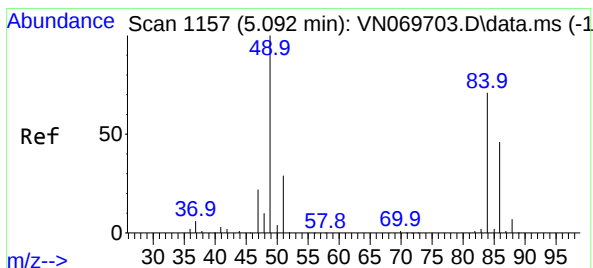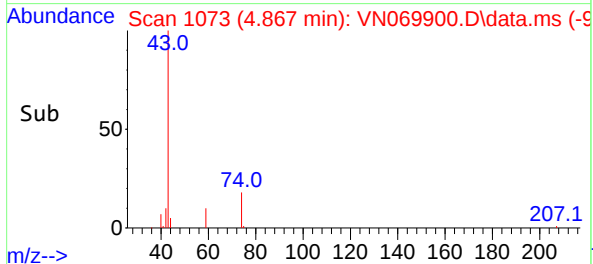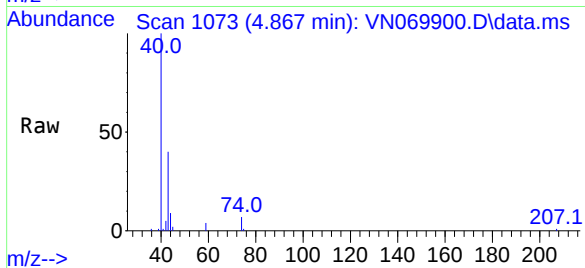

#20

Methylene Chloride

Concen: 2.758 ug/l

RT: 5.100 min Scan# 1160

Delta R.T. 0.008 min

Lab File: VN069900.D

Acq: 9 Dec 2021 8:35

Tgt Ion: 84 Resp: 42442




Ion Ratio Lower Upper


84 100

49 136.9 93.5 140.3

51 41.4 29.4 44.2

86 59.8 53.0 79.4


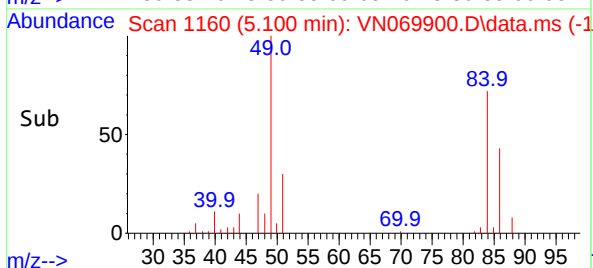
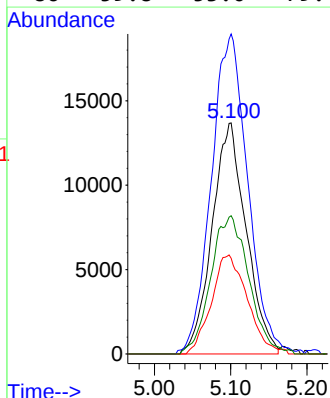
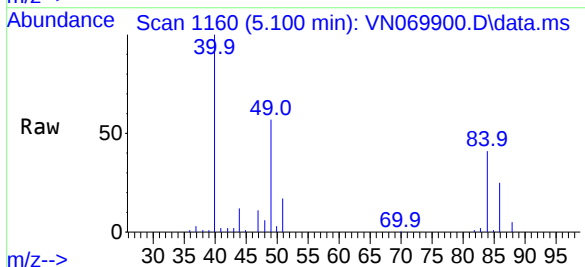


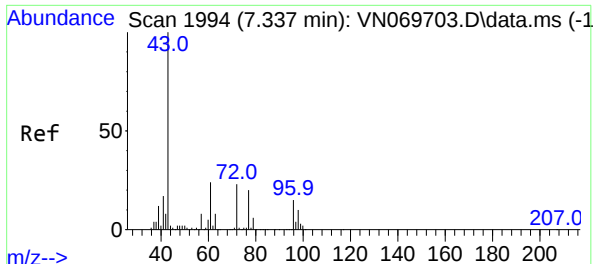

#25
2-Butanone
Concen: 1.190 ug/l
RT: 7.345 min Scan# 1994
Delta R.T. 0.008 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion: 43 Resp: 18713
Ion Ratio Lower Upper
43 100
72 20.7 21.7 32.5#

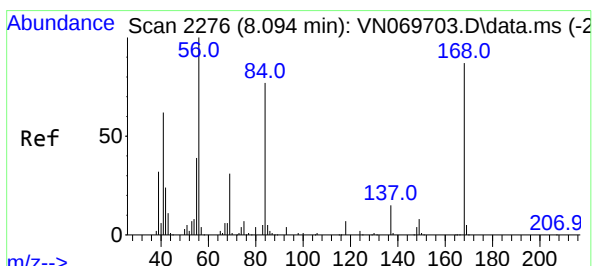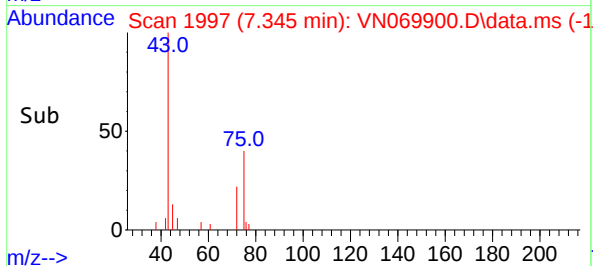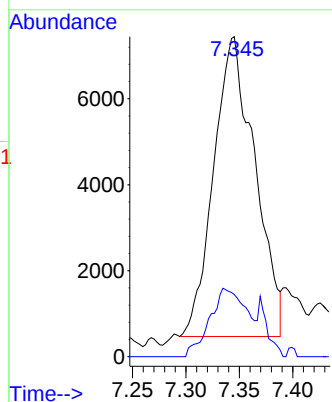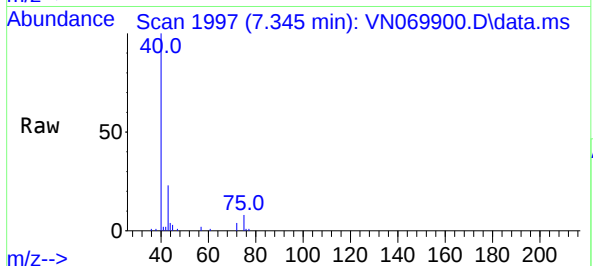

#31
Cyclohexane
Concen: 1.208 ug/l
RT: 8.085 min Scan# 2273
Delta R.T. -0.008 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 56 Resp: 32360
Ion Ratio Lower Upper
56 100
69 157.0 27.1 40.7#
84 103.8 73.4 110.0


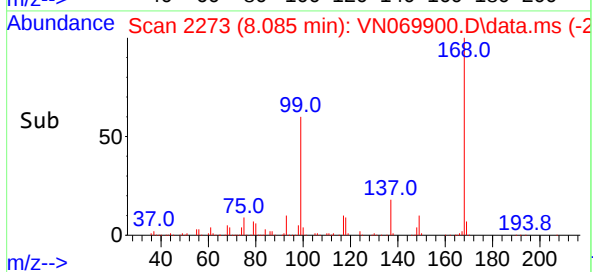
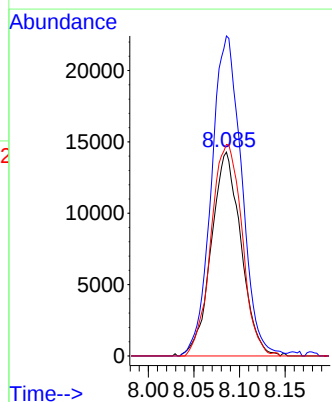
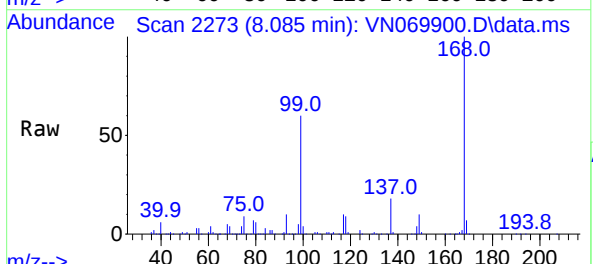




#33
1,2-Dichloroethane-d4
Concen: 52.426 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. -0.000 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion: 65 Resp: 1008931
Ion Ratio Lower Upper
65 100
67 50.8 0.0 103.0

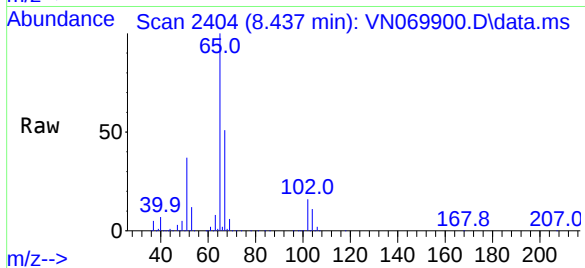

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. -0.000 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 114 Resp: 2338213
Ion Ratio Lower Upper
114 100
63 24.0 0.0 37.8
88 16.3 0.0 27.4


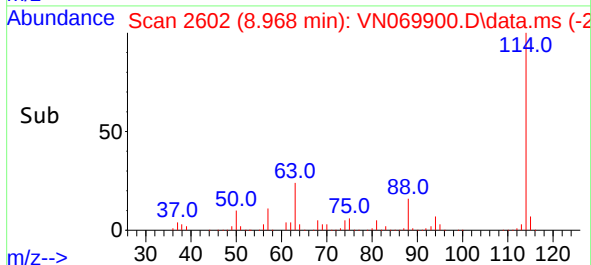

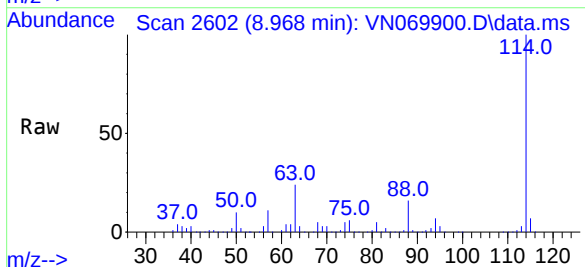




#35
Dibromofluoromethane
Concen: 49.480 ug/l
RT: 8.024 min Scan# 2113
Delta R.T. -0.000 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion:113 Resp: 724693
Ion Ratio Lower Upper
113 100
111 103.6 82.2 123.2
192 18.7 16.9 25.3

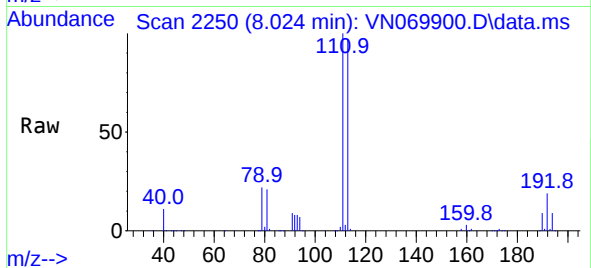

#36
1,1-Dichloropropene
Concen: 4.835 ug/l
RT: 8.085 min Scan# 2273
Delta R.T. -0.137 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35


Tgt Ion: 75 Resp: 107627
Ion Ratio Lower Upper
75 100
110 8.5 18.4 55.2#
77 0.1 24.4 36.6#

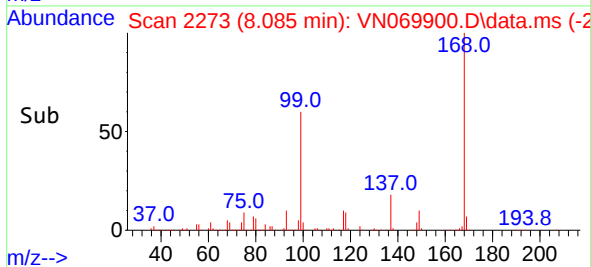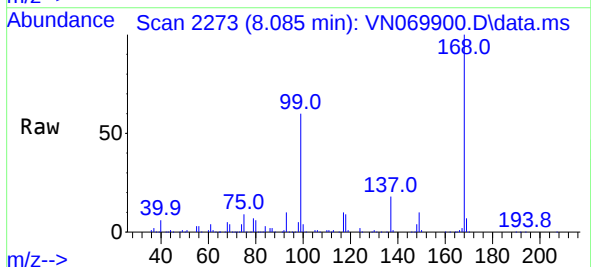






#38
Carbon Tetrachloride
Concen: 5.814 ug/l
RT: 8.085 min Scan# 2129
Delta R.T. -0.121 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP



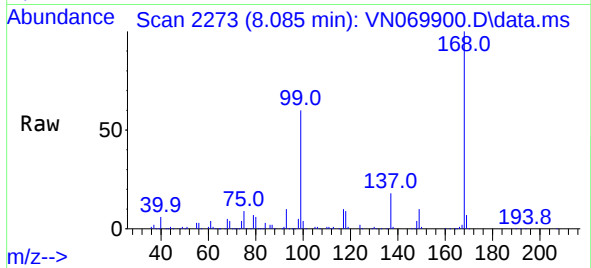



Tgt Ion:117 Resp: 126913
Ion Ratio Lower Upper
117 100
119 5.0 76.1 114.1#
121 0.0 24.2 36.2#

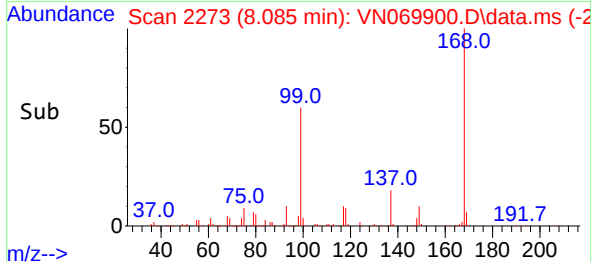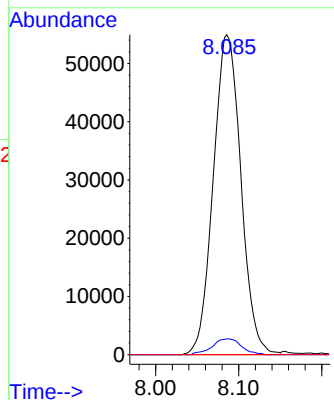

#41
Methacrylonitrile
Concen: 0.213 ug/l
RT: 7.699 min Scan# 2129
Delta R.T. 0.059 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 41 Resp: 3306
Ion Ratio Lower Upper
41 100
39 39.3 48.1 72.1#
67 0.0 68.3 102.5#
52 0.0 29.6 44.4#


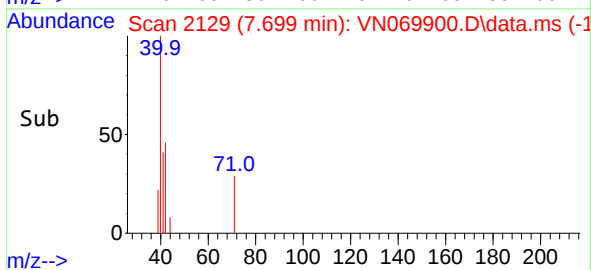
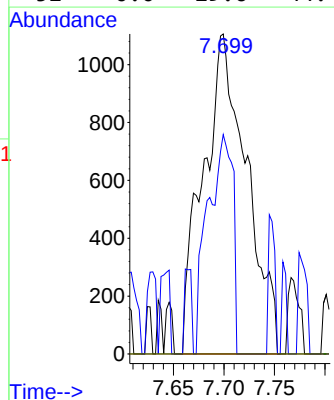





#43
Isopropyl Acetate
Concen: 3.854 ug/l
RT: 8.563 min Scan# 2451
Delta R.T. -0.000 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument : MSVOA_N
ClientSampleId : BLUE-CONCRETE-COMP


Tgt Ion: 43 Resp: 188956
Ion Ratio Lower Upper
43 100
61 14.8 20.4 30.6#
87 8.5 11.2 16.8#

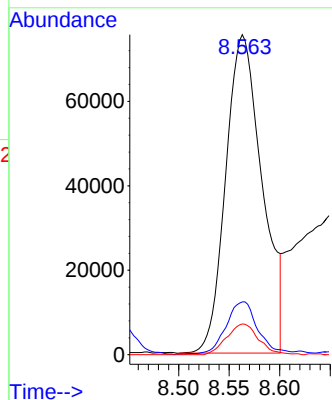

#48
Methyl methacrylate
Concen: 2.286 ug/l
RT: 9.544 min Scan# 2817
Delta R.T. -0.017 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 41 Resp: 52312
Ion Ratio Lower Upper
41 100
69 0.6 72.4 108.6#
39 0.0 58.4 87.6#


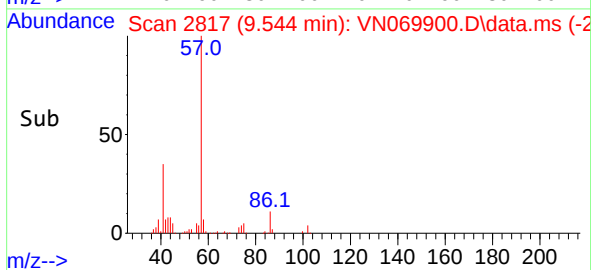
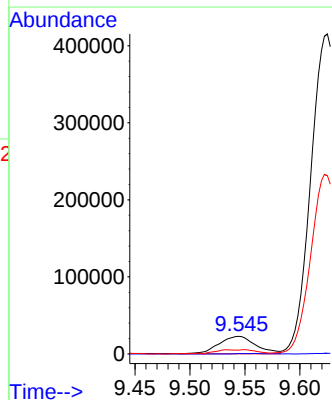



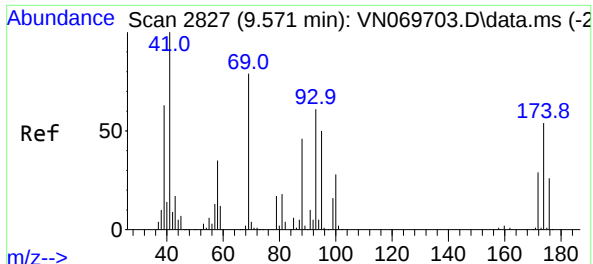

#49
1,4-Dioxane
Concen: 3.047 ug/l
RT: 9.625 min Scan# 21
Delta R.T. 0.054 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion: 88 Resp: 1251
Ion Ratio Lower Upper
88 100
43 645259.1 23.4 35.2#
58 2552.5 50.6 75.8#

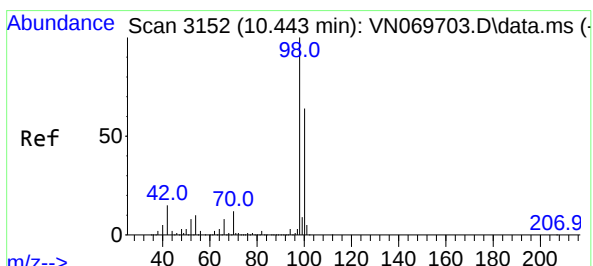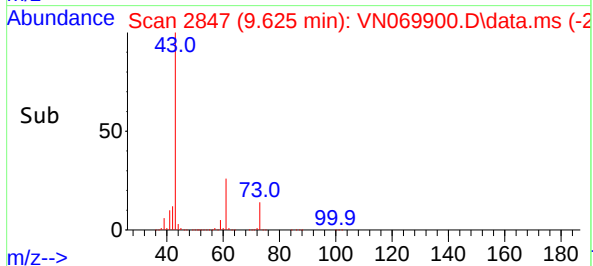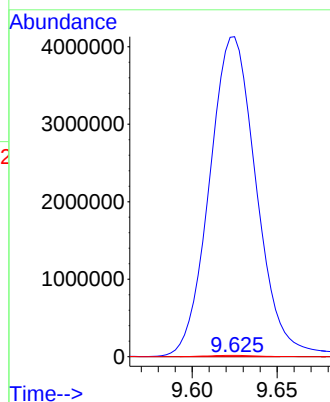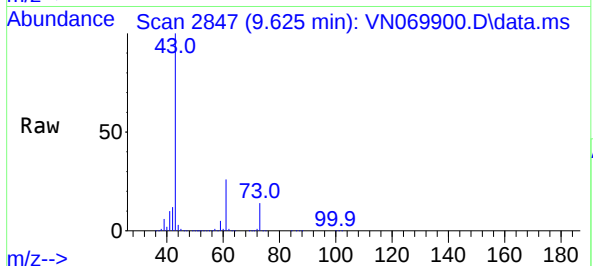

#50
Toluene-d8
Concen: 52.815 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. -0.003 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 98 Resp: 3105956
Ion Ratio Lower Upper
98 100
100 64.0 50.4 75.6


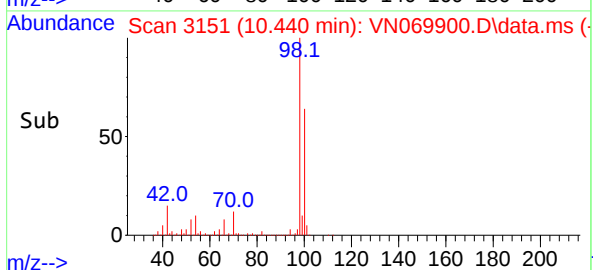

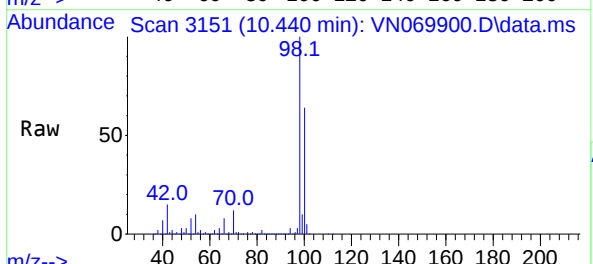




#51
4-Methyl-2-Pentanone
Concen: 0.776 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. -0.000 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion: 43 Resp: 24682
Ion Ratio Lower Upper
43 100
58 47.0 30.4 45.6#

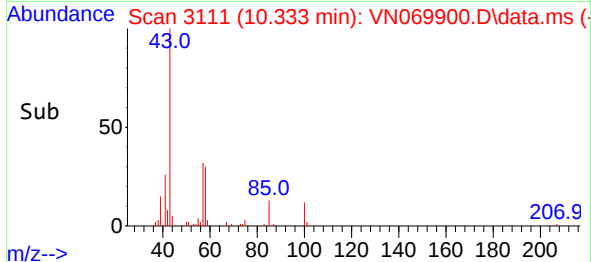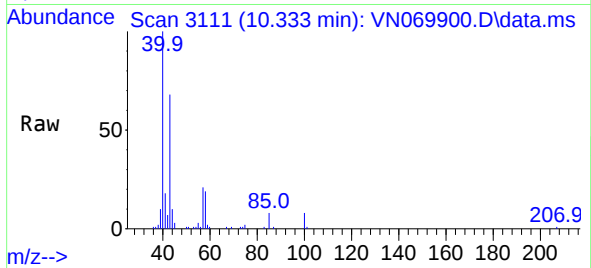

#53
t-1,3-Dichloropropene
Concen: 2.797 ug/l
RT: 10.725 min Scan# 3257
Delta R.T. 0.006 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 75 Resp: 91
Ion Ratio Lower Upper
75 100
77 30.4 25.6 38.4


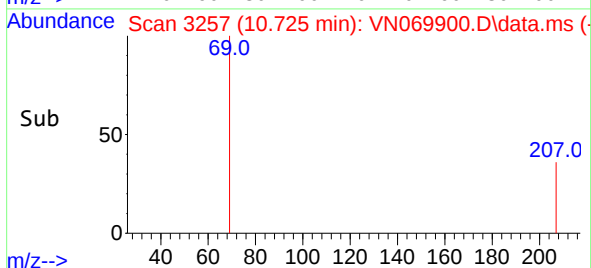
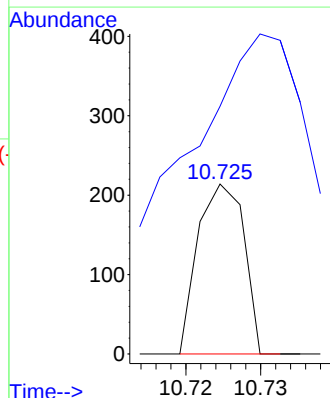





#54
cis-1,3-Dichloropropene
Concen: 8.863 ug/l
RT: 10.242 min Scan# 3058
Delta R.T. 0.051 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion: 75 Resp: 204796
Ion Ratio Lower Upper
75 100
77 0.5 26.4 39.6#
39 45.2 42.5 63.7

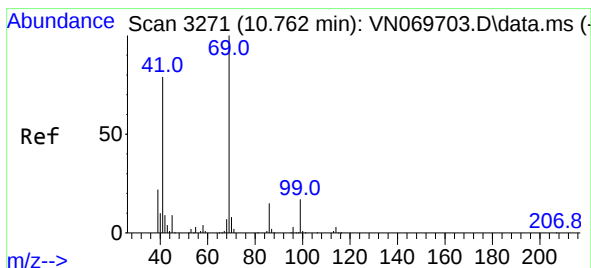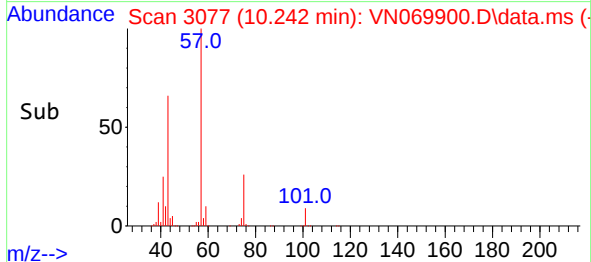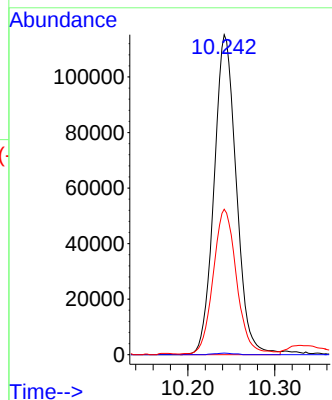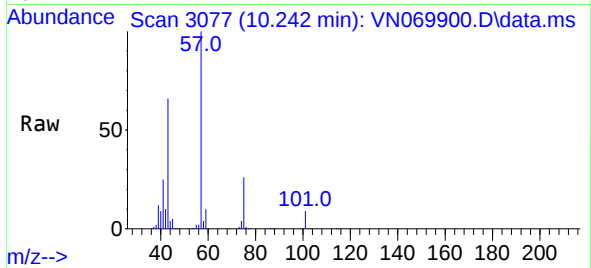

#56
Ethyl methacrylate
Concen: 2.296 ug/l
RT: 10.703 min Scan# 3249
Delta R.T. -0.059 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 69 Resp: 555
Ion Ratio Lower Upper
69 100
41 0.0 51.4 77.0#
39 0.0 34.6 52.0#

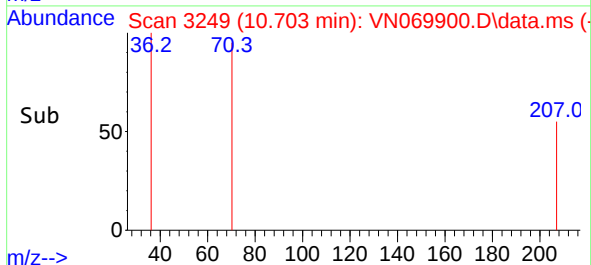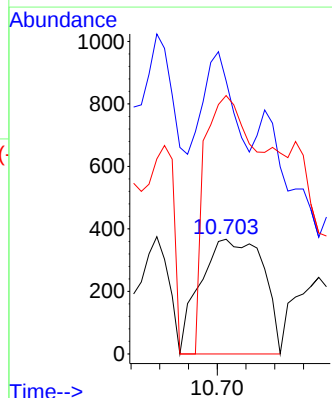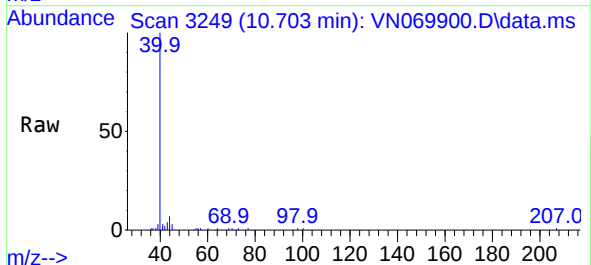



#57

1,3-Dichloropropane

Concen: 3.875 ug/l

RT: 11.089 min Scan# 31

Delta R.T. 0.043 min

Lab File: VN069900.D

Acq: 9 Dec 2021 8:35

Instrument :

MSVOA_N

ClientSampleId :





BLUE-CONCRETE-COMP

Tgt Ion: 76 Resp: 114356

Ion Ratio Lower Upper

76 100

78 0.4 25.7 38.5#

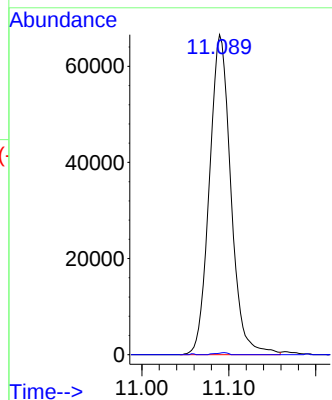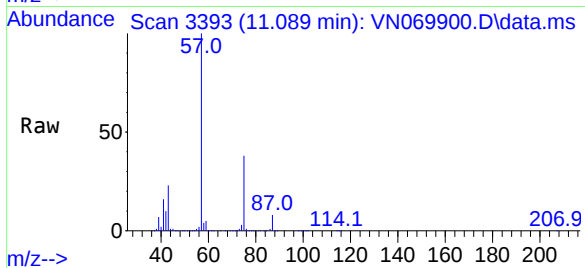

#59

2-Hexanone

Concen: 85.230 ug/l

RT: 11.089 min Scan# 3393

Delta R.T. 0.002 min

Lab File: VN069900.D




Acq: 9 Dec 2021 8:35


Tgt Ion: 43 Resp: 2050581

Ion Ratio Lower Upper

43 100

58 16.2 26.9 80.7#


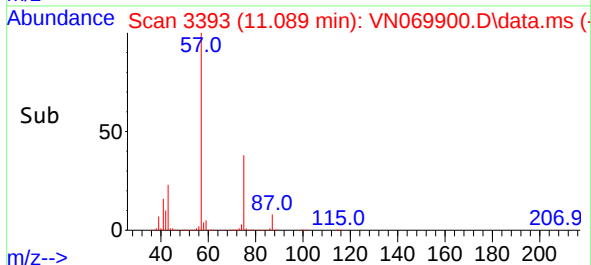
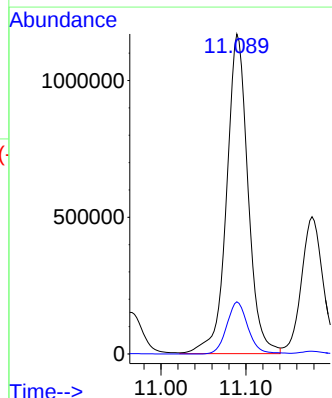
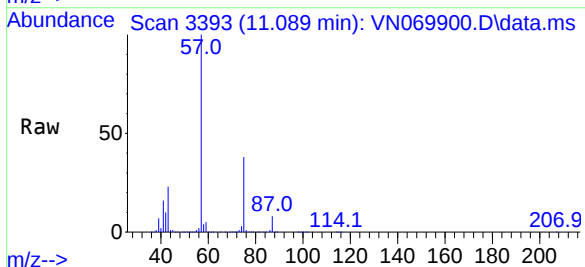




#60
Dibromochloromethane
Concen: 2.426 ug/l
RT: 11.494 min Scan# 311
Delta R.T. 0.254 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion:129 Resp: 942
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#

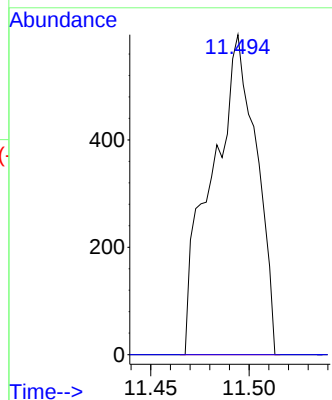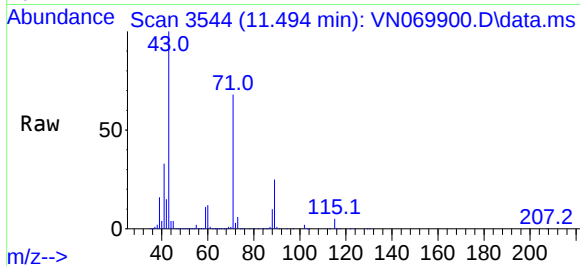

#62
4-Bromofluorobenzene
Concen: 60.187 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 95 Resp: 1282300
Ion Ratio Lower Upper
95 100
174 76.2 0.0 187.2
176 73.4 0.0 181.4

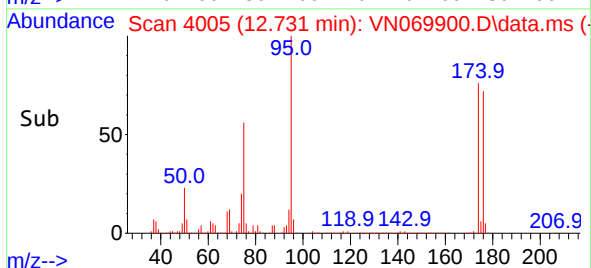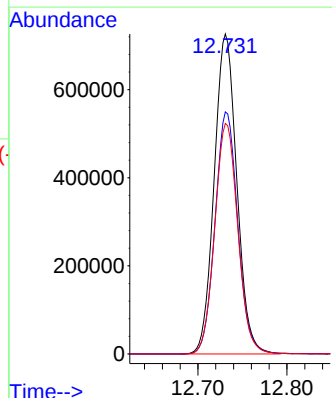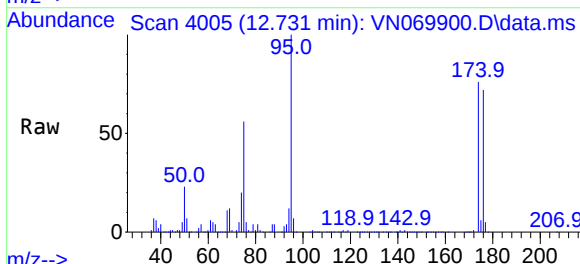




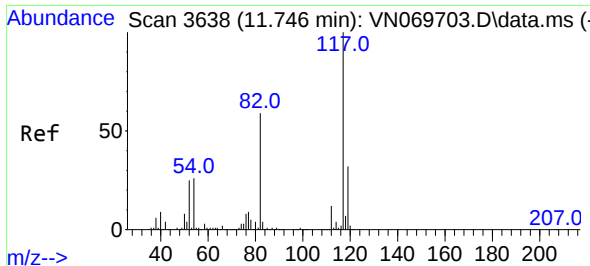


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3638
Delta R.T. -0.002 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP

Tgt Ion:117 Resp: 2644833




Ion	Ratio	Lower	Upper
117	100		
82	59.3	42.4	63.6
119	31.6	25.4	38.2

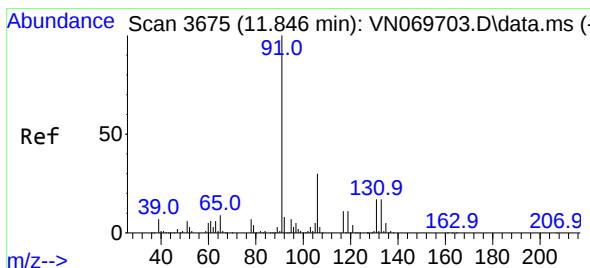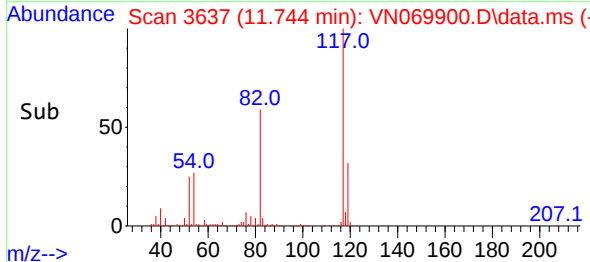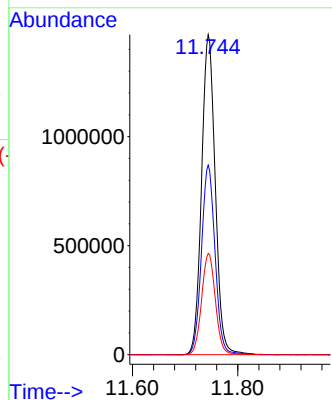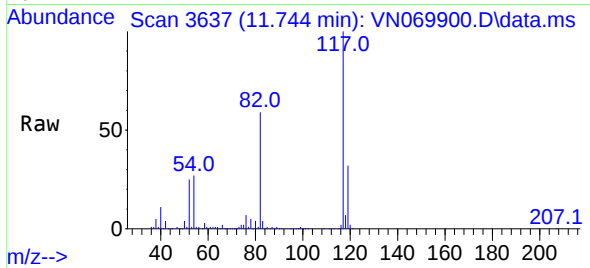


#67
Ethyl Benzene
Concen: 0.328 ug/l
RT: 11.846 min Scan# 3675
Delta R.T. -0.000 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 91 Resp: 31989

Ion	Ratio	Lower	Upper
91	100		
106	24.4	25.7	38.5


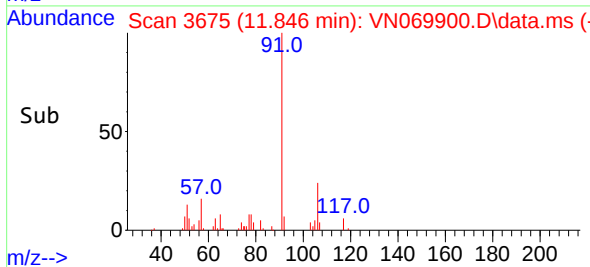
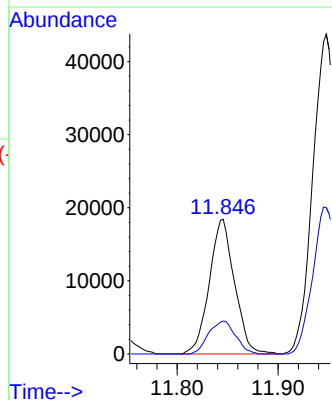
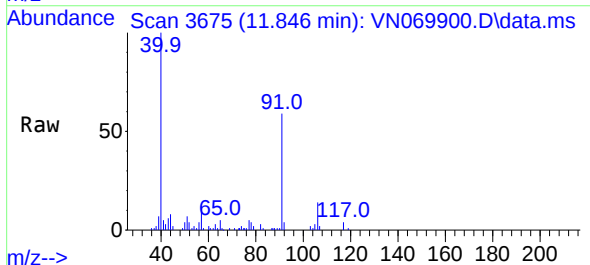


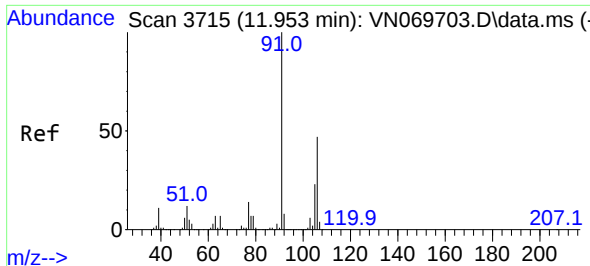

#68
m/p-Xylenes
Concen: 1.030 ug/l
RT: 11.945 min Scan# 3712
Delta R.T. -0.008 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion:106 Resp: 36538
Ion Ratio Lower Upper
106 100
91 216.4 160.6 240.8

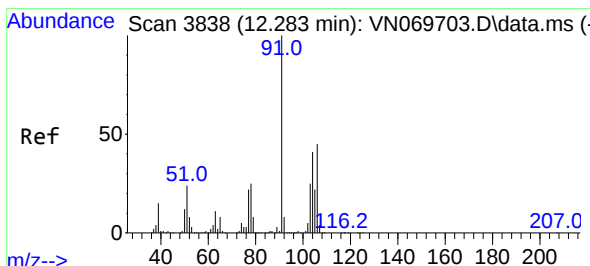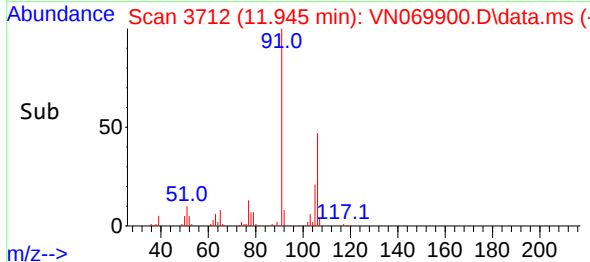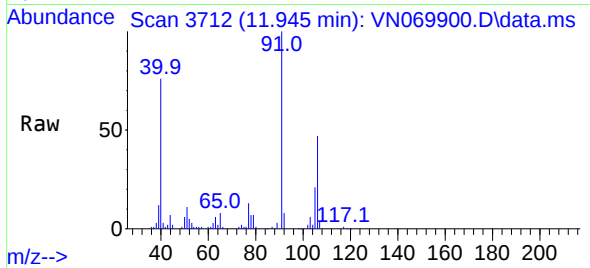

#69
o-Xylene
Concen: 0.539 ug/l
RT: 12.280 min Scan# 3837
Delta R.T. -0.003 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion:106 Resp: 19258
Ion Ratio Lower Upper
106 100
91 220.5 105.8 317.3


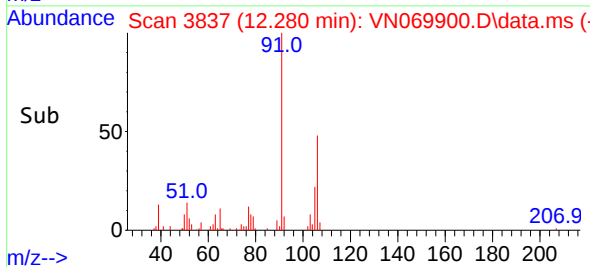

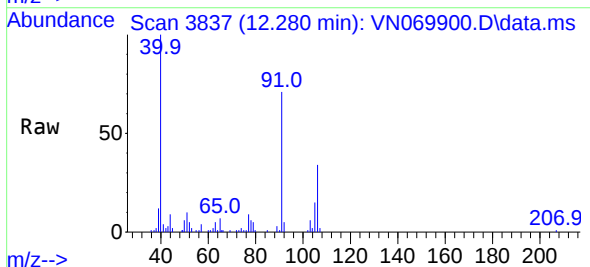


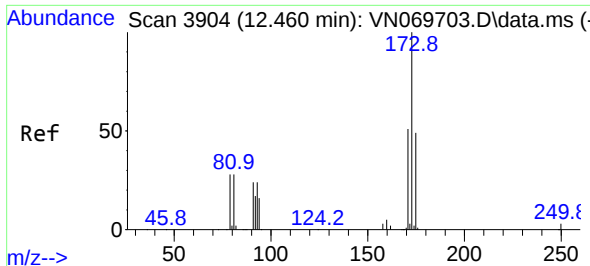

#71
Bromoform
Concen: 2.735 ug/l
RT: 12.701 min Scan# 3904
Delta R.T. 0.241 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion:173 Resp: 72
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0

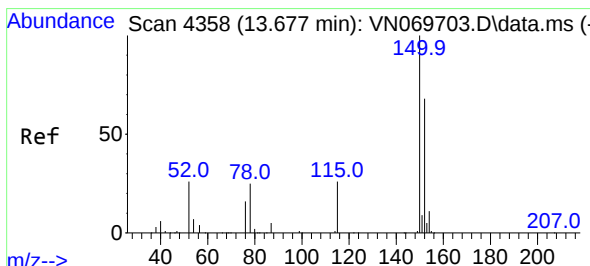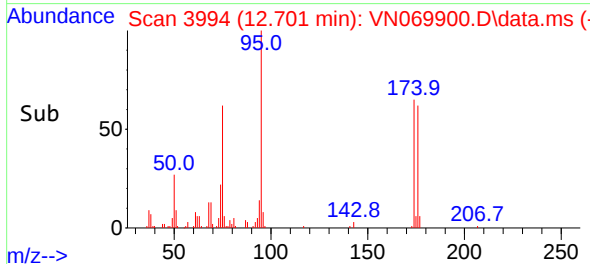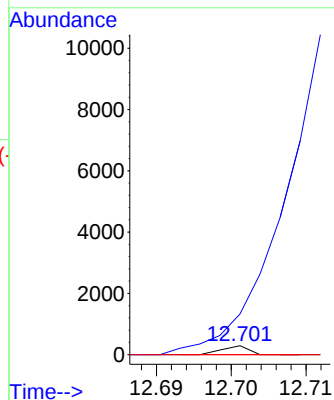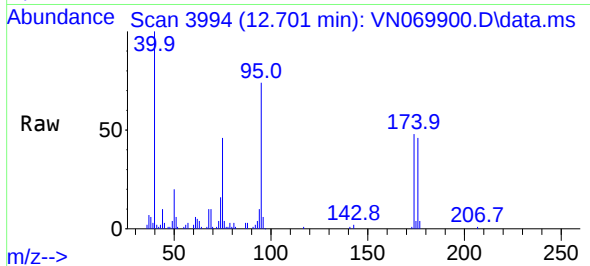

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.003 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion:152 Resp: 1093657
Ion Ratio Lower Upper
152 100
115 60.5 27.5 82.5
150 157.7 0.0 344.4


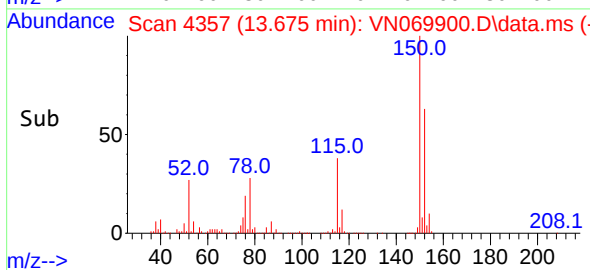
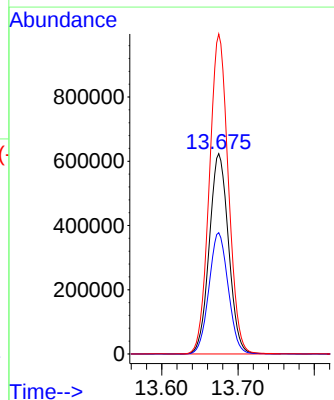
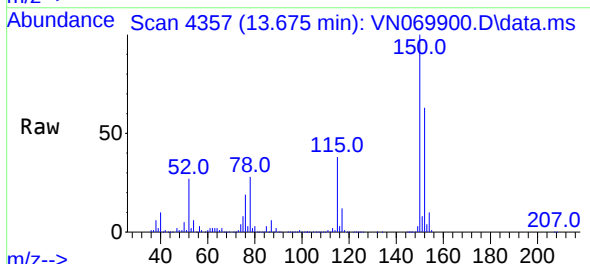




#76
1,2,3-Trichloropropane
Concen: 23.075 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.150 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion: 75 Resp: 723705
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#

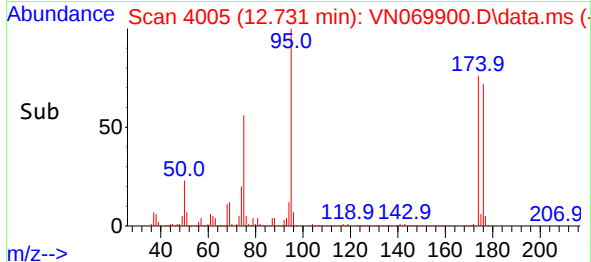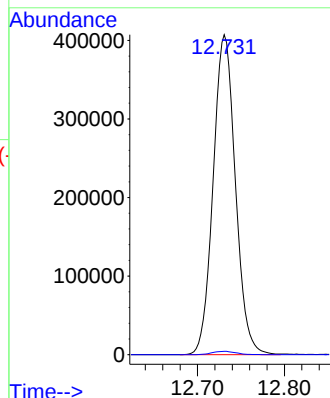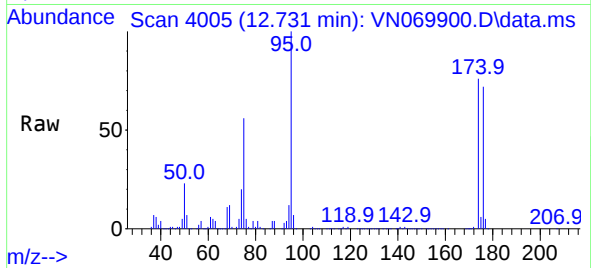

#81
trans-1,4-Dichloro-2-butene
Concen: 73.448 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion: 75 Resp: 723705
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#


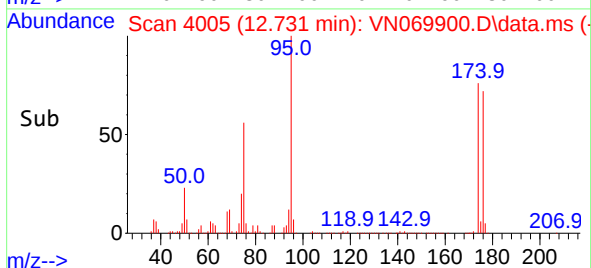
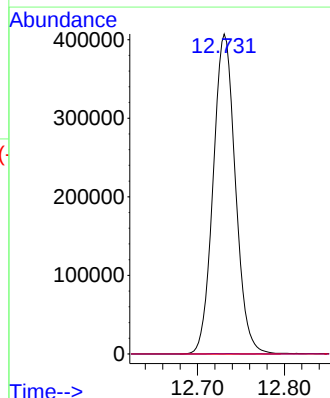





#84
1,2,4-Trimethylbenzene
Concen: 0.471 ug/l
RT: 13.396 min Scan# 41
Delta R.T. 0.027 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35




Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP


Tgt Ion:105 Resp: 35164
Ion Ratio Lower Upper
105 100
120 0.0 22.8 68.4#

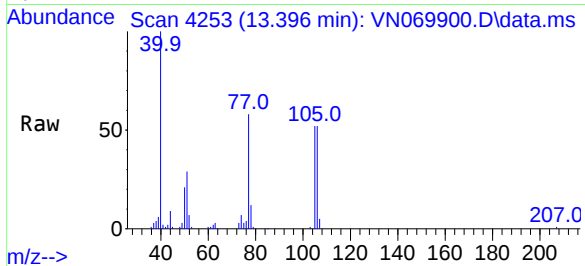

#85
sec-Butylbenzene
Concen: 0.374 ug/l
RT: 13.396 min Scan# 4253
Delta R.T. -0.107 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion:105 Resp: 35164
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


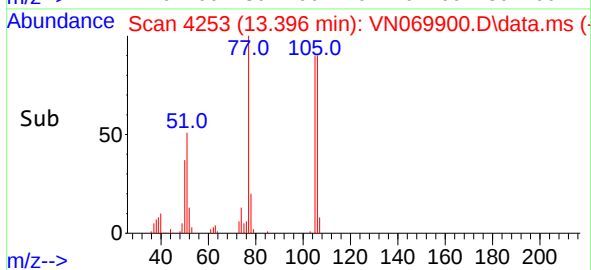

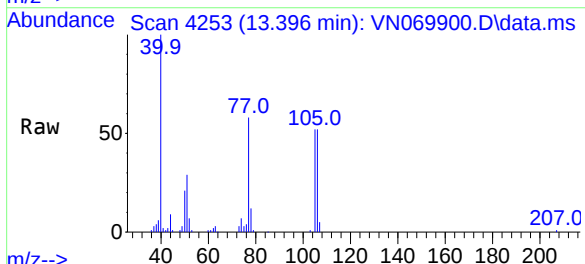




#95
Naphthalene
Concen: 3.998 ug/l
RT: 15.504 min Scan# 5040
Delta R.T. -0.003 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Instrument :
MSVOA_N
ClientSampleId :
BLUE-CONCRETE-COMP

Tgt Ion:128 Resp: 737
Ion Ratio Lower Upper
128 100
127 0.0 10.5 15.7#
129 0.0 8.7 13.1#

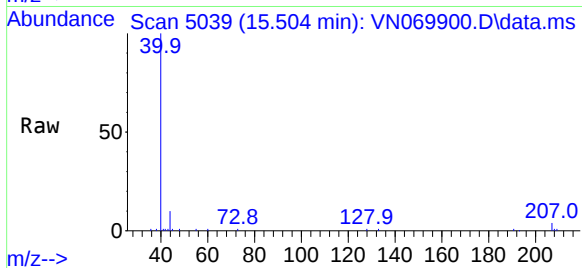

#96
1,2,3-Trichlorobenzene
Concen: 2.444 ug/l
RT: 15.708 min Scan# 5115
Delta R.T. 0.006 min
Lab File: VN069900.D
Acq: 9 Dec 2021 8:35

Tgt Ion:180 Resp: 146
Ion Ratio Lower Upper
180 100
182 0.0 47.4 142.2#
145 0.0 15.0 45.1#

