

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN120821\  
 Data File : VN069854.D  
 Acq On : 8 Dec 2021 12:01  
 Operator : JC/MD  
 Sample : VN1208WBL01  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 VN1208WBL01

Quant Time: Dec 09 11:35:17 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N120221W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Dec 03 08:46:47 2021  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 8.086  | 168  | 1306311  | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.968  | 114  | 2372097  | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.744 | 117  | 2520909  | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.675 | 152  | 935029   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.437  | 65    | 1007745  | 49.964   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 61 - 141 | Recovery | =    | 99.920%  |
| 35) Dibromofluoromethane    | 8.024  | 113   | 705962   | 47.513   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 69 - 133 | Recovery | =    | 95.020%  |
| 50) Toluene-d8              | 10.441 | 98    | 3063696  | 51.352   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 65 - 126 | Recovery | =    | 102.700% |
| 62) 4-Bromofluorobenzene    | 12.731 | 95    | 1155559  | 53.464   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 58 - 135 | Recovery | =    | 106.920% |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN120821\  
Data File : VN069854.D  
Acq On : 8 Dec 2021 12:01  
Operator : JC/MD  
Sample : VN1208WBL01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
VN1208WBL01

Quant Time: Dec 09 11:35:17 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N120221W.M  
Quant Title : SW846 8260  
QLast Update : Fri Dec 03 08:46:47 2021  
Response via : Initial Calibration




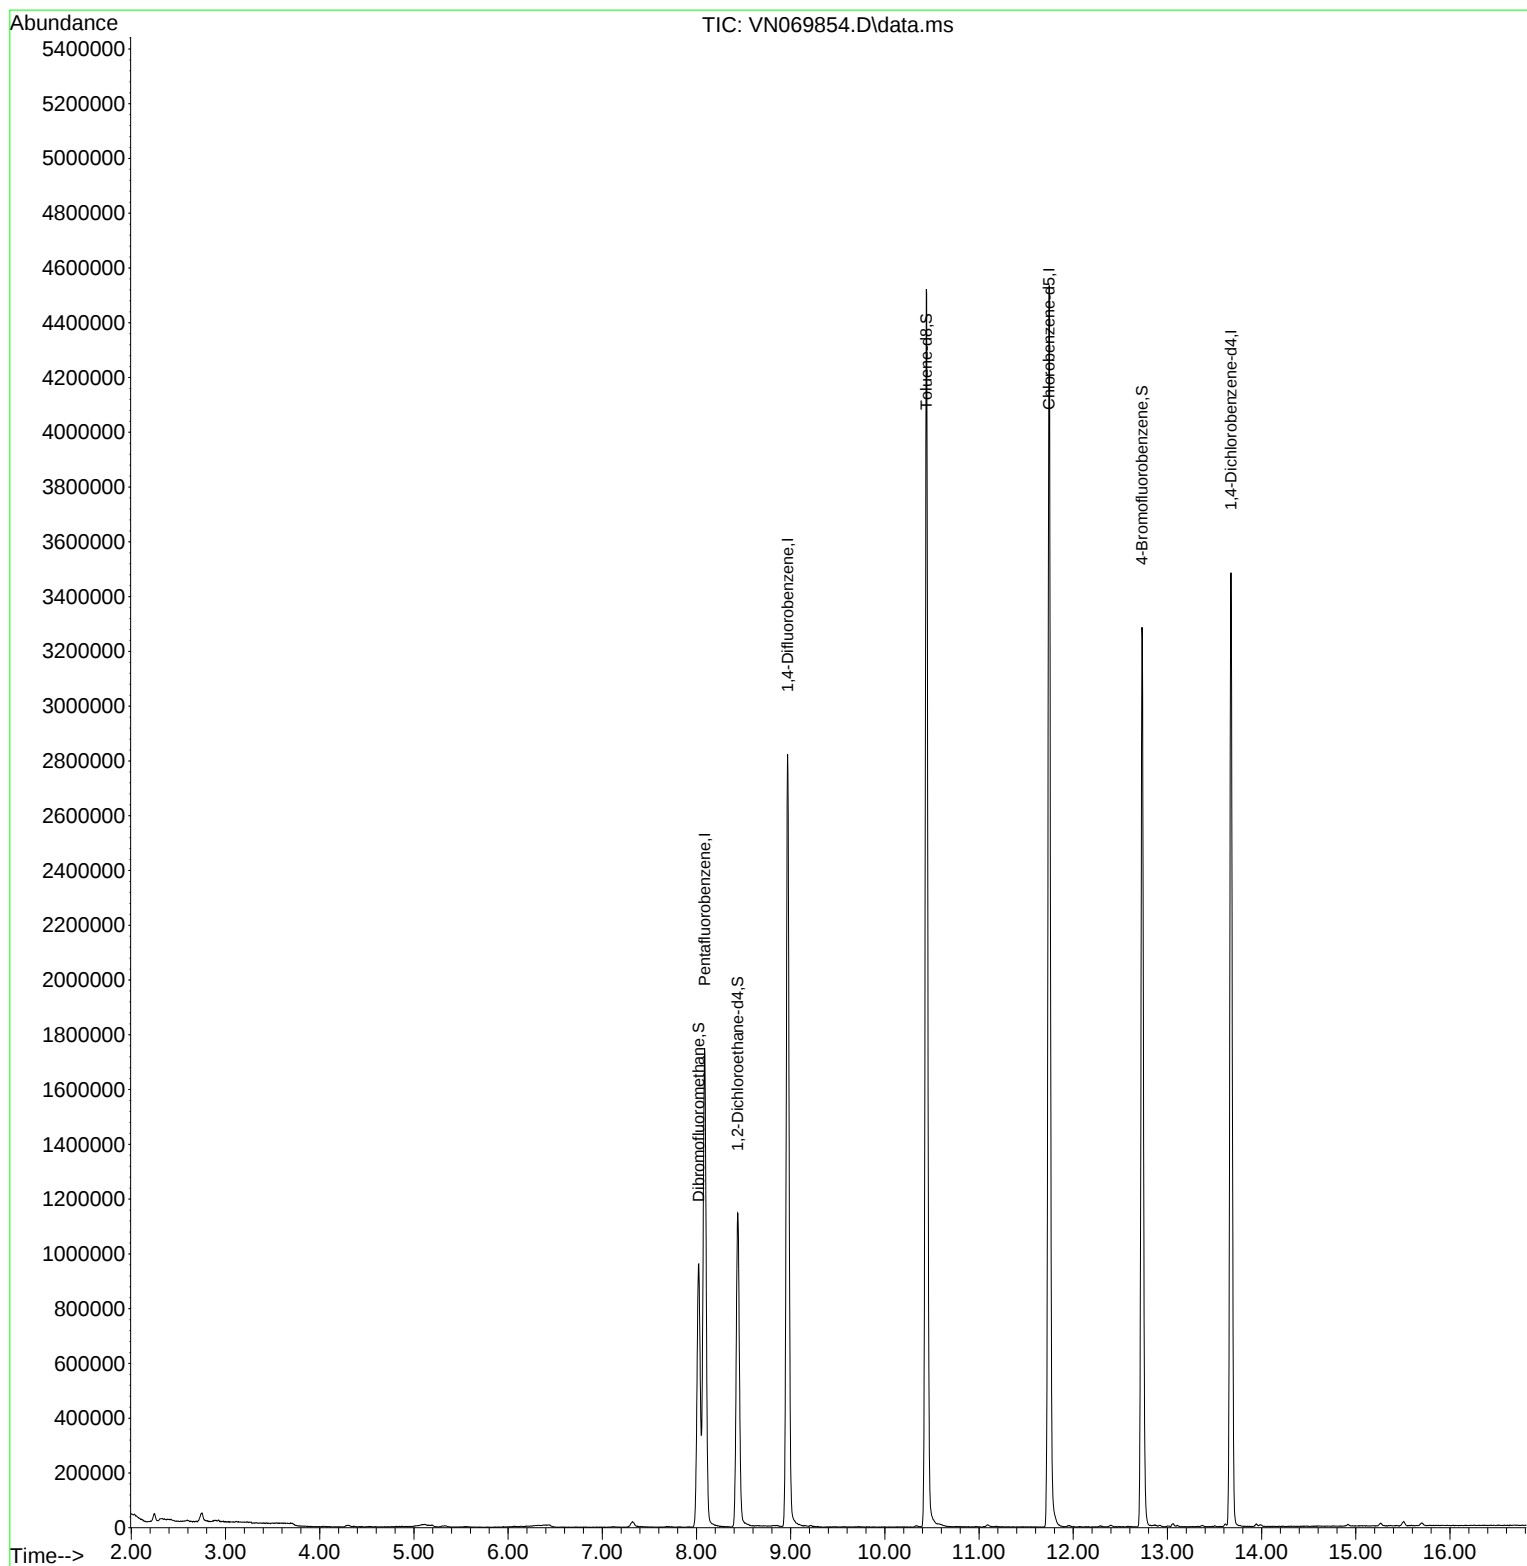


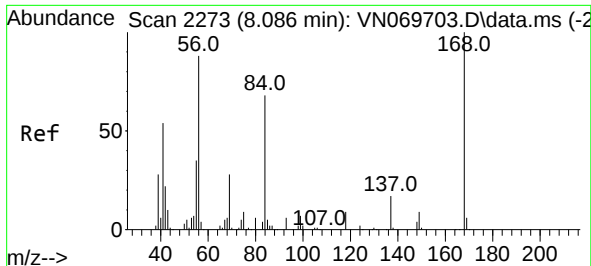

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.086 min Scan# 21  
Delta R.T. -0.000 min  
Lab File: VN069854.D  
Acq: 8 Dec 2021 12:01




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN1208WBL01


Tgt Ion:168 Resp: 1306311  
Ion Ratio Lower Upper  
168 100  
99 60.4 41.3 61.9

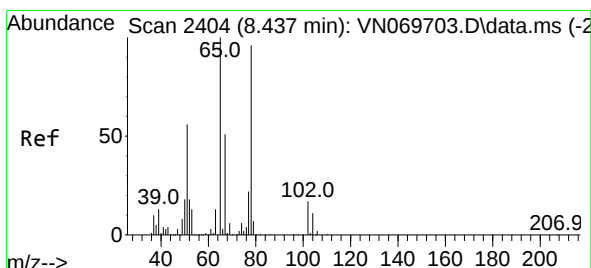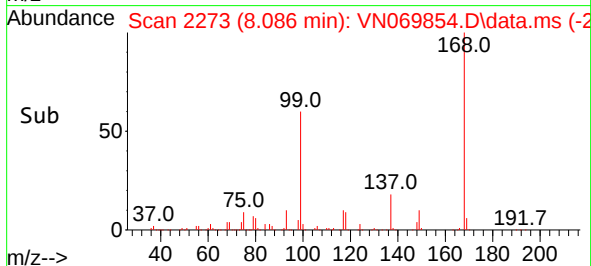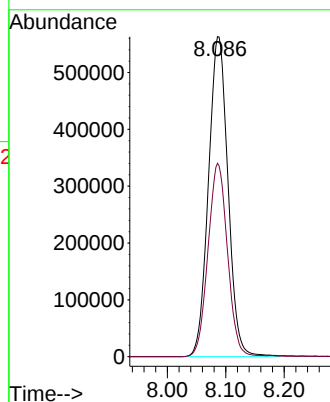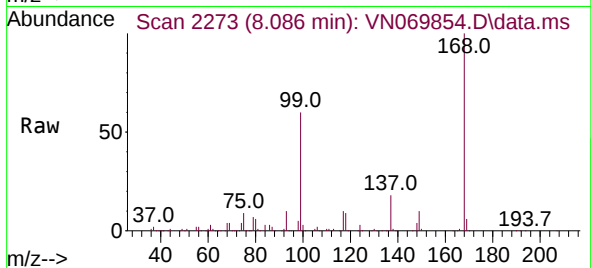

#33  
1,2-Dichloroethane-d4  
Concen: 49.964 ug/l  
RT: 8.437 min Scan# 2404  
Delta R.T. 0.000 min  
Lab File: VN069854.D  
Acq: 8 Dec 2021 12:01

Tgt Ion: 65 Resp: 1007745  
Ion Ratio Lower Upper  
65 100  
67 51.2 0.0 103.0


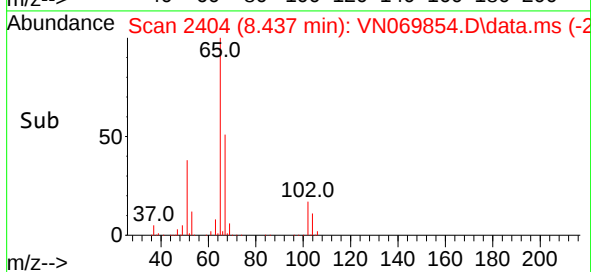
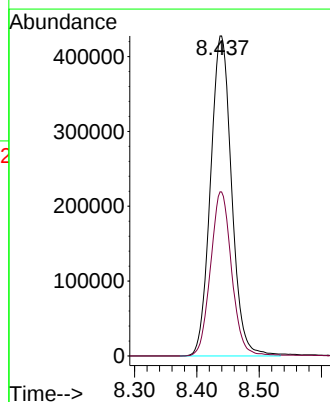
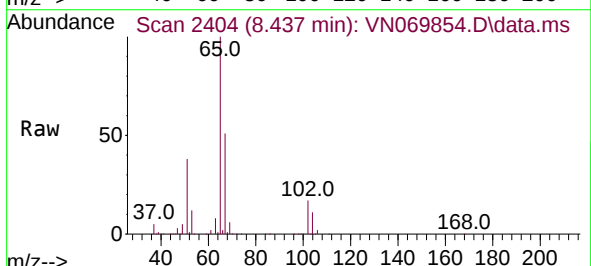


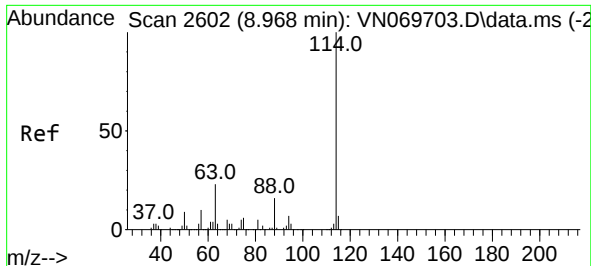

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 8.968 min Scan# 2602  
Delta R.T. 0.000 min  
Lab File: VN069854.D  
Acq: 8 Dec 2021 12:01




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN1208WBL01


Tgt Ion:114 Resp: 2372097  
Ion Ratio Lower Upper  
114 100  
63 23.4 0.0 37.8  
88 16.1 0.0 27.4

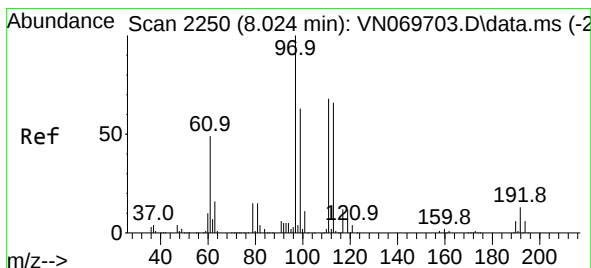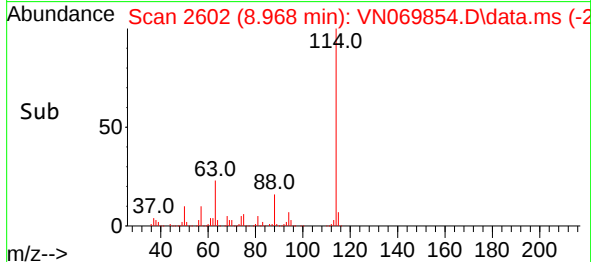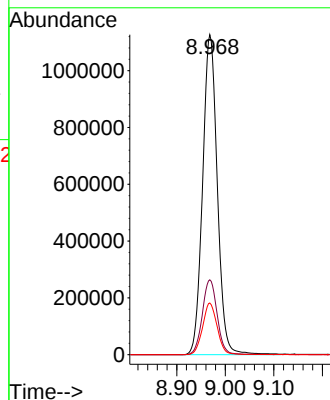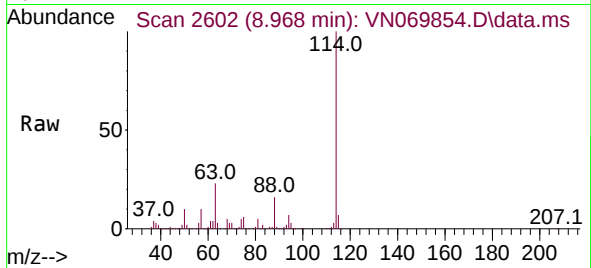

#35  
Dibromofluoromethane  
Concen: 47.513 ug/l  
RT: 8.024 min Scan# 2250  
Delta R.T. 0.000 min  
Lab File: VN069854.D  
Acq: 8 Dec 2021 12:01

Tgt Ion:113 Resp: 705962  
Ion Ratio Lower Upper  
113 100  
111 102.2 82.2 123.2  
192 18.8 16.9 25.3


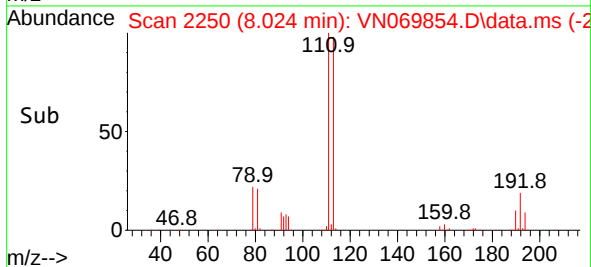
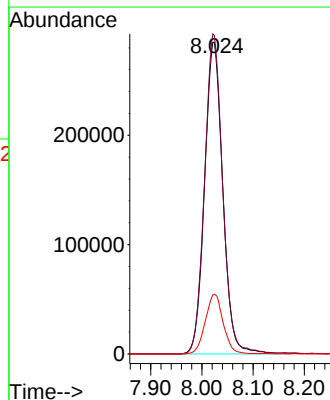
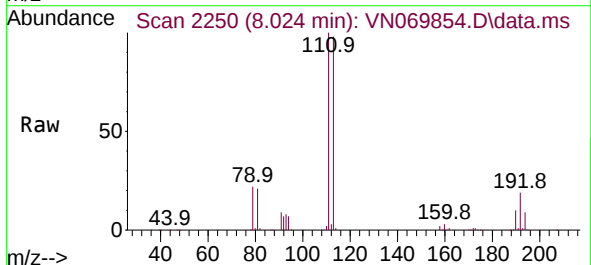


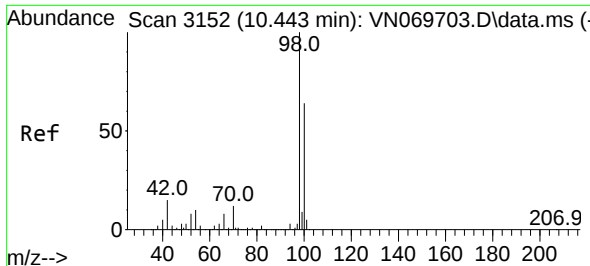

#50  
Toluene-d8  
Concen: 51.352 ug/l  
RT: 10.441 min Scan# 3152  
Delta R.T. -0.002 min  
Lab File: VN069854.D  
Acq: 8 Dec 2021 12:01




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN1208WBL01


Tgt Ion: 98 Resp: 3063696  
Ion Ratio Lower Upper  
98 100  
100 63.9 50.4 75.6

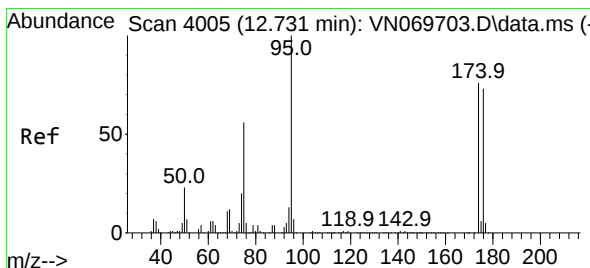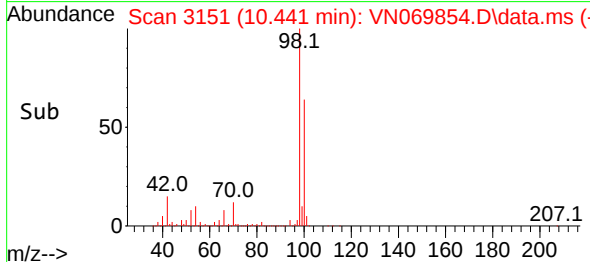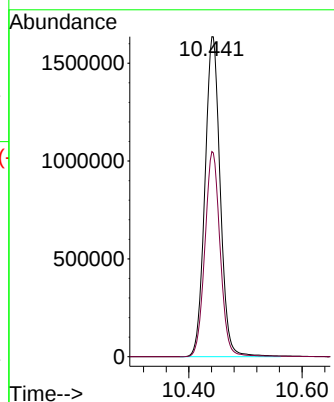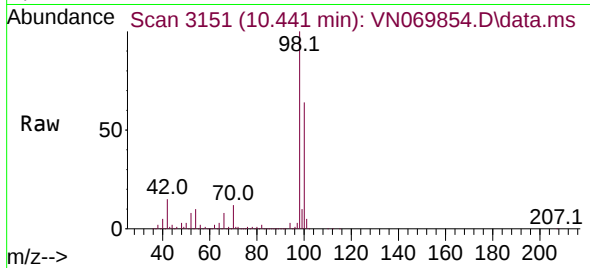

#62  
4-Bromofluorobenzene  
Concen: 53.464 ug/l  
RT: 12.731 min Scan# 4005  
Delta R.T. -0.000 min  
Lab File: VN069854.D  
Acq: 8 Dec 2021 12:01

Tgt Ion: 95 Resp: 1155559  
Ion Ratio Lower Upper  
95 100  
174 76.1 0.0 187.2  
176 73.2 0.0 181.4


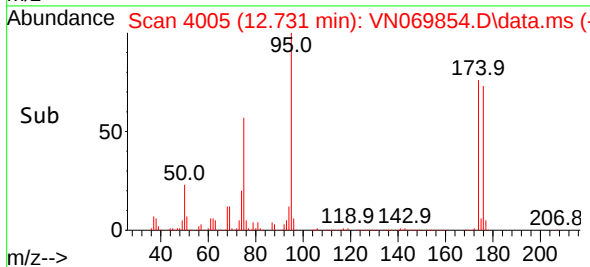
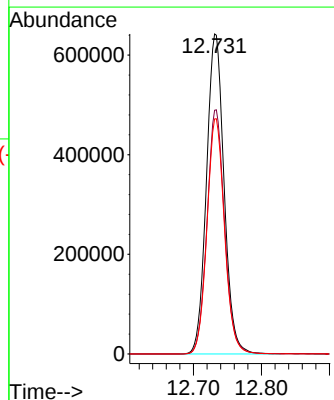
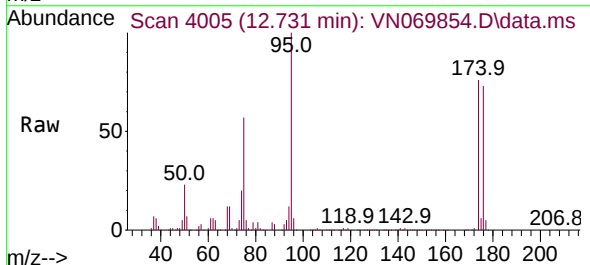


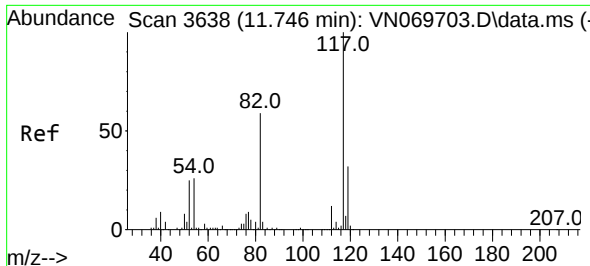

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.744 min Scan# 3637  
Delta R.T. -0.002 min  
Lab File: VN069854.D  
Acq: 8 Dec 2021 12:01

Instrument :  
MSVOA\_N  
ClientSampleId :  
VN1208WBL01

Tgt Ion:117 Resp: 2520909  
Ion Ratio Lower Upper  
117 100  
82 59.0 42.4 63.6  
119 32.5 25.4 38.2

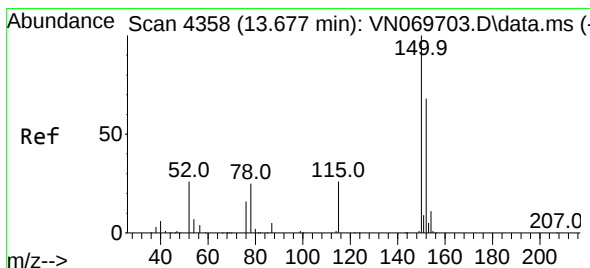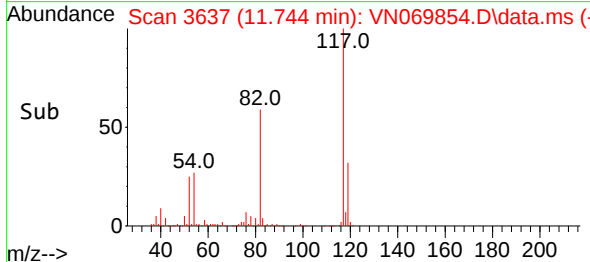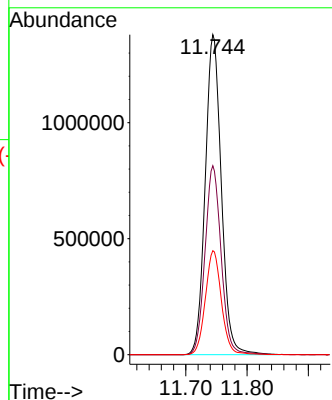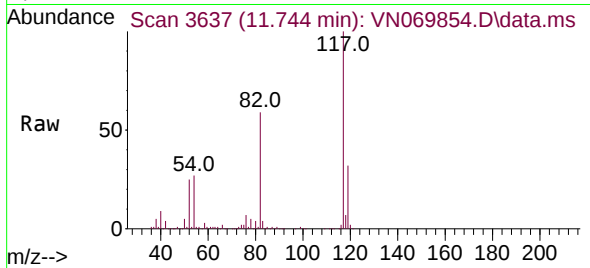

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.675 min Scan# 4357  
Delta R.T. -0.002 min  
Lab File: VN069854.D  
Acq: 8 Dec 2021 12:01

Tgt Ion:152 Resp: 935029  
Ion Ratio Lower Upper  
152 100  
115 61.3 27.5 82.5  
150 157.9 0.0 344.4

