

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120822\
 Data File : VN075655.D
 Acq On : 08 Dec 2022 18:32
 Operator : JC\MD
 Sample : N5947-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 NYE-WATER-1208

Quant Time: Dec 09 02:30:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 23 00:18:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	171261	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	276265	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	240180	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	106436	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	46129	50.178	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 100.360%	
35) Dibromofluoromethane	8.171	113	60295	55.558	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 111.120%	
50) Toluene-d8	10.571	98	122488	50.112	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.220%	
62) 4-Bromofluorobenzene	12.853	95	86723	48.068	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 96.140%	
Target Compounds						
						Qvalue
3) Chloromethane	2.383	50	452	0.277	ug/l #	42
11) Tert butyl alcohol	5.542	59	1697	4.397	ug/l #	72
16) Acetone	4.453	43	3018	3.520	ug/l	95
18) Methyl Acetate	5.053	43	1757	Below Cal	#	58
20) Methylene Chloride	5.295	84	138	Below Cal	#	7
25) 2-Butanone	7.506	43	863	0.721	ug/l #	43
27) cis-1,2-Dichloroethene	7.489	96	542	0.265	ug/l	85
29) Tetrahydrofuran	7.847	42	2937	4.033	ug/l	95
31) Cyclohexane	8.230	56	2884	0.987	ug/l #	9
36) 1,1-Dichloropropene	8.230	75	11537	4.875	ug/l #	51
38) Carbon Tetrachloride	8.230	117	16571	6.374	ug/l #	17
41) Methacrylonitrile	7.853	41	2157	1.980	ug/l #	37
43) Isopropyl Acetate	8.759	43	2238	0.654	ug/l #	53
44) Trichloroethene	9.359	130	1771	0.893	ug/l	87
51) 4-Methyl-2-Pentanone	10.453	43	900	0.413	ug/l #	67
52) Toluene	10.635	92	6347	1.359	ug/l	99
59) 2-Hexanone	11.200	43	952	0.582	ug/l	92
60) Dibromochloromethane	11.100	129	1755	0.899	ug/l #	11
64) Tetrachloroethene	11.100	164	1724	0.940	ug/l #	75
68) m/p-Xylenes	12.071	106	1053	0.306	ug/l	92
76) 1,2,3-Trichloropropane	12.853	75	44739	22.231	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	44739	65.778	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.488	105	1304	0.201	ug/l	81
87) 1,3-Dichlorobenzene	13.735	146	872	0.240	ug/l	78
88) 1,4-Dichlorobenzene	13.735	146	872	0.236	ug/l	78
91) 1,2-Dichlorobenzene	14.112	146	937	0.264	ug/l	92
93) 1,2,4-Trichlorobenzene	15.400	180	977	0.538	ug/l #	83
95) Naphthalene	15.641	128	5620	0.983	ug/l #	95
96) 1,2,3-Trichlorobenzene	15.847	180	1374	0.769	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120822\
Data File : VN075655.D
Acq On : 08 Dec 2022 18:32
Operator : JC\MD
Sample : N5947-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208

Quant Time: Dec 09 02:30:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 23 00:18:03 2022
Response via : Initial Calibration




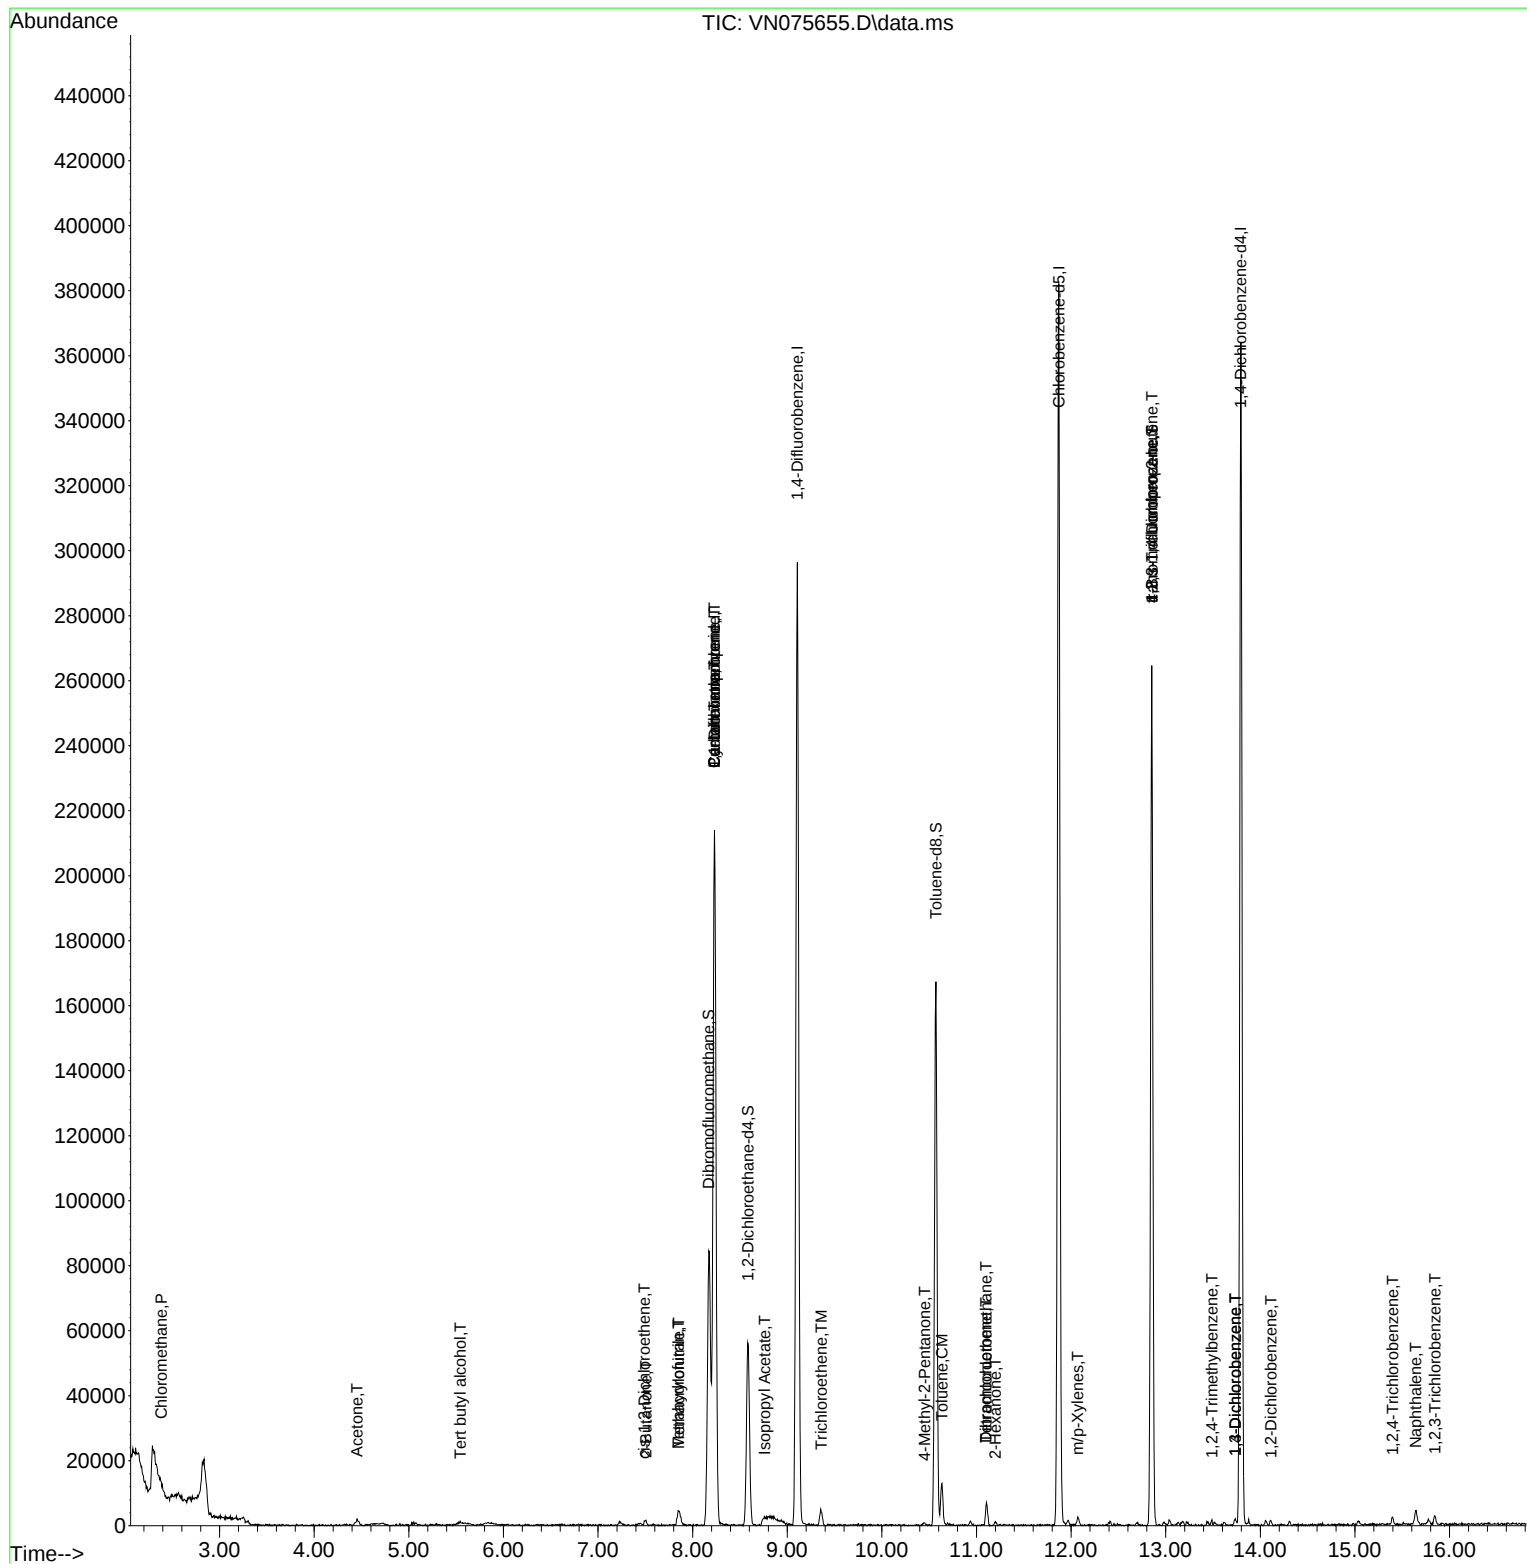


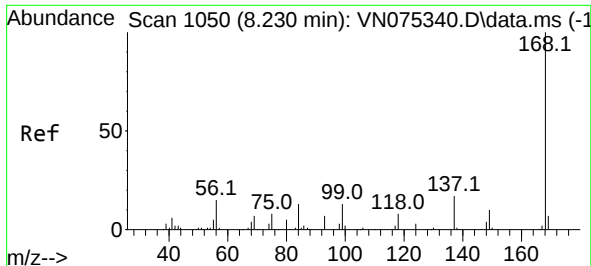

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion:168 Resp: 171261
Ion Ratio Lower Upper
168 100
99 55.3 51.6 77.4

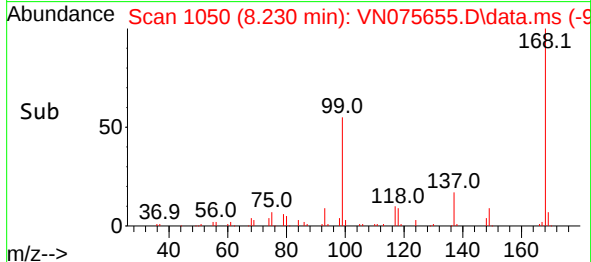

#3
Chloromethane
Concen: 0.277 ug/l
RT: 2.383 min Scan# 56
Delta R.T. 0.012 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion: 50 Resp: 452
Ion Ratio Lower Upper
50 100
52 0.0 25.8 38.6#




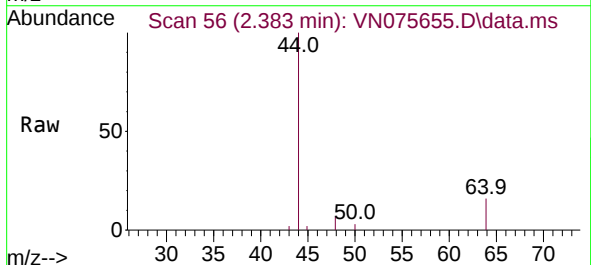


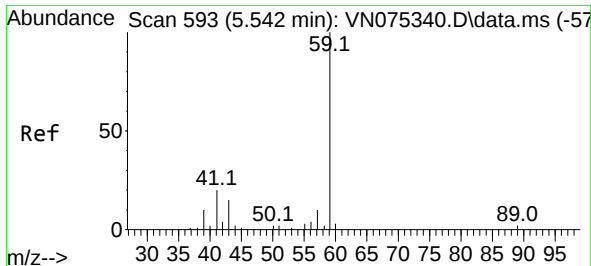

#11
Tert butyl alcohol
Concen: 4.397 ug/l
RT: 5.542 min Scan# 59
Delta R.T. -0.000 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion: 59 Resp: 1697
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#

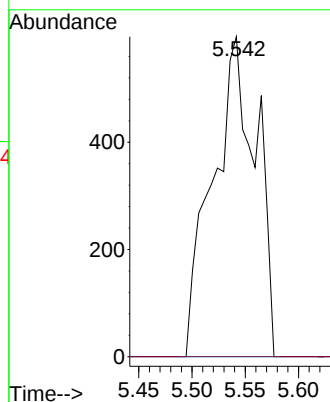

#16
Acetone
Concen: 3.520 ug/l
RT: 4.453 min Scan# 408
Delta R.T. 0.017 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion: 43 Resp: 3018
Ion Ratio Lower Upper
43 100
58 34.7 25.5 38.3


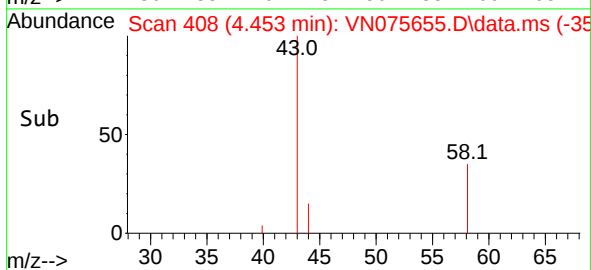
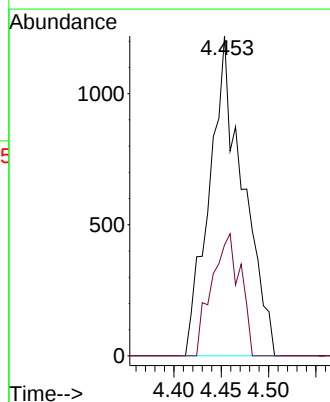





#18
Methyl Acetate
Concen: Below Cal
RT: 5.053 min Scan# 51
Delta R.T. 0.017 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion: 43 Resp: 1757
Ion Ratio Lower Upper
43 100
74 5.5 22.0 33.0#



#20
Methylene Chloride
Concen: Below Cal
RT: 5.295 min Scan# 551
Delta R.T. 0.006 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion: 84 Resp: 138
Ion Ratio Lower Upper
84 100
49 0.0 94.9 142.3#
51 0.0 26.8 40.2#
86 0.0 53.7 80.5#

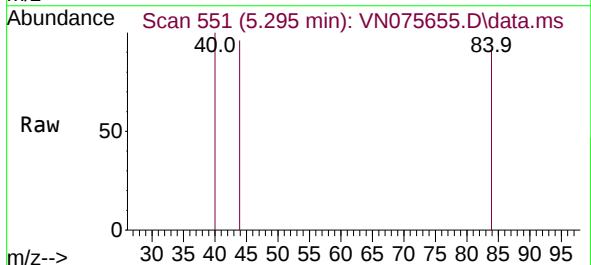

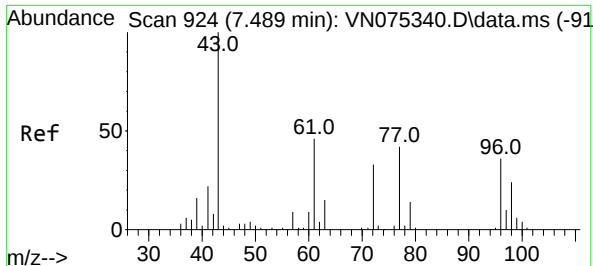

#25

2-Butanone

Concen: 0.721 ug/l

RT: 7.506 min Scan# 91

Delta R.T. 0.017 min

Lab File: VN075655.D

Acq: 08 Dec 2022 18:32

Instrument :

MSVOA_N

ClientSampleId :





NYE-WATER-1208

Tgt Ion: 43 Resp: 863

Ion Ratio Lower Upper

43 100

72 0.0 25.5 38.3#

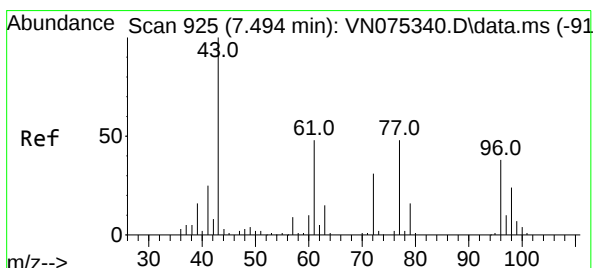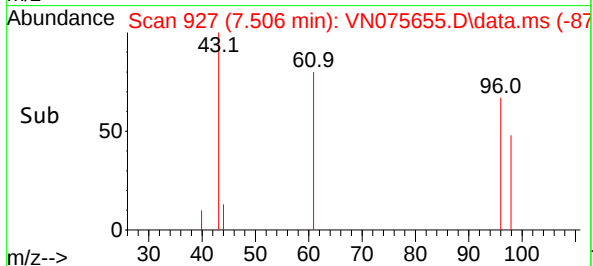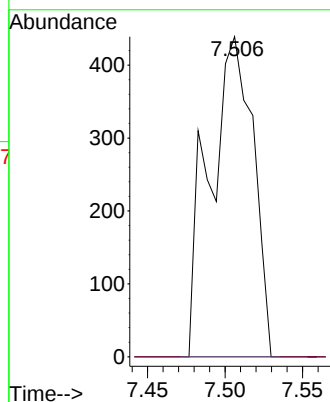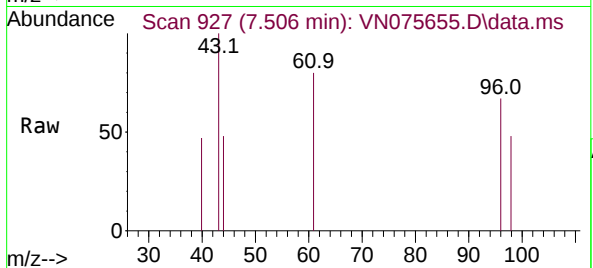

#27

cis-1,2-Dichloroethene

Concen: 0.265 ug/l

RT: 7.489 min Scan# 924

Delta R.T. -0.005 min

Lab File: VN075655.D

Acq: 08 Dec 2022 18:32




Tgt Ion: 96 Resp: 542


Ion Ratio Lower Upper

96 100

61 114.2 0.0 278.8

98 67.3 0.0 128.4

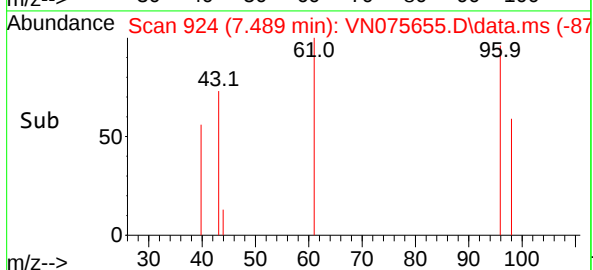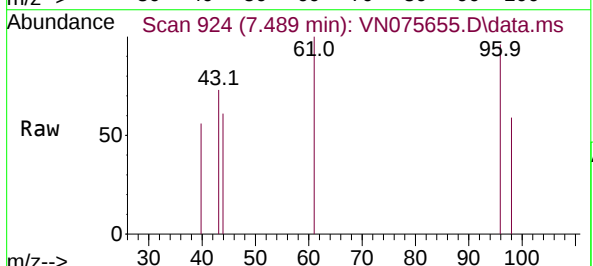

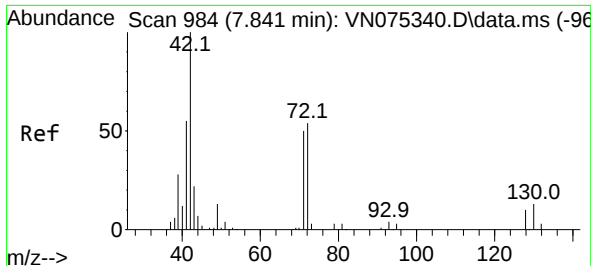

#29

Tetrahydrofuran

Concen: 4.033 ug/l

RT: 7.847 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN075655.D

Acq: 08 Dec 2022 18:32

Instrument :

MSVOA_N

ClientSampleId :

NYE-WATER-1208





Tgt Ion: 42 Resp: 2937

Ion Ratio Lower Upper

42 100

72 61.1 43.0 64.6

71 50.2 39.9 59.9

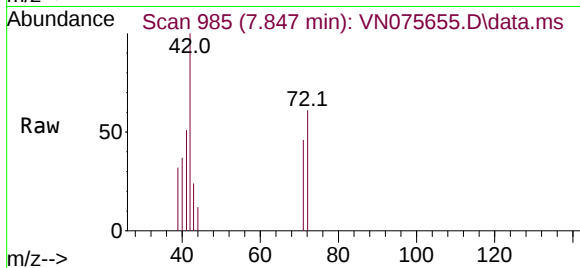

#31

Cyclohexane

Concen: 0.987 ug/l

RT: 8.230 min Scan# 1050

Delta R.T. -0.029 min

Lab File: VN075655.D

Acq: 08 Dec 2022 18:32




Tgt Ion: 56 Resp: 2884


Ion Ratio Lower Upper

56 100

69 146.0 25.2 37.8#

84 149.8 77.8 116.8#

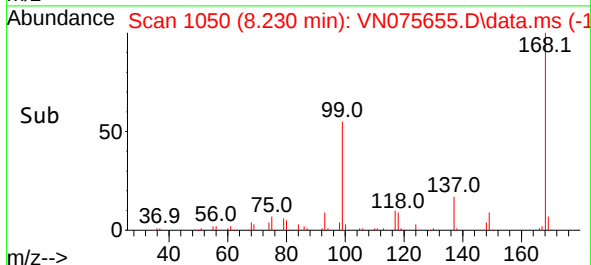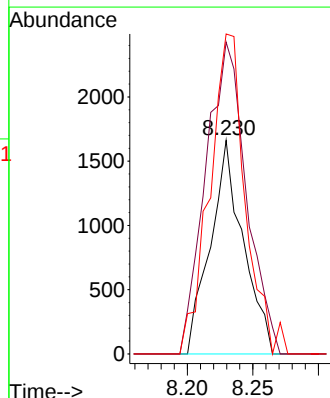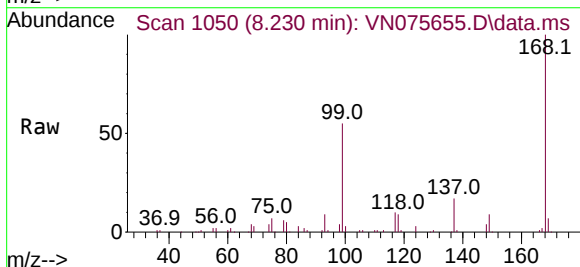

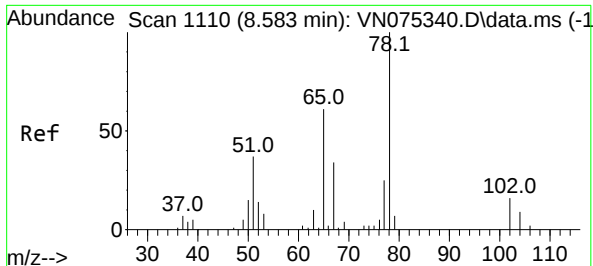

#33

1,2-Dichloroethane-d4

Concen: 50.178 ug/l

RT: 8.583 min Scan# 1110

Delta R.T. -0.000 min

Lab File: VN075655.D

Acq: 08 Dec 2022 18:32

Instrument :

MSVOA_N

ClientSampleId :





NYE-WATER-1208

Tgt Ion: 65 Resp: 46129

Ion Ratio Lower Upper

65 100

67 50.2 0.0 102.0

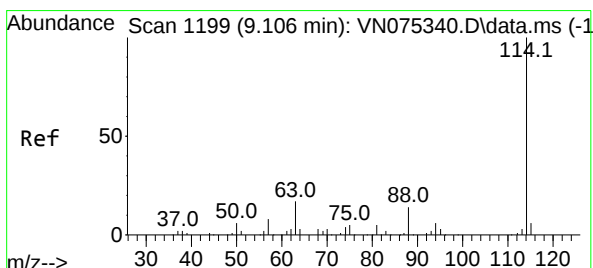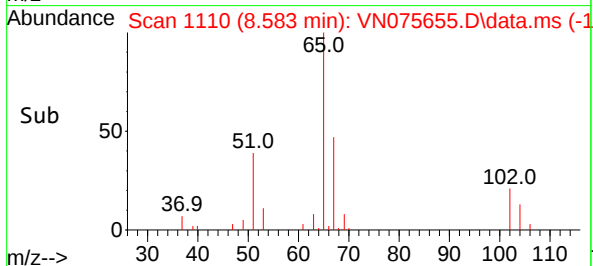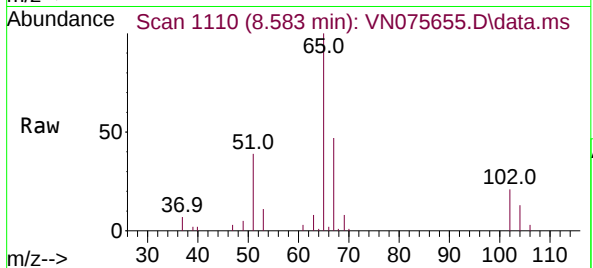

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN075655.D

Acq: 08 Dec 2022 18:32




Tgt Ion: 114 Resp: 276265


Ion Ratio Lower Upper

114 100

63 17.6 0.0 39.6

88 14.4 0.0 29.0

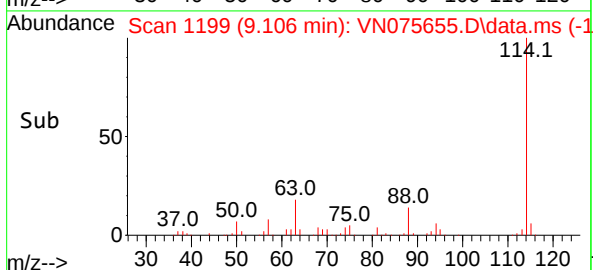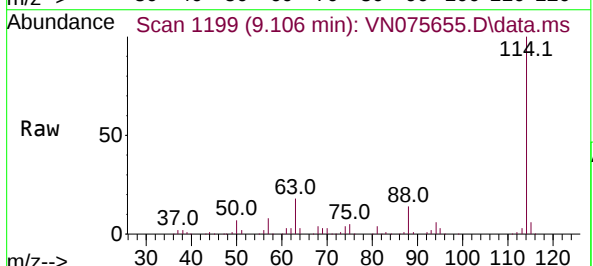

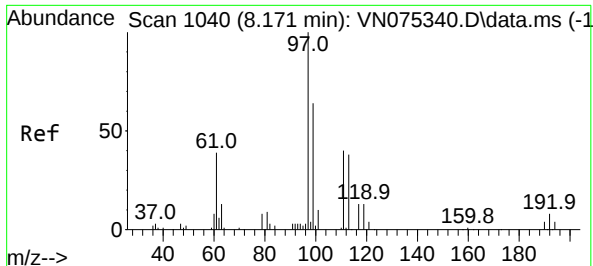

#35

Dibromofluoromethane

Concen: 55.558 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN075655.D

Acq: 08 Dec 2022 18:32

Instrument :

MSVOA_N

ClientSampleId :

NYE-WATER-1208





Tgt Ion:113 Resp: 60295

Ion Ratio Lower Upper

113 100

111 104.1 80.5 120.7

192 21.0 13.2 19.8#

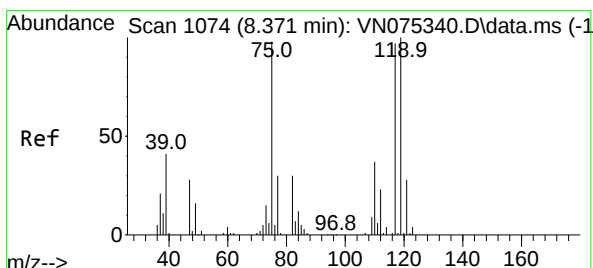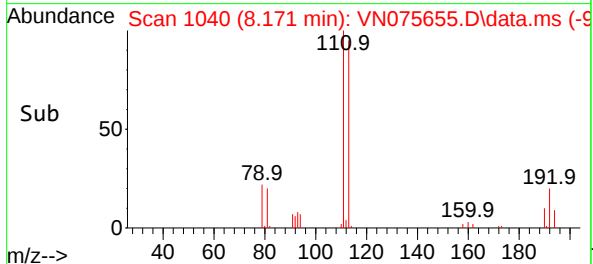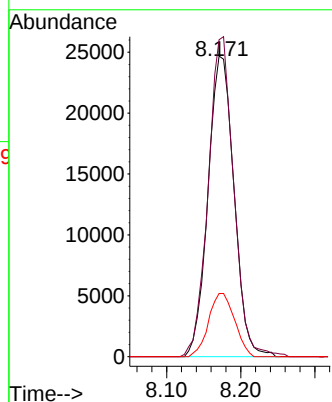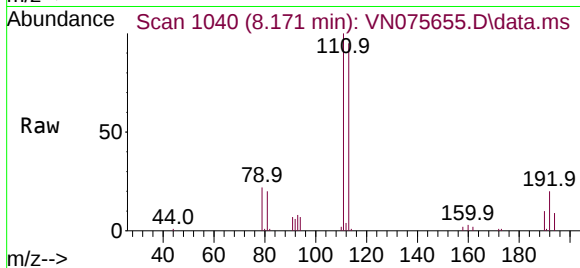

#36

1,1-Dichloropropene

Concen: 4.875 ug/l

RT: 8.230 min Scan# 1050

Delta R.T. -0.141 min

Lab File: VN075655.D

Acq: 08 Dec 2022 18:32




Tgt Ion: 75 Resp: 11537


Ion Ratio Lower Upper

75 100

110 10.4 17.8 53.3#

77 0.0 24.6 37.0#


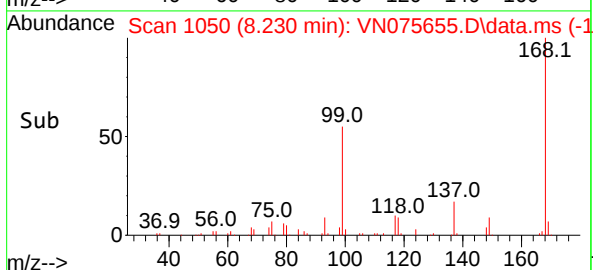

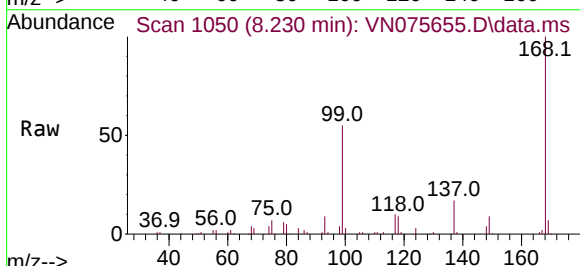


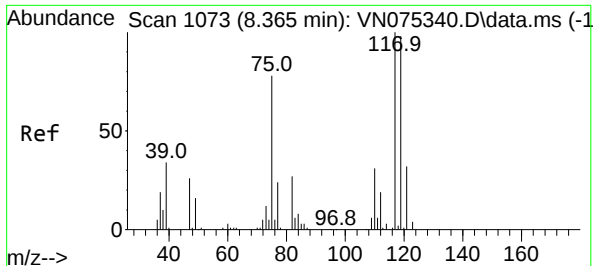

#38
Carbon Tetrachloride
Concen: 6.374 ug/l
RT: 8.230 min Scan# 1
Delta R.T. -0.135 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion:117 Resp: 16571
Ion Ratio Lower Upper
117 100
119 6.1 76.7 115.1#
121 0.0 23.9 35.9#

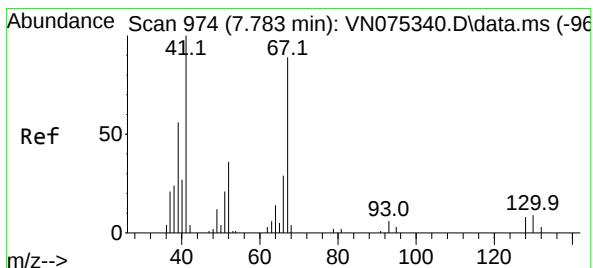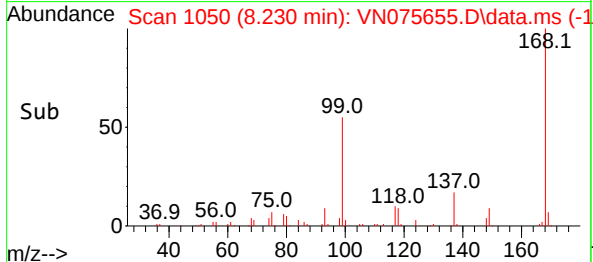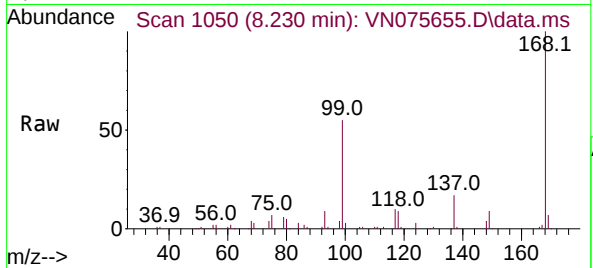

#41
Methacrylonitrile
Concen: 1.980 ug/l
RT: 7.853 min Scan# 986
Delta R.T. 0.070 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion: 41 Resp: 2157
Ion Ratio Lower Upper
41 100
39 43.6 44.4 66.6#
67 0.0 69.8 104.6#
52 0.0 27.3 40.9#


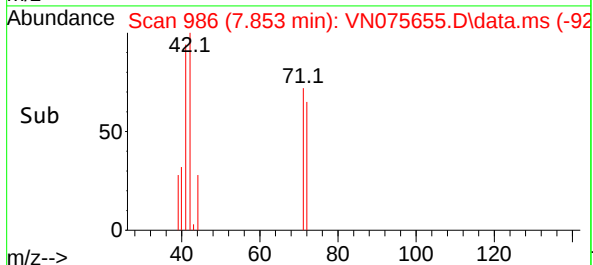
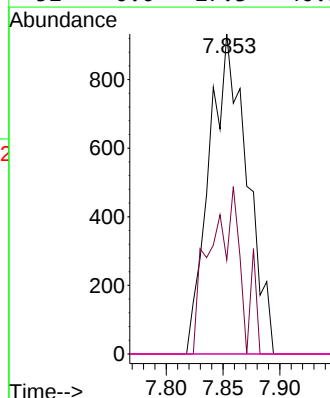
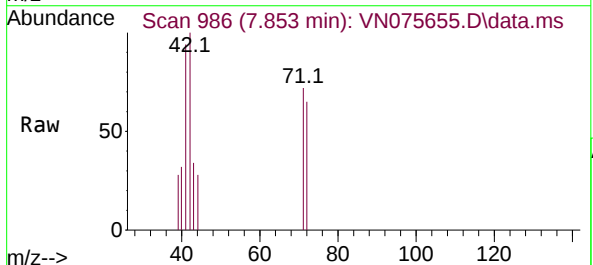


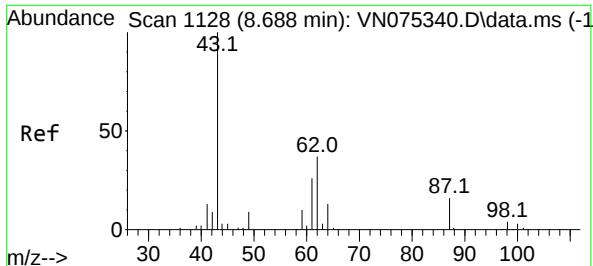

#43
Isopropyl Acetate
Concen: 0.654 ug/l
RT: 8.759 min Scan# 1140
Delta R.T. 0.071 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion: 43 Resp: 2238
Ion Ratio Lower Upper
43 100
61 0.0 22.4 33.6#
87 0.0 12.5 18.7#

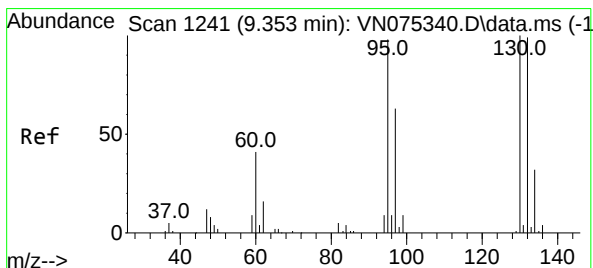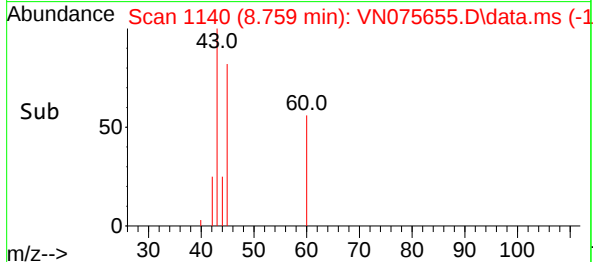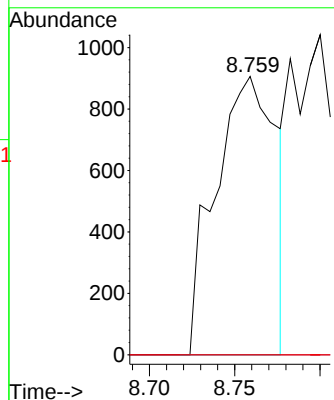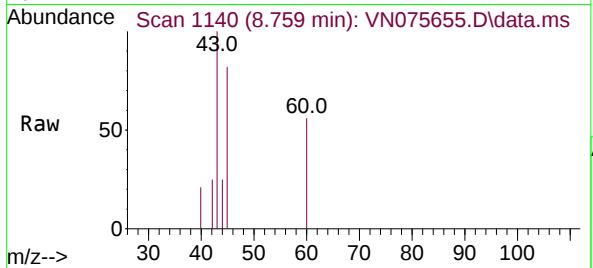

#44
Trichloroethene
Concen: 0.893 ug/l
RT: 9.359 min Scan# 1242
Delta R.T. 0.006 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion: 130 Resp: 1771
Ion Ratio Lower Upper
130 100
95 111.9 0.0 198.4


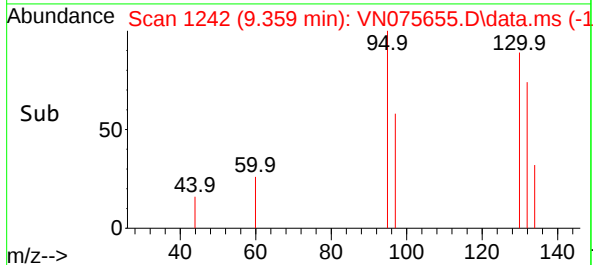
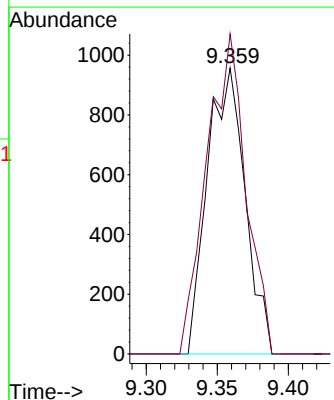
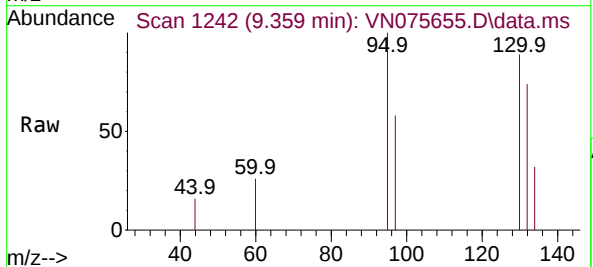




#50
Toluene-d8
Concen: 50.112 ug/l
RT: 10.571 min Scan# 1447
Delta R.T. 0.006 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion: 98 Resp: 122488
Ion Ratio Lower Upper
98 100
100 64.9 53.0 79.6

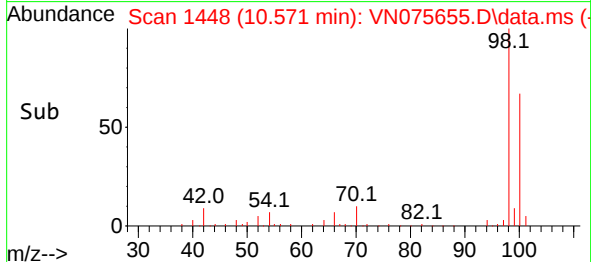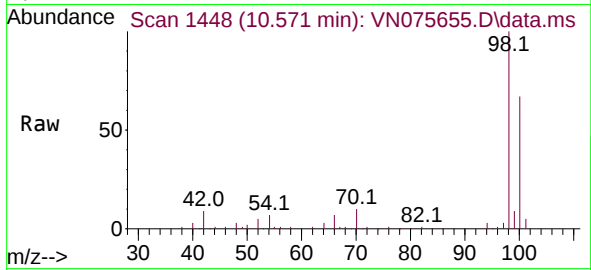

#51
4-Methyl-2-Pentanone
Concen: 0.413 ug/l
RT: 10.453 min Scan# 1428
Delta R.T. 0.006 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion: 43 Resp: 900
Ion Ratio Lower Upper
43 100
58 21.4 33.6 50.4#


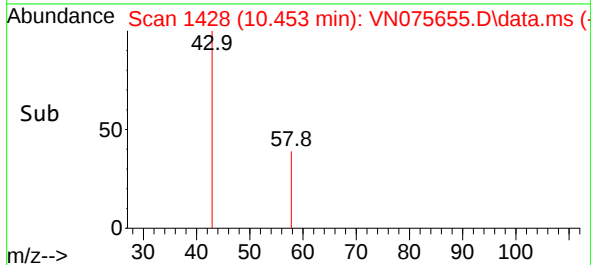






#52
Toluene
Concen: 1.359 ug/l
RT: 10.635 min Scan# 1458
Delta R.T. 0.005 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion: 92 Resp: 6347
Ion Ratio Lower Upper
92 100
91 168.3 135.4 203.2



#59
2-Hexanone
Concen: 0.582 ug/l
RT: 11.200 min Scan# 1555
Delta R.T. 0.006 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion: 43 Resp: 952
Ion Ratio Lower Upper
43 100
58 53.0 29.6 88.8


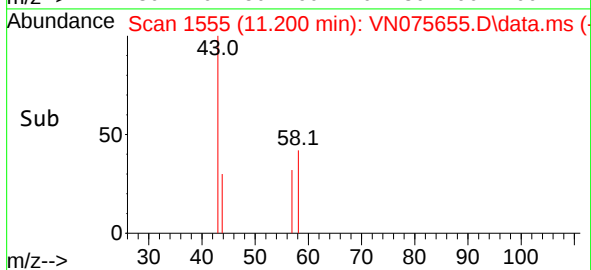




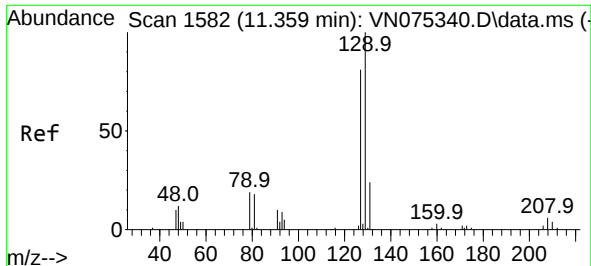

#60
Dibromochloromethane
Concen: 0.899 ug/l
RT: 11.100 min Scan# 11
Delta R.T. -0.259 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion:129 Resp: 1755
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

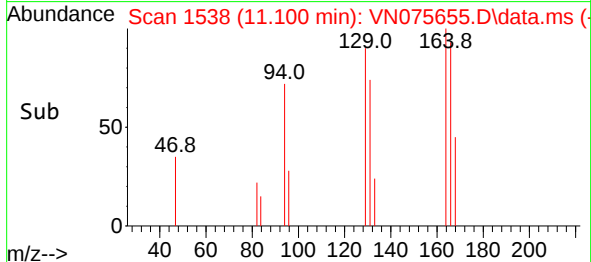

#62
4-Bromofluorobenzene
Concen: 48.068 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion: 95 Resp: 86723
Ion Ratio Lower Upper
95 100
174 89.4 0.0 147.4
176 86.0 0.0 142.2




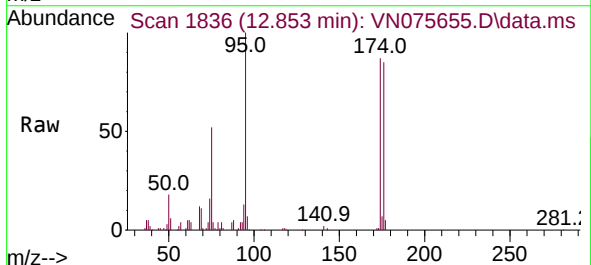




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion:117 Resp: 240180
Ion Ratio Lower Upper
117 100
82 52.6 43.1 64.7
119 29.8 25.5 38.3

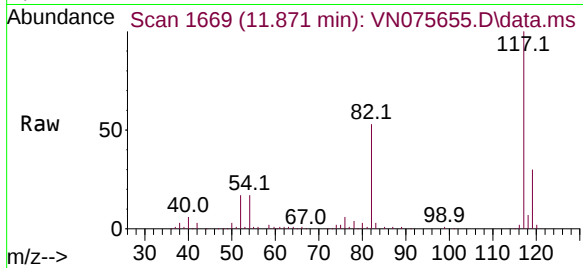

#64
Tetrachloroethene
Concen: 0.940 ug/l
RT: 11.100 min Scan# 1538
Delta R.T. -0.006 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion:164 Resp: 1724
Ion Ratio Lower Upper
164 100
166 93.3 106.5 159.7#
129 90.0 81.9 122.9
131 74.3 81.4 122.2#


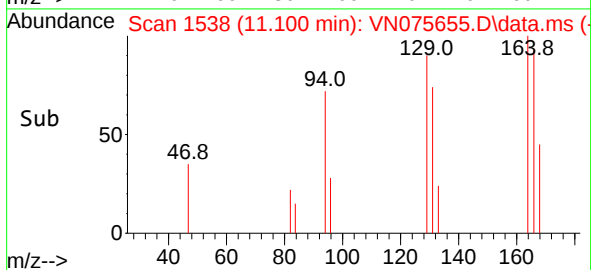

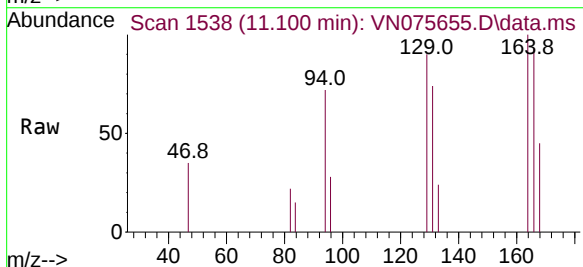


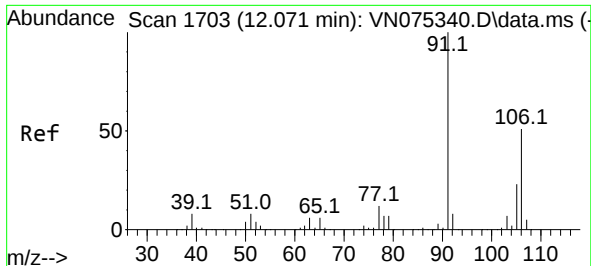

#68
m/p-Xylenes
Concen: 0.306 ug/l
RT: 12.071 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion:106 Resp: 1053
Ion Ratio Lower Upper
106 100
91 207.4 156.0 234.0

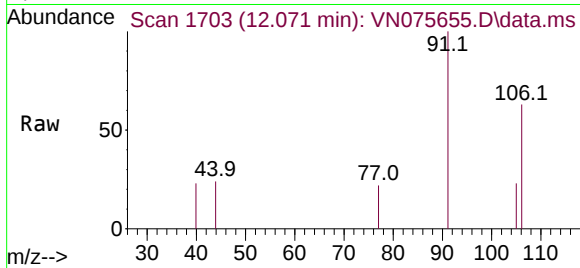

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion:152 Resp: 106436
Ion Ratio Lower Upper
152 100
115 55.9 30.2 90.6
150 153.4 0.0 348.4




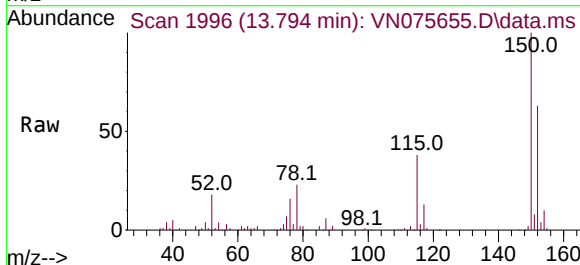


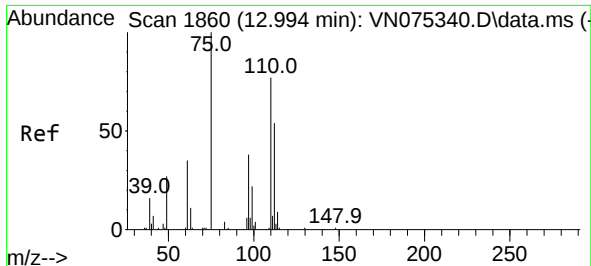

#76
1,2,3-Trichloropropane
Concen: 22.231 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion: 75 Resp: 44739
Ion Ratio Lower Upper
75 100
77 0.9 75.6 226.8#



#81
trans-1,4-Dichloro-2-butene
Concen: 65.778 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.118 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion: 75 Resp: 44739
Ion Ratio Lower Upper
75 100
53 0.0 78.5 117.7#
89 0.0 37.7 56.5#


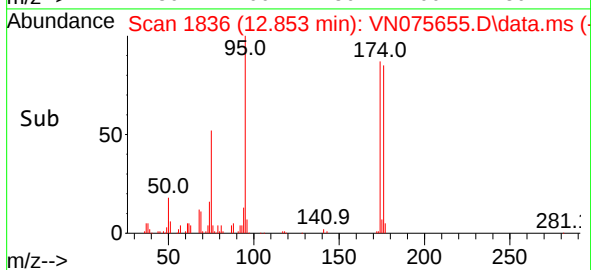




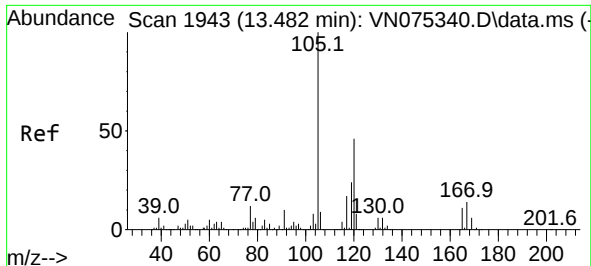

#84
1,2,4-Trimethylbenzene
Concen: 0.201 ug/l
RT: 13.488 min Scan# 1943
Delta R.T. 0.006 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion:105 Resp: 1304
Ion Ratio Lower Upper
105 100
120 32.8 22.7 68.1

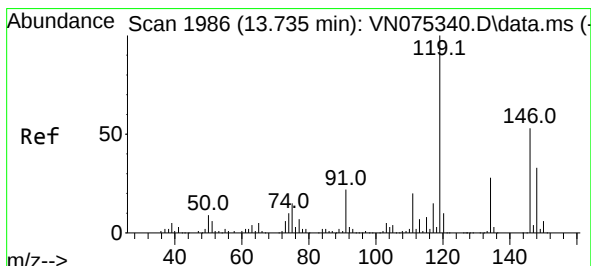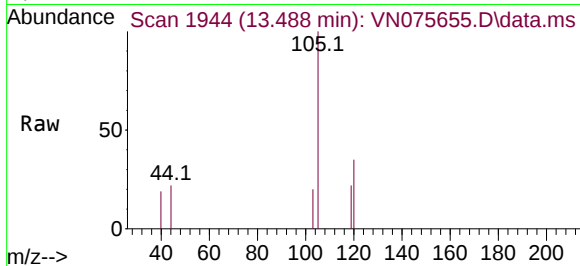

#87
1,3-Dichlorobenzene
Concen: 0.240 ug/l
RT: 13.735 min Scan# 1986
Delta R.T. 0.000 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32

Tgt Ion:146 Resp: 872
Ion Ratio Lower Upper
146 100
111 31.3 20.8 62.5
148 43.0 31.1 93.5




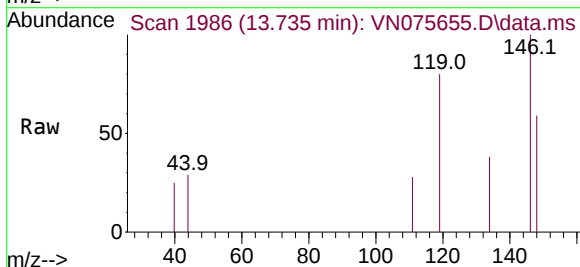


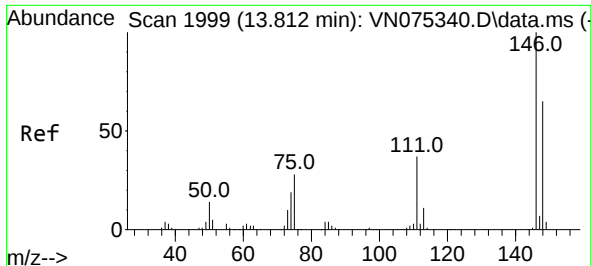

#88
 1,4-Dichlorobenzene
 Concen: 0.236 ug/l
 RT: 13.735 min Scan# 1999
 Delta R.T. -0.077 min
 Lab File: VN075655.D
 Acq: 08 Dec 2022 18:32




Instrument :
 MSVOA_N
 ClientSampleId :
 NYE-WATER-1208


Tgt Ion:146 Resp: 872
 Ion Ratio Lower Upper
 146 100
 111 31.3 20.1 60.3
 148 43.0 31.9 95.7



#91
 1,2-Dichlorobenzene
 Concen: 0.264 ug/l
 RT: 14.112 min Scan# 2050
 Delta R.T. 0.006 min
 Lab File: VN075655.D
 Acq: 08 Dec 2022 18:32

Tgt Ion:146 Resp: 937
 Ion Ratio Lower Upper
 146 100
 111 34.6 21.3 63.9
 148 58.9 31.4 94.2


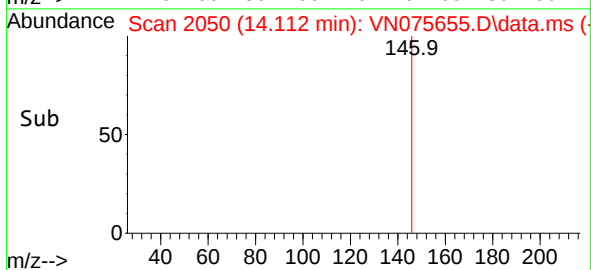






#93
1,2,4-Trichlorobenzene
Concen: 0.538 ug/l
RT: 15.400 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32




Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208


Tgt Ion:180 Resp: 977
Ion Ratio Lower Upper
180 100
182 106.1 47.8 143.4
145 14.3 16.8 50.3#



#95
Naphthalene
Concen: 0.983 ug/l
RT: 15.641 min Scan# 2310
Delta R.T. -0.000 min
Lab File: VN075655.D
Acq: 08 Dec 2022 18:32


Tgt Ion:128 Resp: 5620
Ion Ratio Lower Upper
128 100
127 12.0 10.4 15.6
129 7.8 8.6 12.8#

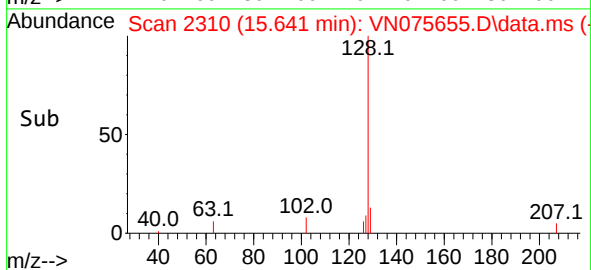



#96
 1,2,3-Trichlorobenzene
 Concen: 0.769 ug/l
 RT: 15.847 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN075655.D
 Acq: 08 Dec 2022 18:32

Instrument :
 MSVOA_N
 ClientSampleId :
 NYE-WATER-1208

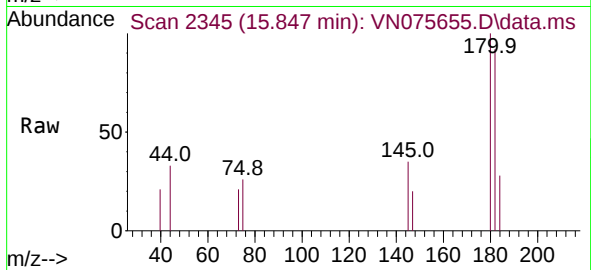

Tgt Ion:	180	Resp:	1374
Ion	Ratio	Lower	Upper
180	100		
182	100.9	47.3	141.8
145	32.2	17.6	52.9

