

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120822\
 Data File : VN075647.D
 Acq On : 08 Dec 2022 14:56
 Operator : JC\MD
 Sample : N5924-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 EFF1222

Quant Time: Dec 09 02:07:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 23 00:18:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.235	168	165635	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	269600	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	232593	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	97140	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	44641	50.209	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	100.420%
35) Dibromofluoromethane	8.177	113	57385	54.184	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	108.360%
50) Toluene-d8	10.571	98	113615	47.631	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	95.260%
62) 4-Bromofluorobenzene	12.853	95	79216	44.993	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.980%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120822\
Data File : VN075647.D
Acq On : 08 Dec 2022 14:56
Operator : JC\MD
Sample : N5924-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
EFF1222

Quant Time: Dec 09 02:07:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 23 00:18:03 2022
Response via : Initial Calibration




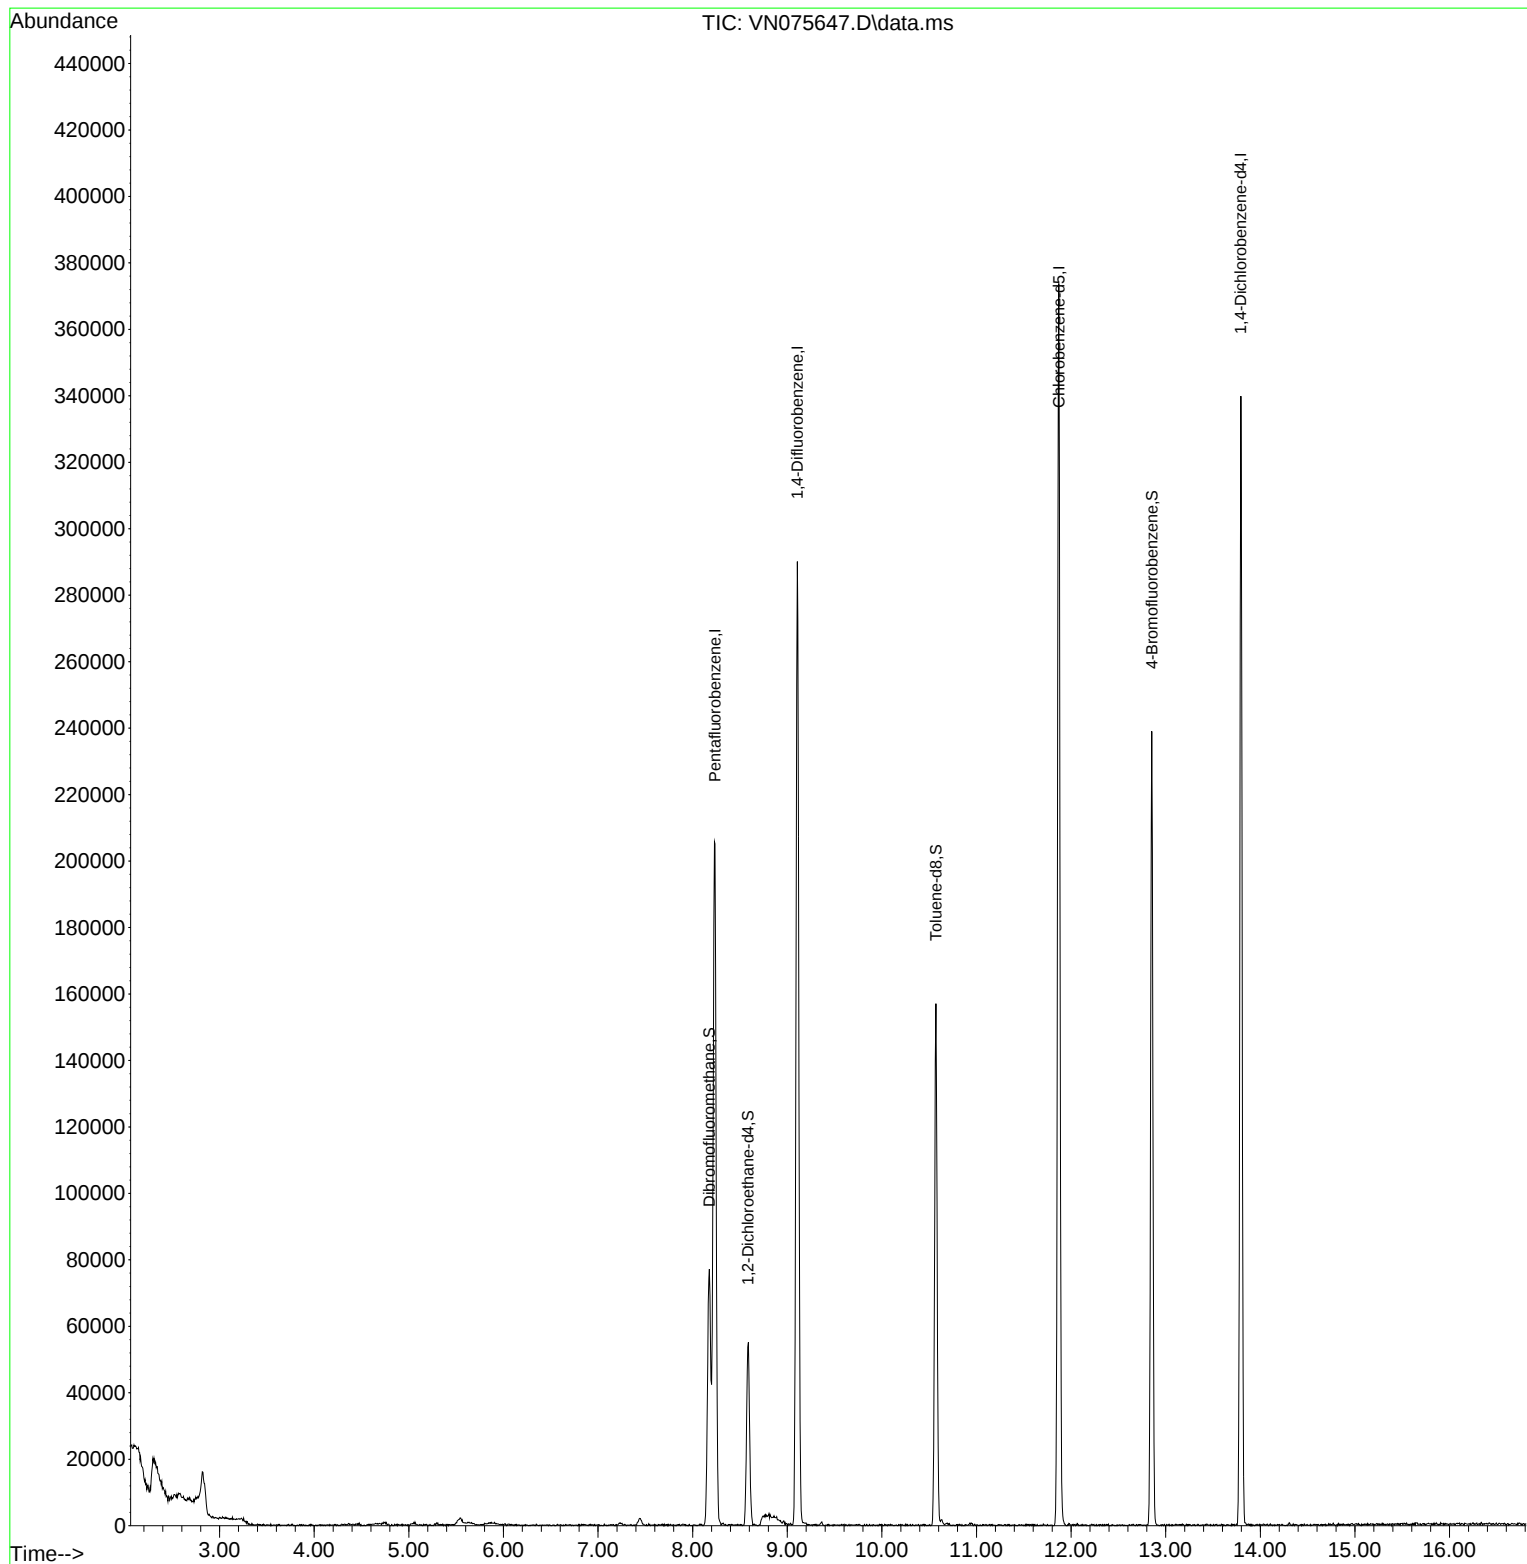


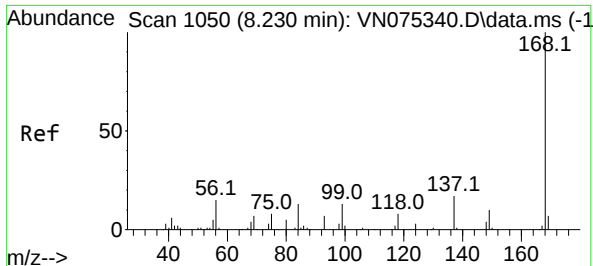

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1050
Delta R.T. 0.005 min
Lab File: VN075647.D
Acq: 08 Dec 2022 14:56




Instrument :
MSVOA_N
ClientSampleId :
EFF1222


Tgt Ion:168 Resp: 165635
Ion Ratio Lower Upper
168 100
99 52.9 51.6 77.4

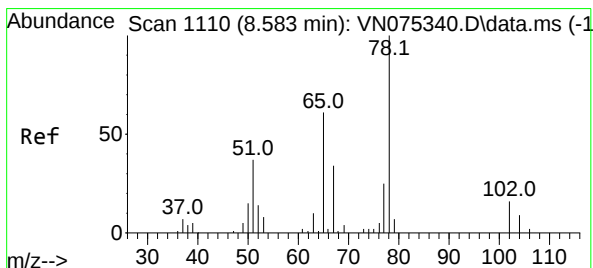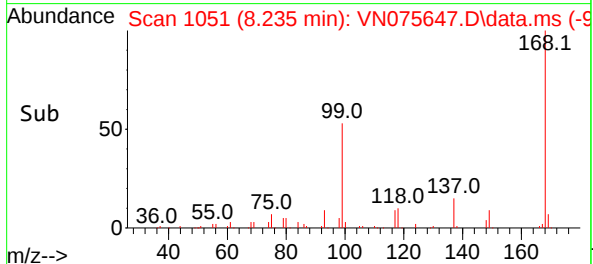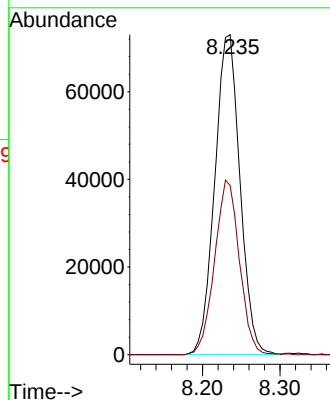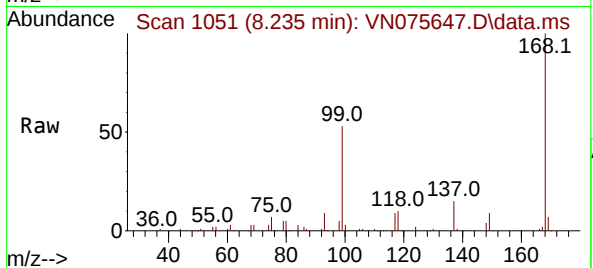

#33
1,2-Dichloroethane-d4
Concen: 50.209 ug/l
RT: 8.582 min Scan# 1110
Delta R.T. -0.001 min
Lab File: VN075647.D
Acq: 08 Dec 2022 14:56

Tgt Ion: 65 Resp: 44641
Ion Ratio Lower Upper
65 100
67 52.4 0.0 102.0

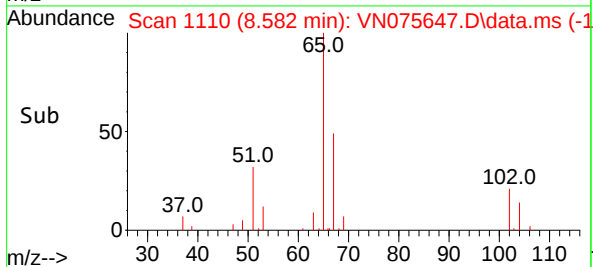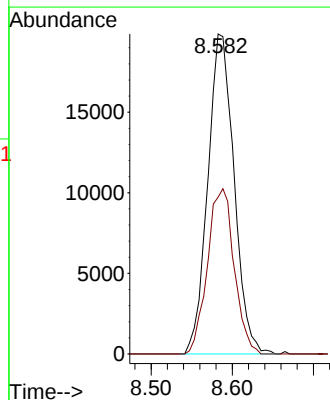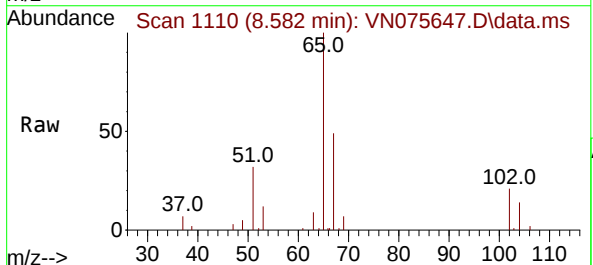

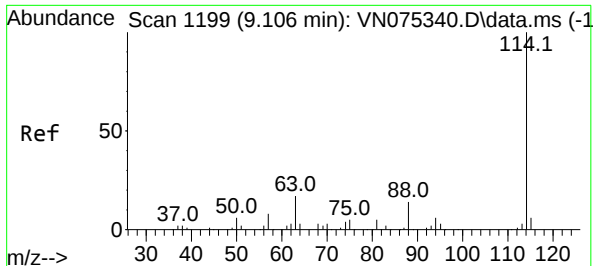

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN075647.D

Acq: 08 Dec 2022 14:56

Instrument :

MSVOA_N

ClientSampleId :

EFF1222




Tgt Ion:114 Resp: 269600

Ion Ratio Lower Upper

114 100

63 18.3 0.0 39.6

88 14.2 0.0 29.0

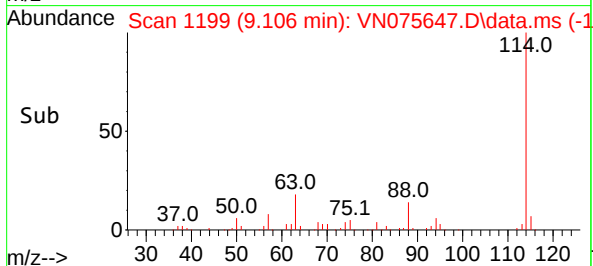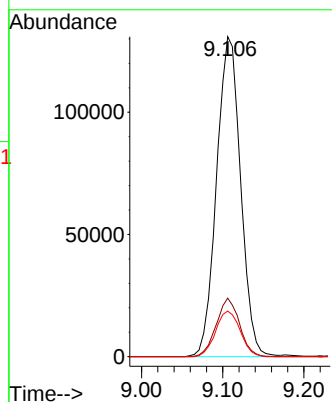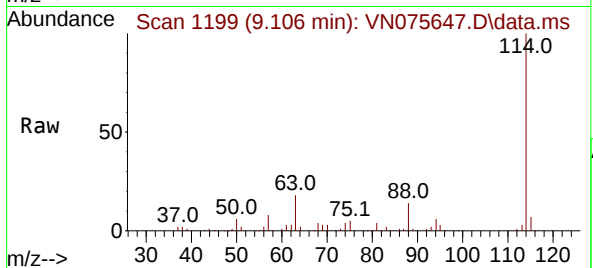

#35

Dibromofluoromethane

Concen: 54.184 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN075647.D

Acq: 08 Dec 2022 14:56




Tgt Ion:113 Resp: 57385


Ion Ratio Lower Upper

113 100

111 101.6 80.5 120.7

192 19.5 13.2 19.8


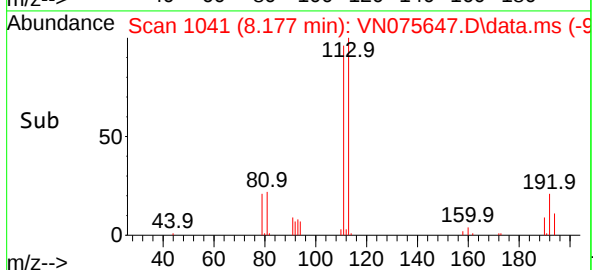
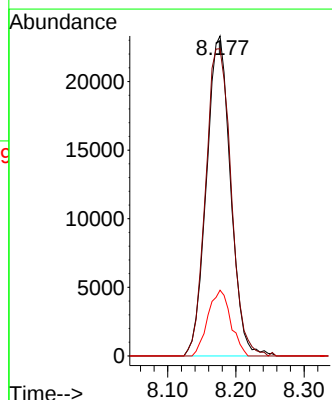
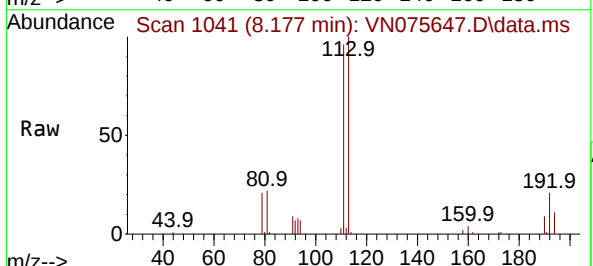


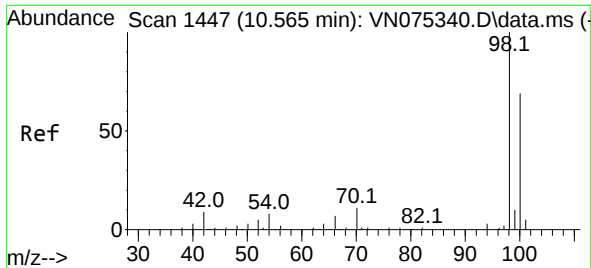

#50
Toluene-d8
Concen: 47.631 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. 0.006 min
Lab File: VN075647.D
Acq: 08 Dec 2022 14:56




Instrument :
MSVOA_N
ClientSampleId :
EFF1222


Tgt Ion: 98 Resp: 113615
Ion Ratio Lower Upper
98 100
100 64.5 53.0 79.6

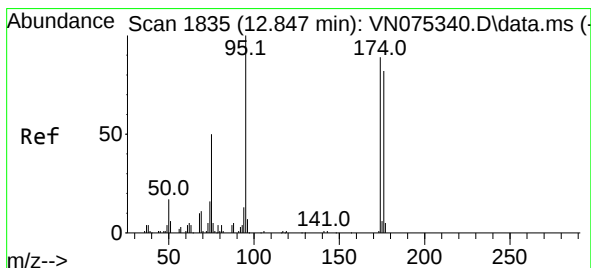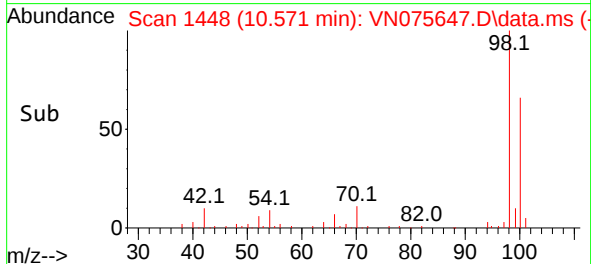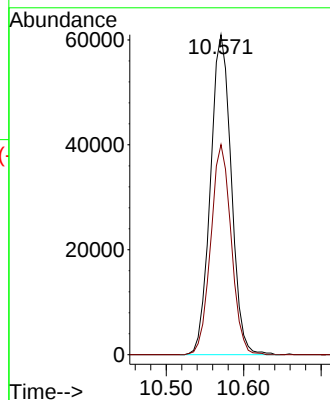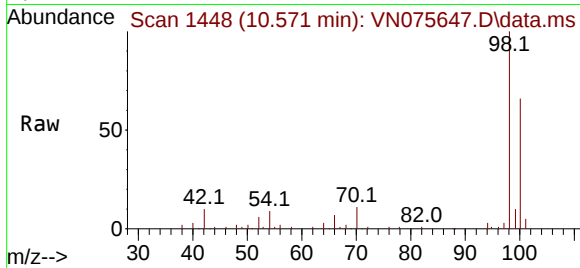

#62
4-Bromofluorobenzene
Concen: 44.993 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN075647.D
Acq: 08 Dec 2022 14:56

Tgt Ion: 95 Resp: 79216
Ion Ratio Lower Upper
95 100
174 88.1 0.0 147.4
176 86.9 0.0 142.2


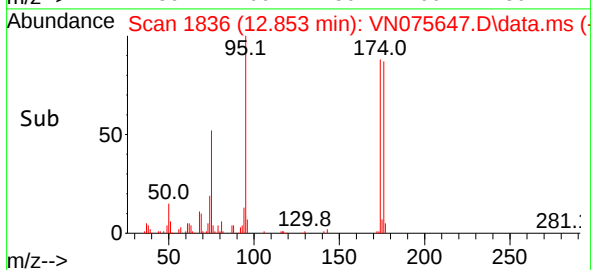
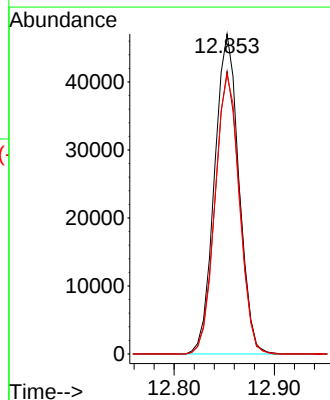
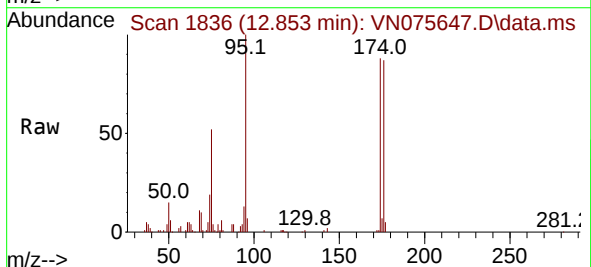


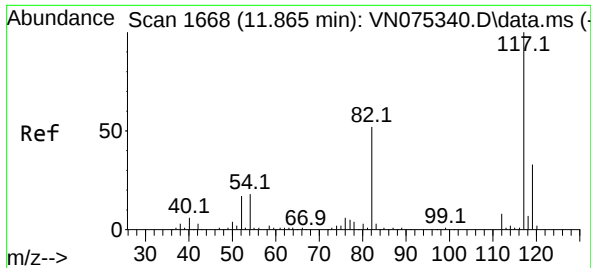

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN075647.D
Acq: 08 Dec 2022 14:56

Instrument :
MSVOA_N
ClientSampleId :
EFF1222

Tgt Ion:117 Resp: 232593
Ion Ratio Lower Upper
117 100
82 50.3 43.1 64.7
119 32.9 25.5 38.3

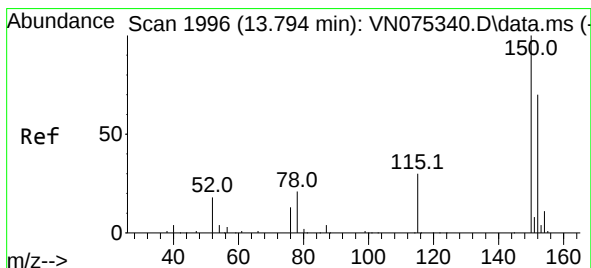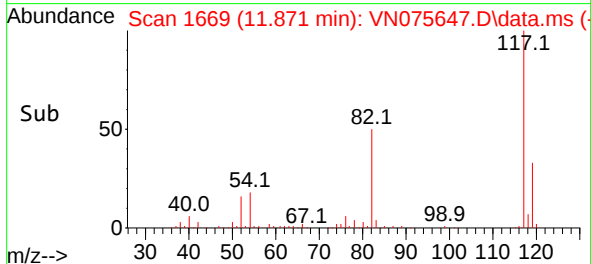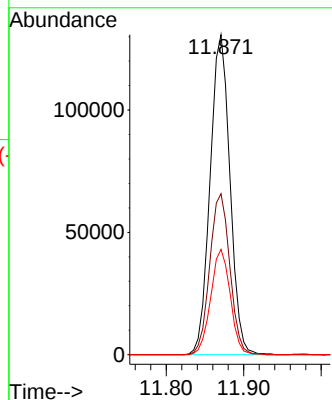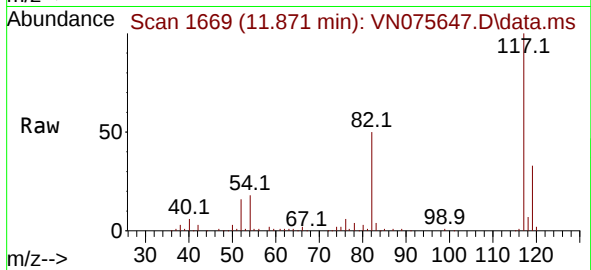

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075647.D
Acq: 08 Dec 2022 14:56

Tgt Ion:152 Resp: 97140
Ion Ratio Lower Upper
152 100
115 58.3 30.2 90.6
150 157.0 0.0 348.4

