

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120822\
 Data File : VN075655.D
 Acq On : 08 Dec 2022 18:32
 Operator : JC\MD
 Sample : N5947-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 NYE-WATER-1208

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Title : SW846 8260

Signal : TIC: VN075655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.289	37	40	51	rBV2	13145	41539	6.07%	1.165%
2	2.818	125	130	131	rBV2	9265	11068	1.62%	0.310%
3	7.847	980	985	994	rBV4	4448	11112	1.62%	0.312%
4	8.171	1031	1040	1045	rBV	84426	206765	30.20%	5.798%
5	8.230	1045	1050	1059	rVB	213312	464466	67.84%	13.025%
6	8.583	1102	1110	1121	rBV2	56297	129224	18.87%	3.624%
7	8.759	1133	1140	1143	rBV2	2806	6972	1.02%	0.196%
8	9.106	1190	1199	1211	rBV	296266	601039	87.78%	16.855%
9	9.353	1236	1241	1249	rBB4	5049	9510	1.39%	0.267%
10	10.571	1440	1448	1455	rBV	167397	308979	45.13%	8.664%
11	10.635	1455	1459	1466	rVB	12748	22443	3.28%	0.629%
12	11.106	1534	1539	1544	rVB3	7167	11546	1.69%	0.324%
13	11.871	1659	1669	1681	rBV	382252	684691	100.00%	19.200%
14	12.853	1826	1836	1844	rBV	264693	438179	64.00%	12.288%
15	13.794	1989	1996	2006	rVB	363719	608814	88.92%	17.073%
16	15.647	2305	2311	2320	rVB2	4572	9691	1.42%	0.272%




Sum of corrected areas: 3566038

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120822\
Data File : VN075655.D
Acq On : 08 Dec 2022 18:32
Operator : JC\MD
Sample : N5947-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

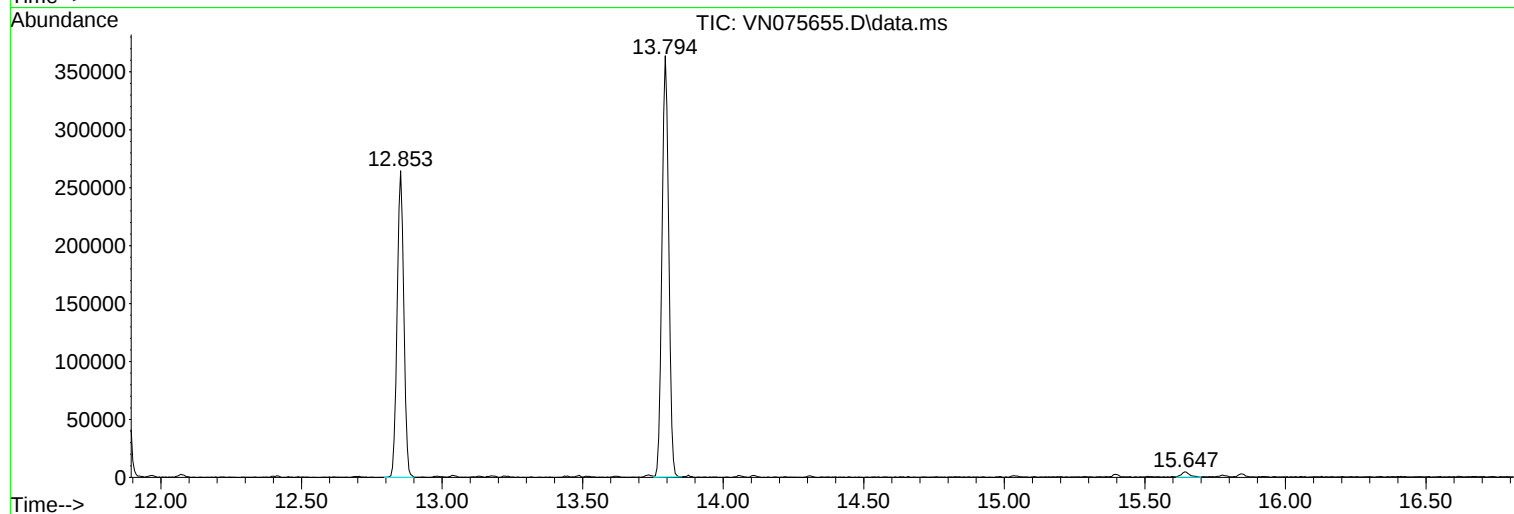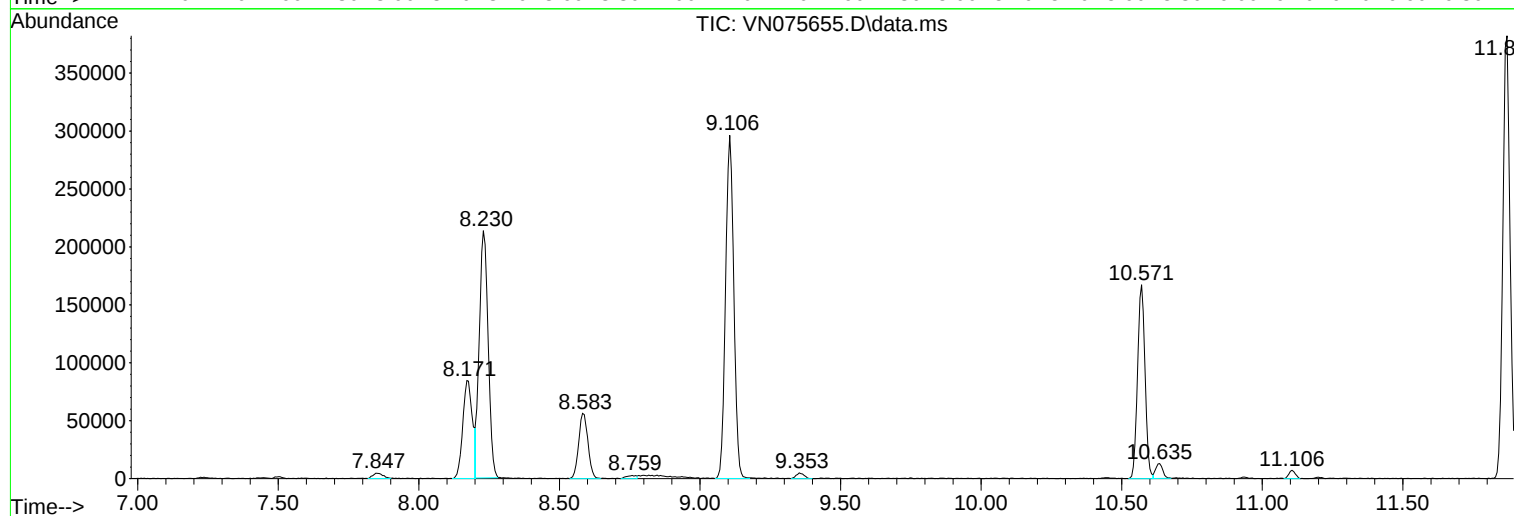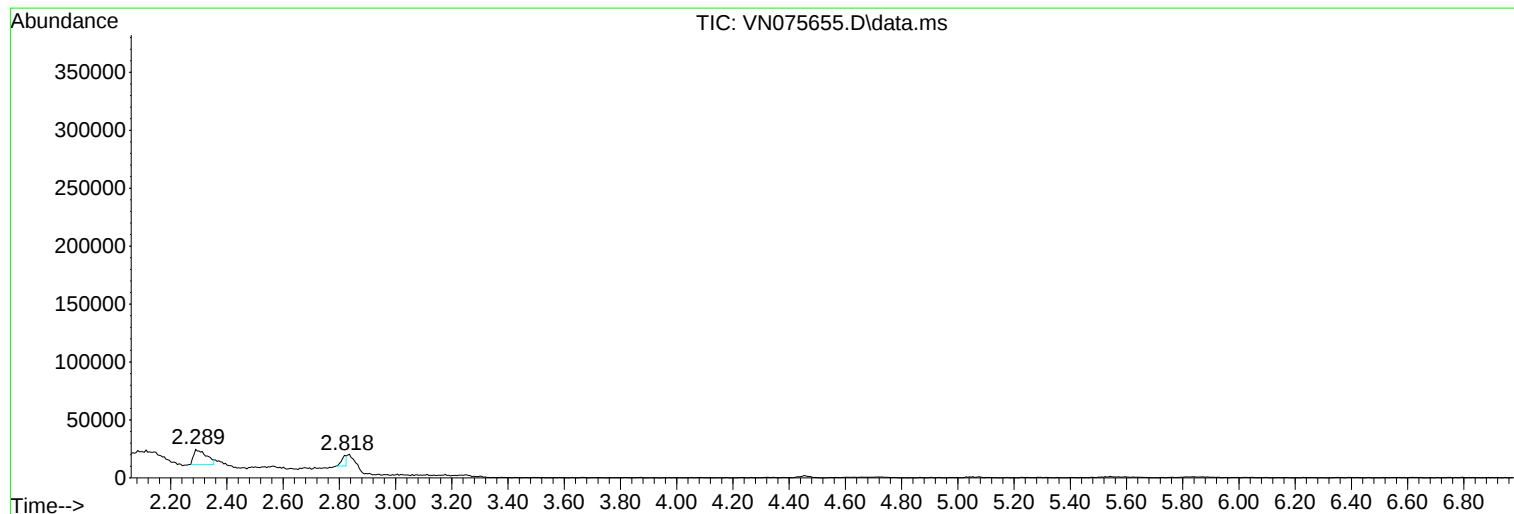

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120822\
Data File : VN075655.D
Acq On : 08 Dec 2022 18:32
Operator : JC\MD
Sample : N5947-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120822\
Data File : VN075655.D
Acq On : 08 Dec 2022 18:32
Operator : JC\MD
Sample : N5947-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NYE-WATER-1208

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc