
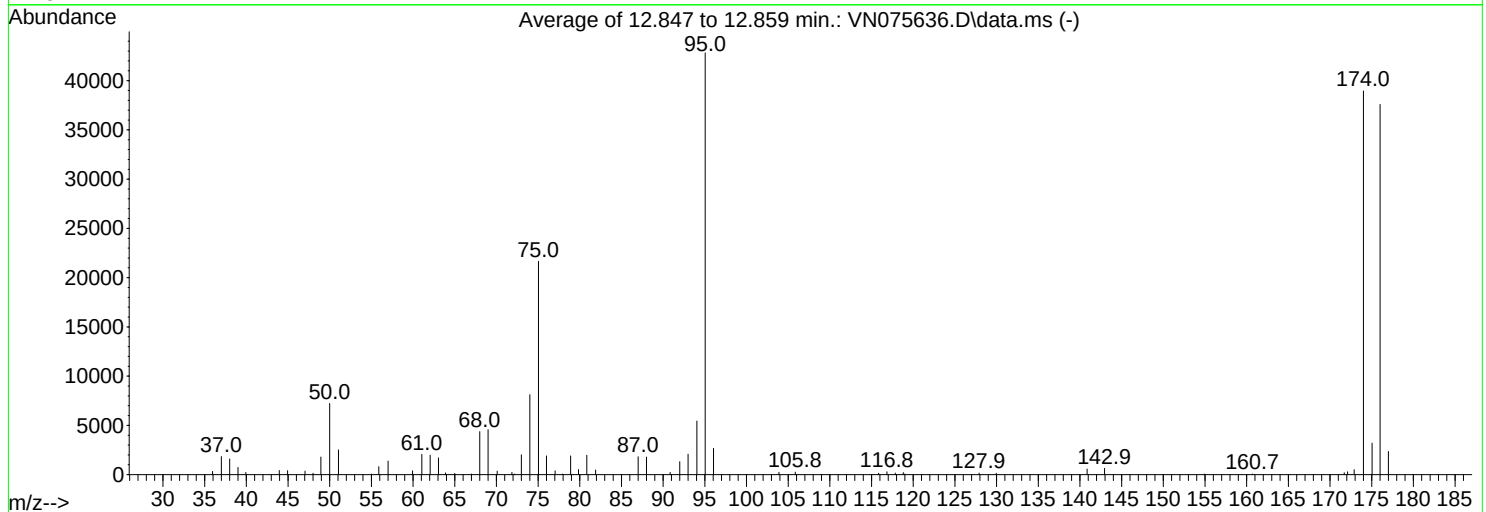


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120822\
Data File : VN075636.D
Acq On : 08 Dec 2022 09:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Title : SW846 8260
Last Update : Wed Nov 23 00:18:03 2022

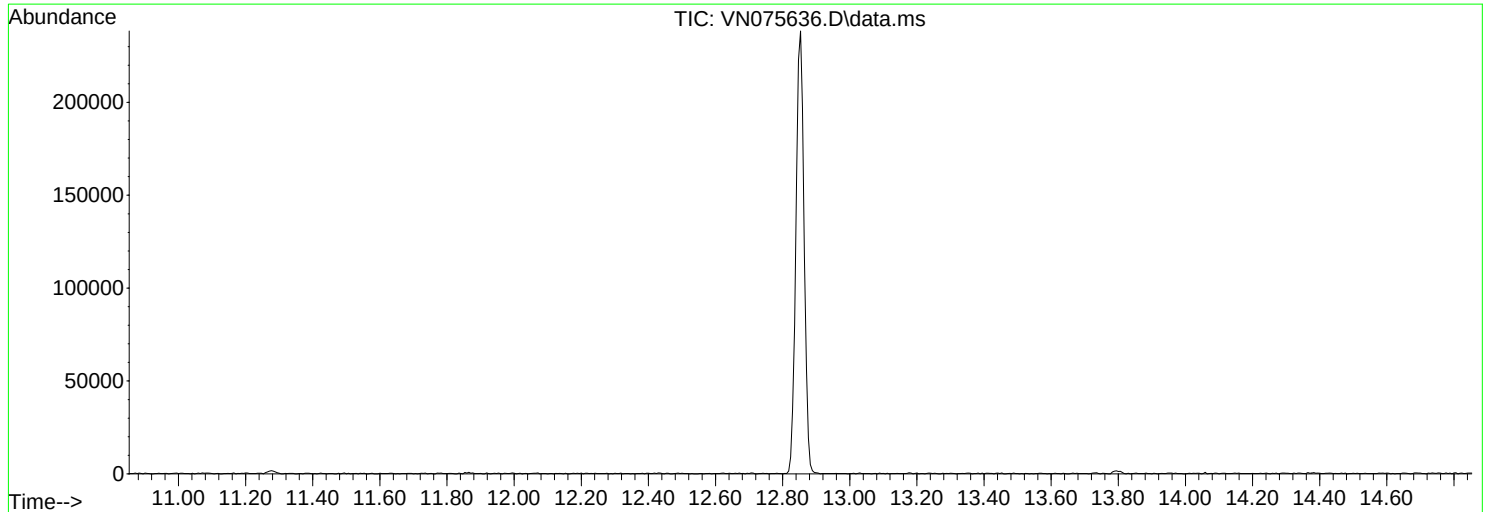

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	7226	PASS
75	95	30	60	50.6	21648	PASS
95	95	100	100	100.0	42821	PASS
96	95	5	9	6.2	2668	PASS
173	174	0.00	2	1.3	496	PASS
174	95	50	100	91.0	38947	PASS
175	174	5	9	8.2	3200	PASS
176	174	95	101	96.5	37581	PASS
177	176	5	9	6.3	2359	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	326	51.05	2513	68.00	4369	78.90	1901
37.00	1836	55.00	66	69.00	4570	79.85	511
38.00	1601	55.90	818	70.10	362	80.85	196
39.00	727	57.00	1389	71.85	227	81.90	47
39.95	236	59.95	391	72.20	72	87.00	1822
43.95	417	61.05	2058	73.00	2013	88.00	1794
44.95	415	62.05	1984	74.00	8131	90.85	228
47.05	360	63.05	1698	75.05	21648	92.00	1321
48.00	147	63.90	181	76.00	1900	93.00	2078
48.95	1787	65.00	132	77.05	386	94.05	5446
50.00	7226	67.00	59	77.90	68	95.05	42821

Average of 12.847 to 12.859 min.: VN075636.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.05	2668	142.95	626				
103.90	251	154.90	58				
105.85	258	160.70	73				
115.85	144	171.70	195				
116.85	300	172.10	292				
117.85	167	172.90	496				
118.80	219	174.00	38947				
119.00	63	175.05	3200				
127.90	163	176.00	37581				
129.95	154	177.00	2359				
140.85	570						

Instrument :

MSVOA_N

ClientSampleId :

BFB