
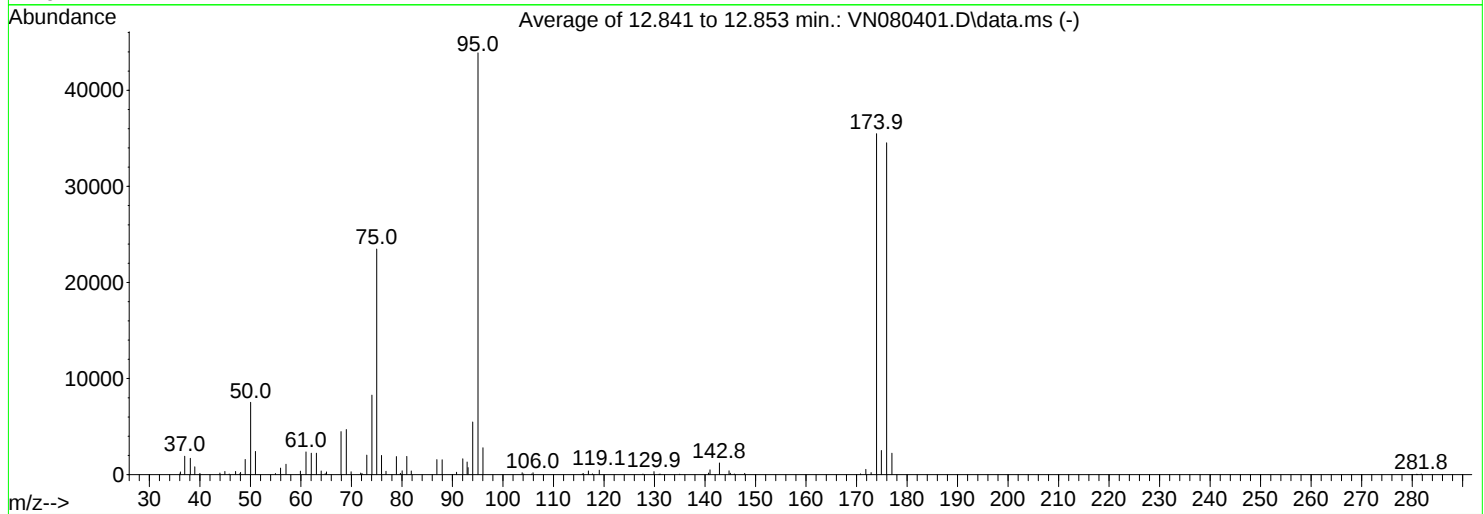


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120823\
Data File : VN080401.D
Acq On : 08 Dec 2023 12:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

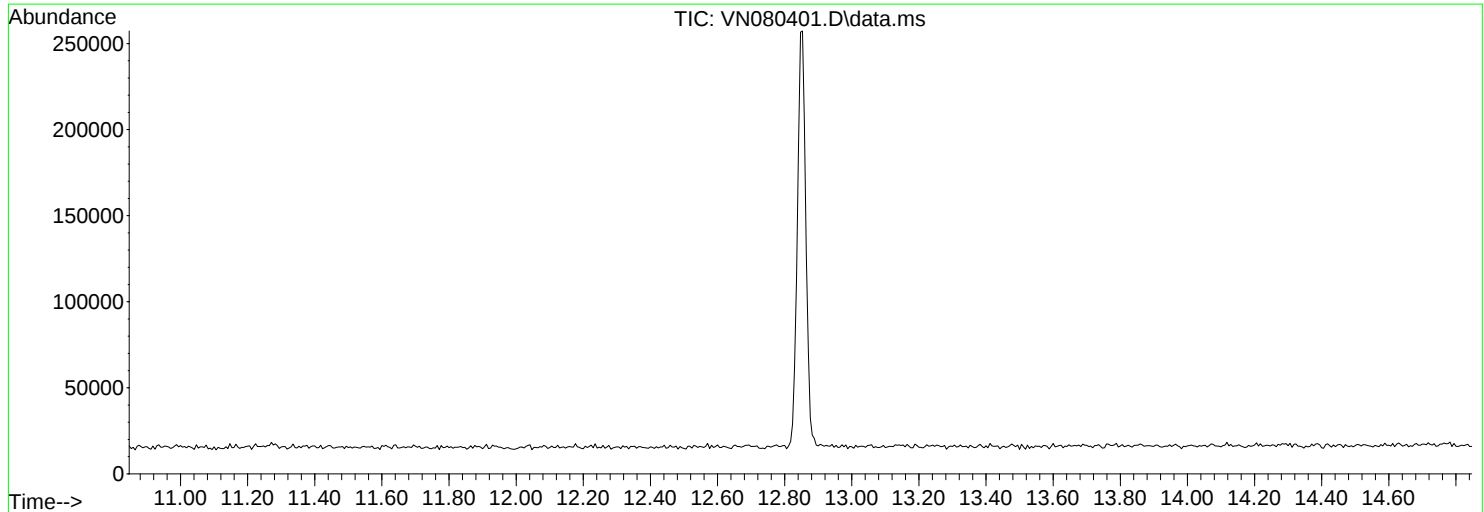

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	7521	PASS
75	95	30	60	53.5	23485	PASS
95	95	100	100	100.0	43896	PASS
96	95	5	9	6.4	2790	PASS
173	174	0.00	2	0.6	214	PASS
174	95	50	100	80.8	35477	PASS
175	174	5	9	7.1	2512	PASS
176	174	95	101	97.3	34531	PASS
177	176	5	9	6.5	2234	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	71	48.05	226	64.00	379	75.95	199
36.15	277	48.95	1585	64.80	96	76.85	34
37.00	1911	50.05	7521	65.05	285	78.90	189
38.10	1697	51.00	2415	67.95	4485	79.70	14
39.00	825	54.95	120	69.00	4700	80.05	408
40.00	133	55.95	682	69.95	295	80.95	1901
43.95	174	57.05	1081	71.85	164	81.85	390
44.95	341	59.90	368	72.10	122	86.90	1560
45.80	64	61.00	2372	73.05	2035	87.95	1547
47.05	328	62.05	2231	74.05	8268	90.80	248
47.90	80	63.05	2235	75.00	23485	92.05	1654

Average of 12.841 to 12.853 min.: VN080401.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.90	1322	116.90	378	144.75	403	280.90	57
93.10	738	117.70	78	145.00	155	281.10	32
94.00	5475	119.05	461	145.80	62	281.80	75
95.05	43896	127.70	69	147.85	142		
96.05	2790	129.90	315	170.80	84		
103.80	199	130.90	55	171.85	545		
104.10	61	131.10	65	172.90	214		
105.70	66	135.00	55	173.95	35477		
105.95	199	140.70	168	174.90	2512		
115.70	66	141.00	498	175.95	34531		
115.90	118	142.85	1209	177.00	2234		

Instrument :

MSVOA_N

ClientSampleId :

BFB